

GC AND GC/MS

Your Essential Resource for Columns & Supplies



The Measure of Confidence

Agilent Technologies

GC AND GC/MS

Achieve excellent, reproducible performance for difficult samples

For over 40 years, Agilent has broken new ground with innovations in Gas Chromatography. And now, we continue our tradition of leadership by offering you the industry's broadest selection of GC and GC/MS columns and supplies. All are manufactured to Agilent's exact specifications to minimize downtime and ensure consistent, high-quality results.



Agilent Ultra Inert solutions

provide the flow path inertness vital to analytical success. Ultra Inert split and splitless liners are manufactured and tested to our highest level of scrutiny to ensure quality and consistency. Agilent J&W Ultra Inert GC columns are tested with the industry's most demanding test probe to reduce detection limits and produce more accurate data for difficult analytes. Agilent GC and GC/MS instruments bring together all elements for trace-level analysis, dramatically improving MS resolution, spectral integrity, and detection limits.

GC and GC/MS supplies

include premium non-stick septa, plasma coated to eliminate chemical bleed and contamination, so your GC system will maintain its integrity, stay cleaner, and require less maintenance. General-purpose septa are made from an enhanced injection-molded silicone to withstand over 200 automatic injections at 350 °C. Vespel/graphite ferrules are manufactured to the ideal hardness for GC/MS applications to prevent contamination caused by flaking.





Agilent J&W GC columns

deliver the best inertness for acids, bases, and mixed functional compounds, the lowest bleed levels, and the tightest column-to-column reproducibility. Mass Spec Grade GC columns (VF-ms, DB-ms and HP-ms) give you robust performance, low column bleed, and a wide range of selectivity. LTM column modules combine a fused silica capillary GC column with heating and temperature-sensing components for efficient column heating and cooling. What's more, integrated guard columns protect your analytical columns from non-volatile compounds in the sample matrix.

Table of Contents

Agilent Solutions, Services and Support **2**

Featured Products **6**

Agilent Parts and Supplies **12**

- GC and GC/MS Maintenance Schedule **12**
- Bulk GC Supplies **14**
- Inlet Septa **15**
- Inlet Liners **22**
- Capillary Column Ferrules and Nuts **30**
- Capillary Flow Technology Supplies **36**
- Press-Fit Connectors **38**
- Valves and Loops **40**
- Sample Introduction Systems **43**
- Inlet Systems **55**
- Detector Systems **64**
- GC Standards **108**
- GC/MS Parts and Supplies **109**

Agilent CrossLab GC Parts and Supplies **139**

- Product Introductions **140**
- Supplies for Bruker, Varian GC Systems **154**
- Supplies for PerkinElmer GC Systems **169**
- Supplies for Shimadzu GC Systems **175**
- Supplies for Thermo Scientific GC Systems **182**
- Supplies for CTC GC Autosamplers **187**

Agilent J&W GC Columns **188**

- Column Selection **195**
- Application and Method Guides **210**
- Ultra Inert Columns **237**
- High Efficiency Columns **243**
- Low-bleed GC/MS Columns **244**
- Premium Polysiloxane Columns **269**
- Polyethylene Glycol (PEG) Columns **304**
- Specialty Columns **314**
- PLOT Columns **368**
- Non-Bonded Stationary Columns **387**
- Guard Columns **391**
- LTM Column Modules **393**
- Fused Silica Tubing **397**
- Packed GC Columns **400**
- GC Column Test Standards **411**
- Column Installation and Troubleshooting **413**

Applications **428**

- Environmental **429**
- Hydrocarbons **429**
- Pesticides and Herbicides **434**
- Semivolatiles **458**
- Volatiles **468**
- Food, Flavor and Fragrance **478**
- Industrial Chemicals **501**
- Life Sciences **535**
- Energy and Fuels **552**

Indices **577**

Ordering Information **607**

PUT MORE THAN 40 YEARS OF RELENTLESS INNOVATION BEHIND YOUR EVERY RESULT

By continually raising the standards for technologies that support your routine analyses, Agilent's R&D efforts have led to breakthroughs such as:

- **New GC columns** that help you achieve higher levels of inertness and column-to-column reproducibility
- **LC column choices** that deliver the sensitivity and reliability you need for demanding applications
- **Cutting-edge sample preparation products** that promote reliable extraction and concentration
- **Fresh atomic and molecular spectroscopy ideas** for identifying and confirming targets and unknowns

Longtime Agilent customers have experienced our commitment firsthand. And now, we look forward to demonstrating how Agilent's approach to relentless innovation can work to your advantage, too.

CHEMICAL ANALYSIS SOLUTIONS



Food

From high-volume screening of vegetables for large numbers of pesticides to rapid identification of pathogens, Agilent understands the analytical needs of food producers, shippers, and regulators. When a new toxin appears, we deploy substantial resources to quickly help customers develop robust and reliable methods. Agilent's leading separations, mass spectrometry, and spectroscopy solutions are emerging as valuable food testing techniques.



Environmental

Agilent offers more than 40 years of environmental testing and regulatory expertise. We help government and private labs with the full range of assays, from routine testing of soils for heavy metals to detection of pharmaceuticals in groundwater, in concentrations down to parts per trillion.



Energy and Fuels

Agilent collaborates closely with process industry customers to offer analytical systems that meet their needs for separation, detection, throughput, and support. We'll even preconfigure custom or standard analyzers so they arrive at the lab ready-to-go. Agilent's expertise in both chemical analysis and life science is a powerful combination for researching and producing biofuels, including a wide range of analytical techniques for fatty acid methyl esters (FAMEs). Our newly-expanded portfolio also offers powerful tools for developing and producing photovoltaic films and solar panels.



Forensics

Because the careers of world class athletes and many other individuals hinge on drug testing, it's critical that those doing the testing have the highest level of confidence in the results. Forensics analysts worldwide have grown to depend on Agilent tools for accuracy, reliability, and speed in this high stakes, high-throughput field. Our best selling GC, GC/MS and popular LC and LC/MS are workhorses in forensics labs.



Traditional Lab Informatics

The ways labs generate and store data profoundly affect their efficiency. Agilent offers a rich, integrated suite of software products built on a set of customer-driven architectural values with the Agilent OpenLAB Laboratory Software Suite. OpenLAB delivers superior performance, open systems integration and investment protection. Our commitment is to deliver more value across each step in the life cycle of scientific data – from data collection and analysis to interpretation and management.



Materials Science

Agilent offers a newly expanded portfolio of instruments used for the research, manufacturing and testing of advanced materials, from precision optics to pulp, paper and polymers. Tools for chromatography, atomic absorption spectroscopy, molecular spectroscopy, X-ray crystallography, and nuclear magnetic resonance all support continuous progress in materials science.

LIFE SCIENCE SOLUTIONS



Biopharmaceutical

As "multi-omics" studies gain momentum in the search for new therapeutics, Agilent is uniquely positioned to provide the instruments, reagents, and powerful software needed for performing experiments in multiple disciplines and combining the massive amounts of data into biological insight.



Pharmaceutical

Drug manufacturing requires the accuracy, sensitivity and high throughput of other analytical applications, along with the demands of regulatory record-keeping and validation requirements. Agilent provides a potent combination of rugged, high-throughput tools and unmatched compliance services. Agilent now offers the market-leading family of dissolution apparatus and sampling systems that pair perfectly with our HPLC and UV systems.



Proteomics

Research into how large sets of proteins affect the health of an organism requires special sets of analytical tools. Agilent has built a formidable arsenal of liquid chromatograph/mass spectrometers, bioinformatics systems, multiple affinity protein removal columns, and OFFGEL electrophoresis for protein identification and protein biomarker discovery. Accurate-Mass mass spectrometry and the microfluidic HPLC-Chip/MS are two Agilent innovations speeding the work of proteomics researchers around the globe.




Metabolomics

Collections of small molecules are increasingly being seen as rich sources of biomarkers, but studying metabolites presents many challenges. The need for speed, accuracy, and powerful interpretation capabilities in looking at chemical profile snapshots is underscored because molecules are constantly entering, leaving or changing within the metabolome. Agilent's GC, LC, NMR and MS portfolios, along with our excellent bioinformatics offerings, user-customizable METLIN metabolite database for LC/MS, and the industry's first commercial GC/MS retention time locked metabolite library align well with needs of metabolomics researchers.



Genomics

Agilent is a global leader in microarrays, scanners, and reagents used in a wide variety of genomic-based disease research experiments. Our SureSelect Target Enrichment System dominates the category, streamlining next generation sequencing studies worldwide. Agilent offers a wide range of catalog microarrays and a highly-developed capability to produce custom arrays featuring ink jet-based SurePrint fabrication and the eArray on-line design tool. All Agilent microarrays feature highly sensitive, selective 60-mer probes. With as many as eight arrays printed on a standard 1 x 3 in. slide, the cost per experiment becomes very affordable.



Life Science Informatics

Mirroring its extensive instrument portfolio, Agilent offers the industry's most extensive suite of bioinformatics software, helping users derive knowledge from complex genomic, proteomic, metabolomic and other biological data. This includes DNA Analytics for analyzing CGH, ChIP and methylation microarray data. The GeneSpring suite includes informatics software for microarray-based gene expression data, genotyping data, and GeneSpring MS, which are useful for analyzing mass spec data from proteomics and metabolomics experiments and comparing complex datasets to explore biological questions from multiple perspectives.



Lab Automation

To meet the skyrocketing demand for more throughput and automation, Agilent has substantially expanded its lab automation offerings. The Agilent line of liquid handlers and microplate processors are designed to streamline high-volume life science workflows. Agilent is also continually upgrading its advanced autosamplers for LC, GC, LC/MS and GC/MS, adding functionality and speed to reflect the performance of its advanced instruments.



Vacuum Technology

Agilent works with customers to solve vacuum challenges from experiments in high-energy physics to developing systems for producing flat panel displays. Agilent manufactures vacuum systems used in its own mass spectrometry instruments as well as those of other manufacturers. Agilent's vacuum technology has been proven by the most powerful physics experiment ever built, CERN's Large Hadron Collider machine, which was used in the discovery of the Higgs boson particle.



Get the Agilent Service Guarantee

Should your instrument require service while covered by an Agilent service agreement, we guarantee repair or we will replace your instrument for free.

No other company offers this level of commitment to keep your lab up and running at peak efficiency.



Laboratory decision makers and users ranked Agilent as their first choice for general laboratory compliance services.

Agilent Service and Support for Instrument Systems

Focus on what you do best

For over 40 years, Agilent has been building and maintaining the instruments you count on to stay competitive and successful. Trust us to protect your investment with a broad portfolio of services, backed by a global network of experienced service professionals dedicated to the productivity of your lab.

Agilent Advantage Service Plans

The best service available for your Agilent instruments

Agilent offers a flexible range of service plans so that you can choose the level of coverage that is best for your lab.

- **Agilent Advantage Gold** – Priority-one coverage for ultimate uptime and productivity
- **Agilent Advantage Silver** – Comprehensive coverage for dependable laboratory operations
- **Agilent Advantage Bronze** – Total repair coverage at a fixed annual price
- **Agilent Repair Service** – Basic coverage for reliable instrument repair

Agilent Advantage service plans include Agilent Remote Advisor for real-time remote monitoring and diagnostics. Through secure internet connections, you can interact with Agilent service professionals, receive detailed asset reports, and configure text or email alerts to notify you before problems occur – helping you to maximize instrument uptime and optimize laboratory workflows.

Agilent Compliance Services

Equipment qualification that meets the most stringent requirements

Enterprise Edition Compliance was developed to streamline compliance across your entire lab. Used globally in regulated labs, including standards organizations and regulatory agencies, Enterprise Edition enables you to:

- Improve qualification efficiency by automating protocols across platforms to ensure greater efficiency and minimize regulatory risk
- Standardize your entire compliance operation with robust test designs that work with all your instruments
- Add, remove or reconfigure tests based upon your unique user requirements
- Significantly reduce staff review time with consistently formatted, computer generated, tamper-proof reports

Agilent Education and Consulting Services



Our best minds, working for you

Make the most of your instrument with training and consulting from the same experts who designed the instruments, software and processes you use every day.

- Classroom and on-site training in instrument operation, troubleshooting and maintenance
- Customized consulting services to meet your lab's unique needs

The Agilent Value Promise – 10 Years of Guaranteed Value

In addition to continually evolving products, we offer something else unique to the industry – our 10-year value guarantee. The Agilent Value Promise guarantees you at least 10 years of instrument use from your date of purchase, or we will credit you with the residual value of the system toward an upgraded model. Not only does Agilent ensure a reliable purchase now, but we also ensure that your investment is just as valuable in the future.

For more detailed information,
please go to **www.agilent.com/chem/services**
or contact your local Agilent Services and Support representative.

Technical Support at work for you



Have a hardware, software, application, instrument repair or troubleshooting question? Agilent's technical experts are available to answer your questions. With years of laboratory experience, our technical support specialists can provide in-depth knowledge and experience.

For questions pertaining to supplies found in this catalog, contact your local Agilent office or Authorized Agilent Distributor or visit **www.agilent.com/chem/techsupport**

Need more information?

Visit **www.agilent.com/chem/contactus** to:

- Locate your nearest Agilent office or distributor for expert technical support.
- Get fast sales and product assistance by phone. Simply use the scroll-down menu to select your country.
- Receive email assistance using our convenient online forms.

Agilent GC and GC/MS Systems

Achieve the highest level of Productivity and Performance

The industry leader in Gas Chromatography

The Agilent 7890 GC



Gives you everything you need to take your lab to the next level of performance, including advanced separation capabilities and powerful productivity tools

The Agilent 7820A GC



An affordable, high-quality solution for small- to medium-sized labs that are require with routine analyses using standard GC methods

The Agilent 6850 Series II GC



An excellent choice for any laboratory where bench space, ease of use, and independent channel flexibility are important

The information you need, wherever you need it

The Agilent 490 Micro GC and 490-PRO



The right GC solution If you want the ability to measure anywhere, and get the results you need in seconds

The customer-proven worldwide bestseller, Agilent 5975 Series GC/MSD

5975C GC/MSD



Superior performance, reliability, and productivity with industry-leading 7890 GC

5975T LTM GC/MSD



Compact, transportable GC/MS with fast, lab-quality performance

5975E GC/MSD



Affordable GC/MSD with economical 7820GC

Flexible, sensitive, and affordable EI, CI, and MS/MS, Agilent 240/220 Ion Trap GC/MS



240 Ion Trap GC/MS

The most powerful EI, CI and MS/MS analysis with unmatched full scan sensitivity



220 Ion Trap GC/MS

Compact and budget-friendly design – No.1 Ion Trap system in universities worldwide

Our most powerful trace analysis system

Agilent 7000B Triple Quadrupole GC/MS

You can rely on Agilent's 7000B Triple Quadrupole GC/MS system for extraordinary sensitivity, selectivity, and day-after-day reliability with your most complex matrices





Your choice for exceptional qualitative analysis, Agilent 7200 Q-TOF GC/MS

The world's first Q-TOF GC/MS combines the proven separation power of Agilent's 7890A GC with the high detection selectivity and accurate mass information of a TOF analyzer



Agilent Analyzers and Application Kits

Bring a new Application online can stretch your lab to the limit. Agilent solves this problem with our GC, Micro GC, GC/MS and GC/MS/MS Analyzers, which are factory preconfigured and pre-tested to get you up and running in the shortest possible time.

Agilent Gas Clean Filters



The Agilent Gas Clean Filter System provides enhanced gas quality for maximum productivity. Clean gases reduce the risk of column damage, sensitivity loss, and instrument downtime. Oxygen, hydrocarbons and moisture can cause loss of sensitivity and accuracy of the GC, and damage your column and consumables. Inserting a Gas Clean Filter System in the gas line immediately before the instrument inlet greatly reduces the level of impurities and helps you detect any problems before they occur.

Turn to pages 132-133.



Ultra Inert GC Columns

The Agilent J&W Ultra Inert GC column family pushes industry standards for consistent column inertness and exceptionally low column bleed, resulting in lower detection limits and more accurate data for difficult analytes. And, each column is tested with the most demanding Ultra Inert test probe mixture in the industry, and an individual performance summary sheet is shipped with each column.

Turn to page 237.

Ultra Inert Liners



Agilent Ultra Inert Inlet liners provide a robust, reproducible and reliable inert flow path, even when containing wool. These liners are rigorously tested and certified to ensure exceptional batch-to-batch uniformity, low bleed and superior coverage, even with highly active compounds.

Turn to pages 22-29.



Bulk GC Supplies

Ideal for high-usage laboratories, Agilent bulk gas chromatography supplies provide the high quality and consistency of Agilent chromatography supplies in convenient and economical packaging.

Turn to page 14.

Agilent CrossLab

Agilent CrossLab Supplies

Agilent CrossLab offers a growing portfolio of GC supplies manufactured for seamless performance with a variety of non-Agilent analytical instruments in your lab. Look inside this catalog to find a wide range of products for your applications.

Agilent CrossLab is more than supplies:

- Over 40 years of chromatography expertise
- The right supplies for both routine and challenging applications
- Hassle-free operations and reproducible results
- High-quality products manufactured to Agilent standards
- Technical and application support
- Dependable worldwide availability and delivery
- Convenience of consolidating purchasing
- 90-day risk free money back guarantee

All with our risk-free, 90-day, money-back guarantee.



Agilent CrossLab GC supports instruments from PerkinElmer, Shimadzu, Dionex (now part of Thermo Scientific), CTC Analytics, and more. The comprehensive range includes premium non-stick inlet septa, Ultra Inert inlet liners, liner-O-rings, column ferrules and nuts, autosampler syringes, and vials and closures.

All Agilent CrossLab high quality supplies are backed by Agilent's worldwide technical support and dependable availability and delivery.

Turn to page 139.

Agilent Parts and Supplies

GC and GC/MS Maintenance Schedule

Item	Typical Schedule	Actions/Comments
Gas Management		
Gas purifiers (carrier gas and detector gas)	Every 6 to 12 months	Replacement schedule is based on capacity and grade of gas. In general, replace non-indicating traps every 6 to 12 months or when indicating traps start to change color. Replace indicating traps when indicating material is starting to change color.
Internal split vent trap	Every 6 months*	Replace to prevent material backing up into EPC control and to avoid costly repair.
External split vent trap	Every 6 months*	Replace to prevent sample analytes from escaping into the laboratory environment.
Flow meter calibration	Every 1 to 2 years	Re-calibrate electronic flow meters – follow recommended schedule for the unit (shown on the calibration certificate).
Sample Introduction and Inlets		
Syringes and/or syringe needles	Every 3 months*	Replace syringe if dirt is noticeable in the syringe, if it cannot be cleaned, if the plunger doesn't slide easily, or if clogged. Replace needle if septa wear is abnormal or the needle becomes clogged.
Inlet liner	Weekly*	Check often. Replace when dirt is visible in the liner or if chromatography is degraded.
Liner O-rings	Monthly*	Replace with every liner change.
Inlet septum	Daily*	Check often. Replace when signs of deterioration are visible (gaping holes, fragments in inlet liner, poor chromatography, low column pressure, etc.)
Inlet hardware	Every 6 months Every year	Check for leaks and clean. Check parts and replace when parts are worn, scratched, or broken.
Inlet gold or stainless steel seal	Monthly*	For highest level of reproducibility, change inlet seal with every liner change, but minimally replace monthly or when scratched, corroded, or if there is build-up of non-volatile sample components.

*Schedule is an approximation of average usage requirements. Frequency may vary widely based upon application and sample type.

(Continued)



GC and GC/MS Maintenance Schedule

Item	Typical Schedule	Actions/Comments
Columns		
Front-end maintenance	Weekly-monthly*	Remove 1/2 to 1 m from the front of the column when experiencing chromatographic problems (peak tailing, decreased sensitivity, retention time changes, etc.). Replace inlet liner and septum, and clean inlet as necessary. Guard column may be useful for increasing column lifetime.
Solvent rinse	As needed	Perform when chromatography degradation is due to column contamination. Only for bonded and cross-linked phases.
Replacement	As needed	Replace when trimming and/or solvent rinsing no longer restore chromatographic performance.
Ferrules	As needed	Replace when changing columns and inlet/detector parts.
Detectors		
FID/NPD jets and collector	As needed	Clean when deposits are present. Replace when they become scratched, bent, or damaged, or when having difficulty lighting FID or keeping flame lit.
NPD bead	As needed	Replace when signal drifts or there is a dramatic change in sensitivity.
FID	Every 6 months	Measure hydrogen, air, and makeup gas flows.
TCD	As needed	Thermally clean by "baking-out" when a wandering baseline, increased noise, or a change in response is present. Replace when thermal cleaning does not resolve the problem.
ECD	Every 6 months or as needed	Wipe test. Thermally clean by "baking-out" when baseline is noise, or the output value is abnormally high. Replace when thermal cleaning does not resolve the problem.
FPD	Every 6 months or as needed	Measure hydrogen, air, and makeup gas flows. Clean/replace FPD windows and seals when detector sensitivity is reduced.
NCD and SCD	Every 3 months*	Change pump oil, oil coalescing filter and chemical trap.
Mass Selective Detectors		
Tune MSD	As needed	Keep plenty of PFTBS (P/N 05971-60571) on hand.
Check the calibration vial	Every 6 months	Vial can be refilled without venting the system.
Replace the foreline pump oil	Every 6 months	Check the fluid weekly. Change when the fluid becomes discolored or every 6 months.
Replace the diffusion pump fluid	Every year or as needed	Check the fluid weekly. Too little fluid will cause the pump to run at a higher temperature, resulting in degradation and loss of high vacuum. Change when the fluid is discolored or contains particulates.
Clean the ion source	As needed	Clean when performance deteriorates to remove contamination and to restore the electrostatic properties of the ion lens system. Replace scratched parts to maintain optimal performance.

*Schedule is an approximation of average usage requirements. Frequency may vary widely based upon application and sample type.

Bulk GC Supplies



Single taper splitless liner, no wool, 5190-2270



Certified gold plated seal kit, 5190-2209



Liner O-rings, 5190-2269



Non-stick BTO septa, 5190-3157

Ideal for high usage laboratories, our bulk supplies provide the quality and consistency of Agilent chromatography supplies in convenient and economical packaging. We currently offer Agilent inlet liners, septa, gold inlet seals, and liner O-rings in bulk packaging.

- Economical and convenient packaging
- Overall cost of ownership reduced
- Same great quality Agilent products

Bulk GC Supplies

Description	Unit	Part No.
Ultra Inert Liners		
Ultra Inert Liner, low pressure drop, glass wool	100/pk	5190-3173
Ultra Inert Liner splitless liner, single taper, no wool	100/pk	5190-3170
Ultra Inert splitless liner, single taper, glass wool	100/pk	5190-3171
Ultra Inert split liner, straight, glass wool	100/pk	5190-3172
Liners		
Single taper split liner, low pressure drop	100/pk	5190-2275
Single taper splitless liner, no wool	100/pk	5190-2270
Single taper splitless liner, glass wool	100/pk	5190-2271
Double taper splitless liner, no wool	100/pk	5190-2272
Seals		
Certified gold plated seal kit, includes washer	10/pk	5190-2209
O-Rings		
Non-stick fluorocarbon O-ring for Flip Top	100/pk	5190-2268
Certified non-stick fluorocarbon O-ring	100/pk	5190-2269
Septa		
Non-stick BTO septa, 11 mm	400/pk	5190-3157
Non-stick Advanced Green septa, 11 mm	400/pk	5190-3158
Siltite Ferrule Bulk packs		
Ferrules, Siltite,0.1 to 0.25 mm column	100/pk	5190-4022
Ferrules, Siltite, 0.32 mm column	100/pk	5190-4023
Ferrules, Siltite, 0.53 mm column	100/pk	5190-4024

Inlet Septa



Septa are available for a variety of different applications and have different upper temperature limits. Lower temperature septa are usually softer, seal better, and can withstand more punctures (injections) than their high-temperature counterparts. If septa are used above their recommended temperatures, they can leak or decompose, causing sample loss, lower column flow, decreased column life and ghosting. To minimize problems:

- Use within the recommended temperature range
- Change regularly
- Install the retainer nut "finger-tight"
- Use septum purge when available
- Use autoinjectors
- Use sharp syringe needles

Premium Non-Stick Septa

Agilent premium non-stick inlet septa are designed and manufactured to provide a reliable non-contaminating seal. Our tri-fold blister pack ensures that each septum remains clean and ready to use.

- Proprietary plasma treatment prevents sticking and unnecessary inlet cleaning
- Innovative blister packaging keeps each septum clean and ready for use
- Center point guides the needle for easy penetration, less coring and longer life
- Precision molding assures accurate fit in the inlet
- Each batch is tested for bleed on Agilent 7890 GC-FID
- Premium formulations selected for sealing and chromatographic cleanliness
- No need to bake septa before using



Inlet Septa

Summary of Premium Inlet Septum Characteristics

Septum Type	Bleed	Lifetime	Temperature Limits
Non-Stick BTO (Bleed and Temperature Optimized)	✓✓✓	✓	to 400 °C injection port temp
Non-Stick Advanced Green	✓✓	✓✓	to 350 °C
Non-Stick Long-Life	✓	✓✓✓	to 350 °C

✓✓✓ = best ✓✓ = very good ✓ = good

TIPS & TOOLS

Need inlet septa for your non-Agilent instruments? Check the Agilent CrossLab septa starting on page 147



Inlet Septa

Non-Stick Bleed and Temperature Optimized (BTO) Septa

- Extended temperature range, lowest bleed
- Maximum injection port temperature 400 °C
- Plasma treatment eliminates sticking in the injection port
- Pre-conditioned; ready to use
- Blister packaging for cleanliness and convenience
- Ideal for use with low-bleed, "Mass Spec" capillary columns




BTO septa, 5183-4757


Non-Stick Bleed and Temperature Optimized (BTO) Septa

Description	Unit	Part No.
11 mm septa	50/pk	5183-4757
11 mm septa	100/pk	5183-4757-100
11 mm septa	400/pk	5190-3157
5 mm septa through-hole for on-column, in glass jar	50/pk	5183-4758

Comparison of septum purity: TIC profile of iso-octane extractions

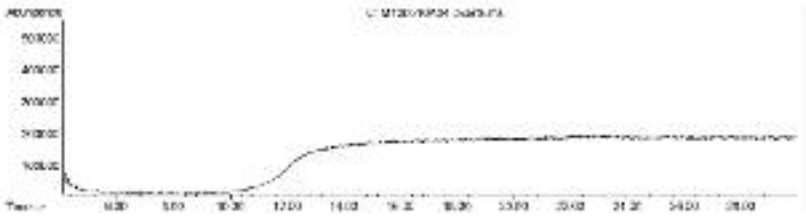

Agilent BTO Septa with CenterGuide

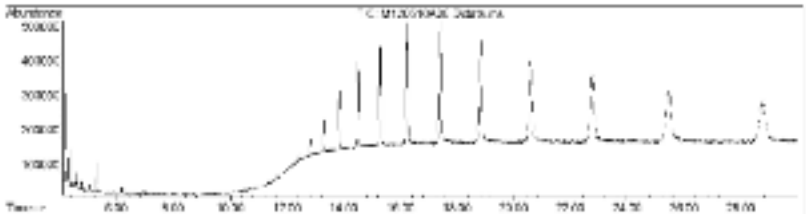

Competitor's High-Temperature Septa without CenterGuide

Non-Stick Advanced Green Septa

- True long-life, high temperature green septa
- More injections per septum
- Plasma treatment eliminates sticking in the injection port
- Maximum injection port temperature 350 °C
- High-performance alternative to competitors' "green" septa
- Blister packaging for cleanliness and convenience



Advanced green septa, 5183-4759

Non-Stick Advanced Green Septa

Description	Unit	Part No.
11 mm septa	50/pk	5183-4759
11 mm septa	100/pk	5183-4759-100
11 mm septa	400/pk	5190-3158
5 mm septa through-hole for on-column, in glass jar	50/pk	5183-4760

Non-Stick Long-Life Septa

- The preferred septa for autosamplers
- Pre-pierced for extended life and reduced coring
- Ideal for overnight runs
- Up to 400 injections per septum
- Plasma treatment eliminates sticking
- Maximum injection port temperature 350 °C
- Soft, 45 durometer, easy on autosampler needles
- Blister packaging for cleanliness and convenience





Long-life septa, 5183-4761

Non-Stick Long-Life Septa

Description	Unit	Part No.
11 mm septa	50/pk	5183-4761
11 mm septa	100/pk	5183-4761-100
5 mm septa through-hole for on-column, in glass jar	50/pk	5183-4762

Septa Troubleshooting

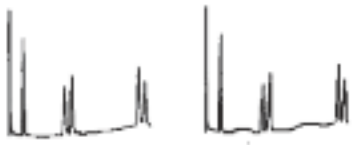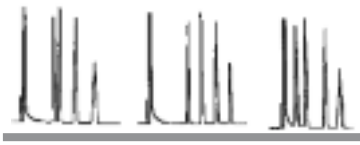Symptom	Possible Causes	Remedy
Extra Peaks/Humps 	Septum bleed	Turn off injector heater. If extra peaks disappear, use septum specified for higher temperature or analyze at lower inlet temperature.
Baseline Change After Large Peak 	Large leak at septum during injection and for a short time thereafter (common with large diameter needles)	Replace septum and use smaller diameter needles.
Retention Times Prolonged 	Carrier gas leaks at septum or column connection	Check for leaks. Replace septum or tighten connections if necessary.



General Purpose Septa

Agilent's general purpose septa are made from an enhanced injection-molded silicone rubber. The septa material, gray in color, is specified to withstand over 200 automatic injections at an injection port temperature of 350 °C.



General purpose gray septa

General Purpose Septa

Description	Unit	Part No.
11 mm septa	50/pk	5080-8896-50
11 mm septa	100/pk	5080-8894-100
9.5 mm (3/8 in) septa*	50/pk	5080-8728-50
9.5 mm (3/8 in) septa*	100/pk	5080-8728-100
5 mm through hole septa for on-column inlets, automatic or manual injections**	25/pk	5181-1260
5 mm septa for high column backpressure, on-column inlets**	25/pk	5181-1261

*For 5700 series and 5830/40 GCs

**5 mm septa are packaged in glass jars



Merlin Microseal

- Low bleed, longer life alternative to standard septa for split/splitless injection and SPME
- Requires 23 gauge syringe needle
- Has a lifetime of more than 2000 injections, depending on samples and operating conditions
- Greatly reduced instrument downtime for septa changes and injection port liner changes due to septa particulates
- Two distinct sealing mechanisms: double O-ring type seal around the syringe needle and spring assisted duckbill to seal the injection port
- Temperature range 50-400 °C

Merlin Microseal

Description	Part No.
General Purpose Merlin Microseal (3-100 psi)	
General purpose Merlin Microseal starter kit Includes Microseal septum and nut	5182-3442
Merlin Microseal general purpose replacement septum 3 to 100 psi	5182-3444
Merlin Microseal high pressure nut	5182-3445
High sample volume septum kit Contains general purpose Merlin Microseal, six 23-gauge syringes, 500 vials and caps	5181-8839
Low Pressure Merlin Microseal (1-45 psi)	
Merlin Microseal kit, low pressure Includes nut and septum	5181-8816
Merlin Microseal kit, low pressure Includes nut and 2 septa	5181-8833
Merlin Microseal low pressure replacement septum	5181-8815
Microseal PTFE nut liners, 2/pk	5182-0853

(Continued)

Merlin Microseal

Description	Part No.
For Bruker/Varian GCs*	
Merlin microseal SPME kit, 1079 23 gauge, 1/p	392609901
Merlin Microseal adapter kit for 1177 inlets Contains adapter, nut and general purpose Merlin Microseal septum	392609903
Merlin microseal SPME replacement seal, 23GA, 1/pk	392609902
Syringes for Merlin Microseal	
Autosampler syringe Gold Standard, 5 µL, 23 gauge	9301-0892
Autosampler syringe, Gold Standard plunger, 10 µL, 23 gauge	9301-0713
Autosampler syringe, Blue Line, 5 µL, 23 gauge	G4513-80213
Autosampler syringe, Blue Line, 10 µL, 23 gauge	G4513-80209
Manual syringe, 5 µL, 23 gauge	5182-3438
Manual syringe, 10 µL, 23 gauge	5182-3439

*Varian GC systems are now Bruker products

TIPS & TOOLS

Agilent Blue Line autosampler syringes are specifically designed to support the higher productivity features of the 7693A ALS, while increasing plunger life and reducing costly downtime. Learn more at **www.agilent.com/chem/BlueLineSyringes**



Inlet Liners

Injection port liners have a variety of features to help vaporize the sample so that a true representation of the sample enters the column. Additionally, Agilent liners are individually packaged to maintain cleanliness until used. The part number and lot are silk screened on the liner for quality control and user convenience, and lot tracking is available for quality assurance.

Liner Dimensions Driven by Inlet Operation

Well-controlled glass dimensions promote better liner-to-liner consistency, ensuring GC system accuracy and reproducibility. That is why Agilent liners are made to the following precise tolerances:

Outer Diameter (OD)

- Larger od liners fit tightly to improve analyte recovery and limit sample migration onto the inlet's metal surface. Ideal for splitless injection.
- Smaller od liners are less resistant to carrier and split flow inside the inlet. Best for split injection.

Internal Diameter (ID)

- Ensures that the sample vapor is small enough to fit within the volume of the liner.
- Prevents backflash, sample loss into the septum purge, and split lines – all of which can lower reproducibility and sensitivity.

TIPS & TOOLS

Clearly Better Inertness

Confidently quantify active analytes with industry leading Ultra Inert GC solutions

- Agilent industry leading GC/MS instruments
- Ultra Inert columns
- Ultra Inert liners

To learn more and order your free poster, visit **www.agilent.com/chem/ultrainert**



Length

- Regulates internal volume and ensures proper sealing between the septum and the inlet seal.
- Precise glass bumps on the bottom of the liner allow you to repeatably position the liner relative to the inlet bottom. This is especially critical if you install liners by measuring the distance from the O-ring to the top of the liner.

Tapers

None	Bottom Tapers	Dual Tapers
• Straight tubes used in split injection with autosamplers	• Directs sample onto head of column and limits analyte exposure to bottom of inlet • Minimizes decomposition and discrimination	• Contain sample within glass liner limiting contact with metal inlet surface • Thought to limit loss through septum purge

Glass Wool

- Less molecular weight discrimination
- Provides additional surface area for sample vaporization, increasing reproducibility
- Serves as a trap for non-volatiles

For split liners, Agilent specifies the placement of glass wool in the liner so that the syringe penetrates the glass wool, wiping the syringe, to provide the most repeatable results with Agilent autosampler and split/splitless inlet design thermal profile.

Agilent Ultra Inert deactivated liners are recommended for samples with active analytes – such as phenols, amines, organic acids, pesticides and drugs of abuse – that could be irreversibly adsorbed on active surfaces in the inlet.

Deactivation

Developed for your high sensitivity analyses, Ultra Inert deactivation provides extreme surface inertness – even for liners containing glass wool. Agilent Original deactivation is recommended for your everyday analyses With use, even deactivated liners become active. Replace the liner regularly.

TIPS & TOOLS

Tight control of liner dimensions is critical to reproducibility of GC results.





Single taper, Ultra Inert Liner with glass wool, 5190-2293



Agilent Ultra Inert Liners

Agilent Ultra Inert Liners



Agilent Ultra Inert Liners are the perfect companion to Agilent J&W Ultra Inert GC columns. They provide reproducible inertness liner after liner, maintained through a sequence of samples, and for a range of analytes. Agilent's Ultra Inert Liners were developed – and are manufactured and certified – using a suite of tests specifically designed to ensure batch-to-batch uniformity.

- Exceptional batch-to-batch liner uniformity
- Low to no bleed or background contamination
- Superior coverage, allowing use of glass wool even with highly active compounds

Only Ultra Inert Liners are delivered in Agilent's exclusive touchless packaging with a pre-cleaned, conditioned and non-stick plasma treated O-ring pre-installed. Touchless packaging aids in removal of the old liner, and easy installation of the new, clean, preconditioned liner – without risk of contamination from touching.

Agilent Ultra Inert Liners

Description	Volume (µL)	ID (mm)	1/pk	5/pk	25/pk	100/pk*
Split Inlet Liners						
Low pressure drop, Ultra Inert Liner with glass wool	870	4	5190-2295	5190-3165	5190-3169	5190-3173
Straight, Ultra Inert Liner with glass wool	990	4	5190-2294	5190-3164	5190-3168	5190-3172
Splitless Inlet Liners						
Single taper, Ultra Inert Liner	900	4	5190-2292	5190-3162	5190-3166	5190-3170
Single taper, Ultra Inert Liner with glass wool	900	4	5190-2293	5190-3163	5190-3167	5190-3171
Splitless, double taper Ultra Inert Liner, no wool	800	4	5190-3983	5190-4007		
Dimpled, splitless, Ultra Inert Liner	200	2	5190-2297	5190-4006		
Straight, Ultra Inert Liner		1	5190-4047			
Straight Ultra Inert Liner for SPME		.75	5190-4048			

*The 100/pk is not in the Touchless packaging. O-rings must be purchased separately.

TIPS & TOOLS

Remove the risk of contamination with touchless packaging.

Ultra Inert Inlet Liners are delivered in exclusive Agilent touchless packaging with a pre-cleaned, conditioned, and non-stick plasma treated O-ring pre-installed. Now you can quickly and easily install the new, clean liner – without searching for the O-ring pack or risking contamination from touching.

View a demonstration of the touchless packaging at **www.agilent.com/chem/touchless**

Agilent Original Deactivation Split Liners

Agilent single taper split liners are made to strict dimension specifications for optimal inlet performance and feature the tightest tolerances for od, id, taper, and glass wool placement. For ease-of-use and reproducibility, some liners have a positioning bead, a restriction to secure the position of the glass wool, and a feature to consistently self-position to the recommended height. The liners also feature Agilent's Original proprietary deactivation.

TIPS & TOOLS

Agilent recommends part number 5190-2295 as the top split liner and for splitless injection UI part number 5190-2293

Agilent Original Deactivation Split Liners


Description	Volume (µL)	ID (mm)	1/pk	5/pk	25/pk	100/pk
Single Taper Split Liners						
Single taper, glass wool, deactivated, low pressure drop	870	4	5183-4647	5183-4701	5183-4702	5190-2275
Single taper, glass wool, deactivated	870	4	5183-4711	5183-4712	5183-4713	
Straight Split Liners						
Straight, glass wool, non-deactivated	990	4	19251-60540	5183-4691	5183-4692	
Focus Liners						
Deactivated with glass wool	935	4		210-4004-5		
Tapered, deactivated with glass wool	880	4		210-4022-5		



Single taper split liner, 5183-4647, 5183-4711



Straight split liner, 19251-60540



Focus liners, 210-4004-5, 210-4022-5

TIPS & TOOLS

To learn more about our comprehensive portfolio of Agilent CrossLab GC supplies – including our Agilent CrossLab original deactivation liners – go to **www.agilent.com/chem/CrossLab**

Agilent Original Deactivation Splitless Liners



Single taper splitless liner, 5181-3316, 5181-3316i



Single taper, glass wool splitless liner, 5062-3587



Double taper splitless liner, 5181-3315



Straight, non-deactivated, quartz splitless liner, 18740-80220, 5181-8818



Straight, non-deactivated splitless liner, 210-3003



Direct inject liner, 18740-80200

Agilent Splitless Liners

Description	Volume (µL)	ID (mm)	1/pk	5/pk	25/pk	100/pk
Single Taper Splitless Liners						
Single taper, deactivated	900	4	5181-3316	5183-4695	5183-4696	5190-2270
Single taper, inert	900	4	5181-3316i			
Single taper, glass wool, deactivated	900	4	5062-3587	5183-4693	5183-4694	5190-2271
Double Taper Splitless Liners						
Double taper, deactivated	800	4	5181-3315	5183-4705	5183-4706	5190-2272
Straight Splitless Liners						
Straight, deactivated, quartz	250	2	5181-8818	5183-4703	5183-4704	
Straight, non-deactivated, quartz	250	2	18740-80220	5183-4707	5183-4708	
Straight, non-deactivated	990	4	210-3003	210-3003-5		
Direct Inlet Liners						
Straight, non-deactivated (for gas samples, headspace, or purge & trap)	140	1.5	18740-80200	5183-4709	5183-4710	

TIPS & TOOLS


Need inlet liners and O-rings for your non-Agilent instruments? Check out the Agilent CrossLab inlet liners. See pages 140-141.




Agilent Specialty Injection Liners

MultiMode Inlet Heavy Matrix

Description	Volume (µL)	ID (mm)	1/pk	5/pk	25/pk
Dimpled					
Dimpled splitless single taper, deactivated	200	2	5190-2296		
Ultra Inert Deactivated Dimpled liners					
Dimpled, splitless, Ultra Inert Liner	200	2	5190-2297	5190-4006	
Manual Injection					
Straight, with cup (for manual injections)	800	4	18740-80190	5183-4699	5183-4700
Straight split liner with cup, glass wool, and packing, 18740-60840	800	4	18740-60840	5183-4697	5183-4698
	800	4			
	800	4			
Straight, with cup (for manual injections)	800	4			
SPME					
SPME, deactivated	70	0.75	5188-6471		
SPME, Ultra Inert deactivation	70	0.75	5190-4048		
Volatiles					
Volatiles Organic Analysis liner	1		5190-4047		





Single taper dimpled splitless liner, 5190-2296, 5190-2297




Straight split liner with cup, glass wool, and packing, 18740-60840


Programmed Temperature Vaporization (PTV) Liners

Description	Volume (µL)	ID (mm)	Part No.
PTV Liners			
PTV liner, single baffle, glass wool, deactivated	180	2	5183-2038
PTV liner, single baffle, deactivated	200	2	5183-2036
PTV liner, multi baffled, deactivated	150	1.8	5183-2037
PTV liner, sintered glass, deactivated	112	1.5	5190-1426
Liners for High Temperature PTV Inlet, G3506A			
PTV liner, high temperature, quartz	713	3.4	5188-5313
PTV liner, high temperature, borosilicate	668	3.4	5188-5356

Direct Connect



Single taper direct connect liner, G1544-80730



Dual taper direct connect liner, G1544-80700

Description	ID (mm)	Part No.
Direct Connect		
Direct column connect	4	G1544-80730
Dual taper direct connect liner, splitless, Agilent proprietary deactivation	4	G1544-80700
Single taper direct connect liner, splitless, deactivated, inert	4	G1544-80731

Liner O-Rings



Liner O-rings, 5190-2269

- Liners are sealed in the inlet with O-rings or graphite seals
- Graphite seals are used when inlet temperatures exceed 350 °C
- Fluorocarbon O-ring seals are easier to replace than graphite that deforms and flakes apart

Only Agilent Fluorocarbon Liner O-rings are:

- Pre-cleaned, then conditioned to eliminate out-gassing of contaminants, which is especially important for trace, ECD and MSD analyses
- Plasma treated for a non-stick, contaminant-free surface that won't stick to the inlet metal surface
- Packaged for convenience and cleanliness in a novel dial package that delivers 1 clean O-ring at a time

Liner O-Rings

Description	Unit	Part No.
Certified non-stick fluorocarbon O-ring	10/pk	5188-5365
	100/pk	5190-2269
Graphite O-ring for splitless liner	10/pk	5180-4173
Graphite O-ring for split liner	10/pk	5180-4168
Non-stick fluorocarbon liner O-ring for Flip Top	10/pk	5188-5366
	100/pk	5190-2268
High temperature PTV inlet liner fluorocarbon O-ring	10/pk	5188-5311

TIPS & TOOLS

Agilent's Ultra Inert GC liners are delivered in Touchless packaging with a certified, non-stick O-ring pre-installed. See page 24.



Capillary Column Ferrules and Nuts

Using the wrong ferrule or a worn-out ferrule to seal your column connection can result in inconsistent and unreliable chromatography. An improper ferrule can cause leaks, which allow air and other contaminants to enter the instrument through the column seal, causing major interference with column and detector performance.

For optimum performance, ferrules should be replaced every time the column is replaced and when performing column maintenance.

To minimize problems, follow these general techniques for ferrule installation:

- Don't overtighten – finger tighten the column nut, then use wrench to tighten
- Maintain cleanliness
- Bake out ferrules prior to use (Vespel and Vespel/Graphite only)
- Avoid contamination, such as fingerprint oils
- Inspect used ferrules with magnifier for cracks, chips, or other damage before reusing them
- Change ferrules when new columns or injector/detector parts are installed



Vespel/Graphite ferrules, 5181-3323

Caution: Agilent capillary column ferrules are manufactured to tolerances specific for Agilent J&W HP and DB brand columns. Fused silica tubing used for Agilent J&W VF columns has slightly different tolerances for the outer diameter. Turn to pages 32-33.

Ferrule Selection Recommendations

Ferrule Type	Upper Temp. Limit	Usages	Advantages	Limitations
Graphite (100%)	450 °C	• General purpose for capillary columns • Suitable for FID and NPD • Recommended for high temperature and cool on-column applications	• Easy-to-use stable seal • Higher temperature limit • Can be removed easily	• Not for MS or oxygen-sensitive detectors • Soft, easily deformed or destroyed • Possible system contamination
Vespel/Graphite (85%/15%)	350 °C	• General purpose for capillary columns • Recommended for MS and oxygen-sensitive detectors • Most reliable leak-free connection	• Mechanically robust • Long lifetime	• Not reusable • Flows at elevated temperature • Must re-tighten frequently
Vespel (100%)	280 °C	• Isothermal operation • Can be reused or removed easily • Excellent sealing material when making metal or glass connections	• Mechanically robust • Long lifetime • Can be reused or removed easily	• Leaks after temperature cycle • Flows at elevated temperature • Must re-tighten frequently

TIPS & TOOLS

Look for the following signals that indicate ferrule damage:

- Background noise from oxygen diffusing into the system
- Column bleed catalyzed by oxygen
- Sample degradation
- Sample loss
- Increase in detector signal/noise
- Poor retention time reproducibility



Short and Long Ferrules

Short Ferrules (height 3 mm)



Vespel/Graphite ferrules, 5181-3323



Universal column nut, 5181-8830

Standard fitting for Agilent GC inlet and detectors (FID, NPD, ECD) column connections use short ferrules and the Universal nut

Long Ferrules (height 3.6 mm)



Pre-conditioned long ferrule for MSD connection, 5062-3508



MS interface column nut, 05988-20066

Pre-conditioned graphite/vespel ferrules are recommened with MSD Interface nut



Column nut for long or long two-hole ferrules, 05921-21170

Alternative nut for Agilent standard inlet or detector fittings used with long graphite/vespel ferrules

TIPS & TOOLS

100% Vespel ferrules should only be used for isothermal applications.

Capillary Column Ferrules – for use with the most brands of column, including DB and HP columns

Column ID (mm)	Ferrule Nom ID	Graphite Ferrule Short Part No.	Vespel Short Ferrule Part No.	85% Vespel/15% Graphite Short Ferrule Part No.	Pre-Conditioned Long Ferrule 85% Graphite/15% Vespel for MSD connection
0.1-0.25	0.4	500-2114	5181-3322	5181-3323	5062-3508
0.32	0.5	5080-8853	5062-3513	5062-3514	5062-3506
0.45	0.8	500-2118	5062-3511	5062-3512	5062-3538
0.53	0.8	500-2118	5062-3511	5062-3512	5062-3538
No hole				5190-4054	5181-3308

Capillary Column Ferrules – for use with CP, VF and Select columns

Column ID (mm)	Factor 4, Select and CP Column Brands	Ferrule Nom ID	Graphite Ferrule Short Part No.	Vespel Ferrule Short Part No.	85% Vespel/ 15% Graphite Short Ferrule	Pre-Conditioned Long Ferrule 85% Graphite/15% Vespel for MSD*
0.025-0.05	CP, VF, Select	0.4	500-2114	5062-3515	5062-3516	5062-3507
0.075	CP, VF, Select	0.4	500-2114	5062-3515	5062-3516	5062-3507
0.1-0.25	CP, VF, Select	0.5	5080-8853	5062-3513	5062-3514	5062-3508
0.32	CP, VF, Select	0.5	5080-8853	5062-3513	5062-3514	5062-3508
	CP-silica PLOT	0.8	500-2118	5062-3511	5062-3512	5062-3538
0.53	CP, VF, Select	0.8	500-2118	5062-3511	5062-3512	5062-3538
No hole					5190-4054	5181-3308

*These ferrules are recommended for GC/MS

For additional capillary column ferrule selection, please refer to our CrossLab portfolio.Turn to page 143.



Vespel ferrule, 5181-3322



Graphite ferrules, 5080-8853



Vespel/Graphite ferrule, 5062-3514



Universal column nut, 5181-8830



MS interface column nut, 05988-20066

Column Nuts

Description	Part No.
Short Nuts	
Universal column nut, 1/16 in hex, 2/pk	5181-8830
Finger tight column nut for 530 µm columns*	5020-8293
Finger tight column nut for 320 µm columns and smaller*	5020-8292
Blanking plug, finger tight style	5020-8294
6850 column nut, 2/pk	5183-4732
Extended column nut, VI inlet	G3504-20504
High Temperature SimDis PTV inlet, 4 mm hex	5188-5312
Long Nuts	
MS interface column nut, female	05988-20066
Column nut for long or long two-hole ferrules	05921-21170
Accessories	
Open end wrench, 1/4 and 5/16 in	8710-0510

*For use with graphite ferrules only

Specialty Ferrules, 85% Vespel/15% Graphite

Ferrule ID (mm)	Column ID (mm)	Unit	Part No.
Two Hole			
0.5	0.1	10/pk	5181-3388
0.5	0.10.20.25	10/pk	5062-3580
0.5	0.32	10/pk	5062-3581
No Hole			
Capillary column long ferrule		10/pk	5181-3308
Capillary column short ferrule		10/pk	5190-4054
High Temperature PTV Inlet SS/Graphite			
0.4	0.32	10/pk	5188-5315
0.4	0.53	10/pk	5188-5314

Straight Ferrules

Description	Unit	Part No.
1/4 in PTFE	10/pk	0100-1378
1/4 in Graphite	10/pk	0100-1324
1/8 in PTFE	10/pk	0100-1365
1/8 in Graphite	10/pk	0100-1325
1/8 in 85% Vespel/15% Graphite	10/pk	0100-1332
1/16 in PTFE	10/pk	0100-1375
1/16 in Graphite	10/pk	0100-1326
1/16 in VG-2 Vespel, 40% Graphite	10/pk	0100-1379
6.4 mm Vespel		0100-1104
1/4 in 85% Vespel/15% Graphite	10/pk	0100-1331



1/8 in 85% Vespel/15% Graphite, 0100-1332

Reducing Ferrules

Description	Unit	Part No.
1/8 to 1/16 in Vespel	10/pk	0100-1342
1/8 to 1/16 in VG-1 Vespel, 15% Graphite	10/pk	0100-1344
1/16 in to 0.4 mm VG-2 Vespel, 40% Graphite	10/pk	0100-1381

Ferrules for LTM Rapid Heating/Cooling System

Description	Original Design (5/pk)	2010+ Siltite/ Ultimate Union (10/pk)
For use with 0.25-0.4 mm id LTM columns	5190-1437	5188-5361
For use with 0.4-0.5 mm id LTM columns	5190-1438	5188-5362
For use with 0.5-0.8 mm id LTM columns	5190-1439	5188-5363

Ferrules and Nuts for NCD and SCD

Description	Part No.
Spare column nut and ferrule kit	G6600-80018

Capillary Flow Technology Supplies

Agilent offers a family of GC accessories based on our proprietary Capillary Flow Technology. These accessories increase system productivity and performance:

- Deans Switch device simplifies the analysis of complex samples
- Purged Effluent Splitter for inert, leak-free column effluent splitting



Ultimate Union

Ultimate Union

The Ultimate Union is part of Agilent's Capillary Flow Technology family, providing extremely low dead volume column connections. Like the QuickSwap, Deans Switch and Purged Effluent Splitter, the Ultimate Union uses special fittings and SilTite ferrules to create an inert, leak-free and robust seal that doesn't need re-tightening after temperature cycles.

Each Agilent Ultimate Union kit contains:

- 1 Union (your choice of deactivated or non-deactivated)
- 2 Internal nuts
- 1 Swaging nut
- 1 Oven wall clip

Ultimate Union Kits, Fittings and Ferrules

Description	Part No.
Ultimate union kit, deactivated	G3182-61580
Ultimate union kit, non-deactivated	G3182-61581

Fittings, Ferrules and Supplies

For leak-free, low dead volume and inert column connections with capillary flow accessories, such as the Deans Switch or QuickSwap MS Interface, use SilTite ferrules and specified nuts. For Capillary Flow devices, use deactivated fused silica tubing. Do not use tubing that has been coated with stationary phase.

Fittings, Ferrules and Supplies

Description	Unit	Part No.
Internal nut		G2855-20530
Swaging nut		G2855-20555
Tee, inert		G3184-60065
Column storage fitting		G2855-20590
SilTite metal ferrules, 0.10-0.25 mm id capillary columns	10/pk	5188-5361
SilTite metal ferrules, 0.32 mm id capillary columns	10/pk	5188-5362
SilTite metal ferrules, 0.53 mm id capillary columns	10/pk	5188-5363
Ferrule pre-swaging tool		G2855-60200



Internal nut, G2855-20530



Tee, inert, G3184-60065

Column/Retention Gap Installation Supplies

Description	Part No.
250 µm retention gap, one 5 m piece	160-2255-5
320 µm retention gap, one 5 m piece	160-2325-5
530 µm retention gap, 5 m length	160-2535-5
Fused silica, deactivated, 0.15 mm x 1 m	160-2625-1
Fused silica, deactivated, 0.15 mm x 5 m	160-2625-5
Fused silica, deactivated, 0.15 mm x 10 m	160-2625-10

Press-fit Capillary Column Connectors



Glass press-fit connections

In the past it was necessary to use press-fit connectors with specific dimensions to connect columns of those dimensions. Modern press-fit connectors are "laser-milled" to provide highly reproducible taper angles throughout the length of the press-fit, ensuring an excellent seal. Now the only choice you have to make is between a glass union for standard applications, and fused silica unions or deactivated quartz unions for applications demanding maximum inertness.

Glass and Fused Silica Press-fit Connectors

Description	Unit	Part No.
Glass union, universal, 2-way	25/pk	705-0825
Fused silica union, universal, 2-way	5/pk	705-0905
Fused silica union, universal, 2-way	25/pk	705-0925
Fused silica union, universal, 3-way		705-0903
Polymide sealing resin, 5 g		500-1200



Quartz splitter

Quartz Press-fit Connectors/Splitters

Description	Unit	Part No.
Quartz column connector, 0.1 to 0.53 mm	5/pk	5181-3395
Deactivated quartz column connector	5/pk	5181-3396
Quartz splitter		5181-3397
Quartz deactivated splitter		5181-3398

Graphpak Capillary Column Connectors (2.5 mm)*

Column ID (mm)	Connector ID (mm)	Part No.
Capillary Detector Port Connector		
0.32/0.25	0.4	5021-7166
0.53	0.7	5021-7164
Capillary Divider for Simultaneous Sampling		
0.32/0.25	0.53	5021-7148
0.53	0.7	5021-7146
Capillary Injection Port Connector		
0.2	0.3	5021-7169
0.32/0.25	0.4	5021-7170
0.53	0.7	5021-7168

*The 2.5 mm Graphpak is not compatible with the Graphpak 2M used for the PTV.



Graphpak connector for Agilent capillary detectors



Graphpak divider for simultaneous sampling

Note: Order ferrules in addition to the connector to fit your column. Ferrules must be ordered separately.

Ferrules for Connectors

Column ID (mm)	ID (mm)	Unit	Part No.
0.2	0.3	10/pk	5021-7136
0.32/0.25	0.4	10/pk	5021-7137
0.53	0.7	10/pk	5021-7134
Graphpak plug ferrule		10/pk	5021-7133
Replacement Graphpak column nut		5/pk	5062-3525



Capillary injection port connector, 5021-7170

Valves and Loops



General purpose gas sampling valves

Gas Sampling General Purpose Valves

Description	Part No.
6-port replacement valve WE series, 400 psi, 225 °C	5062-9508
6-port replacement valve WE series, Hastelloy C, 400 psi, 225 °C	5062-9509
10-port replacement valve WE series, 400 psi, 225 °C	5062-9510
10-port replacement valve WE series, Hastelloy C, 400 psi, 225 °C	5062-9511
6-port replacement valve WT series, 300 psi, 350 °C	0101-0584
10-port replacement valve WT series, 300 psi, 350 °C	0101-0585



General purpose liquid sampling valves

Liquid Sampling General Purpose Valves

Description	Part No.
0.2 µL replacement valve UWP series, 1,000 psi, 175 °C	0101-0636
0.5 µL replacement valve UWP series, 1,000 psi, 175 °C	0101-0637
1.0 µL replacement valve UWP series, 1,000 psi, 175 °C	0101-0638
0.5 µL replacement valve UWP series, 5,000 psi, 75 °C	0101-0639

Replacement Rotors for Gas Sampling Valves

Description	Part No.
6-port replacement rotor WE series, 400 psi, 225 °C	5181-7459
10-port replacement rotor WE series, 400 psi, 225 °C	5181-7460
6-port valve, replacement rotor, WT series, 300 psi, 350 °C	1535-4952
10-port replacement rotor WT series, 300 psi, 350 °C	1535-4954

Valve Supplies


Description	Part No.
1/16 in stainless steel nut	5181-1291
1/16 in front ferrule, stainless steel	5181-1292
Straight metering valve, 1/16 in, stainless steel, for LSVs as a sample-out restrictor or as a flow-balancer for 10-100 mL/min	0101-0355
Micrometering valve, for flow balancing gas flows of 2-50 mL/min	0101-0633
Air actuator	19325-60660
Angle metering valve, 1/16 in, stainless steel	0101-0403
7 µm gas line filter	0101-0532




Front ferrules, stainless steel, 5181-1292

Valve Column Connections

Description	Part No.
1/16 in Tube Assembly, inert (50 cm, 0.010 in id)	G1580-60060
1/16 in Tube Assembly, non-inert (50 cm, 0.010 in id)	G1580-80060
1/16 in Tube Assembly, inert (50 cm, 0.020 in id)	G1580-60062
1/16 in Tube Assembly, non-inert (50 cm, 0.020 in id)	G1580-80062
Swaging nut	G2855-20555
Internal nut	G2855-20530
Hex nut, 5/16 in-20	2950-0232
Nut Plate Assembly	05890-80660
Ferrule pre-swaging tool	G2855-60200
SilTite metal ferrules, 0.10-0.25 mm id capillary columns	5188-5361
SilTite metal ferrules, 0.32 mm id capillary columns	5188-5362
SilTite metal ferrules, 0.53 mm id capillary columns	5188-5363

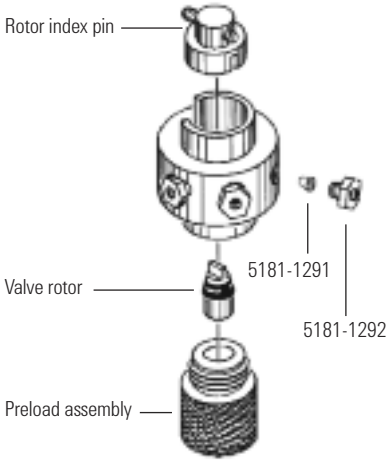

Valve body, disassembled

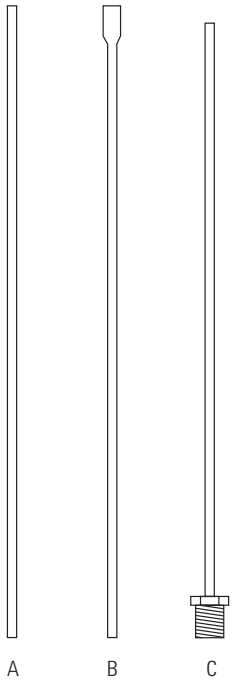

Valve Loops for GC
(Includes loop, nut and ferrule, 1/16 in)

Description	Part No.
Sample loop, 0.25 cc	0101-0303
Sample loop, 0.50 cc	0101-0282
Sample loop, 1.00 cc	0101-0299
Sample loop, 2.00 cc	0101-0300
Sample loop, 5.00 cc	0101-0301
Sample loop, 10.00 cc	0101-0302

Valve Supplies for GC

Description	Part No.
A. Tube, 1/16 in stainless steel, 280 mm long	18900-20250
Tube, 1/16 in stainless steel, 400 mm long	18900-20280
Tube, 1/16 in stainless steel, 375 mm long	18900-20281
Tube, 1/16 in stainless steel, 560 mm long	18900-20300
B. Tube, 1/16 in with 1/8 in flare, stainless steel, 360 mm long	1530-2163
Tube, 1/16 in with 1/8 in flare, stainless steel, 520 mm long	1530-2167
C. Tube, 1/16 in with 1/8 in bulkhead fitting, 520 mm long	07675-80050
Tube, 1/16 in with 1/8 in bulkhead fitting, nickel, 460 mm long	18900-80255

Sample Introduction Systems

7693A Automatic Liquid Sampler Replacement Parts and Supplies

To support the higher productivity, performance, and flexibility offered by the 7693A ALS, Agilent has expanded its supplies offering. Agilent Blue Line autosampler syringes are specifically designed to support the 7693A, while increasing plunger life and reducing costly downtime. For cost-conscious laboratories, economical shell vials and caps provide quality at an attractive price. Additional accessories, such as color-coded sample trays and vial caps, add to system ease-of-use.



7693A Automatic Liquid Sampler

7693A Replacement Parts and Supplies

Description	Unit	Part No.
Gripper finger caps	16/pk	G4514-60710
Injector mounting post		G4513-20561
Dual parking post for autosampler		05890-61525
Needle support insert, standard		G4513-40525
Needle support insert, on-column		G4513-40529
Vial rack, set of 3, Includes 3 white label tags		G4514-67505
Vial rack label kit		G4525-60701
Vial rack label kit, red	3/pk	G4525-60702
Vial rack label kit, yellow	3/pk	G4525-60703
Vial rack label kit, green	3/pk	G4525-60704

Wash Vials (also for standards, diluents)

Description	Unit	Part No.
4 mL wash vials with fill markings and caps	25/pk	5182-0551
Diffusion caps for 4 mL vials	12/pk	07673-40180
Septa for 4 mL vials*	144/pk	9301-1031
4 mL wash vial with screw caps	144/pk	9301-0723

*Septa for 4 mL vials should only be used for sample storage

Automatic Liquid Sampler Supplies

Automatic Liquid Sampler Supplies

Description	Part No.
Screw for mounting syringe	07673-20570
Quadrant tray (4 tray sections)	18596-40015
7673 Basic Supply Kit Contains 10 µL syringes (6/ea), 23/26 gauge needles, 4 mL vials with diffusion caps (144/pk), 2 mL automatic sampler vials with screw caps (1,000/pk), GC septa (25/pk), vial racks (5/pk)	07673-60840

Bar Code Reader Labels

Description	Part No.
Labels numbered (1,000/roll)	
1 to 1,000	5958-9450
1,001 to 2,000	5958-9441
2,001 to 3,000	5958-9442
3,001 to 4,000	5958-9443
4,001 to 5,000	5958-9444
5,001 to 6,000	5958-9445



7697A Headspace Sampler Supplies

The new 7697A Headspace Sampler from Agilent utilizes advanced designs based on our industry-leading gas chromatography architecture. The headspace sampling technique allows introduction of volatile compounds to the GC or GC/MS from virtually any sample matrix, while leaving unwanted components in a disposable sample vial. With up to 111 sample vial positions and removable vial racks, the 7697A supports nearly continuous operation to satisfy even the busiest laboratory.

- Built-in legendary Agilent pneumatics for superior control and easier setup
- Proven valve and loop sampling technology
- Fully-automatic sample vial leak checking and available bar code reader help ensure greater confidence in results method compatibility
- Instrument control software that is fully integrated in Agilent data systems
- Resource conserving programmable instrument scheduler



7697A Headspace Sampler

7697A Headspace Replacement Parts and Supplies

Description	Part No.
Tray vial racks	G4556-60019
Vial rack label	G4556-90500
Universal/external split vent trap with 3 cartridges, 1/8 in Swagelok fitting	RDT-1020
Leak test kit Includes instruction sheet, no-hole ferrule, 1/8 in nylon tube fitting plug, headspace leak test vial, 1/16 in stainless steel ZDV plug, 11 mm low bleed septa (5/pk)	G4556-67010
Sample probe, deactivated SN 1030	G4556-60690
Sample probe, deactivated SN 2000	G4556-60125
6-port valve, replacement rotor, WT series, 300 psi, 350 °C	1535-4952

TIPS & TOOLS

The transfer line heater assembly is 1 m in length and accommodates the following tubing types:

- Fused silica capillary of 0.25 mm, 0.32 mm, and 0.53 mm id with maximum od of 0.67 mm
- Metal capillary of 0.53 mm id, such as Agilent UltiMetal or ProSteel, with maximum od of 0.67 mm

For one transfer line, a piece of fused silica or ProSteel approximately 1 m in length is required in addition to one ferrule and one nut and reducing union. Order a ProSteel sleeve to protect the transfer line when operating above 200 °C. ProSteel operated above 200 °C in the transfer line without the sleeve can permanently bind to the heated conduit tube.



7697A Headspace Sampler

7697A Headspace Replacement Parts and Supplies

Description	Part No.
Tray vial racks	G4556-60019
Vial rack label	G4556-90500
Universal/external split vent trap with 3 cartridges, 1/8 in Swagelok fitting	RDT-1020
Leak test kit Includes instruction sheet, no-hole ferrule, 1/8 in nylon tube fitting plug, headspace leak test vial, 1/16 in stainless steel ZDV plug, 11 mm low bleed septa (5/pk)	G4556-67010
Sample probe, deactivated SN 1030	G4556-60690
Sample probe, deactivated SN 2000	G4556-60125
6-port valve, replacement rotor, WT series, 300 psi, 350 °C	1535-4952
Transfer Line Components	
Deactivated fused silica, 5 m length	
0.25 mm	160-2255-5
0.32 mm	160-2325-5
0.45 mm	160-2455-5
0.53 mm	160-2535-5
ProSteel deactivated stainless steel, 5 m length	
0.53 mm	160-4535-5
Polyimide sleeve for ProSteel	4177-0607
Polyimide, Valcon ferrule, 5/pk	
Ferrule, low thermal mass, column id 320 µm, 0.5 mm id, 5/pk	5190-1438
Ferrule, low thermal mass, column id up to 250 µm, 0.4 mm id, 5/pk	5190-1437
Nut and reducing union for 6 port valve and transfer line connection	0100-2594
Septum nut, transfer line, split/splitless and multimode inlets	G3452-60835

G3520A XLSI Accessory Supplies

Description	Part No.
G3520A XLSI Accessory kit	G3520-67001
Ceramic wafer column cutter	5181-8836
Transfer line nut fitting	G3520-20210
Column storage fitting	G2855-20590
Magnifier, 3x, 6x, paddle, plastic	G2855-40001
Plug for microfluidic manifold or unions	G2855-60570
Ferrule pre-swaging tool	G2855-60200

Sampling Loops

Description	Part No.
Sampling Loops, SN 2000	
Sample loop, 0.025 mL	G4556-80101
Sample loop, 0.05 mL	G4556-80102
Sample loop, 0.10 mL	G4556-80103
Sample loop, 0.50 mL	G4556-80105
Sample loop, 1.00 mL	G4556-80106
Sample loop, 5.00 mL	G4556-80109
Sample loop, 3.00 mL	G4556-80108
Certified Sample Loops*	
Certified sample loop, 1.00 mL	G4556-80126
Certified sample loop, 3.00 mL	G4556-80128
Sampling Loops, SN 1030	
Sample loop, 0.025 mL	G4556-80111
Sample loop, 0.05 mL	G4556-80112
Sample loop, 0.10 mL	G4556-80113
Sample loop, 0.50 mL	G4556-80115
Sample loop, 1.00 mL	G4556-80116
Sample loop, 3.00 mL	G4556-80118
Sample loop, 5.00 mL	G4556-80119

*Certified sample loops are validated by Micro Precision Calibration, Inc and come with a calibration certificate. Loops can be recertified yearly by contacting Micro Precision directly at +1 (530) 268 1860.

Vials and Caps for 7697A

Description	Unit	Part No.
Vial kit 20 mL Headspace crimp top, flat bottom vials, silver aluminum one-piece crimp caps with safety feature, PTFE/white silicone septa	100/pk	5182-0840
Headspace crimp top, flat bottom vials, 10 mL	100/pk	5182-0838
Headspace crimp top, flat bottom vials, 20 mL	100/pk	5182-0837
Silver aluminum crimp caps with 20 mm, PTFE/silicone septa	100/pk	5183-4477
20 mm electronic crimper		5062-0208
Ergonomic manual crimper for 20 mm caps		5040-4669



Certified headspace crimp top vials, 5182-0837



Aluminum crimp caps, 5183-4477



Manual crimper and decapper, 5040-4669



G1888A Network Headspace Sampler Supplies

Description	Part No.
Stainless Steel Sample Loops	
Certified sample loop, 1 mL, deactivated	5190-2265
Certified sample loop, 3 mL, deactivated	5190-2266
Sample loop, 1 mL, deactivated	2321700003
Sample loop, 3 mL, deactivated	2321700004
Probes and Unions	
Sample probe, deactivated	2322700011
M6 union, brass	2302533140
Union, zero dead volume, deactivated	2307230001
Union	2307232901
Transfer Line Needles and Unions	
Needle only, headspace transfer line, deactivated 0.5 mm od	2322590004
Needle only, headspace transfer line, deactivated 0.7 mm od	2322590005
Strain relief septum nut	6410090050
Tubing	
Tubing, solenoids to 6-port valve, deactivated	0410105017
Tubing, probe to 6-port valve, deactivated	1300502506
Standards	
OQ/PV Headspace Sample Contains 0.2-0.3% t-butyl disulfide, 1,2-dichlorobenzene, and nitrobenzene in ethanol	5182-9733
PM Kits	
G1888A PM kit with 1 mL loop	G1888-60702
G1888A PM kit with 3 mL loop	G1888-60703
G1888A enhanced PM kit	G1888-60704



G1888A Headspace unit

G1883A Network Headspace Supplies

Description	Part No.
Needles	
Needle only, headspace transfer line, deactivated 0.5 mm od	2322590004
Needle for transfer line, 0.25 mm id, 0.5 mm od, nickel	301-016-HSP
Needle only, headspace transfer line, deactivated 0.7 mm od	2322590005
Needle for transfer line, 0.4 mm id, 0.8 mm od, nickel	301-015-HSP
Needle assembly vial probe, deactivated	232-2790012-EHS
Needle assembly vial probe, nickel	232-2790010-EHS
Fittings	
Union elbow M5	998-0000053-EHS
Transfer line nut	19258-20830
Transfer line ferrule	19258-20870
Union FF 6MB, 5-piece set	325-062-HSP
Union T6 MB, 5-piece set, brass	325-132-HSP
Union T5 MA	325-185-HSP
Valves	
Restrictor, stainless steel	321-002-HSP
Valve, solenoid vent Kalrez	3600500001
Valve, solenoid vial pressurization	3600500002
Tubing and Transfer Lines	
Sample loop, 1 mL, deactivated	2321700003
Sample loop, 1 mL, nickel	321-055-HSP
Sample loop, 3 mL, deactivated	2321700004
Sample loop, 3 mL, nickel	321-056-HSP
Oven adaptor for 10 mL vials	301-017-HSP
Tube, needle, 6-port valve, deactivated	301-212-HSP
Tube, needle, 6-port valve, nickel	301-169-HSP
Tube, vent-valve stainless steel	301-170-HSP
Sensor tube, 125 mm PTFE	321-057-HSP
Transfer line, deactivated, 1 m	301-211-HSP
Transfer line, 1 m, nickel	301-152-HSP
Transfer line, 80 cm, nickel	301-011-HSP
Repair, Leak Test, and OQ/PV Supplies	
Strain relief septum nut	301-205-HSP
Headspace leak test kit	G1888-60701
OQ/PV Headspace Sample	5182-9733

Teledyne Tekmar Purge and Trap Supplies



Stratum PTC Sample Concentrator

Glassware for Teledyne Tekmar Purge and Trap Concentrators, 1/2 in Mount

Description	Part No.
5 mL frit sparger (glassware only)	5182-0852
5 mL frit sparger kit with fittings	5182-0846
25 mL frit sparger (glassware only)	5182-0851
25 mL frit sparger kit with fittings	5182-0845
5 mL fritless sparger (glassware only)	5182-0850
5 mL fritless sparger kit with fittings	5182-0844
25 mL fritless sparger (glassware only)	5182-0849
25 mL fritless sparger kit with fittings	5182-0796
5 mL needle sparger (glassware only)	5182-0848
5 mL needle sparger kit	5182-0795
25 mL needle sparger (glassware only)	5182-0847
25 mL needle sparger kit	5182-0794

Traps for Teledyne Tekmar Stratum and Atomx Purge and Trap Concentrator

Description	Part No.
Trap, BTEX + MTBE	5188-8813
Trap #5, OV-1/Tenax/Silica Gel/Charcoal	5188-8814
Trap #8, Carbopak B/Carbosieve S-III	5188-8815
Trap #9, Proprietary	5188-8816
Trap, Tenax/Silica Gel/Carbosieve S-III	5188-8817
Strat-Trap, Tenax/Silica Gel, #2	5188-8818
Strat-Trap, Tenax/Silica Gel/Charcoal, #3	5188-8819
Strat-Trap, OV-1/Tenax, #7	5190-1445
Strat-Trap, Tenax, #1	5190-1446
Trap, VOCARB 3000	5188-8820
Trap, VOCARB 4000	5188-8821
Trap, BTEX	5188-8822
Trap, Tenax	5188-1447
Trap, VPH	5188-1448

Stratum and Atomx traps are U-shaped



Trap, BTEX + MTBE, 5188-8813

Atomx VOC Autosampler Supplies

Description	Part No.
Antifoam agent, Antifoam 1520, 10 mL	5190-2235
Syringe with side port, 27 mL	5190-2234
Vessel, amber IS, 15 mL	5190-2233
Frit sparge glassware kit, 25 mL	5190-2232
Fritless sparge glassware kit, 25 mL	5190-2231



Atomx Purge and Trap Concentrator

Traps for Teledyne Tekmar Velocity Purge and Trap Concentrator

Description	Part No.
Trap, Vocarb 3000 (K Trap)	5182-0775
Trap, Vocarb 4000 (I Trap)	5182-0774
Trap, Tenax (A Trap)	5182-0783
Trap, Tenax/Silica Gel/Charcoal (C Trap)	5182-0781
Trap, BTEX	5182-0773
DryFlow moisture trap	14-8911-003

Velocity traps are straight

TIPS & TOOLS

Compared to a frit sparger, the fritless sparger may be the better choice when a water sample has a tendency to foam. This sparger is not appropriate for soil samples, which tend to clog the capillary tube.



Agilent ARCHON Purge and Trap Autosampler



Agilent ARCHON Purge and Trap Autosampler with removable tray



ARCHON removable 51 position sample tray

Archon Purge and Trap Supplies

Description	Part No.
Vial kit, 40 mL, precleaned vials, caps, and septa, 72/pk	5183-4741
Bottle without cap, 80 oz.	DY50390600
22 mm septa, PTFE/silicone, 72/pk	5190-3978
22 mm septa, EPA lowbleed, 60/pk	5190-3976
Syringe mount O-ring	DY50549500
Water probe replacement kit, for S/N above 995	DY50573990
Sparge probe replacement kit, for S/N above 13160	DY70007791
Sparge probe replacement kit, for S/N 995-13160	DY50574190
Sparge probe replacement kit, for S/N below 995	DY50549290
Standard reservoir	DY50548400
Water transfer line	DY50551400
I.S. pickup/waste lines	DY70001990
Soil transfer line	DY50574500
75-micron screen for water probe	DY50559800
Water probe, cleaned, for S/N 695-995	DY50549100
Sparge probe cleaned, for S/N above 13160	DY70007701
10-micron soil probe frit	DY50559900
Valco rotor loop, 1 µL	DY50572600
Flangeless nuts and ferrules, 8/pk	DY70008101
PTFE stir bar for 40 mL vials	DY50295500
Spin bar for soil vial	DY50402400
Stir magnet	DY50546100
Valco valve and actuator	DY50540700
Glass barrel with decal, 26 mL	DY50296800
Kit, chiller option, field	DY70008590

Markes Thermal Desorption


Agilent now offers a comprehensive line of supplies for Markes Thermal Desorption (TD) instrumentation. Thermal desorption allows the introduction of volatile and semivolatile compounds from a wide range of sample matrices, directly into a GC or GC/MS.



Markes Thermal Desorption system



Sampling tube, MKI-UTD-5105



Silcosteel Difflok cap, MKI-MTD-1204

Markes Thermal Desorption Supplies

Description	Unit	Part No.
O-rings, Markes 7 mm cold trap seals	10/pk	MKI-U-COV07
O-rings, Markes 6 mm cold trap seals	10/pk	MKI-U-COV06
PTFE filter disks, 5.1 mm Markes TD	10/pk	MKI-U-DISK1
PTFE filter disks, 6.3 mm Markes TD	10/pk	MKI-U-DISK3
Spare general purpose carbon cold trap		MKI-U-T11GPC
Sampling tube, Tenax TA, Markes Unity		MKI-UTD-5105
Quick fit connectors, Markes Unity	10/pk	MKI-C-QSC10
Stainless steel Difflok cap, Markes Unity	10/pk	MKI-MTD-1169
Silcosteel Difflok cap, Markes Unity	10/pk	MKI-MTD-1204
O-ring insertion tool, Markes Unity TDI		MKI-Z-0285
O-ring extraction tool, Markes Unity TDI		MKI-Z-0351
Cold trap alignment tool, Markes Unity		MKI-UTD-5064
Cold trap, air toxics, C_2-C_{14}, Unity 2		MKI-U-T3ATX-2S
Cold trap, air toxics, C_2-C_{14}, Unity		MKI-U-T3ATX
Cold trap, materials emissions, Unity		MKI-U-T12ME
Cold trap, GP Carbon, $C_{4/5}$-$C_{30/32}$, Unity 2		MKI-U-T11GPC-2S
O-rings, 010 Markes Unity	10/pk	MKI-U-COV10
Cold trap, materials emissions, Unity 2		MKI-U-T12ME-2S
Empty stainless steel TD tubes	10/pk	C-TBE10
Tenax stainless steel tubes, preconditioned/capped	10/pk	C-TBP1TC
Empty glass TD tubes	10/pk	C-GT010
PTFE inserts	10/pk	C-PL010
Long term TD tube storage caps	10/pk	C-CF020
Cap-LOK Tool for long term storage caps		C-CPLOK
Diffusive sampling caps	10/pk	C-DF010
Bio-VOC breath samplers	10/pk	C-BIO10
Disposable card mouth piece for Bio-VOC	10/pk	C-B010M
Tenax TA 34-60 Mesh, 10 g		C-TNXTA

(Continued)



Markes Thermal Desorption system

Markes Thermal Desorption Supplies

Description	Unit	Part No.
General purpose hydrophobic tubes, stainless steel Preconditioned and capped with 1/4 in brass storage caps. For pumped sampling n-C_5 to n-C_{20}.	10/pk	C-HY010C
Tenax/S'carb 'Sulphur' tubes Preconditioned and capped with 1/4 in brass storage caps. For odor and landfill gas analysis.	10/pk	C-102SSC
Carbograph 1 stainless steel tubes Preconditioned and capped with 1/4 in brass storage caps. For pumped sampling C_5 to C_{14}, plus diffusion of BTX.	10/pk	C-TBP1C1C
Carb X stainless steel tubes Preconditioned and capped with 1/4 in brass storage caps. For pumped/diffusion of 1.3-butadiene & benzene.	10/pk	C-TBP1CXC
Air toxics (TO-17) stainless steel tubes Preconditioned and capped with 1/4 in brass storage caps. For pumped sampling VOCs n-C_3 to n-C_{12}.	10/pk	C-AT010C
Universal stainless steel tubes Preconditioned and capped with 1/4 in brass storage caps	10/pk	C-UN010C
Glass tubes with 1 cm Tenax For direct liquid injection	10/pk	C-G1CM10
Glass air toxics (TO-17) tubes Pre-packed with 2 carbon-based sorbents; preconditioned and capped with 1/4 in brass storage caps	10/pk	C-GAT010C
CRS BTX Standards, 1 µg	10/pk	C-BTX1UG

Inlet Systems

Agilent Inlet Convenience Kits

Convenience kits are an easy way to get all the supplies you need using one part number. Agilent's new preventative maintenance kits include septa, liners, O-rings, gold seals and traps.



QuickPick Splitless PM Kit, 5188-6497



QuickPick Purged Packed PM Kit, 5188-6498



Split Vent Trap PM Kit, 5188-6495

Agilent Inlet Convenience Kits

Description	Part No.
QuickPick Split Inlet PM Kit Includes 5 non-stick BTO septa, 1 split liner, 1 non-stick liner O-ring, and inlet gold seal kit	5188-6493
QuickPick Split Vent and Inlet PM Kit Includes 5 non-stick BTO septa, 1 split liner, 1 non-stick liner O-ring, inlet gold seal kit, and split vent trap with 2 O-rings	5188-6496
QuickPick Splitless Inlet PM Kit Includes 5 non-stick BTO septa, 1 splitless liner, 1 non-stick liner O-ring, and inlet gold seal kit	5188-6494
QuickPick Splitless Vent and Inlet PM Kit Includes 5 non-stick BTO septa, 1 splitless liner, 1 non-stick liner O-ring, inlet gold seal kit, and split vent trap with 2 O-rings	5188-6497
QuickPick Purged Packed Inlet PM Kit Includes 5 non-stick BTO septa, 1 O-ring, 1 ferrule, and 1 disposable glass liner	5188-6498
Internal split vent trap PM kit for split/splitless, volatiles, and PTV septumless inlet split vent line Includes 1 cartridge and 2 O-rings	5188-6495

Split/Splitless Inlet Seals

To ensure that you have a consistent and inert surface to properly seal the inlet and prevent sample degradation, Agilent has revolutionized production of the gold inlet seal. Unlike traditional machined seals, the new format Agilent Gold Inlet Seal has a very reproducible smooth surface, eliminating traces of machining grooves that can be the source of minute leaks. With Agilent's proprietary metal injection molding (MIM) manufacturing process, every gold inlet seal provides a high quality, leak-free seal so critical for reproducible results.

Our new package keeps the gold seal clean and scratch-free. For your added convenience, an inlet washer is provided with each inlet seal.



Gold plated seal kit, 5188-5367



Certified gold plated seal kit, 5190-2209

Split/Splitless Inlet Seals

Description	Unit	Part No.
Certified gold plated seal kit, includes washer		5188-5367
	10/pk	5190-2209
Gold plated seal with cross*		5182-9652
Stainless steel seal		18740-20880

*Use with total flow rates above 200 mL/min

Flip Top Inlet Sealing System

Agilent's Flip Top Inlet Sealing System is the faster, smarter way to change inlet liners on Agilent 6890, 6850 and 5890 GC systems.

- Cuts liner replacement time to as little as 30 seconds
- Eliminates frustrating searches for special wrenches or tools
- Improves inlet ergonomics – no more handling of heated parts, no more burns or scrapes
- Decreases downtime and increases productivity
- Minimizes exposure to ambient air, extending column life
- Easily installed by user in 15 minutes

Available exclusively from Agilent, the Flip Top has a levered arm that attaches to any 6890/6850/5890 insert weldment and locks to the injection port using an adapter ring screwed onto the inlet. Once installed, simply lift the arm of the Flip Top which releases the insert weldment from the injection port, and allows instant access to the liner. The process is simply reversed to reseal the weldment to the port.





Flip Top Inlet Sealing System

Description	Unit	Part No.
Flip Top Inlet Sealing System For 6890, 6850, 5890 only; not compatible with 7890		5188-2717
Non-stick fluorocarbon liner O-ring for Flip Top	10/pk	5188-5366
	100/pk	5190-2268



Flip Top Inlet Sealing System installation kit, 5188-2717

Split/Splitless Inlets

The combined split/splitless inlet is the most popular inlet for capillary column gas chromatography. Because it can be used in either split or splitless mode, it provides a very effective combination that can cover most analysis requirements.

Split Inlet Troubleshooting

Split inlets are spared from most band-broadening phenomena, since the splitting process generates narrow peaks. Peak broadening or tailing is usually due to:

- Improper column installation
- Low inlet temperature
- Low split flow (<20 mL/min on 6890)
- Inlet and needle discrimination and decomposition

If your results are inaccurate or inconsistent:

- Check the column and reinstall if necessary
- Increase inlet temperature by 50 °C and compare results
- Check inlets and needles for wear and replace as necessary

Splitless Inlet Troubleshooting

Most problems encountered with a splitless injection are related to:

- Incorrect purge time
- Degradation
- Improper focusing
- Inappropriate column temperature
- Backflash


You can also improve the reproducibility and linearity of peak areas and avoid backflash by matching:

- Inlet temperature
- Liner volume
- Injection volume

Decomposition

Loss of peak area or generation of new peaks can sometimes be dramatically reduced by changing liner type or by deactivating the liner and inlet with silanizing reagents. Removing or reducing the amount of liner packing can also decrease inlet activity.

Column Troubleshooting




Normal Peaks

Correct column positioning in both injection port and FID



Tailing Solvent Peaks

Column positioned incorrectly in the injection port or possible ferrule particle in the carrier gas flow path



Wrong Peak Ratios

Column positioned in the inlet (either too far or not far enough; verify 4-6 mm installation distance)

For the most reproducible split injection results, try Agilent's low pressure drop split liner (part number 5183-4647), with built in positioning bead, tight dimension tolerances, glass wool placement, and proprietary deactivation.


Split Mode Variables, Practices and Rationales

Parameter	Selection/Setting	Rationale
Inlet temperature	Try 250 °C or BP of last eluting compound	Ensures flash vaporization Minimizes inlet discrimination
Inlet liner	Large volume, deactivated	Minimizes backflash Minimizes degradation
Inlet packing	Silanized glass wool	Retains non-volatiles Minimizes inlet discrimination
	Glass beads or frit None	Less active than wool Least active
Injection volume	0.5-3 µL liquid 0.10-10 mL gas	Split easily adjusted Split adjusted accordingly
Injection technique	Fast autoinjection Hot-needle fast manual injection	Less needle discrimination Reproducible discrimination
Split ratio	50:1 to 500:1	Depends on sample and injection volume, and column id
Initial column temperatures	Not critical	Narrow initial peaks
Septum purge	2-3 mL/min	Minimizes ghosting

Splitless Mode Variables, Practices and Rationales

Parameter	Selection/Setting	Rationale
Inlet temperature	Just above highest boiling point of solutes (+20 °C)	Ensures flash vaporization Reduce if degradation occurs Use higher for dirty samples and higher-boiling solutes
Inlet liner	Large volume > 0.8 mL Small volume < 0.2 mL	Use with autoinjector Use only for slow manual injections and gas injections
Inlet packing	None	Use only with slow injection Decreases degradation
	Silanized glass wool	Use for fast autoinjection and dirty samples
Injection volume	0.5-2 µL liquid	Depends on solvent, liner and conditions
Injection technique	Fast autoinjection Hot-needle slow manual Hot-needle fast manual	Most reproducible Less needle discrimination Inject 1-2 µL/sec if narrow liner is used and > 1 µL injection Use for < 1 µL injections
Purge flow	20-50 mL/min	Higher if using constant flow
Purge delay time	20-80 sec	Adjust according to column flow rate/liner type and sample conditions
Oven temperature	10-25 °C below solvent BP	Necessary for solvent focusing
Column flow	> 2 mL/min when possible	Clears inlet fast Reduces backflash and decomposition
Septum purge	2-3 mL/min	Reduces ghosting
Quantification	Internal standard External standard addition	Maximizes reproducibility Use only with constant injection volume
Retention gap	1-3 m, deactivated (1-2 m per µL injected)	Reduces peak distortion Promotes solvent and stationary phase focusing

Split/Splitless Inlet Maintenance

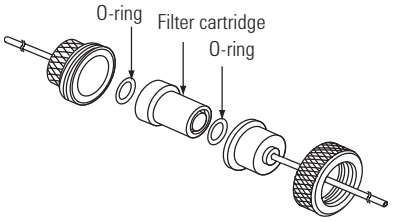

Split vent trap, 5188-6495


Changing the Split Vent Trap*

1. Remove the retaining clip.
2. Remove the old filter cartridge and two O-rings.
3. Verify the new O-rings are seated properly on the new filter cartridge.
4. Install the new filter cartridge then reassemble the trap. Do not fully tighten yet.
5. Place the filter trap assembly in the mounting bracket and install the retaining clip.
6. Fully tighten the split vent front weldment onto the trap.
7. Check for leaks.

*Change every 6 months


Installing a Capillary Column in a Split/Splitless Inlet

1. Prepare the column for installation.
2. Position the column so it extends 4 to 6 mm past the end of the ferrule.
3. Slide the septum to place the nut and ferrule in the correct position.
4. Insert the column in the inlet.
5. Slide the nut up the column to the inlet base and finger tighten the nut.
6. Adjust the column position so the septum is even with the bottom of the column nut.
7. Tighten the column nut an additional 1/4 to 1/2 turn. The column should not slide with a gentle tug.
8. Start carrier gas flow.
9. Verify flow by submerging the free end of the column in isopropanol. Look for bubbles.

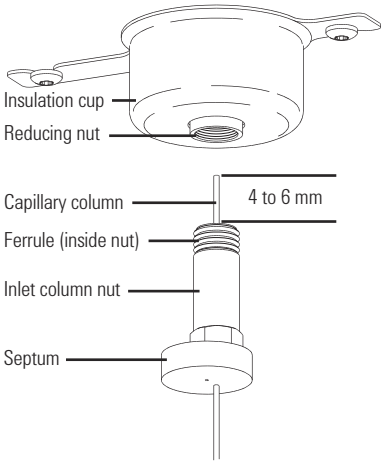

WARNINGS & CAUTION

The split vent trap may contain residual amounts of any samples or other chemicals you have injected into the GC. Follow your company's safety procedures for handling these types of substances while replacing the trap filter cartridge.

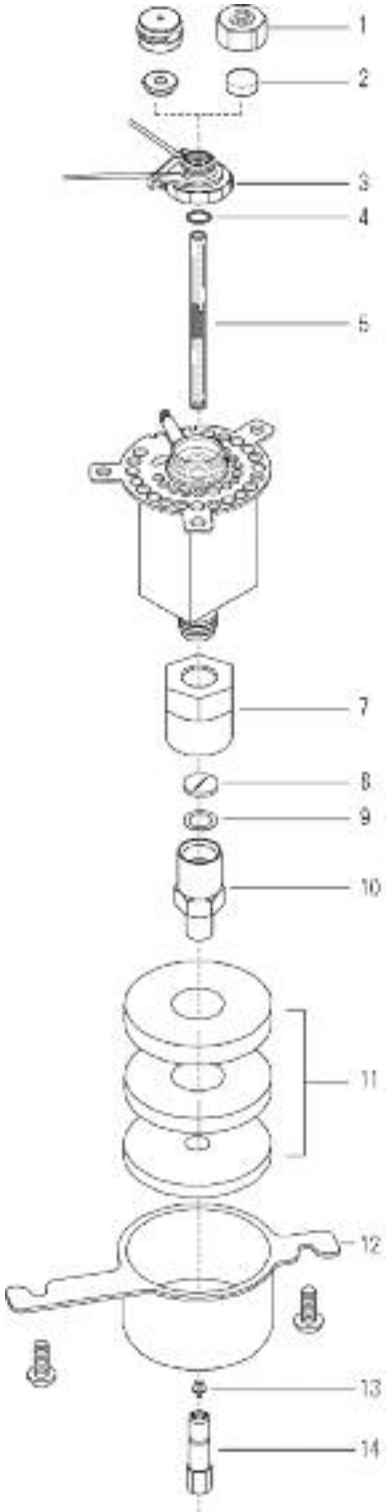

Split/Splitless Inlet assembly

7890/6890/6850 Split/Splitless Inlet Supplies

Item	Description	Unit	Part No.
	Low pressure drop, Ultra Inert Liner with glass wool		5190-2295
	Universal, low pressure drop, Ultra Inert Liner with glass wool		5190-3169
	Single taper, Ultra Inert Liner		5190-3166
	QuickPick Split Inlet PM Kit		5188-6493
	QuickPick Split Vent and Inlet PM Kit		5188-6496
	QuickPick Splitless Inlet PM Kit		5188-6494
	QuickPick Splitless Vent and Inlet PM Kit		5188-6497
1	Headspace septum retainer nut		18740-60830
	Septum retainer nut		18740-60835
	Strain relief septum nut		301-205-HSP
2	11 mm Certified BTO septa	50/pk	5183-4757
	For complete offering of premium septa, see page 15		
3	7890 Insert Weldment		
	Top insert weldment assembly, standard		G3452-60730
	Turn top		G3430-40035
	Split ring		0510-1306
	Top insert weldment assembly, headspace		G3452-60100
	Top insert, AC gang fitting weldment		G3430-60011
	Top insert assembly, valve		G3480-67585
	6890 Insert Weldment		
	S/SL insert weldment Used with large charcoal canister type filter, for 6890/6850		G1544-60585
	S/SL insert assembly for G1540A with valved system option This insert assembly uses the large charcoal canister split vent filter, for 6890/6850		G1580-60585
	Similar to G1544-60575 except carrier lines separated for interface to valved systems of a G1540A instrument		G1580-60575
	Original standard EPC using 1/4 in split vent filter		G1544-60575
	Similar to G1544-60575 except allows insertion of 1/4 in chemical filters to clean carrier gas for ECD operation		G1544-80580
	Insert Weldment Standard manual pneumatics		19251-60575
4	Certified non-stick fluorocarbon O-ring	10/pk	5188-5365
	Graphite O-ring for split liner	10/pk	5180-4168
	Graphite O-ring for splitless liner	10/pk	5180-4173
	Non-stick fluorocarbon liner O-ring for Flip Top	10/pk	5188-5366
5	Split liner, single taper, low pressure drop, glass wool	1/pk 25/pk	5183-4647 5183-4702
	Splitless liner, single taper, without glass wool	1/pk 25/pk	5181-3316 5183-4696
	For complete offering of liners, see pages 25		

(Continued)

7890/6890/6850 Split/Splitless Inlet Supplies

Item	Description	Unit	Part No.
6	Split vent trap kit		G1544-60610
	Replacement cartridge Includes 2 cartridges and 4 O-rings		G1544-80530
	Split vent trap PM kit Includes 1 cartridge and 2 O-rings		5188-6495
7	Retaining nut		G1544-20590
8	Stainless steel seal		18740-20880
	Certified gold plated seal kit, includes washer		5188-5367
	Gold plated seal with cross		5182-9652
9	Washers, 0.375 od	12/pk	5061-5869
10	Reducing nut		18740-20800
11	Insulation kit, 3 pieces		5188-5241
12	Lower insulation cover		19243-00070
13	Ferrules		
	For complete offering of ferrules, see pages 33-34		
14	Universal column nut	2/pk	5181-8830
	6850 column nut	2/pk	5183-4732
	Split/splitless septum nut angled wrench		19251-00100
	Flip Top Inlet Sealing System For 6890, 6850, 5890 only; not compatible with 7890		5188-2717
	Capillary Inlet Evaluation Sample (Split Mode)		8500-4789
	Capillary Inlet Supplies Kit, Includes:		5181-8838
	Certified gold plated seal kit, includes washer		5188-5367
	Liner, split, straight, glass wool, non-deactivated	4 each	19251-60540
	Liner, splitless, single-taper, glass wool, deactivated	2 each	5062-3587
	Certified non-stick fluorocarbon O-ring	10/pk*	5188-5365
	Liner, direct, 2 mm id, deactivated		5181-8818
	11 mm Certified BTO septa	50/pk*	5183-4757
	Capillary inlet cleaning wires	5/pk*	5180-4153

*Quantity when part ordered individually



Item 6, split vent trap, G1544-60610




Reducing nut, 18740-20800



Gold plated seal kit, 5188-5367

Gold seal on the split/splitless inlet

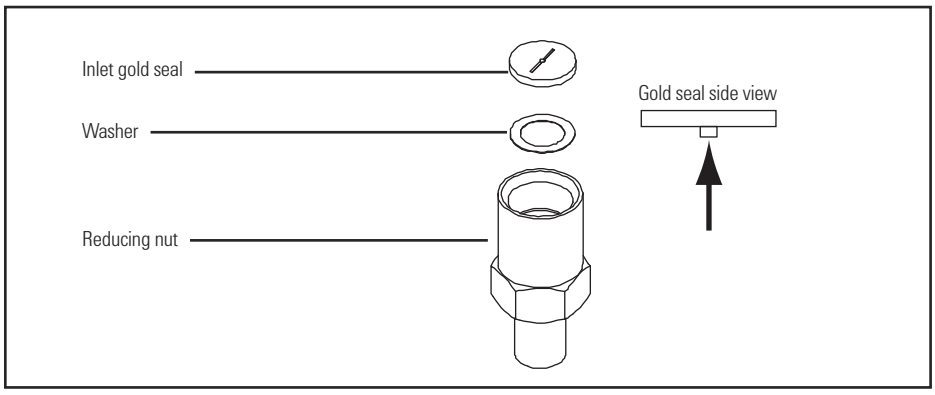


Multimode Inlet

Agilent's premium inlet – two inlets in one for maximum performance and flexibility for the 7890A

Whether you need to increase your system sensitivity with large volume injection capabilities, analyze thermally labile compounds or inject dirty samples, the Multimode Inlet delivers the performance and flexibility you need.

Multimode Inlet Body

Item	Description	Part No.
1	Merlin cap	5182-3445
2	Merlin Microseal	5182-3444
3	Septum retainer nut	18740-60835
4	11 mm Certified BTO septa 50/pk For complete offering of premium septa, turn to page 15.	5183-4757
5	Top insert assembly, standard	G3452-60730
6	Certified non-stick fluorocarbon O-ring	5188-5365
7	Dimpled splitless single taper, deactivated	5190-2296
8	Column nut adapter	G3510-20018
9	Foil (LN_2 only)	
10	Multimode Inlet insulation	19243-000681
11	Ferrule	For complete offering of ferrules, turn to pages 33-34.
12	MMI Metal Insulation Cup	G3431-00005

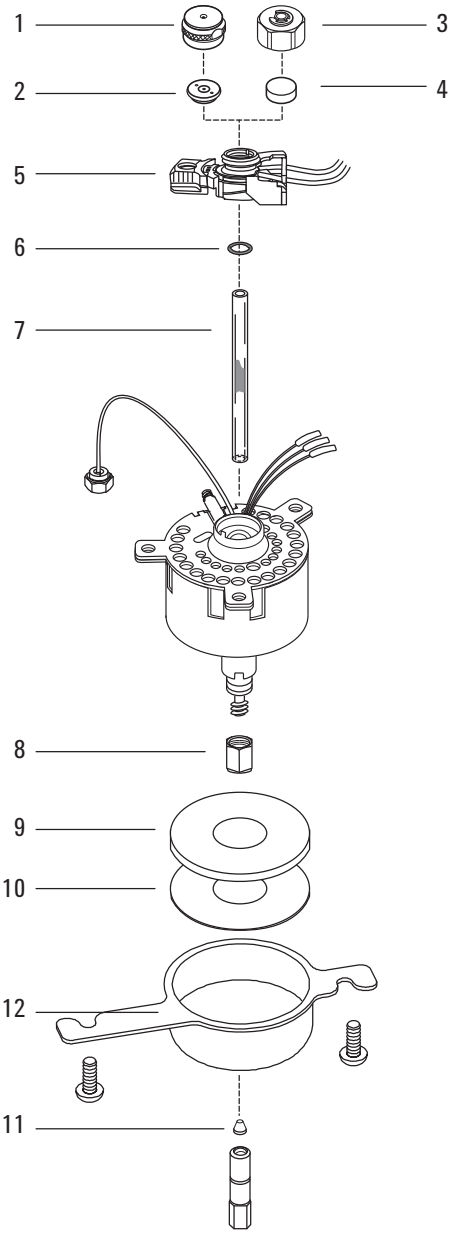

Exploded Parts View of the Multimode Inlet

TIPS & TOOLS


Because of the temperature programmability, graphite is preferred ferrule for the MMI. However, Graphite/Vespel ferrules can be used if they are temperature cycled and retightened. After the initial shrinkage, they do not show a detrimental leak for air.

Turn to pages 62-63.


Installing a Capillary Column in a Multimode Inlet

1. Prepare the column for installation.
2. Thread the column adapter nut onto the base of the inlet and make sure it can spin freely.
3. Place a septum, capillary nut, and graphite ferrule on the column.
4. Score and snap off the end of the column.
5. Position the column so it extends 10 to 12 mm past the end of the ferrule.
6. Slide the septum to place the nut and ferrule in the correct position.
7. Insert the column in the inlet.
8. While holding the adapter with a wrench thread the column nut into the inlet (but do not tighten).
9. Adjust the column position so that the septum contacts the bottom of the column nut. Finger-tighten the column nut until it begins to grip the column.
10. While holding the inlet base with one wrench, use the second wrench to tighten the column nut an additional 1/4 to 1/2 turn so that the column cannot be pulled from the fitting with gentle pressure.

Step 2

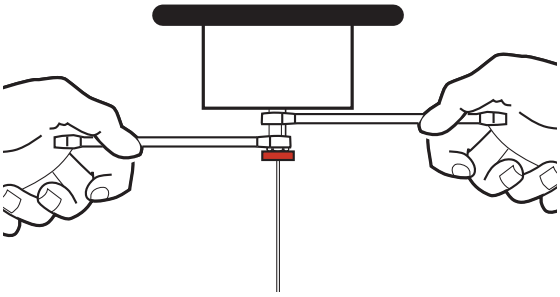

Step 5

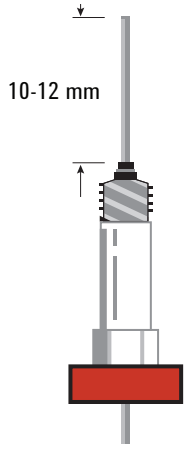

Cleaning the Multimode Inlet


Agilent recommends using the G3510-60820 Multimode Cleaning Kit, which ships with detailed cleaning instructions.

Depending on the inlet mode used, the liner installed, and the cleanliness of the sample, the frequency of cleaning may range from weekly to monthly. When establishing your cleaning frequency, start with a visual inspection of the inlet bottom whenever a liner is changed. A small ring of material will collect at the bottom of the inlet when dirty samples such as food extracts or solid waste extracts are injected. An initial cleaning schedule of every two weeks for dirty samples and every two months for clean samples is appropriate and can be adjusted subsequently.

WARNINGS & CAUTION

The inside of the wall of the inlet is only 0.005 in thick and can be damaged with hard scrubbing.

Cool On-Column Inlets

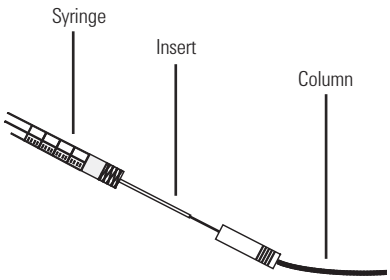

Cool On-Column Inlet Maintenance

Installing a Capillary Column into a Cool On-Column Inlet

1. Gently insert the column into the inlet until it bottoms.
2. Insert the column nut into the inlet fitting and finger tighten.
3. Tighten the column nut an additional 1/4 turn with a wrench or until the column does not move. Use two wrenches to support inlet (5/16 in and 1/4 in).
4. If using an automatic injection system with a 0.25 mm or 0.32 mm column, verify that the column installation by manually pushing the syringe into the inlet.

Checking the Needle-to-Column Size on the Cool On-Column Inlet


1. Check the needle-to-column size to make certain that the needle fits in the column.
2. Identify the correct insert for the column size. Use the insert that is the same size as the syringe needle to verify that the column you plan to use is the correct size.
3. Insert the column into one end of the insert.
4. Insert the syringe needle through the other end of the insert and into the column. If the needle cannot pass easily into the column, reverse the insert to try the needle and column in the other end.


Changing the Septum on the Cool On-Column Inlet

1. Replace the septum.

   If you are using a septum nut, grasp the knurling and unscrew. Remove the old septum with tweezers. Use tweezers to install a new septum. Push the septum into the septum nut until properly seated. Firmly tighten the nut.

   If you are using a cooling tower, grasp the three rings and unscrew. The spring and duck bill septum may pop out of the inlet when you remove the cooling tower. Be careful not to lose them. If they do not pop out, use a thin wire to remove them from the inlet. Insert the replacement duck bill septum into the spring and place in the inlet. Reattach the cooling tower assembly, then finger tighten.
2. Before making an injection, check the alignment of the entire assembly using the proper size syringe.
3. Restore the analytical method.
4. Reset the septum counter.

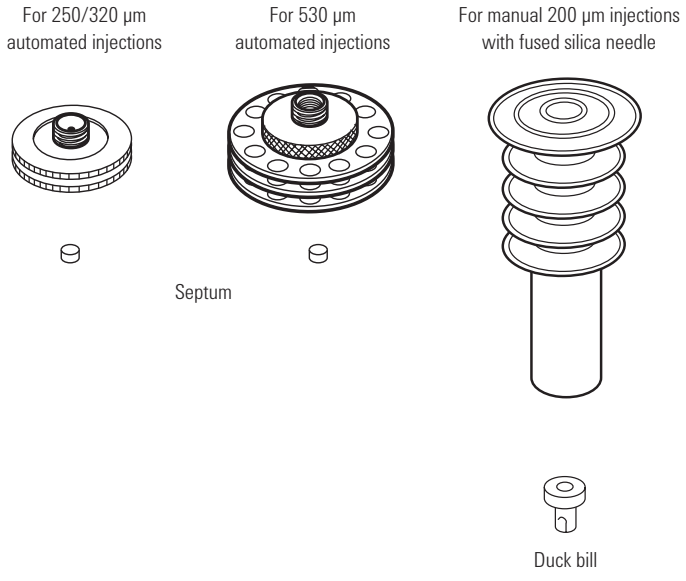

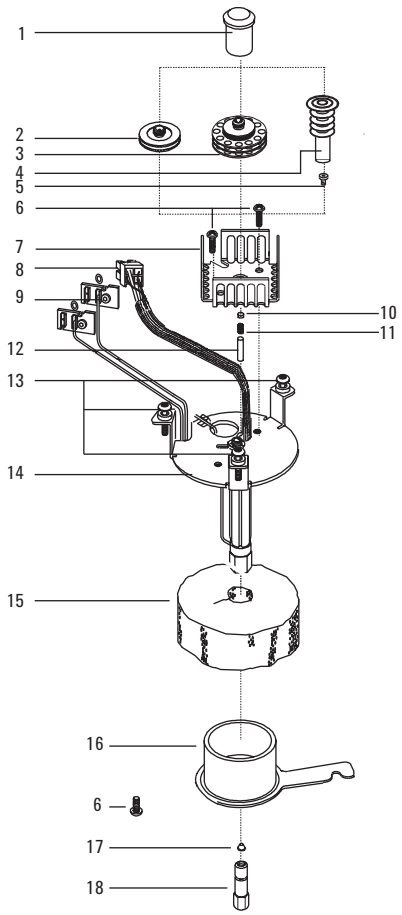

Cool On-Column Inlet assembly

7890/6890 Cool On-Column Inlet Supplies

Item	Description	Part No.	Quantity
1	Needle guide top (optional)	19245-20670	
2	Septum nut base assembly, for 0.250/0.320-mm columns	19245-80521	1
3	Septum nut base, for 0.530 mm columns	G1545-80520	1
4	Manual cooling tower assembly (optional), for 0.200 mm columns	19320-80625	1
5	Duckbill for use with cooling tower, 10/pk	19245-40050	
6	Screw, M4 x 8, Torx T-20 chromeplate	0515-2711	3
7	Heatsink fin	G1545-00010	1
8	Heater/Sensor assembly	G1545-60520	1
9	Screw, M3 x 16 mm	1390-1022	1
10	Septa	Turn to page 15.	
11	Insert spring	19245-60760	1
12	Inserts (identify by number of rings on insert)		
13	Screw, M4 x 12 mm, T-20	0515-2496	3
14	Inlet weldment	G3454-80500	1
15	Inlet weldment insulation	G1545-20630	1
16	Cavity sleeve	19245-00060	1
17	Ferrules (identify by internal diameter)	Turn to pages 30-31.	
18	Column nut	Turn to pages 33-34.	

7673/7683 On-Column Autosampler Syringes

Volume (µL)	Description	Unit	Part No.
5	Removable needle, syringe only*		5182-0836
	Stainless steel needle for 0.53 mm column	3/pk	5182-0832
	Stainless steel needle for 0.32 mm column	3/pk	5182-0831
	Stainless steel needle for 0.25 mm column	3/pk	5182-0833
	Plunger button	10/pk	5181-8866

*Order appropriate needle

Programmable Temperature Vaporizer (PTV) Inlets



PTV inlets combine the benefits of split, splitless and on-column inlets. The sample is usually injected into a cool liner, so syringe needle discrimination does not occur. Then the inlet temperature is increased to vaporize the sample. The user programs vent times and temperature to achieve the equivalent of split or splitless transfer of sample vapors to the column. PTV injection is considered the most universal sample introduction system because of its flexibility.

Advantages

- No syringe-needle discrimination
- Minimal inlet discrimination
- Use of large injection volumes
- Removal of solvent and low boiling components
- Trapping of nonvolatile components in liner
- Split or splitless operation
- Retention time and area reproducibility approaching cool on-column injection

PTV inlets are actively cooled before and during injection by Peltier devices or by forced gases (air, liquid N_2, or liquid CO_2). Cryogenic cooling of the inlet can reduce inlet temperature enough to thermally focus gas injections from other sampling devices in the liner. This is a distinct advantage of using PTV inlets in comparison to conventional inlets for coupling auxiliary sampling devices to capillary columns.

Post-injection, PTV inlets are heated using electrical heaters or preheated compressed air. Depending on design, inlet temperature ramps are either ballistic (i.e., ramped to the maximum temperature at an uncontrolled maximum rate) or programmable.

PTV Inlet Practices and Rationales (Cold Split/Splitless Modes)


Parameter	Selection/Setting	Rationale
Injection mode	Cold split	For general use and sample screening
	Cold splitless	For trace analysis
	Cold solvent vent	LVI
Inlet temperature ramp rate	Adjustable (i.e., 2 °C/sec to 720 °C/sec max)	Use slower ramp rates for labile, complex, or large volume samples Use faster ramp rates for most samples Use faster ramp rates to shorten splitless purge delay time
	Ballistic	Simpler, less expensive instrumentation
Inlet liner	Straight with silanized wool	For general use
	Baffled	For labile samples
	Packed with an adsorbent	For focusing gaseous injections from auxiliary sampling devices
Injection volume	0.1-1.5 µL 5-50 µL for LVI	Use lower volumes for volatile solvents and fast ramp rates Use volumes larger than 1.5 µL only in solvent-elimination mode
Sample Injection technique	Autosampler or manual, fast or slow	Not critical for cold split and splitless modes
Oven temperature	10-25 °C below solvent BP	For proper solvent effect in splitless mode
	Sample dependent	For split mode
Column flow	30-50 cm/sec	Clears inlet faster Less backflash
Septum purge	1-5 mL/min	Minimizes ghosting
Quantification	Any method	Inherently reproducible Low discrimination in cold injection modes
Retention gap	1-3 m, deactivated	Compensates for extended flooded zone and solvent-column incompatibility



PTV Inlet Maintenance


Installing a Capillary Column into the PTV Inlet

1. Position the column so it extends 17 mm above the end of the ferrule. Mark the column behind the ferrule with correction fluid or a marker. Slide the nut over the column.
2. Insert the column into the adapter and finger tighten the column nut. Looking through the slot in the nut, adjust the column until the mark is correctly positioned below the Graphpak 2M ferrule.
3. Tighten the column nut an additional 1/8 to 1/4 turn with a wrench. Do not overtighten.

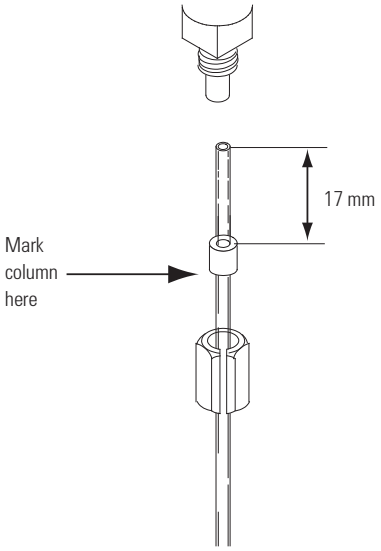

7890/6890 Septumless PTV Inlet Supplies


Description	Column ID (mm)	Unit	Part No.
Microseal high pressure nut			5182-3445
Merlin Microseal			5182-3444
Septumless head			G2617-60507
Septum head			G2618-80500
Septum retainer nut			18740-60835
PTV inlet assembly			G2617-60506
PTV LCO_2 cooling jacket			G2617-60508
PTV LN_2 cooling jacket			G2619-60501
Silver seal		5/pk	5182-9763
Graphpak 2M inlet adapter	0.20		5182-9754
	0.25-0.33		5182-9761
	0.53		5182-9762
Ferrules for Graphpak 2M inlet	0.20		5182-9756
	0.25		5182-9768
	0.32		5182-9769
	0.53		5182-9770
Replacement Graphpak column nut			5062-3525
PTV insulation block			G2617-20510
PTV Cryo insulator			G2617-60510
PTFE ferrule (needle seal)		10/pk	5182-9748
Kalrez seal			5182-9759
Valve body			5182-9757
Pressure spring			5182-9758
Viton seal		5/pk	5182-9775
Sealing element			5182-9760
CO_2 Cryo inline filter			3150-0602
Service kit for septumless head Contains Kalrez seal, valve body, and pressure spring			5182-9747
Graphpak 3D ferrules		5/pk	5182-9749
Assembly tool for Graphpak 3D ferrules			G2617-80540

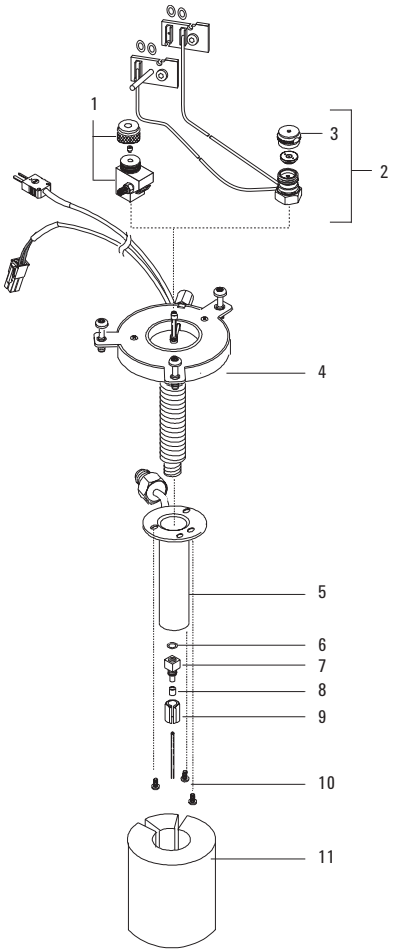

PTV Inlet Body

Item	Description	Part No.
NS	Septumless head weldment	G3500-80000
1	Septumless head	G2617-60507
2	Septum head	G3500-80001
3	Septum nut	18740-60835
4	PTV inlet assembly	G2617-60506
5	Cooling jacket	
	PTV LCO_2 cooling jacket	G2617-60508
	PTV LN_2 cooling jacket	G2619-60501
NS	PTV inlet assembly with cooling jacket	
	PTV inlet with CO2 cooling jacket	G2617-60518
	PTV inlet with LN2 cooling jacket	G2617-60517
6	Silver seal	5182-9763
7	Graphpak inlet adapter	
8	Ferrules for Graphpak inlet	Turn to pages 30-31.
9	Replacement Graphpak column nut	5062-3525
10	Screw, M3 x 3 mm	
11	PTV insulation block	G2617-20510
NS	PTV Cryo insulator	G2617-60510

NS = not shown

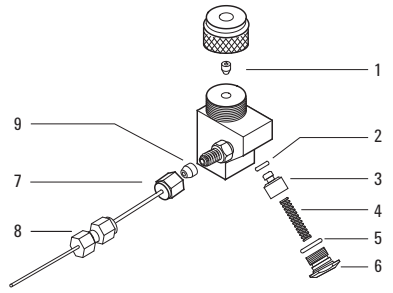

PTV Septumless Head

Item	Description	Part No.
	Septumless head	G2617-60507
1	PTFE ferrule (needle seal)	5182-9748
2	Kalrez seal	5182-9759
3	Valve body	5182-9757
4	Pressure spring	5182-9758
5	Viton seal	5182-9775
6	Sealing element	5182-9760
7	PTV column adapter tube (includes 1/6-inch nut and ferrule)	G2617-80550
8	Septumless head weldment	G3500-80000
9	Straight ferrule, 1/16 in, 10/pk	0100-1375

Programmable Temperature Vaporizing (PTV) Liners

Description	ID (mm)	Volume (µL)	Part No.
Liners for Septumless PTV Inlet, G3501A, G3502A, G3503A			
PTV liner, single baffle, glass wool, deactivated	2	180	5183-2038
PTV liner, single baffle, deactivated	2	200	5183-2036
PTV liner, multi baffled, deactivated	1.8	150	5183-2037
PTV liner, sintered glass, deactivated	1.5	112	5190-1426
Liners for High Temperature PTV Inlet, G3506A			
PTV liner, high temperature, quartz	3.4	713	5188-5313
PTV liner, high temperature, borosilicate	3.4	668	5188-5356

Syringes for Septumless and High Temperature PTV Inlets

Volume (µL)	Description	Needle	Part No.
0.5	Removable	23/70/HP	5182-9651
5	Straight, fixed	23/42/HP	9301-0892
10	Straight, fixed	23/42/HP	9301-0713
50	Straight, fixed, for large volume injections	23/42/HP	5183-0318
100	Straight, fixed, for large volume injections	23/42/HP	5183-2058

Purged Packed Inlets

Packed column analysis is frequently done when high efficiency separations are not needed or when gases are analyzed by gas-solid chromatography. Purged packed inlets are simple in both design and use. Few parameters need to be set, and all carrier gas flow flushes through the inlet into the column in the standard configuration.

Purged Packed Inlet Practices and Rationales

Parameter	Selection/Setting	Rationale
Inlet temperature	BP of solvent +50 °C BP of major solute(s)	Ensures flash vaporization Use for neat samples
Insert type	1/8 in stainless steel 1/4 in stainless steel 530 µm	Use for stainless steel column only Inserts permit connection of columns up to 1/4 in od
Liner	Glass	Use to lower activity (replaceable)
Initial column temperature	Temperature programming	Sharpens peaks and reduces run time
Column type	1/8 in packed stainless 1/4 in packed glass 530 µm	Will not break Better for polar or labile compounds
Carrier gas flow	10-40 mL/min 10-60 mL/min	Use with N_2 carrier gas Use with He or H_2 carrier gas

For more information on our new expanded and refreshed Agilent packed column portfolio see pages 400-409

Purged Packed Inlet Troubleshooting

Purged packed inlets are active, have low volume and are generally flow controlled. This means that most packed column inlet problems involve sample decomposition, flashback, or leaks.

Decomposition

Diagnose inlet sample decomposition by comparing retention times for decomposition products to their standard retention times. Then try these options to improve results:

- Intracolumn direct injection
- Deactivated glass liners
- Lower inlet temperatures
- Remove column packing in the inlet zone
- Increase flow rates

Backflash


Large sample injections can exceed liner capacity and backflash into the gas supply lines and onto the septum. This can cause:

- Ghost peaks
- Sample losses
- Irreproducible peak areas
- Decomposition

Leaks

Septum and column leaks can cause column degradation and stationary phase decompositions on flow-controlled column inlets.

- Change the septum on a regular basis and check column connections to help eliminate leak holes.
- Keep the oven and inlet at room temperature when not in use or while changing the septum.

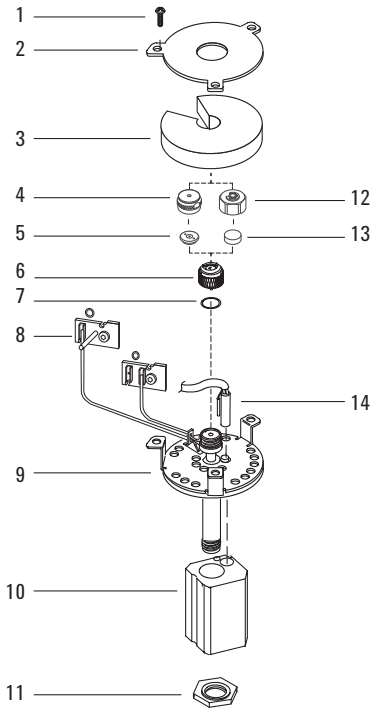


Purged Packed Inlet Upper Body

Purged Packed Inlet Upper Body

Item	Description	Part No.
1	Screw, Torx T-20, M4 x 12 mm	1390-1023
2	Top cover plate	G1543-00085
3	Top insulation	G1543-00100
4	Merlin cap	5182-3445
5	Septum, Merlin Microseal	5182-8815
6	Top insert weldment	19243-80570
7	O-ring, fluorocarbon	5080-8898
8	Screw, Torx T-10, M3 x 16 mm	G1946-20168
9	Inlet weldment	G3451-80501
10	Thermal block	G1543-20765
11	Bottom nut	G1543-20580
12	Septum retainer nut	18740-60835
13	11 mm septa	5183-4757
14	Heater/Sensor assembly	G1543-61540
NS	PTV Cryo insulator	G1543-00155

NS = not shown

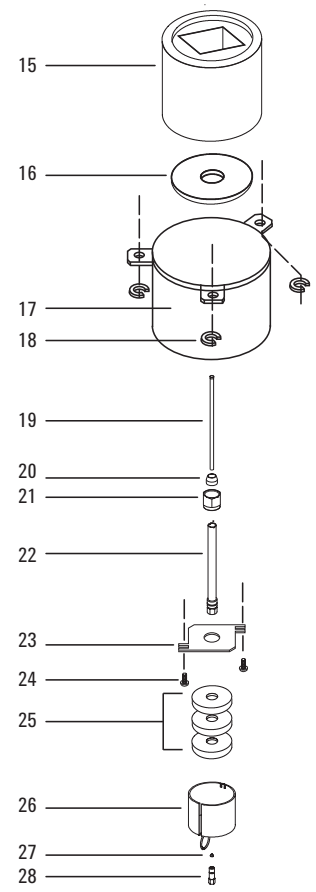


Purged Packed Inlet assembly

Purged Packed Inlet

Item	Description	Part No.
15	PP insulation	G3432-00004
16	PP bottom insulation	G3432-00003
17	PP insulation cup	G3431-00005
18	C-clip	0515-1799
19	Disposable glass liner, 170 µL internal volume	5080-8732
20	Vespel ferrule, 1/4 in	5080-8774
21	1/4 in nut, brass	5180-4105
22	530 µm column adapter for use with glass liners	19244-80540
23	Bottom plate for oven	G1543-00060
24	Screw, T-20, M4 x 12 mm	0515-2711
25	Adapter insulation	19234-60715
26	Insulating cup	19234-60700
27	Ferrules	Turn to pages 30-31.
28	Column nut (capillary, universal, 2/pk)	5180-8830

7890/6890/6850 Purged Packed Inlet Supplies


Description	Unit	Part No.
QuickPick Purged Packed Inlet PM Kit Includes 5 non-stick BTO septa, 1 O-ring, 1 ferrule, and 1 disposable glass liner		5188-6498
Merlin Microseal		5182-3444
Microseal high pressure nut		5182-3445
Septum retainer nut		18740-60835
11 mm Certified BTO septa	50/pk	5183-4757
Top insert weldment		19243-80570
O-ring, Fluorocarbon	12/pk	5080-8898
Disposable glass liner, 170 µL internal volume	25/pk	5080-8732
Disposable glass insert, deactivated, 170 µL internal volume	5/pk	5181-3382
Vespel ferrule, 1/4 in	10/pk	5080-8774
1/4 in nut, brass	10/pk	5180-4105
530 µm column adapter for use with glass liners		19244-80540
1/8 in column adapter for use with glass liners		19243-80530
1/4 in column adapter for use with glass liners		19243-80540
Insulating cup		19234-60720
Universal column nut	2/pk	5181-8830

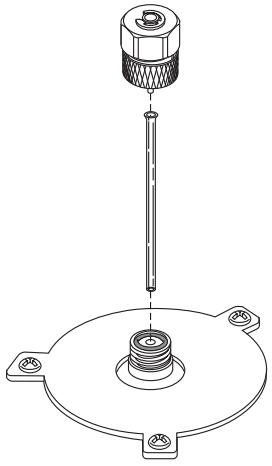

How to install glass liner on Purged Packed Inlet

Nuts and Ferrules for 1/8 in Packed Columns

Description	Unit	Part No.
1/8 in stainless steel nut and ferrule set	20/pk	5080-8751
1/8 in brass nut and ferrule set	20/pk	5080-8750
Vespel/graphite ferrule, 1/8 in	10/pk	0100-1332

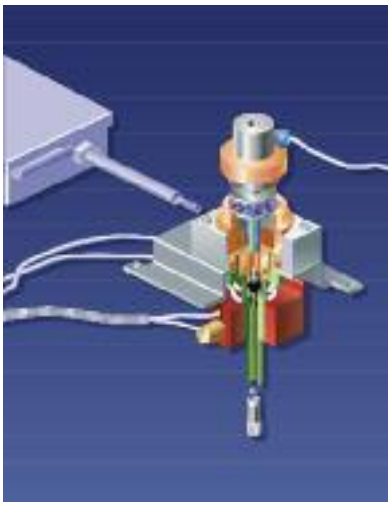

Detector Systems

Flame Ionization Detector (FID)

The FID requires routine maintenance to ensure optimum performance. Maintenance requirements are application dependent, but Agilent recommends periodically cleaning or replacing the following items:

FID Routine Maintenance

Item	Comments
FID Jet	A plugged jet results in longer retention times as the column exit/detector pressure increases. Once the jet becomes completely plugged, it is difficult to light or sustain a flame.
Ignitor Glow-Plug	Replace if corroded or burned out.
FID Collector/Insulators	Contamination can contribute to detector noise or loss of sensitivity.
Column Adapter/Seals For Adaptable FID only	Leaks at column fittings can result in difficulty lighting the FID or sustaining a flame after injection.

Typical FID Problems

Condensation

Since the FID combustion process results in water formation, the detector temperature must be kept above 300 °C to prevent condensation. At detector block temperatures below 300 °C, the castle assembly drops below 100 °C, resulting in condensation and possible rusting. Such condensation, especially when combined with chlorinated or fluorinated solvents or samples, causes corrosion, with resulting increase in detector noise and loss of sensitivity.

Flame Ignition

If the flame goes out or will not light:

- Measure the hydrogen/air and makeup flow rates – Low H_2 or makeup flows indicate a plugged jet, or a leak at the column fitting. Measure each gas flow independently.
- Confirm that the ignitor is glowing during the FID ignition sequence.
- Check for partially or completely plugged jet – Formation of silica or carbon deposits at the tip of the jet can cause plugging. Incorrect capillary column installation can also cause plugging.

It is best to replace a plugged jet, rather than try to clean it.

- Check that the capillary column is not installed all the way to the jet tip (withdraw 1-2 mm).
- Check that the correct type of jet is installed for the column you are using.
- Check for leaking column or adapter fitting at the base of the FID.
- Check the lit offset value to make sure it is not too low or too high. Adjust the value (normally set to 2.0 pA).

Injecting large volumes of aromatic solvent or water can cause the flame to go out. Switch to a non-aromatic solvent or reduce injection volume.



FID collector assembly

Increased FID Noise or Loss in Sensitivity

FID noise is affected by:

- The cleanliness of the GC gases and gas delivery system – Ensure that the carrier/H_2 and air purity is ≥ 99.9995%. Check traps and filters in the gas supply lines. The FID background signal should be ≤ 20 pA when the flame is lit and stablized.
- Dirty collector/PTFE insulators – Clean or replace.
- Dirty jet – An incorrect flame pattern can increase noise or affect sensitivity.

TIPS & TOOLS

For optimal sensitivity, use Agilent gas purifiers to ensure cleanliness of your GC gases, see pages 12-13

Installing a Capillary Column in the FID

WHAT YOU NEED:

- Column
- Ferrule(s)
- Column nut
- Column cutter
- 1/4 in open end wrench
- Septum
- Isopropanol
- Lab tissue
- Lint-free gloves
- Column ferrule installation tool (P/N 19251-80680)

WARNINGS & CAUTION

- The oven and/or inlet may be hot enough to cause burns. If either is hot, wear heat-resistant gloves to protect your hands.
- Wear safety glasses to protect your eyes from flying particles while handling, cutting or installing glass or fused silica capillary columns. Use care in handling these columns to prevent puncture wounds.
- Wear clean, lint-free gloves to prevent contamination of parts with dirt and skin oils.

1. Gather the required supplies and tools.
2. Load the GC maintenance method and wait for the GC to become ready.
3. If using the adaptable detector, verify that the adapter is installed.
4. Place a septum, capillary column nut, and ferrule on the column.
5. Score the column using a glass scribing tool. The score must be square to ensure a clean break.
6. Break off the column end by supporting it against the column cutter opposite the scribe. Inspect the end with a magnifying loupe to make certain there are no burrs or jagged edges.
7. Wipe the column walls with a tissue dampened with isopropanol to remove fingerprints and dust.
8. Install the capillary column.

   If the column id is greater than 0.1 mm:

   a. Gently insert the column into the detector until it bottoms; do not attempt to force it further.


   b. Finger-tighten the column nut, then withdraw the column about 1 mm. Tighten the nut an additional 1/4 turn with a wrench.

   If the column id is 0.1 mm or less, position the column so it extends above the ferrule by 48 mm (capillary optimized fitting) or 68 mm (adaptable fitting). Slide the septum up to hold the column nut and ferrule at this fixed position.

   c. Insert the column into the detector. Slide the nut and ferrule up the column to the detector base. Finger-tighten the column nut until it grips the column.

   d. Adjust the column (not the septum) position so that the septum is even with the bottom of the column nut. Tighten the nut an additional 1/4 turn with a wrench.

Positioning the column

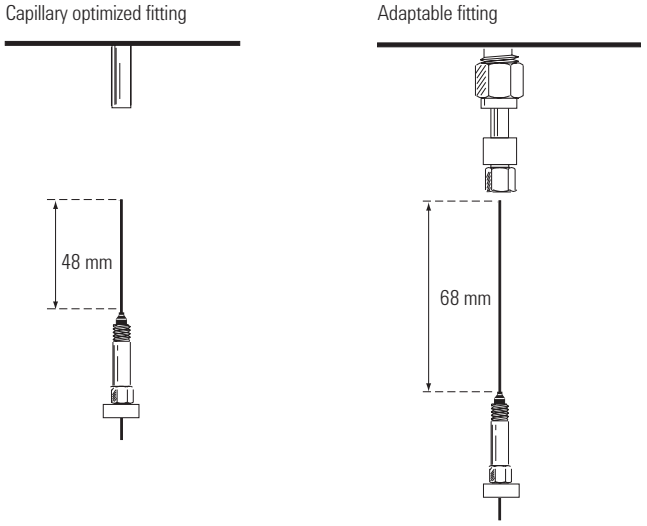


FID Jet Identification and Selection

Before ordering parts for FID maintenance, determine which type of FID is installed on your GC.
The FID is available in two versions:

- Dedicated, Capillary Optimized: for capillary columns only
- Adaptable: for packed or capillary columns

To determine the type of FID installed on your GC, open the oven door and examine the fitting at the base of the detector. Compare to the following diagram.

Hint: Adaptable jets are longer than dedicated capillary jets.

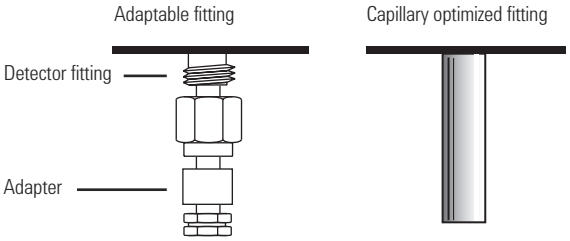

FID Jets

Description	Jet Tip ID	Length (mm)	Part No.
Jets for capillary optimized fittings			
Capillary	0.29 mm (0.011 in)	42.8	G1531-80560
Capillary Optimized for simulated distillation	0.47 mm (0.018 in)	42.8	G1531-80620
Jets for adaptable fittings			
Capillary	0.29 mm (0.011 in)	61.5	19244-80560
Capillary Optimized for simulated distillation	0.47 mm (0.018 in)	61.5	19244-80620
Packed	0.46 mm (0.018 in)	63.5	18710-20119
Packed, wide-bore Use with high-bleed applications	0.76 mm (0.030 in)	63.5	18789-80070



Plugged FID Jet, 19244-80560



Dedicated capillary, G1531-80560

Adaptable capillary, 19244-80560

Adaptable packed capillary, 18710-20119



FID cleaning kit, 9301-0985

Jet Cleaning Procedure

Use Agilent FID Cleaning Kit, part number 9301-0985

1. Run a cleaning wire through the top of the jet. Run it back and forth a few times until it runs smoothly. Be careful not to scratch the jet. (Do not force too large a wire or probe into the jet opening or the opening will become distorted. A loss of sensitivity, poor peak shape, and/or lighting difficulties may result if the opening is deformed.)
2. Fill an ultrasonic cleaning bath with aqueous detergent, and place the jet in the bath. Sonicate for five minutes.
3. Use a jet reamer to clean the inside of the jet.
4. Sonicate again for five minutes.

   Note: from this point on, handle the parts only with forceps!
5. Remove the jet from the bath and rinse it thoroughly, first with hot tap water and then with a small amount of GC-grade methanol.
6. Blow the jet dry with a burst of compressed air or nitrogen, and then place the jet on a paper towel and allow to air dry.


7890/6890/6850 Flame Ionization Detector (FID) Supplies

Item	Description	Unit	Part No.
	PTFE chimney (optional)		19231-21050
1	Screw, M4 x 25 mm, Torx T-20		0515-2712
2	FID collector assembly		G1531-60690
	FID collector cleaning brush	2/pk	8710-1346
	FID retainer nut wrench 5880, 5890, 6890		19301-00150
	1/4 in nut driver for FID jet, drilled shaft		8710-1561
3	Collector nut		19231-20940
4	Spring washer	10/pk	5181-3311
5	Ignitor castle		19231-20910
	Hastelloy ignitor castle (optional)		19231-21060
6	Collector insulator		G1531-20700
7	Collector body		G1531-20690
	Hastelloy collector body		G1531-21090
8	Nut, collector spanner		19231-20980
9	Collector mount		G1531-20550
10	Collector housing		G1531-20740
11	Silicone gaskets, 0.890-inch od/0.709-inch id, 12/pk		5180-4165
12	Ignitor glow plug assembly		19231-60680
13	FID ignitor cable, 7890A only		G3431-60680
	FID ignitor cable for 6890/6850 only		G1531-60680

(Continued)

7890/6890/6850 Flame Ionization Detector (FID) Supplies


Item	Description	Unit	Part No.
	FID performance evaluation sample kit This sample is used for the HP 5880, 5890 and 6890 with a FID or TCD. Solution of 0.033% C14, C15, and C16 normal alkanes in hexane. Three 0.5 mL ampoules.		18710-60170
	FID MDL test sample for 7890 only 3 x 0.5 mL ampoules. Contains 2.36 mg/L n-Tridecane, 2.36 mg/L n-Tetradecane, 23.6 mg/mL n-Penta-decane, 23.6 mg/mL n-Hexadecane in iso-octane		5188-5372
	O-rings	12/pk	5080-4978
	FID/NPD adapter for capillary column		19244-80610
	FID/NPD 1/8 in packed column		19231-80520
	FID/NPD 1/4 in packed column		19231-80530
	1/4 in nut driver for FID jet, drilled shaft		8710-1561
	FID collector cleaning brush	2/pk	8710-1346
	FID Supplies Kit, Includes:		5182-3450
	Jet, packed standard 0.018 in id tip	3 each	18710-20119
	FID and TCD sample	2 each	18710-60170
	Ignitor glow plug assembly	2 each	19231-60680
	Jet, 0.011 in id tip, capillary adaptable	3 each	19244-80560
	FID flow measuring insert	2 each	19301-60660
	Cleaning wires for 0.03 in id jet	5/pk	5180-4150
	Cleaning wire for 0.018 in id/530 µm jet For use with 0.018 and 0.011 in id jets	5/pk	5180-4152
	Cleaning wire for 0.011 in id jet	5/pk	19301-20720
	Capillary inlet cleaning wires	5/pk	5180-4153
	FID cleaning kit		9301-0985

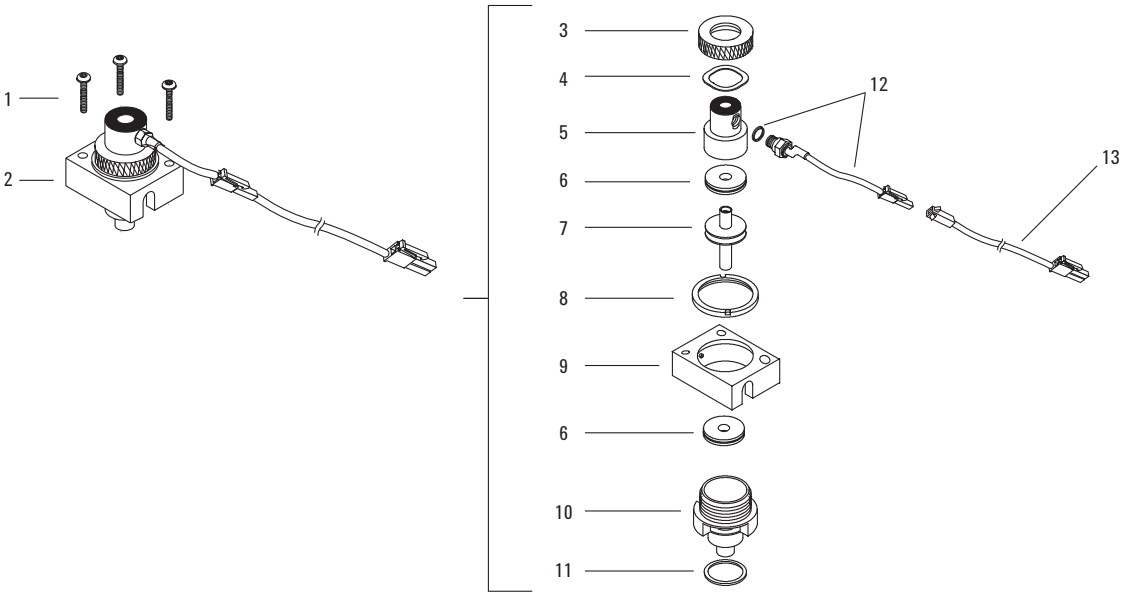

Flame Ionization Detector (FID) assembly

FID Base Assembly

Item	Description	Part No.
1	Base spanner nut	19231-20990
2	Thermal strap	G1531-00105
3	Screw, Torx T-10, M3 x 16 mm	G1946-20168
	Replacement O-rings	5180-4181
4	Jets	Turn to page 81.
5	Adaptable FID, base weldment with jet	G3431-80509
	Capillary column FID, base weldment with jet	G3431-80507
6	Screw, M4 x 25 mm, Torx T-20	0515-2712
7	FID block insulation	G1531-60700
8	Adaptable FID column adapters:	
	FID/NPD adapter for capillary column	19244-80610
	FID/NPD 1/8 in packed column	19231-80520
	FID/NPD 1/4 in packed column	19231-80530
9	Nut warmer insulation and cup assembly	19234-60720
10	Heater/sensor assembly	G1530-61950

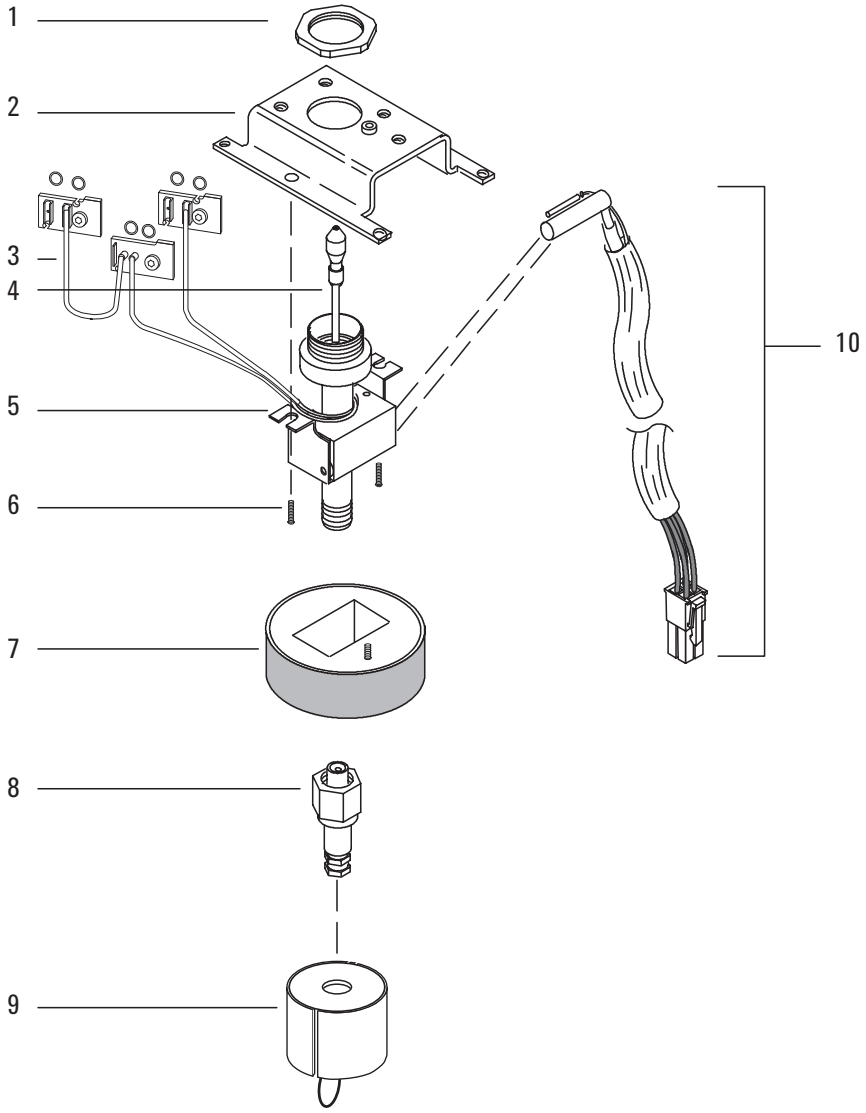

FID Base Assembly



Electron Capture Detector (ECD)

The Agilent micro ECD is the most sensitive on the market, with a detection zone volume 10 times smaller than any other ECD. The replaceable liner serves as a physical stop for the column, ensuring reproducible column installation and decreasing column contamination of the cell.

Liner Selection

The only assembly that requires routine maintenance is the glass liner in the makeup gas assembly, especially for the µECD. All sample passes through the indent in the mixing liner of the µECD. The mixing liner should be replaced if there is a significant loss of sensitivity or any time the column is removed/reinstalled in the detector.

- Gigabore Liner (P/N 19233-20625): for original ECD design (5890 and 6890), brown, polyamide coating
- Mixing Liner (P/N G2397-20540): for µECD, clear glass with indent

Makeup Gas Adapter Maintenance/Installation Procedure

1. Remove the Makeup Gas Adapter from the ECD fitting with a 9/16 in wrench. Be careful not to stress the 1/16 in stainless steel gas supply tube.
2. Unscrew the end cap of the Makeup Gas Adapter and ultrasonically clean in solvent.
3. Remove the old liner.
4. Clean the Makeup Gas Adapter body with solvent in a Nalgene squeeze bottle.
5. Wipe the Makeup Gas Adapter with a clean laboratory wipe.
6. Install the replacement liner.
7. Reinstall the tip of the Makeup Gas Adapter and tighten securely.
8. Reinstall the Makeup Gas Adapter. Make sure it is fully inserted into the detector.
9. Reinstall the column.
10. Reinstall the insulation cup.

Thermal Cleaning

If your baseline is noisy or the output value is abnormally high (> 1000 Hz), and you have determined that these problems are not being caused by leaks in the GC system, you may have contamination in the detector from column bleed and sample residues. To remove contamination, you should perform a thermal cleaning (bakeout) of the detector. Bakeout the detector at 20 to 30 degrees higher than normal operating temperature (375 °C Max), with 50 to 100 mL/min of makeup gas flow.

WARNINGS & CAUTION

Detector disassembly and/or cleaning procedures other than thermal should be performed only by personnel trained and licensed appropriately to handle radioactive materials. Trace amounts of radioactive ^{63}Ni may be removed during other procedures, causing possible hazardous exposure to β and x-radiation.

Radioactivity Leak Test

Electron capture detectors must be tested for radioactive leakage at least every six months. Records of tests and results must be maintained for possible inspection by the Nuclear Regulatory Commission and/or responsible local agency. More frequent tests may be conducted when necessary.


The procedure used is a "wipe test." A Wipe Test Kit is supplied with each new detector. Refer to the information card supplied in the kit for instructions on performing the test.

Gas Purity

For successful EC detection, it's important that the carrier and purge gases are very clean and dry (99.9995% minimum purity). Moisture, oxygen, or other contaminants can result in higher detector response but usually at the expense of both sensitivity and linear range. Always precondition the column before connection to the detector.

ECD Wipe Test

The Wipe Test Kit (P/N 18713-60050) included with each new ECD includes an information card with instructions for performing the test. Records of tests and results must be maintained for possible inspection by the Nuclear Regulatory Commission (NRC) and/or responsible state agency.

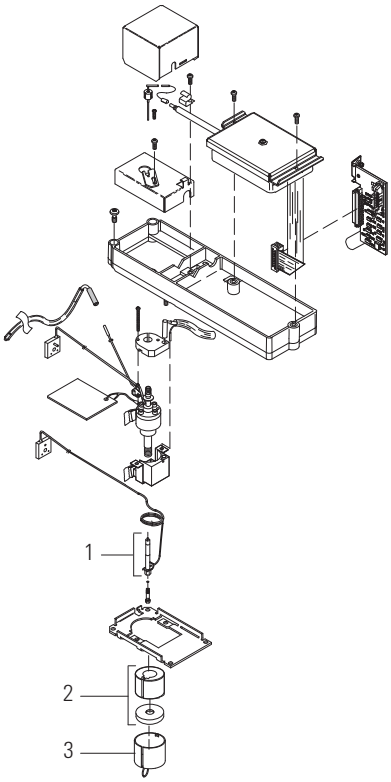

Electron Capture Detector (ECD) assembly

7890/6890/6850 Electron Capture Detector (ECD) Supplies

Item	Description	Part No.
1	Standard ECD makeup gas adapter*	G1533-80565
	Micro ECD makeup gas adapter	G2397-80520
	Micro ECD mixing liner, also compatible with standard ECD design	G2397-20540
	Gigabore liner for standard ECD, polyamide coating, not compatible with micro ECD	19233-20625
	ECD makeup gas adapter, 7890 only	G3433-63000
2, 3	Insulating cup	19234-60720
	ECD adapter end cap	19233-20755
	Vespel ferrule, 1/4 in	5080-8774
	1/4 in nut, brass	5180-4105
	Electron Capture Detector sample	18713-60040
	ECD test sample	5183-0379
	Micro ECD wipe test kit	18713-60050

*Includes one each of P/N 19233-20625 and 19233-20755

ECD WARNINGS

Although beta particles at this energy level have little penetrating power – the surface layer of the skin or a few sheets of paper will stop most of them – they may be hazardous if the isotope is ingested or inhaled. For this reason the cell must be handled with care. Radioactive leak tests must be performed at the required intervals, the inlet and outlet fittings must be capped when the detector is not in use, corrosive chemicals must not be introduced into the detector, and the effluent from the detector must be vented outside the laboratory environment.

Thermal Conductivity Detector (TCD)

The TCD compares the thermal conductivities of two gas flows – pure carrier gas (also called the reference gas) and carrier gas plus sample components (also called column effluent).

Filament Maintenance

The primary maintenance for a TCD involves the filament. Most procedures involve improving filament life or keeping the filament from becoming damaged or contaminated. To avoid filament damage and contamination:

- Check for leaks
- Use gas purifiers to remove oxygen
- Avoid chemically-active sample components, such as acids and halogenated compounds
- Turn off the filament when not in use

Increasing Filament Lifetime

Use the following startup process to increase filament lifetime:

Purge the detector with carrier and makeup gas for 10-15 minutes before turning on the filaments. This prevents oxidation of the filaments due to the presence of oxygen that has diffused into the cell under no flow conditions.

Cell Contamination

Cell contamination is a problem when a lower detector temperature is used to improve sensitivity. If the cell becomes contaminated, a solvent flush of the detector may help to remove the condensed material.

Solvent Flush

1. Cool the cell to room temperature and remove the column.
2. Place a septum in a nut or fitting assembly that fits onto the detector entrance (7 mm septum in a 1/8 in nut).
3. Place the nut or assembly on the detector fitting and tighten. Verify the presence of makeup gas flow.
4. Inject 20-100 µL volumes of toluene or benzene into the detector through the septum. Inject a total volume of at least 1 mL of solvent. Do not inject halogenated solvents such as methylene chloride and chloroform into the detector.
5. After the final injection, allow makeup gas to flow for 10 minutes or more. Slowly raise the temperature of the cell to 20-30 °C above the normal operating temperature.
6. After 30 minutes, decrease the temperature to the normal value and install the column as usual.

Thermal Cleaning

The TCD can become contaminated with deposits from such things as column bleed or dirty samples. A wandering baseline, increased noise level, or changes in response on a checkout chromatogram all indicate contamination. Thermal cleaning, or bakeout (heating the detector block to evaporate the contaminant), should be performed only after you have confirmed that the carrier gas and the flow system components are leak-free and contaminant-free.


Watch out for decreased sensitivity caused by samples that react with the filament, originating from oxygen-contaminated carrier gas, leaks in plumbing, or column bleeding. Samples with active components, such as acids and halogenated compounds can chemically attack the filament as well. Also, sample condensation will contaminate the detector cell if the temperature is too low.

7890/6890/6850 Thermal Conductivity Detector (TCD) Supplies


Item	Description	Unit	Part No.
For 1/8 in SS Packed Column Installation			
1	Vespel/graphite ferrule, 1/8 in	10/pk	0100-1332
2	1/8 in nut, brass	10/pk	5180-4103
For 1/4 in SS Packed Column Installation			
3	Vespel/graphite ferrule, 1/8 in	10/pk	0100-1332
4	1/8 in nut, brass	10/pk	5180-4103
5	1/4 in packed column adapter		G1532-20710
6	Vespel ferrule, 1/4 in	10/pk	5080-8774
7	1/4 in nut, brass	10/pk	5180-4105
For Capillary Column Installation (Standard)			
	TCD capillary column adapter		G1532-80540
8	Vespel/graphite ferrule, 1/8 in	10/pk	0100-1332
9	1/8 in nut, brass	10/pk	5180-4103
	Universal column nut	2/pk	5181-8830
	6850 column nut	2/pk	5183-4732
	530 µm, 1.0 mm id graphite ferrule	10/pk	5080-8773
	320 µm, 0.5 mm id graphite ferrule	10/pk	5080-8853
	TCD sample		18711-60060
	FID and TCD sample		18710-60170



1/8 in SS packed column

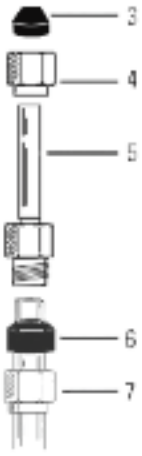

1/4 in SS packed column



Standard design

Installing a Capillary Column in the TCD

WHAT YOU NEED:

- Front ferrule
- Back ferrule
- Column nut
- Column cutter
- 7/16 in wrench
- Lab tissue
- Lint-free gloves


1. Gather the required supplies and tools.
2. Assemble the ferrules and 1/8 in brass Swagelok nut on the column.
3. Score the column using a glass scribing tool. The score must be square to ensure a clean break.
4. Break off the column end by supporting it against the column cutter opposite the scribe. Inspect the end with a magnifying loupe to make certain that there are no burrs or jagged edges.
5. Wipe the column walls with a tissue dampened with isopropanol to remove fingerprints and dust.
6. Insert the column into the detector until it bottoms.
7. Slide the column nut and ferrules up the column to the detector and finger tighten the nut.
8. Pull out 1 mm of column. Tighten the nut an additional 1/4 turn with a wrench or until the column does not move.

WARNINGS & CAUTION

- The oven and/or inlet may be hot enough to cause burns. If either is hot, wear heat-resistant gloves to protect your hands.
- Wear safety glasses to protect your eyes from flying particles while handling, cutting or installing glass or fused silica capillary columns. Use care in handling these columns to prevent puncture wounds.
- Wear clean, lint-free gloves to prevent contamination of parts with dirt and skin oils.

TCD Ferrules

Column ID (mm)	Back Ferrules	Front Ferrules, 10/pk
0.53	5182-3477	5182-9673
0.32	5182-3477	5182-9676
0.25/0.2/0.1	5182-3477	5182-9677
No hole	5182-3477	5182-9679
1/8 in nut, brass, 10/pk	5180-4103	

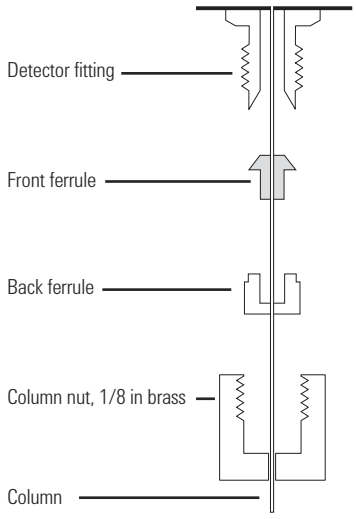

Determining the TCD Electronic Pressure Control (EPC)

If you have a 6890A or 6890A Plus GC, you may have an older design EPC flow manifold for the TCD. The older design requires removal of sheet metal panels to attach the TCD reference flow gas supply inside the GC. The new "Minifold" design allows TCD reference gas to be connected directly to the back of the GC. Replacement TCD filament block assemblies have different part numbers depending on the EPC design type.

Once you have determined the type of EPC module, consider ordering a passivated filament block assembly, which is recommended for fatty acid analysis or reactive/acidic samples.

TCD Filament Block Assemblies

Instrument	Passivated	Applications	Specifications	EPC Design	Part No.
7890A	Yes	Standard TCD Analysis Gases/Hydrocarbons	Complete Detector Assembly Includes detector palette and heater/sensor assembly	Original	G3432-60220
7890A	Yes	Standard TCD Analysis Gases/Hydrocarbons	Complete Detector Assembly Includes detector palette and heater/sensor assembly Third detector, side mounted	Original	G3432-60221
6890	No	Standard TCD Analysis Gases/Hydrocarbons	Filament Block Only Must reuse heater/sensor	Original	G1532-60675
6890	No	Standard TCD Analysis Gases/Hydrocarbons	Filament Block Only Must reuse heater/sensor	Minifold	G1532-60685
6890	Yes	Recommended for Fatty Acid Analysis	Filament Block Only Must reuse heater/sensor	Original	G1532-60690
6890/6850	Yes	Recommended for Fatty Acid Analysis	Filament Block Only Must reuse heater/sensor	Minifold	G1532-60695
6890/6850	No		Complete Detector Assembly Includes detector palette and heater/sensor assembly	Minifold	G2630-61230

Flame Photometric Detector (FPD)

In 2005, Agilent released an improved FPD with minimum detectable levels (MDL) of 3.6 pg/s for sulfur and 60 fg/s for phosphorus. This is more than a 5 times improvement for sulfur. The updated design is based on a one-piece, deactivated transfer line jet assembly and improved optics. Upgrade kits are available.

Operation

The FPD uses three gases: air and hydrogen to support the flame, and nitrogen makeup for capillary columns. The flow rates are critical for optimizing performance. Using nitrogen as a makeup gas is essential to obtaining low MDLs. Do not use helium for the makeup gas.

Recommended Gas Flows

Detector Gas Flows	Phosphorus Mode	Sulfur Mode
Air	100 mL/min	60 mL/min
Hydrogen	75 mL/min	50 mL/min
Nitrogen makeup	60 mL/min	60 mL/min

Maintenance

Managing gas purity; contamination from column bleed, sample residue, and corrosion; and air leaks can help keep your FPD at peak performance.



Glow plug, 0854-0141

Gas Purity

Sulfur contamination is a common problem and causes noise and/or a higher baseline offset in the FPD. To minimize sulfur contamination and achieve the lowest MDLs, use at least 99.9995% pure gases, clean tubing, and regulators with metal diagrams. To protect your FPD over its lifetime, Agilent recommends gas generators or supply gas filters designed to remove sulfur.

For more information on Gas Clean Filters, see pages 132-133

Contamination

The FPD is susceptible to build up of residue on the surfaces of the ignitor coil, jet, combustion chamber, and chamber window. The residue increases detector offset and reduces the signal-to-noise ratio. The sample or column bleed usually cause the residue. After a period of time, you may need to rebuild the detector and replace the transfer line. Do not clean the transfer line, jet, or other parts with brushes or solvents.

To increase the time between servicing, remove the column, cap off the detector, and run it at 250 °C with the flame to bake off some of the residue. Replacing the ignitor may reduce baseline output. If these tactics are not effective, rebuild the detector.

If your solvent or sample is corrosive, it can erode the aluminum vent tube. Agilent recommends using alternative stainless steel vent tubes for these applications.

Air Leaks

The original FPD design has three more internal seals than the new design. Temperature cycling of the detector causes the ferrules to shrink and leaks to occur. The most common leaks are around the fused silica transfer line. To eliminate these leaks, remove the detector from the GC and tighten the transfer line fittings.

For both the original and new FPD, leaks can develop at the column nut or capillary column adapter, the gang fitting at the EPC module, around the vent tube, or around the ignitor glow plug. If you are replacing fittings or O-rings, always use conditioned, graphitized-vespel ferrules and Agilent's low sulfur O-rings. Make sure ferrules are the correct size for your column.

Flame Ignition Problems

You can tell if your FPD is lit by checking the detector "Output" and "Flame" on the display. The detector senses that the flame is on by comparing the output with the offset. An optimized FPD normally runs with an output in the range of 30 to 80 with the offset point at 2.0. If the flame is out and the electrometer is on, the output usually displays less than 1.

Most FPD ignition problems are caused by incorrect gas flows, incorrect column installation, or a dirty or defective ignitor. To troubleshoot:

1. Make sure the FPD is at operating temperature before trying to light.
2. Remove the rubber drip tube while lighting the FPD.
3. Increase air supply pressure by 10-20 psi.
4. Check the detector gas flows to see if they match the Recommended Gas Flows table.
5. Check the detector output when you turn the flame on. The photomultiplier will see the glow of the ignitor and jump to about 68000 pA.
6. Remove the column and check the tip for residue or burnt polymide coating. If it appears damaged, cut off the damaged portion and reinstall to the proper height.
7. Remove the ignitor glow plug. If dirty or damaged, replace it.

Less common problems include leaks, quenching, and condensation:

- Large air leaks at the inlet or detector can reduce the percentage of the hydrogen-air mixture at the detector and cause ignition problems.
- Large injections of certain samples can cause flameouts or quenching that cause the detector to attempt to relight, interrupting your analysis.
- Condensation is a by-product of the burning of your sample. For many analyses, the liquid is collected from the vent tube. If the liquid drips back into the detector, it will extinguish the flame. Agilent recommends that you wait to light the flame until the detector is at temperature and equilibrated.
- Light leaks at the vent tube can cause a higher baseline offset. Make sure the vent tube ferrule seals tightly against the emission block. Keep the lid closed over the detector.


TIPS & TOOLS



Helium is not a good makeup gas for the FPD. You will not be able to light or keep the detector lit in the sulfur mode with helium.

Installing a Capillary Column Adapter to the FPD

1. Gather the required supplies and tools.
2. Load the GC maintenance method and wait for the GC to become ready.
3. Insert the capillary adapter into the 1/8 inch nut as shown, then thread the nut onto the detector fitting.
4. Finger-tighten the nut, then tighten an additional 1/8 turn with a wrench.

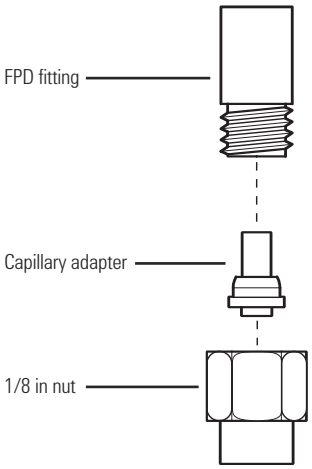

WHAT YOU NEED:

- FPD capillary column adapter
- Column cutter
- 1/4 in and 9/16 in wrenches
- Metric ruler
- 1/8 in nut
- Lint-free gloves

WARNINGS & CAUTION

- The oven and/or inlet may be hot enough to cause burns. If either is hot, wear heat-resistant gloves to protect your hands.
- Wear safety glasses to protect your eyes from flying particles while handling, cutting or installing glass or fused silica capillary columns. Use care in handling these columns to prevent puncture wounds.
- Wear clean, lint-free gloves to prevent contamination of parts with dirt and skin oils.


WHAT YOU NEED:

- Column measuring tool, P/N 19256-80640
- Column cutter
- 1/4 in and 7/16 in wrenches
- Column nut
- Ferrule
- Capillary column
- Lint-free gloves

Attaching a Capillary Column to the FPD

1. Gather the required supplies and tools.
2. Load the GC maintenance method and wait for the GC to become ready.
3. Assemble a septum, column nut, and ferrule on the end of the column.
4. Insert the end of the column through the column measuring tool so that the end protrudes beyond the tool.
5. Tighten the column nut until it grips the column. Tighten the nut an additional 1/8 to 1/4 turn with a pair of wrenches. Snug the septum against the base of the column nut.
6. Use a wafer cutter at 45° to score the column.
7. Snap off the column end. The column may protrude about 1 mm beyond the end of the tool. Inspect the end with a magnifying loupe to make certain that there are no burrs or jagged edges.
8. Remove the column, nut, and swaged ferrule from the tool.
9. Wipe the column walls with a tissue dampened with isopropanol to remove fingerprints and dust.
10. Verify that a capillary adapter is installed in the detector fitting.
11. Carefully thread the swaged column up into the adapter. Finger-tighten the column nut, then use a wrench to tighten an additional 1/8 turn.

If you are using a capillary column, the tip of the column must be at least 1 mm below the surface of the jet. When you install the column, measure the distance from the sealing surface of the ferrule to the tip of the column. This measurement is 153 mm for the original FPD and 145 mm for the new FPD. For the new design, Agilent recommends using the column measuring tool, part number 19256-80640.

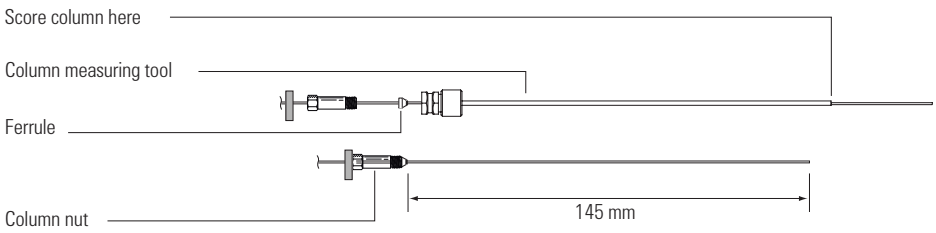


7890/6890/6850 FPD Ignitor and Heat Shield Assembly

Item	Description	Part No.
1	FPD Exit Tube Assembly	
	Aluminum	19256-60700
	Stainless steel	19256-20705
2	Vespel ferrule, 1/4 in, 10/pk	5080-8774
3	Emission chamber	
	FPD, single	19256-80560
	FPD, dual	19256-80600
4	FPD ignitor replacement kit	19256-60800
	O-ring, size 2-010	0905-1610
	Spacer, ignitor	19256-20590
	Glow plug	0854-0141
5	Ignitor cable assembly	G1535-60600
6	Heat shield gasket, white	19256-80045
7	First heat shield window	19256-80030
8	Heat shield disk	19256-20580
9	Stainless steel coupling	19256-20550
10	Lock washer (4 required)	2190-0584
11	Screw, M3 x 12 mm, T10 (4 required)	0515-1084
12	Collar	19256-20690
13	Screw, M3 x 66 mm, T10	0515-0680
	FPD check out sample	5188-5953
	FPD sample	5188-5245



Glow plug, 0854-0141

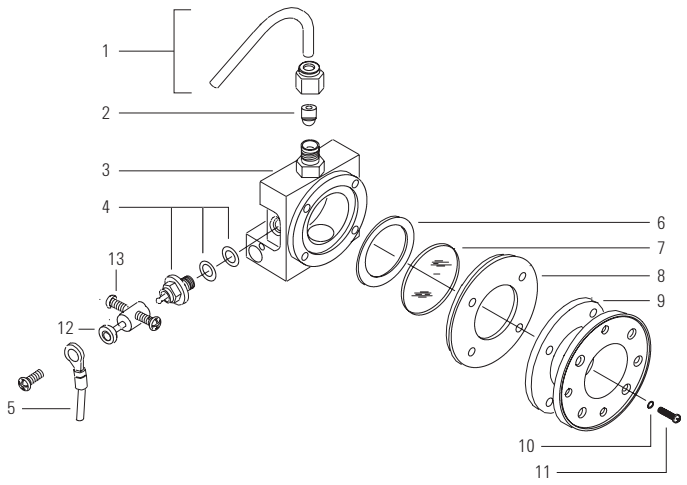


FPD ignitor and heat shield assembly

FPD Lens Assembly

Item	Description	Part No.
1	Clamp	19256-00090
2	Screw, M3 x 25 mm (4 required)	0515-0683
3	Window O-ring, inner, 0.926 in id, orange	5061-5886
4	Convex lens	1000-1438
5	Lens housing	19256-20900
6	Flange ring	19256-00200
7	Fluorocarbon Elastomer O-ring, brown, 1.239 in id	5061-5890

TIPS & TOOLS

Track detector output – when it increases by 50%, remove the column, bake it out, replace the ignitor, or rebuild the detector.

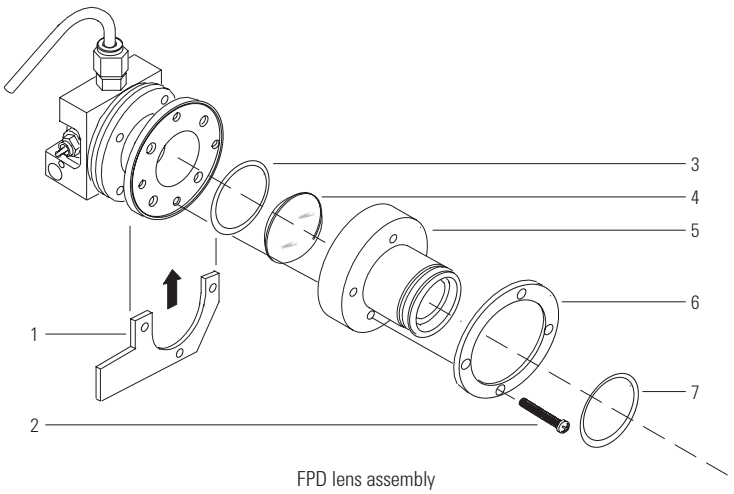

FPD lens assembly

FPD Photomultiplier Tube (PMT) and Bracket Assemblies

Description	Part No.
Chimney back cover	G1535-80520
Heator/sensor assembly	G1535-60610
Transfer line support bracket	19256-00320
Bracket/support	G1535-00010
Sulfur filter, 7890 and late model 6890*	1000-1437
Sulfur filter, blue, early model 6890*	19256-80000
Phosphorus filter, yellow	19256-80010
Filter spacer (used only with sulfur filter)	19256-20910
PMT housing assembly	19256-60510
Dual FPD chimney front	G1535-00030

*Please contact Agilent technical support for assistance in selecting the correct sulfur filter for your 6890 FPD detector.

Nitrogen Phosphorus Detector (NPD)



NPD Beads

The NPD for the 7890/6890 GC features a ceramic bead selective for nitrogen and phosphorous compounds. Agilent offers three beads:

- Blos bead
- White ceramic bead
- Black ceramic bead

Compared to the white ceramic bead, the new Blos bead provides:

- Superior bead lifetime
- Faster attainment of stable operation at initial start-up, as well as more stable operation throughout bead's lifetime
- Superior sensitivity and selectivity for phosphorous-containing compounds
- Similar sensitivity and selectivity for nitrogen-containing compounds
- Superior immunity to moisture

The white ceramic bead exhibits some tailing for phosphorous compounds. The black ceramic bead does not exhibit peak tailing and typically has a longer lifetime than the white bead; however, it is less sensitive.

All Agilent NPD beads are preconditioned, self-aligning for installation and include a proof-of-performance chromatogram.

NPD Beads

Description	Part No.
Blos NPD bead assembly	G3434-60806
NPD white ceramic bead assembly	G1534-60570
NPD black ceramic bead assembly	5183-2007



Blos NPD bead assembly, G3434-60806



NPD Gas Flow

The hydrogen, air and makeup gas flows should be measured frequently. They can drift over time or be changed unintentionally without knowledge of it occurring. Each gas flow should be measured independently to obtain the most accurate values. NPDs are very sensitive to changes in the gas flows and consistent flows are necessary to maintain performance levels.

Measuring NPD Flows

1. Set the bead voltage to 0.0 V.
2. Cool the NPD to 100 °C.
3. Remove the bead and store it carefully until re-installation.
4. Insert the NPD flow meter adapter tool into the NPD collector.
5. Attach the flow-measuring insert to the NPD flow meter adapter tool.
6. Place the flow meter tubing over the flow-measuring insert to begin measuring flows.

NPD Gas Purity

Because of its high sensitivity, the NPD requires very pure gases (99.999% or better). We strongly recommend that moisture and hydrocarbon traps be used on the carrier gas and all detector gases, including the detector hydrogen, air, and makeup gases. Dirty gases will not only give poor chromatographic performance, but will shorten the bead life as well.

TIPS & TOOLS

Agilent has a comprehensive offering of GC columns, designed and manufactured to provide excellent and reproducible performance for the benign to the most difficult types of samples. Learn more at **www.agilent.com/chem/mygccolumns**



Cleaning and Replacement

The NPD requires periodic cleaning. In most cases, this only involves the collector and the jet. Agilent provides brushes and wires that simplify the cleaning of all detector parts. The brushes are used to dislodge particulates clinging to the metal surfaces. A fine wire is used to clean the jet opening of particulates. Do not force too large a wire or probe into the jet opening or the opening will become distorted. A loss of sensitivity or poor peak shape may result if the opening is deformed. The various parts can be ultrasonicated after cleaning with a brush. Eventually the jet needs to be replaced, so it is strongly recommended to have spare jets on hand.

Over time, residue from the bead or sample can build up in the collector and cause baseline problems. You should clean the collector after you have damaged the bead two or three times.

The metal C-rings wear slightly with each assembly and disassembly. After several assemblies and disassemblies (five or more), the rings may not seal effectively, causing an erratic baseline. A ceramic insulator and seal kit is available (P/N 5182-9722). Always cool the detector to near-ambient when changing seals and insulators.

Because there is no flame in the NPD, the jet does not collect silica and soot as does the FID jet. Although you can clean the jet, it is more practical to simply replace dirty jets with new ones. If you do clean the jet, use the cleaning wire, taking care not to damage the inside of the jet. You can also use a sonicator bath to clean the jet.

Contaminants

Some chemical problems can also arise when using the NPD. Because it is a trace detector, be careful not to contaminate the analytical system.

Glassware

Glassware must be very clean. Phosphate detergents should be avoided, so acid washing of glassware followed by distilled water and solvent rinsing is recommended.

Solvents

Solvents should be checked for purity. Chlorinated solvents and silanizing reagents can decrease the useful lifetime of the alkali source; excess reagent should be removed prior to injection, if possible.

Other Contamination Sources

Phosphate-containing leak detectors, phosphoric acid-treated columns or glass wool, polyimide-coated columns, or nitrogen-containing liquid phases can add noise to the system and should be avoided.

NPD Jet Identification and Selection


Before ordering parts for NPD maintenance, determine which type of NPD is installed on your GC. The NPD is available in two versions:

- Dedicated, Capillary Optimized: for capillary columns only
- Adaptable: for packed or capillary columns

Hint: Adaptable jets are longer than dedicated capillary jets.


NPD Jets

Description	Jet Tip ID	Length (mm)	Part No.
Jets for capillary optimized fittings			
Capillary with extended jet (recommended)	0.29 mm (0.011 in)	51.5	G1534-80580
Capillary	0.29 mm (0.011 in)	42.8	G1531-80560
Capillary	0.47 mm (0.018 in)	42.8	G1531-80620
Jets for adaptable fittings			
Capillary with extended jet (recommended)	0.29 mm (0.011 in)	70.5	G1534-80590
Capillary	0.29 mm (0.011 in)	61.5	19244-80560
Capillary	0.47 mm (0.018 in)	61.5	19244-80620
Packed	0.46 mm (0.018 in)	63.5	18710-20119

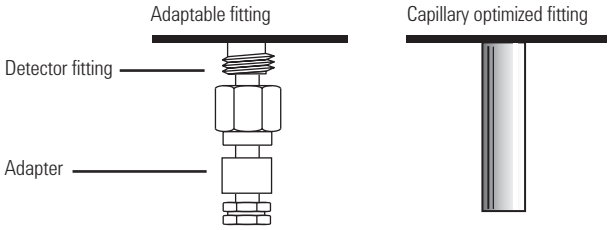

7890/6890/6850 Nitrogen Phosphorus Detector (NPD) Supplies

Item	Description	Part No.
1	Screws, M3 x 0.5, 8 mm (Pozidriv)	0515-0655
2	NPD white ceramic bead assembly	G1534-60570
	NPD black ceramic bead assembly	5183-2007
3	Lid weldment	G1534-80510
4	Metal C-ring, top	0905-2580
5	Alumina insulator, upper	G1534-40020
6	Collector funnel	G1534-20530
7	Alumina insulator, lower	G1534-40030
8	Metal C-ring, bottom	0905-1284
9	Screw, M4 x 07, 10 mm	0515-2495
10	J-Clamp	1400-0015
11	Screw, M4 x 07, 10 mm	0515-2495
12	NPD interconnect assembly	G1534-60610
13	Mounting pallet	G1531-40020
14	Jet, 0.011 in/0.29 mm id tip, capillary dedicated	G1531-80560
	Jet, 0.011 in id tip, capillary adaptable	19244-80560
	Jet, packed standard 0.018 in id tip	18710-20119
15	Base weldment, capillary NPD for 6890/6850 only	G1534-80500
	Base weldment, packed NPD for 6890/6850 only	G1534-80540
	Base weldment, capillary NPD, 7890A	G3434-67500
	Base weldment, packed NPD, 7890A	G3434-67540
16	Lid stop	G1534-20590
	NPD ceramic insulator kit Includes items 4, 5, 7, and 8	5182-9722
17	FID/NPD adapter for capillary column	19244-80610
	FID/NPD 1/8 in packed column	19231-80520
	FID/NPD 1/4 in packed column	19231-80530
18	Insulating cup	19234-60720
	Vespel ferrule, 1/4 in, 10/pk	5080-8774
	530 µm, 1.0 mm id graphite ferrule, 10/pk	5080-8773
	320 µm, 0.5 mm id graphite ferrule, 10/pk	5080-8853
	1/4 in nut, brass, 10/pk	5180-4105
	Universal column nut, 2/pk	5181-8830
	Nitrogen Phosphorus Detector sample	18789-60060

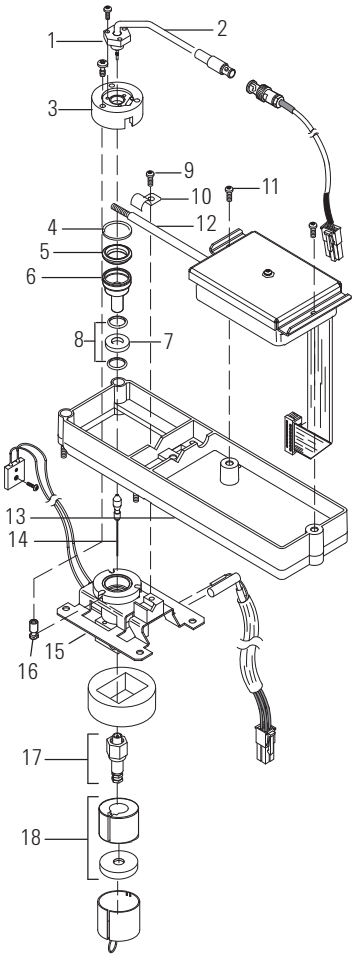

Nitrogen Phosphorus Detector (NPD) assembly



Nitrogen Chemiluminescence Detector (NCD)

Nitrogen and Sulfur Chemiluminescence Detectors

The Agilent 355 Sulfur Chemiluminescence Detector (SCD) is the most sensitive and selective chromatographic sulfur detector available for the analysis of sulfur compounds.

The Agilent 255 Nitrogen Chemiluminescence Detector (NCD) is a nitrogen-specific detector that produces a linear and equimolar response to nitrogen compounds based on a chemiluminescent reaction of NO with ozone. Even complex sample matrices can be analyzed with little or no interference.



Dual plasma burner accessory kit, G6600-60038



Replacement oil coalescing filter, G6600-80042



Replacement oil coalescing filter for oil mist filter, G6600-80044



Replacement odor filtration element, G6600-80045

Nitrogen Chemiluminescence Detector (NCD) Supplies

Description	Part No.
Dual plasma burner accessory kit Includes ferrules, fittings and quartz tube	G6600-60038
PM Kit, DP RV5 oil pump Includes 6 chemical traps for ozone destruction, 3 oil coalescer elements and 4 (1 qt) bottles of synthetic oil	G6600-67007
PM Kit, dry piston pump Includes 4 chemical traps for ozone destruction and 2 repair kits for pump	G6600-67008
12-month maintenance kit Includes 6 qt oil, 12 chemical traps, 4 oil filter elements, 2 sets of ceramic tubes, and 2 O-rings	G6600-67009
Replacement oil coalescing filter	G6600-80042
Oil mist filter for RV5 pump	G6600-80043
Replacement oil coalescing filter for oil mist filter	G6600-80044
Replacement odor filtration element	G6600-80045
O-ring, 1.3614 in id	G6600-80050
O-ring, 1.301 in id	G6600-80051
Dual plasma quartz tube	G6600-80063
Mobil 1 synthetic oil	G6600-85001
Oil, Edwards Ultragrade for RV3 and RV5 pumps	G6600-85002
Spare column nut and ferrule kit	G6600-80018

Sulfur Chemiluminescence Detector (SCD) Supplies

Description	Part No.
PM Kit, dry piston pump Includes dry piston seal, 6 Moleculite vacuum pump traps and 1 set of ceramic tubes	G6600-67006
PM Kit, dry piston pump Includes 4 chemical traps for ozone destruction and 2 repair kits for pump	G6600-67008
Dual plasma burner accessory kit	G6600-60037
Mobil 1 synthetic oil	G6600-85001
Oil mist filter for RV5 pump	G6600-80043
Oil, Edwards Ultragrade for RV3 and RV5 pumps	G6600-85002
O-ring, 1.301 in id	G6600-80051
Ozone destruction chemical trap	G6600-85000
Replacement oil coalescing filter for oil mist filter	G6600-80044
Sulfur chemiluminescence test sample	G2933-85001
Sulfur trap For carrier H_2 and air gases; one required for each cylinder of gas (3 total)	G2933-85003
Spare column nut and ferrule kit	G6600-80018

Miscellaneous Instrument Parts and Supplies

Description	Part No.
Oven exhaust deflector for 6890	G1530-80650
Oven exhaust deflector for 6850	G2630-60710



Sulfur Chemiluminescence Detector (SCD)



PM kit, G6600-67008



Dual plasma burner accessory kit, G6600-60037



Oil mist filter, G6600-80043

GC Standards

GC Qualitative Standards

Description	Part No.
Qualitative Simulated Distallation Standards	
Boiling Point Calibration Sample No. 1	5080-8716
Low Boiling Point Calibration Sample No. 220	5080-8768
Boiling Point Calibration Sample No. 320	5080-8769
PolyWax 500, 1 g, neat	5188-5316
PolyWax 655, 1 g, neat	5188-5317
Qualitative Petrochemical Standards	
Alcohol in Gasoline Sample	18900-60640
Natural Gas Sample	5080-8756
Transformer Gas Sample	5080-8759
Refinery Gas Sample	5080-8755
Reference Gas Oil No. 1, Batch 2	5060-9086
Miscellaneous Qualitative Standards	
Nickel Catalyst Test Sample	19354-60510
Nickel Catalyst refill	5080-8761
MIDI System Calibration Standard	19298-60500
Oral Fluids Analyzer Test Sample	G1540-85010

GC/MS Parts and Supplies



Your mass spectrometer is a sensitive, specialized device that delivers a higher level of functionality than other GC detectors. To continue achieving optimal results, it is critical to maintain your system properly by performing the essential tasks within this section. Some of the benefits of maintaining your GC/MSD include:

- Less downtime for repairs
- Longer lifetime for your MSD system
- Reduction in overall operating costs

It is advisable to keep a log book of system performance, Autotune, and maintenance operations performed. This makes it easier to identify variations from normal performance and to take corrective action.

Maintenance Schedule

Task	Every week	Every 6 months	Every year	As needed
Tune the MSD				✓
Change injection port liners	✓			
Check the foreline pump oil level	✓			
Gas ballast the foreline pump	✓			
Check the calibration vial		✓		
Replace the foreline pump oil		✓		
Check the diffusion pump fluid	✓			
Replace the diffusion pump fluid			✓	
Replace the dry pump diaphragm seals (MVP55)				✓
Replace the dry pump tip seals (IDP3)			✓	
Replace the traps and filters			✓	
Clean the ion source				✓
Change the carrier gas trap(s) and purifier				✓
Replace worn out parts				✓
Lubricate seals (where appropriate)				✓
Replace column				✓

MSD Contamination

Contamination is usually identified by excessive background in the mass spectra, which can come from the GC or MSD. The source of contamination can sometimes be determined by identifying the contaminants. Some contaminants are much more likely to originate in the GC, while others are likely to originate in the MSD.

Contamination Sources in the GC

- Column or septum bleed
- Dirty injection port
- Injection port liner
- Contaminated syringe
- Poor quality carrier gas
- Dirty carrier gas tubing
- Fingerprints
- Air leaks
- Cleaning solvents and materials

Contamination Sources in the MSD

- Air leaks
- Cleaning solvents and materials
- Fingerprints inside the manifold
- Diffusion pump fluid
- Foreline pump oil

The action required to remove contamination depends on the type and level of contamination. Minor contamination by water or solvents can usually be removed by allowing the system to pump (with a flow of clean carrier gas) overnight. Serious contamination by rough pump oil, diffusion pump fluid or fingerprints is much more difficult to remove and may require extensive cleaning.

Air Leaks

Air leaks are a problem for any instrument that requires a vacuum to operate. Leaks are generally caused by vacuum seals that are damaged or not fastened correctly.

Symptoms of leaks


- Higher than normal vacuum manifold pressure or foreline pressure
- Higher than normal background
- Peaks characteristic of air (m/z 18, 28, 32, and 44 or m/z 14 and 16)
- Poor sensitivity
- Low relative abundance of m/z 502 (this varies with the tune program and MSD used)

Remedy

- Check interface nut for tightness. Replace if necessary.
- Check and leak test the GC injection port.

Leaks can occur in other places in the MSD, including the following:

- GC/MSD interface column nut
- Side/top plate O-ring (all the way around)
- Vent valve O-ring
- Calibration valve
- High vacuum gauge tube/controller fitting
- Cracked ion gauge tube (5973/5972/5971)
- Front and rear end plate O-rings
- GC/MSD interface O-ring (where the interface attaches to the vacuum manifold)
- Diffusion pump co-seal
- Baffle adapter O-ring
- Turbomolecular pump O-ring
- Vespel/Graphite ferrules, when heated

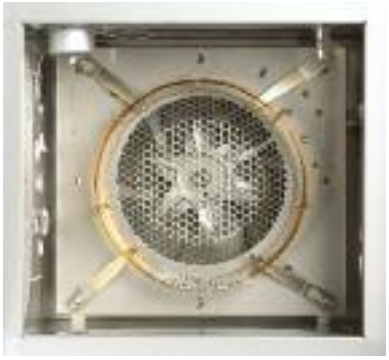

Cleaning Solvents

It is common to see cleaning solvent peaks in the mass spectra shortly after the ion source is cleaned.

Remedy

- Dry all cleaned metal parts in the GC oven before reassembling and reinstalling them. Refer to specific cleaning procedures in your MSD Hardware Manual or MSD Maintenance and Troubleshooting Manual.
- Use a temperature above the boiling point of the solvent but below the limit of the column.

Fingerprints

Fingerprints contain hydrocarbons that can appear in mass spectra. Hydrocarbon contamination is characterized by a series of mass peaks 14 m/z apart. The abundances of these peaks decrease as peak mass increases. Fingerprint contamination is usually caused by the failure to wear lint-free, nylon gloves during ion source cleaning, GC inlet maintenance, or from installing the column. Use special care to avoid recontamination of parts after you clean them. This typically occurs after some maintenance or part replacement.

Remedy

Reclean using clean, nylon gloves and proper cleaning techniques.

MSD Contamination Identification

The following table lists some of the more common contaminants, the ion characteristics of those contaminants, and the likely sources of those contaminants.

Common Contaminants

Ions (m/z)	Compound	Possible Source
13, 14, 15, 16	Methane	CI gas
18, 28, 32, 44 or 14, 16	H_20, N_2, O_2, CO_2, CO_2 or N, O	Residual air and water, air leaks, outgassing from Vespel ferrules
31, 51, 69, 100, 119, 131, 169, 181, 214, 219, 264, 376, 414, 426, 464, 502, 576, 614	PFTBA and related ions	PFTBA (tuning compound)
31	Methanol	Cleaning solvent
43, 58	Acetone	Cleaning solvent
78	Benzene	Cleaning solvent
91, 92	Toluene or Xylene	Cleaning solvent
105, 106	Xylene	Cleaning solvent
151, 153	Trichloroethane	Cleaning solvent
69	Foreline pump fluid or PFTBA	Foreline pump oil vapor or calibration valve leak
73, 147, 207, 221, 281, 295, 355, 429	Dimethylpolysiloxane	Septum bleed or methyl silicone column coating
77, 94, 115, 141, 168, 170, 262, 354, 446	Diffusion pump fluid	Diffusion pump fluid and related ions
149	Plasticizer (phthalates)	Vacuum seals (O-rings) damaged by high temperatures, use of vinyl or plastic gloves
Peaks spaced 14 amu apart	Hydrocarbons	Fingerprints, foreline pump oil

The easiest way to insure that you minimize background contamination and remove damaging oxygen from your carrier gas system is to use a carrier gas purifying trap right before the gas enters your GC system.

Column bleed generally appears as a continuous and increased rise in the baseline at higher column temperatures, especially at or near the upper temperature limit of the GC column. Septum bleed usually appears as discrete peaks, and can occur at any temperature.

A crude sign of a "leak-free" MS system is when the ion ratio of m/z 28 (nitrogen) over m/z 32 (oxygen) is approximately two or greater.

Even preconditioned ferrules can shrink slightly at very high temperatures. If leak problems persist upon a new column installation, check this fitting first.

Mass Spectrometer Symptoms

Mass spectrometer symptoms can typically be classified as either affecting system sensitivity or affecting the repeatability of a measurement. Most symptoms can be corrected by following the suggested corrective actions.

Mass Spectrometer Symptoms

Symptoms	Remedy
Sensitivity	
Wrong retention time	Check GC, method, application and carrier gas velocity.
Low signal	Check GC, tune vacuum system.
Leaking injection port	Clean the injection port. Replace the injection port liner and septa.
Air leak	Check and tighten interface nut, leak test GC injection port.
Peak widths	Do Autotune, check flow rate and temperature stability.
Interfering peaks	Check time parameters, coeluting peaks, column type.
Excessive background	Do Autotune and compare to background specifications. Check time parameters.
Incorrect mass assignment	Retune.
Abnormal spectra – excessive background contamination	Check for contamination.
Incorrect tuning	Check tune file, retune, check sample.
Repeller voltage is too low	Raise voltage to test for response.
Dirty ion source	Clean source.

(Continued)

Mass Spectrometer Symptoms	
Symptoms	**Remedy**
Repeatability	
Dirty syringe needle	Clean or replace the syringe.
Wrong syringe needle	Replace syringe and septa.
Leaking injection port	Perform injection port maintenance. Replace the injection port liner, septa and liner O-ring.
Injection is too large	Check method and injection volume, split ratio and/or splitless purge time.
Loose column connections	Tighten column nuts on injection port or transfer line. Replace column nuts and ferrule.
Variations in pressure, column flow and temperature	Ensure the MSD is located in an environment where the temperature is stable. Keep MSD out of drafts and direct sunlight. Check that the carrier gas is steady and well regulated. Service the foreline pump and/or diffusion pump.
Dirty ion source	Clean source.
Loose connections in the analyzer	Check internal and external analyzer wiring conections, make sure all are secure.
Ground loops	Check main electrical lines.



5975 MSD

Cleaning and Maintenance Supplies

Description	Part No.
One Year Maintenance Kit (for diffusion pump systems) Includes Big Universal Trap for He (1/8 in), abrasive sheets (5/pk), lint-free cloths (15/pk), cotton swabs (100/pk), SantoVac Ultra, 18.5 mL (2 each), rough pump oil (1 L), filament assembly, octafluoronapthalene (OFN)	5183-2096
Nylon gloves, lint-free, large, 1 pair	8650-0030
Nylon gloves, lint-free, small, 1 pair	8650-0029
Lint-free industrial wipes, 100% cotton, 9 x 9 in, 300/pk	9310-4828
Ion source cleaning kit Includes lint-free cloths (15/pk), abrasive sheets (5/pk), cotton swabs (100/pk), lint-free nylon gloves, abrasive Alumina powder	5181-8863
Cloths, lint-free, 15/pk	05980-60051
Cotton swabs, 100/pk	5080-5400
Abrasive sheets, aluminum oxide green lapping paper, 600 mesh, 5/pk	5061-5896
Alumina powder, abrasive, 1 kg	8660-0791
PFTBA sample, certified, 10 g, 5.32 mL	8500-0656
Replacement glass bulb for PFTBA and PFDTD test sample	G3170-80002
Replacement glass vial for PFTBA and PFDTD test sample	05980-20018
Activated alumina, absorbent pellets for Edwards rough pump traps, non-LC/MS, 1 lb can	8500-1233
MSD Tool Kit, 5975/5973 Includes source hold tool, lint-free cloth, cotton swabs, lint-free nylon gloves, abrasive sheets, wrenches and driving tools	G1099-60566
MSD Tool Kit, 5972/5971 Includes small cleaning rod, large cleaning rod, source hold tool, cotton swabs, lint-free nylon gloves, abrasive sheets, wrenches and driving tools	05971-60561

(Continued)

Cleaning and Maintenance Supplies

Description	Part No.
MS Interface Supplies	
MS interface column nut, female	05988-20066
Column nut for long or long two-hole ferrules	05921-21170
Universal column nut, 2/pk	5181-8830
MS interface column installation tool for 5973 and 5975	G1099-20030
Column installation tool for 5975T	G3880-20030
Tools	
Screwdriver, 3 in Pozidriv shaft No. 1 pt, fits no. 2-4 screws	8710-0899
Screwdriver, 4 in Pozidriv shaft No. 2 pt, fits no. 5-10 screws	8710-0900
Open end wrench, 1/4 and 5/16 in	8710-0510
Hex nut driver, 5.5 mm	8710-1220
Screwdriver, Torx T20	8710-1615
Screwdriver, Torx T15	8710-1622
Screwdriver, Torx T10	5182-3466
Ferrules	
0.4 mm Vespel/Graphite ferrule for 200/250 µm columns, 10/pk	5062-3508
0.5 mm Vespel/Graphite ferrule for 320 µm columns, 10/pk	5062-3506
250 µm Vespel/Graphite ferrule, 10/pk	5181-3323
SilTite metal ferrules for 1/16 in od tubing, 10/pk Includes 2 column nuts	5184-3571
SilTite metal ferrules, 1/16 in x 0.4 mm id, 10/pk Includes 2 column nuts	5184-3569
SilTite metal ferrules, 1/16 in x 0.5 mm id, 10/pk Includes 2 column nuts	5184-3570
Ferrule pre-swaging tool	G2855-60200
Plug for microfluidic manifold or unions	G2855-60570



MS interface column nut, 05988-20066



Universal column nut, 5181-8830



Column installation tool, G1099-20030



Vespel/Graphite ferrules, 5181-3323



Electron Impact (EI) Ion Source

Ion Source

The ion source operates by electron ionization (EI) or chemical ionization (CI). The sample enters the ion source from the GC/MSD interface. Electrons emitted by a filament enter the ionization chamber, guided by a magnetic field. The high-energy electrons interact with the sample molecules, ionizing and fragmenting them. The positive voltage on the repeller pushes the positive ions into the lens stack, where they pass through several electrostatic lenses. These lenses concentrate the ions into a tight beam, which is directed into the mass filter.

Maintaining the Ion Source

Cleaning procedures for MSDs vary. Refer to your Troubleshooting and Maintenance Manual for specific ion source cleaning procedures.

Common Measures of Instrument Performance

- Abundance of certain ions (e.g., percentage of the 502 ion from the Autotune report)
- Shape of lens ramps and the chosen voltages, especially Repeller Ramp
- Sensitivity obtainable for a given analysis
- Ability to tune to a given reference compound (e.g., DFTPP)

Preparing to Clean

Prior to cleaning, the mass spectrometer must be vented and the ion source must be removed. Before venting the system, the following conditions must be met:

- Heated zones are less than 100 °C
- The diffusion pump is off and cool
- The turbo pump is off and not spinning
- The rough pump is off

Always allow the automatic venting routine to run its full course. Improper venting may cause diffusion pump fluid to be deposited into the analyzer (backstreaming). It can also reduce the life of the multiplier or other sensitive MS parts.

MSD Flow Rates (mL/min)

	Min	Max Diff Pump	Max Turbo Pump	Tuning Max
5975	0.1	2.0	4.0	2.0
5973	0.1	2.0	4.0	2.0
5972	0.1	2.0	N/A	2.0
5971	0.1	1.5	N/A	1.0
GCD	0.1	1.0	N/A	1.0

WARNINGS & CAUTION

Important: Do not abrasively or ultrasonically clean the insulators.

Abrasively clean the surfaces that contact the sample or ion beam. Use an abrasive slurry of alumina powder and reagent-grade methanol on a cotton swab. Use enough force to remove all discoloration. Polishing the parts is not necessary; small scratches will not harm performance. Abrasively clean discoloration where electrons from filaments enter the source body.

Take care to avoid contaminating cleaned and dried parts. Put on new, clean gloves before handling the parts. Do not put the cleaned parts on a dirty surface. Place them only on clean, lint-free cloths.

TIPS & TOOLS

It is good practice to replace scratched lenses and other ion source parts regularly. Scratched source parts lead to poor performance.

Electron Impact (EI) Ion Source

The recommended cleaning material for the EI ion source is abrasive, aluminum oxide powder.

Do not immerse filaments or lens insulators in solvent. If insulators are dirty, clean them with a cotton swab dampened with reagent-grade methanol. If that does not clean the insulators, replace them.




Electron Impact (EI) Ion Source



Lens insulator, G3170-20530

5975/5973 MSD Electron Impact Ion Source Parts (EI)

Item	Description	Part No.	Inert Part No.
1	Ion source body	G1099-20130	G2589-20043
2	Drawout plate, 3 mm	05971-20134	G2589-20100
	Drawout plate, 6 mm	G3163-20530	G2589-20045
3	Drawout cylinder	G1072-20008	G1072-20008
4	Ion focus lens	05971-20143	05971-20143
4	Lens insulator	G3170-20530	G3170-20530
6	Entrance lens	G3170-20126	G3170-20126
7	Cap screw, gold plated	G1999-20021	G1999-20021
8	High temperature filament	G3170-60050	G3170-60050
9	Transfer line socket	G1099-20136	G1099-20136
10	Repeller insulator	G1099-20133	G1099-20133
11	Repeller	G1099-20132	G2589-20044

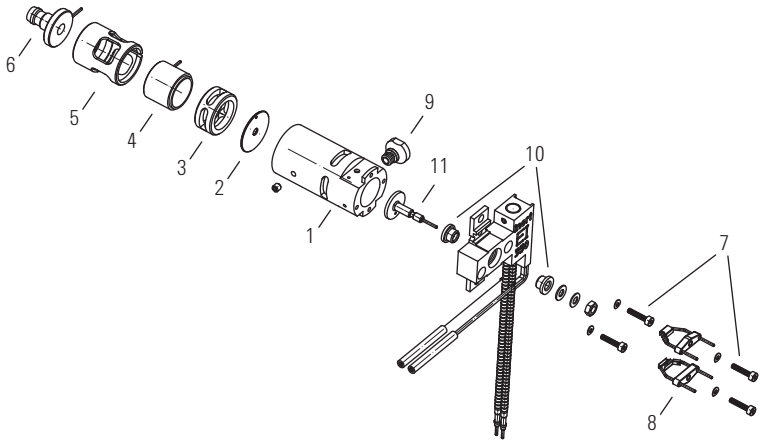

5975/5973 MSD Electron Impact (EI) ion source assembly

Chemical Ionization (CI) Ion Source



Agilent 5975 Ion Source

Because the CI ion source operates at much higher pressures than the EI ion source, it will probably require more frequent cleaning than the EI ion source.

The source should be cleaned whenever there are performance anomalies that are associated with a dirty ion source. Let analytical performance be your guide.

When cleaning the CI ion source, concentrate on the CI repeller, ion source body, and drawout plate. Be sure to clean the 0.5 mm diameter holes in the ion source body and drawout plate.

Cleaning the ion source is very similar to cleaning the EI ion source. Use the same EI cleaning procedure with the following exceptions:


- The CI ion source may not look dirty, but deposits left by chemical ionization are very difficult to remove. Clean the CI ion source thoroughly.
- Use a round wooden toothpick to gently clean out the electron entrance hole in the source body and the ion exit hole in the drawout plate.
- Do not use halogenated solvents. Use hexane for the final rinse.

5975/5973 MSD Chemical Ionization Ion Source Parts (CI)

Item	Description	Part No.
1	Source body	G1999-20430
2	Drawout plate	G1999-20446
3	Drawout cylinder	G1999-20444
4	Ion focus lens	G1999-20443
4	Lens insulator	G3170-20540
6	Entrance lens	G3170-20126
7	Repeller insulator	G1999-20433
8	Repeller	G1999-20432
9	High temperature filament	G1099-80053
10	Cap screw, gold plated	G1999-20021
11	Interface tip seal/spring	G1999-60412

TIPS & TOOLS

Visual appearance is not an accurate guide to cleanliness of the CI ion source. The CI ion source can show little or no discoloration, yet still need cleaning.

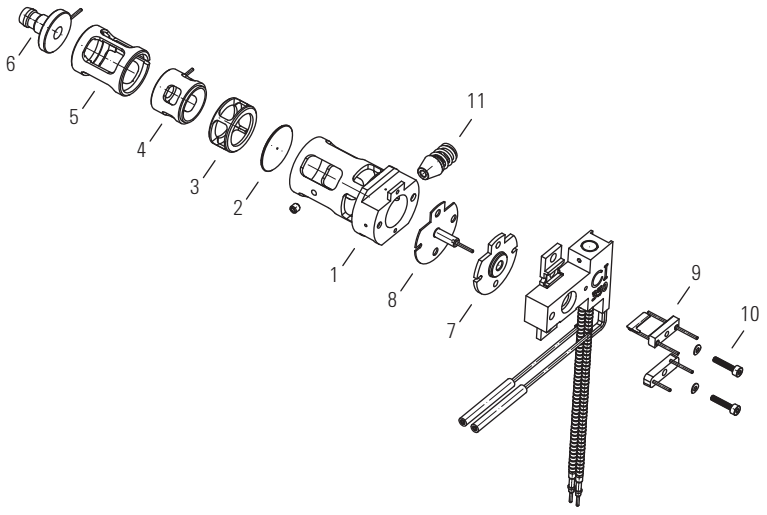


5975/5973 MSD Chemical Ionization (CI) ion source assembly

Installing a Capillary Column in the GC/MSD Interface

1. Condition the column.
2. Vent the MSD and open the analyzer chamber. Be sure you can see the end of the GC/MSD interface.
3. If the CI interface is installed, remove the spring-loaded tip seal from the MSD end of the interface.
4. Slide an interface nut and conditioned ferrule onto the free end of the GC column. The tapered end of the ferrule must point towards the nut.
4. Slide the column into the GC/MSD interface until you can pull it out through the analyzer chamber.
6. Score the column using a glass scribing tool. The score must be square to ensure a clean break.
7. Trim 1 cm off the end of the column. Do not let any column fragments fall into the analyzer chamber. They could damage the turbo pump.
8. Clean the outside of the free end of the column with a lint-free cloth moistened with methanol.
9. Adjust the column.
   - 5975 – Push the column through, and then let it pass the end of the Transferline by 1-2 mm. With the analyzer door partially open, view through the glass plate to see the column protrude.
   - 5973 – Push the column through, and then let it pass the end of the Transferline by 1-2 mm as seen with the analyzer door open from that side.
   - 5972 – Push the column in all the way and then pull it back about 1-2 mm.

   Use the flashlight and magnifying glass if necessary to see the end of the column inside the analyzer changer. Do not use your finger to feel for the column end.
10. Hand-tighten the nut. Make sure the position of the column does not change as you tighten the nut. Reinstall the spring-loaded tip seal if it was removed earlier.
11. Check the GC oven to be sure that the column does not touch the oven walls.
12. Tighten the nut 1/4 to 1/2 turn. Check the tightness after one or two heat cycles.

Installing a capillary column in the GC/MSD interface

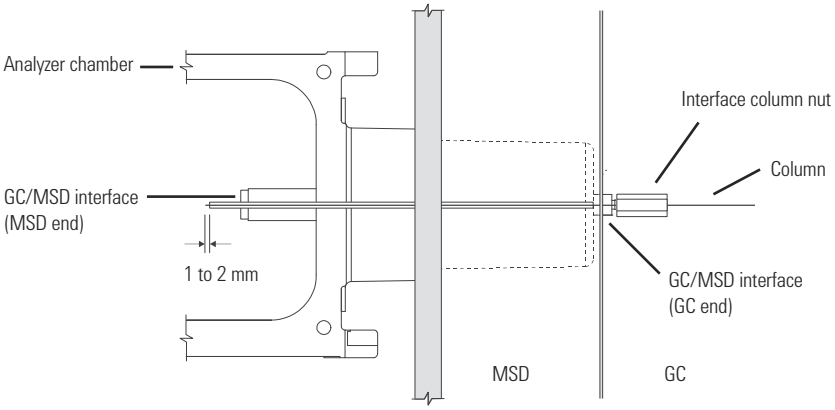


TIPS & TOOLS

The column installation procedure for 5975 MSDs is different from that for most previous MSDs. Using the procedure from another instrument may result in poor sensitivity and possible damage to the MSD.

TIPS & TOOLS

Agilent J&W GC Columns offer the lowest bleed levels, the best inertness for acids/bases/mixed functional compounds, and the tightest column-to-column reproducibility. Learn more at **www.agilent.com/chem/mygccolumns**

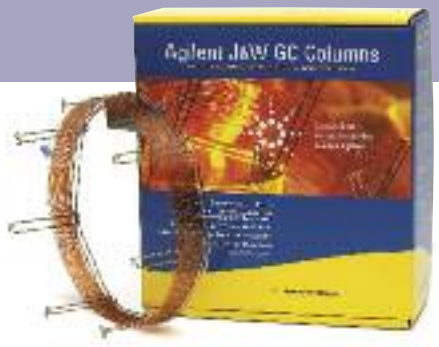



QuickSwap Capillary Flow Technology module

QuickSwap MS Interface Restrictors

Agilent's QuickSwap Capillary Flow Technology module and pre-swaged fused silica tubing restrictors can increase the productivity of your Agilent 5973N and 5975 Inert MSD Systems, allowing you to change columns without venting the MSD. QuickSwap not included.

These restrictors are prefabricated for convenience and ease-of-use. For applications requiring other restrictor sizes, Agilent offers a wide variety of deactivated fused silica tubing, SilTite ferrules and swaging tools.

QuickSwap MS Interface Restrictors

Description	ID (mm)	Unit	Part No.
QuickSwap restrictor	0.092	4/pk	G3185-60361
QuickSwap restrictor	0.100	4/pk	G3185-60362
QuickSwap restrictor	0.110	4/pk	G3185-60363
QuickSwap restrictor	0.120	4/pk	G3185-60364
QuickSwap restrictor variety pack, 2 each of the above id restrictors			G3185-60300



SilTite metal ferrules, 5188-5361

SilTite Metal Ferrules

Description	Unit	Part No.
For use with 0.25 mm id capillary columns	10/pk	5188-5361
For use with 0.32 mm id capillary columns	10/pk	5188-5362
For use with 1/16 in od stainless steel tubing Includes 2 column nuts	10/pk	5184-3571
For use with 0.53 mm id capillary columns	10/pk	5188-5363

MSD Filaments



Filament assembly (EI), G3170-60050

Like the filaments in an incandescent light bulb, the ion source filaments will eventually burn out. Certain practices will reduce the chance of early failure.

- When setting up data acquisition parameters, set the solvent delay so that the analyzer will not turn on while the solvent peak is eluting
- When the software prompts 'Override solvent delay at the beginning of a run' always select 'No'
- Higher emission current will reduce filament life
- If you control your MSD from the Edit Parameters screen, always select 'MS Off' before changing any of the filament parameters

MSD Filaments

Description	5975 Series	5975T Series	5973 Series	5972 Series	5971 Series
Filament assembly (EI)	G3170-60050		G3170-60050	G3170-60050	05971-60140
Filament assembly (CI)	G1099-80053		G1099-80053		
Micro ion vacuum gauge	G3170-80001				
Triode gauge tube for measuring vacuum			0960-0897		
Ion gauge controller		G3880-80010			
Ion gauge tube		G3880-80011			

TIPS & TOOLS

It is very useful to switch from one filament to the other every three months so that when a filament fails, you know the other will fail soon. This will allow you to change both filaments at the same time. Since the GC/MS system is already vented, it's a good idea to replace other supplies in the flowpath at the same time as the filaments.



Quadrupole Mass Filter

The mass filter does not require periodic maintenance. It should not be removed from the radiator or disturbed in any way.

- Never put the quadrupole in an ultrasonic cleaner.
- Never change the physical orientation of the quadrupole mass filter.
- The fused-quartz quadrupole is fragile and will break if dropped or handled roughly.
- The material in the cusps of the quadrupole is very hygroscopic. If exposed to water, the quadrupole must be dried very slowly to prevent damage.
- Cleaning techniques that are appropriate for other manufacturers' instruments are not suitable for Agilent MSDs – and may actually harm the mass filter.
- To save time and effort, use only Agilent MSD mass filters, which do not require periodic cleaning or maintenance.
- In case of extreme contamination, contact a trained Agilent service representative to perform the mass filter cleaning.

MSD Electron Multipliers and Replacement Horn



Electron multiplier replacement horn

The lifetime of an electron multiplier is directly related to the current that flows through it and the extent of contamination or condensation that it experiences. Replace the electron multiplier or replacement horn when voltage is over 2500 V. To maximize electron multiplier life:

- Maintain the best possible vacuum, especially in the analyzer manifold
- Use extreme caution and be conservative with venting, pumpdown, and all vacuum system procedures to keep pump fluid background to a minimum
- After venting, allow four hours for pumpdown and thermal equilibration before scanning
- Actively look for background contamination and leaks and repair them immediately
- Don't tune excessively – PFTBA can result in higher background over an extended period of time
- Replace the electron multiplier if vacuum is poor or voltage is over 2500 V

MSD Electron Multipliers and Replacement Horn

Description	5975 Series	5973 Series	5972/5971 Series
Electron multiplier replacement horn Use with electron multipliers with "straight" horns	05971-80103	05971-80103	05971-80103
Triple axis detector assembly*	G3170-80100		
Triple axis electron multiplier	G3170-80103		
EM signal wire, low noise detector	G3170-80008		
High energy dynode		G1099-80001	
Electron multiplier			05971-80102

*Included on 5975 triple axis detector systems

TIPS & TOOLS

The Agilent multipliers and horns listed are recommended for your MSD. Other manufacturers' products may be incompatible with Agilent instruments and can result in reduced sensitivity, lifetime, and noise problems.



Vacuum Systems and Pumps

The vacuum system creates the high vacuum (low pressure) required for the MSD to operate. Without this vacuum, the molecular mean free path is too short.

Ions cannot travel from the ion source through the mass filter to the electron multiplier (detector) without colliding with other molecules.

The main components of the vacuum system are:

- Vacuum manifold
- Foreline gauge
- Calibration valve
- Gauge controller (optional)
- Vacuum seals
- Foreline pump and/or trap
- Diffusion/turbo pump and fan
- High vacuum gauge tube

Pressure Symptoms

This section describes unusual pressure readings and their possible causes. The symptoms in this section are based on typical pressures. At typical column flow rates (0.5-2.0 mL/min), the foreline pressure will be approximately 20 to 100 m Torr. The vacuum manifold pressure will be approximately 1 x 10^{-6} to 1.4 x 10^{-4} Torr.

These pressures can vary widely from instrument to instrument, so it is important that you are familiar with the pressures that are typical for your instrument at a given carrier gas flow and oven temperature.

The foreline pressures listed can only be measured on diffusion pump-equipped systems. Turbomolecular pumps are controlled according to their speed and do not have foreline pressure gauges.

The vacuum manifold pressures can only be measured if your system is equipped with the optional gauge controller.

TIPS & TOOLS

Keeping a pan under the vacuum pump helps to detect and identify the origin of oil leaks.

Pressure Symptoms

Symptoms	Possible Causes
Foreline pressure is too high	
• Pressure is above 100 m Torr. • Pressure for a given column flow has increased over time	• Column (carrier gas) flow is too high • Wrong carrier gas • Air leak (normally at transferline interface) • Foreline pump oil level is low or oil is contaminated • Foreline hose is constricted • Foreline gauge is not working correctly • Foreline pump is not working correctly
Foreline pressure is too low	
• Pressure is below 20 m Torr.	• Column (carrier gas) flow is too low • Wrong carrier gas • Column plugged or crushed by an overtightened nut • Empty or insufficient carrier gas supply • Bent or pinched carrier gas tubing • Foreline gauge is not working correctly
Vacuum manifold pressure is too high	
• Pressure is above 1.4×10^{-4} Torr. • Pressure for a given column flow has increased over time	• Column (carrier gas) flow is too high • Wrong carrier gas • Air leak • Foreline pump is not working correctly • Diffusion pump fluid level is low or fluid is contaminated • Defective gauge controller • Faulty ion gauge tube
Vacuum manifold pressure is too low	
• Pressure is below 1.4×10^{-4} Torr.	• Column (carrier gas) flow is too low • Wrong carrier gas • Column plugged or crushed by an overtightened nut • Empty or insufficient carrier gas supply • Bent or pinched carrier gas tubing • Defective gauge controller • Faulty ion gauge tube



Diffusion Pump

It is not necessary to change the diffusion pump fluid more than once a year, unless you observe symptoms that suggest a problem with the fluid. The MSD must be vented in order to check the diffusion pump fluid (except for the 5975/5973). Therefore, the best time to check the fluid is when the instrument is already vented for other maintenance.

How to Check the Fluid Level

5972/5971 Series

1. If it is not vented already, shut down and vent the MSD according to instrument manual.
2. Unplug the MSD power cord.
3. Remove the pump and cover the top with aluminum foil.
4. After heating the pump in a GC oven at 60 °C for 15 minutes to make the fluid flow down into the reservoir at the bottom, remove the stack parts.
4. Inspect the pump fluid. If the fluid is discolored or contains particulate material, the fluid must be changed.
6. Use a metal ruler to determine the depth of the fluid. A pump that has been in operation should have a pool 9 mm +/- 1 mm deep. Fluid in freshly charged pumps will be 12 mm deep. It is normal that up to 2 mL of oil may be in the rear portion of the vacuum manifold. The recommended total fluid charge for the 5971/5972 is 18 mL (+/- 2 mL).

5975/5973 Series

- Use the sight glass to determine the depth of the fluid. The recommended total fluid charge is approximately 37 mL.

Foreline Pump

The oil in the foreline or rough pump should be replaced on average once every six months, but can vary depending upon applications. If a foreline trap is present, the molecular sieves should also be replaced after an oil change.

Avoid contact with the pump oil. The residue from some samples may be toxic. Dispense of used oil properly.



Foreline Pump

Pump Oils

Description	Part No.
Foreline pump (rotary pump) oil, Inland 45, 1 L	6040-0834
High vacuum grease, 25 g	6040-0289
Diffusion pump fluid, 18.5 mL	6040-0809*
IDP Series tip seal kit for 5975T	IDP3TS
Oil mist exhaust filter	G1099-80039

*2 required for 5975 and 5973 Series



General Instructions on How to Replace the Pump Oil

1. Vent and shut down the MSD.
2. Place a container under the drain plug on the foreline pump.
3. Remove the fill cap from the top of the pump to expose the fill hole.
4. Remove the drain plug from the pump.
5. Reconnect the MSD to its power source. Switch on for 2 or 3 seconds, and then switch it off again. This displaces old oil from the internal pump cavities. Disconnect the power cord again.
6. Reinstall the drain plug and pour pump oil into the fill hole.
7. Reinstall the fill cap.
8. Reconnect the MSD power cord.
9. Start up and pump down the MSD according to the Instrument Manual procedure.



7000A Triple Quadropole GC/MS

7000A Triple Quadropole GC/MS Parts and Supplies

Engineered from the ground up for ease-of-use and routine high performance operation, the 7000A Triple Quadrapole GC/MS delivers advanced high-speed GC/MS/MS quantitation for ultra-trace analysis of even the most complex samples. Combined with the Agilent 7890 GC, the result is an optimally robust GC/MS/MS system.

Gas Filters

Description	Part No.
Chemical Ionization Gas Purifier	G1999-80410
Gas Clean GC/MS starter kit 1/8 in	CP17974
Agilent Gas Clean GC/MS filter	CP17973
Mounting clip	UMC-2



Agilent Gas Clean GC/MS filter, CP17973

Foreline Pump Supplies

Description	Part No.
Diffusion pump fluid, 18.5 mL	6040-0809
Foreline pump oil, P3, 0.5 L	6040-0621
Rough pump inlet flange	0905-1463
Oil return kit	3162-1057
Pump oil drip pan	G1946-00034
Oil mist exhaust filter	G1099-80039
Oil mist filter for RV5 pump	G6600-80043



Oil mist filter, G6600-80043

Maintenance Supplies

Description	Part No.
Abrasive sheets	5061-5896
Alumina powder, abrasive, 1 kg	8660-0791
Cloths, lint-free	05980-60051
Lint-free industrial wipes, 100% cotton	9310-4828
Cotton swabs	5080-5400
Nylon gloves, lint-free, large	8650-0030
Nylon gloves, lint-free, small	8650-0029
High vacuum grease, 25 g	6040-0289
Electron multiplier replacement horn	05971-80103
Low noise EM horn	G3170-80103
Filament assembly, high temperature (EI)	G3170-60050
Filament assembly (CI)	G1099-80053
Micro ion vacuum gauge	G3170-80001
Replacement glass bulb for PFTBA and PFDTD test sample	G3170-80002



Low noise EM horn, G3170-80103



Filament assembly (EI), G3170-60050



240-MS Ion Trap Parts and Supplies

The Agilent 240-MS Ion Trap delivers unparalleled capabilities for both research and routine applications. Advanced ionization, including positive and negative chemical ionization, improves selectivity and limits of detection. Enhanced scanning techniques ensure compound confirmation. The MS/MS and MS^n reduce matrix influences and provide more detailed structural information. The software comes with a full complement of productivity, reporting, and regulatory compliance tools.

- Accurate identification and quantification of trace analytes
- Unsurpassed sensitivity (200 femtogram OFN full scan)
- Choice of internal or external ionization configurations
- Powerful MS/MS and CI options
- Low maintenance and high reliability
- Intuitive software for increased productivity

240-MS Ion Trap Parts and Supplies

Description	Part No.
Manifold O-ring	393010924
Transfer line inner O-ring	393010920
Transfer line outer O-ring	393010918
Internal filaments (2 filaments on one disk)	392017401
Internal transfer line tip	393171201
External filament (single filament)	393161001
Electrode, end cap, SilChrom	393164493
Electrode set kit, SilChrom, DFC (inert) tested Includes 2 end cap electrodes, 1 RF electrode, cleaning instructions	9300003590
Electrode, RF, SilChrom	393167593
Spacer, RF, Silco-quartz	393053502
Electron multiplier	393175101
Transfer line assembly upgrade field kit Contains a complete transfer line and side-mounted block for vacuum manifold	393101291
EPA volatile kit for EPA methods 524.2 & 8260B	393082491
ChromatoProbe microvials, 100/pk	392567111

TIPS & TOOLS

Need GC supplies for your non-Agilent instruments? Check out the Agilent CrossLab supplies for Bruker/Varian GC Systems.

See pages 154-168

240-MS Ion Trap Parts and Supplies

Description	Part No.
GC/MS Standards	
Evaluation standard (Internal EI & CI) 2 pg/µL OFN, 5 pg/µL	393112601
Test standard for external EI (5 pg/µL OFN)	393112702
Benzophenone CI sensitivity standard 50 pg/mL	392030500
Test standard for external NCI (1 pg /µL DFB)	393113001
Tuning calibration compound PFTBA (FC-43)	392035300
GC/MS column test mix	392027300
Vacuum Supplies	
Oil mist exhaust filter, DS42	393847701
Oil mist eliminator	2735000500
Replacement cartridge for oil exhaust filter, 2/pk	2710100200
Foreline (roughing) pump oil, 1 L	8829951700
Premium foreline (roughing) pump oil, 1 L	8829953800
IDP-3 dry scroll pump tip seal maintenance kit	2710100400
IDP-3 dry scroll replacement module	2710100500





220-MS Parts and Supplies

The 220-MS is a high sensitivity, flexible gas chromatograph/mass spectrometer that delivers outstanding qualitative and quantitative data in a range of applications. This simple and robust system is easy to operate and maintain.

- Accurately identify and quantify trace analytes
- Take advantage of powerful CI and MS/MS upgrades for advanced applications
- Spend less time on maintenance and more time on analysis

220-MS Parts and Supplies

Description	Part No.
Electron multiplier assembly	393031501
Exit end cap electrode, chrome	393050292
Exit end cap electrode, SilChrom	393050293
Filament end cap electrode, chrome	393050392
Filament end cap electrode, SilChrom	393050393
RF ring electrode, chrome	393050492
RF ring electrode, SilChrom	393050493
Complete set of SilChrom electrodes and Silco-quartz spacers	393001991
Spacer, RF, quartz	393053501
Spacer, RF, Silco-quartz	393053502
Filament disk assembly with wire connectors	393060191
Filament disk assembly User must solder on 3 wire connectors	392043700
Thermocouple vacuum gauge	2722990700
Mass spectrometer expendable supplies kit for 2x0MS Includes PFTBA calibration compound, cal-gas glass chamber, capillary injector nut, O-rings, cotton tipped applicators, end cap insulator, vacuum pump oil	393011391
GC/MS Standards	
Hexachlorobenzene EI sensitivity standard 100 pg/mL	392027500
Benzophenone CI sensitivity standard 50 pg/mL	392030500
Tuning calibration compound PFTBA (FC-43)	392035300
Hexachlorobenzene EI sensitivity standard 2 pg/mL	392047100
GC/MS column test mix	392027300

GC/MS Standards



MS standards

GC/MS Analyzer Kit Standards

Description	Part No.
GC/MS semivolatiles analyzer checkout mixture	5190-0473
GC/MS pesticide analyzer internal standard, phenanthrene-d10 at 1000 µg/mL in methylene chloride, 4 x 1 mL	5190-0472
Pesticide analyzer checkout solution, 20 pesticides at 10 µg/mL each in acetone, 3 x 1 mL	5190-0468
Pesticide checkout standard, 100 µg/L, 3 x 1 mL	5190-0494
GC/MS toxicology checkout mixture	5190-0471
Residual solvent revised method 467, class C	5190-0493
Residual solvent revised method 467, class 1	5190-0490
Butanetriol internal standard #1 for biodiesel	5982-0024
Tricaprin internal standard #2 for biodiesel	5982-0025
Pesticide retention locking standard, 3 pesticides at 10 µg/mL each in n-hexane, 3 x 1 mL	5190-1441

MS Test and Performance Samples

	Description	Part No.	5975 Series	5973 Series	5972 Series	5971 Series	GCD	7000 Series	7200 Series
Tuning Samples									
EI Tune	PFTBA sample, certified, 10 g, 5.32 mL	8500-0656	✓	✓	✓	✓	✓	✓	✓
CI Tune	PFDTD calibrant	8500-8510	✓	✓				✓	✓
Performance Verification Samples									
EI	OFN, 1 pg/µL	5188-5348	✓	✓					
	Hexachlorobenzene 10 pg/µL, 1 ng/µL	8500-5808			✓				
	Methyl stearate (in methanol), 1 ng/µL, 2 ea	05990-60075				✓			
	MSD Sampler	05970-60045					✓	✓	
Negative Mode CI	OFN, 100 fg/µL	5188-5347	✓						
Positive Mode CI	Benzophenone, 100 pg/µL	8500-5440	✓	✓	✓	✓			
	1 pg/µL OFN, 5 pg/µL BZ	393065201						✓	
Checkout Samples									
HighMass	PHFT, 100 pg/µL	5188-5357	✓						
Semivolatile	GC/MS tuning standard, DFTPP	8500-5995	✓	✓	✓	✓	✓		
Volatile	p-Bromofluorobenzene (BFB), 25 µg/mL	8500-5851	✓	✓	✓	✓	✓		
MSD sampler	Solution of dodecane, biphenyl, p-cholorodiphenyl, and methyl palmitate in isooctane. Six 1.0 mL ampoules: 4 at 10 ng/µL, 1 at 100 ng/µL, 1 at 100 pg/µL.	05970-60045	✓	✓	✓	✓	✓	✓	

TIPS & TOOLS

Each GC/MS has a specific test and performance sample. Refer to the chart above for the exact sample. All volumes are approximately 0.5-1 mL unless otherwise specified.

Agilent CrossLab

Supplies for Non-Agilent GC Systems

Agilent CrossLab is a growing portfolio of supplies critical to instrument performance and productivity. Agilent CrossLab GC supplies are designed and manufactured to perform seamlessly with a variety of non-Agilent GCs in your lab. Look inside this catalog to find a comprehensive range of GC supplies to use across your lab.

We currently support:

- Bruker, Varian*
- CTC
- PerkinElmer
- Shimadzu
- Thermo Scientific

*Formerly Varian GC systems, now Bruker products

Our growing GC Supplies portfolio includes the following products, featuring easy-to-use packaging for improved productivity:

- Premium non-stick inlet septa
- Ultra Inert inlet liners
- Liner O-rings
- Column ferrules and nuts
- Autosampler syringes
- Vials and closures
  (See the complete CrossLab Vials and Closures section of our General Chromatography catalog, publication number 5991-1056EN)





Agilent CrossLab is more than supplies:

- Offering a comprehensive portfolio of GC supplies
- Over 40 years of chromatography expertise and ongoing innovation
- Optimal performance for both routine and challenging applications
- Dependable worldwide product availability and delivery
- Convenience of consolidated purchasing

Agilent CrossLab works with BRUKER | CTC | PERKINELMER | SHIMADZU | THERMO SCIENTIFIC | AND MORE



Agilent CrossLab Inlet Liners

Liners are the centerpiece of the inlet system where sample is vaporized and mixed with the carrier gas. CrossLab GC inlet liners have the perfect mix of liner configurations and chemistries to solve your application challenges.

Choose from split, splitless, PTV, and other inlet liner designs in either the new, innovative Ultra Inert deactivation or Agilent's popular proprietary deactivation, now referred to as Agilent Original deactivation. With part number and lot number silk screened on CrossLab liners, identification and re-ordering have never been easier.


Agilent CrossLab Liners with Ultra Inert Deactivation

Developed for high sensitivity analysis, Agilent's Ultra Inert deactivation provides extreme surface inertness – even for liners containing glass wool. Ultra Inert chemistry was developed using a suite of tests specifically designed to stress then evaluate liner activity, resulting in liners featuring:

- **Reproducibility** – highest level and consistent inertness for active compounds such as acids and bases
- **Robustness** – tested with a sequence of 100 injections of Endrin/DDT with < 20% degradation, allowing use of glass wool even with highly active compounds at trace (0.5 ng on-column) levels
- **Reliability** – lot-tested for inertness to ensure consistent and efficient deactivation using both acidic and basic probes at trace level (2 ng) on-column, with low to no bleed or background contamination

Ultra Inert liners are delivered in Agilent's exclusive Touchless packaging. Touchless packaging aids in easy installation of the new, clean, preconditioned liner – without risk of contamination from touching.

To view a demonstration of the Touchless Packaging for CrossLab Ultra Inert Liners please visit **www.agilent.com/chem/CLTouchless**

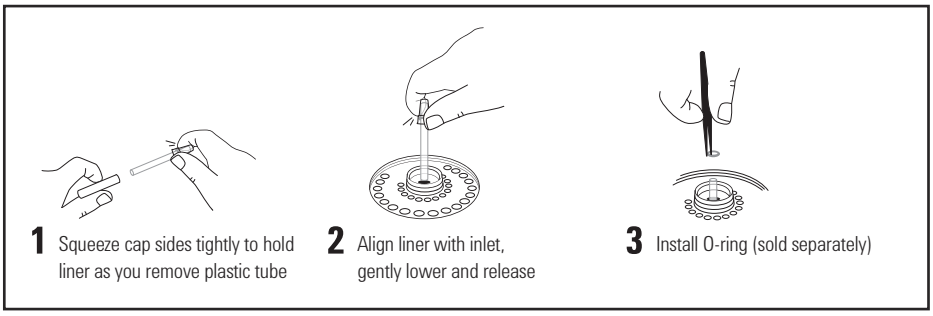

CrossLab Ultra Inert Touchless liner packaging includes visual installation guide.

Consider the following to determine how often to change your liners:


- Previous use pattern
- Sample cleanliness
- Chromatographic abnormalities, such as
  - ✓ Peak shape changes
  - ✓ Peak discrimination
  - ✓ Poor reproducibility
  - ✓ Sample pyrolysis
  - ✓ Active analyte response loss or decomposition

Get a robust, reproducible, and reliable inert flow path with Agilent CrossLab Ultra Inert Inlet Liners – even when containing glass wool

Forensic basic drugs test conditions

Column:	**DB-5ms Ultra Inert 122-5512UI 15 m x 0.25 mm, 0.25 µm**
Sample:	5 mg/L Checkout mixture for GC/MS forensic/toxicology analyzer (P/N 5190-0471)
Injection:	1 µL splitless @ 280 °C (hold 0.75 min)
Oven:	100 °C (0.5 min) to 325 °C at 20 °C/min and hold 2.5 min
Carrier:	He, 18.74 psi (adj to RT lock), constant pressure
Detector:	MSD; Source temp @ 300 °C, Quad temp @ 150 °C, Transfer line @ 300 °C; Acquisition mode, SIM/scan

Agilent CrossLab Ultra Inert single taper liner with wool

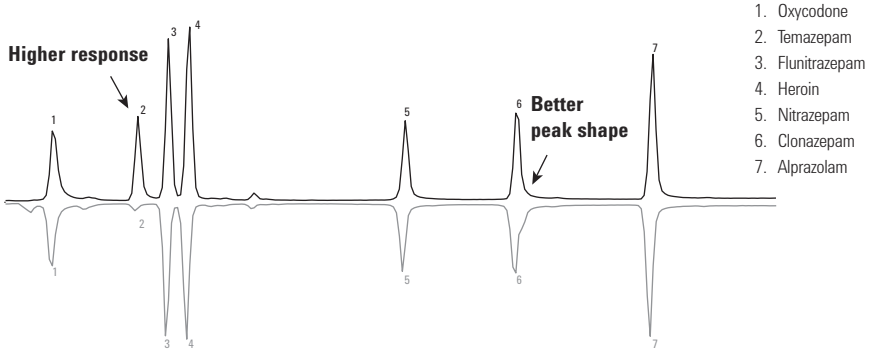

Restek Siltek deactivated gooseneck liner with deactivated wool (cat. no. 22406.213.5)

Agilent CrossLab Ultra Inert deactivated liners with wool contribute to higher response and better peak shape for very active forensic basic drug compounds than similar Restek Siltek liners.

Agilent CrossLab Liners with Agilent Original Deactivation

Developed to complement fused silica capillary column technology, Agilent's proprietary deactivation, now referred to as Agilent Original deactivation, has been successfully used for years. Proven to deliver a long-lasting surface deactivation, this proprietary chemistry and manufacturing process was previously available for Agilent gas chromatographs only, but is now available for other GC systems. Agilent Original deactivation is recommended for everyday analysis.

Agilent CrossLab Liner O-rings

- Liners are sealed in the inlet with fluoroelastomer or graphite O-rings
- Graphite O-rings are used when inlet temperatures exceed 350 °C
- Fluoroelastomer O-rings are easier to replace than graphite O-rings, which deform and flake apart more easily

Ready for chromatographic use, CrossLab fluoroelastomer O-rings feature:

- Proprietary two-step cleaning and conditioning process eliminates out-gassing of contaminants, which is especially important for trace, ECD, and MSD analyses
- Plasma-treatment for a non-stick, contaminant-free surface that won't stick to the inlet metal surface
- Novel translucent dial package that conveniently delivers one clean O-ring at a time and makes it easy to know when to reorder



Agilent CrossLab Column Ferrules

A variety of column ferrules are available to meet your application requirements, including 100% Graphite, 100% Vespel, and Vespel/Graphite ferrules.

Using the wrong ferrule or a worn-out ferrule to seal your column connection can result in inconsistent and unreliable chromatography. An improper ferrule can cause leaks, which allow air and other contaminants to enter the instrument through the column seal, causing major interference with column and detector performance.

The ideal ferrule provides a leak-free seal, accommodates various column outer diameters, seals with minimum torque, withstands temperature cycling, and does not stick to the column or fittings.

For optimum performance, ferrules should be replaced every time the column is replaced and when performing column maintenance.

To minimize problems, follow these general techniques for ferrule installation:

- Don't overtighten – finger tighten the column nut, then use wrench to tighten
- Maintain cleanliness
- Bake out ferrules prior to use (Vespel and Vespel/Graphite only)
- Avoid contamination, such as fingerprint oils
- Inspect used ferrules with magnifier for cracks, chips, or other damage before reusing them
- Change ferrules when new columns or injector/detector parts are installed

TIPS & TOOLS

Look for the following signals that indicate ferrule damage:

- Background noise from oxygen diffusing into the system
- Column bleed catalyzed by oxygen
- Sample degradation
- Sample loss
- Increase in detector signal/noise
- Poor retention time reproducibility



Ferrule Selection Recommendations

Ferrule Type	Upper Temp. Limit	Usages	Advantages	Limitations
Graphite (100%)	450 °C	• General purpose for capillary columns • Suitable for FID and NPD • Recommended for high temperature and cool on-column applications	• Easy-to-use stable seal • Higher temperature limit • Can be removed easily	• Not for MS or oxygen-sensitive detectors • Soft, easily deformed or destroyed • Possible system contamination
Vespel/Graphite (85%/15% or 60%/40%)	350 °C	• General purpose for capillary columns • Recommended for MS and oxygen-sensitive detectors • Most reliable leak-free connection	• Mechanically robust • Long lifetime	• Not reusable • Flows at elevated temperature • Must re-tighten frequently
Vespel (100%)	280 °C	• Isothermal operation • Can be reused or removed easily • Excellent sealing material when making metal or glass connections	• Mechanically robust • Long lifetime • Can be reused or removed easily	• Leaks after temperature cycle • Flows at elevated temperature • Must re-tighten frequently

TIPS & TOOLS

100% Vespel ferrules should only be used for isothermal applications.



Agilent CrossLab Autosampler Syringes

With a broad selection of syringes for auto injection, CrossLab autosampler syringes provide what you need for accurate and effective sampling. CrossLab syringes meet all fit, form, and function criteria for specific autosampler models. Agilent delivers more value in every autosampler syringe:


- Lot number printed directly on the barrel with a corresponding Certificate of Conformance
- Illuminating backing strip, for effortless viewing of the volume scale
- Environmentally friendly packaging and improved design that reduces waste
- Individually packaged for contaminant-free use right out of the box

Typical Needle Gauge Dimensions


	OD		ID	
Gauge	**mm**	**inches**	**mm**	**inches**
23	0.64	0.0248	0.11	0.0043
25	0.50	0.0197	0.20	0.0079
26	0.47	0.0184	0.11	0.0043



Needle Gauge

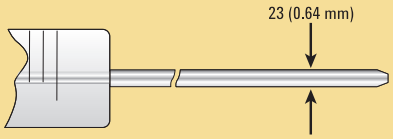

Single Gauge 23 (0.64 mm)
Packed column injector ports
Split/splitless injector ports

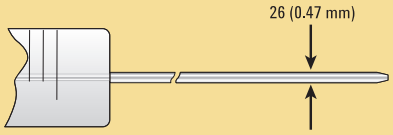

Single Gauge 26 (0.47 mm)
Packed column injector ports
Split/splitless injector ports

Needle Termination

Needle terminations are available in fixed or removable, with various tip styles.

Fixed (cemented)

- Economical, reproducible injections for autosamplers
- Preferred for applications requiring trace level samples
- Recommended for use where probability of needle bending is minimal
- Can be heated up to 70 °C

Removable needle

- Versatile option for injections
- Needle can be replaced if damaged or clogged
- Allows needle to be changed for different applications
- Can be heated up to 120 °C



Agilent CrossLab Inlet Septa

Inlet septa are a key component of sample introduction. Septa maintain the leak-free seal and exclude air from the inlet. They come in many different sizes and are made from different types of materials specific to inlet type and analysis needs.

Replace septa regularly to avoid:

- Leaks
- Decomposition
- Sample loss
- Reduced column or split vent flow
- Ghost peaks
- Column degradation

Septa are available for a variety of different applications and have different upper temperature limits. Lower temperature septa are usually softer, seal better, and can withstand more punctures (injections) than their high-temperature counterparts. If septa are used above their recommended temperatures, they can leak or decompose, causing sample loss, lower column flow, decreased column life, and ghosting. To minimize problems:

- Use within the recommended temperature range
- Change regularly
- Use septum purge when available
- Use autoinjectors
- Regularly inspect needle tips for wear




Agilent CrossLab Inlet Septa Selection Guide

GC Manufacturer	Instrument Model	Diameter (mm)	Diameter (in)
Bruker, Varian*	1177 Split/Splitless Injector	9	
	1078/1079 Programmable Temperature Vaporizing Injector	11.5	
	1093 Cold On-Column Injector	11	7/16
	1075/1077 Split/Splitless Injector	11	7/16
	1061 Packed/0.53 mm Capillary Column Flash Vaporization Injector	9.5	3/8
	1041 Packed/Wide Bore On-Column Injector	9.5	3/8
PerkinElmer	Clarus System	11	7/16
	AutoSystem	11	7/16
	AutoSystem XL	11	7/16
	8000 Series	11	7/16
	Sigma Series	11	7/16
Thermo Scientific Trace GC Ultra and Focus GC	Split/Splitless Injector	17	
	Large Volume Splitless Injector	9	
	Programmable Temperature Vaporizing Injector	12.7	1/2
	Purged Packed Column Injector	11	
	Packed Column Injector	11	
Thermo Scientific Finnigan	Trace 2000 Series	9.5	
	9001 GC	9.5	
Shimadzu	All Models	Shimadzu Plug	

*Formerly Varian GC systems, now Bruker products

Septa Diameters

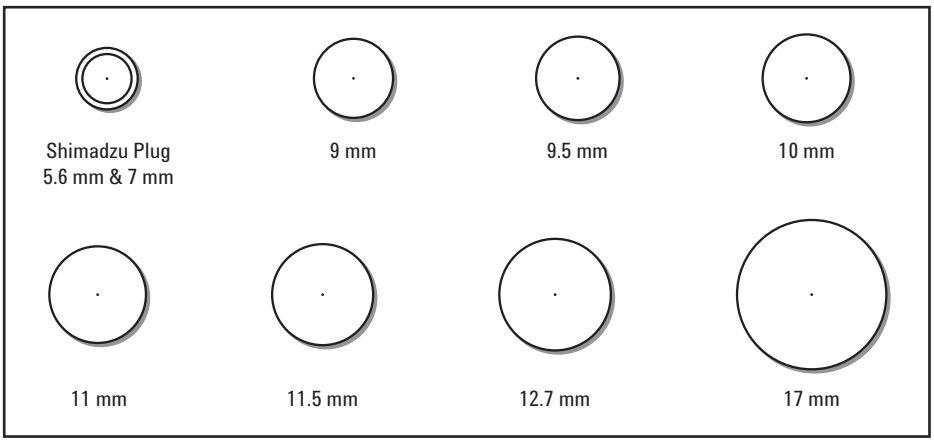

Premium Non-Stick Septa



CrossLab premium non-stick inlet septa are designed and manufactured to provide a reliable noncontaminating seal. Our tri-fold blister pack ensures that each septum remains clean and ready to use.

- Proprietary plasma treatment prevents sticking and unnecessary inlet cleaning
- Innovative blister packaging keeps each septum clean and ready for use
- Center point guides the needle for easy penetration, less coring, and longer life
- Precision molding assures accurate fit in the inlet
- Each batch is tested for bleed
- Premium formulations selected for sealing and chromatographic cleanliness
- No need to bake septa before using

Summary of Premium Inlet Septum Characteristics

Septum Type	Bleed	Lifetime	Temperature Limits
Non-Stick BTO (Bleed and Temperature Optimized)	✓✓✓	✓	to 400 °C injection port temp
Non-Stick Advanced Green	✓✓	✓✓	to 350 °C
Non-Stick Long-Life	✓	✓✓✓	to 350 °C

✓✓✓ = best ✓✓ = very good ✓ = good



Agilent CrossLab Non-Stick Bleed Temperature Optimized (BTO) Inlet Septa

- Extended temperature range, lowest bleed
- Maximum injection port temperature 400 °C
- Plasma treatment eliminates sticking in the injection port
- Pre-conditioned; ready to use
- Blister packaging maintains cleanliness and convenience
- Ideal for use with low-bleed, "Mass Spec" capillary columns



BTO septa, 8010-0223, 8010-0224

Non-Stick Bleed and Temperature Optimized (BTO) Septa

Description	Agilent CrossLab Part No. 50/pk	Agilent CrossLab Part No. 100/pk
9 mm, CenterGuide	8010-0217	8010-0218
9.5 mm	8010-0219	8010-0220
10 mm	8010-0221	8010-0222
11 mm, CenterGuide	8010-0223	8010-0224
11.5 mm, CenterGuide	8010-0225	8010-0226
Shimadzu plug	8010-0231	8010-0232
Description	**24/pk**	**48/pk**
12.7 mm, CenterGuide	8010-0227	8010-0228
17 mm, CenterGuide	8010-0229	8010-0230

Comparison of Coring, With and Without CenterGuide (30x magnification)



High-Temperature Septa without CenterGuide

Major coring before 100 autoinjections

CrossLab BTO Septa with CenterGuide

Very little coring, even after 700 autoinjections

Agilent CrossLab Non-Stick Advanced Green Inlet Septa

- True long-life, high-temperature green septa
- More injections per septum
- Plasma treatment eliminates sticking in the injection port
- Maximum injection port temperature 350 °C
- High-performance alternative to competitors' "green" septa
- Blister packaging for cleanliness and convenience

Non-Stick Advanced Green Septa

Description	Agilent CrossLab Part No. 50/pk	Agilent CrossLab Part No. 100/pk
9 mm, CenterGuide	8010-0201	8010-0202
9.5 mm	8010-0203	8010-0204
10 mm	8010-0205	8010-0206
11 mm, CenterGuide	8010-0207	8010-0208
11.5 mm, CenterGuide	8010-0209	8010-0210
Shimadzu plug	8010-0215	8010-0216
Description	**24/pk**	**48/pk**
12.7 mm, CenterGuide	8010-0211	8010-0212
17 mm, CenterGuide	8010-0213	8010-0214



Advanced green septa, 8010-0207, 8010-0208

Agilent CrossLab Non-Stick Long-Life Inlet Septa

- Preferred septa for autosamplers
- Pre-pierced for extended life and reduced coring
- Ideal for overnight runs
- Up to 400 injections per septum
- Plasma treatment eliminates sticking
- Maximum injection port temperature 350 °C
- Soft, 45 durometer, easy on autosampler needles
- Blister packaging for cleanliness and convenience



Long-life septa, 8010-0239, 8010-0240

Non-Stick Long-Life Septa

Description	Agilent CrossLab Part No. 50/pk	Agilent CrossLab Part No. 100/pk
9 mm, CenterGuide	8010-0233	8010-0234
11 mm, CenterGuide	8010-0239	8010-0240
11.5 mm, CenterGuide	8010-0241	8010-0242
Description	**24/pk**	**48/pk**
12.7 mm, CenterGuide	8010-0243	8010-0244
17 mm, CenterGuide	8010-0245	8010-0246



Agilent CrossLab Gray General Purpose Inlet Septa

Agilent CrossLab general purpose septa are made from an enhanced injection-molded silicone rubber and are good for routine use. The septa material, gray in color, is specified to withstand over 200 automatic injections at an injection port temperature of 350 °C.





CrossLab general purpose inlet septa, 8010-0257

General Purpose Septa

Description	Agilent CrossLab Part No. 50/pk	Agilent CrossLab Part No. 100/pk
9 mm	8010-0249	8010-0250
9.5 mm	8010-0251	8010-0252
10 mm	8010-0253	8010-0254
11 mm	8010-0255	8010-0256
11.5 mm	8010-0257	8010-0258
12.7 mm	8010-0259	8010-0260
17 mm	8010-0261	8010-0262
Shimadzu plug	8010-0263	8010-0264

Septa Troubleshooting

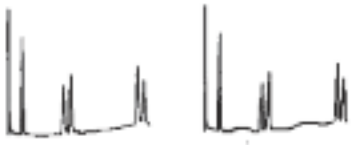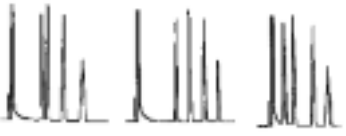Symptom	Possible Causes	Remedy
Extra Peaks/Humps 	Septum bleed	Turn off injector heater. If extra peaks disappear, use septum specified for higher temperature or analyze at lower inlet temperature.
Baseline Change After Large Peak 	Large leak at septum during injection and for a short time thereafter (common with large diameter needles)	Replace septum and use smaller diameter needles.
Retention Times Prolonged 	Carrier gas leaks at septum or column connection	Check for leaks. Replace septum or tighten connections if necessary.

Agilent CrossLab Supplies for Bruker, Varian* GC Systems

Liners for 1177 Split/Splitless Injector Ports

	Description	ID (mm)	OD (mm)	Length (mm)	Volume (µL)	Unit	Similar to OEM Part No.	Agilent Ultra Inert Deactivation	Similar to OEM Part No.	Agilent Original Deactivation
Split/Splitless Liners										
	Single taper	4.0	6.3	78.5	1000	5/pk	RT207992145 SG092017	8004-0151	SG092017	8004-0101
	Single taper, with wool	4.0	6.3	78.5	1000	5/pk	SG092019	8004-0152	SG092019	8004-0102
	Double taper	4.0	6.3	78.5	1000	5/pk	SG092018	8004-0155	SG092018	8004-0105
	Gooseneck, with wool	4.0	6.5	78.5	1000	5/pk	392611936	8004-0170	392611936	8004-0114
	Recessed gooseneck, with wool	4.0	6.3	78.5	1000	5/pk	SG092010	8004-0153	SG092010	8004-0103
	Gooseneck	2.0	6.5	78.5	250	5/pk	392611926	8004-0178	392611926	8004-0119
Splitless Liners										
	Straight, with wool	4.0	6.5	78.5	1000	5/pk	392611937	8004-0173	392611937	8004-0116
	Gooseneck	4.0	6.5	78.5	1000	5/pk	392611927	8004-0165	392611927	8004-0113
Split Liners										
	Straight-through	4.0	6.3	78.5	1000	5/pk	RT207732145 SG092007	8004-0156	SG092007	8004-0106
	Straight, with wool	4.0	6.3	78.5	1000	5/pk	SG092001 392611934	8004-0154	SG092001 392611934	8004-0104
	With frit, gooseneck	4.0	6.3	78.5	1000	5/pk	RT210462145	8004-0158		
Direct Liners										
	Straight-through	1.2	6.3	78.5	90	5/pk	SG092016	8004-0157	SG092016	8004-0107

***Formerly Varian GC systems, now Bruker products**

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Supplies for Bruker, Varian* GC Systems

Liners for 1078/1079 Injector Ports

	Description	ID (mm)	OD (mm)	Length (mm)	Volume (µL)	Unit	Similar to OEM Part No.	Agilent Ultra Inert Deactivation	Similar to OEM Part No.	Agilent Original Deactivation
Split/Splitless Liners										
	Single taper	3.4	5.0	54	500	5/pk	RT209012145 SG092038	8004-0160	SG092038	8004-0108
	Gooseneck, with wool	2.0	5.0	54	250	5/pk			392611953	8004-0118
Splitless Liners										
	Single taper	2.0	5.0	54	170	5/pk	RT207122145 SG092039	8004-0161	SG092039	8004-0109
Split Liners										
	Gooseneck	3.4	5.0	54	500	5/pk	392611945	8004-0164	392611945	8004-0112
	With frit, gooseneck	3.4	5.0	54	500	5/pk	RT217092145	8004-0159		
	With frit, gooseneck	3.4	5.0	54	500	5/pk	392611946	8004-0171		
Other Liners										
	SPME, straight	0.8	5.0	54	30	5/pk	392611948	8004-0176		

Liners for 1093/1094 Injector Ports

	Description	ID (mm)	OD (mm)	Length (mm)	Volume (µL)	Unit	Similar to OEM Part No.	Agilent Ultra Inert Deactivation	Similar to OEM Part No.	Agilent Original Deactivation
Direct Liners										
	SPI for 0.25/0.32 mm id columns	0.5	4.6	54	10	5/pk	190010906	8004-0167		
	SPI with 0.5 mm restriction for 0.53 mm id on-column	0.8	4.6	54	30	5/pk	SG092034 190010907	8004-0162	SG092034 190010907	8004-0110

***Formerly Varian GC systems, now Bruker products**

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Supplies for Bruker, Varian* GC Systems

Liners for 1075/1077 Injector Ports

	Description	ID (mm)	OD (mm)	Length (mm)	Volume (µL)	Unit	Similar to OEM Part No.	Agilent Ultra Inert Deactivation	Similar to OEM Part No.	Agilent Original Deactivation
Split Liners										
	With wool	4.0	6.3	72	1000	5/pk	SG092021 190010901	8004-0163	SG092021 190010901	8004-0111

Liners for 1060/1061 Injector Ports

	Description	ID (mm)	OD (mm)	Length (mm)	Volume (µL)	Unit	Similar to OEM Part No.	Agilent Ultra Inert Deactivation	Similar to OEM Part No.	Agilent Original Deactivation
Direct Liners										
	Double gooseneck	0.9	6.3	72	1000	5/pk	392611943	8004-0168		



Graphite O-ring, 8004-0202

Liner O-rings

Description	Unit	Similar to OEM Part No.	Agilent CrossLab Part No.
Non-stick fluoroelastomer O-ring, 1177 split/splitless, 6.3/6.5 mm od	10/pk	8850103100	8004-0201
Graphite O-ring, 1177 split/splitless, 6.5 mm od	10/pk	392611930	8004-0202
Graphite O-ring, 1177 split/splitless, 6.3 mm od	10/pk	392611935	8004-0203
Graphite liner seal, 1078/1079 injector, 5 mm id	10/pk	392534201	8004-0204

***Formerly Varian GC systems, now Bruker products**

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Supplies for Bruker, Varian* GC Systems

Column Ferrules

Capillary Column Ferrules

Injector	Fitting Size (in)	Ferrule ID (mm)	Column ID (mm)	Hole	Unit	Similar to OEM Part No.	Agilent CrossLab Part No.
60% Vespel/40% Graphite Capillary Column Ferrules							
1177, 1079	1/16	0.3	0.18 or smaller	1	10/pk	CR213103	8004-0211
	1/16	0.4	0.25	2	10/pk	CR213124	8004-0213
	1/16	0.425	0.25	1	10/pk	CR213104	8004-0212
	1/16	0.5	0.32	1	10/pk	CR213105	8004-0214
	1/16	0.5	0.32	2	10/pk	CR213125	8004-0215
1177, 1079, 1061, 1041	1/16	0.8	0.53	1	10/pk	CR213108	8004-0216
Vespel Capillary Column Ferrules							
1177, 1079	1/16	0.3	0.18	1	10/pk	CR212103	8010-0306
	1/16	0.4	0.25	1	10/pk		8010-0307
	1/16	0.425	0.25	1	10/pk	CR212104	8004-0219
	1/16	0.5	0.32	1	10/pk	CR212105	8010-0308
	1/16	0.5	0.32	2	10/pk	CR212125	8004-0218*
1177, 1079, 1061, 1041	1/16	0.8	0.53	1	10/pk	CR212108	8010-0309
Graphite Capillary Column Ferrules							
1177, 1079	1/16	0.4	0.25	1	10/pk	CR211104	8010-0301
	1/16	0.5	0.32	1	10/pk	CR211105	8010-0302
	1/16	0.5	0.32	2	10/pk	CR211125	8010-0303
1177, 1079, 1061, 1041	1/16	0.8	0.53	1	10/pk	CR211108	8010-0304

*1177 Injector only

***Formerly Varian GC systems, now Bruker products**

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Supplies for Bruker, Varian* GC Systems

Packed Column Ferrules

Injector	Fitting Size (in)	Ferrule ID (in)	Column OD (in)	Hole	Unit	Similar to OEM Part No.	Agilent CrossLab Part No.
60% Vespel/40% Graphite Packed Column Ferrules							
1093, 1061, 1041	1/4	1/4	1/4	1	10/pk	CR213400	8004-0217*
Graphite Packed Column Ferrules							
1093, 1061, 1041	1/4	1/4	1/4	1	10/pk	CR211400	8010-0305*

*Straight body

Column Nuts

Description	Unit	Similar to OEM Part No.	Agilent CrossLab Part No.
Column nut, brass, 1177, 1079, 1061, or 1041 injector	2/pk	394955100	8004-0311
Column nut, stainless steel, 1093 injector	2/pk	CP743117	8004-0312

Autosampler Syringes for Bruker/Varian GC Systems, 1/pk

Model	Volume (µL)	Description	Needle Gauge/Length (mm)/Tip	Similar to OEM syringe Part No.	Agilent CrossLab Syringe Part No.	Agilent CrossLab Replacement Needle Part No.	Agilent CrossLab Replacement Plunger Part No.
Varian* CP8400, CP8410, CP9010, CP9050	10	Fixed needle	23/50/cone tip	SG002981	8010-0351		
		Fixed needle	26/50/bevel tip		8004-0001		
		Removable needle	26/50/cone tip	SG002982	8004-0003	8004-0004, 2/pk	
Varian* 8035, 8100, 8200		Fixed needle, gas tight	26/53/side hole tip		8004-0002		8004-0007
		Removable needle, gas tight	25/53/side hole tip		8004-0005	8004-0006, 2/pk	8004-0007

***Formerly Varian GC systems, now Bruker products**

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the Agilent CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts.



Autosampler syringe, 10 µL fixed needle, 8010-0351

Agilent CrossLab Supplies for Bruker, Varian* GC Systems

Inlet Septa



Non-stick bleed and temperature optimized septa, 10 mm, 50/pk, 8010-0221

Non-Stick Bleed and Temperature Optimized (BTO) Septa

Description	Agilent CrossLab Part No. 50/pk	Similar to OEM Part No.	Agilent CrossLab Part No. 100/pk
9 mm, CenterGuide	8010-0217	CR298713	8010-0218
9.5 mm	8010-0219	CR298705	8010-0220
10 mm	8010-0221	CR298745	8010-0222
11 mm, CenterGuide	8010-0223	CR298717	8010-0224
11.5 mm, CenterGuide	8010-0225	CR298777	8010-0226

Non-Stick Advanced Green Septa

Description	Agilent CrossLab Part No. 50/pk	Similar to OEM Part No.	Agilent CrossLab Part No. 100/pk
9 mm, CenterGuide	8010-0201	CR246713	8010-0202
9.5 mm	8010-0203	CR246124	8010-0204
10 mm	8010-0205		8010-0206
11 mm, CenterGuide	8010-0207	CR246225	8010-0208
11.5 mm, CenterGuide	8010-0209	CR246725	8010-0210

***Formerly Varian GC systems, now Bruker products**

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Supplies for Bruker, Varian* GC Systems



Long-life septa, 8010-0239, 8010-0240

Non-Stick Long-Life Septa

Description	Agilent CrossLab Part No. 50/pk	Similar to OEM Part No.	Agilent CrossLab Part No. 100/pk
9 mm, CenterGuide	8010-0233	CR239778	8010-0234
11 mm, CenterGuide	8010-0239	CR239287	8010-0240
11.5 mm, CenterGuide	8010-0241	CR239287	8010-0242

General Purpose Septa

Description	Agilent CrossLab Part No. 50/pk	Agilent CrossLab Part No. 100/pk
General Purpose Septa		
9 mm	8010-0249	8010-0250
9.5 mm	8010-0251	8010-0252
10 mm	8010-0253	8010-0254
11 mm	8010-0255	8010-0256
11.5 mm	8010-0257	8010-0258

***Formerly Varian GC systems, now Bruker products**

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

TIPS & TOOLS


For a comprehensive vial compatibility chart, identification guide, septum recommendations, and ordering information, see the complete CrossLab Vials and Closures section of our General Chromatography catalog, publication number 5991-1056EN.

Agilent CrossLab Supplies for Bruker, Varian* GC Systems

Injector Replacement Parts and Supplies


1177 Split/Splitless Injector

Item	Description	Agilent CrossLab and Agilent Part No.
1	Injector nut	392597501
	Injector nut wrench	390842300
2	Knob	392597101
3	Automatic start switch	390820601
4	Septum, 9 mm	
	BTO	8010-0217
	Long Life	8010-0233
	Advanced Green	8010-0201
	Septum pick	7200008400
5	Septum purge head	
	EFC21 (stainless steel)	392597301
	EFC21 (UltiMetal)	392597303
	EFC25 or Manual Pneumatics	392597302
6	Purge head screw	391866308
7	Graphite liner O-ring, splitless, 6.5 mm	8004-0202
	Non-stick fluoroelastomer liner O-ring, 6.3 mm	8004-0201
8	Glass liner	8004-0165
9	Injector body	
	Stainless steel	392599401
	UltiMetal	392599411
	Manual	392599501
10	For replacement ferrules, see complete CrossLab column ferrules ordering information, see page 157	
11	Bottom nut	8004-0311

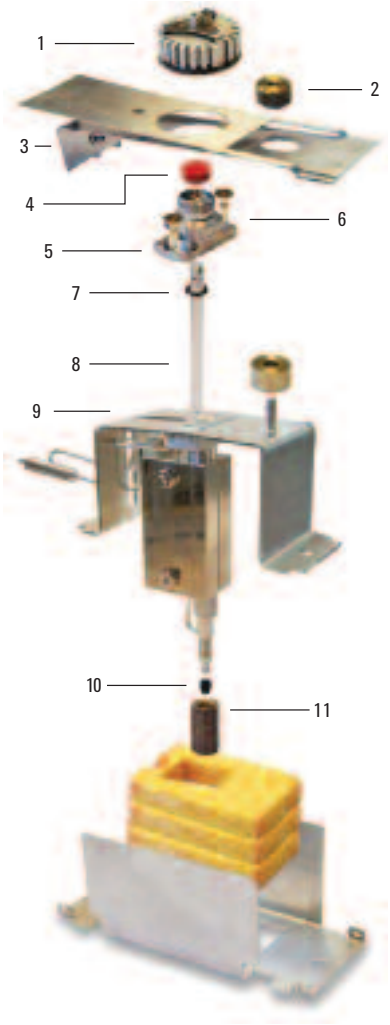

***Formerly Varian GC systems, now Bruker products**

Agilent CrossLab Supplies for Bruker, Varian* GC Systems

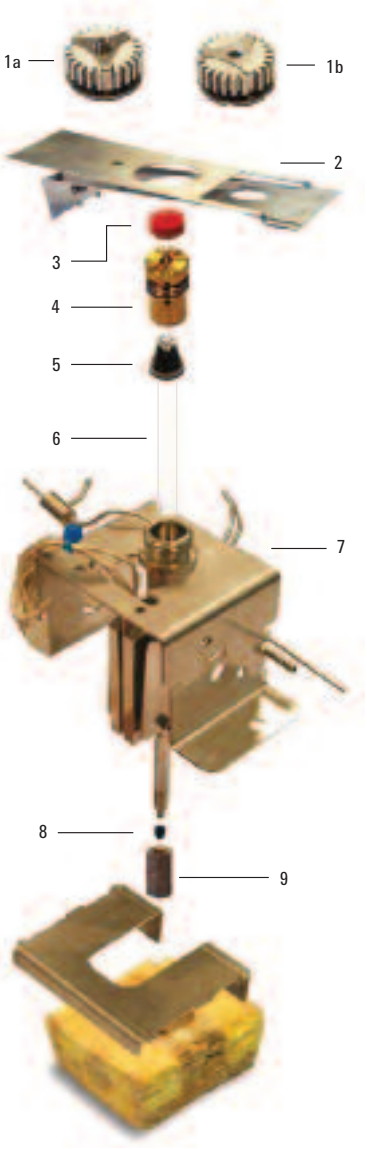

1079 Large Volume Injector (LVI)

Item	Description	Agilent CrossLab and Agilent Part No.
1a	Injector nut	394966601
1b	Injector nut	394966601
	Injector nut wrench	390842300
2	Automatic start switch	390820601
3	Septum, 11.5 mm	
	BTO	8010-0225
	Long Life	8010-0241
	Advanced Green	8010-0209
	Septum pick	7200008400
4	Septum support	391867600
5	Graphite liner seal	8004-0204
6	Glass liner	8004-0164
7	Injector body, EFC type	
	Stainless steel	392544001
	UltiMetal	392544011
8	For replacement ferrules, see complete CrossLab column ferrules ordering information, see page 157	
9	Bottom nut	8004-0311

***Formerly Varian GC systems, now Bruker products**

TIPS & TOOLS


For a comprehensive vial compatibility chart, identification guide, septum recommendations, and ordering information, see the complete CrossLab Vials and Closures section of our General Chromatography catalog, publication number 5991-1056EN.

Agilent CrossLab Supplies for Bruker, Varian* GC Systems


1093 Cool On-Column (COC) Injector

Item	Description	Agilent CrossLab and Agilent Part No.
1	Injector nut	394966601
	Injector nut wrench	390842300
2	Automatic start switch	390820601
3	Septum, 11.5 mm	
	BTO	8010-0225
	Long Life	8010-0241
	Advanced Green	8010-0209
	Septum pick	7200008400
4	Septum support	391821100
5	Glass liner	
	Default	8004-0162
	High performance	8004-0167
6	Screw	391866306
7	Graphite/Vespel ferrule	8004-0217
	Graphite ferrule	8010-0305
8	Bottom nut	
	Brass	8004-0311
	Stainless steel	8004-0312

***Formerly Varian GC systems, now Bruker products**

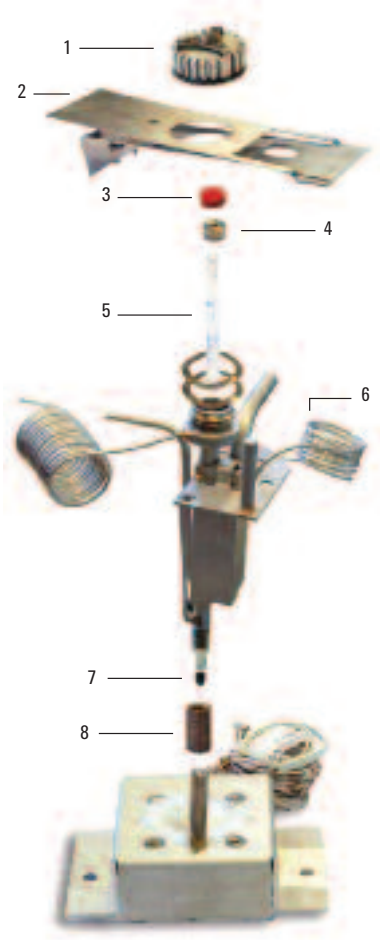

Agilent CrossLab Supplies for Bruker, Varian* GC Systems

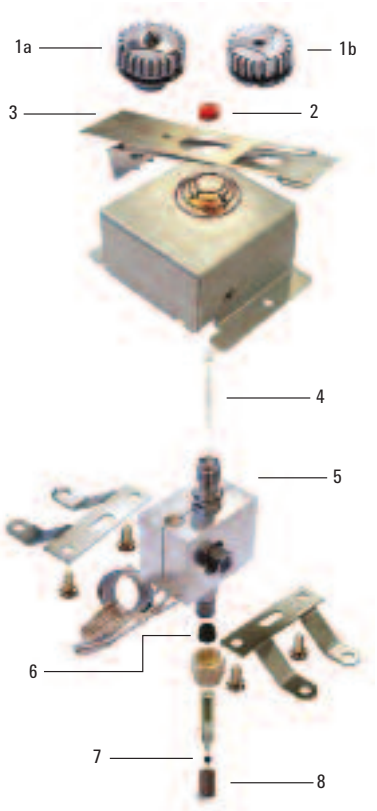

1061 Packed/530 µm Capillary Column Injector

Item	Description	Agilent CrossLab and Agilent Part No.
1a	Injector nut	390812700
1b	Injector nut	392595501
	Injector nut wrench	390842300
2	Septum, 9.5 mm	
	BTO	8010-0219
	Advanced Green	8010-0203
	Septum pick	7200008400
3	Automatic start switch	390820601
4	Glass liner	8004-0168
5	Injector body, EFC23	392548301
6	Graphite/Vespel ferrule	8004-0217
	Graphite ferrule	8010-0305
7	For replacement ferrules, see complete CrossLab column ferrules ordering information, see page 157	
8	Bottom nut	8004-0311


***Formerly Varian GC systems, now Bruker products**

Agilent CrossLab Supplies for Bruker, Varian* GC Systems

1041 Packed/Wide Bore On-Column (PWOC) Injector

Item	Description	Agilent CrossLab and Agilent Part No.
1a	Injector nut	390812700
1b	Injector nut	392595501
	Injector nut wrench	390842300
2	Septum, 9.5 mm	
	BTO	8010-0219
	Advanced Green	8010-0203
	Septum pick	7200008400
3	Automatic start switch	390820601
4	Injector body, EFC type	392548201
5	Graphite/Vespel ferrule	8004-0217
	Graphite ferrule	8010-0305
6	Injector insert, stainless steel	392543101
7	For replacement ferrules, see complete CrossLab column ferrules ordering information, see page 157	
8	Bottom nut	8004-0311

***Formerly Varian GC systems, now Bruker products**

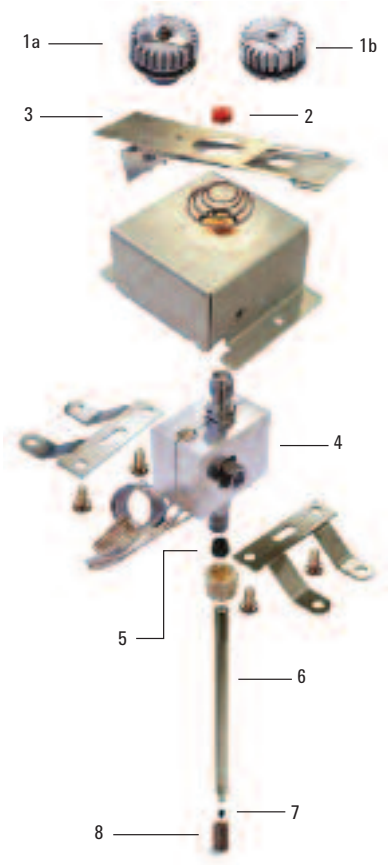

Agilent CrossLab Supplies for Bruker, Varian* GC Systems

Detector Replacement Parts and Supplies

Thermal Conductivity Detector (TCD)

Description	Agilent Part No.
Adapter TCD/DEFC capillary make-up	392585291
Adapter TCD/DEFC reference gas kit	392585292
Adapter TCD capillary make-up, MPC, 3800	392560591
TCD DEFC 14 (Non-H_2), 2 channels	392561290

Flame Ionization Detector (FID)

Description	Agilent Part No.
Tube collector	394958700
Lower FID insulator #17311	2100003200
FID flame tip jet, 0.010 in	200187500
FID flame tip jet with nut, 0.020 in	200193800
Crunch washer, 25/pk	1500334701

***Formerly Varian GC systems, now Bruker products**

Agilent CrossLab Supplies for Bruker, Varian* GC Systems

Pulsed Flame Photometric Detector (PFPD)

Description	Agilent Part No.
Photomultiplier tube (PFPD) #R647-08	392517100
O-Ring, silicone, 0.53 in id, PFPD	2740292400
PFPD light pipe	392515500
Sapphire window assembly	392514500
Sapphire window washer	392514300
Wrench, PFPD combustor support	392519200
Seal, combustor support	392513800
Combustor holder (2 mm)	392517800
Combustor Sulfur (2 mm), cleaned	392517600
Holder, combustor, 3 mm, cleaned	392517901
Combustor Phosphorus, 3 mm, cleaned	392517700

PFPD Filter Assemblies

Description	Agilent Part No.
Arsenic (As)	392515105
Manganese (Mn)	392544391
Nitrogen (N)	392511901
Sulfur and Phosphorus (S and P)	392515104
Phosphorus (P)	392515102
Sulfur (S)	392515101
Tin (Sn)	392515103

***Formerly Varian GC systems, now Bruker products**

TIPS & TOOLS

For a comprehensive vial compatibility chart, identification guide, septum recommendations, and ordering information, see the complete CrossLab Vials and Closures section of our General Chromatography catalog, publication number 5991-1056EN.

Agilent CrossLab Supplies for Bruker, Varian* GC Systems

PFPD Nitrogen Mode Maintenance

Description	Agilent Part No.
Photomultiplier tube, Nitrogen R-5070A	392512800
O-Ring, 0.987 in id	2740236100
PFPD filter assembly, Nitrogen	392511901
PFPD light pipe	392515500
Sapphire window assembly	392514500
Sapphire window washer	392514300

Thermionic Specific Detector (TSD)

Description	Agilent Part No.
TSD bead probe, unconditioned and untested	390607400
TSD bead probe, conditioned and tested	390607401
Upper TSD insulator #17310 TSD	2100003100
O-Ring, 30/pk	2740928202
TSD collector assembly	390607900
Lower FID insulator #17311	2100003200
Crunch washer, 25/pk	1500334701
FID flame tip jet with nut, 0.020 in	200193800
Flow tube assembly	200187600

***Formerly Varian GC systems, now Bruker products**

Agilent CrossLab Parts and Supplies for PerkinElmer GC Systems

Liners for AutoSystem, AutoSystem XL, Clarus Systems

	Description	ID (mm)	OD (mm)	Length (mm)	Volume (µL)	Unit	Similar to OEM Part No.	Agilent Ultra Inert Deactivation	Similar to OEM Part No.	Agilent Original Deactivation
Split/Splitless Liners										
	PSS straight	2.0	4.0	86.2		5/pk	N6502002	8003-0153		8003-0103
	PSS straight with bottom restriction	2.0	4.0	86.2	260	5/pk	N6121004	8003-0158		
	PSS on-column	2.0	4.0	86.2	250	5/pk	N6101539	8003-0165	N6101539	8003-0110
	PSS straight	1.0	4.0	86.2	65	5/pk	N6121006	8003-0157		
Split/Large Volume Splitless Liners										
	Straight with bottom restriction	4.0	6.2	92.1	1150	5/pk	N6121001	8003-0159	N6121001	8003-0105
Splitless Liners										
	Straight	2.0	6.2	92.1	300	5/pk	N6101372	8003-0162	N6101372	8003-0107
	Straight-through	2.0	6.2	92.1	300	5/pk	N6502004	8003-0152	N6502004	8003-0102
Split Liners										
	Straight-through	4.0	6.2	92.1	1150	5/pk		8003-0151		8003-0101
	Straight, wool	4.0	6.2	92.1	1100	5/pk	N6121020	8003-0160	N6121020	8003-0106
	Straight with bottom restriction	4.0	6.2	92.1	1100	5/pk	N6101052	8003-0166	N6101052	8003-0111

(Continued)

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Parts and Supplies for PerkinElmer GC Systems

Liners for AutoSystem, AutoSystem XL, Clarus Systems

	Description	ID (mm)	OD (mm)	Length (mm)	Volume (µL)	Unit	Similar to OEM Part No.	Agilent Ultra Inert Deactivation	Similar to OEM Part No.	Agilent Original Deactivation
Direct Liners										
	Gooseneck, drilled hole on top, wool	4.0	6.2	92.1		5/pk	N6121022	8003-0155		
Other Liners										
	Packed column, straight	3.0	6.2	112	800	5/pk	N6121000	8003-0163	N6121000	8003-0108
	Programmable on-column, hour glass	2.2	4.0	16		5/pk			N6101703	8003-0109*
	PTV, 0.25 mm id restriction, recessed gooseneck	1.0	2.0	88	70	5/pk		8003-0154		8003-0104

*P/N 8003-0109 is not deactivated



Graphite O-rings, 8003-0205

Liner O-rings

Description	Unit	Similar to OEM Part No.	Agilent CrossLab Part No.
Non-stick fluoroelastomer O-ring	10/pk	N9302783	8010-0401
Non-stick fluoroelastomer O-ring, PSS Injector	10/pk	N6101747	8003-0202
Silicone O-ring	10/pk	N6101374	8003-0203
Graphite O-ring, PSS Injector	10/pk	N6101751	8003-0204
Graphite O-ring	10/pk	N6101378	8003-0205

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Parts and Supplies for PerkinElmer GC Systems

Column Ferrules

Capillary Column Ferrules

Model	Fitting Size (in)	Ferrule ID (mm)	Column ID (mm)	Hole	Unit	Similar to OEM Part No.	Agilent CrossLab Part No.
85% Vespel/15% Graphite Capillary Column Ferrules							
AutoSystem, AutoSystem XL, Clarus	1/16	0.4	0.25	1	10/pk	09920104	8010-0310
	1/16	0.4	0.25	2	10/pk	04972392	8010-0312
	1/16	0.5	0.32	1	10/pk	09920105	8010-0311
	1/16	0.5	0.32	2	10/pk	N9306000	8003-0216
	1/16	0.8	0.53	1	10/pk	09920107	8010-0313
Graphite Capillary Column Ferrules							
AutoSystem, AutoSystem XL, Clarus	1/16	0.4	0.25	1	10/pk		8010-0301
	1/16	0.5	0.32	1	10/pk	09903700	8010-0302
	1/16	0.5	0.32	2	10/pk	N9306001	8010-0303
	1/16	0.8	0.53	1	10/pk	09920141	8010-0304
Vespel Capillary Column Ferrules							
AutoSystem, AutoSystem XL, Clarus	1/16	0.3	0.18 or smaller	1	10/pk		8010-0306
	1/16	0.4	0.25	1	10/pk		8010-0307
	1/16	0.5	0.32	1	10/pk		8010-0308
	1/16	0.8	0.53	1	10/pk		8010-0309

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Parts and Supplies for PerkinElmer GC Systems

Packed Column Ferrules

Model	Fitting Size (in)	Ferrule ID (in)	Column OD (in)	Hole	Unit	Similar to OEM Part No.	Agilent CrossLab Part No.
85% Vespel/15% Graphite Packed Column Ferrules							
AutoSystem, AutoSystem XL, Clarus	1/4	1/4	1/4	1	10/pk	09903739	8010-0314
	1/8	1/8	1/8	1	10/pk	N9302081	8003-0219
	1/16	1/16	1/16	1	10/pk	09920127	8010-0315
Graphite Packed Column Ferrules							
AutoSystem, AutoSystem XL, Clarus	1/4	1/4	1/4	1	10/pk	09920140	8010-0305
	1/8	1/8	1/8	1	10/pk	09903915	8003-0212
	1/16	1/16	1/16	1	10/pk	02450972	8003-0211
Vespel Packed Column Ferrules							
AutoSystem, AutoSystem XL, Clarus	1/4	1/4	1/4	1	10/pk	N9301361	8003-0223
	1/8	1/8	1/8	1	10/pk	N9301360	8003-0222
	1/16	1/16	1/16	1	10/pk		8003-0221

Column Nuts

Description	Unit	Similar to OEM Part No.	Agilent CrossLab Part No.
Column nut, 1/16 in	2/pk	09903392	8003-0311

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Autosampler Syringes for PerkinElmer GC Systems, 1/pk

Model	Volume (µL)	Description	Needle Gauge/ Length (mm)/Tip	Similar to OEM Syringe Part No.	Agilent CrossLab Syringe Part No.	Similar to OEM Replacement Needle and Plunger Repair Kit Part No.	Agilent CrossLab Replacement Needle and Plunger Repair Kit Part No.
AutoSystem, AutoSystem XL, Clarus	0.5	Removable needle	23/70/cone tip	N6101252	8003-0005	N6101469	8003-0006
AutoSystem, AutoSystem XL, Clarus		Removable needle	26/70/bevelled cone tip		8003-0007		8003-0008
AutoSystem, AutoSystem XL, Clarus	5	Fixed needle	23/70/cone tip	N6101251	8003-0001		
AutoSystem, AutoSystem XL, Clarus		Fixed needle, gas tight	23/70/cone tip	N6101390	8003-0002		
AutoSystem, AutoSystem XL, Clarus		Fixed needle	26/70/cone tip	N6101380	8003-0003		
AutoSystem, AutoSystem XL, Clarus	50	Fixed needle	23/70/cone tip	N6101760	8003-0004		

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Parts and Supplies for PerkinElmer GC Systems

Inlet Septa

Non-Stick Bleed and Temperature Optimized (BTO) Septa

Description	Agilent CrossLab Part No. 50/pk	Similar to OEM Part No.	Agilent CrossLab Part No. 100/pk
11 mm, CenterGuide	8010-0223	N9302972	8010-0224

Non-Stick Advanced Green Septa

Description	Agilent CrossLab Part No. 50/pk	Similar to OEM Part No.	Agilent CrossLab Part No. 100/pk
11 mm, CenterGuide	8010-0207	N6621028 N9306219	8010-0208



Long-life septa, 8010-0239, 8010-0240

Non-Stick Long-Life Septa

Description	Agilent CrossLab Part No. 50/pk	Agilent CrossLab Part No. 100/pk
11 mm, CenterGuide	8010-0239	8010-0240

General Purpose Septa

Description	Agilent CrossLab Part No. 50/pk	Similar to OEM Part No.	Agilent CrossLab Part No. 100/pk
11 mm	8010-0255	54019985	8010-0256

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

TIPS & TOOLS

For a comprehensive vial compatibility chart, identification guide, septum recommendations, and ordering information, see the complete CrossLab Vials and Closures section of our General Chromatography catalog, publication number 5991-1056EN.

Agilent CrossLab Supplies for Shimadzu GC Systems

Liners for 2014 Systems

	Description	ID (mm)	OD (mm)	Length (mm)	Volume (µL)	Unit	Similar to OEM Part No.	Agilent Ultra Inert Deactivation	Similar to OEM Part No.	Agilent Original Deactivation
Splitless Liners										
	Single taper, wool	3.5	5.0	95		5/pk	221-48876-02	8001-0160		
	Double taper, drilled hole near top	3.5	5.0	95		5/pk	220-94734-01	8001-0158		
	Double taper, drilled hole near bottom	3.5	5.0	95		5/pk	220-94734-02	8001-0159		
	Straight-through	2.6	5.0	95	500	5/pk	220-94767-00	8001-0151	220-94767-00	8001-0101
Split Liners										
	Straight with middle restriction	3.5	5.0	95	800	5/pk	221-41444-01	8001-0156	221-41444-01	8001-0106
	Straight with middle restriction, wool	3.5	5.0	95	800	5/pk	220-90784-00	8001-0157		
	Straight-through	3.4	5.0	95	860	5/pk		8001-0153		8001-0103
Direct Liners										
	For 0.53 mm id column	2.6	5.0	95	450	5/pk	220-94768-00	8001-0152	220-94768-00	8001-0102

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Supplies for Shimadzu GC Systems

Liners for 2010 and 2010 Plus Systems

	Description	ID (mm)	OD (mm)	Length (mm)	Volume (µL)	Unit	Similar to OEM Part No.	Agilent Ultra Inert Deactivation	Similar to OEM Part No.	Agilent Original Deactivation
Split/Splitless Liners										
	Single taper	3.4	5.0	95		5/pk	961-01480-07 221-48335-01	8001-0154	221-48335-01	8001-0104
Splitless Liners										
	Single taper, wool	3.5	5.0	95		5/pk	221-48876-02	8001-0160		
	Double taper, drilled hole near top	3.5	5.0	95		5/pk	220-94734-01	8001-0158		
	Double taper, drilled hole near bottom	3.5	5.0	95		5/pk	220-94734-02	8001-0159		
	Straight-through	2.6	5.0	95	500	5/pk	220-94767-00	8001-0151	220-94767-00	8001-0101
Split Liners										
	Straight-through	3.4	5.0	95	860	5/pk		8001-0153		8001-0103
	Straight with middle restriction	3.5	5.0	95	800	5/pk	221-41444-01	8001-0156	221-41444-01	8001-0106
	Straight with middle restriction, wool	3.5	5.0	95	800	5/pk	220-90784-00	8001-0157		
Other Liners										
	PTV	1.25	3.5	95	100	5/pk	221-49300-00	8001-0163		
	SPME or Purge and Trap, straight	0.75	5.0	95	50	5/pk	220-94769-00	8001-0162		

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Supplies for Shimadzu GC Systems

Liners for 17A Systems

	Description	ID (mm)	OD (mm)	Length (mm)	Volume (µL)	Unit	Similar to OEM Part No.	Agilent Ultra Inert Deactivation	Similar to OEM Part No.	Agilent Original Deactivation
Splitless Liners										
	Single taper, wool	3.5	5.0	95		5/pk	221-48876-02	8001-0160		
	Double taper, drilled hole near top	3.5	5.0	95		5/pk	220-94734-01	8001-0158		
	Double taper, drilled hole near bottom	3.5	5.0	95		5/pk	220-94734-02	8001-0159		
	Straight-through	2.6	5.0	95	500	5/pk	220-94767-00	8001-0151	220-94767-00	8001-0101
Split Liners										
	Straight with middle restriction, wool	3.5	5.0	95	800	5/pk	220-90784-00	8001-0157		
	Straight-through	3.4	5.0	95	860	5/pk		8001-0153		8001-0103
Direct Liners										
	For 0.53 mm id column	2.6	5.0	95	450	5/pk	220-94768-00	8001-0152	220-94768-00	8001-0102

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.



Agilent CrossLab Supplies for Shimadzu GC Systems

Liners for 14 Systems

	Description	ID (mm)	OD (mm)	Length (mm)	Volume (µL)	Unit	Agilent Ultra Inert Deactivation	Agilent Original Deactivation
Split/Splitless Liners								
	2.0 mm middle gooseneck	3.4	5.0	99	850	5/pk	8001-0155	8001-0105



Graphite O-rings

Liner O-rings

Description	Unit	Similar to OEM Part No.	Agilent CrossLab Part No.
Non-stick fluoroelastomer O-ring	10/pk	036-11203-84	8001-0201
Graphite O-ring, split	10/pk	221-48393-91	8001-0202
Graphite O-ring, splitless	10/pk	221-47222-91	8001-0203

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Supplies for Shimadzu GC Systems

Column Ferrules

Capillary Column Ferrules

Model	Fitting Size (in)	Ferrule ID (mm)	Column ID (mm)	Hole	Unit	Similar to OEM Part No.	Agilent CrossLab Part No.
85% Vespel/15% Graphite Capillary Column Ferrules							
QP5000/5050 Standard MS	1/16	0.3	0.18 or smaller	1	10/pk	220-90700-01	8001-0224
	1/16	0.4	0.25	1	10/pk	220-90700-02	8001-0221
	1/16	0.5	0.32	1	10/pk	220-90700-03	8001-0222
	1/16	0.8	0.53	1	10/pk	220-90700-04	8001-0223
QP2010	1/16	0.4	0.25	1	10/pk	220-90418-14	8010-0310
	1/16	0.4	0.25	2	10/pk	225-19056-00	8010-0312
	1/16	0.5	0.32	1	10/pk	220-90418-15	8010-0311
	1/16	0.8	0.53	1	10/pk	220-90418-18	8010-0313
Graphite Capillary Column Ferrules							
2010, 2010 Plus, 2014, 17A, 14A	1/16	0.4	0.25	1	10/pk	220-90765-00	8001-0211
	1/16	0.5	0.32	1	10/pk	221-32126-05	8001-0212
	1/16	0.8	0.53	1	10/pk	221-32126-08	8001-0213

Packed Column Ferrules

Model	Fitting Size (in)	Ferrule ID (in)	Column OD (in)	Hole	Unit	Similar to OEM Part No.	Agilent CrossLab Part No.
85% Vespel/15% Graphite Packed Column Ferrules							
QP5000/5050 Standard MS	1/4	1/4	1/4	1	10/pk	225-09028-00	8010-0314
QP5000/5050 Wide Bore MS	1/16	1/16	1/16	1	10/pk	220-90418-28	8010-0315
QP2010	1/16	1/16	1/16	1	10/pk		8010-0315
17A	5 mm	5 mm	5 mm od	1	10/pk	221-46403-92	8001-0214

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.



Graphite capillary column ferrules, 8001-0213

Agilent CrossLab Supplies for Shimadzu GC Systems

Column Nuts

Description	Unit	Similar to OEM Part No.	Agilent CrossLab Part No.
Column nut, slotted, 6-sided	2/pk	221-32705-00	8001-0311
Column nut, no slot, 6-sided	2/pk	221-41533-00	8001-0312

Autosampler Syringes for Shimadzu GC Systems, 1/pk

Model	Volume (µL)	Description	Needle Gauge/ Length (mm)/ Tip	Similar to OEM Syringe Part No.	Agilent CrossLab Syringe Part No.	Similar to OEM Replacement Needle and Plunger Repair Kit Part No.	Agilent CrossLab Replacement Needle Part No.
AOC-14, AOC-17, AOC-20	5	Removable needle	23/42/cone tip		8001-0010		8001-0011
AOC-14, AOC-17, AOC-20	10	Removable needle	23/42/cone tip	220-90282-20	8001-0004	220-90281-20	8001-0005, 2/pk
AOC-14, AOC-17, AOC-20		Removable needle	26/42/cone tip	220-90282-21	8001-0006	220-90281-21	8001-0007, 2/pk
AOC-14, AOC-17, AOC-20	50	Removable needle	23/42/cone tip	221-45243-00	8001-0012		8001-0014
AOC-14, AOC-17, AOC-20	250	Removable needle, gas tight	23/42/cone tip	221-45244-00	8001-0013		8001-0014

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

TIPS & TOOLS

For a comprehensive vial compatibility chart, identification guide, septum recommendations, and ordering information, see the complete CrossLab Vials and Closures section of our General Chromatography catalog, publication number 5991-1056EN.

Agilent CrossLab Supplies for Shimadzu GC Systems

Inlet Septa

Non-Stick Bleed and Temperature Optimized (BTO) Septa

Description	Agilent CrossLab Part No. 50/pk	Agilent CrossLab Part No. 100/pk
Shimadzu plug	8010-0231	8010-0232

Non-Stick Advanced Green Septa

Description	Agilent CrossLab Part No. 50/pk	Similar to OEM Part No.	Agilent CrossLab Part No. 100/pk
Shimadzu plug	8010-0215	220-90547-00 220-94781-00	8010-0216

General Purpose Septa

Description	Agilent CrossLab Part No. 50/pk	Agilent CrossLab Part No. 100/pk
Shimadzu plug	8010-0263	8010-0264

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Supplies for Thermo Scientific GC Systems

Liners for Trace, Focus Systems

	Description	ID (mm)	OD (mm)	Length (mm)	Volume (µL)	Unit	Similar to OEM Part No.	Agilent Ultra Inert Deactivation	Similar to OEM Part No.	Agilent Original Deactivation
Splitless Liners										
	Single taper	5.0	8.0	105	1750	5/pk	45350033	8002-0153	45350033	8002-0103
	Single taper	3.0	8.0	105		5/pk	45350032	8002-0154	45350032	8002-0104
Split Liners										
	Straight	5.0	8.0	105	2000	5/pk	45350030	8002-0151	45350030	8002-0101
	Straight	3.0	8.0	105	750	5/pk	45350031	8002-0152	45350031	8002-0102
PTV Liners										
	Straight	2.0	2.75	120	375	5/pk	45322045	8002-0156*	45322045	8002-0106*
	Straight with bottom restriction	2.0	2.75	120	375	5/pk	45352057	8002-0157	45352057	8002-0107
	6 baffles	2.0	2.75	120		5/pk	453T2120	8002-0160*		
	Straight	1.75	2.75	120	300	5/pk		8002-0155		8002-0105
	Straight	1.0	2.75	120	90	5/pk	45352054	8002-0161		
	3 baffles	1.0	2.75	120		5/pk	45352062	8002-0159*		

*Use in Trace systems only

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Supplies for Thermo Scientific GC Systems

Liner O-rings

Description	Unit	Similar to OEM Part No.	Agilent CrossLab Part No.
Non-stick fluoroelastomer O-ring, sintered liner	10/pk	29031305	8002-0201
Non-stick fluoroelastomer O-ring	10/pk	29030306	8010-0401
Graphite O-ring, 8 mm od	2/pk	29033406	8002-0203
Graphite O-ring, PTV	2/pk	29013417	8002-0204

Column Ferrules

Capillary Column Ferrules

Model	Fitting Size (in)	Ferrule ID (mm)	Column ID (mm)	Hole	Unit	Similar to OEM Part No.	Agilent CrossLab Part No.
85% Vespel/15% Graphite Capillary Column Ferrules							
Injectors/Detectors	1/16	0.4	0.25	1	10/pk	290VT186	8002-0220
	1/16	0.5	0.32	1	10/pk	290VT187	8002-0221
	1/16	0.8	0.53	1	10/pk	290VT188	8002-0222
Any GC/MS Interface	1/16	0.4	0.25	1	10/pk	29033496	8010-0310
	1/16	0.5	0.32	1	10/pk	29033497	8010-0311
Graphite Capillary Column Ferrules							
Trace/Focus Injectors/Detectors (not for GC/MS Interface)	M4	0.3	0.18	1	10/pk		8002-0211
	M4	0.4	0.25	1	10/pk	29053488	8002-0212
	M4	0.5	0.32	1	10/pk	29053487	8002-0213
	M4	0.8	0.53	1	10/pk	29053486	8002-0214
Injectors/Detectors	1/16	0.4	0.25	1	10/pk		8002-0215
	1/16	0.5	0.32	1	10/pk		8002-0216
	1/16	0.8	0.53	1	10/pk		8002-0217

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Supplies for Thermo Scientific GC Systems

Column Nuts

Description	Unit	Similar to OEM Part No.	Agilent CrossLab Part No.
Column nut, stainless steel, split/splitless injector	2/pk	35032423	8002-0311
Column nut, brass	2/pk	290BT239	8002-0312

Autosampler Syringes for Thermo GC Systems, 1/pk

Model	Volume (µL)	Description	Needle Gauge/ Length (mm)/Tip	Similar to OEM Syringe Part No.	Agilent CrossLab Syringe Part No.	Similar to OEM Replacement Needle or Plunger Part No.	Agilent CrossLab Replacement Needle or Plunger Part No.
TriPlus, AS3000	0.5	Plunger-in-needle	23/50/cone tip	36504045	8010-0355		8010-0367*
TriPlus	5	Fixed needle	26/50/cone tip	36504047	8010-0353		
TriPlus, AS3000, AS2000, AS200, AS800	10	Fixed needle	23/50/cone tip	36520060	8010-0351		
		Fixed needle	26/50/cone tip	365D3711	8010-0352		
		Fixed needle	25/50/cone tip	36500525	8002-0003		
TriPlus, AS2000		Fixed needle	23/80/cone tip	36520061	8002-0002		
		Fixed needle	26/80/cone tip	36502019	8002-0001		
TriPlus, AS2000, AS200, AS800	100	Fixed needle, gas tight	23/50/cone tip		8010-0354		8010-0368**
TriPlus, AS2000		Removable needle, gas tight	23/50/side hole tip	36520050	8002-0004	36540040	8002-0005***

*Needle and plunger repair kit

**Replacement plunger

***Replacement needle

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts.

Agilent CrossLab Supplies for Thermo Scientific GC Systems

Inlet Septa

Non-Stick Bleed and Temperature Optimized (BTO) Septa

Description	Similar to OEM Part No.	Agilent CrossLab Part No. 50/pk	Similar to OEM Part No.	Agilent CrossLab Part No. 100/pk
9 mm, CenterGuide	31303240	8010-0217		8010-0218
9.5 mm		8010-0219		8010-0220
10 mm		8010-0221		8010-0222
11 mm, CenterGuide		8010-0223		8010-0224
11.5 mm, CenterGuide	31303230	8010-0225		8010-0226
Description		**24/pk**		**48/pk**
12.7 mm, CenterGuide		8010-0227	31303228	8010-0228
17 mm, CenterGuide		8010-0229	31303211	8010-0230

Non-Stick Advanced Green Septa

Description	Similar to OEM Part No.	Agilent CrossLab Part No. 50/pk	Similar to OEM Part No.	Agilent CrossLab Part No. 100/pk
9 mm, CenterGuide	313G3240	8010-0201		8010-0202
9.5 mm		8010-0203		8010-0204
10 mm		8010-0205		8010-0206
11 mm, CenterGuide	313G3230	8010-0207		8010-0208
11.5 mm, CenterGuide		8010-0209		8010-0210
Description		**24/pk**		**48/pk**
12.7 mm, CenterGuide		8010-0211	313G3228	8010-0212
17 mm, CenterGuide		8010-0213	313G3211	8010-0214



Non-stick advanced green septum, 11 mm, CenterGuide, 8010-0207

The cross references to the original equipment manufacturer (OEM) part numbers listed here serve as a recommendation that the CrossLab products are viable alternatives to OEM products. CrossLab products are compatible with the corresponding OEM instruments, although in some cases, the CrossLab products may have slightly different designs as compared to the OEM counterparts. All Agilent CrossLab supplies are backed by Agilent's 90-day money-back warranty.

Agilent CrossLab Supplies for Thermo Scientific GC Systems



Long-life septa, 8010-0239, 8010-0240

Non-Stick Long-Life Septa

Description	Agilent CrossLab Part No. 50/pk	Agilent CrossLab Part No. 100/pk
9 mm, CenterGuide	8010-0233	8010-0234
11 mm, CenterGuide	8010-0239	8010-0240
11.5 mm, CenterGuide	8010-0241	8010-0242
Description	**24/pk**	**48/pk**
12.7 mm, CenterGuide	8010-0243	8010-0244
17 mm, CenterGuide	8010-0245	8010-0246

General Purpose Septa

Description	Agilent CrossLab Part No. 50/pk	Agilent CrossLab Part No. 100/pk
9 mm	8010-0249	8010-0250
9.5 mm	8010-0251	8010-0252
10 mm	8010-0253	8010-0254
11 mm	8010-0255	8010-0256
11.5 mm	8010-0257	8010-0258
12.7 mm	8010-0259	8010-0260
17 mm	8010-0261	8010-0262

TIPS & TOOLS

For a comprehensive vial compatibility chart, identification guide, septum recommendations, and ordering information, see the complete CrossLab Vials and Closures section of our General Chromatography catalog, publication number 5991-1056EN.

For more information, please visit
www.agilent.com/chem/CrossLabGC

Agilent CrossLab Supplies for CTC GC Autosamplers



Autosampler Syringes for CTC CombiPAL and GC PAL, 1/pk

Volume (µL)	Description	Needle Gauge/ Length (mm)/Tip	Agilent CrossLab Syringe Part No.	Agilent CrossLab Replacement Needle or Plunger Part No.
0.5	Plunger-in-needle	23/50/cone tip	8010-0355	8010-0367*
5	Fixed needle	23/50/cone tip	8010-0356	
	Fixed needle	26/50/cone tip	8010-0353	
10	Fixed needle	23/50/cone tip	8010-0351	
	Fixed needle	25/50/cone tip	8002-0003	
	Fixed needle	26/50/cone tip	8010-0352	
	Fixed needle, gas tight	26/50/cone tip	8010-0357	8010-0359**
	Fixed needle	26/50/bevel tip	8010-0358	
25	Fixed needle	26/50/cone tip	8010-0360	
100	Fixed needle, gas tight	23/50/cone tip	8010-0354	
	Removable needle, gas tight	23/50/side hole tip	8002-0004	8002-0005***
	Fixed needle	26/50/cone tip	8010-0361	
250	Fixed needle, gas tight	26/50/cone tip	8010-0362	

Volume (mL)	Description	Needle Gauge/ Length (mm)/Tip	Agilent CrossLab Syringe Part No.	Agilent CrossLab Replacement Needle or Plunger Part No.
1	Fixed needle, gas tight, headspace	23/56/side hole tip	8010-0363	8010-0365
2.5	Fixed needle, gas tight, headspace	23/56/side hole tip	8010-0364	8010-0366

*Needle and plunger repair kit

**Replacement plunger

***Replacement needle

Product Index

Agilent J&W GC Columns

Application and Method Guides
ASTM Methods 229-236
Application Cross Reference Guide 210-212
EPA Methods
Drinking Water 213-216
Solid Waste 220-227
Waste Water 217-220
United States Pharmacopoeia (USP) GC Phases 228
Capillary Columns
By Group
Foods, Flavors and Fragrances 352
High Temperature 314
Life Sciences 362
Low-bleed GC/MS 244
Non-Bonded 387
PAH 338
PLOT 368
Pesticides 315
Petroleum 318
Polyethylene Glycol (PEG) 304
Premium Polysiloxane 269
Semivolatiles 340
Ultra Inert 237
Volatiles 344
By Stationary Phase
Biodiesel 328
CAM 388
CP Wax 58 FFAP CB 312
CP-1301 300
CP-Al2O3/KCl 375-377
CP-Al2O3/Na2SO4 375-377
CP-Carbowax 400 for Volatiles in Alcohol 356
CP-Chirasil Val 360
CP-Chirasil-Dex CB 360
CP-Cyclodextrin-B-2,3,6-M-19 361
CP-FFAP CB for Free Fatty Acids in Dairy Products 358
CP-Molsieve 5Å 385
CP-Select 624 CB 346
CP-Select CB for MTBE 350
CP-Sil 13 CB 288
CP-Sil 19 CB 302-303
CP-Sil 19 CB for Pesticides 336
CP-Sil 2 CB 325
CP-Sil 24 CB 293
CP-Sil 43 CB 298
CP-Sil 5 CB 275-278
CP-Sil 5 CB for Formaldehyde 319
CP-Sil 5 CB for Sulfur 326
CP-Sil 5/C18 CB for PCB 342
CP-Sil 8 CB 286-287
CP-Sil 8 CB for Amines 332
CP-Sil 8 CB for PCB 340
CP-Sil 8 CB for Pesticides 335
CP-Sil 88 353
CP-Sil 88 for Dioxins 343
CP-Sil 88 for FAME 354
CP-Sil PAH CB UltiMetal 339
CP-Sil PONA CB 320
CP-Sil PONA for ASTM D 5134 320
CP-SilicaPLOT 381
CP-SimDist 323
CP-TAP CB for Triglycerides 357
CP-TCEP for Alcohols in Gasoline 325
CP-Volamine 331
CP-Wax 52 CB 308-309
CP-Wax 57 CB 355
CP-Wax 57 CB for Glycols and Alcohols 356
CP-Wax for Volatile Amines and Diamines 332
CarboBOND 382
CarboPLOT P7 382
Carbowax 20M 313
CycloSil-B 358
Cyclodex-B 359
DB-1 269-272
DB-1301 299
DB-17 291
DB-1701 301
DB-1701P 334
DB-17ht 316
DB-17ms 258
DB-1ht 314
DB-1ms 245
DB-1ms Ultra Inert 240
DB-200 295
DB-210 296
DB-225 297
DB-225ms 262
DB-23 294
DB-2887 322
DB-35 289
DB-35ms 256
DB-35ms Ultra Inert 242
DB-5 281-283
DB-5.625 341
DB-502.2 349
DB-5ht 315
DB-5ms 249-250
DB-5ms EVDX 363
DB-5ms Ultra Inert 241
DB-608 336
DB-624 344-345
DB-624 Ultra Inert 242, 344
DB-ALC 1 362
DB-ALC 2 362
DB-CLP 1 333
DB-CLP 2 333
DB-Dioxin 343
DB-EUPAH 338
DB-FFAP 310
DB-HT Sim Dis 322
DB-MTBE 349
DB-Petro 321
DB-Select 624 UI for <467> 364
DB-TPH 350
DB-UI 8270D 242
DB-UI 8270D for Semivolatiles 340
DB-VRX 347
DB-WAX 304-305
DB-WAX FF 304-305
DB-WAXetr 306
DB-XLB 254
DX-1 389
DX-4 389
GS-Alumina 379
GS-Alumina KCl 375
GS-CarbonPLOT 383
GS-GasPro 380
GS-OxyPLOT 318
GS-Q 372
HP-1 273-274
HP-1 Aluminum Clad 321
HP-101 387
HP-17 387
HP-1ms 246
HP-1ms Ultra Inert 240
HP-20M 313
HP-35 290
HP-5 284-285
HP-50+ 292
HP-5ms 251
HP-5ms Semivolatile 342
HP-5ms Ultra Inert 241
HP-88 352
HP-Blood Alcohol 363
HP-Chiral B 359
HP-FFAP 311
HP-Fast Residual Solvent 364
HP-INNOWax 307
HP-PAS5 336-337
HP-PLOT Al2O3 KCl 374
HP-PLOT Al2O3 M 380
HP-PLOT Al2O3 S 378
HP-PLOT Molesieve 384
HP-PLOT Q 371
HP-PLOT U 374
HP-PONA 319
HP-VOC 346-348
Lowox 318
PoraBOND Q 368
PoraBOND U 369
PoraPLOT Amines 332
PoraPLOT Q 369-370
PoraPLOT Q-HT 369-370
PoraPLOT S 372-373
PoraPLOT U 372-373
Rapid-MS 337
SE-30 390
SE-54 390
Select Al2O3 MAPD 327
Select Biodiesel 330
Select FAME 353-354
Select Low Sulfur 326
Select Mineral Oil 351
Select PAH 338
Select Silanes 331
Select for Permanent Gases 327
Ultra 1 278-279
Ultra 2 280
VF-1301ms 266
VF-1701 Pesticides 335
VF-1701ms 267-268
VF-17ms 259
VF-1ms 247-248
VF-200ms 261
VF-23ms 260

VF-35ms....257
VF-5 Pesticides....333-334
VF-5ht....317
VF-5ms....252-253
VF-624ms....265
VF-DA....362
VF-WAXms....263-264
VF-Xms....255
Metal Columns....365
Column Selection
Column Diameter....204-205
Column Film Thickness....208-209
Column Length....206-207
Polarity....200-201
Selecting Stationary Phases....196-199
Custom Ordering....410
Fused Silica Tubing
Deactivated....397-398
Undeactivated....399
Guard Columns
DuraGuard....391
EZ-Guard....392
Installation and Troubleshooting
Causes of Column Performance Degradation....417-419
Quick Reference Guide....414-416
Troubleshooting Guides
Baseline Instability or Disturbances....424
Change in Peak Size....426
Excessive Baseline Noise....424
Loss of Resolution....427
Retention Time Shift....426
Split Peaks....425
Tailing Peaks....425
LTM Column Modules....393-394
Packed Columns
For Agilent 7820, 7890, and 6890 Instruments
0.1% SP-1000....407
1.5% OV-101....405
10% OV-101....405
10% PEG-20M....405
10% UC W982....407
12% UC W982....407
15% Carbowax 1540....400
15% Hallcomid m-18....402
20% Carbowax 20M....400
20% OV-101....405
20% PEG-20M....405
20% Sebaconitrile....406
20% Sebaconitrile/2% H3PO4....407
20% TCEP....407
25% DC-200....401
25% SP-2100....407
30% DC 200/500....402
30% DC-200....401
35% DC-200....401
5% Carbowax 20M....400
7% Carbowax M + 3% Polyphenolether 6 ring + 2% KOH....401
Carbosieve S....400
Carboxen-1000....401
Chromosorb 101....401
Chromosorb 102....401
HayeSep D....402
HayeSep DB....402
HayeSep N....402
HayeSep N + HayeSep R 1:1....402
HayeSep Q....403
HayeSep R....403
HayeSep T....403
MolSieve 13X....404
MolSieve 5Å....404
Porapak N....405
Porapak N + Porapak R 1:1....405
Porapak Q....406
Porapak QS....406
Porapak R....406
Porapak T....406
Silica Gel....407
For All Instruments
1.5% OV-101....409
10% SE-30....409
20% TCEP....409
30% DC 200/500....408
HayeSep D....408
HayeSep DB....408
HayeSep N....408
HayeSep P....408
HayeSep Q....408
HayeSep R....408
MolSieve 13X....409
MolSieve 5Å....409
Porapak QS....409
Silica Gel....409
Test Standards....411-412

Agilent Supplies

Bulk GC Supplies....14
Capillary Column Ferrules
Column Nuts....33-34
Ferrule Selection Recommendations....30-31
For LTM Rapid Heating/Cooling System....35
For NCD and SCD....35
Reducing....35
Specialty....33-34
Straight....35
Capillary Flow Technology
Column/Retention Gap Installation....37
Ferrules....37
Fittings....37
Ultimate Union....36-37
Column Connectors and Splitters
Graphpak....39
Press-fit....38
Column Nuts....33-34
Detector Systems
Electron Capture Detector (ECD)....86-87
Flame Ionization Detector (FID)....78
Flame Photometric Detector (FPD)....94
Nitrogen Chemiluminescence Detector (NCD)....106
Nitrogen Phosphorus Detector (NPD)....101
Sulfur Chemiluminescence Detector (SCD)....107
Thermal Conductivity Detector (TCD)....89-91
GC/MS
220-MS....136
240-MS Ion Trap....134-135
7000A Triple Quadropole GC/MS....132-133
Cleaning and Maintenance....116-117
Electron Multipliers....127
GC/MSD Interface....122-123
Ion Source
Chemical Ionization (CI) Ion Source....121
Electron Impact (EI) Ion Source....119-120
MSD Contamination....110-111
MSD Filaments....125
Maintenance Schedule....109
Mass Spectrometer Symptoms....114-116
Quadropole Mass Filter....126
QuickSwap MS Interface....124
Standards
Analyzer Kit Standards....137
Test and Performance Samples....137-138
Vacuum Systems and Pumps
Diffusion Pump....130
Foreline Pump....131
Pressure Symptoms....128-129
Inlet Liners
Specialty Injection
Direct Connect....28
MultiMode Inlet Heavy Matrix....27
PTV....28
Split, Original Deactivation....25
Splitless, Original Deactivation....26
Ultra Inert....24
Inlet Septa
Advanced Green....17
Bleed and Temperature Optimized (BTO)....16
General Purpose....19
Long-Life....17
Inlet Systems
Cool On-Column....66
Flip Top Inlet Sealing System....57
Inlet Convenience Kits....55
Multimode....64
Programmable Temperature Vaporizer (PTV)....69-70
Purged Packed....74-75
Split/Splitless Inlet Seals....56, 58-59
Liner O-rings....29
Maintenance Schedule....12-13
Markes Thermal Desorption....53-54
Merlin Microseal....20-21
Oven Exhaust Deflector....107
Purge and Trap Systems
Archon....52
Teledyne Tekmar....50-51
Sample Introduction Systems
7693A Automatic Liquid Sampler....43-44
7697A Headspace Sampler....45-47
Automatic Liquid Sampler....44
G1883A Network Headspace Sampler....49
G1888A Network Headspace Sampler....48
G3520A XLSI Accessory....46
Standards....108
Valves and Loops....40

Applications

Energy and Fuels....552
Environmental
Air Analysis....473
Hydrocarbons....429
Pesticides and Herbicides....434
Semivolatiles....458
Volatiles....468
Food, Flavor and Fragrance....478

Industrial Chemical 487
Life Science....521

CrossLab Supplies

Bruker, Varian GC Systems
Autosampler Syringes....158
Capillary Column Ferrules 157
Column Nuts 158
Detector Replacement
Flame Ionization Detector (FID)....166
Pulsed Flame Photometric Detector (PFPD)....167-168
Thermal Conductivity Detector (TCD)....166
Thermionic Specific Detector (TSD)....168
Injector Replacement
1041 Packed/Wide Bore On-Column (PWOC) injector 165
1061 Packed/530 µm Capillary Column Injector....164
1079 Large Volume Injector (LVI)....162
1093 Cool On-Column (COC) Injector 163
1177 Split/Splitless Injector....161-168
Inlet Liners
1060/1061 Injector....156
1075/1077 Injector....156
1078/1079 Injector....155-156
1093/1094 Injector....155-156
1177 Injector 154-160
Inlet Septa....159-160
Liner O-rings....156
Packed Column Ferrules....158
CTC GC Autosamplers
Autosampler Syringes....187
Column Ferrules....143
Inlet Liners 140-141
Inlet Septa
Advanced Green 151
Bleed and Temperature Optimized (BTO) 150
General Purpose 153
Long-Life....152
Liner O-rings 142
Perkin Elmer GC Systems
Autosampler Syringes....173
Capillary Column Ferrules 171
Column Nuts 172
Inlet Liners
AutoSystem....169-174
AutoSystem XL....169-174
Clarus....169-174
Inlet Septa....174
Liner O-rings....170
Packed Column Ferrules....172
Shimadzu GC Systems
Autosampler Syringes....180
Capillary Column Ferrules 179
Column Nuts 180
Inlet Liners
14 Systems....178
17A Systems....177
2010 and 2010 Plus Systems....176
2014 Systems....175-180
Inlet Septa....181
Liner O-rings....178
Packed Column Ferrules....179
Syringes 145-146
Thermo Scientific GC Systems
Autosampler Syringes....184
Capillary Column Ferrules 183
Column Nuts 184
Inlet Liners
Focus Systems....182-186
Trace Systems....182-186
Inlet Septa....185-186
Liner O-rings....183

Part Number Index

0100-1104 35
0100-1324 35
0100-1325 35
0100-1326 35
0100-1331 35
0100-1332 ..... 35, 77, 91
0100-1342 35
0100-1344 35
0100-1365 35
0100-1375 ..... 35, 72
0100-1378 35
0100-1379 35
0100-1381 35
0100-2594 46
0101-0282 42
0101-0299 42
0101-0300 42
0101-0301 42
0101-0302 42
0101-0303 42
0101-0355 41
0101-0403 41
0101-0532 41
0101-0584 40
0101-0585 40
0101-0633 41
0101-0636 40
0101-0637 40
0101-0638 40
0101-0639 40
0410105017 48
0510-1306 62
0515-0655 105
0515-0680 99
0515-0683 100
0515-1084 99
0515-1799 76
0515-2495 105
0515-2711 76
0515-2712 84
05890-61525 43
05890-80660 41
05921-21170 ..... 34, 117
05970-60045 138
05971-20134 120
05971-20143 120
05971-60140 125
05971-60561 116
05971-80102 127
05971-80103 ..... 127, 133
05980-20018 116
05980-60051 ..... 116, 133
05988-20066 ..... 34, 117
05990-60075 138
07673-20570 44
07673-40180 43
07673-60840 44
07675-80050 42
0854-0141 99
0905-1284 105
0905-1463 132
0905-1610 99
0905-2580 105
0960-0897 125
1000-1437 100
1000-1438 100
112-2032 313
112-2032LTM 313
112-2112 388
112-2112LTM 388
112-2132 388
112-2132LTM 388
112-2133 388
112-2133LTM 388
112-2162 388
112-2532 359
112-2532E 359
112-2532LTM 359
112-2562 359
112-5432 390
112-5432LTM 390
112-5462 390
112-6632 358
112-6632LTM 358
112-8837 352
112-8837E 352
112-8837LTM 352
112-8867 352
112-8867E 352
112-88A7 352
112-88A7E 352
113-2032 313
113-2032LTM 313
113-2062 313
113-2132 388
113-2132E 388
113-2132LTM 388
113-2133 388
113-2133E 388
113-2133LTM 388
113-2532 359
113-2532E 359
113-2532LTM 359
113-3032 390
113-3032LTM 390
113-3112 383
113-3132 383
113-3132LTM 383
113-3133 383
113-3133LTM 383
113-3162 383
113-3432 372
113-3432E 372
113-3432LTM 372
113-4302 380
113-4312 380
113-4332 ..... 234, 380
113-4362 ..... 229, 380
113-5432 390
113-5432LTM 390
113-6632 358
113-6632LTM 358
115-2132 ..... 233, 388
115-2132LTM 388
115-3113 383
115-3133 383
115-3133LTM 383
115-3332 375
115-3332LTM 375
115-3352 375
115-3352E 375
115-3412 372
115-3412LTM 372
115-3422 372
115-3422LTM 372
115-3432 372
115-3432E 372
115-3432LTM 372
115-34H2 372
115-34H2LTM 372
115-3532 ..... 229-230, 379
115-3532E 379
115-3532LTM 379
115-3552 ..... 230, 236, 379
115-4912 318
115-4912E 318
121-0122 245
121-0122E 245
121-0122LTM 245
121-0122UI 240
121-0713 301
121-0713LTM 301
121-0722 ..... 214, 301
121-0722LTM 301
121-1012 270
121-1012E 270
121-1012LTM 270
121-1013 270
121-1013E 270
121-1013LTM 270
121-101A 270
121-101ALTM 270
121-1022 270
121-1022E 270
121-1022LTM 270
121-1023 270
121-1023LTM 270
121-1043 270
121-1043E 270
121-1222 254
121-1222E 254
121-1222LTM 254
121-1232 254
121-1313 299
121-1313LTM 299
121-1324 ..... 215, 219, 225-226, 235, 345
121-1324E 345
121-1324LTM 345
121-1324UI 226, 242, 344
121-1524 ..... 215, 219, 225-226, 235, 347
121-1524LTM 347
121-1544 347
121-1544E 347
121-1544LTM 347
121-1722 291
121-1722LTM 291
121-1723 291
121-1723LTM 291
121-2223 297
121-2223LTM 297
121-2323 294
121-2323LTM 294
121-3822 256
121-3822E 256
121-3822LTM 256
121-3822UI 242
121-4722 258
121-4722E 258
121-4722LTM 258
121-5012 281
121-5012E 281
121-5012LTM 281
121-5013 281
121-5013LTM 281
121-5022 281
121-5022E 281
121-5022LTM 281
121-5023 281
121-5023E 281
121-5023LTM 281
121-5042 281
121-5522 250
121-5522E 250
121-5522LTM 250
121-5522UI 214, 241
121-5522UILTM 241
121-5523 250
121-5523LTM 250
121-5523UI 241
121-5523UILTM 241
121-5542 250
121-5621 341
121-5621LTM 341
121-5622 341
121-5622G5 391
121-5622LTM 341
121-6822 336
121-6822LTM 336
121-7012 305
121-7012LTM 305
121-7022 305
121-7022E 305
121-7022LTM 305
121-7023 305
121-7023E 305
121-7023LTM 305
121-7042 305
121-7042E 305
121-7043 305
121-9627 338
121-9723 ..... 212, 226, 242, 340
122-0112 245
122-0112E 245
122-0112LTM 245
122-0112UI 240
122-0112UIE 240
122-0131 245
122-0132 ..... 223, 245
122-0132E 245
122-0132UI 240
122-0132UIE 240
122-0162 245
122-0162UI 240
122-0212 296
122-0212LTM 296
122-0232 296
122-0232E 296
122-0232LTM 296
122-0233 ..... 215, 296
122-0233LTM 296
122-0334UI 364
122-0364UI 364

122-0712 301
122-0712LTM 301
122-0713 301
122-0713LTM 301
122-0731 301
122-0731LTM 301
122-0732 ..... 214, 216, 301
122-0732E 301
122-0732LTM 301
122-0733 ..... 223, 301
122-0733E 301
122-0733LTM 301
122-0761 301
122-0762 301
122-0763 301
122-0763E 301
122-0766 301
122-1011 270
122-1011LTM 270
122-1012 270
122-1012LTM 270
122-1013 270
122-1013LTM 270
122-1022 270
122-1022LTM 270
122-1031 270
122-1031LTM 270
122-1032 270
122-1032E 270
122-1032G 391
122-1032LTM 270
122-1033 ..... 215, 270
122-1033E 270
122-1033LTM 270
122-103E 270
122-103ELTM 270
122-1052 270
122-1061 270
122-1062 270
122-1063 270
122-106E 229, 270
122-10A6 321
122-10A6E 234, 321
122-10AE 270
122-10G3 270
122-1111 314
122-1111E 314
122-1131 314
122-1211 254
122-1211LTM 254
122-1212 254
122-1231 254
122-1232 ..... 215, 217, 221, 233-236, 254
122-1232G 391
122-1232LTM 254
122-1233 254
122-1236 ..... 213, 254
122-1262 254
122-1262E 254
122-1332 299
122-1332E 299
122-1332LTM 299
122-1333 ..... 215, 299
122-1333LTM 299
122-1334 ..... 213, 217, 220-221, 345
122-1334E 345
122-1334LTM 345
122-1334UI 213, 220-221, 242, 344
122-1362 299
122-1363 299
122-1363E 299
122-1364 ..... 213, 215, 217, 219, 235, 345
122-1364E 345
122-1364UI 213, 215, 225, 242, 344
122-1464 349
122-1534 ..... 213, 217, 220-221, 347
122-1534LTM 347
122-1564 ..... 213, 215, 217, 219-220, 225-226, 235, 347
122-1564E 347
122-1711 291
122-1711LTM 291
122-1712 291
122-1712LTM 291
122-1713 291
122-1713E 291
122-1713LTM 291
122-1731 291
122-1731E 291
122-1731LTM 291
122-1732 291
122-1732E 291
122-1732LTM 291
122-1733 291
122-1733LTM 291
122-1762 291
122-1801 316
122-1801LTM 316
122-1811 316
122-1831 316
122-1831LTM 316
122-1932 289
122-1932LTM 289
122-1962 289
122-2032 295
122-2032LTM 295
122-2033 295
122-2033LTM 295
122-2212 297
122-2212LTM 297
122-2231 297
122-2231LTM 297
122-2232 297
122-2232LTM 297
122-2312 294
122-2312LTM 294
122-2331 294
122-2331LTM 294
122-2332 294
122-2332E 294
122-2332LTM 294
122-2361 294
122-2361E 294
122-2362 ..... 236, 294
122-2362E 294
122-2461 343
122-2461E 343
122-2462 343
122-2912 262
122-2912LTM 262
122-2932 ..... 234, 262
122-2932E 262
122-2932LTM 262
122-2962 262
122-3212 310
122-3212LTM 310
122-3232 310
122-3232E 310
122-3232LTM 310
122-3233 310
122-3233LTM 310
122-3262 310
122-3262E 310
122-3263 310
122-3812 256
122-3812UI 242
122-3831 256
122-3832 ..... 213, 218, 224, 234-235, 256
122-3832E 256
122-3832LTM 256
122-3832UI 219, 242
122-3862 256
122-4711 258
122-4711LTM 258
122-4712 258
122-4712LTM 258
122-4731 258
122-4731LTM 258
122-4732 ..... 218, 223, 258
122-4732E 258
122-4732LTM 258
122-4762 258
122-5011 282
122-5011LTM 282
122-5012 ..... 234, 282
122-5012LTM 282
122-5013 282
122-5013LTM 282
122-501E 282
122-501ELTM 282
122-5022 282
122-5022LTM 282
122-5031 282
122-5031LTM 282
122-5032 ..... 235, 282
122-5032E 282
122-5032LTM 282
122-5033 ..... 220, 282
122-5033E 282
122-5033LTM 282
122-503E 282
122-503ELTM 282
122-5052 282
122-5061 282
122-5062 282
122-5063 282
122-506E 282
122-5511 250
122-5511LTM 250
122-5512 250
122-5512LTM 250
122-5512UI 215, 241
122-5512UILTM 241
122-5513 250
122-5513LTM 250
122-5513UI 241
122-5513UILTM 241
122-5516 250
122-5516LTM 250
122-5522 250
122-5522LTM 250
122-5522UI 241
122-5522UILTM 241
122-552A 250
122-552ALTM 250
122-5531 250
122-5531LTM 250
122-5532 ..... 213, 215-216, 221-224, 250
122-5532E 250
122-5532G 391
122-5532LTM 250
122-5532UI 214, 216-219, 241
122-5532UIE 241
122-5532UILTM 241
122-5533 ..... 215, 222-223, 227, 250
122-5533E 250
122-5533G 391
122-5533LTM 250
122-5533UI 214, 224, 241
122-5533UIE 241
122-5533UILTM 241
122-5536 ..... 218, 250
122-5536E 250
122-5536G 391
122-5536LTM 250
122-5536UI 241
122-5536UILTM 241
122-5552 250
122-5552UI 241
122-5561 250
122-5562 250
122-5562E 250
122-5562G 391
122-5562UI 218-219, 227, 241
122-5563 250
122-5563UI 241
122-5631 341
122-5631G5 391
122-5631LTM 341
122-5632 341
122-5632LTM 341
122-5633 341
122-5633LTM 341
122-5661 341
122-5711 315
122-5711E 315
122-5711LTM 315
122-5731 315
122-5731LTM 315
122-6133 389
122-6432 389
122-6432LTM 389
122-6462 389
122-6832 ..... 217-218, 336
122-6832LTM 336
122-7012 305
122-7012E 305
122-7012LTM 305
122-7013 ..... 221, 305
122-7013LTM 305
122-7031 305
122-7031LTM 305
122-7032 ..... 229, 305
122-7032E 305
122-7032LTM 305
122-7033 ..... 220, 227, 305
122-7033E 305
122-7033LTM 305
122-7061 305
122-7062 305
122-7062E 305
122-7063 305
122-7063E 305
122-7332 306
122-7332E 306
122-7332LTM 306

122-7333 306
122-7333LTM 306
122-7362 306
122-7363 306
122-7732 ..... 234-235, 334
122-7732LTM 334
122-96L2 338
122-9732 ..... 226, 242, 340
122-9736 ..... 242, 340
123-0112 245
123-0112UI 240
123-0131 245
123-0132 245
123-0132LTM 245
123-0132UI 240
123-0162 245
123-0213 296
123-0213LTM 296
123-0232 296
123-0232LTM 296
123-0233 296
123-0233LTM 296
123-0334UI 364
123-0364UI 364
123-0712 301
123-0712LTM 301
123-0713 301
123-0713LTM 301
123-0731 301
123-0731LTM 301
123-0732 301
123-0732E 301
123-0732LTM 301
123-0733 301
123-0733E 301
123-0733LTM 301
123-0753 301
123-0762 301
123-0763 301
123-0763E 301
123-100E 271
123-100ELTM 271
123-1011 271
123-1011LTM 271
123-1012 271
123-1012LTM 271
123-1013 271
123-1013LTM 271
123-1014 271
123-1014LTM 271
123-1015 271
123-1015LTM 271
123-1022 ..... 234, 271
123-1022LTM 271
123-1026 271
123-1026LTM 271
123-1027 271
123-1027LTM 271
123-102F 271
123-102FLTM 271
123-1031 271
123-1031LTM 271
123-1032 271
123-1032LTM 271
123-1033 ..... 233, 271
123-1033E 271
123-1033LTM 271
123-1034 271
123-1034LTM 271
123-1035 271
123-1035LTM 271
123-103B 271
123-103BLTM 271
123-103E 218, 223-224, 271
123-103ELTM 271
123-1052 271
123-1055 271
123-1056 271
123-105C 271
123-105F 271
123-1061 271
123-1062 271
123-1062E 271
123-1063 271
123-1063E 271
123-1064 271
123-1064E 271
123-1065 271
123-1065E 271
123-106B 271
123-106BE 271
123-106E 230, 271
123-106G 271
123-1111 314
123-1111LTM 314
123-1131 314
123-1131E 314
123-1131LTM 314
123-1232 254
123-1236 ..... 214, 216, 218, 222, 254
123-1262 254
123-1332 299
123-1332LTM 299
123-1333 299
123-1333LTM 299
123-1334 345
123-1334E 345
123-1334LTM 345
123-1334UI 242, 344
123-1363 299
123-1363E 299
123-1364 345
123-1364E 345
123-1364UI 226, 242, 344
123-1464 349
123-1534 ..... 234, 347
123-1534LTM 347
123-1564 347
123-1564E 347
123-1632 ..... 235, 350
123-1632LTM 350
123-1711 291
123-1711LTM 291
123-1712 291
123-1712LTM 291
123-1713 291
123-1713LTM 291
123-1730 ..... 214, 233, 336
123-1730LTM 336
123-1731 291
123-1731LTM 291
123-1732 291
123-1732E 291
123-1732LTM 291
123-1733 291
123-1733E 291
123-1733LTM 291
123-1762 291
123-1811 316
123-1831 316
123-1831E 316
123-1861 316
123-1932 289
123-1932LTM 289
123-1933 289
123-1933E 289
123-1933LTM 289
123-2032 295
123-2032LTM 295
123-2033 295
123-2033LTM 295
123-2232 297
123-2232E 297
123-2232LTM 297
123-2332 294
123-2332E 294
123-2332LTM 294
123-2362 294
123-2461 343
123-2462 343
123-2932 262
123-2932LTM 262
123-3212 310
123-3212LTM 310
123-3223 310
123-3223LTM 310
123-3232 ..... 232, 310
123-3232E 310
123-3232LTM 310
123-3233 310
123-3233LTM 310
123-3234 310
123-3234LTM 310
123-3253 310
123-3262 310
123-3263 310
123-3264 310
123-3812 256
123-3812UI 242
123-3832 ..... 222, 225, 256
123-3832E 256
123-3832UI 214, 216, 218, 225, 242
123-4712 258
123-4712LTM 258
123-4732 ..... 218, 258
123-4732LTM 258
123-500E 282
123-500ELTM 282
123-5011 282
123-5011LTM 282
123-5012 282
123-5012E 282
123-5012LTM 282
123-5013 282
123-5013E 282
123-5013LTM 282
123-5022 282
123-5022LTM 282
123-5026 282
123-5026LTM 282
123-502D 282
123-502DLTM 282
123-502F 282
123-502FLTM 282
123-5031 282
123-5031LTM 282
123-5032 282
123-5032E 282
123-5032LTM 282
123-5033 ..... 233, 282
123-5033E 282
123-5033LTM 282
123-503B 282
123-503BLTM 282
123-503E 282
123-503ELTM 282
123-5052 282
123-5053 282
123-5056 282
123-5062 282
123-5063 282
123-5063E 282
123-5511 250
123-5511LTM 250
123-5512 250
123-5512LTM 250
123-5513 250
123-5513E 250
123-5513LTM 250
123-5526 250
123-5526LTM 250
123-5531 250
123-5531LTM 250
123-5532 ..... 218, 223, 250
123-5532E 250
123-5532LTM 250
123-5532UI 225, 241
123-5532UIE 241
123-5532UILTM 241
123-5533 ..... 227, 250
123-5533G 391
123-5533LTM 250
123-5533UI 241
123-5533UILTM 241
123-5536 ..... 218, 223-224, 250
123-5536LTM 250
123-5536UI 241
123-5536UILTM 241
123-5561 250
123-5562 250
123-5563 250
123-5563UI 241
123-5566 250
123-5631 341
123-5631LTM 341
123-5632 341
123-5632LTM 341
123-5701 315
123-5701LTM 315
123-5711 315
123-5711E 315
123-5731 315
123-5731E 315
123-5731LTM 315
123-6133 389
123-6133LTM 389
123-6412 389
123-6412LTM 389
123-6432 389
123-6432LTM 389
123-6462 389
123-7012 305
123-7012LTM 305
123-7013 305
123-7013LTM 305
123-7031 305
123-7031LTM 305
123-7032 305
123-7032E 305
123-7032LTM 305

123-7033 305
123-7033E 305
123-7033LTM 305
123-7062 ..... 232, 305
123-7063 305
123-7063E 305
123-7312 306
123-7312LTM 306
123-7314 306
123-7314LTM 306
123-7332 306
123-7332LTM 306
123-7333 306
123-7333LTM 306
123-7334 306
123-7334LTM 306
123-7354 306
123-7354E 306
123-7362 306
123-7363 306
123-7364 ..... 236, 306
123-7722 334
123-7722LTM 334
123-7732 334
123-7732E 334
123-7732LTM 334
123-8232 ..... 213-214, 216, 222, 225, 333
123-8336 ..... 213-214, 216, 222, 225, 333
123-9134 362
123-9134LTM 362
123-9234 362
123-9234E 362
123-9234LTM 362
123-9612 338
123-BD01 329
123-BD11 329
123-BD34 329
124-0034 349
124-0034LTM 349
124-1032 271
124-1032LTM 271
124-1034 271
124-1034LTM 271
124-1334 ..... 231, 234, 345
124-1334LTM 345
124-1374 ..... 217, 345
124-1474 349
124-14A4 349
124-1534 ..... 232, 347
124-1534LTM 347
124-1574 ..... 232, 347
124-1632 350
124-1730 336
124-1730LTM 336
124-3232 ..... 233, 310
124-3232LTM 310
124-5012 283
124-5012LTM 283
124-5032 283
124-5032LTM 283
124-5037 283
124-5037LTM 283
124-7032 ..... 231, 233, 305
124-7032LTM 305
125-0034 349
125-0034E 349
125-0034LTM 349
125-0212 ..... 230, 296
125-0212LTM 296
125-0232 296
125-0232LTM 296
125-0334UI 364
125-0712 301
125-0712E 301
125-0712LTM 301
125-0731 301
125-0731LTM 301
125-0732 301
125-0732E 301
125-0732G 391
125-0732LTM 301
125-0733 301
125-0733LTM 301
125-0737 301
125-0737LTM 301
125-0762 301
125-0762E 301
125-1002 272
125-1002LTM 272
125-1005 272
125-1005LTM 272
125-100A 272, 274
125-100ALTM 272
125-100B 272
125-100BLTM 272
125-1011 272
125-1011E 272
125-1011LTM 272
125-1012 272
125-1012E 272
125-1012LTM 272
125-1014 272
125-1014LTM 272
125-1015 272
125-1015LTM 272
125-1017 272
125-1017LTM 272
125-101J 272
125-101JLTM 272
125-101K 272
125-101KLTM 272
125-1025 272
125-1025LTM 272
125-102J 272
125-102JLTM 272
125-1032 272
125-1032LTM 272
125-1034 ..... 234, 272
125-1034E 272
125-1034LTM 272
125-1035 ..... 229, 235-236, 272
125-1035E 272
125-1035LTM 272
125-1037 272
125-1037LTM 272
125-1039 272
125-103B 272
125-103BLTM 272
125-103J 272
125-103JLTM 272
125-103K 272
125-103KE 272
125-103KLTM 272
125-1055 272
125-1062 272
125-1062E 272
125-1064 272
125-1065 272
125-1065E 272
125-106J 272
125-106JE 272
125-10B5 272
125-10H5 272
125-10H5LTM 272
125-10HB 272
125-10HBE 272
125-10HBLTM 272
125-1131 314
125-1212 254
125-1212LTM 254
125-1232 254
125-1232LTM 254
125-1312 299
125-1312LTM 299
125-1314 345
125-1332 299
125-1332LTM 299
125-1333 299
125-1333LTM 299
125-1334 ..... 230-231, 236, 345
125-1334E 345
125-1334G5 391
125-1334LTM 345
125-1334UI 242, 344
125-1364 345
125-1364E 345
125-1374 ..... 217, 345
125-1374E 345
125-1374UI 242, 344
125-14A4 349
125-1704 291
125-1704LTM 291
125-1710 336
125-1710LTM 336
125-1711 291
125-1711LTM 291
125-1712 291
125-1712LTM 291
125-1713 291
125-1713LTM 291
125-1717 291
125-1717LTM 291
125-1730 ..... 233, 336
125-1730LTM 336
125-1731 291
125-1731LTM 291
125-1732 291
125-1732E 291
125-1732LTM 291
125-1733 291
125-1733LTM 291
125-1737 291
125-1737LTM 291
125-1762 291
125-1912 289
125-1912LTM 289
125-1932 289
125-1932LTM 289
125-1937 289
125-1937LTM 289
125-2032 295
125-2032LTM 295
125-2212 ..... 223, 297
125-2212LTM 297
125-2232 297
125-2232LTM 297
125-2237 297
125-2237LTM 297
125-2312 294
125-2312LTM 294
125-2332 294
125-2332LTM 294
125-2814 ..... 230-231, 234, 322
125-2814E 322
125-2814LTM 322
125-3212 310
125-3212LTM 310
125-3217 310
125-3217LTM 310
125-3231 310
125-3231LTM 310
125-3232 310
125-3232E 310
125-3232LTM 310
125-3233 310
125-3233LTM 310
125-3237 310
125-3237LTM 310
125-3262 310
125-32H2 310
125-32H2LTM 310
125-3832 256
125-3832LTM 256
125-3837 256
125-3837LTM 256
125-5012 ..... 223, 283
125-5012E 283
125-5012LTM 283
125-5017 283
125-5017LTM 283
125-501J 283
125-501JLTM 283
125-501K 283
125-501KLTM 283
125-5025 283
125-5025LTM 283
125-5032 ..... 233, 283
125-5032E 283
125-5032LTM 283
125-5034 283
125-5034E 283
125-5034LTM 283
125-5035 283
125-5035E 283
125-5035LTM 283
125-5037 283
125-5037LTM 283
125-503B 283
125-503BLTM 283
125-503D 283
125-503DLTM 283
125-503J 283
125-503JLTM 283
125-503K 283
125-503KLTM 283
125-5062 283
125-5062E 283
125-5065 283
125-5065E 283
125-50HB 283
125-50HBLTM 283
125-5512 250
125-5512LTM 250
125-5532 250
125-5532LTM 250
125-5537 250
125-5537G 391
125-5537LTM 250

125-553J....250
125-553JLTM....250
125-6837....220-222, 225-226, 336
125-6837LTM....336
125-7012....305
125-7012E....305
125-7012LTM....305
125-7017....305
125-7017LTM....305
125-7031....305
125-7031LTM....305
125-7032....230-231, 305
125-7032E....305
125-7032LTM....305
125-7037....305
125-7037LTM....305
125-7062....305
125-7062E....305
125-7312....306
125-7312LTM....306
125-7314....306
125-7314LTM....306
125-7332....306
125-7332E....306
125-7332LTM....306
125-7333....306
125-7333LTM....306
125-7334....306
125-7334E....306
125-7334LTM....306
125-7362....306
125-7732....334
125-7732LTM....334
125-9134....362
125-9134E....362
125-9134LTM....362
125-9234....362
125-9234LTM....362
126-1012....269
126-1012LTM....269
126-1013....269
126-1013LTM....269
126-1713....291
126-1713LTM....291
126-7012....304
126-7012LTM....304
126-7013....304
126-7013LTM....304
127-0112....245
127-0112LTM....245
127-0113....245
127-0122....245
127-0123....245
127-0123LTM....245
127-0722....301
127-0722LTM....301
127-0723....301
127-0723LTM....301
127-100A....269
127-100ALTM....269
127-1012....269
127-1012E....269
127-1012LTM....269
127-1013....269
127-1013E....269
127-1013LTM....269
127-1022....269
127-1022E....269
127-1022LTM....269
127-1023....269
127-1023E....269
127-1023LTM....269
127-1043....269
127-1046....269
127-1046E....269
127-1712....291
127-1712LTM....291
127-1713....291
127-1713LTM....291
127-1722....291
127-1722LTM....291
127-2222....297
127-2222LTM....297
127-3212....310
127-3212LTM....310
127-32H2....310
127-32H2LTM....310
127-5012....281
127-5012E....281
127-5012LTM....281
127-5013....281
127-5013LTM....281
127-501E....281
127-501EE....281
127-501ELTM....281
127-501N....281
127-501NLTM....281
127-5022....281
127-5022E....281
127-5022LTM....281
127-5023....281
127-5023LTM....281
127-7012....304
127-7012E....304
127-7012LTM....304
127-7013....304
127-7013LTM....304
127-7022....304
127-7022LTM....304
127-7023....304
127-7023E....304
127-7023FF....305
127-7023LTM....304
128-0112....245
128-0112LTM....245
128-0122....245
128-0122E....245
128-0122LTM....245
128-1012....270
128-1012LTM....270
128-1022....270
128-1022LTM....270
128-1034....270
128-1034LTM....270
128-1052....270
128-1056....235, 321
128-1212....254
128-1212E....254
128-1222....254
128-1324....345
128-1324E....345
128-1324LTM....345
128-3812....256
128-3822....256
128-5012....282
128-5012LTM....282
128-5022....282
128-5022LTM....282
128-5052....282
128-50H7....282
128-50H7LTM....282
128-5512....250
128-5512LTM....250
128-5522....250
128-5522LTM....250
128-5552....250
128-7022....305
128-7022LTM....305
128-7032....305
128-7032LTM....305
128-7052....305
128-7323....306
128-7323LTM....306
128-8522....363
12A-1015....270
12A-1015LTM....270
12A-5015....281
12A-5015LTM....281
1300502506....48
1390-1023....76
14-8911-003....51
1400-0015....105
145-1001....236, 322, 365-366
145-1009....322, 365-366
145-1011....234, 366
145-1032....366
145-1334....367
145-2814....365-366
145-7032....367
1500334701....166, 168
1530-2163....42
1530-2167....42
1535-4952....40, 46
1535-4954....40
160-1010-1....397
160-1010-10....397
160-1010-5....397
160-2200-10....399
160-2200-5....399
160-2205-1....397
160-2205-10....397
160-2205-5....397
160-2250-10....399
160-2250-5....399
160-2255-1....398
160-2255-10....398
160-2255-30....398
160-2255-5....37, 46, 398
160-2320-10....399
160-2320-5....399
160-2325-1....398
160-2325-10....398
160-2325-30....398
160-2325-5....37, 46, 398
160-2450-10....399
160-2450-5....399
160-2455-1....398
160-2455-10....398
160-2455-5....46, 398
160-2530-10....399
160-2530-5....399
160-2535-1....398
160-2535-10....398
160-2535-30....398
160-2535-5....37, 46, 398
160-2610-10....399
160-2610-5....399
160-2615-1....397
160-2615-10....397
160-2615-5....397
160-2625-1....37, 397
160-2625-10....37, 397
160-2625-5....37, 397
160-2634-10....399
160-2634-5....399
160-2635-1....397
160-2635-10....397
160-2635-5....397
160-2644-10....399
160-2644-5....399
160-2650-10....399
160-2650-5....399
160-2655-1....397
160-2655-10....397
160-2655-5....397
160-2660-5....399
160-2815-5....398
160-2825-5....398
160-2845-10....398
160-2845-5....398
160-2855-10....398
160-2855-5....398
160-2865-10....398
160-2865-5....398
160-4535-5....46, 398
18596-40015....44
18710-20119....81, 85, 104-105
18710-60170....85, 91
18711-60060....91
18713-60040....88
18713-60050....88
18740-20800....63
18740-20880....56, 63
18740-60830....62
18740-60835....62, 64, 71-72, 76-77
18740-60840....27
18740-80190....27
18740-80200....26
18740-80220....26
18789-60060....105
18789-80070....81
18900-20250....42
18900-20280....42
18900-20281....42
18900-20300....42
18900-60640....108
18900-80255....42
19091-20050....399
19091-21050....399
19091-60010....387
19091-60010E....387
19091-60312....273
19091-60620E....397
19091A-002....279
19091A-002LTM....279
19091A-005....279
19091A-008....279
19091A-008LTM....279
19091A-012....279
19091A-012LTM....279
19091A-015....279
19091A-101....279
19091A-101LTM....279
19091A-102....279
19091A-102E....279
19091A-102LTM....279
19091A-105....279
19091A-108....279
19091A-108LTM....279
19091A-112....279

19091A-112LTM....279
19091A-115....279
19091B-002....280
19091B-002LTM....280
19091B-005....280
19091B-012....280
19091B-012E....280
19091B-012LTM....280
19091B-015....280
19091B-101....280
19091B-101LTM....280
19091B-102....280
19091B-102E....280
19091B-102LTM....280
19091B-105....280
19091B-105E....280
19091B-112....280
19091B-112LTM....280
19091B-115....280
19091B-115E....280
19091F-102....311
19091F-102E....311
19091F-102LTM....311
19091F-105....311
19091F-105E....311
19091F-112....311
19091F-112E....311
19091F-112LTM....311
19091F-115....311
19091F-115E....311
19091F-413....311
19091F-413LTM....311
19091F-433....311
19091F-433E....311
19091F-433LTM....311
19091G-113....290
19091G-113LTM....290
19091G-131....290
19091G-131E....290
19091G-131LTM....290
19091G-133....290
19091G-133LTM....290
19091G-213....290
19091G-213LTM....290
19091G-B113....359
19091G-B133....359
19091G-B213....359
19091G-B213E....359
19091G-B233....359
19091G-B233E....359
19091J-002....284
19091J-002LTM....284
19091J-005....284
19091J-012....285
19091J-012E....285
19091J-012LTM....285
19091J-015....285
19091J-015E....285
19091J-101....284
19091J-101LTM....284
19091J-102....284
19091J-102E....284
19091J-102LTM....284
19091J-105....284
19091J-105E....284
19091J-108....284
19091J-112....285
19091J-112E....285
19091J-112LTM....285
19091J-113....285
19091J-113E....285
19091J-113LTM....285
19091J-115....285
19091J-115E....285
19091J-202....284
19091J-202LTM....284
19091J-205....284
19091J-212....285
19091J-212LTM....285
19091J-213....285
19091J-213E....285
19091J-213LTM....285
19091J-215....285
19091J-215E....285
19091J-216....285
19091J-216E....285
19091J-231....284
19091J-231LTM....284
19091J-233....220, 284
19091J-233LTM....284
19091J-236....284
19091J-236E....284
19091J-313....285
19091J-313LTM....285
19091J-330....284
19091J-330LTM....284
19091J-333....284
19091J-333LTM....284
19091J-411....285
19091J-411LTM....285
19091J-413....285
19091J-413E....285
19091J-413LTM....285
19091J-416....285
19091J-431....284
19091J-431E....284
19091J-431LTM....284
19091J-433....284
19091J-433E....284
19091J-433LTM....284
19091J-436....284
19091J-436E....284
19091J-577....284
19091J-577E....284
19091J-577LTM....284
19091L-101....292
19091L-101LTM....292
19091L-111....292
19091L-111LTM....292
19091L-113....292
19091L-113E....292
19091L-113LTM....292
19091L-133....292
19091L-133LTM....292
19091L-330....292
19091L-330LTM....292
19091L-333....292
19091L-333LTM....292
19091L-413....292
19091L-413E....292
19091L-413LTM....292
19091L-416....292
19091L-431....292
19091L-431LTM....292
19091L-433....292
19091L-433LTM....292
19091L-577....292
19091L-577LTM....292
19091N-013....307
19091N-013LTM....307
19091N-030....307
19091N-030LTM....307
19091N-033....307
19091N-033LTM....307
19091N-036....307
19091N-102....307
19091N-102LTM....307
19091N-105....307
19091N-105E....307
19091N-111....307
19091N-111LTM....307
19091N-113....233, 307
19091N-113E....307
19091N-113LTM....307
19091N-116....229, 236, 307
19091N-130....307
19091N-130LTM....307
19091N-131....307
19091N-131E....307
19091N-131LTM....307
19091N-133....307
19091N-133E....307
19091N-133LTM....307
19091N-136....229, 307
19091N-136E....307
19091N-202....307
19091N-202LTM....307
19091N-205....307
19091N-205E....307
19091N-213....307
19091N-213E....307
19091N-213LTM....307
19091N-216....232-233, 307
19091N-216E....307
19091N-231....221, 307
19091N-231LTM....307
19091N-233....227, 307
19091N-233E....307
19091N-233LTM....307
19091N-236....307
19091N-330....307
19091N-331....307
19091N-577....307
19091N-577E....307
19091N-577LTM....307
19091P-K15....374
19091P-K15E....374
19091P-K33....374
19091P-K33E....374
19091P-K33LTM....374
19091P-M15....380
19091P-M15E....380
19091P-MS4....384
19091P-MS4E....384
19091P-MS4LTM....384
19091P-MS7....384
19091P-MS7LTM....384
19091P-MS8....384
19091P-MS8LTM....384
19091P-QO3....371
19091P-QO3LTM....371
19091P-QO4....371
19091P-QO4E....371
19091P-QO4LTM....371
19091P-S12....378
19091P-S12LTM....378
19091P-S15....378
19091P-S15E....378
19091P-S33....378
19091P-S33LTM....378
19091P-UO4....374
19091P-UO4E....374
19091P-UO4LTM....374
19091R-303....348
19091R-303LTM....348
19091R-306....215, 219, 225, 348
19091R-316....348
19091R-319....348
19091S-001....233-234, 319
19091S-001E....319
19091S-010....337
19091S-010LTM....337
19091S-101....251
19091S-101LTM....251
19091S-102....251
19091S-102E....251
19091S-102LTM....251
19091S-105....251
19091S-112....251
19091S-112E....251
19091S-112LTM....251
19091S-113....218, 223-224, 251
19091S-113LTM....251
19091S-133....215, 218, 222-223, 226-227, 251
19091S-133LTM....251
19091S-133UI....219, 224, 241
19091S-133UILTM....241
19091S-139....342
19091S-139LTM....342
19091S-213....227, 233, 251
19091S-213LTM....251
19091S-213UI....241
19091S-213UILTM....241
19091S-231....251
19091S-231LTM....251
19091S-233....251
19091S-233E....251
19091S-233LTM....251
19091S-233UI....214, 241
19091S-233UIE....241
19091S-233UILTM....241
19091S-313....251
19091S-313LTM....251
19091S-331....251
19091S-331LTM....251
19091S-333....251
19091S-333LTM....251
19091S-336....251
19091S-413....236, 251
19091S-413E....251
19091S-413LTM....251
19091S-413UI....225, 241
19091S-413UILTM....241
19091S-416....251
19091S-431....251
19091S-431LTM....251
19091S-431UI....215, 241
19091S-431UILTM....241
19091S-433....215, 234-235, 251
19091S-433E....251
19091S-433LTM....251
19091S-433UI....214, 216, 219, 241
19091S-433UIE....241
19091S-433UILTM....241
19091S-436....251
19091S-436E....251
19091S-436UI....241
19091S-510....363
19091S-510E....363

19091S-510LTM....363
19091S-577....251
19091S-577LTM....251
19091S-577UI....214, 241
19091S-577UILTM....241
19091S-602....246
19091S-602E....246
19091S-602LTM....246
19091S-612....246
19091S-612LTM....246
19091S-612UI....240
19091S-633....246
19091S-633LTM....246
19091S-633UI....240
19091S-677....246
19091S-677E....246
19091S-677LTM....246
19091S-677UI....240
19091S-677UIE....240
19091S-713....231, 234, 246
19091S-713LTM....246
19091S-713UI....240
19091S-733....246
19091S-733E....246
19091S-733LTM....246
19091S-733UI....240
19091S-733UIE....240
19091S-833....246
19091S-833LTM....246
19091S-911....246
19091S-911LTM....246
19091S-911UI....240
19091S-913....246
19091S-913E....246
19091S-913LTM....246
19091S-913UI....240
19091S-913UIE....240
19091S-916....246
19091S-931....246
19091S-931E....246
19091S-931LTM....246
19091S-931UI....240
19091S-931UIE....240
19091S-933....246
19091S-933E....246
19091S-933LTM....246
19091S-933UI....240
19091S-933UIE....240
19091S-936....246
19091S-936E....246
19091W-012....313
19091W-012E....313
19091W-012LTM....313
19091W-015....313
19091W-015E....313
19091W-102....313
19091W-102LTM....313
19091W-105....313
19091Y-012....387
19091Y-012E....387
19091Y-012LTM....387
19091Y-015....387
19091Y-101....387
19091Y-102....387
19091Y-102LTM....387
19091Y-105....387
19091Z-002....273
19091Z-002LTM....273
19091Z-005....273
19091Z-008....273
19091Z-008LTM....273
19091Z-012....274
19091Z-012E....274
19091Z-012LTM....274
19091Z-015....274
19091Z-102....273
19091Z-102E....273
19091Z-102LTM....273
19091Z-105....273
19091Z-112....274
19091Z-112E....274
19091Z-112LTM....274
19091Z-115....232, 236, 274
19091Z-115E....274
19091Z-202....273
19091Z-202LTM....273
19091Z-205....273, 319
19091Z-205E....319
19091Z-211....274
19091Z-211LTM....274
19091Z-212....274
19091Z-212LTM....274
19091Z-213....274
19091Z-213E....274
19091Z-213LTM....274
19091Z-215....274
19091Z-216....274
19091Z-216E....274
19091Z-231....273
19091Z-231LTM....273
19091Z-233....273
19091Z-233E....273
19091Z-233LTM....273
19091Z-236....235-236, 273
19091Z-236E....273
19091Z-313....274
19091Z-313E....274
19091Z-313LTM....274
19091Z-331....273
19091Z-331LTM....273
19091Z-333....273
19091Z-333LTM....273
19091Z-411....274
19091Z-411E....274
19091Z-411LTM....274
19091Z-413....274
19091Z-413E....274
19091Z-413LTM....274
19091Z-416....274
19091Z-431....273
19091Z-431LTM....273
19091Z-433....273
19091Z-433E....273
19091Z-433LTM....273
19091Z-436....273
19091Z-513....274
19091Z-513E....274
19091Z-513LTM....274
19091Z-530....234, 273, 319
19091Z-530E....273, 319
19091Z-577....273
19091Z-577E....273
19091Z-577LTM....273
19091Z-613....235, 274
19091Z-613LTM....274
19091Z-713....274
19091Z-713E....274
19091Z-713LTM....274
19091Z-716....274
19095F-120....311
19095F-120E....311
19095F-120LTM....311
19095F-121....311
19095F-121LTM....311
19095F-123....311
19095F-123E....311
19095F-123LTM....311
19095J-023....285
19095J-023E....285
19095J-023LTM....285
19095J-121....285
19095J-121E....285
19095J-121LTM....285
19095J-123....285
19095J-123E....285
19095J-123LTM....285
19095J-321....223, 285
19095J-321LTM....285
19095J-323....285
19095J-323E....285
19095J-323LTM....285
19095J-621....285
19095J-621LTM....285
19095J-623....236, 285
19095J-623E....285
19095J-623LTM....285
19095L-021....292
19095L-021LTM....292
19095L-023....292
19095L-023E....292
19095L-023LTM....292
19095L-121....387
19095L-121LTM....387
19095L-523....292
19095L-523E....292
19095L-523LTM....292
19095N-121....307
19095N-121E....307
19095N-121LTM....307
19095N-123....307
19095N-123E....307
19095N-123LTM....307
19095N-126....307
19095P-K23....229, 374
19095P-K23LTM....374
19095P-K25....236, 374
19095P-K25E....374
19095P-M23....380
19095P-M23LTM....380
19095P-M25....380
19095P-MS0....229, 384
19095P-MS0E....384
19095P-MS0LTM....384
19095P-MS5....384
19095P-MS5LTM....384
19095P-MS6....384
19095P-MS6E....384
19095P-MS6LTM....384
19095P-MS9....229, 384
19095P-MS9LTM....384
19095P-QO3....229, 233, 235, 371
19095P-QO3E....371
19095P-QO3LTM....371
19095P-QO4....234-235, 371
19095P-QO4E....371
19095P-QO4LTM....371
19095P-S21....378
19095P-S21LTM....378
19095P-S23....229, 378
19095P-S23LTM....378
19095P-S25....232, 378
19095P-S25E....378
19095P-UO3....374
19095P-UO3LTM....374
19095P-UO4....235, 374
19095P-UO4E....374
19095P-UO4LTM....374
19095R-420....348
19095R-429....348
19095S-100....274
19095S-100E....274
19095S-100LTM....274
19095S-200....321
19095S-205....321
19095V-420....364
19095V-420E....364
19095V-420LTM....364
19095W-121....313
19095W-121LTM....313
19095W-123....313
19095W-123LTM....313
19095Z-020....230, 274
19095Z-021....230, 274
19095Z-021E....274
19095Z-021LTM....274
19095Z-023....274
19095Z-023E....274
19095Z-023LTM....274
19095Z-121....274
19095Z-121E....274
19095Z-121LTM....274
19095Z-123....274
19095Z-123E....274
19095Z-123LTM....274
19095Z-220....274
19095Z-221....274
19095Z-221E....274
19095Z-321....274
19095Z-321LTM....274
19095Z-323....274
19095Z-323E....274
19095Z-323LTM....274
19095Z-421....274
19095Z-421LTM....274
19095Z-423....274
19095Z-423E....274
19095Z-423LTM....274
19095Z-621....233, 274
19095Z-621LTM....274
19095Z-623....274
19095Z-623E....274
19095Z-623LTM....274
19095Z-626....236, 274
19095Z-627....234, 274
19095Z-627E....274
19095Z-627LTM....274
1909BD-113....329
19231-20910....84
19231-20940....84
19231-20990....84
19231-21050....84
19231-21060....84
19231-60680....84-85
19231-80520....84-85, 105
19231-80530....84-85, 105
19233-20625....88
19233-20755....88
19234-60700....76
19234-60715....76
19234-60720....77, 84, 88, 105

19243-000681 64
19243-00070 63
19243-80530 77
19243-80540 77
19243-80570 76-77
19244-80540 76-77
19244-80560 ..... 81, 85, 104-105
19244-80610 ..... 84-85, 105
19244-80620 ..... 81, 104
19251-00100 63
19251-60540 ..... 25, 63
19251-60575 62
19256-00090 100
19256-00200 100
19256-00320 100
19256-20550 99
19256-20580 99
19256-20590 99
19256-20690 99
19256-20705 99
19256-20900 100
19256-20910 100
19256-60510 100
19256-60700 99
19256-60800 99
19256-80000 100
19256-80010 100
19256-80030 99
19256-80045 99
19256-80560 99
19256-80600 99
19258-20830 49
19258-20870 49
19298-60500 108
19301-00150 85
19301-20720 85
19301-60660 85
19325-60660 41
19354-60510 108
200-0010 411
200-0032 411
200-0070 411
200-0110 411
200-0113 411
200-0185 411
200-0310 411
200-0370 411
200187500 166
200187600 168
200193800 ..... 166, 168
210-3003 26
210-3003-5 26
210-4004-5 25
210-4022-5 25
2100003100 168
2100003200 ..... 166, 168
2190-0584 99
221-0122LTM 245, 395
221-1324LTM 345, 396
221-1524LTM 347, 396
221-3822LTM 256, 396
221-4722LTM 258, 396
221-5522LTM 250, 395
221-5522UILTM 395
221-6822LTM 336, 396
222-0112LTM 245, 395
222-0132LTM 245, 395
222-0732LTM 396
222-1032LTM 395
222-1111LTM 314, 395
222-1131LTM 314, 395
222-1334LTM 345, 396
222-1534LTM 347, 396
222-2912LTM 262, 396
222-2932LTM 262, 396
222-3212LTM 310, 396
222-3232LTM 310, 396
222-3812LTM 256, 396
222-3832LTM 256, 396
222-4712LTM 258, 396
222-4732LTM 258, 396
222-5512LTM 250, 395
222-5512UILTM 395
222-5532LTM 250, 395
222-5532UILTM 395
222-5711LTM 315, 395
222-5731LTM 315, 395
222-7013LTM 304, 396
222-7033LTM 305, 396
2302533140 48
2307230001 48
2307232901 48
232-2790010-EHS 49
232-2790012-EHS 49
2321700003 48-49
2321700004 48-49
2322590004 48-49
2322590005 48-49
2322700011 48
2710100200 135
2710100400 135
2710100500 135
2722990700 136
2735000500 135
2740236100 168
2740292400 167
2740928202 168
29091N-133LTM 307, 396
29091N-577LTM 307, 396
29091R-303LTM 348, 396
29091S-431UILTM 395
29091S-433LTM 246, 251, 396
29091S-433UILTM 395
29091S-577UILTM 395
29091S-677LTM 246, 395
29091S-833LTM 246, 395
29091S-931LTM 246, 395
2950-0232 41
301-011-HSP 49
301-015-HSP 49
301-016-HSP 49
301-017-HSP 49
301-152-HSP 49
301-169-HSP 49
301-170-HSP 49
301-205-HSP 49, 62
301-211-HSP 49
301-212-HSP 49
3150-0602 71
3162-1057 132
321-002-HSP 49
321-055-HSP 49
321-056-HSP 49
321-057-HSP 49
325-062-HSP 49
325-132-HSP 49
325-185-HSP 49
3600500001 49
3600500002 49
390607400 168
390607401 168
390607900 168
390812700 164-165
390820601 161-165
390842300 161-165
391821100 163
391866306 163
391866308 161
391867600 162
392017401 134
392027300 135-136
392027500 136
392030500 135-136
392035300 135-136
392043700 136
392047100 136
392511901 167-168
392512800 168
392513800 167
392514300 167-168
392514500 167-168
392515101 167
392515102 167
392515103 167
392515104 167
392515105 167
392515500 167-168
392517100 167
392517600 167
392517700 167
392517800 167
392517901 167
392519200 167
392543101 165
392544001 162
392544011 162
392544391 167
392548201 165
392548301 164
392560591 166
392561290 166
392567111 134
392585291 166
392585292 166
392595501 164-165
392597101 161
392597301 161
392597302 161
392597303 161
392597501 161
392599401 161
392599411 161
392599501 161
392609901 21
392609902 21
392609903 21
393001991 136
393010918 134
393010920 134
393010924 134
393011391 136
393031501 136
393050292 136
393050293 136
393050392 136
393050393 136
393050492 136
393050493 136
393053501 136
393053502 ..... 134, 136
393060191 136
393065201 138
393082491 134
393101291 134
393112601 135
393112702 135
393113001 135
393161001 134
393164493 134
393167593 134
393171201 134
393175101 134
393847701 135
394958700 166
394966601 162-163
4177-0607 46
500-1200 38
500-2114 33
500-2118 33
5020-8292 34
5020-8293 34
5020-8294 34
5021-7133 39
5021-7134 39
5021-7136 39
5021-7137 39
5021-7146 39
5021-7148 39
5021-7164 39
5021-7166 39
5021-7168 39
5021-7169 39
5021-7170 39
5040-4669 47
5060-9086 108
5061-5869 63
5061-5886 100
5061-5890 100
5061-5896 ..... 116, 133
5062-0208 47
5062-3506 ..... 33, 117
5062-3507 33
5062-3508 ..... 33, 117
5062-3511 33
5062-3512 33
5062-3513 33
5062-3514 33
5062-3515 33
5062-3516 33
5062-3525 ..... 39, 71-72
5062-3538 33
5062-3587 ..... 26, 63
5062-9508 40
5062-9509 40
5062-9510 40
5062-9511 40
5080-4978 85
5080-5400 ..... 116, 133
5080-8716 108
5080-8728-100 19
5080-8728-50 19
5080-8732 76-77
5080-8750 77
5080-8751 77
5080-8755 108
5080-8756 108
5080-8759 108
5080-8761 108
5080-8768 108
5080-8769 108

5080-8773 ..... 91, 105
5080-8774 ..... 76-77, 88, 91, 99, 105
5080-8853 ..... 33, 91, 105
5080-8858 411
5080-8894-100 19
5080-8896-50 19
5080-8898 76-77
5180-4103 91-92
5180-4105 ..... 76-77, 88, 91, 105
5180-4150 85
5180-4152 85
5180-4153 ..... 63, 85
5180-4165 82
5180-4168 ..... 29, 62
5180-4173 ..... 29, 62
5180-4181 84
5180-8830 76
5181-1260 19
5181-1261 19
5181-1291 41
5181-1292 41
5181-3308 33
5181-3311 84
5181-3315 26
5181-3316 ..... 26, 62
5181-3316i 26
5181-3322 33
5181-3323 ..... 33, 117
5181-3351 386
5181-3352 386
5181-3382 77
5181-3395 38
5181-3396 38
5181-3397 38
5181-3398 38
5181-7459 40
5181-7460 40
5181-8815 20
5181-8816 20
5181-8818 ..... 26, 63
5181-8830 ..... 34, 63, 77, 91, 105, 117
5181-8833 20
5181-8836 46
5181-8838 63
5181-8839 20
5181-8863 116
5181-8866 68
5182-0551 43
5182-0739 76
5182-0773 51
5182-0774 51
5182-0775 51
5182-0781 51
5182-0783 51
5182-0794 50
5182-0795 50
5182-0796 50
5182-0831 68
5182-0832 68
5182-0833 68
5182-0836 68
5182-0837 47
5182-0838 47
5182-0840 47
5182-0844 50
5182-0845 50
5182-0846 50
5182-0847 50
5182-0848 50
5182-0849 50
5182-0850 50
5182-0851 50
5182-0852 50
5182-0853 20
5182-3438 21
5182-3439 21
5182-3442 20
5182-3444 ..... 20, 64, 71, 77
5182-3445 ..... 20, 64, 71, 76-77
5182-3450 85
5182-3466 117
5182-3477 92
5182-8815 76
5182-9651 73
5182-9652 ..... 56, 63
5182-9673 92
5182-9676 92
5182-9677 92
5182-9679 92
5182-9722 105
5182-9733 48-49
5182-9747 71
5182-9748 71-72
5182-9749 71
5182-9754 71
5182-9756 71
5182-9757 71-72
5182-9758 71-72
5182-9759 71-72
5182-9760 71-72
5182-9761 71
5182-9762 71
5182-9763 71-72
5182-9768 71
5182-9769 71
5182-9770 71
5182-9775 71-72
5183-0318 73
5183-0379 88
5183-2007 ..... 101, 105
5183-2036 ..... 28, 73
5183-2037 ..... 28, 73
5183-2038 ..... 28, 73
5183-2058 73
5183-2096 116
5183-4477 47
5183-4647 ..... 24-26, 62
5183-4691 25
5183-4692 25
5183-4693 26
5183-4694 26
5183-4695 26
5183-4696 ..... 26, 62
5183-4697 27
5183-4698 27
5183-4699 27
5183-4700 27
5183-4701 24-28
5183-4702 ..... 24-28, 62
5183-4703 26
5183-4704 26
5183-4705 26
5183-4706 26
5183-4707 26
5183-4708 26
5183-4709 26
5183-4710 26
5183-4711 25
5183-4712 25
5183-4713 25
5183-4732 ..... 34, 63, 91
5183-4741 52
5183-4757 ..... 16, 62-64, 77
5183-4757-100 16
5183-4758 16
5183-4759 17
5183-4759-100 17
5183-4760 17
5183-4761 17
5183-4761-100 17
5183-4762 17
5184-3569 117
5184-3570 117
5184-3571 ..... 117, 124
5188-1447 51
5188-1448 51
5188-2717 ..... 57, 63
5188-5241 63
5188-5245 99
5188-5311 29
5188-5312 34
5188-5313 ..... 28, 73
5188-5315 35
5188-5316 108
5188-5317 108
5188-5347 138
5188-5348 138
5188-5356 ..... 28, 73
5188-5357 138
5188-5361 ..... 35, 37, 41, 124
5188-5362 ..... 35, 37, 41, 124
5188-5363 ..... 35, 37, 41, 124
5188-5365 ..... 29, 62-64
5188-5366 ..... 29, 57, 62
5188-5367 ..... 56, 63
5188-5372 85
5188-5379 411
5188-5953 99
5188-6471 27
5188-6493 ..... 55, 62
5188-6494 ..... 55, 62
5188-6495 ..... 55, 63
5188-6496 ..... 55, 62
5188-6497 ..... 55, 62
5188-6498 ..... 55, 77
5188-8813 51
5188-8814 51
5188-8815 51
5188-8816 51
5188-8817 51
5188-8818 51
5188-8819 51
5188-8820 51
5188-8821 51
5188-8822 51
5190-0468 137
5190-0471 137
5190-0472 137
5190-0473 137
5190-0490 137
5190-0493 137
5190-0494 137
5190-1407 329
5190-1408 329
5190-1409 329
5190-1410 329
5190-1426 ..... 28, 73
5190-1437 46
5190-1438 46
5190-1441 137
5190-1445 51
5190-1446 51
5190-2209 ..... 14, 56
5190-2231 51
5190-2232 51
5190-2233 51
5190-2234 51
5190-2235 51
5190-2265 48
5190-2266 48
5190-2268 ..... 14, 29, 57
5190-2269 ..... 14, 29
5190-2270 ..... 14, 26
5190-2271 ..... 14, 26
5190-2272 ..... 14, 26
5190-2275 ..... 14, 25
5190-2292 24
5190-2293 24
5190-2294 24
5190-2295 ..... 24, 62
5190-2296 ..... 27, 64
5190-2297 ..... 24, 27
5190-3157 ..... 14, 16
5190-3158 ..... 14, 17
5190-3162 24
5190-3163 24
5190-3164 24
5190-3165 24
5190-3166 ..... 24, 62
5190-3167 24
5190-3168 24
5190-3169 ..... 24, 62
5190-3170 ..... 14, 24
5190-3171 ..... 14, 24
5190-3172 ..... 14, 24
5190-3173 ..... 14, 24
5190-3976 52
5190-3978 52
5190-3983 24
5190-4006 ..... 24, 27
5190-4007 24
5190-4022 14
5190-4023 14
5190-4024 14
5190-4047 ..... 24, 27
5190-4048 ..... 24, 27
5190-4054 33
5958-9441 44
5958-9442 44
5958-9443 44
5958-9444 44
5958-9445 44
5958-9450 44
5982-0024 137
5982-0025 137
6040-0289 ..... 131, 133
6040-0621 132
6040-0809 131-132
6040-0834 131
621-9723 ..... 242, 340
622-9732 ..... 242, 340
6410090050 48
705-0825 38
705-0903 38
705-0905 38
705-0925 38
7200008400 161-165
8001-0004 180
8001-0005 180
8001-0006 180
8001-0007 180

8001-0010 180
8001-0011 180
8001-0012 180
8001-0013 180
8001-0014 180
8001-0101 175-177
8001-0102 175, 177
8001-0103 175-177
8001-0104 176
8001-0105 178
8001-0106 175-176
8001-0151 175-177
8001-0152 175, 177
8001-0153 175-177
8001-0154 176
8001-0155 178
8001-0156 175-176
8001-0157 175-177
8001-0158 175-177
8001-0159 175-177
8001-0160 175-177
8001-0162 176
8001-0163 176
8001-0201 178
8001-0202 178
8001-0203 178
8001-0211 179
8001-0212 179
8001-0213 179
8001-0214 179
8001-0221 179
8001-0222 179
8001-0223 179
8001-0224 179
8001-0311 180
8001-0312 180
8002-0001 184
8002-0002 184
8002-0003 184, 187
8002-0004 184, 187
8002-0005 184, 187
8002-0101 182
8002-0102 182
8002-0103 182
8002-0104 182
8002-0105 182
8002-0106 182
8002-0107 182
8002-0151 182
8002-0152 182
8002-0153 182
8002-0154 182
8002-0155 182
8002-0156 182
8002-0157 182
8002-0159 182
8002-0160 182
8002-0161 182
8002-0201 183
8002-0203 183
8002-0204 183
8002-0211 183
8002-0212 183
8002-0213 183
8002-0214 183
8002-0215 183
8002-0216 183
8002-0217 183
8002-0220 183
8002-0221 183
8002-0222 183
8002-0311 184
8002-0312 184
8003-0001 173
8003-0002 173
8003-0003 173
8003-0004 173
8003-0005 173
8003-0006 173
8003-0007 173
8003-0008 173
8003-0101 169
8003-0102 169
8003-0103 169
8003-0104 170
8003-0105 169
8003-0106 169
8003-0107 169
8003-0108 170
8003-0109 170
8003-0110 169
8003-0111 169
8003-0151 169
8003-0152 169
8003-0153 169
8003-0154 170
8003-0155 170
8003-0157 169
8003-0158 169
8003-0159 169
8003-0160 169
8003-0162 169
8003-0163 170
8003-0165 169
8003-0166 169
8003-0202 170
8003-0203 170
8003-0204 170
8003-0205 170
8003-0211 172
8003-0212 172
8003-0216 171
8003-0219 172
8003-0221 172
8003-0222 172
8003-0223 172
8003-0311 172
8004-0001 158
8004-0002 158
8004-0003 158
8004-0004 158
8004-0005 158
8004-0006 158
8004-0007 158
8004-0101 154
8004-0102 154
8004-0103 154
8004-0104 154
8004-0105 154
8004-0106 154
8004-0107 154
8004-0108 155
8004-0109 155
8004-0110 155
8004-0111 156
8004-0112 155
8004-0113 154
8004-0114 154
8004-0116 154
8004-0118 155
8004-0119 154
8004-0151 154
8004-0152 154
8004-0153 154
8004-0154 154
8004-0155 154
8004-0156 154
8004-0157 154
8004-0158 154
8004-0159 155
8004-0160 155
8004-0161 155
8004-0162 155, 163
8004-0163 156
8004-0164 155, 162
8004-0165 154, 161
8004-0167 155, 163
8004-0168 156, 164
8004-0170 154
8004-0171 155
8004-0173 154
8004-0176 155
8004-0178 154
8004-0201 156, 159, 161, 174, 181, 185
8004-0202 156, 161
8004-0203 156
8004-0204 156, 162
8004-0211 157
8004-0212 157
8004-0213 157
8004-0214 157
8004-0215 157
8004-0216 157
8004-0217 158, 163-165
8004-0218 157
8004-0219 157
8004-0311 158, 161-165
8004-0312 158, 163
8010-0201 151, 159, 161, 185
8010-0202 151, 159, 185
8010-0203 151, 159, 164-165, 185
8010-0204 151, 159, 185
8010-0205 151, 159, 185
8010-0206 151, 159, 185
8010-0207 151, 159, 174, 185
8010-0208 151, 159, 174, 185
8010-0209 151, 159, 162-163, 185
8010-0210 151, 159, 185
8010-0211 151, 185-186
8010-0212 151, 185-186
8010-0213 151, 185
8010-0214 151, 185
8010-0215 151, 181
8010-0216 151, 181
8010-0217 150, 159-161, 185
8010-0218 150-153, 159, 174, 181, 185-186
8010-0219 150, 159, 164-165, 185
8010-0220 150, 159, 185
8010-0221 150, 159, 185
8010-0222 150, 159, 185
8010-0223 150, 159, 174, 185
8010-0224 150, 159, 174, 185
8010-0225 150, 159, 162-163, 185
8010-0226 150, 159, 185
8010-0227 150, 185
8010-0228 150, 185
8010-0229 150, 185
8010-0230 150, 185
8010-0231 150, 181
8010-0232 150, 181
8010-0233 152, 160-161, 186
8010-0234 152, 160, 186
8010-0239 152, 160, 174, 186
8010-0240 152, 160, 174, 186
8010-0241 152, 160, 162-163, 186
8010-0242 152, 160, 186
8010-0243 152, 186
8010-0244 152, 186
8010-0245 152, 186
8010-0246 152, 186
8010-0249 153, 160, 186
8010-0250 153, 160, 186
8010-0251 153, 160, 186
8010-0252 153, 160, 186
8010-0253 153, 160, 186
8010-0254 153, 160, 186
8010-0255 153, 160, 174, 186
8010-0256 153, 160, 174, 186
8010-0257 153, 160, 186
8010-0258 153, 160, 186
8010-0259 153, 186
8010-0260 153, 186
8010-0261 153, 186
8010-0262 153, 186
8010-0263 153, 181
8010-0264 153, 181
8010-0301 157, 171
8010-0302 157, 171
8010-0303 157, 171
8010-0304 157, 171
8010-0305 158, 163-165, 172
8010-0306 157, 171
8010-0307 157, 171
8010-0308 157, 171
8010-0309 157, 171
8010-0310 171, 179, 183
8010-0311 171, 179, 183
8010-0312 171, 179
8010-0313 171, 179
8010-0314 172, 179
8010-0315 172, 179
8010-0351 158, 184, 187
8010-0352 184, 187
8010-0353 184, 187
8010-0354 184, 187
8010-0355 184, 187
8010-0356 187
8010-0357 187
8010-0358 187
8010-0359 187
8010-0360 187
8010-0361 187
8010-0362 187
8010-0363 187
8010-0364 187
8010-0365 187
8010-0366 187
8010-0367 184, 187
8010-0368 184
8010-0401 170, 183
8500-0656 116, 138
8500-1233 116
8500-4789 63
8500-5440 138
8500-5808 138
8500-5851 138
8500-5995 138
8500-6812 411

8500-6813....411
8500-8510....138
8650-0029....116, 133
8650-0030....116, 133
8660-0791....116, 133
8710-0510....34, 117
8710-0899....117
8710-0900....117
8710-1220....117
8710-1346....85
8710-1561....85
8710-1615....117
8710-1622....117
8829951700....135
8829953800....135
9300003590....134
9301-0713....21, 73
9301-0723....43
9301-0892....21, 73
9301-0985....85
9301-1031....43
9310-4828....116, 133
998-0000053-EHS....49
C-102SSC....54
C-AT010C....54
C-B010M....53
C-BIO10....53
C-BTX1UG....54
C-CF020....53
C-CPLOK....53
C-DF010....53
C-G1CM10....54
C-GAT010C....54
C-GT010....53
C-HY010C....54
C-PL010....53
C-TBE10....53
C-TBP1C1C....54
C-TBP1CXC....54
C-TBP1TC....53
C-TNXTA....53
C-UN010C....54
CP0005....412
CP0031....412
CP1305....408
CP1306....409
CP1307....408
CP1308....408
CP1309....409
CP1480....408
CP1481....409
CP1482....408
CP1483....409
CP17973....132
CP17974....132
CP2045....409
CP2046....409
CP2047....408
CP2050....409
CP2055....408
CP2056....409
CP2057....408
CP2058....408
CP2059....409
CP2060....409
CP2062....408
CP2065....409
CP2068....408
CP2071....409
CP2072....409
CP2073....409
CP4016....386
CP4017....386
CP4018....386
CP4788....386
CP4789....386
CP4795....386
CP4796....386
CP5850....230
CP5881....247
CP5882....259
CP5883....259
CP5884....259
CP5885....260
CP5886....260
CP5887....257
CP5888....257
CP5889....257
CP5891....261
CP5892....261
CP5893....261
CP6172....353
CP6172I5....353
CP6173....353
CP6173I5....353
CP6174....353
CP6174I5....353
CP6175....353
CP6530....330
CP6540....324, 365-366
CP6550....324, 365-366
CP6560....324
CP6666....278, 366
CP6666I5....278, 366
CP6670....278, 366
CP6671....278, 366
CP6680....287, 367
CP6681....367
CP67569....366
CP6918....367, 376
CP6937....367, 385
CP6937I5....367, 385
CP6938....367, 385
CP6938I5....367, 385
CP6953....367, 370
CP6953I5....367, 370
CP6954....367, 370
CP6954I5....367, 370
CP6955....367, 370
CP6968....367, 377
CP7120....278, 366
CP7121....367
CP7125....366
CP7128....309
CP7129....367
CP7130....366
CP7135....278, 366
CP7135I5....278, 366
CP7138....309, 367
CP7140....278, 366
CP7141....367
CP7148....309, 367
CP7150....278, 366
CP7158....309, 367
CP7160....278, 366
CP7168....309, 367
CP7170....278, 366
CP7177....309, 367
CP7178....309, 367
CP7179....309, 367
CP7195....278, 366
CP7196....287, 367
CP7198....309, 367
CP7300....275
CP7310....275
CP7310I5....275
CP7311....275
CP7312....275
CP7313....275
CP7319....286
CP7319I5....286
CP7331....302
CP7334....308
CP7334I5....308
CP7335....308
CP7340....302
CP7347....368-369
CP7347I5....368
CP7348....368
CP7348I5....368
CP7350....231, 368
CP7350I5....368
CP7351....232-233, 368
CP7351I5....368
CP7352....368
CP7352I5....368
CP7353....231, 368
CP7353I5....368
CP7354....221, 232-233, 368
CP7354I5....368
CP7355....368
CP7360....302
CP7371....382
CP7372....382
CP7374....229, 382
CP7375....382
CP7406....336
CP7407....336
CP7407I5....336
CP7408....336
CP7409....336
CP7411....346
CP7411I5....346
CP7412....346
CP7413....346
CP7413I5....346
CP7414....230, 346
CP7414I5....346
CP7415....346
CP7415I5....346
CP7416....346
CP7416I5....346
CP7417....230, 346
CP7418....346
CP7419....354
CP7419I5....354
CP7420....354
CP7420I5....354
CP7421....354
CP7422....332
CP7422I5....332
CP7424....332
CP7428....232
CP7429....327
CP7430....327
CP7431....327
CP7432....327
CP7433....327
CP7434....331
CP7435....331
CP7437....331
CP7440....339, 367
CP7441....276
CP7442....276
CP7443....276
CP7443I5....276
CP7444....276
CP7444I5....276
CP7446....331
CP7447....331
CP7447I5....331
CP7448....331
CP7448I5....331
CP7451....286
CP7451I5....286
CP7452....287
CP7453....286
CP7453I5....286
CP7454....287
CP7461....338
CP7462....338
CP7463....357, 367
CP7475....319
CP7475I5....319
CP7476....342
CP7477....342
CP7478....342
CP7481....335
CP7482....232, 340
CP7483....357
CP7485....358
CP7485I5....358
CP7486....230, 358
CP7486I5....358
CP7487....354
CP7488....229-230, 354
CP7489....354
CP7491....351
CP749103....351
CP749106....351
CP7491I5....351
CP7493....351
CP7494....360
CP7494I5....360
CP7495....360
CP7495I5....360
CP7497....343
CP7498....343
CP7499....343
CP7500....361
CP7500I5....361
CP7501....361
CP7502....360
CP7502I5....360
CP7503....360
CP7503I5....360
CP7504....335
CP7511....376
CP7511I5....376
CP7512....324, 365-366
CP7512I5....324
CP7513....382
CP7514....382
CP7515....230, 376
CP7515I5....376
CP7516....376
CP7517....376
CP7518....229-230, 376
CP7519....376
CP7519I5....376

CP7521....323
CP7522....323
CP7522I5....323
CP7525....231-233, 235, 325
CP7525I5....325
CP7527....356
CP7527I5....356
CP7528....350
CP7529....234, 326
CP7529I5....326
CP7530....320
CP7530I5....320
CP7531....233, 320
CP7531I5....320
CP7532....230, 324, 365-366
CP7532I5....324, 365
CP7533....229, 385
CP7534....385
CP7534I5....385
CP7535....385
CP7535I5....385
CP7536....385
CP7536I5....385
CP7537....229, 385
CP7538....385
CP7538I5....385
CP7539....385
CP7540....385
CP7540I5....385
CP7541....323
CP7542....324, 365-366
CP7542I5....324, 365
CP7543....385
CP7544....385
CP7544I5....385
CP7548....369
CP7549....369
CP7549I5....369
CP7550....369
CP7550I5....369
CP7551....369
CP7551I5....369
CP7552....369
CP7553....369
CP7553I5....369
CP7554....230, 369
CP7554I5....369
CP7555....369
CP7556....370
CP7557....370
CP7557I5....370
CP7558....229, 370
CP7558I5....370
CP7559....370
CP7559I5....370
CP7561....377
CP7562....324, 365-366
CP7565....377
CP7565I5....377
CP7567....232, 377
CP7568....377
CP7569....324, 365-366
CP7569I5....324, 365
CP7570....230, 324, 365-366
CP7571....324, 365-366
CP7572....324, 365-366
CP7574....373
CP7574I5....373
CP7576....376
CP7577....376
CP7577I5....376
CP7579....373
CP7580....373
CP7581....373
CP7582....230, 324, 365-366
CP7582I5....324
CP7583....373
CP7583I5....373
CP7584....373
CP7584I5....373
CP7586....377
CP7587....377
CP7588....218-219, 227, 343
CP7591....332
CP7591I5....332
CP7592....231, 324, 365-366
CP7593....324, 365-366
CP7594....332
CP7595....332
CP7595I5....332
CP7596....217, 332
CP7596I5....332
CP7597....222, 332
CP7597I5....332
CP7598....224, 332
CP7598I5....332
CP7599....332
CP7602....275
CP7604....275
CP7608....277
CP7609....288
CP7614....233, 312
CP7614I5....312
CP7615....236, 356
CP7615I5....356
CP7617....356
CP7617I5....356
CP7619....288
CP7620....277
CP7620I5....277
CP7621....287
CP7622....275
CP7624....312
CP7625....277
CP7628....309
CP7629....288
CP7630....277
CP7631....287
CP7633....275
CP7634....287
CP7635....277
CP7635I5....277
CP7636....287
CP7637....303
CP7638....309
CP7640....277
CP7641....287
CP7642....275
CP7643....275
CP7643I5....275
CP7644....275
CP7644I5....275
CP7645....277
CP7646....287
CP7647....303
CP7648....309
CP7649....288
CP7650....277
CP7653....325
CP7654....221, 312
CP7656....287
CP7657....303
CP7658....309
CP7658I5....309
CP7659....288
CP7664....312
CP7665....312
CP7666....287
CP7667....303
CP7668....309
CP7669....288
CP7670....276
CP7670I5....276
CP7671....286
CP7672....302
CP7673....308
CP7673I5....308
CP7675....277
CP7675I5....277
CP7676....287
CP7678....309
CP7680....276
CP7680I5....276
CP7681....287
CP7681I5....287
CP7682....275
CP7682I5....275
CP7684....275
CP7684I5....275
CP7685....236, 277
CP7685I5....277
CP7686....358
CP7686I5....358
CP7688....277
CP7690....276
CP7690I5....276
CP7691....287
CP7691I5....287
CP7692....275
CP7692I5....275
CP7693....275
CP7694....275
CP7695....277
CP7696....287
CP7697....303
CP7698....309
CP7698I5....309
CP7700....276
CP7702....302
CP7703....308
CP7709....276
CP7710....276
CP7710I5....276
CP7711....286
CP7712....302
CP7713....308
CP7713I5....308
CP7714....325
CP7714I5....325
CP7715....298
CP7715I5....298
CP7717....312
CP7717I5....312
CP7719....276
CP7719I5....276
CP7720....276
CP7721....286
CP7722....302
CP7723....308
CP7723I5....308
CP7724....325
CP7725....298
CP7725I5....298
CP7727....312
CP7730....276
CP7731....287
CP7732....303
CP7733....309
CP7733I5....309
CP7735....298
CP7739....276
CP7740....276
CP7741....287
CP7741I5....287
CP7742....303
CP7743....309
CP7745....298
CP7747....312
CP7747I5....312
CP7749....276
CP7749I5....276
CP7750....276
CP7750I5....276
CP7751....287
CP7751I5....287
CP7752....303
CP7753....309
CP7753I5....309
CP7754....325
CP7754I5....325
CP7757....312
CP7758....276
CP7758I5....276
CP7759....286
CP7760....276
CP7760I5....276
CP7761....287
CP7762....303
CP7763....309
CP7763I5....309
CP7764....325
CP7765....308
CP7767....312
CP7769....286
CP7770....276
CP7770I5....276
CP7771....287
CP7772....303
CP7773....309
CP7773I5....309
CP7774....325
CP7775....308
CP7777....312
CP7778....312
CP7779....287
CP7785....308
CP7787....312
CP7787I5....312
CP7789....287
CP7791....308
CP7791I5....308
CP7792....308
CP7792I5....308
CP7797....312
CP7809....302
CP7813....288
CP7819....302
CP7819I5....302
CP7820....293
CP7821....293

CP7822....293
CP7822I5....293
CP7824....293
CP7825I5....293
CP7829....303
CP7830....293
CP7830I5....293
CP7831....293
CP7831I5....293
CP7832....293
CP7834....293
CP7834I5....293
CP7839....303
CP7870....293
CP7871....293
CP7871I5....293
CP7879....309
CP7884....286
CP7885....286
CP7889....309
CP7894....286
CP7900....286
CP7906....288
CP7907....288
CP7916....288
CP7917....288
CP7921....286
CP7926....288
CP7926I5....288
CP7927....288
CP7936....288
CP7937....288
CP7941....286
CP7945....320
CP7946....288
CP7947....288
CP7950....286
CP7977....288
CP7977I5....288
CP8014....287
CP8014I5....287
CP8015....351
CP8073....309
CP8073I5....309
CP81025....409
CP81069....408
CP81071....409
CP81073....408
CP8120....355
CP8121....337
CP8131....337
CP8132....337
CP8133....337
CP8134....337
CP8430....231, 276
CP8430I5....276
CP8431....287
CP8502....302
CP8510....276
CP8511....286
CP8512....302
CP8512I5....302
CP8513....308
CP8521....286
CP8529....276
CP8530....276
CP8531....287
CP8533....309
CP8540....276
CP8541....287
CP8542....303
CP8542I5....303
CP8543....309
CP8550....276
CP8550I5....276
CP8553....309
CP8560....276
CP8560I5....276
CP8562....302
CP8562I5....302
CP8564....381
CP8565....381
CP8566....381
CP8566I5....381
CP8567....381
CP8567I5....381
CP8568....381
CP8568I5....381
CP8570....381
CP8570I5....381
CP8571....381
CP8574....381
CP8575....326
CP8587....318
CP8587I5....318
CP8592....302
CP8592I5....302
CP8602....300
CP8604....300
CP8605....300
CP8607....300
CP8608....300
CP8610....300
CP8611....300
CP8613....300
CP8662....303
CP8663....303
CP86677....408
CP86678....408
CP8673....277
CP8673I5....277
CP8674....277
CP8674I5....277
CP8675....277
CP8676....277
CP8677....231-232, 277
CP8677I5....277
CP8678....287
CP8685....277
CP8687....231-232, 276
CP8687I5....276
CP8688....276
CP8688I5....276
CP8689....276
CP8690....276
CP8690I5....276
CP8710....276
CP8712....302
CP8712I5....302
CP8713....308
CP8713I5....308
CP8716....287
CP8718....309
CP8722....302
CP8723....308
CP8723I5....308
CP8730....277
CP8730I5....277
CP8735....229-232, 277
CP8735I5....277
CP8736....220, 287
CP8736I5....287
CP8737....303
CP8738....230-231, 236, 309
CP8738I5....309
CP8741....276
CP8741I5....276
CP8742....276
CP8742I5....276
CP8743....276
CP8743I5....276
CP8744....276
CP8744I5....276
CP8745....308
CP8746....308
CP8746I5....308
CP8748....308
CP8750....286
CP8751....227, 286
CP8751I5....286
CP8752....287
CP8752I5....287
CP8753....286
CP8754....287
CP8756....287
CP8756I5....287
CP8760....230, 232, 276
CP8760I5....276
CP8761....287
CP8761I5....287
CP8762....303
CP8763....230-231, 236, 309
CP8763I5....309
CP8770....276
CP8771....286
CP8771I5....286
CP8772....303
CP8772I5....303
CP8773....233, 309
CP8774....277
CP8775....235, 277
CP8775I5....277
CP8780....276
CP8780I5....276
CP8781....286
CP8791....287
CP8796....287
CP8798....231, 309
CP8799....277
CP8800....255
CP8801....255
CP8802....255
CP8803....255
CP8805....255
CP8806....255
CP8806I5....255
CP8807....255
CP8808....255
CP8809....255
CP8810....255
CP8811....255
CP8812....255
CP8813....255
CP8814....255
CP8815....255
CP8816....255
CP8817....255
CP8818....255
CP8819....260
CP8820....260
CP8820I5....260
CP8821....260
CP8821I5....260
CP8822....260
CP8822I5....260
CP8823....260
CP8824....260
CP8824I5....260
CP8825....260
CP8826....260
CP8827....260
CP8828....260
CP8829....260
CP8830....260
CP8831....260
CP8842....303
CP8843....309
CP8843I5....309
CP8852....303
CP8853....309
CP8855....261
CP8855I5....261
CP8856....261
CP8857....261
CP8858....219, 261
CP8859....261
CP8859I5....261
CP8860....218, 261
CP8860I5....261
CP8861....261
CP8862....261
CP8863....261
CP8864....261
CP8865....261
CP8865I5....261
CP8866....223, 261
CP8867....261
CP8868....224, 261
CP8868I5....261
CP8870....276
CP8871....287
CP8871I5....287
CP8872....257
CP8873....257
CP8874....257
CP8875....257
CP8876....257
CP8877....218, 225, 257
CP8877I5....257
CP8878....257
CP8878I5....257
CP8879....222, 257
CP8880....257
CP8881....257
CP8882....257
CP8883....257
CP8883I5....257
CP8884....257
CP8885....257
CP8886....257
CP8887....257
CP8888....224, 257
CP8900....247
CP8901....247
CP8902....247
CP8903....247
CP8904....247
CP8905....247
CP8906....231-232, 235, 248
CP8906I5....248

CP8907....248
CP8907I5....248
CP8908....248
CP8908I5....248
CP8909....248
CP8910....248
CP8911....248
CP8911I5....248
CP8912....248
CP8912I5....248
CP8913....215, 248
CP8913I5....248
CP8914....248
CP8915....248
CP8916....248
CP8916I5....248
CP8917....248
CP8917I5....248
CP8918....248
CP8918I5....248
CP8919....248
CP8920....248
CP8920I5....248
CP8921....248
CP8922....248
CP8923....248
CP8924....213, 220, 248
CP8925....248
CP8926....213, 248
CP8927....248
CP8928....248
CP8929....248
CP8930....248
CP8933....252
CP8934....252
CP8935....252
CP8935I5....252
CP8936....252
CP8936I5....252
CP8937....252
CP8938....253
CP8939....215, 253
CP8940....253
CP8941....253
CP8941I5....253
CP8942....253
CP8943....218, 253
CP8943I5....253
CP8944....214-219, 223-224, 226-227, 253
CP8944I5....253
CP8945....218, 226-227, 253
CP8946....214, 222, 226-227, 253
CP8947....253
CP8948....218, 253
CP8948I5....253
CP8949....253
CP8950....253
CP8951....253
CP8952....253
CP8953....253
CP8954....253
CP8954I5....253
CP8955....213, 227, 253
CP8955I5....253
CP8956....253
CP8957....215, 225, 253
CP8957I5....253
CP8958....253
CP8959....253
CP8960....219, 253
CP8960I5....253
CP8961....253
CP8961I5....253
CP8962....253
CP8963....253
CP8964....362
CP8965....248
CP8967....223, 248
CP8968....248
CP8969....224, 248
CP8970....248
CP8971....253
CP8972....253
CP8973....223, 253
CP8974....253
CP8975....224, 253
CP8976....218, 221-222, 224, 253
CP8977....259
CP8979....259
CP8980....259
CP8981....259
CP8982....218, 259
CP8982I5....259
CP8983....219, 259
CP8984....259
CP8986....259
CP8987....259
CP8990....259
CP8990I5....259
CP8991....213, 259
CP8994....259
CP8996....259
CP8998....259
CP9000....259
CP9001....221, 259
CP9002....222, 259
CP9010....392
CP9011....392
CP9012....392
CP9013....392
CP9014....392
CP9015....392
CP9016....392
CP9018....392
CP9019....392
CP9020....392
CP9021....392
CP9022....392
CP9023....392
CP9024....392
CP9025....392
CP9026....392
CP9027....392
CP9030....247
CP9031....247
CP9032....247
CP9032I5....247
CP9034....252
CP9034I5....252
CP9035....252
CP9036....252
CP9036I5....252
CP9037....252
CP9038....252
CP9039....252
CP9039I5....252
CP9040....252
CP9041....255
CP9042....260
CP9044....317
CP9045....317
CP9046....317
CP9047....317
CP9048....317
CP9050....266
CP9051....266
CP9052....266
CP9053....266
CP9054....215, 266
CP9055....266
CP9056....266
CP9057....266
CP9058....266
CP9059....266
CP9060....266
CP9060I5....266
CP9061....266
CP9062....266
CP9063....266
CP9064....266
CP9066....266
CP9070....213-214, 218-219, 225, 335
CP9071....335
CP9072....335
CP9073....334
CP9074....213-215, 218-219, 225, 334
CP9075....334
CP9076....330, 367
CP9077....330, 367
CP9078....236, 330, 367
CP9079....330, 367
CP9080....330
CP9083....330
CP9090....317, 365
CP9091....317, 366
CP9092....317, 365
CP9092I5....317
CP9093....317, 366
CP9094....317, 365
CP9094I5....317, 365
CP9095....317, 366
CP9096....317, 365
CP9097....317, 366
CP9100....265
CP9101....265
CP9101I5....265
CP9102....213, 215, 217, 265
CP9102I5....265
CP9103....213, 215, 221, 225-226, 265
CP9103I5....265
CP9104....265
CP9104I5....265
CP9105....217, 219, 226, 265
CP9105I5....265
CP9106....265
CP9106I5....265
CP9107....221, 265
CP9108....217, 219, 265
CP9109....265
CP9110....265
CP9140....267
CP9141....267
CP9142....267
CP9143....267
CP9144....267
CP9145....267
CP9146....267
CP9147....267
CP9148....267
CP9149....267
CP9149I5....267
CP9150....267
CP9151....214, 216, 267
CP9151I5....267
CP9152....267
CP9152I5....267
CP9153....267
CP9154....267
CP9154I5....267
CP9155....267
CP9155I5....267
CP9156....267
CP9157....268
CP9158....268
CP9159....268
CP9160....268
CP9161....268
CP9162....268
CP9163....213, 268
CP9164....268
CP9165....268
CP9166....268
CP9166I5....268
CP9167....268
CP9168....268
CP9169....268
CP9170....268
CP9171....221-224, 268
CP9172....268
CP9173....268
CP9174....268
CP9175....267
CP9176....392
CP9177....392
CP9200....263
CP9201....263
CP9202....263
CP9203....263
CP9204....263
CP9205....263
CP9205I5....263
CP9206....217, 263
CP9207....263
CP9208....264
CP9209....264
CP9210....264
CP9211....264
CP9212....264
CP9212I5....264
CP9213....264
CP9214....264
CP9215....220, 224, 227, 264
CP9216....264
CP9217....264
CP9218....263
CP9219....263
CP9220....263
CP9221....263
CP9222....263
CP9223....263
CP9224....264
CP9225....264
CP9225I5....264
CP9226....221, 264
CP9226I5....264
CP9227....264
CP9228....264
CP9229....263
CP9229I5....263

CP97638....355
CP97638I5....355
CP97658....355
CP97658I5....355
CP97711....355
CP97711I5....355
CP97713....355
CP97721....355
CP97723....355
CP97723I5....355
CP97743....355
CP97753....355
CP97753I5....355
CP97763....355
CP97763I5....355
CP97773....355
CP97773I5....355
CR213105....157
DY50295500....52
DY50296800....52
DY50390600....52
DY50402400....52
DY50540700....52
DY50546100....52
DY50548400....52
DY50549100....52
DY50549290....52
DY50549500....52
DY50551400....52
DY50559800....52
DY50559900....52
DY50572600....52
DY50573990....52
DY50574190....52
DY50574500....52
DY70001990....52
DY70007701....52
DY70007791....52
DY70008101....52
DY70008590....52
G1072-20008....120
G1099-20030....117
G1099-20130....120
G1099-20132....120
G1099-20133....120
G1099-20136....120
G1099-60566....116
G1099-80001....127
G1099-80039....131-132
G1099-80053....121, 125, 133
G1530-61950....84
G1530-80650....107
G1531-00105....84
G1531-20550....82
G1531-20690....84
G1531-20700....84
G1531-20740....85
G1531-21090....84
G1531-40020....105
G1531-60680....85
G1531-60690....85
G1531-60700....84
G1531-80560....81, 104-105
G1531-80620....81, 104
G1532-20710....91
G1532-60675....93
G1532-60685....93
G1532-60690....93
G1532-60695....93
G1532-80540....91
G1533-80565....88
G1534-20530....105
G1534-20590....105
G1534-40020....105
G1534-40030....105
G1534-60570....101, 105
G1534-60610....105
G1534-80500....105
G1534-80510....105
G1534-80540....105
G1534-80580....104
G1534-80590....104
G1535-00010....100
G1535-00030....100
G1535-60600....99
G1535-60610....100
G1535-80520....100
G1540-85010....108
G1543-00060....76
G1543-00085....76
G1543-00100....76
G1543-00155....76
G1543-20580....76
G1543-20765....76
G1543-61540....76
G1544-20590....63
G1544-60575....62
G1544-60585....62
G1544-60610....63
G1544-80530....63
G1544-80580....62
G1544-80700....28
G1544-80730....28
G1544-80731....28
G1580-60060....41
G1580-60062....41
G1580-60575....62
G1580-60585....62
G1580-80060....41
G1580-80062....41
G1888-60701....49
G1888-60702....48
G1888-60703....48
G1888-60704....48
G1946-00034....132
G1946-20168....76, 84
G1999-20021....120-121
G1999-20430....121
G1999-20432....121
G1999-20433....121
G1999-20443....121
G1999-20444....121
G1999-20446....121
G1999-60412....121
G1999-80410....132
G2397-20540....88
G2397-80520....88
G2589-20043....120
G2589-20044....120
G2589-20045....120
G2589-20100....120
G2617-20510....71-72
G2617-60506....71-72
G2617-60507....71-72
G2617-60508....71-72
G2617-60510....71-72
G2617-60517....72
G2617-60518....72
G2617-80540....71
G2617-80550....72
G2618-80500....71
G2619-60501....71-72
G2630-60710....107
G2630-61230....93
G2855-20530....37, 41
G2855-20555....37, 41
G2855-20590....37, 46
G2855-40001....46
G2855-60200....37, 41, 46, 117
G2855-60570....46, 117
G2933-85001....107
G2933-85003....107
G3163-20530....120
G3170-20126....120-121
G3170-20530....120
G3170-20540....121
G3170-60050....120, 125, 133
G3170-80001....125, 133
G3170-80002....116, 133
G3170-80008....127
G3170-80100....127
G3170-80103....127, 133
G3182-61580....36
G3182-61581....36
G3184-60065....37
G3185-60300....124
G3185-60361....124
G3185-60362....124
G3185-60363....124
G3185-60364....124
G3430-40035....55, 62
G3430-60011....62
G3431-00005....64, 76
G3431-60680....85
G3431-80507....84
G3431-80509....84
G3432-00003....76
G3432-00004....76
G3432-60220....93
G3432-60221....93
G3433-63000....88
G3434-60806....101
G3434-67500....105
G3434-67540....105
G3451-80501....76
G3452-60100....62
G3452-60730....64
G3452-60730....62
G3452-60835....46
G3480-67585....62
G3500-80000....72
G3500-80001....72
G3504-20504....34
G3510-20018....64
G3520-20210....46
G3520-67001....46
G3591-70001....406
G3591-70002....404
G3591-70003....404
G3591-70004....404
G3591-70005....403
G3591-70006....403
G3591-70007....403
G3591-70008....404
G3591-70009....406
G3591-70010....406
G3591-70011....403
G3591-70013....404
G3591-70014....406
G3591-70015....404
G3591-70017....404
G3591-70018....406
G3591-74001....403
G3591-80000....407
G3591-80001....401
G3591-80002....403
G3591-80003....404
G3591-80004....403
G3591-80005....406
G3591-80006....407
G3591-80007....407
G3591-80008....407
G3591-80011....402
G3591-80012....404
G3591-80013....406
G3591-80014....407
G3591-80015....407
G3591-80016....406
G3591-80017....404
G3591-80019....403
G3591-80020....403
G3591-80021....401
G3591-80022....404
G3591-80023....403
G3591-80025....405
G3591-80026....406
G3591-80027....401
G3591-80028....404
G3591-80029....406
G3591-80030....401
G3591-80031....404
G3591-80032....401
G3591-80033....403
G3591-80034....407
G3591-80035....404
G3591-80036....405
G3591-80037....402
G3591-80039....401
G3591-80040....407
G3591-80043....404
G3591-80044....405
G3591-80045....402
G3591-80046....404
G3591-80047....403
G3591-80048....405
G3591-80049....407
G3591-80050....401
G3591-80051....406
G3591-80052....406
G3591-80053....406
G3591-80054....404
G3591-80055....401
G3591-80056....404
G3591-80058....404
G3591-80059....405
G3591-80060....402
G3591-80061....404
G3591-80062....404
G3591-80063....407
G3591-80064....404
G3591-80065....404
G3591-80066....406
G3591-80067....402
G3591-80068....407
G3591-80071....406
G3591-80072....405
G3591-80074....404
G3591-80075....404
G3591-80077....404
G3591-80082....401
G3591-80083....406

G3591-80084....400
G3591-80085....404
G3591-80086....405
G3591-80087....405
G3591-80088....402
G3591-80090....404
G3591-80091....402
G3591-80093....405
G3591-80094....407
G3591-80095....400
G3591-80096....406
G3591-80097....404
G3591-80098....404
G3591-80099....400
G3591-80100....403
G3591-80101....404
G3591-80102....403
G3591-80103....404
G3591-80104....404
G3591-80105....400
G3591-80106....406
G3591-80107....404
G3591-80108....407
G3591-80110....405
G3591-80119....405
G3591-80120....406
G3591-80121....403
G3591-80122....405
G3591-80123....405
G3591-80125....401
G3591-80135....406
G3591-80136....406
G3591-80137....406
G3591-80138....406
G3591-80139....401
G3591-80140....401
G3591-80141....407
G3591-80142....407
G3591-80157....406
G3591-80158....402
G3591-80162....405
G3591-81000....407
G3591-81001....401
G3591-81002....403
G3591-81003....404
G3591-81004....403
G3591-81005....406
G3591-81006....407
G3591-81007....407
G3591-81008....407
G3591-81011....402
G3591-81012....404
G3591-81013....406
G3591-81014....407
G3591-81015....407
G3591-81016....406
G3591-81017....404
G3591-81019....403
G3591-81020....403
G3591-81021....401
G3591-81022....404
G3591-81023....403
G3591-81025....405
G3591-81026....406
G3591-81027....401
G3591-81028....404
G3591-81029....406
G3591-81031....404
G3591-81032....401
G3591-81033....403
G3591-81034....407
G3591-81035....404
G3591-81036....405
G3591-81037....402
G3591-81039....401
G3591-81040....407
G3591-81043....404
G3591-81044....405
G3591-81045....402
G3591-81046....404
G3591-81047....403
G3591-81048....405
G3591-81049....407
G3591-81050....401
G3591-81051....406
G3591-81052....406
G3591-81053....406
G3591-81054....404
G3591-81055....401
G3591-81056....404
G3591-81058....404
G3591-81059....405
G3591-81060....402
G3591-81061....404
G3591-81062....404
G3591-81063....407
G3591-81064....404
G3591-81065....404
G3591-81066....406
G3591-81067....402
G3591-81068....407
G3591-81071....406
G3591-81072....405
G3591-81074....404
G3591-81075....404
G3591-81077....404
G3591-81082....401
G3591-81083....406
G3591-81084....400
G3591-81085....404
G3591-81086....405
G3591-81087....405
G3591-81088....402
G3591-81090....404
G3591-81091....402
G3591-81093....405
G3591-81094....407
G3591-81095....400
G3591-81096....406
G3591-81097....404
G3591-81098....404
G3591-81099....400
G3591-81100....403
G3591-81101....404
G3591-81102....403
G3591-81103....404
G3591-81104....404
G3591-81105....400
G3591-81106....406
G3591-81119....405
G3591-81120....406
G3591-81121....403
G3591-81122....405
G3591-81123....405
G3591-81125....401
G3591-81135....406
G3591-81136....406
G3591-81137....406
G3591-81138....406
G3591-81139....401
G3591-81140....401
G3591-81141....407
G3591-81142....407
G3591-81148....403
G3591-81149....404
G3591-81150....403
G3591-81160....402
G3591-81161....402
G3591-81162....405
G3591-82000....407
G3591-82001....401
G3591-82002....403
G3591-82003....404
G3591-82004....403
G3591-82005....406
G3591-82006....407
G3591-82007....407
G3591-82008....407
G3591-82011....402
G3591-82012....404
G3591-82013....406
G3591-82014....407
G3591-82015....407
G3591-82016....406
G3591-82017....404
G3591-82019....403
G3591-82020....403
G3591-82021....401
G3591-82022....404
G3591-82023....403
G3591-82025....405
G3591-82026....406
G3591-82027....401
G3591-82028....404
G3591-82029....406
G3591-82030....401
G3591-82031....404
G3591-82032....401
G3591-82033....403
G3591-82034....407
G3591-82035....404
G3591-82036....405
G3591-82037....402
G3591-82039....401
G3591-82040....407
G3591-82043....404
G3591-82044....405
G3591-82045....402
G3591-82046....404
G3591-82047....403
G3591-82048....405
G3591-82049....407
G3591-82050....401
G3591-82051....406
G3591-82052....406
G3591-82053....406
G3591-82054....404
G3591-82055....401
G3591-82056....404
G3591-82058....404
G3591-82059....405
G3591-82060....402
G3591-82061....404
G3591-82062....404
G3591-82063....407
G3591-82064....404
G3591-82065....404
G3591-82066....406
G3591-82067....402
G3591-82068....407
G3591-82071....406
G3591-82072....405
G3591-82074....404
G3591-82075....404
G3591-82077....404
G3591-82082....401
G3591-82083....406
G3591-82084....400
G3591-82085....404
G3591-82086....405
G3591-82087....405
G3591-82088....402
G3591-82090....404
G3591-82091....402
G3591-82093....405
G3591-82094....407
G3591-82095....400
G3591-82096....406
G3591-82097....404
G3591-82098....404
G3591-82099....400
G3591-82100....403
G3591-82101....404
G3591-82102....403
G3591-82103....404
G3591-82104....404
G3591-82105....400
G3591-82106....406
G3591-82119....405
G3591-82120....406
G3591-82121....403
G3591-82122....405
G3591-82123....405
G3591-82125....401
G3591-82135....406
G3591-82136....406
G3591-82137....406
G3591-82138....406
G3591-82139....401
G3591-82140....401
G3591-82141....407
G3591-82142....407
G3591-82159....403
G3591-82162....405
G3880-20030....117
G3880-80010....125
G3880-80011....125
G3900-63001....395
G3900-63002....395
G3900-63003....396
G3900-63004....395
G3900-63005....395
G3900-63006....396
G3900-63007....396
G3900-63008....396
G3900-63009....395
G3900-63010....396
G3900-63011....396
G3900-63012....396
G3900-63013....395
G3900-63014....395
G3900-63015....396
G3900-63016....395
G3900-63017....395
G3900-63018....395
G3900-63019....395
G3900-63020....396
G3900-63021....396
G3900-63022....396
G3900-63023....396

G3900-63024....396
G3900-63025....396
G3900-63026....396
G3900-63027....396
G3900-63028....396
G3900-63029....396
G3900-63030....395
G3900-63031....395
G3900-63032....395
G3900-63033....395
G3900-63034....396
G3900-63035....396
G3900-63036....396
G3900-63037....396
G3900-63038....395
G3900-63039....395
G3900-63040....395
G3900-63041....395
G3900-63042....395
G4513-20561....43
G4513-40525....43
G4513-40529....43
G4513-80209....21
G4513-80213....21
G4514-60710....43
G4514-67505....43
G4525-60701....43
G4525-60702....43
G4525-60703....43
G4525-60704....43
G4556-60019....46
G4556-60125....46
G4556-60690....46
G4556-67010....46
G4556-80101....47
G4556-80102....47
G4556-80103....47
G4556-80105....47
G4556-80106....47
G4556-80108....47
G4556-80109....47
G4556-80111....47
G4556-80112....47
G4556-80113....47
G4556-80115....47
G4556-80116....47
G4556-80118....47
G4556-80119....47
G4556-80126....47
G4556-80128....47
G4556-90500....46
G6600-60037....107
G6600-60038....106
G6600-67006....107
G6600-67007....106
G6600-67008....106-107
G6600-67009....106
G6600-80018....35, 106-107
G6600-80042....106
G6600-80043....106-107, 132
G6600-80044....106-107
G6600-80045....106
G6600-80050....106
G6600-80051....106-107
G6600-80063....106
G6600-85000....107
G6600-85001....106-107
G6600-85002....106-107
IDP3TS....131
MKI-C-QSC10....53
MKI-MTD-1169....53
MKI-MTD-1204....53
MKI-U-COV06....53
MKI-U-COV07....53
MKI-U-COV10....53
MKI-U-DISK1....53
MKI-U-DISK3....53
MKI-U-T11GPC....53
MKI-U-T11GPC-2S....53
MKI-U-T12ME....53
MKI-U-T12ME-2S....53
MKI-U-T3ATX....53
MKI-U-T3ATX-2S....53
MKI-UTD-5064....53
MKI-UTD-5105....53
MKI-Z-0285....53
MKI-Z-0351....53
RDT-1020....46
UMC-2....132

Application Title Index

1,3-Butadiene 561
1,3-Butadiene Purity 562
122-5512UI 141
15+1 EU Priority PAHs 433
69 Component FAME Mix 496

A

Acids 495
Acrylate Impurities I 527
Acrylate Impurities II 528
Acrylates 528
Agilent's Ultra Inert Test Probe Mixture 458
Alcohol Beverage Standard 492
Alcohols I 501
Alcohols II 505
Alcohols III 505
Aldehydes and Acids 511
Aldehydes and Ketones 512
Alditol Acetates 493
Amines and Alcohols 506
Amines and Nitriles 510
Amines in Water 511
Amphetamines and Precursors – TMS Derivatives 536
Anabolic Steroids 548
Analysis of Acetylenes Mixture 534
Analysis of Amino Alcohols in Water 506
Analysis of Ethanolamines 506
Analysis of Fragrance and Allergens 485
Analysis of Gases C1 to C4 576
Analysis of Oxygenates in a C1 to C5 Hydrocarbon Mix 575
Analysis of Polycyclic Aromatic Hydrocarbons 431
Analysis of Semivolatiles 437
Analysis of Solvents 526
Anesthetics 543
Anilines 529
Anticonvulsants 543
Antiepileptic Drugs 544
Antihistamines 544
Aroclors 1016-1268 (without 1221) 441
Aromatic Solvents 503
Aromatics Analysis – ASTM D16 Analytes 568
Aromatics Analysis – Ethylbenzene Impurities 568
Aromatics I 514
Aromatics II 515
Aromatics in Finished Gasoline – ASTM Method 5769 571
Aspirin and Ibuprofen in Methanol 547

B

Bacterial Fatty Acid Methyl Esters 495
Barbiturates 537
Baseline Resolution of Air/CO, COBenzodiazepines I 536
Benzodiazepines II 540
Blood Alcohols I (Static Headspace/Split) 538
Blood Alcohols II (Static Headspace/Split) 538
Blood Pollutants I 549
Blood Pollutants II 549
Boiling Point Elution Order for Homologous Series 197
Bourbon 493
Butter Triglycerides I 499
Butter Triglycerides II 499

C

CCLP Pesticides 441
Canola Oil Margarine Partially Hydrogenated FAMEs AOCS Method 1c-89 499
Chiral Compounds in Essential Oils and Fragrances 484
Chlorinated Isooctane 523
Chlorinated Pesticides, EPA Method 508 448
Citrus Flavored Carbonated Beverage (Soda) 492
Cold-Pressed Orange Oil 489
Common Drug Screen 541
Common Industrial Solvents 525
Congeners in DIN Method PCBs 459

D

DNPH Derivative 513
Denatured Fuel Ethanol – ASTM D5501 570
Detailed Hydrocarbon Analysis of Petroleum Naphthas Through N-nonane Using ASTM D-5134 576
Determination of Chlorophenols in Water and Soil 430
Deviation from Boiling Point Order 197
Diesel Analysis 575
Diesel Fuel 431
Dioxins and Dibenzofurans 432
Dipole Interactions 198
Direct Comparison for Rapid CLP (Contract Laboratory Program) Pesticide Analysis 440
Direct Injection of Gasoline and Diesel Fuel in Methylene Chloride 575
Drug Screen 540

E

EPA 625 Halogenated Pesticides on "1701" Type Phases 455
EPA Air Analysis Compendium Method TO-14 Standard 473
EPA Air Analysis Method TO-15 (1 ppbV Standard) 477
EPA Method 525.2 445
EPA Method 551 470
EPA Method 552.2 467
EPA Volatiles by GC/MS (Split Injector) 444, 471
Esters I 517
Esters II 518
Esters III 518
Ethers 519
Ethoxyethanol 507
Ethylene 559
Ethylene Glycol Mixture 521
Ethylene Oxide 531
Ethylene Oxide Synthetic Standard 569
European Red List Volatiles 470
Extended Analyte List for EPA Method 8021 468
Extended Hydrocarbon Analysis I 563
Extended Hydrocarbon Analysis II 564
Extended Temperature Program Resolving Congeners 52 and 138 460

F

FAME Standard 497-498
FAMEs 485
Fast Analysis of Aromatic Solvent 552
Fast Analysis of Permanent Gases and COFast Separation of Silanes 533
Fast VOC Analysis 469
Fast analysis of lemon oil using Rapid-MS 488
Fast screening of FAME isomers in butter 500
Fentanyls 545
Flavor Mixture 487
Formaldehyde Underivatized 513
Formaldehyde, 50ppb 474
Fragrance Allergens 487
Fragrance Reference Standard 482-483
Free Organic Acids/C4-C5 Isomers 508
Free Phenols 455
Free Steroids 548

G

Gasoline Unleaded ASTM D 5769 574
Glycols I 519
Glycols II 520
Glycols III 520
Glycols/Diols 522

H

Hallucinogens 545
Halocarbons 531
Halogenated Hydrocarbons I 502
Halogenated Hydrocarbons II 522
Halothane 532
Herbicides I 453
Herbicides II 453
High Resolution Phenol Analysis by GC/MS 466
High Resolution Separation of Xylene Isomers 532
High Speed VOC, EPA Method 8260 442
Hydrogen Bonding Interactions 199

I

Impurities in Ethylbenzene 516
Impurities in Ethylene 559
Impurities in Mixed Xylenes 532
Impurities in Propylene 560
Impurities in Styrene 516
Impurities in p-Xylene – ASTM D3798 569
Inorganic Gases 504
Inorganic Hydride Gases 533

L

Lavender Oil Characterization....480
Lemon Oil....488

M

Marijuana (Δ9-THC) and Major Metabolites – TMS Derivatives....548
Menthol....484
Mercaptans....567
Methyl Tert-Butyl Ether (MTBE) FID, Extended 8020 Analysis....429

N

Narcotics....537
Narcotics and Adulterants....546
Natural Gas....558
Nitrogen Based Solvents I....526
Nitrogen Based Solvents II....527
Nitrogen Containing Herbicides (EPA Method 507)....454
Nitrogen/Phosphorus Containing Pesticides, EPA Method 507....452
Noble Gases....557
n-Paraffin Standard....554

O

Organic Acids....494, 507
Organochlorine Pesticides....452
Organochlorine Pesticides I....449
Organochlorine Pesticides I EPA Method 8081A....447, 456
Organochlorine Pesticides II....449
Organochlorine Pesticides II EPA Method 8081A....457
Organochlorine Pesticides III....450
Organochlorine Pesticides IV....450
Organochlorine Pesticides to EPA 625 via GC/MS....456
Organochlorine Pesticides, DB-5/DB-1701P....451
Organohalide Pesticides in Water, EPA Method 505....448
Organophosphorus Pesticide Residues in Olive Oil Extract....486
Organotin Compounds I....461
Organotin Compounds II....461
Over-the-Counter Pain Killers – TMS Derivatives....547
Oxygenates....570
Oxygenates in Gasoline ASTM D5599 (GC-OFID)....570

P

PAHs....465
PBDEs....443
PBDEs by ECD....430
PCBs by EPA Method 8082....460
PFBHA Derivative....514
PONA Mix as Specified by AFNOR Method #2....571
Peppermint Oil....489
Perfume....484
Permanent Gases....557
Permanent Gases on a Thick Film Molsieve Column....476
Pesticides in sunflower oil....500
Pesticides, EPA 508.1....438
Phenols....464
Phenols According to EPA Method 8040....466
Phenols I....504
Phenols II....530
Phenols III....530
Phenoxy Acid Herbicides – Methyl Derivatives, EPA 8151A....439
Phenyl Content Retention....199
Polarity – Retention Relationship....200
Polyethylene....574
Polyethyleneamines....509
Polymer Additives....533
Primary Amines....509
Propylene....560
Pyrethrins....461
Pyrolysates of Polystyrene....517

R

Reference Gas Oil....572
Refinery Gas....565
Refinery Gas I....553
Regular Unleaded Gasoline (California Phase 1) – "Normal" GC Run I....573
Regular Unleaded Gasoline (California Phase 1) – "Normal" GC Run II....573
Residual Solvents....551
Residual Solvents, DMI Diluent....539
Residual Solvents, USP 467....550
Rosemary Oil....491

S

Sedative Hypnotics....546
Selected Oxygenates....557
Semivolatile Compounds, US EPA Method 8270....462
Separation of TMS-derivatized sugars using VF-1ms....494
Separation of *cis*-trans FAME isomers....496
Simulated Distillation....572
Solvents I....523
Solvents II....524
Solvents III....524
Solvents IV....525
Spearmint Oil (Western)....490
Strawberry Syrup....493
Substituted Anilines....529
Sulfur Compounds in Naphtha....568
Sulfur Compounds in Natural Gas – Synthetic Mixture....567
Sulfur Compounds in Propylene (1 ppm)....555, 566
Sulfur Gas Analysis in Light Hydrocarbon Streams I....565
Sulfur Gas Analysis in Light Hydrocarbon Streams II....566
Sulfur Gases....534
Sulfur Impurities in Propylene....555
Sulfur in Air....474

T

Tetrachlorodibenzo-p-furans....459
Tocopherols....545
Trace Active Amines, 10 ng on-column....508
Trace Level Polycyclic Aromatic Hydrocarbon (PAH) Analyses....458
Trace Oxygenates in Light Hydrocarbon Matrices....556
Trace Sulfur Compounds in Methane (50 ppbv)....556
Tricyclic Antipsychotics....544
Triethylene Glycol and Impurities....521

U

US EPA Method 551.1....436
US EPA Method 8061 (Phthalate Esters)....463
US EPA Method 8270 Short Mix....463
Underivatized Drugs of Abuse – Agilent Fast Toxicology Analyzer....539
Unleaded Gasoline....429, 553
Urine Drug Screen....542

V

Volatile Amines....508
Volatile Sulfur Compounds....554

Y

Ylang Ylang Oil....490-491

Compound Index

A

Acealdehyde....556
Acenaphthalene....465
Acenaphthalene-d10....446
Acenaphthene....431, 458, 462, 465
Acenaphthene-d10....445, 462-463
Acenaphthylene....431, 445, 458, 462
Acephate....486
Acetal (acetaldehyde diethyl acetal)....519
Acetaldehyde....474, 477, 492-493, 512, 538, 549, 575
Acetaminophen....541, 547
Acetic acid....435, 492-495, 507, 511
Acetic acid, ethyl ester....570
Acetic acid, methyl ester....570
Acetone....442, 444, 471, 474, 477-478, 482-483, 492, 494, 512, 524-526, 532, 538-539, 549-550, 556-557, 575
Acetone-d6....474
Acetonitrile....442, 524, 526-527, 535, 539, 549-550
Acetyl aldehyde....478
Acetylcedrene....484
6-Acetylcodeine....537, 546
Acetylene....559-565
Acetylsalicylic acid (aspirin)....547
Acifluorofen....439
Acrolein....442, 512, 526-527
Acrylamide....510
Acrylic acid....435
Acrylonitrile....442, 444, 471, 526-527
Adrin....448
Alachlor....435, 438, 445, 447-448, 451-453, 456-457
Aldrin....434-435, 438, 440-441, 445, 447-452, 456-457
Alfentanyl....545
Allobarbital....537, 541
Allyl acrylate....528
Allyl alcohol....442, 556
Allyl butyrate....482-483
Allyl chloride....442, 444, 468, 471
Allyl ether....519
Allyl ethyl ether....519
Alphenal....537
Alprazolam....141, 536, 539-540
Ametryn....445, 452-453
2-Aminoazotoluene....529
4-Aminobiphenyl....463
2-Amino-1-butanol....506
2-Amino-ethanol....506
Aminoethylethanolamine....511
n-(2-Aminoethyl) piperazine....511
2-Aminonaphthalene....529
1-Amino-4-nitronaphthalene....465
5-Amino-1-pentanol....506
1-Amino-2-propaol....506
Amitriptyline....542
Amobarbital....537, 541
Amphetamine....536, 539, 542
Amyl acetate....478, 493, 517-518
Amyl alcohol....478, 549
n-Amyl alcohol....492
Amyl butyrate....493
Amyl cinnamic alcohol....485
Amyl cinnamyl alcohol....487
Amyl cinnamyl aldehyde....485
n-Amyl mercaptan....567
tert-Amyl mercaptan....567
tert-Amyl methyl ether (TAME)....429, 442, 519, 556, 570, 574-575
n-Amyl salicylate....482-484
5α-Androstan-17α-ol-3-one (Stanolone)....548
Androsterone....548
5-β-Androsterone....548
Aniline....462-463, 510, 529
Anisic alcohol....485
Anisyl alcohol....487
Antazoline....544
Anthracene....431, 445, 458, 462, 465
Anthracene-d10....446
Aprobarbital....537, 541
Arabinitol....493
Arabitol....494
Arachidic acid (eicosanoic acid)....494
Arachidic acid methyl ester....497-498
Arachidonic acid methyl ester....497-498
Argon....476, 557
Arsine....533
Atraton....452-453
Atrazine....438, 445-446, 448, 452-454
Azinphos-ethyl....486
Azinphos-methyl....486
Azobenzene....462
Azulene....465

B

Balan....454
Barbital....537
Behenic acid methyl ester....497-498
Benactyzine....541
Bentazone....439
Benthiocarb....446
Benylamine....509
Benzaldehyde....482-483, 487, 512
Benzaldehyde, 3 methoxy....478
Benz[a]anthracene....433, 445, 458
Benz[a]anthracene-7,12-dione....465
1,2-Benzanthracene....465
Benzene....429, 442, 444, 468-469, 471, 473, 477, 503, 514-516, 523-524, 526, 532, 535, 549-553, 561-564, 568, 571, 574, 576
Benzene-d6....571
Benzene ethanol....482-484
α-Benzene hexachloride (BHC)....434-435, 438, 440-441, 445, 447-452, 456-457
β- Benzene hexachloride....434-435, 438, 440-441, 445, 447-452, 456-457
δ-Benzene hexachloride....434-435, 438, 440-441, 445, 447-452, 456-457
γ-Benzene hexachloride....434-435, 438, 440-441, 445, 447-452, 456-457
Benzidene....432
Benzidine....462-463, 529
Benzo[a]anthracene....431, 462
Benzocaine....543
Benzo[b]fluoranthene....431, 433, 445, 458, 462-463, 465
Benzo[j]fluoranthene....433
Benzo[k]fluoranthene....431, 433, 445, 458, 462-463, 465
Benzo[c]fluorene....433
2,3-Benzofluorene....465
Benzo[g,h,i]perylene....431-433, 445, 458, 462, 465
Benzo[a]pyrene....431, 433, 445, 458, 462, 465
Benzo[e]pyrene....465
Benzoic acid....462
Benzonitrile....510, 526-527
Benzophenone....482-483
5,6-Benzoquinoline....465
Benzothiophene....568
Benzphetamine....536, 541
Benzyl acetate....482-484, 490-491, 517-518
Benzyl alcohol....462, 482-483, 485, 487, 501, 505
Benzylamine....510
Benzyl benzoate....463, 482-485, 487, 490-491, 493
Benzyl butyl phthalate....445
Benzyl chloride....442, 468, 477
Benzyl cinnamate....485, 487
Benzyl ether....519
n-Benzylmethylamine....510
Benzyl salicylate....482, 484-485, 487, 490-491
α-Bergamotene....480
trans-α-Bergamotene....488
Bifenthrin....446
Bioallethrin....446
Biphenyl....465
β-Bisabolene....483, 488, 491
α-Bisabolol....480
Borneol....480, 482-484, 491
Borneol acetate....480
Bornyl acetate....481-482
α-Bourbonene....479
β-Bourbonene....479, 489-490
Bromacil....445-446, 452-454
Bromazepam....536, 540
Bromoacetic acid....467
Bromoacetone....442
4-Bromoaniline....510, 529
Bromobenzene....442, 444, 468-469, 471, 514-515
2-Bromobiphenyl....447, 456-457
Bromochloroacetic acid....467
Bromochloroacetonitrile....436, 470
Bromochlorodifluoromethane....454
Bromochloromethane....442, 444, 468-469, 471, 473-474, 477, 522
Bromodichloroacetic acid....467
Bromodichloromethane....436, 442, 444, 468-471, 477, 522
2-Bromo-4,6-dinitroaniline....529
Bromoethane (ethyl bromide)....477, 522
Bromofluorobenzene....469
4-Bromofluorobenzene....442, 444, 471, 473-474, 477
Bromoform....436, 442, 444, 468-471, 477, 522
Bromofos....500
Bromomethane....442, 444, 468-469, 471, 473, 477
1-Bromo-2-nitrobenzene....435, 447, 456-457
Bromopheniramine....541, 544
4-Bromophenyl-phenylether....462
3-Bromopyridine....510
Bromotrifluoromethane....454
Buclizine....544
Bufotenine....545
Butabarbital....537, 541
Butacaine....543
Butachlor....445, 452-453
1,2-Butadiene....534, 561-562
1,3-Butadiene....477, 534, 559-566
Butalbital....537
Butanal....511
Butane....574, 576
n-Butane....534, 553, 558-565, 570-571
n-Butane/*cis*-2-Butene....566
1,3-Butanediol....519-520, 522
1,4-Butanediol....519-520
2,3-Butanediol....519-520
2,3-Butanedione....478, 482-483
1-Butanethiol....554-556, 566
Butanol....526-528
1-Butanol....442, 478, 501, 505, 549, 570, 575
2-Butanol....535, 478, 539, 551
n-Butanol....492, 524, 550
sec-Butanol....492, 501, 505, 524-525, 550, 570
tert-Butanol....501, 505, 524, 550, 570
2-Butanone (MEK)....442, 444, 471, 474, 477, 512, 526, 539, 549, 551, 575
2-Butanthiol....556
Butene....517
Butene-1....559, 561-562
1-Butene....517, 534, 559-560, 563-566
cis-2-Butene....559-565
trans-2-Butene....559-566
1-Butene/methyl acetylene....565
2-Buten-1-ol (crotyl alcohol)....501, 505
3-Buten-1-ol....501, 505
Butethal....537
bis(2-n-butoxyethyl) phthalate....463
Butyl acetate....517-518, 527-528
n-Butyl acetate....525
sec-Butyl acetate....517-518
tert-Butyl acetate....517-518
Butyl acrylate....527-528
n-Butyl acrylate....528
n-Butyl alcohol....525, 556

sec-Butyl alcohol 524, 549, 556
tert-Butyl alcohol 442, 549, 556
Butylaldehyde 478, 556
Butylate 445, 452
Butylated hydroxy toluene (BHT) 485, 492, 533
Butylbenzene 442, 514-515, 553
n-Butylbenzene 444, 468, 471, 503, 532, 552, 568, 571
sec-Butylbenzene 442, 444, 468-469, 471, 503, 514-515, 552-553, 568
tert-Butylbenzene 442, 444, 468-469, 471, 503, 514-515, 552, 568,576
Butyl benzyl phthalate 462-463
Butyl caproate 518
Butyl cellosolve 501, 505, 525
Butyl cellosolve acetate 525
Butyl ether 519
Butyl ethyl ether 519
Butyl heptanoate 518
1-Butyl mercaptan 567
n-Butyl mercaptan 567
sec-Butyl methacrylate 528
Butyl methyl ether 519
tert-Butyl methyl ether (MTBE) 477
Butylpentyltin 461
Butyl propionate 518, 527-528
Butyl valerate 518
2-Butyne (dimethylacetylene) 561-562
1-Butyne (ethylacetylene) 561-562
2-*sec*-Butyl-4,-dinitrophenol (Dinoseb) 466
tert-Butyl mercaptan 556, 567
4-*tert*-Butyltoluene 514-515
Butyraldehyde 512, 575
Butyric acid 494-495, 507-508, 511
n-Butyric acid 435
Butyric acid methyl ester 497-498

C

Cadinene 489
δ-Cadinene 481-483, 491
γ-Cadinene 480-481
Caffeine 536, 540-541, 546-547
Camphene 480, 482-484, 488, 491
Camphor 480, 482-483, 491
Capric acid methyl ester 497-498
Caproic acid (hexanoic acid) 494, 507
Caproic acid methyl ester 497-498
Caprylic acid methyl ester 497-498
Captafol 435, 447, 456-457
Captan 447, 451, 456-457
Carbamazepine 543
Carbazepine 540
Carbazole 462, 465
Carbepoxide 10/11 544
Carbinoxamine 544
Carbon dioxide (CO2) 473, 476, 504, 553, 558, 576
Carbon disulfide (CS2) 444, 471, 474, 477, 554-555, 566
Carbon monoxide (CO-air) 476, 553, 557-558, 576
Carbon tetrachloride 436, 442, 444, 468-471, 473, 477, 502, 522, 535, 549
Carbonyl sulfide (COS) 474, 504, 534, 553-556, 566
Carbophenothion 451, 486
Carboxin 445, 452-453
3-Carene 480
Δ-Carane 481
Carfentanyl 545
cis-Carveol 487, 490
trans-Carveol 479, 487, 490
l-Carvone 479
(+/-)-Carvone 490
cis-Carvyl acetate 479, 490
Caryophyllene 480
α-Caryophyllene 491
β-Caryophyllene 479, 481-483, 488-491
Caryophyllene oxide 480
Celestocide 482
Cellosolve acetate 525
Cetearyl decanoate 482-483
Cetearyl octanoate 482-483
Chloral hydrate 436, 470
Chloramben 439
Chlorcyclizine 541, 544
α-Chlordane 434-435, 438, 440-441, 445, 447-451, 456-457
δ-Chlordane 448
γ-Chlordane 434-435, 438, 440-441, 445, 447-451, 456-457
Chlordiazepoxide 536
Chloroacetic acid 467
Chloroacetonitrile 442, 444, 471
2-Chloroaniline 510, 529
3-Chloroaniline 510, 529
4-Chloroaniline 462, 510, 529
Chlorobenzene 442, 444, 468-469, 471, 473, 477, 503, 514-515, 523
Chlorobenzene-d5 ....473-474, 477
Chlorobenzilate 435, 438, 445, 447-448, 451, 456-457
4-Chlorobenzonitrile 510
2-Chlorobiphenyl 445
1-Chlorobutane 442, 444, 471, 502, 522, 549
2-Chlorobutane 549
Chlorodibromoacetic acid 467
1-Chloro-1,1-difluoroethane 454
Chlorodifluoromethane 454
2-Chloro-4,6-dinitroaniline 529
Chloroethane 442, 444, 454, 468-469, 471, 473, 477
2-Chloroethanol 442, 531
bis(2-chloroethoxy) methane 462
bis(2-chloroethyl) ether 462
2-Chloroethyl vinyl ether 468
1-Chloro-3-fluorobenzene 444, 468, 471
Chloroform 436, 442, 444, 468-471, 473, 477, 502, 522, 524, 535, 549-551
1-Chlorohexane 442, 502, 522
1-Chloro isooctane 523
3-Chloro isooctane 523
4-Chloro isooctane 523
bis(2-chloroisopropyl) ether 462, 468
Chloromethane 442, 444, 454, 468-469, 471, 473, 477
4-Chloro-2-methylaniline 529
4-Chloromethyl 2,2'-dimethyl pentane 523
2-Chloro-5-methylphenol 464
4-Chloro-2-methylphenol 464
4-Chloro-3-methylphenol 455, 462, 464, 466, 504
2-Chloronaphthalene 462
Chloroneb 435, 438, 445, 447-448, 451, 456-457
2-Chloro-4-nitroaniline 529
4-Chloro-2-nitroaniline 529
1-Chloro-4-nitrobenzene 514-515
4-Chloro-3-nitrobenzotrifluoride 447, 456-457
Chloropentafluoroethane 454
2-Chlorophenol 430, 455, 462, 464, 466, 504, 530
3-Chlorophenol 430
4-Chlorophenol 430, 464
4-Chlorophenyl-phenyl ether 462
Chloropicrin 436, 470
Chloroprene 468
2-Chloropropane 468, 569
3-Chloropropene (allyl chloride) 477, 502, 522
3-Chloropropionitrile 442
Chloropropylate 435, 447, 456-457
Chloropyrifos 500
4-Chlorostyrene 514-515
2-Chloro-1,1,1,2-tetrafluoroethane 454
Chlorothalonil 435, 438, 445, 447-448, 456-457
2-Chlorotoluene 442, 444, 468-469, 471, 503, 514-515
3-Chlorotoluene 503, 514-515
4-Chlorotoluene 442, 444, 468, 471, 503, 514-515, 523
Chlorotrifluoromethane 454
Chlorpheniramine 541, 544
Chlorpothixene 544
Chlorpropham 445, 452
Chlorpyrifos 451, 453, 486
4-Chlortestosterone-17-acetate (Clostebal) 548
Cholesterol 548
Chrysene 431, 433, 445, 458, 462, 465
Chrysene-d12 ....445-446, 462-463
1,8-Cineol 479, 482-483, 489-490
Cineole 484
Cinerin I 461
Cinerin II 461
Cinnamaldehyde 485, 487
trans-Cinnamaldehyde 484
Cinnamic alcohol 487
Cinnamyl acetate 487, 490
trans-Cinnamyl acetate 491
Cinnamyl alcohol 485
Cinnamyl cinnamate 482-483
Cinnamyl phenyl acetate 482-483
Cinnanzine 544
Citral (geranial) 487
Citronellal 482, 484, 488-489
Citronellic acid 435
Citronellol 481-485, 487, 493
Citronellyl acetate 482-483
Citronellyl formate 481-482
Citronellyl propionate 482
Citronellyl tiglate 482-483
cis-Citronellyl tiglate 487
trans-Citronellyl tiglate 487
Clemizole 544
Clobazam 536, 540
Clonazepam 141, 536, 539-540
Cocaine 539-542, 546
Codeine 537, 539, 541-542, 546
Commamyl acetate 484
α-Copaene 479, 482-483, 491
Coprostane (5-α-cholestane) 548
Cotinine 542
Coumarin 484-485, 487
2-Cresol 530
3-Cresol 530
4-Cresol 530
m-Cresol 466, 530
o-Cresol 466, 530
p-Cresol 466, 530
Crotonaldehyde 442, 512
Cumene 429, 516, 523, 532, 552, 568
Cumic aldehyde 480
Cyanazine 438, 445, 453
2-Cyanopyridine 510
3-Cyanopyridine 510
Cyclizine 544
Cycloate 445, 452
Cyclohexane 477, 523-524, 526, 535, 539, 550, 552-553, 563-564, 568
Cyclohexanol 501, 505
Cyclohexanone 512, 525
2-Cyclohexyl-4,6-dinitrophenol 464
Cyclohexyl methacrylate 528
Cyclopentane 563-564, 571, 576
Cyclopenta[c,d]pyrene 433
Cyclopentanol 501, 505
Cyclopentanone 512
Cyclopentene 563-564
1-Cyclopentene 571
Cyclopentylbarbital 537
Cyclopropane 559-562
Cyheptamide 542
o-Cymene 480
p-Cymene 482-483, 492
r-Cymene 479,488-490

D

Dacthal (DCPA methyl ester) 445, 447, 453, 456-457
Dalapon 439, 467
Decachlorobiphenyl 434-435, 440-441, 449-451, 460
Decanal 488-489, 511
Decane 197, 199-200, 523, 552, 568, 574
n-Decane 197, 208, 458, 553, 571-572
1,10-Decanediol 519-520, 522
Decanoic acid 494, 511
Decanol 492
1-Decanol 501, 505
n-Decylamine 509-510

Dehydroisoandrosterone (Prasterone) 548
1-Dehydrotestosterone (Boldenone) 548
1-Dehydrotestosterone acetate 548
1-Dehydrotestosterone benzoate 548
1-Dehydrotestosterone undecylenate 548
Delorazepam 540
Demoxepam 536, 540
Desalkyl Aurazepam 536
Desipramine 540
Desmethyldiazepam 540
n-Desmethyl methsuximide 543
Dextromethorphan 537
Diacetone-alcohol 525
Diacetyl 492
Diacetylmorphine (Heroin) 141, 537, 539-541, 546
Di-allate A 447, 456-457
Di-allate B 447, 456-457
Diallate isomers 435
2,4-Diaminoanisole 529
2,4-Diaminotoluene 529
3,4-Diaminotoluene 510
Diamyl phthalate 463
Diazepam 536, 539-542
Diazinon 445, 452, 486
Dibenz[a,h]anthracene 431, 433, 445, 458, 462
1,2,3,4-Dibenzanthracene 465
1,2,5,6-Dibenzanthracene 465
Dibenzo-p-dioxin 465
Dibenzofuran 462, 465
Dibenzo[a,e]pyrene 433
Dibenzo[a,h]pyrene 433
Dibenzo[a,i]pyrene 433
Dibenzo[a,l]pyrene 433
Dibenzothiophene 465
Dibenzyl ether 482-483
Dibenzyl phthalate 463
Diborane 533
Dibromoacetic acid 467
Dibromoacetonitrile 436, 470
1,2-Dibromobenzene 473
4,4'-Dibromobiphenyl 438
Dibromochloromethane 436, 442, 444, 468-471, 477
1,2-Dibromo-3-chloropropane 435-436, 442, 444, 447, 456-457, 468-471
1,2-Dibromo-3-chloropropane (DBCP) 502, 522
1,2-Dibromoethane 436, 442, 444, 468, 470-471, 473, 477, 502, 522
Dibromofluoromethane 442
Dibromomethane 442, 444, 468-469, 471, 522
1,2-Dibromomethane 469
2,6-Dibromo-4-nitroaniline 529
4,4'-Dibromooctafluorobiphenyl 439
2,4-Dibromophenol 464
1,2-Dibromopropane 470
2,3-Dibromopropionic acid 467
1,2-Dibromo-1,1,2,2-tetrafluoroethane 454
α,α-Dibromo-m-xylene 447, 456-457
Dibucaine 543
Dibutylchlorendate 447, 456-457
tert-Dibutyl disulfide 567
Dibutyl ether 527-528
Dibutylpentyltin 461
Di-n-butyl phthalate 445, 462-463
Dicamba 439
Dichlobenil 453
Dichlone 435
Dichloroacetic acid 467
Dichloroacetonitrile 436, 470
3,4-Dichloroaniline 510, 529
1,2-Dichlorobenzene 442, 444, 462, 468-469, 471, 473, 477, 503, 514-515, 523
1,3-Dichlorobenzene 204, 206, 442, 444, 462, 468-469, 471, 473, 477, 503, 514-515, 523
1,4-Dichlorobenzene 204, 206, 442, 444, 462-463, 468-469, 471, 473, 477, 503, 514-515, 523
1,4-Dichlorobenzene-d4 442, 462-463
3,3'-Dichlorobenzidine 462-463, 529
3,5-Dichlorobenzoic acid 439
2,3-Dichlorobiphenyl 445
p,p'-Dichlorobiphenyl 451
cis-Dichlorobutene 442
cis-1,4-Dichlorobutene 468
trans-Dichlorobutene 442
trans-1,4-Dichloro-2-butene 444, 471, 502, 522
Dichlorodifluoromethane 442, 444, 454, 468, 471, 473, 477
Dichlorodimethyl silane 533
1,1-Dichloroethane 442, 444, 468-471, 473, 477, 502, 522
1,2-Dichloroethane 442, 444, 468, 470-471, 473, 477, 502, 522, 535
Dichloroethane-d4 442
1,1-Dichloroethene 442, 444, 468-469, 471, 473, 477, 502, 522
cis-1,2-Dichloroethene 442, 444, 468, 471, 473, 477
trans-1,2-Dichloroethene 442, 444, 468-469, 471, 477, 522
1,1-Dichloroethylene 470, 535
cis-1,2-Dichloroethylene 535
trans-1,2-Dichloroethylene 535
1,1-Dichloro-1-fluoroethane 454
Dichlorofluoromethane 454, 469
Dichloromethane 454, 525-526, 533, 535, 570
Dichloromethyl silane 533
2,6-Dichloro-4-nitroaniline 529
2,3-Dichlorophenol 430, 464
2,4-Dichlorophenol 430, 455, 462, 464, 466, 504, 530
2,5-Dichlorophenol 430, 464
2,6-Dichlorophenol 430, 464, 466
3,4-Dichlorophenol 430, 464
3,5-Dichlorophenol 430, 464
1,1-Dichloropropane 522
1,2-Dichloropropane 442, 444, 468-469, 471, 473, 477, 502, 522
1,3-Dichloropropane 442, 444, 468, 471, 522
2,2-Dichloropropane 442, 444, 468-469, 471, 522
1,3-Dichloro-2-propanol 442
1,1-Dichloro-2-propanone 436, 444, 470-471
1,1-Dichloropropene 442, 444, 468, 471
cis-1,2-Dichloropropene 502
trans-1,2-Dichloropropene 502
cis-1,3-Dichloropropene 442, 444, 468-469, 471, 473, 477, 522
trans-1,3-Dichloropropene 442, 444, 468-469, 471, 473, 477, 522
Dichlorotetrafluoroethane 477
1,2-Dichloro-1,1,2,2-tetrafluoroethane 454, 473
2,2-Dichloro-1,1,1-trifluoroethane 454
Dichlorvos 445, 452
Dicyclohexylamine 509-510
Dicyclohexyl phthalate 463
Dieldrin 434-435, 438, 440-441, 445, 447-452, 456-457, 500
Diethanolamine (DEA) 506
Diethylamine 510
2,6-Diethylaniline 510
n,n-Diethylaniline 510
Diethylbenzene 568
1,2-Diethylbenzene 552, 571
1,3-Diethylbenzene 552, 571
1,4-Diethylbenzene 571
Diethylene glycol 520-521
Diethylene glycol dimethyl ether (diglyme) 519-520
Diethylene glycol monobutyl ether 519-520
Diethylene glycol monoethyl ether 519-520
Diethylene glycol monomethyl ether 519-520
Diethylenetriamine 511
Diethyl ether 444, 471, 526, 532, 535, 549, 551, 556, 570, 575
1,2-Diethyl-4-ethylbenzene 571
1,3-Diethyl-5-ethylbenzene 571
Diethyl formamide (DEF) 445
Diethyl phthalate 445, 462-463, 484
Diethyl sulfide 554-556
Diethyltryptamine 545
1,4-Difluorobenzene 444, 471, 473-474, 477
1,1-Difluoroethane 454
Difolotan 453
Dihexyl phthalate 463
9,10-Dihydroanthracene 465
trans-Dihydrocarveol acetate 479
Dihydrocarvone 479, 490
trans-Dihydrocarvyl 490
Dihydrocodeine 537
Dihydropentaborane 533
Diisobutyl phthalate 463
Diisopropylamine 510
1,3-Diisopropylbenzene 503, 514-515
1,4-Diisopropylbenzene 503, 514-515
Diisopropyl ether (DIPE) 442, 429, 556, 570, 575
Dimenhydrinate 541, 544
Dimethoate 446, 486
3,3'-Dimethoxybenzidine 529
1,2-Dimethoxyethane 539, 570
n,n-Dimethylacetamide 539
Dimethylamine 508
Dimethylamphetamine 536
2,4-Dimethylaniline 510
2,6-Dimethylaniline 510, 529
7,12-Dimethylbenz[a]anthracene 465
1,2-Dimethylbenzene 484
n,n -Dimethylbenzylamine 510
2,2-Dimethylbutane 563-564, 571, 574
2,3-Dimethylbutane 563-564, 571, 574
Dimethyl ether 556
Dimethylformamide (DMF) 524, 526-527, 550
n,n-Dimethylformamide (DMF) 526, 539
2,6-Dimethylhept-5-enal 482-483
2,2-Dimethylhexane 444, 471, 574
1,3-Dimethyl-2-imidazolidinone (DMI) 539
2,6-Dimethylnaphthalene 465
1,2-Dimethyl-2-nitrobenzene 446
1,3-Dimethyl-2-nitrobenzene 445
2,2-Dimethylpentane 571, 574
2,3-Dimethylpentane 563-564, 574
2,4-Dimethylpentane 563-564, 571, 574
Dimethylpentyltin 461
3,6-Dimethylphenanthrene 465
2,3-Dimethylphenol 464
2,4-Dimethylphenol 455, 462, 464, 466, 504
2,5-Dimethylphenol 464
2,6-Dimethylphenol 464
3,4-Dimethylphenol 464
Dimethyl phthalate 445, 462-463
Dimethyl sulfide 474, 526, 554-556, 566-567
Dimethyl sulfoxide (DMSO) 526-527, 539, 549
Dimethyl-tetrachloro-terephthalate (DCPA) 435, 438-439, 448, 451
2,5-Dimethylthiophene 554
Dimethyltryptamine 545
2,4-Dinitroaniline 529
2,2'-Dinitrobiphenyl 465
2,7-Dinitrofluorene 465
4,6-Dinitro-2-methylphenol 462
1,3-Dinitronaphthalene 465
1,5-Dinitronaphthalene 465
2,4-Dinitrophenol 455,462-464, 466, 504, 530
2,5-Dinitrophenol 464
2,4-Dinitrotoluene 445, 462
2,6-Dinitrotoluene 445, 462
Di-n-octyl phthalate 462-463
Dinonyl phthalate 463
Dinoseb 439, 464
1,3-Dioxalane 519
1,4-Dioxane 442, 477, 519, 524-526, 535, 550, 552, 568
Diphenamid 445, 452-453
Diphenhydramine 544
Diphenylaniline 510
9,10-Diphenylanthracene 465
Diphenyl isophthalate 463
Diphenyl oxide 482-483
Diphenyl phthalate 463
Diphenylpyraline 544
Dipropylene glycol 519-520
Dipropyl ether 575
Disulfoton 445, 452
Diuron 453

cis-13,16-Docosadienoic acid methyl ester....497-498
cis-4,7,10,13,16,19-Docosahexaenoic acid methyl ester....497-498
Dodecahydrotriphenylene....465
γ-Dodecalactone....482-483
Dodecane....197, 199-200, 523, 552-553, 568
n-Dodecane....197, 208, 557, 571-572
Dodecanoic acid....494
Dodecanal....489
Dodecanol....482-483
n-Dotriacontane....572
Doxylamine....541, 544
Droperidol....546
Dursban (Chlorpyrifos)....445-446

E

cis-11,14-Eicosadienoic acid methyl ester....497-498
Eicosane....482
n-Eicosane....572
cis-5,8,11,14,17-Eicosapentaenoic acid methyl ester....497-498
cis-8,11,14-Eicosatrienoic acid methyl ester....498
cis-11,14,17-Eicosatrienoic acid methyl ester....497-498
cis-11-Eicosenoic acid methyl ester....497-498
Elaidic acid methyl ester....497-498
Endosulfan I....434-435, 438, 440-441, 445, 447-452, 456-457
Endosulfan II....434-435, 438, 440-441, 445, 447-452, 456-457
α-Endosulfan....500
b Endosulfan....500
Endosulfan sulfate....434-435, 438, 440-441, 445, 447-452, 456-457, 500
Endrin....434-435, 438, 440-441, 445, 447-452, 456-457
Endrin aldehyde....434-435, 438, 440-441, 445, 447-452, 456-457
Endrin ketone....434-435, 440-441, 445, 447, 449-451, 456-457
Ephedrine....536
Epiandrosterone (*trans*-androsterone)....548
Epichlorohydrin....442, 519
Eptam....454
EPTC....445, 452-453
Erucic acid methyl ester....497-498
Erythritol....494
Esfenvalerate....446
Estazolam....536
17-α-Estradiol....548
β-Estradiol....548
Estriol....548
Estrone....548
Ethane....534, 558-560, 563-566, 571, 576
Ethanol....442, 478, 492-493, 501, 505, 523-528, 535, 538-539, 549-551, 556, 570-571, 575
Ethchlorvynol....546
Ethinamate....546
2-(Ethlamino)-ethanol....506
Ethoprop....445, 452-453
Ethosuximide....543
Ethotoin....544
2-Ethoxyethanol (Cellosolve)....501, 505, 507, 535, 539
2-Ethoxyethyl acetate....507, 517-518
bis(2-ethoxyethyl) phthalate....463
Ethyl acetate....551
Ethyl acelytene....534
Ethyl acetate....442, 477-478, 482-483, 492-493, 517-518, 524-528, 535, 539, 549-550
Ethyl acrylate....517-518, 526-528
Ethyl alcohol....507
Ethyl and dimethyl thiophenes....568
Ethylbenzene....429, 442, 444, 468-469, 471, 473, 477, 503, 514-516, 523, 532, 539, 549, 552-553, 563-564, 568-569, 571, 574, 576
Ethylbenzene-d10....571
Ethyl benzoate....493, 517-518
2-Ethyl-1-butanol....505
Ethyl butanonate....478
Ethyl butyrate....482-483, 493, 518
Ethyl caprate....478
Ethyl caproate....518
Ethyl caprylate....478
Ethyl cellosolve....525
Ethyl decanoate....482-483
Ethyl disulfide....554
Ethyl dodecanoate....482-483
Ethylene....534, 553, 559-560, 563-565, 576
Ethylene/acetylene....566
Ethylenediamine....511
Ethylene glycol....501, 505, 519-522, 531, 549
Ethylene glycol/monoacetate....507
Ethylene glycol monobutyl ether....519-520
Ethylene glycol monoethyl ether....519-520
Ethylene glycol/monoformate....507
Ethylene glycol monomethyl ether....519-520
Ethylene glycol phenyl ether....522
Ethylene oxide....504, 507, 531, 569
Ethyl ether....442, 519, 524, 550
Ethyl formate....492, 507, 517-518, 524, 549
Ethyl heptanoate....482-483
Ethyl hexadecanoate....482-483
Ethyl hexanoate....482-483
2-Ethyl hexanoic acid....435
2-Ethyl-1-hexanol....492, 501, 505
bis-2-ethylhexyl adipate....445
bis(2-ethylhexyl) phthalate....445, 462-463
Ethyl isovalerate....482-483
Ethyl mercaptan....554-556, 566-567
Ethyl methacrylate....442, 444, 471, 528
Ethyl methyl sulfide....554
Ethylmorphine....537
Ethyl nonanoate....482-483
Ethyl octadecanoate....482-483
Ethyl octanoate....482-483
Ethyl parathion....500
Ethyl pentadecanoate....482-483
Ethyl pentanoate....482-483
a-Ethylphenethyl alcohol....501, 505
b-Ethylphenethyl alcohol....501, 505
2-Ethylphenol....530
4-Ethylphenol....530
Ethyl-3-phenyl oxiran carboxylate....493
Ethyl propanoate....478
Ethyl propionate....482-483, 517-518, 527-528
Ethyl-*tert*-butyl ether (ETBE)....429, 442, 556, 570, 575
Ethyl tetradecanoate....482-483
2-Ethylthiophene....554
4-Ethyltoluene....477
m-Ethyltoluene....552, 568
p-Ethyltoluene....552, 568
Ethyl undecanoate....482-483
Ethyl valerate....518
Ethyl vinyl ether....519
Etridiazole....435, 438, 448, 451
Eucalyptol....480-481
Eugenol....485, 487
Eugenyl acetate....482-483
Eugenyl methyl ether....483
Evernyl....482

F

Faneosolacetate....490
Farnescene....491
β-Farnesene....480
trans-β-Farnesene....479, 481, 490
Farnesol....487
Farnesol 1....487
Farnesyl acetate....491
Fenamiphos....445-446, 452
Fenarimol....445, 452
Fenchone....487
Fenchyl acetate....482
Fenitrothion....486, 500
Fentanyl....540, 545
Fenthion....486
Fenvalerate....446
Florazone....482-483
Flunitrazepam....141, 536, 539-540
Fluoranthene....431-432, 458, 462, 465
Fluorene....431, 445, 458, 462, 465
Fluorobenzene....442, 444, 468-469, 471, 514-515
2-Fluorobiphenyl....462
2-Fluorophenol....462
Flurazepam....540, 542
Fluridone....445, 452-453
Fonofos....453
Formaldehyde....474, 477, 513
Formaldehyde-DNPH....513
Formaldehyde-PFBHA....514
Formic acid....435, 494, 507
Frambione (raspberry ketone)....482-483
Fucitol....493
Furan....519
Furfural....482-483, 512
Furfuryl alcohol....501, 505

G

Galactitol....493-494
Geranial....482-483, 488-489
Geranial acetate....491
Geraniol....482-483, 485, 487, 490, 493
cis-Geraniol....480
trans-Geraniol....487
Geranyl acetate....480, 482-483, 488, 490
Geranyl butyrate....483
Geranyl formate....482-483
Geranyl-2-methyl valerate....482
Geranyl tiglate....482-483
Germacrene-d....479-480, 489-491
Gesatamine (Atraton)....445
Glucitol....493
Glucuron acid....494
Glucuron acid-1,5-lacton....494
Glutethimide....540, 546
Glycidol....501, 505
3,7-Guaiadiene....482
α-Gurjunene....491

H

Halazepam....536, 540
Haloperidol....546
Halothane....532
Helium....476
Heneicosane....482
Heneicosanoic acid methyl ester....497-498
1,7-Hepatanediol....522
Heptachlor....434-435, 438, 440-441, 445, 447-452, 456-457
Heptachlor epoxide....434-435, 438, 440-441, 445, 447-452, 456-457
2,2',3,3',4,4',6-Heptachlorobiphenyl....445
Heptadecane....461
n-Heptadecane....572
Heptadecanoic acid methyl ester....497-498
Heptadec-1-ene....482
cis-10-Heptadecenoic acid methyl ester....497-498
Heptanal....478, 511-512
Heptane....516, 523, 539, 549, 552, 568, 576
n-Heptane....477, 524, 535, 550, 553, 563-564, 571-572
1,7-Heptanediol....519-520
1-Heptanethiol....554
Heptanoic acid....494, 507, 511
n-Heptanoic acid....435
1-Heptanol....458, 501, 505
2-Heptanol....501, 505
3-Heptanol....501, 505
2-Heptanone....512
3-Heptanone....512
4-Heptanone....512
cis-4-Hepten-1-ol....501, 505
trans-2-Hepten-1-ol....501, 505
Hercolyn D (tetrahydro & dihydro methyl abietate)....482
Hexabromobenzene (HBB)....438, 448, 451

Hexabromobiphenyl....446
Hexachlorobenzene....435, 445, 447-448, 451, 456-457, 462
2,2',4,4',5,6'-Hexachlorobiphenyl....445
Hexachlorobutadiene....442, 444, 462, 468-469, 471, 477, 502, 522
Hexachloro-1,3-butadiene....473
β-Hexachlorocyclohexane (HCH)....500
δ- Hexachlorocyclohexane....500
γ- Hexachlorocyclohexane....500
Hexachlorocyclopentadiene....435, 438, 445, 448, 462, 502, 522
Hexachloroethane....442, 444, 462, 471, 502, 522
Hexachloropentadiene....447, 456-457
n-Hexadecane....197, 572
Hexadecanoic acid....494
2,4-Hexadienal....481
Hexanal....478, 511-512
Hexane....444, 471, 523-524, 526, 539, 549, 551, 570, 574, 576
n-Hexane....477, 524, 535, 550, 553, 558-560, 563-564, 571-572
1,6-Hexanediol....519-520
1-Hexanethiol....554
Hexanoic acid....511
Hexanol....197, 199-200, 482-483
1-Hexanol....478, 501, 505
2-Hexanol....501, 505
3-Hexanol....501, 505
2-Hexanone....444, 471, 477, 512
3-Hexanone....512
n-Hexatriacontane....572
Hexazinone....445-446, 452-454
cis-2-Hexene....563-564
trans-2-Hexene....563-564
cis-2-Hexen-1-ol....501, 505
cis-3-Hexen-1-ol....501, 505
Hexobarbital....537, 541
Hexyl acetate....483
Hexyl butyrate....480
Hexyl cinnamaldeyde....487
Hexyl cinnamic aldehyde....485
Hexylene glycol....482-483
Hexyl 2-ethylhexyl phthalate....463
1-Hexyl mercaptan....567
n-Hexyl mercaptan....567
Hexyl methacrylate....528
α-Humulene....488
Hydrocarbon....516
Hydrocodone....539, 541
Hydrogen sulfide (H2S)....474, 504, 534, 553-556, 558, 566-567
Hydroxy acetate....507
Hydroxy citronellal....482-483, 485, 487
4-Hydroxy-4-methyl-2-pentanone....501, 505
Hydroxyphenamate....541
Hydroxypropionitrile....442
Hydroxypropyl acrylate....528
Hydroxyzine....544

I

Ibogaine....540, 545
Ibuprofen....541, 547
Imipramine....542
Indan....571
Indeno[1,2,3-cd]pyrene....431, 433, 445, 458, 462
Inositol....493
Iodobenzene....514-515
Iodoform....502, 522
Iodomethane....444, 468, 471, 502, 522
Irgafos....533
Irganox....533
Isoamyl acetate....478, 493, 517-518
Isoamyl alcohol....478, 492
Isoamyl butyrate....493
Isoamyl mercaptan....567
Isoamyl salicylate....482, 484
Isoborneol....482-483-484, 491
Isobutane....558-566, 574
Isobutanol....442, 492-493, 501, 505, 525-528, 556, 570
Iso-butene....534
Iso-buteraldehyde....557
Isobutyl acetate....478, 482-483, 517-518, 524, 527-528
Isobutyl acrylate....527-528
Isobutyl alcohol....478
Isobutylaldehyde....478, 556
Isobutylbenzene....503, 514-515, 553
Isobutylene....559-562
Isobutyl mercaptan....567
Isobutyl propionate....527-528
Isobutyraldehyde....512, 575
Isobutyric acid....435, 494-495, 507-508, 511
Isocaproic acid....494, 507
Isodrin....435, 447, 451, 456-457
Isoeugenol....485, 487
trans-Isoeugenol....487
Isomenthol....481
Isomenthone....479, 481-483
d-Isomethone....489
a-Isomethyl ionone....487
Isonox 129....533
Isooctane....429, 523-524, 535, 551, 553, 563-564, 571
Isopentane....553, 558-566, 570-571
Isopentanoic acid....435
Isophorone....445, 462
Isoprene....561-564
Isopropanol....478, 501, 505, 524-525, 538, 550, 556
Isopropyl acetate....517-518, 524-525, 539
Isopropyl acrylate....527-528
Isopropyl alcohol....442, 477, 524, 549
Isopropyl amine (IPA)....506, 549
Isopropylbenzene (cumene)....442, 444, 468-469, 471, 503, 514-516, 553, 563-564, 568
Isopropyl ether....519
Isopropyl mercaptan....567
Isopropylmyristate....482 -483
2-Isopropylphenol....530
Isopropyltoluene....442
4-Isopropyltoluene....469
p-Isopropyltoluene....444, 468, 471
Isovaleraldehyde....556, 575
Isovaleric acid....494-495, 507, 511

J

Jasmolin I....461
Jasmolin II....461
cis-Jasmone....479, 490

K

Kelthane....435, 447, 456-457
Kepone....446
Ketamine....546
Ketimine....545
Krypton....557

L

Lactose....494
Lactulose....494
Lauric acid methyl ester....497-498
Lavandulol....480
Lavandulyl acetate....480
Levulinic acid....435
Lidocaine....540, 543, 546
Lignoceric acid methyl ester....497-498
Lilial....485, 487
Limonen....489
Limonene....479, 482-484, 487, 489-492
δ-Limonene....480-481, 488
Linalool....479, 482-485, 487-492
β-Linalool....480
Linalool acetate....480
cis-Linalool oxide....483
trans-Linalool oxide....482, 483
Linalyl acetate....482-484
Lindane....448
Linoleic acid methyl ester....497-498
Linolelaidic acid methyl ester....497-498
Linolenic acid methyl ester....497-498
γ-Linolenic acid methyl ester....497-498
Lofentanyl....545
Lorazepam....536, 539-540
Lormetazepam....536
Lyral....485
Lyral 1....487
Lyral 2....487
Lysergic acid diethylamide (LSD)....540, 545

M

β-Maaliene....481
Malathion....446, 486, 500
Manitol....494
Mannitol....493
Meclizine....544
Medazepam....536, 540
Menthofuran....481
Menthol....481, 484, 489
Menthone....481-483
Menthyl acetate....489
Meperidine....539, 542
Mephobarbital....537
Mepivacaine....543
Meprobamate....541, 546
Merphos....445, 452
Mescaline....545
Mesitylene....523
Mesityl oxide....525
Mesterolone....548
Methacrolein....512, 526-527
Methacrylic acid....435
Methacrylonitrile....442, 444, 471, 526-527
Methadone....539-540, 542
Methamidophos....486
Methamphetamine....536, 539, 542
Methandrostenolone....548
Methane....476, 526, 534-535, 553, 557-560, 563-566, 576
Methanol (MeOH)....478, 492-493, 501, 505-506, 513, 523-528, 535, 538-539, 549-551, 553, 556-557, 570, 575
Methapyrilene....541, 544
Methaqualone....540, 546
Methidathion....486
Methofuran....489
Methohexital....537
Methone....489-490
Methoprene....461
Methoxychlor....434-435, 438, 440-441, 445, 447-451, 456-457
2-Methoxyethanol (methyl Cellosolve)....501, 505, 526
bis(4-methoxyethyl) phthalate....463
2-Methoxy-5-methylaniline....529
1-Methoxy-2-propanol....539
Methsuximide....543
3-Methy-1-butanol....535
Methycyclohexane....535
Methyl acetate....517-518, 527-528, 535
Methyl acetylene....566
Methyl acrylate....442, 444, 471, 527-528
Methylamine....508
4-Methylaminorex....545
2-Methylanthracene....465
9-Methylanthracene....465
r-Methylansiole....490
Methyl arachidate....495
Methyl benzoate....483, 490-491, 517-518
2-Methyl butanal....511
2-Methylbutane....574
2-Methyl-1-butanol (active amyl alcohol)....493, 501, 505
2-Methyl-2-butanol (*tert*-amyl alcohol)....501, 505
3-Methyl-1-butanol (isoamyl alcohol)....493, 501, 505

3-Methyl-2-butanone 512, 535
2-Methyl-1-butene 571
2-Methyl-2-butene 559, 563-564, 571
3-Methyl-1-butene 561-564
trans-2-Methyl-2-butenoic acid 508
2-Methyl-3-buten-2-ol 501, 505
3-Methyl-2-buten-1-ol 501, 505
2-Methylbutyl acetate 517-518
2-Methylbutyl alcohol 482-483
3-Methylbutyl alcohol 482-483
Methyl-*tert*-butyl ether (MTBE) 429, 442, 444, 471, 519, 523, 539, 549, 556-557, 570-571, 575
Methyl butyrate 482-483
2-Methyl butyric acid 508
Methyl chavicol 485
3-Methylcholanthrene 465
2-Methyl-4-chloro-phenoxy acetic acid (MCPA) 439
Methylchlorophenoxy propionic acid (MCPP) 439
5-Methylchrysene 433
Methyl-cresol 482
Methyl-para-cresol 483
Methyl-ρ-cresol 491
Methylcyclohexane 539, 563-564, 574
Methylcyclopentane 553, 563-564, 571, 574
1-Methyl-1-cyclopentene 571
Methyl decanoate 518
Methyl-2,4-dichlorophenylacetate 439
Methyl diethanolamine (MDEA) 506
4-Methyl-2,5-dimethoxyamphetamine 536
2-Methyl-4,6-dinitrophenol 455, 463-464, 466, 504
Methyl disulfide 554
Methyl dodecanoate 518
Methyl eicosenoate 518
Methyl elaidate 495
Methylene chloride 442, 444, 468-469, 471, 473, 477, 502, 522, 524, 539, 549-550
4,4'-Methylenedianiline 529
Methylenedioxy-amphetamine (MDA) 536, 539, 542
3,4-Methylenedioxy-ethylamphetamine 536, 539, 542
Methylenedioxy methamphetamine (MDMA) 539, 542
3,4-Methylenedioxy methylamphetamine 536
Methyl ephedrine 536
1-Methyl-2-ethylbenzene 571
1-Methyl-3-ethylbenzene 571
1-Methyl-4-ethylbenzene 571
Methyl ethyl ketone (MEK) 524-525, 550, 556
Methyl ethyl sulfide 556
Methyl eugenol 485
2-Methylfluoranthene 465
Methyl formate 517-518, 525
3-0-Methylglucose 1 494
3-0-Methylglucose 2 494
Methyl heptadecanoate 495
2-Methylheptane 553, 563-564, 571
3-Methylheptane 563-564, 571
4-Methylheptane 553
Methyl heptin carbonate 485, 487
Methyl hexadecanoate 518
2-Methylhexane 563-564, 574
3-Methylhexane 563-564, 574
Methyl 2-hydroxydecanoate 495
Methyl 2-hydroxydodecanoate 495
Methyl 3-hydroxydodecanoate 495
Methyl 2-hydroxyhexadecanoate 495
Methyl 2-hydroxytetradecanoate 495
Methyl 3-hydroxytetradecanoate 495
Methyl g-ionone 485
α-Methyl ionone 484
Methyl isobutyl ketone 524-525, 539
Methyl laurate 495
Methyl mercaptan 474, 554-556, 566-567
Methyl methacrylate 442, 444, 471, 527-528
Methyl *cis*-9,10-methylene octadecanoate 495
Methyl *cis*-9,10-methyl hexadecanoate 495
Methyl 14-methylhexadecanoate 495
Methyl 12-methyltetradecanoate 495
Methyl monoethanolamine (MMEA) 506
Methyl myristate 495
1-Methylnaphthalene 465, 571
2-Methylnaphthalene 462, 465, 571
2-Methyl-5-nitroaniline 529
Methyl nonadecanoate 495
Methyl octadecanoate 518
Methyl octine carbonate 485, 487
Methyl oleate 495
Methyl palmitate 495
Methyl palmitoleate 495
2-Methylpantane 574
Methyl paraoxon 445
Methyl parathion 500
Methyl pentadecanoate 495
2-Methylpentane 429, 563-564, 571
3-Methylpentane 429, 523, 563-564, 571, 574
2-Methyl-2 pentanol 556
3-Methyl-3-pentanol 505
4-Methyl-2-pentanol 501, 505
2-Methyl-3-pentanone 512
4-Methyl-2-pentanone (MIBK) 444, 471, 477, 512
2-Methyl-1-pentene 563-564, 571
4-Methyl-1-pentene 563-564
bis(4-methyl-2-pentyl) phthalate 463
2-Methylphenol 462, 464
3-Methylphenol 464
4-Methylphenol 462, 464
a-Methylphenyl alcohol 501
5-Methyl-5-phenylhydantoin 543
2-Methyl-1-propanethiol 554-556, 566
2-Methyl-2-propanethiol 554-555, 566
2-Methyl-1-propanol (isobutanol) 575
2-Methyl-2-propanol (*tert*-butanol) 539, 575
Methyl propionate 517-518, 527-528
1-Methyl-1-propnaethiol 555, 566
1-Methyl-3-propylbenzene 571
1-Methyl-1-propyl mercaptan 567
2-Methyl-1-propyl mercaptan 567
2-Methyl-2-propyl mercaptan 567
2-Methyl pyridine 432
1-Methyl-2-pyrrolidine 510
1-Methyl-2-pyrrolidinone 526-527
n-Methylpyrrolidone 539
Methyl stearate 495
4-Methylstyrene 514-515
α-Methylstyrene 514-516, 552, 568
Methyl sulfide 534
17α-Methyltestosterone 548
Methyl tetradecanoate 518
2-Methylthiophene 554
3-Methylthiophene 554
Methyl thiophenes 568
Methyl tridecanoate 495
Methyltripentyltin 461
Methylundecanoate 495
Metolachlor 438, 445, 452-453
Metribuzin 438, 445, 452-453
Mevinphos 445, 452
MGK 264 ....445, 452
Endo-MGK 264 461
Exo-MGK 264 461
Mirex 435, 446-447, 451, 456-457
Molinate 445, 452-453
6-Monoacetylmorphine 537
Mono-ethanolamine (MEA) 506
Mono ethylene glycol 506
Monuron 453
Morphine 537, 541, 546
Musk ketone 484
Musk T (ethylene brassylate) 482-483
Musk xylene 484
Myrcene 479, 482-484, 488-490
β-Myrcene 480-481
Myristic acid methyl ester 497-498
Myristoleic acid methyl ester 497-498

N

Naphthalene 197, 199-200, 429, 431, 442, 444, 458, 462, 465, 468-469, 471, 523, 553, 571
Naphthalene-d8 ....462-463, 571
1-Naphthol 530
Napropamide 445, 452-453
Nefopam 543
Neomenthol 484, 489
Neon 476, 557
Neral 482-483, 487-489
Nerol 481
Nerol acetate 480
cis-Nerolidol 482
trans-Nerolidol 482
Nervonic acid methyl ester 497-498
Neryl acetate 482-483, 488
Nicotinamine 536
Nicotine 539-541, 547
Nitrazepam 141, 536, 539
2-Nitroaniline 462, 510, 529
3-Nitroaniline 462, 510, 529
4-Nitroaniline 462, 510, 529
Nitrobenzene 442, 444, 462, 471, 514-515
Nitrobenzene-d5 462
2-Nitrobiphenyl 465
3-Nitrobiphenyl 465
4-Nitrobiphenyl 465
Nitrofen 435
Nitrogen 476, 504, 532, 557
Nitromethane 535
1-Nitronaphthalene 465
2-Nitronaphthalene 465
Nitrophen 446
2-Nitrophenol 455, 462, 464, 466, 504, 530
3-Nitrophenol 464
4-Nitrophenol 439, 455, 463-462, 464, 466, 504
Nitropropane 525
2-Nitropropane 442, 444, 471
n-Nitrosodimethylamine 432, 462, 463
n-Nitrosodiphenylamine 462
n-Nitroso-di-n-propylamine 462
2-Nitrotoluene 503, 514-515
3-Nitrotoluene 503, 514-515
4-Nitrotoluene 503, 514-515
cis-Nonachlor 448
trans-Nonachlor 435, 445, 447-448, 456-457
Nonadecane 483
Nonadec-1-ene 482-483
γ-Nonalactone 482-483
Nonanal 488-489
Nonane 523, 552, 568, 574, 576
n-Nonane 458, 553, 563-564, 571-572
1,9-Nonanediol 519-520, 522
Nonanol 492
1-Nonanol 501, 505
Nonyl aldehyde 512
n-Nonylamine 509-510
Nootkatone 489
Norcodeine 537
Nordazepam 536
Norethandrolone 548
Norflurazon 445-446, 452-453
Normorphine 537
19-Nortestosterone (Nandrolone) 548
19-Nortestosterone-17-decanoate 548
19-Nortestosterone-17-propionate 548

O

trans-Ocimene 479
β-*cis*-Ocimene 479-480, 489-490
β-*trans*-Ocimene 480
1,2,3,4,6,7,8,9-OCDF 432
1,2,3,4,6,7,8,9-Octachlorodibenzodioxin (OCDD) 432
2,2',3,3',4,5',6,6'-Octachlorobiphenyl 445
n-Octacosane 572
Octadecane 461

n-Octadecane....572
Octadecanoic acid....494
Octanal....478, 488-489, 511
Octane....523, 552, 568, 574, 576
n-Octane....458, 553, 563-564, 571-572
1,8-Octanediol....519-520
Octanoic acid....494, 511
Octanol....482-483, 488, 492
1-Octanol....501, 505
3-Octanol....479, 489-490
3-Octanone....458, 480
1-Octene....458
1-Octen-3-ol....480, 489
Octen-1-ol acetate....480
Octyl acetate....482-483
3-Octyl acetate....479, 490
Octyl aldehyde....512
n-Octylamine....509-510
n-Octyl mercaptan....567
Oleic acid methyl ester....497-498
Omethoate....486
Ordram....454
Ortho xylene....532
Oxadiazon....454
Oxazepam....536, 539-540
Oxazopam....536
Oxychlordane....446
Oxycodone....141, 539
4,4′-Oxydianiline....529
Oxygen....476, 557
Oxymetholone....548
Oxymorphone....541

P

Paarlan....454
Palmitic acid methyl ester....497-498
Palmitoleic acid methyl ester....497-498
Paraldehyde....442
Parathion....446, 486
Parathion-methyl....486
Pebulate....452-453
Pentaborane....533
Pentachlorobenzene....514-515
2,2',3',4,6-Pentachlorobiphenyl....445
Pentachloroethane....442, 444, 471, 502, 522
Pentachloronitrobenzene....435, 438, 447, 451, 456-457
Pentachlorophenol....439, 445, 455, 462-464, 466, 504
n-Pentadecane....197, 557, 572
Pentadecanoic acid methyl ester....497-498
10-Pentadecenoic acid methyl ester....497-498
cis-1,3-Pentadiene....561-562
trans-1,3-Pentadiene....561-562
Pentafluorobenzene....442, 444, 471
Pentafluoroethane....454
Pentamethylbenzene....571
Pentamethyl disiloxane....533
Pentanal....511
Pentane....502, 517, 526, 570, 574, 576
i-Pentane....576
n-Pentane....553, 558-566, 570-572
1,2-Pentanediol....458
1,5-Pentanediol....519-520
2,3-Pentanedione (acetyl propionyl)....478, 482-483
1-Pentanethiol....554
n-Pentanoic acid....435
1-Pentanol....501, 505, 539
2-Pentanol....478, 501, 505
3-Pentanol....478, 501, 505
2-Pentanone....442, 512, 524
3-Pentanone....512
Pentene-1....559, 561-562
1-Pentene....559-560, 563-564, 571
cis-2-Pentene....559, 561-564
trans-2-Pentene....559, 561-564
4-Pentenoic acid....508
trans-2-Pentenoic acid....508
trans-3-Pentenoic acid....508
1-Penten-3-ol....501, 505
2-Penten-1-ol....501, 505
Pentobarbital....537, 541
Pentyl ether....519
1-Pentyl mercaptan....567
cis-Permethrin....435, 438, 445, 447-448, 451, 456-457
trans-Permethrin....435, 438, 445, 447-448, 451, 456-457
Perthane....435, 447, 456-457
Perylene....465
Perylene-d12....445-446, 462-463
α-Phellandrene....488
Phenacetin....536, 541
Phenanthrene....431, 445, 458, 462, 465
Phenanthrene-d10....445, 462-463
Phencyclidine (PCP)....539-540, 542, 545
Phenethylalcohol....492
Pheniramine....544
Phenmetrazine....541
Phenobarbital....537, 540-541, 543-544
Phenol....197, 199-200, 430, 455, 462, 464, 466, 504, 530
Phenol-d5....462
2-Phenoxyethanol....501, 505
Phensuximide....543
Phentermine....536, 539
Phenyl acetaldehyde....485, 487
Phenylacetone....536
Phenylacetylene....552, 568
9-Phenylanthracene....465
Phenyl ephedrine....536
Phenylethyl acetate....478, 482
Phenylethylamine....510
Phenyl ethyl cinnamate....482-483
Phenylethylmalonamide....543-544
Phenylethyl tiglate....482-483
2-Phenylnaphthalene....465
Phenyltoloxamine....544
Phenytoin....543-544
Phorate....453
Phosphine....533
Picloram....439
4-Picoline....458
α-Pinene....479-483, 489-491
β-Pinene....479, 481-484, 488-491
Piperazine....511
Piperitone....489
Pirimiphos-methyl....486
Polyethylene glycol....521
Polymethoxyflavones....489
Prazepam....536, 540
Prebane (Terbutryne)....445
Primidone....543-544
Procaine....541, 543, 546
Progesterone....548
Promazine....544
Promethazine....544
Prometon....445, 452-453
Prometryn....452
Prometryne....445-446, 453
Promofos....500
Pronamide....445, 452-453
Propachlor....435, 438, 445, 447-448, 451, 453-454, 456-457
Propadiene....534, 559-562
Propanal....477
Propane....517, 558-566, 571, 574, 576
1,3-Propanediol....519-520
1,2-Propanediol (propylene glycol)....519-520
1-Propanethiol....554-555, 566
2-Propanethiol....554-556, 566
Propanil....453
Propanoic acid....511
Propanol....474
1-Propanol....442, 501, 505, 535, 538-539, 549, 570, 575
1-Propanol....478, 526
2-Propanol....526, 535, 539, 570
n-Propanol....492-493, 524-525, 550, 556
2-Propanone....570
Propargyl alcohol....442
Propazine....445-446, 452-454
Propene....477
2-Propen-1-ol (allyl alcohol)....501, 505
Propiolactone....442
Propiomazine....546
Propionaldehyde (propanol)....512, 556, 575
Propionic acid....435, 492, 494-495, 507
1-Propionic acid....458
Propionitrile....442, 444, 471, 510, 526-527
Proposyphene....542
Propyl acetate....478, 517-518, 535
Propylbenzene....442, 514-516, 523, 552-553, 568
n-Propylbenzene....444, 458, 468-469, 471, 503, 516, 563-564, 568, 571
Propyl benzoate....517-518
Propyl butyrate....518
Propyl caproate....518
Propylene....517, 553, 555, 559-566, 576
Propylene glycol....501, 505
Propylene glycol dimethyl ether....519-520
Propyl ether....519, 556
Propyl formate....517-518
1-Propyl mercaptan....567
2-Propyl mercaptan....567
n-Propyl mercaptan....567
2-Propyl pentanoic acid....435
Propyl propionate....517-518
Propyl valerate....518
Propyne (methylacetylene)....559-564
2-Propyn-1-ol (propargyl alcohol)....501, 505
Prowl....454
Psilocin....545
Pulegone....489
Pyrazole....510
Pyrene....431, 445, 458, 462, 465
Pyrene-d10....445
Pyrethrin I....461
Pyrethrin II....461
Pyridazine....510
Pyridine....442, 462, 510, 524, 526-527, 535, 550
Pyrilamine....544
Pyrimidine....510
Pyrimiphos ethyl....500
Pyrimiphos methyl....500
Pyrithyldione....546
Pyrrobutamine....541

Q

Quinine....546

R

Rhamnitol....493-494
Rhamnose 1....494
Rhamnose 2....494
Ribitol....493-494
Ribose 2....494
Rosatol (rosetone)....483
Rose oxide, *cis*-rose....482-483
Rose oxide, *trans*-rose....482-483

S

Sabinene....479, 482, 488-490
trans-Sabinene hydrate....479, 489-490
Salicylamide....543
α-Santoloene....480
Secbumeton....453
Secobarbital....537, 541
Selenide....533
Sencor....454
α-Sinensal....489
β-Sinensal....489
Simazine....438, 445, 448, 452-454
Simetryn....445, 452-453
Sorbitol....494

Stanozolol....548
Stearic acid methyl ester....497-498
Stigmasterol....548
Stirofos....452
Strawberry aldehyde....493
Strychnine....539, 546
Styrene....442, 444, 468, 471, 473, 477, 503, 514-517, 523, 532, 552, 563-564, 568
Styrene dimer....517
Styrene oxide....514-515
Styrene trimer....517
Sucrose....494
Sufentanyl....545
Sulfallate....453
Sulfur dioxide....504, 534
Sulpiride....546
Sutan....454

T

Talbutal....537, 546
Tebuthiuron....445, 452
Temazepam....141, 536, 539-540
Tenocyclidine (TCP)....545
Terbacil....445, 452-454
Terbufos....445, 452-453
Terbus sulfone....446
Terbuthylazine....453
Terbutryn....452-453
Terphenyl-d14....462
Terpinene....489, 491
α-Terpinene....479, 488-490
γ-Terpinene....479, 481-483, 490, 492
Terpinen-4-ol....479-480, 482-483, 488-490, 492
α-Terpineol....482-484, 488-490, 491-492
α-Terpinol....480
Terpinolene....479, 483, 488, 490
γ-Terpinolene....489
Terrazole....445, 447, 456-457
Testosterone....548
Tetraborane....533
Tetrabutyltin....461
Tetracaine....543
1,2,4,5-Tetrachlorobenzene....514-515
2,2',4,4'-Tetrachlorobiphenyl....445
2,3,7,8-Tetrachlorodibenzodioxin (TCDD)....432
2,3,7,8-Tetrachlorodibenzofuran (TCDF)....432
1,1,1,2-Tetrachloroethane....442, 444, 468-469, 471, 502, 522
1,1,2,2-Tetrachloroethane....442, 444, 468, 471, 473, 477, 502, 522
Tetrachloroethene....442, 444, 468-471, 473, 477, 522
Tetrachloroethlyene....436, 470
2,3,4,5-Tetrachlorophenol....430, 464
2,3,4,6-Tetrachlorophenol....430, 464
2,3,5,6-Tetrachlorophenol....430, 464, 466
Tetrachloro-m-xylene....434-435, 440-441, 447, 451, 456-457, 460
2,4,5,6-Tetrachloro-m-xylene....449-450
Tetrachlorvinphos (Stirifos)....445
n-Tetracontane....572
n-Tetracosane....572
Tetradecane....571
n-Tetradecane....197, 557, 572
Tetradecanoic acid....494
Tetraethylenepentamine....511
1,1,1,2-Tetrafluoroethane....454
1,1,2,2-Tetrafluoroethane....454
Tetrahydofuran....526
Tetrahydrocannabinol....539
δ9-Tetrahydrocannabinol....548
1,2,3,4-Tetrahydrofluoranthene....465
Tetrahydrofuran (THF)....444, 471, 477, 519, 524, 539, 550
Tetrahydropyran....519
Tetrahydrothiophene....554
1,2,3,5-Tetramethylbenzene....571
1,2,4,5-Tetramethylbenzene....553, 571
Tetrapentyltin....461
Thenyldiamine....541
Thiamylal....537
Thiazopyr....446
Thioacetamide (TAA)....570
4,4'-Thiodianiline....529
Thiopental....537
Thiophene....554-556, 566-568
Thioridazine....544
Thonzylamine....544
Threhalose....494
Threitol....494
Thujone....487
α-Thujone....482, 488
β-Thujone....488
Tillam (Pebulate)....445, 454
Tinuvin P....533
α-Tocopherol....545
β-Tocopherol....545
δ-Tocopherol....545
γ-Tocopherol....545
Tolban....454
o-Tolidine....529
m-Tolualdehyde....512
o-Tolualdehyde....512
p-Tolualdehyde....512
Toluene....197, 199-200, 429, 442, 444, 468-469, 471, 473, 477, 503, 514-517, 523-525, 532, 535, 539, 549-550, 552-553, 561-564, 568-569, 571, 574, 576
Toluene-d8....442, 473
Tonalid....482-484
Trazodone....539
Treflan....454
γ-Trepinene....488
Triademefon....452
Triadimefon....445
Triazolam....536, 540
Tribromoacetic acid....467
2,4,6-Tribromophenol....462
Tributylpentyltin....461
Trichloroacetic acid....467
Trichloroacetonitrile....436, 470
2,4,5-Trichloroaniline....529
1,2,3-Trichlorobenzene....442, 444, 468-469, 471, 514-515
1,2,4-Trichlorobenzene....442, 444, 462, 468-469, 471, 473, 477, 514-515
1,3,5-Trichlorobenzene....514-515
2,4,5-Trichlorobiphenyl....445
Trichloroethane....524
1,1-Trichloroethane....549
1,1,1-Trichloroethane....436, 442, 444, 468-471, 473, 477, 502, 522, 535
1,1,2-Trichloroethane....436, 442, 444, 468-469, 471, 473, 477, 502, 522
Trichloroethene....442, 444, 468-471, 473, 477, 522
Trichloroethylene....436, 470, 524, 526, 535, 550
Trichlorofluoromethane....442, 444, 454, 468-469, 471, 473, 477
Trichloromethane....526
Trichloromethyl silane....533
2,3,4-Trichlorophenol....430, 464, 466
2,3,5-Trichlorophenol....430, 464, 466
2,3,6-Trichlorophenol....430, 464, 466
2,4,5-Trichlorophenol....430, 462, 464, 466
2,4,6-Trichlorophenol....430, 455, 462, 464, 466, 530
3,4,5-Trichlorophenol....430, 464
2,4,5-Trichlorophenoxyacetic acid....439
1,2,3-Trichloropropane....436, 442, 444, 467-468, 471, 502, 522
1,1,1-Trichloropropanone....470
1,1,1-Trichloro-2-propanone....436
1,1,2-Trichlorotrifluoroethane....502, 522
1,1,2-Trichloro-1,2,2-trifluoroethane....454, 473, 477
Tricosanoic acid methyl ester....497-498
Tricyclazole....445, 452-453
Tridecane....552-553, 568
n-Tridecane....197, 557
Tridecanoic acid methyl ester....497-498
Triethanolamine (TEA)....506
Triethylamine....510, 526-527
Triethylene glycol....521
Triethylene glycol dimethyl ether....519-520
Triethylenetetramine....511
1,1,1-Trifluoroethane....454
Trifluoromethane....454
Trifluorotoluene....468
α,α,α-Trifluorotoluene....429
Triflupromazine....544
Trifluralin....435, 438, 445, 447-448, 451, 456-457
Trimethylamine....508
2,4,5-Trimethylaniline....529
1,2,3-Trimethylbenzene (hemimellitene)....429, 514-515, 553, 571, 574, 576
1,2,4-Trimethylbenzene (pseudocumene)....429, 442, 444, 468-469, 471, 473, 477, 514-515, 523, 553, 563-564, 571
1,3,5-Trimethylbenzene (mesitylene)....429, 442, 444, 468-469, 471, 473, 477, 514-515, 563-564, 571
Trimethylchloro silane....533
3,5,5-Trimethylhexanol....482-483
2,3,3-Trimethylpentane....553, 571
2,3,4-Trimethylpentane....563-564
2,2,4-Trimethylpentane....477
2,3,5-Trimethylphenol....530
Trimethyl phosphate....458
Trimipramine....540
2,4,6-Trinitrophenol....504
1,3,5-Trioxane....478
Tripelennamine....544
Triphenyl phosphate....445-446, 486
Triprolidine....544

U

Undecane....523, 552, 568, 574
n-Undecane....197, 208, 553, 571-572
Undecanoic acid methyl ester....497-498

V

Valencene....489
Valeraldehyde....512, 556, 575
Valeric acid....494, 507, 508, 511
Valerolactone....508
Vanillin....487
Verapamil....539
Vernam....454
Vernolate....445, 452-453
Vertenex....482-483
Vinclozolin....500
Vinclozoline....446
Vinyl acetate....477, 517-518
Vinyl chloride....442, 444, 468-469, 471, 473, 477
Vinyl-trimethyl silane....533
Viridiflorol....479, 489-490

W

Water (H2O)....507, 553, 558, 570

X

Xenon....557
m-Xylene....429, 442, 444, 468-469, 471, 473, 477, 503, 514-516, 523, 525, 532-533, 552, 563-564, 568-569, 571, 574, 576
o-Xylene....429, 442, 444, 468-469, 471, 473, 477, 503, 514-516, 523, 525, 532, 539, 549, 552-553, 563-564, 568-569, 571, 574, 576
p -Xylene....429, 442, 444, 468-469, 471, 473, 477, 503, 514-516, 523, 525, 532, 552-553, 563-564, 568-569, 571, 574, 576
m,p-Xylene....429, 539, 549
2,3-Xylenol....530
2,4-Xylenol....530
2,5-Xylenol....530
2,6-Xylenol....530
3,4-Xylenol....530
3,5-Xylenol....530
Xylose 1....494
Xylose 2....494

Ordering Information

Easy Ordering Terms and Conditions

Discounts and Delivery

Agilent Technologies specializes in fast delivery. In the US, if you call before 2 PM EST, we will ship your order that day. You may also request overnight express delivery before 6 PM EST and you will have your order the next day. Volume discounts on a variety of individual products are offered when the entire quantity is shipped to one address at one time.

A shipping and handling fee will be added to your order unless the purchase is over $2000 US for orders place online or over $4000 for orders place via phone. Special shipping (i.e., overnight in the US) is available in most regions at an additional cost.

Agilent is required to collect all state and local sales taxes unless the buyer's tax-exempt certificate is on file with Agilent Technologies. Please be prepared to provide a copy if it is not on file, when placing your order.

Please check with your Agilent Customer Service Representative, local Authorized Distributor, or the Agilent website for current prices, special offers, promotions and discounts when placing your order.

Satisfaction Guaranteed

If you are not satisfied with your Agilent product within the first 60 days, you may return your purchase in its original condition for a full refund or credit. A return policy statement is included in every Agilent shipment and posted under Product Information on the website. In the US and Canada, please call for a Return Authorization form and return instructions at **1-800-227-9770**. If your Agilent product was purchased from a distributor, please contact the distributor.

Shipping Damages

If items are damages in transit, please follow the instructions below:

- If a shipment is visibly damaged upon arrival, do not accept it until the person making the delivery has endorsed the bill of lading with statement for the extent of the damage.
- If any damage is found after unpacking, retain all cartons and inner packaging and immediately request an inspection from the carrier.
- Notify the Agilent Customer Contact Center at **1-800-227-9770** about the damaged shipment so that we can make the appropriate sales adjustment and/or provide you with return instructions (Sales order number, product number and quantity damaged will be needed).

Easy Ways To Order

- Phone: **1-800-227-9770** (option 1, 1) in the US and Canada – Mon-Fri, 8AM to 8PM EST
- Fax: **1-302-633-8901** in the US
- Email: **cag_sales-na@agilent.com** in the US and Canada
- Online: **www.agilent.com/chem** in the US and Canada

Payment Options

- In the US, Visa, MasterCard, Discover and American Express are accepted with a minimum order of $20 (not applicable in all countries).
- Email ePay@agilent.com to make an electronic payment using the ACH/EFT (Automated Clearing House/Electronic Funds Transfer) method.
- Establish a charge account through your Agilent Customer Service Representative or Your Local Agilent sales office. An account number will be assigned to you for charging your purchases. Payment terms are net 30 days from the invoice date. All orders are subject to credit approval.

We will be happy to supply a price quote via, phone, email or fax if you need it in writing.

Warranties

All Agilent Technologies products in this catalog are designed and manufactured to stringent standards under the Agilent quality system registered to ISO 9001. At Agilent, we back every product with a 90-day warranty and a money-back guarantee. If Agilent receives notice of defects during the warranty period. Agilent shall, at its option, either repair or replace products which prove to be defective. If Agilent is unable, within a reasonable time, to repair or replace any product to a condition as warranted, the buyer shall be entitled to a refund of the purchase price upon return of the product to Agilent. The warranty period for each product begins on the day of shipment.

This warranty shall not apply to any defect, failure, or damage caused by improper use or improper or inadequate maintenance or care. This warranty is exclusive and no other warranty, whether written or oral, is expressed or implied. Agilent specifically disclaims the implied warranties of merchantability and fitness for particular purposes. The remedies provided herein are the buyer's sole and exclusive remedies. In no event shall Agilent be liable for direct, indirect, special, incidental, or consequential damages (including loss of profits) whether based on contract, tort, or any other legal theory.

For more information

Buy online:
www.agilent.com/chem/store

Contact us:
www.agilent.com/chem/contactus

This information is subject to change without notice.

© Agilent Technologies, Inc. 2012
Printed in Canada October 31, 2012
5991-1058EN

Scan the QR code
with your smartphone
for more information



The Measure of Confidence

Agilent Technologies