

GC AND GC/MS

Your Essential Resource for Columns & Supplies



The Measure of Confidence

Agilent Technologies


Agilent J&W GC columns

The story behind Agilent J&W GC Columns

In 2000, Agilent Technologies, the inventor of fused silica GC tubing, merged with J&W Scientific, the creator of the first GC stationary phase made from cross-linked siloxane polymers. In 2010, Agilent acquired Varian adding PLOT, Select, VF, CP-Sil and packed to the existing Ultra Inert, High Efficiency, LTM, PAH, UltiMetal, and Custom GC columns. Our foundation of GC expertise, combined with these vital acquisitions, we have built Agilent J&W into the most extensive and innovative GC column offering in the world.

Put 40 years of Agilent quality and innovation behind your every separation

Agilent J&W offers the broadest portfolio of the most innovative GC columns in the world, with over 3700 part numbers. Our portfolio offers the best inertness for acids/bases/mixed functional compounds, the lowest bleed levels and the tightest column-to-column reproducibility. So when you put industry-leading Agilent J&W GC columns to work in your lab, you can have the utmost confidence in your column, and in every separation.

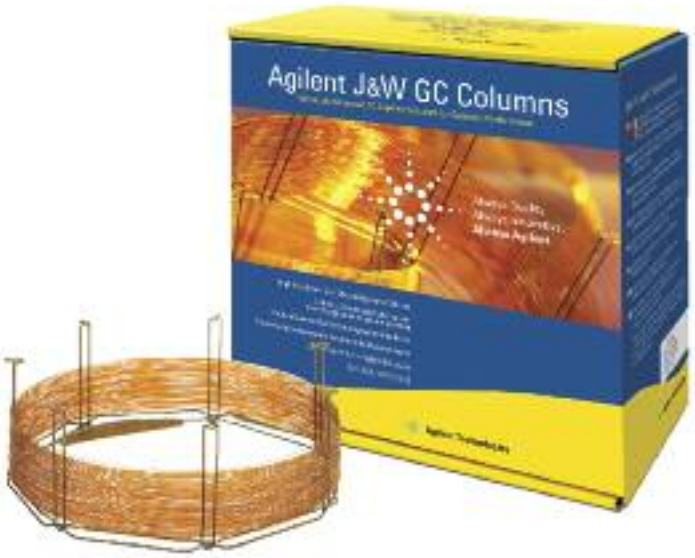

The most inert and lowest bleed columns for sensitivity and performance



Agilent J&W columns have the widest range of standard, GC/MS and Ultra Inert stationary phases proven to deliver consistent column inertness and exceptionally low column bleed with high upper temperature limits, ensuring accurate peak identification and quantification. Column bleed can decrease spectral integrity, reduce uptime, and shorten column life. Column activity contributes to severe peak tailing, as well as compound loss or degradation for active compounds (e.g. acids and bases), leading to inaccurate quantification.

Better precision for better results

Agilent J&W columns adhere to tight retention factor (k) specifications, promoting consistent retention and separation. They also feature narrow retention indexes and a high number of theoretical plates per meter, ensuring narrow peaks and improving the resolution of closely eluting peaks.

The industry's tightest quality control specifications

Agilent's industry-leading testing ensures the most reliable qualitative and quantitative results, and unmatched column-to-column reproducibility, for your most challenging compounds. Offering the industry's only Ultra Inert testing, we test each column for peak height ratios and tailing for acids, bases, and other chromatographically demanding compounds so you can have utmost confidence in your trace-level separations.

And, with Agilent's industry-leading instruments, services, global technical support, and quick shipping, Agilent's whole solution provides you with even more confidence in your column, and in your every separation.

To learn more about Agilent J&W GC columns please visit **www.agilent.com/chem/mygccolumns.**

Agilent J&W LTM Column Modules

Agilent J&W LTM Column Modules for 7890 and 6890 Series GC Systems

This groundbreaking column technology is designed specifically for Agilent 7890A and 6890 series gas chromatographs, and delivers:

- The capacity to run up to four column modules simultaneously – with four different temperature programs – to maximize your productivity
- Rapid temperature programming rates of up to 1800 °C/min for higher analysis speeds
- Faster cooling times – as low as one minute or less – to decrease idling and downtime
- Shorter analytical cycle times than conventional air-bath GC oven techniques
- Excellent retention time repeatability and performance – comparable to conventional GC

Most Agilent J&W Capillary GC columns – including Wall Coated Open Tubular (WCOT) and Porous Layer Open Tubular (PLOT) columns – can be used for LTM column modules.



Agilent J&W LTM Column Modules for 5975T Transportable GC/MS Systems

This groundbreaking column technology is designed specifically for Agilent 5975T GC/MS systems. These modules include an integrated 3 in LTM capillary column toroid assembly with heated transfer lines, cooling fan assembly and sheet metal enclosure. Replacement column toroid assemblies are also available. Benefits of the LTM column modules include:

- Rapid temperature programming rates of up to 1200 °C/min
- Faster heating and cooling times – as low as one minute or less – for more rapid analytical cycle times than standard air-bath GC oven techniques
- Excellent retention time repeatability and performance comparable to conventional GC
- Less power consumption for longer in-field operation
- Integrated module design to facilitate easy column module change in the field

Shorten analytical cycle times and boost your high speed gas chromatography capabilities



Agilent J&W LTM column modules combine a high quality fused silica capillary column with heating and temperature sensing components for a low thermal mass column assembly. The LTM column module contains a patented design which heats and cools the column very efficiently for significantly shorter analytical cycle times compared to conventional air-bath GC oven techniques, while simultaneously using less power.

Agilent offers LTM technology for our popular 7890 and 6890 Series GC systems, as well as the new 5875T GC/MS. Compatible with Agilent LTM and LTM II series GC systems and retrofit upgrades.

All LTM column modules are packaged with:

- Two 1 m guard columns (one each for the inlet and detector) made from deactivated fused silica tubing of the same id as the analytical column
- Five non-reusable ferrules that fit the dimensions of the analytical and guard columns

For more information, visit www.agilent.com/chem/LTMcol



GC Capillary Columns

More than just essential products... reliable results!

With the highest inertness, lowest bleed levels, and the tightest column-to-column reproducibility, Agilent J&W GC Capillary columns perform better than any columns on the market.

Ultra Inert Columns – allow you to perform trace level analysis – including the analysis of acids, bases, or other active compounds – with the utmost confidence. They also help ensure an inert GC flow path that is essential for sensitivity, performance, and the integrity of your analytical results.

High Efficiency Columns – are ideal for applications that require reduced analysis time, such as high throughput screening, fast process monitoring, fast QC analyses, and fast method development.

Low-bleed GC/MS Columns – are specifically designed to chromatograph a broad range of trace-level samples, and offer low bleed and high inertness even at higher temperatures.

Premium Polysiloxane Columns – are stable, robust, and versatile and are available in a wide variety of stationary phases.

Polyethylene Glycol (PEG) Columns – offer a variety of unique phase characteristics to meet the varying needs of your laboratory, thanks to Agilent's strict quality control of the cross-linking and deactivation processes.

Specialty Columns – meet Agilent's uncompromising standards for high-temperature, life science, pesticide, petroleum, semivolatile, and volatile applications.

PLOT Columns – deliver superior separation for compounds that are gases at room temperature. They are also ideal for analyzing fixed gases, low molecular weight hydrocarbon isomers, volatile polymer compounds, and reactive analytes such as gases, amines, and hydrides.

On the following pages you will find details on our complete line of innovative Agilent J&W GC columns. For more information contact your local Agilent representative or Agilent Authorized Distributor. Or you can order online at **www.agilent.com/chem/store**.

Table of Contents

Column Selection **195**

GC Column Application and Method Guides **210**

Ultra Inert Capillary GC Columns **237**

DB-1ms Ultra Inert **240**
HP-1ms Ultra Inert **240**
DB-5ms Ultra Inert **241**
HP-5ms Ultra Inert **241**
DB-35ms Ultra Inert **242**
DB-624 Ultra Inert **242**
DB-UI 8270D **242**

Low-bleed GC/MS Columns **244**

DB-1ms **245**
HP-1ms **246**
VF-1ms **247**
DB-5ms **249**
HP-5ms **251**
VF-5ms **252**
DB-XLB **254**
VF-Xms **255**
DB-35ms **256**
VF-35ms **257**
DB-17ms **258**
VF-17ms **259**
VF-23ms **260**
VF-200ms **261**
DB-225ms **262**
VF-WAXms **263**
VF-624ms and VF-1301ms **265**
VF-1701ms **267**

Premium Polysiloxane Columns **269**

DB-1 ..... **269**
HP-1 ..... **273**
CP-Sil 5 CB **275**
Ultra 1 ..... **279**
Ultra 2 ..... **280**
DB-5 ..... **281**
HP-5 ..... **284**
CP-Sil 8 CB **286**
CP-Sil 13 CB **288**
DB-35 ..... **289**
HP-35 ..... **290**
DB-17 ..... **291**
HP-50+ **292**
CP-Sil 24 CB **293**
DB-23 ..... **294**
DB-200 ..... **295**
DB-210 ..... **296**
DB-225 ..... **297**
CP-Sil 43 CB **298**
DB-1301 ..... **299**
CP-1301 ..... **300**
DB-1701 ..... **301**
CP-Sil 19 CB **302**

Polyethylene Glycol (PEG) Columns **304**

DB-WAX and DB-WaxFF **304**
DB-WAXetr **306**
HP-INNOWax **307**
CP-Wax 52 CB **308**
DB-FFAP **310**
HP-FFAP **311**
CP-Wax 58 FFAP CB **312**
Carbowax 20M and HP-20M **313**

Specialty Columns **314**

High Temperature Columns **314**

DB-1ht **314**
DB-5ht **315**
DB-17ht **316**
VF-5ht and VF-5ht UltiMetal **317**

Petroleum Columns **318**

Lowox **318**
GS-OxyPLOT **318**
CP-Sil 5 CB for Formaldehyde **319**
HP-PONA **319**
CP-Sil PONA CB **320**
CP-Sil PONA for ASTM D 5134 ..... **320**
DB-Petro **321**
HP-1 Aluminum Clad **321**
DB-2887 ..... **322**
DB-HT SimDis **322**
CP-SimDist **323**
CP-SimDist UltiMetal **324**
CP-Sil 2 CB **325**
CP-TCEP for Alcohols in Gasoline **325**
Select Low Sulfur **326**
CP-Sil 5 CB for Sulfur **326**
Select Permanent Gases **327**
Select Al_2O_3 MAPD **327**
Biodiesel Capillary GC Columns **328**
Select Biodiesel **330**
Select Silanes **331**
CP-Volamine **331**
CP-Sil 8 CB for Amines **332**
CP-Wax for Volatile Amines and Diamines **332**
PoraPLOT Amines **332**

(Continued)

Table of Contents (Continued)

Specialty Columns (Continued)
Pesticides Columns ... **333**
DB-CLP 1 and DB-CLP 2 ... **333**
VF-5 Pesticides ... **334**
DB-1701P ... **334**
VF-1701 Pesticides ... **335**
CP-Sil 8 CB for Pesticides ... **335**
CP-Sil 19 CB for Pesticides ... **336**
DB-608 ... **336**
HP-PAS5 ... **337**
Rapid-MS ... **337**
PAH Columns ... **338**
Select PAH ... **338**
DB-EUPAH ... **338**
CP-Sil PAH CB UltiMetal ... **339**
Semivolatiles Columns ... **340**
DB-UI 8270D ... **340**
CP-Sil 8 CB for PCB ... **340**
DB-5.625 ... **341**
HP-5ms Semivolatile ... **342**
CP-Sil 5/C18 CB for PCB ... **342**
DB-Dioxin ... **343**
CP-Sil 88 for Dioxins ... **343**
Volatiles Columns ... **344**
DB-624 ... **344**
CP-Select 624 CB ... **346**
DB-VRX ... **347**
HP-VOC ... **348**
DB-502.2 ... **349**
DB-MTBE ... **349**
CP-Select CB for MTBE ... **350**
DB-TPH ... **350**
Select Mineral Oil ... **351**
Foods, Flavors and Fragrance Columns ... **352**
HP-88 ... **352**
CP-Sil 88 ... **353**
Select FAME ... **354**
CP-Sil 88 for FAME ... **354**
CP-Wax 57 CB ... **355**
CP-Carbowax 400 **356**
CP-Wax 57 CB for Glycols and Alcohols ... **356**
CP-TAP CB ... **357**
CP-FFAP CB ... **358**
CycloSil-B ... **358**
Cyclodex-B ... **359**
HP-Chiral β ... **359**
CP-Chirasil Val ... **360**
CP-Chirasil-Dex CB ... **360**
CP-Cyclodextrin-β-2,3,6-M-19 ... **361**
Life Sciences Columns ... **362**
DB-ALC1 and DB-ALC2 ... **362**
VF-DA ... **362**
HP-Blood Alcohol ... **363**
DB-5ms EVDX ... **363**
DB-Select 624 UI <467> ... **364**
HP-Fast Residual Solvent ... **364**
Metal Columns ... **365**
PLOT Columns ... **368**
PoraBOND Q ... **368**
PoraBOND U ... **369**
PoraPLOT Q and PoraPLOT Q-HT ... **369**
HP-PLOT Q ... **371**
GS-Q ... **372**
PoraPLOT U and PoraPLOT S ... **373**
HP-PLOT U ... **374**
PLOT Columns
HP-PLOT Al_2O_3 KCl ... **374**
GS-Alumina KCl ... **375**
CP-Al_2O_3/KCl and CP-Al_2O_3/Na_2SO_4 ... **375**
HP-PLOT Al_2O_3 S ... **378**
GS-Alumina ... **379**
HP-PLOT Al_2O_3 M ... **380**
GS-GasPro ... **380**
CP-SilicaPLOT ... **381**
CarboBOND and CarboPLOT P7 ... **382**
GS-CarbonPLOT ... **383**
HP-PLOT Molesieve ... **384**
CP-Molsieve 5Å ... **385**
Non-Bonded Stationary Phases ... **387**
Guard Columns ... **391**
LTM Column Modules ... **393**
Fused Silica Tubing ... **397**
Packed GC Columns ... **400**
GC Column Test Standards ... **411**
Column Installation and Troubleshooting ... **413**

Column Selection Principles

Narrow your choices, save time, and reduce trial and error

Selecting the right capillary column for your application can be an uncertain (and sometimes difficult) task. If possible, you should begin by consulting sample applications provided by GC manufacturers and suppliers – or described in published Application Notes.

In addition, the following pages will help you:

- Choose a stationary phase – your most critical decision – based on factors such as selectivity, polarity, and phenyl content.
- Understand how column diameter influences factors like efficiency, solute retention, head pressure, and carrier gas flow rates.
- Determine which column length will affect solute retention, column head pressure, column bleed – and cost.
- Appreciate the difference between thin-film and thick-film columns with regard to capacity, inertness, bleed, and upper temperature limit.

While there are no foolproof techniques, shortcuts, tricks or secrets to column selection, there are some guidelines and concepts that simplify the process. There are four major column parameters to consider: stationary phase, diameter, length, and film thickness.





Selecting Stationary Phases

Choosing the best stationary phase is the most important decision when selecting a capillary column. Unfortunately, it is also the most difficult and ambiguous decision. The most reliable method is to consult the large collection of example applications provided by column manufacturers, GC manufacturers and in published literature. While an exact example application may not be available, enough information can usually be obtained to simplify the decision or reduce the number of potential columns. The most difficult situation is when no previous information is available. Stationary phase selection is much easier even if only one chromatogram is available for all or most of the sample compounds. The most reliable method is to consult the large collection of example applications provided by GC column & hardware manufacturers and published in literature.

The concepts of stationary phase selectivity and polarity are very useful when selecting stationary phases. For best performance, start with the general purpose Agilent J&W Ultra Inert 1ms and 5ms columns to get the lowest column bleed and column activity for a wide range of analytes, including active compounds and trace level samples.

Synonymous use of the terms polarity and selectivity is not accurate, but it is very common. Selectivity is determined by the physicochemical interactions of the solute molecules with the stationary phase. Polarity is determined by the structure of the stationary phase. Polarity does have an effect on separation; however, it is only one of the many stationary phase properties that influence peak separation (see the next section on polarity).

Selectivity can be thought of as the ability of the stationary phase to differentiate between two solute molecules by differences in their chemical or physical properties. Separation is obtained if the interactions between the stationary phase and solutes are different. For liquid or gum stationary phase (polysiloxanes and polyethylene glycols), there are three major interactions: dispersion, dipole, and hydrogen bonding. The following is a simplified and condensed explanation of the interactions for polysiloxane and polyethylene glycol stationary phases.

Dispersion is the dominant interaction for all polysiloxane and polyethylene glycol stationary phases. Dispersion can be simplified into the concept of volatility. Simply stated, the more volatile a solute, the faster it elutes from the column (i.e., shorter retention time). However, this order can be altered by the effect of solute and stationary phase polarities, and the other interactions. Solute boiling points are sometimes used as a measure of compound volatility. That is, compounds elute in the order of their increasing boiling points. Unfortunately, boiling points cannot be universally applied to the dispersion interactions. Boiling points are fairly valid when dealing with compounds with similar structures, functional groups or homologous series (**Figure 1**). When dealing with compounds with mixed functional groups, the boiling points simplification often fails (**Figure 2**). If compound boiling points differ by more than 30 °C, they usually can be separated by most stationary phases (there are exceptions). If compound boiling points differ by less than 10 °C, the boiling point simplification becomes less certain and more likely to be in error (except for compounds in a homologous series).


Figure 1: Boiling Point Elution Order for Homologous Series

Column: **DB-1, 15 m x 0.25 mm id, 0.25 µm**

Carrier: Helium at 30 cm/sec

Oven: 60 °C for 1 min, 60-180 °C at 20 °C/min

	Boiling Point (°C)
1. n-Decane (C_{10})	174
2. n-Undecane (C_{11})	196
3. n-Dodecane (C_{12})	216
4. n-Tridecane (C_{13})	234
5. n-Tetradecane (C_{14})	253
6. n-Pentadecane (C_{15})	268
7. n-Hexadecane (C_{16})	287

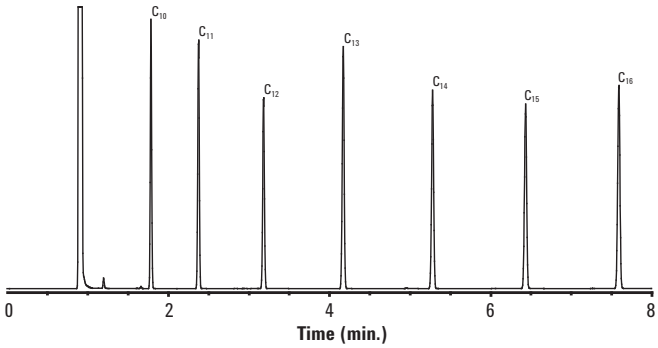


Homologous series of hydrocarbons. The solutes elute in order of their increasing boiling points; however, the peaks are not spaced in proportion to their respective boiling points.

Figure 2: Deviation from Boiling Point Order

Column: **DB-1, 30 m x 0.25 mm id, 0.25 µm**

	Boiling Point (°C)
1. Toluene	111
2. Hexanol	157
3. Phenol	182
4. Decane (C_{10})	174
5. Naphthalene	219
6. Dodecane (C_{12})	216

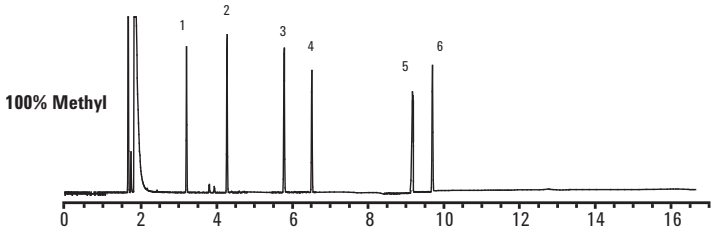

Solutes outside of the homologous series do not elute in the boiling point order.

If the stationary phase is capable of dipole interaction, it enhances its power to separate solutes whose dipole moments are different. Only some stationary phases are able to exploit this interaction. Polyethylene glycols, and cyanopropyl and trifluoropropyl substituted polysiloxanes readily undergo the dipole interactions; methyl or phenyl substituted groups do not undergo a dipole interaction (**Table 1**). The amount of peak separation for solutes with different dipoles often changes if a stationary phase with a different interaction is used (**Figure 3**). If the dipole difference between compounds is small, a greater amount of the appropriate group is needed (e.g., a 50% cyanopropylphenyl-methyl polysiloxane instead of a 14% cyanopropylphenyl-methyl polysiloxane). It is difficult to accurately predict the magnitude of the separation change for all of the peaks. Empirical results have shown that dipole interaction stationary phases are well suited for samples containing compounds that have base or central structures to which different groups are attached in various positions. Examples include substituted aromatics, halocarbons, pesticides and drugs.


Table 1: Stationary Phase Interactions

Functional Group	Dispersion	Dipole	Hydrogen Bonding
Methyl	Strong	None	None
Phenyl	Strong	None to Weak	Weak
Cyanopropyl	Strong	Very Strong	Moderate
Trifluoropropyl	Strong	Moderate	Weak
PEG	Strong	Strong	Moderate

Figure 3: Dipole Interactions

Column: **HP-88, 30 m x 0.25 mm id, 0.25 µm**

Molecular weight and boiling points are virtually identical for these fatty acid methyl ester (FAME) isomers, with only the dipole interactions due to the hydrogen isomeric positions on the molecules being different. Only strong dipole interactions in the stationary phase can provide chromatographic separation for these types of compounds.

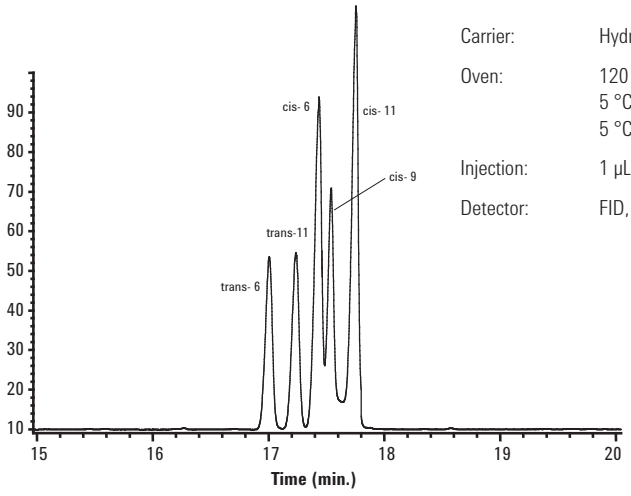

C-18:1 cis and trans isomers on HP-88

Carrier:	Hydrogen, 2 mL/min constant flow
Oven:	120 °C, 1 min, 10 °C/min to 175 °C, 10 min 5 °C/min to 210 °C, 5 min 5 °C/min to 230 °C, 5 min
Injection:	1 µL
Detector:	FID, 250 °C


The hydrogen bonding interaction occurs if there is hydrogen bonding between the solute molecules and the stationary phase. **Table 2** lists the types of compounds that can form hydrogen bonds along with their relative bonding strengths. It is the difference in the strength of the hydrogen bonding that is critical. The same stationary phases that undergo dipole interactions also undergo hydrogen bonding interactions. The amount of peak separation for solutes whose hydrogen bonding potentials differ often changes if a stationary phase with a different amount of hydrogen bonding interaction is used (**Figure 4**). If the hydrogen bonding difference between compounds is small, a great amount of the appropriate group is needed (e.g., a polyethylene glycol instead of a 14% cyanopropylphenyl-methyl polysiloxane). It is difficult to accurately predict the magnitude of the separation change for all of the peaks. Sometimes the desired separation is obtained, but another set of peaks now co-elute with the new stationary phase.

Table 2: Relative Hydrogen Bonding Strengths

Strength	Compounds
Strong	Alcohols, carboxylic acids, amines
Moderate	Aldehydes, esters, ketones
Weak to None	Hydrocarbons, halocarbons, ethers

Figure 4: Hydrogen Bonding Interactions

Column: 15 m x 0.25 mm id, 0.25 µm

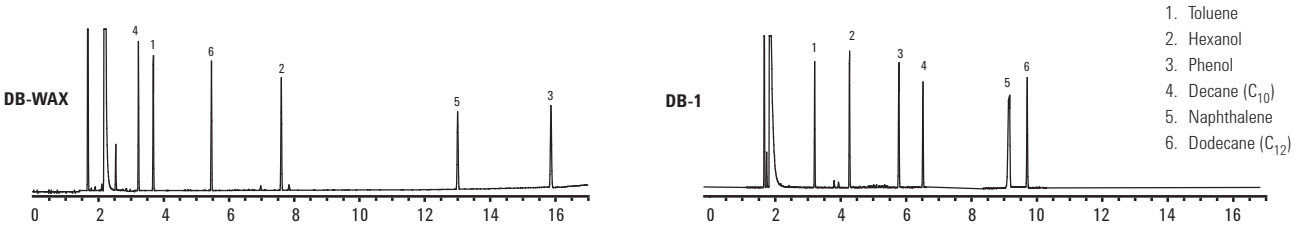


DB-1 does not undergo hydrogen bonding interactions. The change in the elution order of hexanol and phenol with DB-WAX is a combination of the dipole and hydrogen bonding interaction.

Another stationary phase characteristic that may effect retention in a predictable manner is the phenyl content. In general, the higher the phenyl content of the stationary phase, the higher the retention of aromatic solutes relative to aliphatic solutes. This does not mean that aromatic solutes are more retained (e.g., higher k) by high phenyl content stationary phases, but that aromatic solutes are more retained relative to aliphatic solutes. **Figure 5** shows an example of this retention behavior.

Figure 5: Phenyl Content Retention

Column: 15 m x 0.25 mm id, 0.25 µm

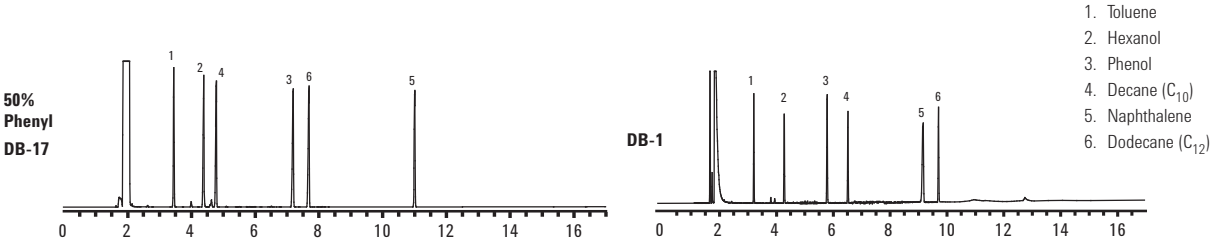

The aromatics increase in retention relative to the hydrocarbons for the DB-17 columns. DB-17 contains 50% phenyl substitution. DB-1 contains no phenyl substitution.

Polarity


Stationary phase polarity is determined by the polarity of the substituted groups and their relative amounts. **Table 3** lists a variety of stationary phases in order of their increasing polarity. Polarity is often erroneously used to select columns or to determine separation characteristics. Stationary phase polarity is only one of many factors that affect retention and separation.

While polarity is not directly related to selectivity, it has a pronounced affect on compound retention, thus separation. For compounds of similar volatility, greater retention is obtained for solutes with polarities similar to the stationary phase. In other words, polar compounds are more strongly retained by a polar stationary phase than a less polar stationary phase, and vice versa. This effect can be seen in **Figure 6**. The changes in retention and elution order can be largely attributed to the changes in stationary phase polarity. Changes in the amount of phenyl substitution, and dipole and hydrogen bonding interactions also contribute to the changes; however, it is difficult to assess the magnitude of their individual contributions.

Separation and efficiency have to be considered together and not as separate column attributes, as each contributes to peak resolution. When the stationary phase provides adequate resolution between peaks, higher efficiency is not needed. Shorter or larger diameter columns and less than optimal GC conditions can be used in these situations. When resolution is not adequate, there is a need for higher column efficiency.

Figure 6: Polarity – Retention Relationship

Column: 15 m x 0.25 mm id, 0.25 µm

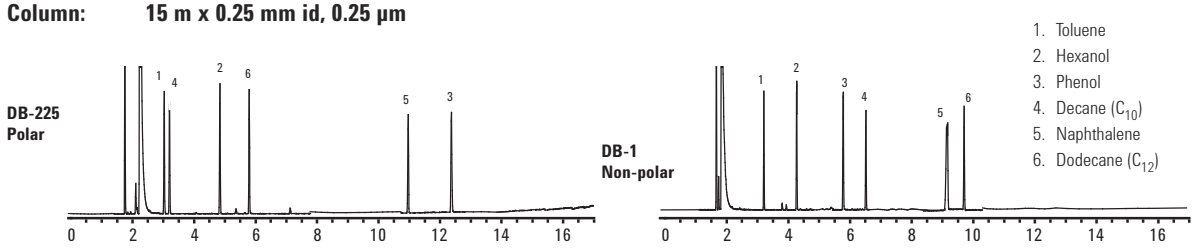

The alcohols (polar) increase in retention relative to hydrocarbon (non-polar) for the DB-225 column. DB-225 is more polar than DB-1.

In addition to retention, stationary phase polarity influences other column characteristics. There is a general trend between stationary phase polarity and column lifetime, temperature limits, bleed and efficiency. Column life, temperature limits and efficiency tend to be higher for more non-polar stationary phases. These are general trends and not absolute certainties. Low bleed stationary phases sometimes go against this trend.

Table 3: Stationary Phase Polarity

Low Polarity			Mid Polarity			High Polarity		
CP-Sil 2	DB & HP-1ms UI	DB & HP-5ms UI	DB-XLB	DB-225ms	DB-ALC1	HP-88	DB-WAX	CP-TCEP
DB-MTBE	DB & HP-1ms	DB & HP-5ms	VF-Xms	DB-225	DB-Dioxin	CP-Sil 88	DB-WAXetr	
CP-Select CB MTBE	VF-1 ms	VF-5ms	DB-35ms UI	CP-Sil 43 CB	DB-200	DB-23	HP-INNOWax	
	DB & HP-1	DB & HP-5	DB & VF-35ms	VF-1701 ms	VF-200ms	VF-23 ms	VF-WAXms	
	CP-Sil 5 CB	CP-Sil 8 CB	DB & HP-35	DB-1701	DB-210		CP-Wax 57 CB	
	Ultra 1	Ultra 2	DB & VF-17ms	CP-Sil 19 CB	DX-4		DB & HP-FFAP	
	DB-1ht	VF-DA	DB-17	HP-Blood Alcohol			DB-WAX FF	
	DB-2887	DB-5.625	HP-50+	DB-ALC2			CP-FFAP CB	
	DB-Petro/ PONA	DB & VF-5ht	DB-17ht	DX-1			CP-WAX 58 FFAP CB	
	CP-Sil PONA CB	CP-Sil PAH CB	DB-608				CP-WAX 52 CB	
	DB-HT SimDis	Select Biodiesel	DB-TPH				CP-WAX 51	
	CP-SimDis	SE-54	DB-502.2				CP-Carbowax 400	
	CP-Volamine		HP-VOC				Carbowax 20M	
	Select Mineral Oil		DB-VRX				HP-20M	
	HP-101		DB-624				CAM	
	SE-30		VF-624ms					
			CP-Select 624 CB					
			DB-1301					
			VF-1301ms					
			CP-Sil 13 CB					

Gas-Solid or PLOT Columns

PLOT (Porous Layer Open Tubular) columns are intended for the separation of very volatile solutes (primarily gases) without the need for cryogenic or sub-ambient cooling of the oven. Separations that would require column temperatures below 35 °C, even with thick film liquid stationary phase can be obtained at temperatures above 35 °C with PLOT columns.

Gas-solid or PLOT column stationary phases are physically different than polysiloxanes and polyethylene glycols. Gas-solid stationary phase are small, porous particles. The particles are stuck to the inner wall of the capillary tubing using a binder or similar means. Solutes are separated based on differences in their adsorption properties. Since the particles are porous, size and shape differentiation also occurs.

Alumina PLOT columns are well suited for the separation of C_1-C_{10} hydrocarbons and small aromatics. The KCl version of the Alumina PLOT column changes the retention order for some of the hydrocarbons. The PLOT Q column provides slightly better separation for C_1-C_3 hydrocarbons, but C_4 and higher hydrocarbons are better separated with an Alumina PLOT column. PLOT Q exhibits extremely long retention times and very broad peaks for C_6 and higher hydrocarbons and aromatics. PLOT Q separates sulfur gases from each other and from most light hydrocarbons. Molesieve PLOT columns are used to separate many noble and permanent gases. GS-GasPro columns combine many of the features of the various other PLOT columns. Light hydrocarbons, inorganic gases and solvents are some of the samples suitable for GS-GasPro.

Primary Selectivity Interactions in PLOT Phases

Dispersive

Shape/Size		**Ionic Surface**
Zeolites	⟷	Alumina/Al_2O_3 GS-OxyPLOT

Dispersive

Shape/Size		**Ionic Surface**
Molecular Sieves Bonded Graphitized Carbon	⟷ **Porous Polymers**	Bonded Silica

PLOT Column Examples

Zeolite/Molesieve:	HP-PLOT Molesieve
Graphitized Bonded Carbon:	GS-CarbonPLOT, CarboBOND
Porous Polymers:	HP-PLOT Q, HP-PLOT U
Bonded Silica:	GS-GasPro, CP-SilicaPLOT
Alumina/Al_2O_3:	GS-Alumina, GS-Alumina KCl, HP-PLOT Al_2O_3 KCl, HP-PLOT Al_2O_3 "S", HP-PLOT Al_2O_3 "M"
Proprietary Phase:	Lowox, GS-OxyPLOT

Stationary Phase Selection Summary

1. If no information or ideas about which stationary phase to use is available, start with a DB-1 or DB-5.
2. Low-bleed ("ms") columns are usually more inert and have higher temperature limits. Ultra Inert 1ms, 5ms and 35ms columns provide the lowest column bleed and highest column inertness for a wide range of analytes, including active compounds and trace level samples.
3. Use the least polar stationary phase that provides satisfactory resolution and analysis times. Non-polar stationary phases have superior lifetimes compared to polar phases.
4. Use a stationary phase with a polarity similar to that of the solutes. This approach works more times than not; however, the best stationary phase is not always found using this technique.
5. If poorly separated solutes possess different dipoles or hydrogen bonding strengths, change to a stationary phase with a different amount (not necessarily more) of the dipole or hydrogen bonding interaction. Other co-elutions may occur upon changing the stationary phase, thus the new stationary phase may not provide better overall resolution.
6. If possible, avoid using a stationary phase that contains a functionality that generates a large response with a selective detector. For example, cyanopropyl containing stationary phases exhibit a disproportionately large baseline rise (due to column bleed) with NPDs.
7. A DB-1 or DB-5, DB-1701, DB-17, and DB-WAX cover the widest range of selectivities with the smallest number of columns.
8. PLOT columns are used for the analysis of gaseous samples at above ambient column temperatures.

TIPS & TOOLS

Ensure a lifetime of peak performance and maximum productivity with Agilent's comprehensive GC supplies portfolio, learn more at **www.agilent.com/chem/GCsupplies**



Table 4:
Column Efficiency vs. Diameter

Column ID Diameter (mm)	Theoretical Plates/Meter
0.10	12,500
0.18	6,600
0.20	5,940
0.25	4,750
0.32	3,710
0.45	2,640
0.53	2,240

Maximum efficiency for a solute with k=5

Column Diameter

Column diameter has an influence over five parameters of primary concern. They are efficiency, retention, pressure, carrier gas flow rate, and capacity.


Column efficiency (N/m) is inversely proportional to column diameter. The efficiencies listed in **Table 4** show that smaller diameter columns have higher theoretical plates per meter. Resolution is a square root function of the theoretical plate number. Therefore, doubling column efficiency theoretically increases resolution only by 1.41 times (the square root of 2), but closer to 1.2-1.3 times in real practice. Smaller diameter columns are used when peak separation is small and high column efficiency (i.e., narrow peaks) is needed. **Figure 7** shows the difference in resolution for two different diameter columns.

Solute retention is inversely proportional to column diameter, for isothermal temperature conditions. For temperature program conditions, the change is 1/3-1/2 of the isothermal value. Column diameters are rarely selected based on retention. **Figure 7** shows the difference in retention for two different diameter columns.

Column head pressure is approximately an inverse squared function of the column radius. For example, a 0.25 mm id column requires about 1.7 times the head pressure of a 0.32 mm id column of the same length (also, carrier gas and temperature). Column head pressures increase or decrease dramatically with changes in column diameter. Column diameters of 0.18 mm id or larger are used for standard GC analysis due to the very high pressures needed for smaller diameter columns. Wider diameter columns, especially shorter ones (e.g., 15 m x 0.32 mm id), are impractical for use in GC/MS systems. The vacuum at the exit of the column greatly reduces the required head pressure, and it is difficult to maintain or control very low head pressures.

Figure 7: Column Diameter –
Comparison of Resolution and Retention

Column: **DB-624, 30 m**

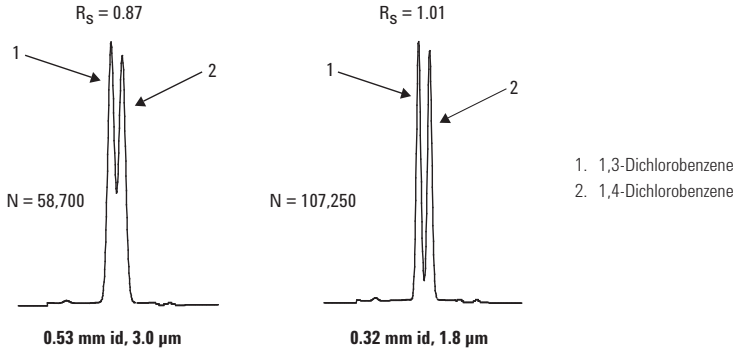

At constant pressure, **carrier gas flow rates** increase as column diameters increase. For applications or hardware requiring high flow rates, larger diameter columns are normally used. Headspace and purge & trap systems require higher carrier gas flow rates for proper operation. 0.45 or 0.53 mm id columns are used with these systems so that the higher flow rates can be used. Special considerations must be taken if small diameter columns are used in these types of systems. This includes the use of cryogenic interfaces or ovens, or interfacing through split injectors. Added complexity and/or cost, or sample loss, are involved with these techniques. For applications or hardware requiring low carrier gas flow rates, smaller diameter columns are normally used. GC/MS is the typical system requiring low carrier gas flow rates, and therefore, 0.25 mm id and smaller id columns are used in these applications.

Column capacity increases as the column diameter increases. The actual column capacity also depends on the stationary phase, solute and film thickness. **Table 5** lists typical capacity ranges for a variety of column diameters.

Table 5: Column Capacity in ng

Film Thickness (µm)	Column Inside Diameter (mm)			
	0.18-0.20	**0.25**	**0.32**	**0.53**
0.10	20-35	25-50	35-75	50-100
0.25	35-75	50-100	75-125	100-250
0.50	75-150	100-200	125-250	250-500
1.00	150-250	200-300	250-500	500-1000
3.00		400-600	500-800	1000-2000
5.00		1000-1500	1200-2000	2000-3000

Column Diameter Selection Summary

1. Use **0.15, 0.18 or 0.25 mm id columns** when higher column efficiencies are needed. 0.15 and 0.18 mm id columns are especially well suited for GC/MS systems with low pumping capacities. Smaller diameter columns have the lowest capacities and require the highest head pressures.
2. Use **0.32 mm id columns** when higher sample capacity is needed. They often provide better resolution of earlier eluting solutes for splitless injections or large injection volumes (> 2 µL) than 0.25 mm id columns.
3. Use **0.45 mm id columns** when only a Megabore direct injector is available and higher column efficiency is desired. Well suited for high carrier gas flow rate situations, such as with purge & trap, headspace samplers, and valve injection applications.
4. Use **0.53 mm id columns** when only a Megabore direct injector is available. Well suited for high carrier gas flow rate situations, such as with purge & trap and headspace samplers. 0.53 mm id columns have the highest sample capacities at constant d_f.




Column Length

Column length influences three parameters of major concern. They are efficiency, retention (analysis time) and carrier gas pressure.

Column efficiency (N) is proportional to column length. Resolution is a square root function of the theoretical plate number. For example, doubling column length (thus efficiency) theoretically increases resolution by only 1.41 times (closer to 1.2-1.3 times in practice). Longer columns are used when peak separation is small and high column efficiency (i.e., narrow peaks) is needed. **Figure 8** shows the difference in resolution for three different lengths.

Figure 8: Column Length – Comparison of Resolution and Retention

Column: **DB-624**
15 m x 0.53 mm id, 0.3 µm
30 m x 0.53 mm id, 0.3 µm
60 m x 0.53 mm id, 0.3 µm

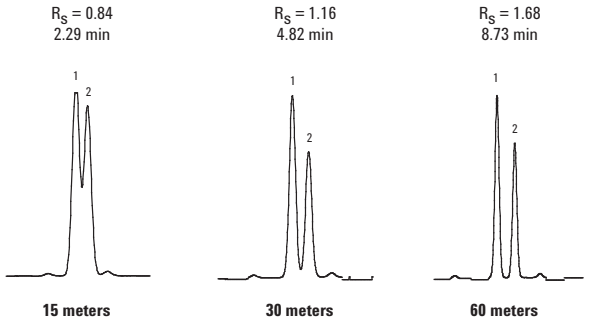

1. 1,3-Dichlorobenzene
2. 1,4-Dichlorobenzene

Solute retention is proportional to column length for isothermal temperature conditions. For temperature program conditions, the change is 1/3-1/2 of the isothermal value. When efficiency is increased by lengthening the column, there is a significant increase in analysis time. Figure 8 shows the difference in retention for three different lengths.

Column head pressure is nearly proportional to column length. Pressure is usually not an issue unless the column has a very small or large diameter. Long, small diameter columns require extremely high head pressures, and short, wide diameter columns require very low head pressures. Neither situation is very practical and may be a limiting factor. Choice of carrier gas will also have an impact on column pressure.

Column bleed increases as column length increases. Longer columns have more stationary phase, thus more degradation products are produced. The increase in bleed with longer columns is not large and should not be a deterrent to using a longer column when one is necessary.

Column cost is directly related to column length. Doubling column length nearly doubles the price of the column. When efficiency is increased by lengthening the column, there is a significant increase in column cost. When considered in conjunction with the increase in analysis time, lengthening the column should be the last reasonable option for increasing efficiency.

Shorter columns cost more per meter than longer columns. Cutting longer columns into shorter lengths seems like a good method to save money, but it is not recommended. The quality of the smaller pieces cannot be guaranteed and may not be the same as the original, intact column. Theoretically, each piece should provide satisfactory and consistent results. In practice, this does not always occur. The probability of individual piece variation is higher when shorter pieces are cut from the original column. Greater variability between individual pieces is observed as column length, film thickness and stationary phase polarity increases, and column diameter decreases. Finally, there is the increased chance of tubing breakage when rewinding the shorter columns on other cages. Technically, cutting a column into shorter pieces voids the performance warranty.

Column Length Selection Summary

1. Start with **25-30 meter columns** when the best length is unknown.
2. **10-15 meter columns** are well suited for samples containing very well separated solutes or very few solutes. Shorter lengths are used for very small diameter columns to reduce head pressures.
3. **50-60 meter columns** should be used when resolution is not possible by other means (smaller diameter, different stationary phase, change in column temperature). Best suited for complex samples containing a large number of solutes. Long columns have long analysis times and higher cost.

Column Film Thickness

Column film thickness influences five major parameters: retention, resolution, bleed, inertness and capacity.

For isothermal conditions, solution retention is directly proportional to film thickness. For temperature program conditions, the change is 1/3-1/2 of the isothermal value. Thicker film columns are used to obtain higher retention for very volatile solutes. Volatile solutes normally requiring cryogenic (subambient) cooling with standard film thickness columns can be sufficiently retained at temperatures above 30 °C. Changing to a thicker film column has a net effect of providing equal or greater retention at a higher column temperature. Thicker film columns are typically used for volatile compounds like solvents and select gases. Thinner film columns are used to reduce the retention of highly retained solutes. Highly retained solutes can be eluted faster or at a lower temperature. Changing to a thinner film column has the net effect of providing equal or less retention at a lower column temperature. Thinner film columns are typically used for high boiling or molecular weight compounds. **Figure 9** shows the difference in retention for two different film thicknesses.


Solutes with k values less than 2 are very difficult to resolve due to insufficient retention by the column. Changing to a thicker film column results in better resolution since solute retention is increased. The resolution improvement depends on the solute k value for the original column. For solutes with k values of about 5 or less, increasing their retention results in improved resolution. For solute peaks with values of 5-10, increasing their retention provides a small to moderate increase in resolution. For peaks with k values above 10, increasing their retention often results in no resolution improvement and sometimes a loss of resolution. Increasing film thickness to improve the resolution of early eluting peaks may result in a resolution loss for later eluting peaks.

Figure 9: Column Film Thickness – Comparison of Resolution and Retention

Column: **DB-1, 30 m x 0.32 mm id**

Carrier: Helium at 38 cm/sec

Oven: 100 °C isothermal

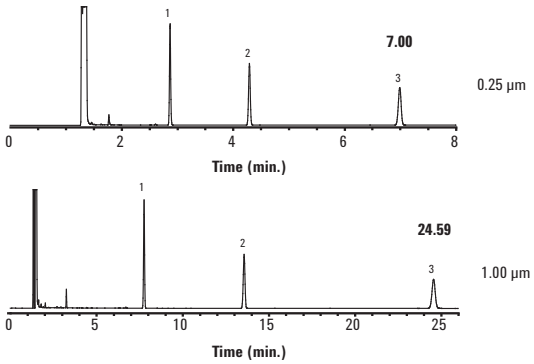

1. n-Decane
2. n-Undecane
3. n-Dodecane

For a given stationary phase, column bleed increases as film thickness increases. Since thicker film columns are more retentive, later eluting peaks may shift into a region of much higher column bleed when increasing film thickness. The upper temperature limits of thick film columns may be lower due to their higher bleed levels.

Thicker film columns are more inert. There is more stationary phase to shield the solutes from the tubing surface. Peak tailing for active compounds can often be reduced or eliminated with a thicker film column.

Thicker film columns have higher solute capacities. When one solute is present in significantly higher amounts, the resulting broad peak may interfere or co-elute with an adjacent peak. Changing to a thicker film column may reduce peak broadening, thus co-eluting. Table 5 lists typical capacity ranges for a variety of film thickness.

Column Film Thickness Selection Summary

1. For **0.18-0.32 mm id columns**, a film thickness of 0.18-0.25 µm is average or standard (i.e., not thin or thick) and used for most analyses.
2. For **0.45-0.53 mm id columns**, a film thickness of 0.8-1.5 µm is average or standard (i.e., not thin or thick) and used for most analyses.
3. **Thick film columns** are used to retain and resolve volatile solutes (e.g., light solvents, gases). Thick columns are more inert and have higher capacities. Thick film columns exhibit higher column bleed and decreased upper temperature limits.
4. **Thin film columns** are used to minimize the retention of high boiling, high molecular weight solutes (e.g., steroids, triglycerides). Thin film columns are less inert, have lower capacities and exhibit lower column bleed.



GC Column Application and Method Guides

Application	Specific Application	Agilent Phases
Biodiesel	EN14105 Free/Total Glycerin	Biodiesel, Select Biodiesel
	ASTM D6584 Free/Total Glycerin	Biodiesel, Select Biodiesel
	EN14103 FAME Analysis	Biodiesel, Select Biodiesel
	EN14110 Residual Methanol	Biodiesel, Select Biodiesel
	EN14106 Free Glycerol	Select Biodiesel
Chiral	Chiral γ-lactones and terpenes	CycloSil-B
	Optical isomers of acids, alcohols, amino acids, aromatic hydrocarbons, diols, flavors, aromas, ketones, organic acids and phenols	Cyclodex-B
	Chiral compounds using a nitrogen selective detector	HP-Chiral β
	Optical isomers of acids, alcohols, amino acids, aromatic, diols, flavor, aromas, ketones, organic acids and phenols	CP-Chirasil-Dex CB, CP-Cyclodextrin-β-2,3,6-M-19
	Amino acids, optical isomers	CP-Chirasil-Dex CB, CP-Cyclodextrin-β-2,3,6-M-19
Foods, Flavors and Fragrances	FAME up to C_{26}, cis, trans, fast resolution FAME	Select FAME
	Best separation for cis, trans FAME analyses up to 260 °C	HP-88, CP-Sil 88 for FAME
	Volatiles	CP-Carbowax 400 for Volatiles in Alcohol
	Unsaturated triglycerides	CP-TAP CB for Triglycerides
	Flavors, aromas, free fatty acids C_1-C_{26}	DB-WAX, HP-WAX, CP-FFAP CB
	Glycols, diols, alcohols	CP-Wax 57 CB for Glycols and Alcohols, DB-WAX
Life Sciences	Blood alcohol analysis	DB-ALC1 and DB-ALC2
	Drugs of abuse confirmation	DB-5ms EVDX
	USP solvents, common solvents	DB-Select 624UI for <467>, DB-624, VF-624ms
	Drugs of abuse confirmation	DB-35ms Ultra Inert, VF-DA
Pesticides	Organochlorine pesticides and PCBs	DB-CLP1 and DB-CLP2, DB-35ms Ultra Inert, DB-17ms, DB-XLB
	Chlorinated pesticides and PCBs	DB-608
	Trace levels of pesticides in food and environmental samples	DB-35ms Ultra Inert, DB-XLB, VF-1701 Pesticides, DB-1701P
	Chlorinated, nitrogen, phosphorus pesticides	CP-Sil 8 CB for Pesticides, DB-35ms Ultra Inert, DB-5ms Ultra Inert
	Chlorinated, nitrogen, phosphorus pesticides, trace level DDT and Endrin	CP-Sil 19 CB for Pesticides, DB-35ms, DB-XLB

(Continued)

Application	Specific Application	Agilent Phases
Polycyclic Aromatic Hydrocarbons	EU regulated PAHs	DB-EUPAH
	PAHs in environmental and food samples	Select PAH
	C_5-C_{80}, PAH and polar compounds	CP-Sil PAH CB UltiMetal
	EU and EPA regulated PAHs	VF-17ms for PAH
Petroleum	Simulated distillation using ASTM Method D2887	DB-2887
	C_5-C_{120} simulated distillation	DB-HT SimDis, CP-SimDist UltiMetal
	PONA and PIANO analysis	HP-PONA, DB-Petro, CP-Sil PONA CB
	ASTM D5134	CP-Sil PONA for ASTM D5134
	C_1-C_{10} hydrocarbons	Select Al_2O_3 MAPD, Alumina PLOT family
	C_1-C_6 alcohols, aromatic C_6-C_{10}	CP-TCEP for Alcohols in Gasoline
	Sulfur impurities in propylene streams	Select Low Sulfur
	Polar and non-polar volatile compounds, especially chlorosilanes with different substituents such as alkyl groups, or groups with ether, hydroxy and nitrile bonds	Select Silanes
	C_1-C_6 amines, alcohols, NH_3, water, solvents, ethanol amines	CP-Volamine
	C_3-C_{20} amines, alkanol amines	CP-Sil 8 CB for Amines
	C_3-C_8 amines and diamines	CP-Wax for Volatile Amines and Diamines
	C_4-C_{10} amines, diamines and aromatic amines	CP-Wax 51 for Amines
	Oxygenates in C_1-C_{10} hydrocarbons	CP-Lowox, GS-OxyPLOT
	C_1-C_{10} hydrocarbons	GS-OxyPLOT
	Methanol, formaldehyde and formic acid in water	CP-Sil 5 CB for Formaldehyde
	C_1-C_{12} hydrocarbons	CP-Squalane
	Volatile oxygenates and halogenated hydrocarbons	CP-Propox
Semivolatiles	Polychlorinated dibenzodioxins (PCDDs) and dibenzofurans (PCDFs)	DB-Dioxin
	Dioxins and dibenzo furan	CP-Sil 88 for Dioxins, DB-Dioxin
	EPA Semivolatiles Methods 625, 1625, 8270 and CLP protocols	DB-UI 8270D, DB-5ms Ultra Inert, DB-5.625, HP-5ms Semivolatile
	PCB, detailed analysis	CP-Sil 5/C18 CB for PCB
	PCB	CP-Sil 8 CB for PCB, DB-XLB

(Continued)

Application	Specific Application	Agilent Phases
Volatiles	EPA Methods 502.2, 524.2 and 8260	DB-624 Ultra Inert, DB-VRX
	Volatile priority pollutants and residual solvents	DB-624 Ultra Inert, DB-624, VF-624ms
	Halogenated hydrocarbons and solvents	CP-Select 624 CB
	EPA Methods 502.2, 524.2 and 8260	HP-VOC
	EPA Method 502.2	DB-502.2
	MTBE in soil and water	DB-MTBE
	Oxygenates and solvents	CP-Select CB for MTBE
	Total petroleum hydrocarbons (TPHs), soil analysis, and LUFT	DB-TPH
	C_5-C_{40} hydrocarbons	Select Mineral Oil
Metal	High temperature analysis and process applications	UltiMetal and DB-ProSteel
Non-Bonded	Amino acid derivatives, essential oils	HP-101
	Drugs, glycols, pesticides, steroids	HP-17
	Amines, basic compounds	CAM
	Alcohols, free acids, essential oils, ethers, glycols, solvents	Carbowax 20M and HP-20M
	Generic	SE-30 and SE-54

TIPS & TOOLS

Search the application library to find GC applications and standard methods of all types, old and new.
To view, please visit **www.agilent.com/chem/library**

EPA Methods

Drinking Water

EPA Methods	Application	Recommended Column	Part No.
501, 501.3	Measurement of trihalomethanes in drinking water by GC/MS and selected ion monitoring	DB-VRX, 30 m x 0.25 mm, 1.40 µm	122-1534
		DB-624, 30 m x 0.25 mm, 1.40 µm	122-1334
		VF-624ms, 30 m x 0.25 mm, 1.40 µm	CP9102
		DB-624 Ultra Inert, 30 m x 0.25 mm, 1.4 µm	122-1334UI
502.2	Volatile organic compounds in water by purge and trap capillary column GC with photoionization and electrolytic conductivity detectors in series	DB-VRX, 60 m x 0.25 mm, 1.40 µm	122-1564
		DB-624, 60 m x 0.25 mm, 1.40 µm	122-1364
		VF-624ms, 60 m x 0.25 mm, 1.40 µm	CP9103
		DB-624 Ultra Inert, 60 m x 0.25 mm, 1.4 µm	122-1364UI
		VF-624ms, 30 m x 0.25 mm, 1.40 µm	CP9102
503.1	Volatile aromatic and unsaturated organic compounds in water by purge and trap gas chromatography	DB-VRX, 30 m x 0.25 mm, 1.40 µm	122-1534
		DB-624, 30 m x 0.25 mm, 1.40 µm	122-1334
504.1	1,2-Dibromoethane (EDB) and 1,2-dibromo-3-chloropropane (DB CP), GC, microextraction	DB-CLP1, 30 m x 0.32 mm, 0.25 µm	123-8232
		DB-CLP2, 30 m x 0.32 mm, 0.5 µm	123-8336
		DB-VRX, 30 m x 0.25 mm, 1.40 µm	122-1534
		DB-624, 30 m x 0.25 mm, 1.40 µm	122-1334
		DB-624 Ultra Inert, 30 m x 0.25 mm, 1.4 µm	122-1334UI
		VF-1ms, 30 m x 0.32 mm, 1.00 µm	CP8926
		VF-1701ms, 30 m x 0.32 mm, 1.00 µm	CP9163
505	Analysis of organohalide pesticides and commercial polychlorinated biphenyl (PCB) products in water by microextraction and GC	DB-CLP1, 30 m x 0.32 mm, 0.25 µm	123-8232
		DB-CLP2, 30 m x 0.32 mm, 0.5 µm	123-8336
		DB-XLB, 30 m x 0.25 mm, 0.50 µm	122-1236
		VF-1ms, 30 m x 0.32 mm, 1.00 µm	CP8926
		VF-17ms, 30 m x 0.32 mm, 0.50 µm	CP8991
506	Determination of phthalate and adipate esters in drinking water by liquid-liquid extraction or liquid-solid extraction and GC with photoionization detection	DB-5ms, 30 m x 0.25 mm, 0.25 µm	122-5532
		VF-5ms, 30 m x 0.32 mm, 0.25 µm	CP8955
		VF-1ms, 30 m x 0.32 mm, 0.25 µm	CP8924
507	Determination of nitrogen and phosphorus-containing pesticides in water by GC with a nitrogen-phosphorus detector	DB-35ms, 30 m x 0.25 mm, 0.25 µm	122-3832
		DB-5ms, 30 m x 0.25 mm, 0.25 µm	122-5532
		VF-5 Pesticides, 30 m x 0.25 mm, 0.25 µm	CP9074
		VF-1701 Pesticides, 30 m x 0.25 mm, 0.25 µm	CP9070

Drinking Water

EPA Methods	Application	Recommended Column	Part No.
508	Determination of chlorinated pesticides in water by GC with an electron capture detector	DB-CLP1, 30 m x 0.32 mm, 0.25 µm	123-8232
		DB-CLP2, 30 m x 0.32 mm, 0.5 µm	123-8336
		DB-35ms Ultra Inert, 30 m x 0.32 mm, 0.25 µm	123-3832UI
		DB-XLB, 30 m x 0.32 mm, 0.50 µm	123-1236
		DB-608, 30 m x 0.32 mm, 0.50 µm	123-1730
		VF-5 Pesticides, 30 m x 0.25 mm, 0.25 µm	CP9074
		VF-1701 Pesticides, 30 m x 0.25 mm, 0.25 µm	CP9070
508.1	Determination of chlorinated pesticides, herbicides, and organohalides by liquid-solid extraction and electron capture GC	DB-CLP1, 30 m x 0.32 mm, 0.25 µm	123-8232
		DB-CLP2, 30 m x 0.32 mm, 0.5 µm	123-8336
		DB-35ms Ultra Inert, 30 m x 0.32 mm, 0.25 µm	123-3832UI
		DB-XLB, 30 m x 0.32 mm, 0.50 µm	123-1236
		VF-5 Pesticides, 30 m x 0.25 mm, 0.25 µm	CP9074
515	Determination of chlorinated herbicides in drinking water	DB-35ms Ultra Inert, 30 m x 0.32 mm, 0.25 µm	123-3832UI
		DB-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	122-5532UI
		HP-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	19091S-433UI
		DB-1701, 30 m x 0.25 mm, 0.25 µm	122-0732
515.3	Determination of chlorinated acids in drinking water by liquid-liquid extraction, derivatization and GC with electron capture detection	DB-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	122-5532UI
		HP-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	19091S-433UI
		DB-1701, 30 m x 0.25 mm, 0.25 µm	122-0732
		VF-1701ms, 30 m x 0.25 mm, 0.25 µm	CP9151
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
515.4	Determination of chlorinated acids in drinking water by liquid-liquid microextraction, derivatization, and fast GC with electron capture detection	DB-5ms Ultra Inert, 20 m x 0.18 mm, 0.18 µm	121-5522UI
		HP-5ms Ultra Inert, 20 m x 0.18 mm, 0.18 µm	19091S-577UI
		DB-1701, 20 m x 0.18 mm, 0.18 µm	121-0722
		VF-1701ms, 30 m x 0.25 mm, 0.25 µm	CP9151
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
521	Determination of nitrosamines in drinking water by solid phase extraction and capillary column gas chromatography with large volume injection and chemical ionization tandem mass spectrometry (MS/MS)	DB-5ms Ultra Inert, 30 m x 0.25 mm, 1.00 µm	122-5533UI
		HP-5ms Ultra Inert, 30 m x 0.25 mm, 1.00 µm	19091S-233UI
		VF-5ms, 30 m x 0.25 mm, 1.00 µm	CP8946

(Continued)

Drinking Water

EPA Methods	Application	Recommended Column	Part No.
524.2	Measurement of purgeable organic compounds in water by capillary GC/MS	DB-VRX, 60 m x 0.25 mm, 1.40 µm	122-1564
		DB-624, 60 m x 0.25 mm, 1.40 µm	122-1364
		DB-624 Ultra Inert, 60 m x 0.25 mm, 1.4 µm	122-1364UI
		HP-VOC, 60 m x 0.20 mm, 1.10 µm	19091R-306
		DB-VRX, 20 m x 0.18 mm, 1.00 µm	121-1524
		DB-624, 20 m x 0.18 mm, 1.00 µm	121-1324
		DB-624 Ultra Inert, 60 m x 0.25 mm, 1.4 µm	122-1364UI
		VF-624ms, 30 m x 0.25 mm, 1.40 µm	CP9102
		VF-624ms, 60 m x 0.25 mm, 1.40 µm	CP9103
		VF-5ms, 30 m x 0.32 mm, 1.00 µm	CP8957
525, 525.2	Determination of organic compounds in drinking water by liquid-solid extraction and capillary column GC/MS	HP-5ms, 30 m x 0.25 mm, 0.50 µm	19091S-133
		VF-5 Pesticides, 30 m x 0.25 mm, 0.25 µm	CP9074
526	Determination of selected semivolatile organic compounds in drinking water by solid phase extraction and capillary column GC/MS	DB-5ms, 30 m x 0.25 mm, 0.25 µm	122-5532
		HP-5ms, 30 m x 0.25 mm, 0.25 µm	19091S-433
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
527	Determination of selected pesticides and flame retardants in drinking water by solid phase extraction and capillary column GC/MS	DB-5ms, 30 m x 0.25 mm, 0.25 µm	122-5532
		HP-5ms, 30 m x 0.25 mm, 0.25 µm	19091S-433
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
528	Determination of phenols in drinking water by solid phase extraction and capillary column GC/MS	DB-5ms, 30 m x 0.25 mm, 0.25 µm	122-5532
		DB-XLB, 30 m x 0.25 mm, 0.25 µm	122-1232
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
529	Determination of explosives and related compounds in drinking water by solid phase extraction and capillary column GC/MS	DB-5ms Ultra Inert, 15 m x 0.25 mm, 0.25 µm	122-5512UI
		HP-5ms Ultra Inert, 15 m x 0.25 mm, 0.25 µm	19091S-431UI
		VF-5ms, 15 m x 0.25 mm, 0.25 µm	CP8939
551	Determination of chlorination disinfection byproducts and chlorinated solvents in drinking water by liquid-liquid extraction and gas chromatography with electron-capture detection	DB-5ms, 30 m x 0.25 mm, 1.00 µm	122-5533
		DB-1, 30 m x 0.25 mm, 1.00 µm	122-1033
		DB-210, 30 m x 0.25 mm, 0.50 µm	122-0233
		VF-1301ms, 30 m x 0.25 mm, 1.00 µm	CP9054
551.1	Determination of chlorination disinfection byproducts, chlorinated solvents, and halogenated pesticides/herbicides in drinking water by liquid-liquid extraction and GC with electron-capture detection	DB-5ms, 30 m x 0.25 mm, 1.00 µm	122-5533
		DB-1, 30 m x 0.25 mm, 1.00 µm	122-1033
		DB-1301, 30 m x 0.25 mm, 1.00 µm	122-1333
		VF-1ms, 30 m x 0.25 mm, 1.00 µm	CP8913
		VF-1301ms, 30 m x 0.25 mm, 1.00 µm	CP9054

(Continued)

Drinking Water

EPA Methods	Application	Recommended Column	Part No.
552	Determination of haloacetic acids in drinking water by liquid-liquid extraction, derivatization, and gas chromatography with electron-capture detection	DB-35ms Ultra Inert, 30 m x 0.32 mm, 0.25 µm	123-3832UI
		DB-XLB, 30 m x 0.32 mm, 0.50 µm	123-1236
		DB-1701, 30 m x 0.25 mm, 0.25 µm	122-0732
		DB-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	122-5532UI
		HP-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	19091S-433UI
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
552.1	Determination of haloacetic acids and dalapon in drinking water by ion-exchange liquid-solid extraction and gas chromatography with an electron-capture detector	DB-CLP1, 30 m x 0.32 mm, 0.25 µm	123-8232
		DB-CLP2, 30 m x 0.32 mm, 0.5 µm	123-8336
		DB-35ms Ultra Inert, 30 m x 0.32 mm, 0.25 µm	123-3832UI
		DB-XLB, 30 m x 0.32 mm, 0.50 µm	123-1236
552.2	Determination of haloacetic acids and dalapon in drinking water by liquid-liquid extraction, derivatization GC with electron-capture detection	DB-CLP1, 30 m x 0.32 mm, 0.25 µm	123-8232
		DB-CLP2, 30 m x 0.32 mm, 0.5 µm	123-8336
		DB-35ms Ultra Inert, 30 m x 0.32 mm, 0.25 µm	123-3832UI
		DB-XLB, 30 m x 0.32 mm, 0.50 µm	123-1236
		VF-1701ms, 30 m x 0.25 mm, 0.25 µm	CP9151
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
552.3	Determination of haloacetic acids and dalapon in drinking water by liquid-liquid microextraction, derivatization, and GC with electron-capture detection	DB-CLP1, 30 m x 0.32 mm, 0.25 µm	123-8232
		DB-CLP2, 30 m x 0.32 mm, 0.5 µm	123-8336
		DB-5ms, 30 m x 0.25 mm, 0.25 µm	122-5532
		DB-1701, 30 m x 0.25 mm, 0.25 µm	122-0732
		VF-1701ms, 30 m x 0.25 mm, 0.25 µm	CP9151
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
556	Determination of carbonyl compounds in drinking water by pentafluorobenzylhydroxylamine derivatization and capillary GC with electron-capture detection	DB-5ms, 30 m x 0.25 mm, 0.25 µm	122-5532
		DB-1701, 30 m x 0.25 mm, 0.25 µm	122-0732
		VF-1701ms, 30 m x 0.25 mm, 0.25 µm	CP9151
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944

Waste Water

EPA Method	Application	Column	Part No.
601	Purgeable halocarbons	DB-VRX, 60 m x 0.25 mm, 1.40 µm	122-1564
		DB-624, 75 m x 0.45 mm, 2.55 µm	124-1374
		DB-624, 60 m x 0.25 mm, 1.40 µm	122-1364
		VF-624ms, 75 m x 0.53 mm, 3.00 µm	CP9108
		VF-624ms, 60 m x 0.32 mm, 1.80 µm	CP9105
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
602	Purgeable aromatics	DB-624, 75 m x 0.53 mm, 3.00 µm	125-1374
		DB-624, 30 m x 0.25 mm, 1.40 µm	122-1334
		DB-VRX, 30 m x 0.25 mm, 1.40 µm	122-1534
		VF-624ms, 75 m x 0.53 mm, 3.00 µm	CP9108
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
		VF-624ms, 30 m x 0.25 mm, 1.40 µm	CP9102
603	Acrolein and acrylonitrile	DB-624, 30 m x 0.25 mm, 1.40 µm	122-1334
		DB-VRX, 30 m x 0.25 mm, 1.40 µm	122-1534
		VF-WAXms, 30 m x 0.25 mm, 1.00 µm	CP9206
		VF-624ms, 30 m x 0.25 mm, 1.40 µm	CP9102
604	Phenols	DB-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	122-5532UI
		DB-XLB, 30 m x 0.25 mm, 0.25 µm	122-1232
		VF-5ms, 60 m x 0.32 mm, 1.80 µm	CP9105
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
605	Benzidines	DB-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	122-5532UI
		DB-608, 30 m x 0.25 mm, 0.25 µm	122-6832
606	Phthalate esters	DB-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	122-5532UI
		DB-608, 30 m x 0.25 mm, 0.25 µm	122-6832
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
607	Nitrosamines	DB-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	122-5532UI
		CP-Sil 8 CB for Amines, 30 m x 0.32 mm, 1.00 µm	CP7596

(Continued)

TIPS & TOOLS

Get fast and easy GC pressure and flow calculations at your fingertips with Agilent's GC Calculator Application – **www.agilent.com/chem/gcapp**



Waste Water

EPA Method	Application	Column	Part No.
608	Organochlorine pesticides and PCBs	DB-35ms Ultra Inert, 30 m x 0.32 mm, 0.25 µm	123-3832UI
		DB-XLB, 30 m x 0.32 mm, 0.50 µm	123-1236
		DB-17ms, 30 m x 0.32 mm, 0.25 µm	123-4732
		VF-5 Pesticides, 30 m x 0.25 mm, 0.25 µm	CP9074
		VF-1701 Pesticides, 30 m x 0.25 mm, 0.25 µm	CP9070
		VF-17ms, 30 m x 0.25 mm, 0.25 µm	CP8982
609	Nitroaromatics and isophorone	HP-5ms, 30 m x 0.25 mm, 0.50 µm	19091S-133
		DB-5ms, 30 m x 0.25 mm, 0.50 µm	122-5536
		DB-608, 30 m x 0.25 mm, 0.25 µm	122-6832
		VF-5ms, 30 m x 0.53 mm, 1.50 µm	CP8976
		VF-5ms, 30 m x 0.25 mm, 0.50 µm	CP8945
610	Polynuclear aromatic hydrocarbons	DB-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	122-5532UI
		DB-5ms, 30 m x 0.32 mm, 0.25 µm	123-5532
		DB-17ms, 30 m x 0.25 mm, 0.25 µm	122-4732
		VF-17ms, 30 m x 0.25 mm, 0.25 µm	CP8982
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
611	Haloethers	VF-5ms, 30 m x 0.53 mm, 1.50 µm	CP8976
		VF-5ms, 30 m x 0.25 mm, 0.50 µm	CP8945
612	Chlorinated hydrocarbons	DB-5ms, 30 m x 0.32 mm, 0.50 µm	123-5536
		HP-5ms, 30 m x 0.32 mm, 0.50 µm	19091S-113
		DB-1, 30 m x 0.32 mm, 0.50 µm	123-103E
		VF-5ms, 30 m x 0.25 mm, 0.10 µm	CP8943
		VF-35ms, 30 m x 0.25 mm, 0.25 µm	CP8877
		VF-200ms, 30 m x 0.25 mm, 1.00 µm	CP8860
613	2,3,7,8-Tetrachlorodibenzo-p-dioxin	DB-5ms Ultra Inert, 60 m x 0.25 mm, 0.25 µm	122-5562UI
		CP-Sil 88 for Dioxins, 50 m x 0.25 mm, 0.20 µm	CP7588
		VF-5ms, 60 m x 0.25 mm, 0.10 µm	CP8948
614	The determination of organophosphorus pesticides in municipal and industrial wastewater	DB-35ms, 30 m x 0.25 mm, 0.25 µm	122-3832
		DB-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	122-5532UI
615	Chlorinated herbicides	DB-35ms Ultra Inert, 30 m x 0.32 mm, 0.25 µm	123-3832UI
		VF-1701 Pesticides, 30 m x 0.25 mm, 0.25 µm	CP9070
		VF-5 Pesticides, 30 m x 0.25 mm, 0.25 µm	CP9074

(Continued)

Waste Water

EPA Method	Application	Column	Part No.
619	Triazine pesticides	DB-35ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	122-3832UI
		DB-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	122-5532UI
		VF-17ms, 30 m x 0.25 mm, 0.50 µm	CP8983
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
622	The determination of organophosphorus pesticides in municipal and industrial wastewater	DB-35ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	122-3832UI
		DB-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	122-5532UI
624	Purgeables	DB-VRX, 60 m x 0.25 mm, 1.40 µm	122-1564
		DB-624, 60 m x 0.25 mm, 1.40 µm	122-1364
		HP-VOC, 60 m x 0.20 mm, 1.10 µm	19091R-306
		DB-VRX, 20 m x 0.18 mm, 1.00 µm	121-1524
		DB-624, 20 m x 0.18 mm, 1.00 µm	121-1324
		VF-624ms, 75 m x 0.53 mm, 3.00 µm	CP9108
		VF-624ms, 60 m x 0.32 mm, 1.80 µm	CP9105
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
625	Base/neutrals and acids	HP-5ms Ultra Inert, 30 m x 0.25 mm, 0.50 µm	19091S-133UI
		VF-5 Pesticides, 30 m x 0.25 mm, 0.25 µm	CP9074
		VF-1701 Pesticides, 30 m x 0.25 mm, 0.25 µm	CP9070
		VF-200ms, 30 m x 0.25 mm, 0.25 µm	CP8858
1613	Tetra- through octa-chlorinated dioxins and furans by isotope dilution HRGC/HRMS	DB-5ms Ultra Inert, 60 m x 0.25 mm, 0.25 µm	122-5562UI
		CP-Sil 88 for Dioxins, 50 m x 0.25 mm, 0.20 µm	CP7588
		VF-5ms, 60 m x 0.25 mm, 0.25 µm	CP8960
1624	Volatile organic compounds by isotope dilution GC/MS	DB-624, 60 m x 0.25 mm, 1.40 µm	122-1364
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
1625	Semivolatile organic compounds by isotope dilution GC/MS	DB-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	122-5532UI
		HP-5ms Ultra Inert, 30 m x 0.25 mm, 0.25 µm	19091S-433UI
		VF-5ms, 30 m x 0.25 mm, 0.25 µm	CP8944
8021	Volatile halogenated & aromatic organic compounds	DB-VRX, 60 m x 0.25 mm, 1.40 µm	122-1564
		DB-624, 60 m x 0.25 mm, 1.40 µm	122-1364

(Continued)

Solid Waste

EPA Method	Application	Column	Part No.
8010	Volatile halogenated organic compounds list by EPA method 8021	DB-VRX 60 m x 0.25 mm, 1.40 µm	122-1564
		DB-608 30 m x 0.53 mm, 0.50 µm	125-6837
8011	1,2-Dibromoethane and 1,2-dibromo-3-chloropropane by microextraction and GC	DB-624 30 m x 0.25 mm, 1.40 µm	122-1334
		DB-624 Ultra Inert 30 m x 0.25 mm, 1.4 µm	122-1334UI
		DB-VRX 30 m x 0.25 mm, 1.40 µm	122-1534
		VF-1ms 30 m x 0.32 mm, 0.25 µm	CP8924
8015	Nonhalogenated organics by GC	DB-624 30 m x 0.25 mm, 1.40 µm	122-1334
		DB-624 Ultra Inert 30 m x 0.25 mm, 1.4 µm	122-1334UI
		DB-VRX 30 m x 0.25 mm, 1.40 µm	122-1534
8015c	Nonhalogenated organics by GC	DB-WAX 30 m x 0.25 mm, 0.50 µm	122-7033
		DB-5 30 m x 0.25 mm, 1.00 µm	122-5033
		HP-5 30 m x 0.25 mm, 1.00 µm	19091J-233
		DB-608 30 m x 0.53 mm, 1.00 µm	CP9215
		CP-Sil 8 CB 30 m x 0.53 mm, 1.50 µm	CP8736
8020	Volatile aromatic organic compounds list by EPA method 8021	DB-624 30 m x 0.25 mm, 1.40 µm	122-1334
		DB-624 Ultra Inert 30 m x 0.25 mm, 1.4 µm	122-1334UI
		DB-VRX 30 m x 0.25 mm, 1.40 µm	122-1534
8021, CLP Volamines	Volatile halogenated & aromatic organic compounds	DB-VRX 60 m x 0.25 mm, 1.40 µm	122-1564
		DB-608 30 m x 0.53 mm, 0.50 µm	125-6837

(Continued)

Solid Waste

EPA Method	Application	Column	Part No.
8021b	Aromatic and halogenated volatiles by GC	VF-624ms 60 m x 0.53 mm, 3.00 µm	CP9107
		VF-624ms 60 m x 0.25 mm, 1.40 µm	CP9103
8031	Acrylonitrile by GC	DB-624 30 m x 0.25 mm, 1.40 µm	122-1334
		DB-624 Ultra Inert 30 m x 0.25 mm, 1.4 µm	122-1334UI
		DB-VRX 30 m x 0.25 mm, 1.40 µm	122-1534
		PoraBOND Q 25 m x 0.53 mm, 10.00 µm	CP7354
8032	Acrylamide by GC	CP-Wax 58 FFAP CB 25 m x 0.53 mm, 2.00 µm	CP7654
8033	Acetonitrile by GC with nitrogen-phosphorus detection	DB-WAX 15 m x 0.25 mm, 0.50 µm	122-7013
		HP-INNOWax 15 m x 0.25 mm, 0.50 µm	19091N-231
		VF-WAXms 15 m x 0.53 mm, 1.00 µm	CP9226
8040, 8041, 8041a	Phenols by gas chromatography	DB-5ms 30 m x 0.25 mm, 0.25 µm	122-5532
		DB-XLB 30 m x 0.25 mm, 0.25 µm	122-1232
		VF-5ms 30 m x 0.53 mm, 1.50 µm	CP8976
		VF-1701ms 30 m x 0.53 mm, 1.00 µm	CP9171
		VF-17ms 30 m x 0.53 mm, 1.00 µm	CP9001
8060	Phthalate esters	DB-5ms 30 m x 0.25 mm, 0.25 µm	122-5532
		DB-608 30 m x 0.53 mm, 0.50 µm	125-6837
8061	Phthalate esters by GC with electron capture detection (GC/ECD)	DB-5ms 30 m x 0.25 mm, 0.25 µm	122-5532
		DB-608 30 m x 0.53 mm, 0.50 µm	125-6837
		VF-1701ms 30 m x 0.53 mm, 1.00 µm	CP9171

(Continued)

Solid Waste

EPA Method	Application	Column	Part No.
8070, 8070a	Nitrosamines by gas chromatography	DB-5ms 30 m x 0.25 mm, 0.25 µm	122-5532
		CP-Sil 8 CB for Amines 30 m x 0.53 mm, 1.00 µm	CP7597
		VF-17ms 30 m x 0.53 mm, 1.50 µm	CP9002
8081, 8081a	Organochlorine pesticides by gas chromatography	DB-CLP1 30 m x 0.32 mm, 0.25 µm	123-8232
		DB-CLP2 30 m x 0.32 mm, 0.5 µm	123-8336
		DB-35ms 30 m x 0.32 mm, 0.25 µm	123-3832
		DB-XLB 30 m x 0.32 mm, 0.50 µm	123-1236
		VF-5ms 30 m x 0.25 mm, 1.00 µm	CP8946
		VF-35ms 30 m x 0.25 mm, 1.00 µm	CP8879
8082, CLP Pesticides, 8082a	Polychlorinated biphenyls (PCBs) by gas chromatography	DB-CLP1 30 m x 0.32 mm, 0.25 µm	123-8232
		DB-CLP2 30 m x 0.32 mm, 0.5 µm	123-8336
		DB-35ms 30 m x 0.32 mm, 0.25 µm	123-3832
		DB-XLB 30 m x 0.32 mm, 0.50 µm	123-1236
		VF-5ms 30 m x 0.25 mm, 1.00 µm	CP8946
		VF-35ms 30 m x 0.25 mm, 1.00 µm	CP8879
8090	Nitroaromatics and isophorone	DB-5ms 30 m x 0.25 mm, 1.00 µm	122-5533
		DB-608 30 m x 0.53 mm, 0.50 µm	125-6837
		HP-5ms 30 m x 0.25 mm, 0.50 µm	19091S-133
8091	Nitroaromatics and cyclic ketones by GC	VF-5ms 30 m x 0.53 mm, 1.50 µm	CP8976
		VF-1701ms 30 m x 0.53 mm, 1.00 µm	CP9171

(Continued)

Solid Waste

EPA Method	Application	Column	Part No.
8095	Explosives by GC	DB-225 15 m x 0.53 mm, 1.00 µm	125-2212
		HP-5 15 m x 0.53 mm, 1.50 µm	19095J-321
		DB-5 15 m x 0.53 mm, 1.50 µm	125-5012
		VF-5ms 15 m x 0.53 mm, 1.50 µm	CP8973
		VF-1ms 15 m x 0.53 mm, 1.50 µm	CP8967
		VF-200ms 15 m x 0.53 mm, 1.00 µm	CP8866
8100	Polynuclear aromatic hydrocarbons	DB-5ms 30 m x 0.25 mm, 0.25 µm	122-5532
		DB-5ms 30 m x 0.32 mm, 0.25 µm	123-5532
		DB-1ms 30 m x 0.25 mm, 0.25 µm	122-0132
		DB-17ms 30 m x 0.25 mm, 0.25 µm	122-4732
		VF-5ms 30 m x 0.25 mm, 0.25 µm	CP8944
8111	Haloethers by GC	DB-5ms 30 m x 0.25 mm, 1.00 µm	122-5533
		HP-5ms 30 m x 0.25 mm, 0.50 µm	19091S-133
		DB-1701 30 m x 0.25 mm, 1.00 µm	122-0733
		VF-5ms 15 m x 0.53 mm, 1.50 µm	CP8973
		VF-1701ms 30 m x 0.53 mm, 1.00 µm	CP9171
8120	Chlorinated hydrocarbons by gas chromatography	DB-5ms 30 m x 0.32 mm, 0.50 µm	123-5536
		HP-5ms 30 m x 0.32 mm, 0.50 µm	19091S-113
		DB-1 30 m x 0.32 mm, 0.50 µm	123-103E

(Continued)

Solid Waste

EPA Method	Application	Column	Part No.
8121	Chlorinated hydrocarbons by GC: capillary column technique	DB-5ms 30 m x 0.32 mm, 0.50 µm	123-5536
		HP-5ms 30 m x 0.32 mm, 0.50 µm	19091S-113
		DB-1 30 m x 0.32 mm, 0.50 µm	123-103E
		VF-200ms 30 m x 0.53 mm, 1.00 µm	CP8868
		VF-WAXms 30 m x 0.53 mm, 1.00 µm	CP9215
		VF-5ms 30 m x 0.53 mm, 1.50 µm	CP8976
		VF-1701ms 30 m x 0.53 mm, 1.00 µm	CP9171
8131	Aniline and selected derivatives by GC	DB-5ms Ultra Inert 30 m x 0.25 mm, 1.00 µm	122-5533UI
		HP-5ms Ultra Inert 30 m x 0.25 mm, 0.50 µm	19091S-133UI
		VF-5ms 30 m x 0.25 mm, 0.25 µm	CP8944
		CP-Sil 8 CB for Amines 30 m x 0.25 mm, 0.25 µm	CP7598
8140	Organophosphorus pesticides by GC-NPD	DB-35ms 30 m x 0.25 mm, 0.25 µm	122-3832
		DB-5ms 30 m x 0.25 mm, 0.25 µm	122-5532
		VF-5ms 30 m x 0.25 mm, 0.25 µm	CP8944
8141a, 8141b	Organophosphorus compounds by gas chromatography: capillary column technique	DB-35ms 30 m x 0.25 mm, 0.25 µm	122-3832
		DB-5ms 30 m x 0.25 mm, 0.25 µm	122-5532
		VF-200ms 30 m x 0.53 mm, 1.00 µm	CP8868
		VF-35ms 30 m x 0.53 mm, 1.00 µm	CP8888
		VF-5ms 30 m x 0.53 mm, 1.00 µm	CP8975
		VF-1ms 30 m x 0.53 mm, 1.00 µm	CP8969

(Continued)

Solid Waste

EPA Method	Application	Column	Part No.
8150	Chlorinated herbicides	DB-35ms 30 m x 0.32 mm, 0.25 µm	123-3832
8151, 8151b	Chlorinated herbicides by GC using methylation or pentafluorobenzylation derivatization: capillary column technique	DB-CLP1 30 m x 0.32 mm, 0.25 µm	123-8232
		DB-CLP2 30 m x 0.32 mm, 0.5 µm	123-8336
		DB-35ms Ultra Inert 30 m x 0.32 mm, 0.25 µm	123-3832UI
		DB-5ms Ultra Inert 30 m x 0.32 mm, 0.25 µm	123-5532UI
		HP-5ms Ultra Inert 30 m x 0.32 mm, 0.25 µm	19091S-413UI
		VF-5 Pesticides 30 m x 0.25 mm, 0.25 µm	CP9074
		VF-5ms 30 m x 0.32 mm, 1.00 µm	CP8957
		VF-35ms 30 m x 0.25 mm, 0.25 µm	CP8877
		VF-1701 Pesticides 30 m x 0.25 mm, 0.25 µm	CP9070
8240	Volatile chlorinated and aromatic hydrocarbons	DB-VRX 20 m x 0.18 mm, 1.00 µm	121-1524
		DB-624 20 m x 0.18 mm, 1.00 µm	121-1324
		DB-624 Ultra Inert 60 m x 0.25 mm, 1.4 µm	122-1364UI
		DB-VRX 60 m x 0.25 mm, 1.40 µm	122-1564
		DB-608 30 m x 0.53 mm, 0.50 µm	125-6837
		HP-VOC 60 m x 0.20 mm, 1.10 µm	19091R-306
		VF-624ms 60 m x 0.25 mm, 1.40 µm	CP9103
		DB-624 Ultra Inert 60 m x 0.25 mm, 1.4 µm	122-1364UI
8260/CLP-VOCs	Volatile organic compounds by gas chromatography/mass spectroscopy (GC/MS): capillary column technique method	DB-VRX 60 m x 0.25 mm, 1.40 µm	122-1564
		DB-608 30 m x 0.53 mm, 0.50 µm	125-6837
		DB-VRX 20 m x 0.18 mm, 1.00 µm	121-1524
		DB-624 20 m x 0.18 mm, 1.00 µm	121-1324

(Continued)

Solid Waste

EPA Method	Application	Column	Part No.
8260b	Volatile organic compounds by GC/MS	DB-VRX 60 m x 0.25 mm, 1.40 µm	122-1564
		DB-608 30 m x 0.53 mm, 0.50 µm	125-6837
		DB-VRX 20 m x 0.18 mm, 1.00 µm	121-1524
		DB-624 20 m x 0.18 mm, 1.00 µm	121-1324
		VF-5ms 30 m x 0.25 mm, 1.00 µm	CP8946
		VF-624ms 60 m x 0.32 mm, 1.80 µm	CP9105
		DB-624 Ultra Inert 60 m x 0.32 mm, 1.8 µm	123-1364UI
8261	Volatile organic compounds by vacuum distillation in combination with GC/MS spectrometry (VD/GC/MS)	DB-VRX 60 m x 0.25 mm, 1.40 µm	122-1564
		DB-608 30 m x 0.53 mm, 0.50 µm	125-6837
		DB-VRX 20 m x 0.18 mm, 1.00 µm	121-1524
		DB-624 20 m x 0.18 mm, 1.00 µm	121-1324
		DB-624 Ultra Inert 20 m x 0.18 mm, 1 µm	121-1324UI
		VF-624ms 60 m x 0.25 mm, 1.40 µm	CP9103
8270, 8270d	Semivolatile organic compounds by gas chromatography/mass spectrometry (GC/MS)	DB-UI 8270D 30 m x 0.25 mm, 0.25 µm	122-9732
		DB-UI 8270D 20 m x 0.18 mm, 0.36 µm	121-9723
		HP-5ms 30 m x 0.25 mm, 0.50 µm	19091S-133
		VF-5ms 30 m x 0.25 mm, 0.25 µm	CP8944
		VF-5ms 30 m x 0.25 mm, 0.50 µm	CP8945
		VF-5ms 30 m x 0.25 mm, 1.00 µm	CP8946

(Continued)

Solid Waste

EPA Method	Application	Column	Part No.
8275a	Semivolatile organic compounds (PAHs and PCBs) in soils/sludges and solid wastes using thermal extraction/gas chromatography/mass spectrometry (TE/GC/MS)	DB-5ms 30 m x 0.25 mm, 1.00 µm	122-5533
		HP-5ms 30 m x 0.25 mm, 0.50 µm	19091S-133
		VF-5ms 30 m x 0.25 mm, 0.25 µm	CP8944
		VF-5ms 30 m x 0.25 mm, 0.50 µm	CP8945
		VF-5ms 30 m x 0.25 mm, 1.00 µm	CP8946
8280b	Polychlorinated dibenzo-p-dioxins (PCDDs) and polychlorinated dibenzofurans (PCDFs) by high resolution gas chromatography/low resolution mass spectrometry (HRGC/LRMS)	DB-5ms Ultra Inert 60 m x 0.25 mm, 0.25 µm	122-5562UI
		CP-Sil 8 CB 30 m x 0.25 mm, 0.25 µm	CP8751
8290b	Polychlorinated dibenzo-p-dioxins (PCDDs) and polychlorinated dibenzofurans (PCDFs) by high resolution gas chromatography/high resolution mass spectrometry (HRGC/HRMS)	DB-5ms Ultra Inert 60 m x 0.25 mm, 0.25 µm	122-5562UI
		CP-Sil 8 CB 30 m x 0.25 mm, 0.25 µm	CP8751
		CP-Sil 88 for Dioxins 50 m x 0.25 mm, 0.20 µm	CP7588
8410	Gas chromatography/Fourier transform infrared (GC/FT-IR) spectrometry for semivolatile organics: capillary column	HP-5ms 30 m x 0.32 mm, 1.00 µm	19091S-213
		DB-5ms 30 m x 0.32 mm, 1.00 µm	123-5533
		VF-5ms 30 m x 0.32 mm, 0.25 µm	CP8955
8430	Analysis of bis(2-chloroethyl) ether and hydrolysis products by direct aqueous injection (GC/FT-IR)	DB-WAX 30 m x 0.25 mm, 0.50 µm	122-7033
		HP-INNOWax 30 m x 0.25 mm, 0.50 µm	19091N-233
		VF-WAXms 30 m x 0.53 mm, 1.00 µm	CP9215

TIPS & TOOLS

The Agilent J&W DB-624UI GC columns are optimized for fast analysis of volatile compounds. Learn more at **www.agilent.com/chem/624UI**

United States Pharmacopoeia (USP) GC Phases		
USP	**Phase Composition**	**Agilent Phase Recommendation**
G1	Dimethylpolysiloxane oil	HP-1*, DB-1*, HP-1ms*, DB-1ms*, VF-1ms, CP-Sil 5 CB, CP-Sil 5 CB Low Bleed/MS
G2	Dimethylpolysiloxane gum	HP-1*, DB-1*, HP-1ms*, DB-1ms*, VF-1ms, CP-Sil 5 CB, CP-Sil 5 CB Low Bleed/MS, CP-SimDist
G3	50% Phenyl 50% methylpolysiloxane	DB-17*, HP-50+*, VF-17ms, CP-Sil 24 CB, CP-Sil 24 CB Low Bleed/MS
G5	3-cyanopropyl polysiloxane	DB-23, VF-23ms, Select for FAME, CP-Sil 88
G6	Trifluoropropylmethylpolysilicone	DB-200, DB-210, VF-200ms
G7	50% 3-cyanopropyl 50% phenylmethylsilicone	DB-225, DB-225ms, CP-Sil 43 CB
G8	80% Bis(3-cyanopropyl) 20% 3-cyanopropylphenylpolysiloxane or 90% 3-cyanopropyl 10% phenylmethylsiloxane	HP-88, VF-23ms
G14	Polyethylene glycol (average molecular weight of 950-1,050)	DB-WAX, VF-WAXms, CP-Wax 52 CB
G15	Polyethylene glycol (average molecular weight of 3,000-3,700)	DB-WAX, VF-WAXms, CP-Wax 52 CB
G16	Polyethylene glycol (average molecular weight of 15,000)	DB-WAX*, VF-WAXms, CP-Wax 52 CB
G17	75% Phenyl 25% methylpolysiloxane	DB-17, HP-50+, VF-17ms, CP-Sil 24 CB, CP-Sil 24 CB Low Bleed/MS
G19	25% Phenyl 25% cyanopropylmethylsilicone	DB-225*, DB-225ms, CP-Sil 43 CB
G20	Polyethylene glycol (average molecular weight of 380-420)	DB-WAX, VF-WAXms, CP-Wax 52 CB
G25	Polyethylene glycol TPA (Carbowax 20M terephthalic acid)	DB-FFAP*, HP-FFAP*, CP-Wax 58 (FFAP) CB, CP-FFAP CB
G27	5% Phenyl 95% methylpolysiloxane	DB-5*, HP-5*, HP-5ms*, DB-5ms, VF-5ms, VF-5ht, CP-Sil 8 CB, CP-Sil 8 CB Low Bleed/MS
G28	25% Phenyl 75% methylpolysiloxane	DB-35, HP-35, DB-35ms, VF-35ms
G32	20% Phenylmethyl 80% dimethylpolysiloxane	DB-35, HP-35, DB-35ms, VF-35ms
G35	Polyethylene glycol & diepoxide esterified with nitroterepthalic acid	DB-FFAP*, HP-FFAP*, CP-Wax 58 (FFAP) CB, CP-FFAP CB
G36	1% Vinyl 5% phenylmethylpolysiloxane	DB-5, HP-5, HP-5ms, DB-5ms, VF-5ms, VF-5ht, CP-Sil 8 CB, CP-Sil 8 CB Low Bleed/MS
G38	Phase G1 plus a tailing inhibitor	DB-1, HP-1, HP-1ms, DB-1ms, VF-1ms, CP-Sil 5 CB, CP-Sil 5 CB Low Bleed/MS
G39	Polyethylene glycol (average molecular weight of 1,500)	DB-WAX, VF-WAXms, CP-Wax 52 CB
G41	Phenylmethyldimethylsilicone (10% phenyl substituted)	DB-5, HP-5, HP-5ms, DB-5ms, VF-5ms, VF-5ht, CP-Sil 8 CB, CP-Sil 8 CB Low Bleed/MS
G42	35% Phenyl 65% dimethylvinylsiloxane	DB-35*, HP-35*, DB-35ms, VF-35ms
G43	6% Cyanopropylphenyl 94% dimethylpolysiloxane	DB-624*, DB-1301, VF-624ms, VF-1301ms, CP-1301, CP-Select 624 CB
G45	Divinylbenzene-ethylene glycol-dimethacrylate	HP-PLOT U*, CP-PoraBOND U, CP-PoraPLOT U
G46	14% Cyanopropylphenyl 86% methylpolysiloxane	DB-1701*, VF-1701ms, CP-Sil 19 CB, CP-Sil 19 CB Low Bleed/MS

*Indicates an exact equivalent

TIPS & TOOLS

Gain extra confidence to meet high standards with Agilent's solution for the revised USP <467>. Visit **www.agilent.com/chem/usp467**

ASTM Methods

Method	Title	Recommended Agilent Column	Part No.
D 1945	Standard Test Method for the Analysis of Natural Gas by GC	HP PLOT, 15 m x 0.53 mm, 50.00 µm	19095P-MS9
		HP PLOT Q, 15 m x 0.53 mm, 40.00 µm	19095P-QO3
		CP-Molsieve 5Å, 10 m x 0.53 mm, 50.00 µm	CP7537
		PoraPLOT Q-HT, 10 m x 0.53 mm, 20.00 µm	CP7558
D 1946	Standard Test Method for the Analysis of Reformed Gas by GC	HP PLOT, 15 m x 0.53 mm, 50.00 µm	19095P-MS9
		HP PLOT Q, 15 m x 0.53 mm, 40.00 µm	19095P-QO3
		CP-Molsieve 5Å, 10 m x 0.53 mm, 50.00 µm	CP7537
		CP-Molsieve 5Å, 25 m x 0.25 mm, 30.00 µm	CP7533
D 1983	Standard Test Method for Fatty Acid Composition by Gas-Liquid Chromatography of Methyl Esters	DB-WAX, 30 m x 0.25 mm, 0.25 µm	122-7032
D 2163	Standard Test Method for the Analysis of Liquified Petroleum (LP) Gases and Propene Concentrates by GC	HP PLOT Al2O3 "KCl", 30 m x 0.53 mm, 15.00 µm	19095P-K23
		HP PLOT Al2O3 "S", 30 m x 0.53 mm, 15.00 µm	19095P-S23
D 2195	Standard Test Methods for Pentaerythritol	CP-Sil 5 CB, 30 m x 0.53 mm, 1.50 µm	CP8735
D 2268	Standard Test Method for Analysis of High-Purity n-Heptane and Isooctane by Capillary GC	DB-1, 60 m x 0.25 mm, 0.50 µm	122-106E
D 2306	Standard Test Method for C8 Aromatic Hydrocarbons by GC	HP-INNOWax, 60 m x 0.25 mm, 0.25 µm	19091N-136
D 2360	Standard Test Method for Trace Impurities in Monocyclic Aromatic Hydrocarbons by GC	HP-INNOWax, 60 m x 0.32 mm, 0.25 µm	19091N-116
D 2426	Standard Test Method for Butadiene Dimer and Styrene in Butadiene Concentrates by GC	DB-1, 30 m x 0.53 mm, 5.00 µm	125-1035
		CP-Sil 5 CB, 30 m x 0.53 mm, 1.50 µm	CP8735
D 2427	Standard Test Method for Determination of C_2 through C_5 Hydrocarbons in Gasoline by GC	DB-1, 30 m x 0.53 mm, 5.00 µm	125-1035
		GS-Alumina, 30 m x 0.53 mm	115-3532
		CP-Al2O3/KCl, 50 m x 0.53 mm, 10.00 µm	CP7518
D 2245	Standard Test Method for Identification of Oils and Oil Acids in Solvent-Reducible Paints	CP-Sil 88 for FAME, 50 m x 0.25 mm, 0.20 µm	CP7488
D 2504	Standard Test Method for Noncondensable Gases in C_2 and Lighter Hydrocarbon Products by GC	HP PLOT, 30 m x 0.53 mm, 50.00 µm	19095P-MS0
		CarboBOND, 25 m x 0.53 mm, 10.00 µm	CP7374
D 2505	Standard Test Method for Ethylene, Other Hydrocarbons, and Carbon Dioxide in High-Purity Ethylene by GC	GS-GasPro, 60 m x 0.32 mm	113-4362

(Continued)

ASTM Methods

Method	Title	Recommended Agilent Column	Part No.
D 2580	Standard Test Method for Phenols in Water by Gas-Liquid Chromatography	CP-Sil 8 CB, 25 m x 0.32 mm, 0.40 µm	CP5850
		CP-FFAP CB, 25 m x 0.53 mm, 1.00 µm	CP7486
D 2593	Standard Test Method for Butadiene Purity and Hydrocarbon Impurities by GC	GS-Alumina, 30 m x 0.53 mm	115-3532
		CP-Al2O3/KCl, 50 m x 0.32 mm, 5.00 µm	CP7515
		CP-Al2O3/KCl, 50 m x 0.53 mm, 10.00 µm	CP7518
D 2712	Standard Test Method for for Hydrocarbon Traces in Propylene Concentrates by GC	GS-Alumina, 50 m x 0.53 mm	115-3552
D 2743	Standard Practices for Uniformity of Traffic Paint Vehicle Solids by Spectroscopy and Gas Chromatography	CP-Sil 88 for FAME, 50 m x 0.25 mm, 0.20 µm	CP7488
D 2804	Standard Test Method for Purity of Methyl Ethyl Ketone by GC	DB-WAX, 30 m x 0.53 mm, 1.00 µm	125-7032
		DB-210, 15 m x 0.53 mm, 1.00 µm	125-0212
		CP-WAX 52 CB, 30 m x 0.32 mm, 0.50 µm	CP8763
		CP-WAX 52 CB, 30 m x 0.53 mm, 1.00 µm	CP8738
D 2887	Standard Test Method for Boiling Range Distribution of Petroleum Fractions by GC	DB-2887, 10 m x 0.53 mm, 3.00 µm	125-2814
		CP-SimDist UltiMetal, 5 m x 0.53 mm, 0.88 µm	CP7570
		CP-SimDist UltiMetal, 10 m x 0.53 mm, 2.65 µm	CP7582
		CP-SimDist UltiMetal, 5 m x 0.53 mm, 0.17 µm	CP7532
Extended D 2887	Standard Test Method for Boiling Range Distribution of Petroleum Fractions by GC, to C_{60}	HP-1, 10 m x 0.53 mm, 0.88 µm	19095Z-021
		HP-1, 5 m x 0.53 mm, 0.88 µm	19095Z-020
D 2908	Standard Practice for Measuring Volatile Organic Matter in Water by Aqueous-Injection GC	CP-Select 624 CB, 30 m x 0.32 mm, 1.80 µm	CP7414
		CP-Select 624 CB, 75 m x 0.53 mm, 3.00 µm	CP7417
		CP-WAX 52 CB, 30 m x 0.32 mm, 0.50 µm	CP8763
		CP-WAX 52 CB, 30 m x 0.53 mm, 1.00 µm	CP8738
D 3054	Standard Test Method for Analysis of Cyclohexane by GC	DB-1, 60 m x 0.32 mm, 0.50 µm	123-106E
D 3168	Standard Practice for Qualitative Identification of Polymers in Emulsion Paints	CP-Sil 5 CB, 30 m x 0.32 mm, 1.00 µm	CP8760
		CP-Sil 5 CB, 30 m x 0.53 mm, 1.50 µm	CP8735
D 3257	Standard Test Method for Aromatics in Mineral Spirits by GC	DB-624, 30 m x 0.53 mm, 3.00 µm	125-1334
D 3271	Standard Practice for Direct Injection of Solvent-Reducible Paints into a Gas Chromatograph for Solvent Analysis	PoraPLOT Q, 25 m x 0.53 mm, 20.00 µm	CP7554
		CP-WAX 52 CB, 30 m x 0.53 mm, 1.00 µm	CP8738

(Continued)

ASTM Methods

Method	Title	Recommended Agilent Column	Part No.
D 3328	Standard Test Methods for Comparison of Waterborne Petroleum Oils by Gas Chromatography	CP-Sil 5 CB, 30 m x 0.32 mm, 3.00 µm	CP8687
		CP-Sil 5 CB, 30 m x 0.53 mm, 3.00 µm	CP8677
D 3329	Standard Test Method for Purity of Methyl Isobutyl Ketone by GC	DB-WAX, 30 m x 0.53 mm, 1.00 µm	125-7032
		DB-624, 30 m x 0.45 mm, 2.55 µm	124-1334
		CP-WAX 52 CB, 60 m x 0.53 mm, 1.00 µm	CP8798
D 3432	Standard Test Method for Unreacted Toluene Diisocyanates in Urethane Prepolymers and Coating Solutions by GC	HP-1ms, 30 m x 0.32 mm, 1.00 µm	19091S-713
D 3447	Standard Test Method for Purity of Halogentated Organic Solvents	DB-624, 30 m x 0.53 mm, 3.00 µm	125-1334
D 3452	Standard Practice for Rubber – Identification by Pyrolysis-Gas Chromatography	CP-Sil 5 CB, 30 m x 0.53 mm, 1.50 µm	CP8735
D 3465	Standard Test Method for Purity of Monomeric Plasticizers by Gas Chromatography	CP-Sil 5 CB, 25 m x 0.32 mm, 0.52 µm	CP8430
		CP-Sil 5 CB, 30 m x 0.53 mm, 1.50 µm	CP8735
D 3524	Standard Test Method for Diesel Fuel Diluent in Used Diesel Engine Oils by Gas Chromatography	CP-SimDist UltiMetal, 10 m x 0.53 mm, 0.53 µm	CP7592
D 3545	Standard Test Method for Alcohol Content and Purity of Acetate Esters by GC	DB-624, 30 m x 0.53 mm, 3.00 µm	125-1334
D 3606	Standard Test Method for Determination of Benzene and Toluene in Finished Motor and Aviation Gasoline by Gas Chromatography	VF-1ms, 15 m x 0.25 mm, 0.10 µm	CP8906
		CP-TCEP for Alcohols in Gasoline, 50 m x 0.25 mm, 0.40 µm	CP7525
D 3687	Standard Test Method for Analysis of Organic Vapors Collected by the Activated Charcoal Tube Adsorption Method	DB-WAX, 30 m x 0.53 mm, 1.00 µm	125-7032
		DB-WAX, 30 m x 0.45 mm, 0.85 µm	124-7032
		CP-WAX 52 CB, 30 m x 0.32 mm, 0.50 µm	CP8763
		CP-WAX 52 CB, 30 m x 0.53 mm, 1.00 µm	CP8738
D 3695	Standard Test Method for Volatile Alcohols in Water by Direct Aqueous-Injection GC	DB-WAX, 30 m x 0.53 mm, 1.00 µm	125-7032
		CP-SimDist UltiMetal, 10 m x 0.53 mm, 0.53 µm	CP7592
D 3710	Standard Test Method for Boiling Range Distribution of Gasoline and Gasoline Fractions by GC	DB-2887, 10 m x 0.53 mm, 3.00 µm	125-2814
D 3749	Standard Test Method for Residual Vinyl Chloride Monomer in Poly(Vinyl Chloride) Resins by Gas Chromatographic Headspace Technique	PoraBOND Q, 10 m x 0.32 mm, 5.00 µm	CP7350
		PoraBOND Q, 10 m x 0.53 mm, 10.00 µm	CP7353

(Continued)

ASTM Methods

Method	Title	Recommended Agilent Column	Part No.
D 3760	Standard Test Method for Analysis of Isopropylbenzene (Cumene) by GC	DB-WAX, 60 m x 0.32 mm, 0.25 µm	123-7062
		HP-1, 50 m x 0.32 mm, 0.52 µm	19091Z-115
		CP-Xylenes, 50 m x 0.53 mm	CP7428
D 3792	Standard Test Method for Water Content of Coatings by Direct Injection Into a Gas Chromatograph	PoraBOND Q, 25 m x 0.32 mm, 5.00 µm	CP7351
		PoraBOND Q, 25 m x 0.53 mm, 10.00 µm	CP7354
D 3797	Standard Test Method for Analysis of o-Xylene by GC	HP-INNOWax, 60 m x 0.32 mm, 0.50 µm	19091N-216
		CP-Xylenes, 50 m x 0.53 mm	CP7428
D 3798	Standard Test Method for Analysis of p-Xylene by GC	HP-INNOWax, 60 m x 0.32 mm, 0.50 µm	19091N-216
		CP-Xylenes, 50 m x 0.53 mm	CP7428
D 3871	Standard Test Method for Purgeable Organic Compounds in Water Using Headspace Sampling	DB-VRX, 75 m x 0.45 mm, 2.55 µm	124-1574
D 3876	Standard Test Method for Methoxyl and Hydroxypropyl Substitution in Cellulose Ether Products by Gas Chromatography	CP-Sil 5 CB, 30 m x 0.32 mm, 1.00 µm	CP8760
		CP-Sil 5 CB, 30 m x 0.53 mm, 1.50 µm	CP8735
D 3893	Standard Test Method for Purity of Methyl Amyl Ketone and Methyl Isoamyl Ketone by GC	DB-VRX, 30 m x 0.45 mm, 2.55 µm	124-1534
D 3973	Standard Test Method for Low-Molecular Weight Halogenated Hydrocarbons in Water	DB-VRX, 30 m x 0.45 mm, 2.55 µm	124-1534
D 4059	Standard Test Method for Analysis of Polychlorinated Biphenyls in Insulating Liquids by Gas Chromatography	CP-Sil 8 CB for PCB, 50 m x 0.25 mm, 0.25 µm	CP7482
D 4275	Standard Test Method for Determination of Butylated Hydroxy Toluene (BHT) in Polymers of Ethylene and Ethylene – Vinyl Acetate (EVA) Copolymers By Gas Chromatography	CP-Sil 5 CB, 30 m x 0.32 mm, 3.00 µm	CP8687
		CP-Sil 5 CB, 30 m x 0.53 mm, 3.00 µm	CP8677
D 4322	Standard Test Method for Residual Acrylonitrile Monomer Styrene-Acrylonitrile Copolymers and Nitrile Rubber by Headspace Gas Chromatography	PoraBOND Q, 25 m x 0.53 mm, 10.00 µm	CP7354
D 4367	Standard Test Method for Benzene in Hydrocarbon Solvents by Gas Chromatography	VF-1ms, 15 m x 0.25 mm, 0.10 µm	CP8906
		CP-TCEP for Alcohols in Gasoline, 50 m x 0.25 mm, 0.40 µm	CP7525
D 4415	Standard Test Method for Determination of Dimer in Acrylic Acid	DB-FFAP, 30 m x 0.32 mm, 0.25 µm	123-3232
D 4424	Standard Test Method for Butylene Analysis by GC	HP PLOT Al_2O_3 S, 50 m x 0.53 mm, 15.00 µm	19095P-S25
		CP-Al2O3/Na2SO4, 25 m x 0.53 mm, 10.00 µm	CP7567
D 4443	Standard Test Method for Residual Vinyl Chloride Monomer Content in PPB Range in Vinyl Chloride Homo- and Co-Polymers by Headspace GC	DB-VRX, 30 m x 0.45 mm, 2.55 µm	124-1534

(Continued)

ASTM Methods

Method	Title	Recommended Agilent Column	Part No.
D 4492	Standard Test Method for Analysis of Benzene by Gas Chromatography	CP-TCEP for Alcohols in Gasoline, 50 m x 0.25 mm, 0.40 µm	CP7525
D 4509	Standard Test Methods for Determining the 24-Hour Gas (AIR) Space Acetaldehyde Content of Freshly Blown PET Bottles	PoraBOND Q, 25 m x 0.32 mm, 5.00 µm	CP7351
		PoraBOND Q, 25 m x 0.53 mm, 10.00 µm	CP7354
D 4534	Test Method for Benzene Content of Cyclic Products by Gas Chromatography	CP-TCEP for Alcohols in Gasoline, 50 m x 0.25 mm, 0.40 µm	CP7525
D 4735	Standard Test Method for Determination of Trace Thiophene in Refined Benzene by GC	DB-FFAP, 30 m x 0.45 mm, 0.85 µm	124-3232
		CP-Wax 58 FFAP CB, 25 m x 0.53 mm, 1.00 µm	CP7614
D 4768	Standard Test Method for Analysis of 2,6-Ditertiary-Butyl Para-Cresol and 2,6-Ditertiary- Butyl Phenol in Insulating Liquids by Gas Chromatography	CP-Wax 58 FFAP CB, 25 m x 0.53 mm, 1.00 µm	CP7614
D 4864	Standard Test Method for Determination of Traces of Methanol in Propylene Concentrates by GC	DB-WAX, 30 m x 0.45 mm, 0.85 µm	124-7032
D 4947	Standard Test Method for Chlordane and Heptachlor Residues in Indoor Air	DB-5, 30 m x 0.53 mm, 1.50 µm	125-5032
		DB-608, 30 m x 0.53 mm, 0.83 µm	125-1730
D 4961	Standard Test Method for GC Analysis of Major Organic Impurities in Phenol Produced by the Cumene Process	DB-FFAP, 30 m x 0.45 mm, 0.85 µm	124-3232
		HP PLOT Q, 15 m x 0.53 mm, 40.00 µm	19095P-QO3
D 4983	Standard Test Method for Cyclohexylamine Morpholine and Diethylaminoethanol in Water and Condensed Steam by Direct Aqueous Injection GC	HP-5ms, 30 m x 0.32 mm, 1.00 µm	19091S-213
		CAM, 30 m x 0.53 mm, 1.00 µm	115-2132
D 5008	Standard Test Method for Ethyl Methyl Pentonal Content and Purity Value of 2-Ethylhexanol by GC	HP-1, 15 m x 0.53 mm, 5.00 µm	19095Z-621
		HP-INNOWax, 30 m x 0.32 mm, 0.25 µm	19091N-113
D 5060	Standard Test Method for Determining Impurities in High-Purity Ethylbenzene by GC	HP-INNOWax, 60 m x 0.32 mm, 0.50 µm	19091N-216
		CP-WAX 52 CB, 60 m x 0.32 mm, 0.50 µm	CP8773
D 5075	Standard Test Method for Nicotine in Indoor Air	DB-5, 30 m x 0.53 mm, 1.50 µm	125-5032
		DB-5, 30 m x 0.32 mm, 1.00 µm	123-5033
D 5134	Standard Test Method for Detailed Analysis of Petroleum Naphthas Through n-Nonane by Capillary GC	HP-PONA, 50 m x 0.20 mm, 0.50 µm	19091S-001
		CP-Sil PONA para ASTM D 5134, 50 m x 0.21 mm, 0.50 µm	CP7531
D 5135	Standard Test Method for Analysis of Styrene by Capillary GC	HP-INNOWax, 60 m x 0.32 mm, 0.50 µm	19091N-216
		CP-WAX 52 CB, 60 m x 0.32 mm, 0.50 µm	CP8773
D 5175	Standard Test Method for Organohalide Pesticides and Polychlorinated Biphenyls in Water by Microextraction and GC	DB-1, 30 m x 0.32 mm, 1.00 µm	123-1033
		DB-608, 30 m x 0.32 mm, 0.50 µm	123-1730
		DB-XLB, 30 m x 0.25 mm, 0.25 µm	122-1232

(Continued)

ASTM Methods

Method	Title	Recommended Agilent Column	Part No.
D 5303	Standard Test Method for Trace Carbonyl Sulfide in Propylene by GC	GS-GasPro, 30 m x 0.32 mm	113-4332
		HP PLOT Q, 30 m x 0.53 mm, 40.00 µm	19095P-QO4
D 5307	Standard Test Method for Determination of Boiling Range Distribution of Crude Petroleum by GC	HP-1, 7.5 m x 0.53 mm, 5.00 µm	19095Z-627
D 5310	Standard Test Method for Tar Acid Composition by Capillary GC	HP-5ms, 30 m x 0.25 mm, 0.25 µm	19091S-433
		DB-225ms, 30 m x 0.25 mm, 0.25 µm	122-2932
D 5316	Standard Test Method for 1, 2-Dibromoethane and 1, 2-Dibromo-3-Chloropropane in Water by Microextraction and GC	HP-1ms, 30 m x 0.32 mm, 1.00 µm	19091S-713
		DB-624, 30 m x 0.45 mm, 2.55 µm	124-1334
D 5317	Standard Test Method for Determination of Chlorinated Organic Acid Compounds in Water by GC with Electron Capture Detector	HP-5ms, 30 m x 0.25 mm, 0.25 µm	19091S-433
		DB-1701P, 30 m x 0.25 mm, 0.25 µm	122-7732
		DB-XLB, 30 m x 0.25 mm, 0.25 µm	122-1232
		DB-35ms, 30 m x 0.25 mm, 0.25 µm	122-3832
D 5320	Standard Test Method for Determination of 1, 1-Trichloroethane and Methylene Chloride in Stabilized Trichloroethylene and Tetrachloroethylene	DB-1, 30 m x 0.53 mm, 3.00 µm	125-1034
		DB-VRX, 30 m x 0.32 mm, 1.80 µm	123-1534
D 5399	Standard Test Method for Boiling Point Distribution of Hydrocarbon Solvents by GC	DB-2887, 10 m x 0.53 mm, 3.00 µm	125-2814
D 5441	Standard Test Method for Analysis of Methyl Tert-Butyl Ether (MTBD) by GC	HP-PONA, 50 m x 0.20 mm, 0.50 µm	19091S-001
		DB-Petro, 100 m x 0.25 mm, 0.50 µm	122-10A6E
D 5442	Standard Test Method for Analysis of Petroleum Waxes by GC	DB-1, 25 m x 0.32 mm, 0.25 µm	123-1022
		DB-5, 15 m x 0.25 mm, 0.25 µm	122-5012
D 5475	Standard Test Method for Nitrogen- and Phosphorus-Containing Pesticides in Water by GC with a Nitrogen Phosphorus Detector	HP-5ms, 30 m x 0.25 mm, 0.25 µm	19091S-433
		DB-1701P, 30 m x 0.25 mm, 0.25 µm	122-7732
		DB-XLB, 30 m x 0.25 mm, 0.25 µm	122-1232
		DB-35ms, 30 m x 0.25 mm, 0.25 µm	122-3832
D 5480	Standard Test Method for Engine Oil Volatility by GC	DB-PS1, 15 m x 0.53 mm, 0.15 µm	145-1011
D 5501	Standard Test Method for Determination of Ethanol Content of Denatured Fuel Ethanol by GC	HP-1, 100 m x 0.25 mm, 0.50 µm	19091Z-530
D 5504	Standard Test Method for Determination of Sulfur Compounds in Natural Gas and Gaseous Fuels by Gas Chromatography and Chemiluminescence	CP-Sil 5 CB for Sulfur, 30 m x 0.32 mm, 4.00 µm	CP7529

(Continued)

ASTM Methods

Method	Title	Recommended Agilent Column	Part No.
D 5507	Standard Test Method for Determination of Trace Organic Impurities in Monomer Grade Vinyl Chloride by Capillary Column/Multi-dimensional GC	HP PLOT Q, 15 m x 0.53 mm, 40.00 µm	19095P-QO3
		HP PLOT U, 30 m x 0.53 mm, 20.00 µm	19095P-UO4
D 5508	Standard Test Method for Determination of Residual Acrylonitrile Monomer in Styrene-Acyrlonitrile Co-polymer Resins and Nitrile-Butadiene Rubber by Headspace Capillary GC	HP PLOT Q, 30 m x 0.53 mm, 40.00 µm	19095P-QO4
D 5580	Standard Test Method for Determination of Benzene, Toluene, Ethylbenzene, p/m-Xylene, C_9 and Heavier Aromatics, and Total Aromatics in Finished Gasoline by GC	DB-1, 30 m x 0.53 mm, 5.00 µm	125-1035
		CP-TCEP for Alcohols in Gasoline, 50 m x 0.25 mm, 0.40 µm	CP7525
		CP-Sil 5 CB, 30 m x 0.53 mm, 5.00 µm	CP8775
		VF-1ms, 15 m x 0.25 mm, 0.10 µm	CP8906
D 5599	Standard Test Method for Determination of Oxygenates in Gasoline by GC and Oxygen Selective Flame Ionization Detection	DB-5, 30 m x 0.25 mm, 0.25 µm	122-5032
D 5623	Standard Test Method for Sulfur Compounds in Light Petroleum Liquids by GC and Sulfur Selective Detection	HP-1, 30 m x 0.32 mm, 4.00 µm	19091Z-613
D 5713	Standard Test Method for Analysis of High Purity Benzene for Cyclohexane Feedstock by Capillary GC	DB-Petro, 50 m x 0.20 mm, 0.50 µm	128-1056
D 5739	Standard Practice for Oil Spill Source Identification by GC and Positive Ion Electron Impact Low Resolution Mass Spectrometry	DB-5, 30 m x 0.25 mm, 0.25 µm	122-5032
		DB-TPH, 30 m x 0.32 mm, 0.25 µm	123-1632
D 5769	Standard Test Method for Determination of Benzene, Toluene, and Total Aromatics in Finished Gasoline by GC/MS	HP-1, 60 m x 0.25 mm, 1.00 µm	19091Z-236
D 5790	Standard Test Method for Measurement of Purgeable Organic Compounds in Water by Capillary Column GC/MS	DB-VRX, 60 m x 0.25 mm, 1.40 µm	122-1564
		DB-VRX, 20 m x 0.18 mm, 1.00 µm	121-1524
		DB-624, 60 m x 0.25 mm, 1.40 µm	122-1364
		DB-624, 20 m x 0.18 mm, 1.00 µm	121-1324
D 5812	Standard Test Method for Determination of Organochlorine Pesticides in Water by Capillary Column GC	HP-5ms, 30 m x 0.25 mm, 0.25 µm	19091S-433
		DB-1701P, 30 m x 0.25 mm, 0.25 µm	122-7732
		DB-XLB, 30 m x 0.25 mm, 0.25 µm	122-1232
		DB-35ms, 30 m x 0.25 mm, 0.25 µm	122-3832

(Continued)

ASTM Methods

Method	Title	Recommended Agilent Column	Part No.
D 5917	Standard Test Method for Trace Impurities in Monocyclic Aromatic Hydrocarbons by GC and External Calibration	HP-INNOWax, 60 m x 0.32 mm, 0.25 µm	19091N-116
D 5974	Standard Test Method for Fatty and Rosin Acids in Tall Oil Fraction Products by Capillary GC	DB-23, 60 m x 0.25 mm, 0.25 µm	122-2362
D 5986	Standard Test Method for Determination of Oxygenates, Benzene, Toluene, C_8-C_{12} Aromatics and Total Aromatics in Finished Gasoline by GC/FTIR	HP-1, 60 m x 0.53 mm, 5.00 µm	19095Z-626
D 6144	Standard Test Method for Trace Impurities in Alpha-Methylstyrene by Capillary GC	HP-1, 60 m x 0.25 mm, 1.00 µm	19091Z-236
D 6159	Standard Test Method for Determination of Hydrocarbon Impurities in Ethylene by GC	HP PLOT Al2O3 "KCl", 50 m x 0.53 mm, 15.00 µm	19095P-K25
		GS-Alumina, 50 m x 0.53 mm	115-3552
		DB-1, 30 m x 0.53 mm, 5.00 µm	125-1035
D 6160	Standard Test Method for Determination of PCBs in Waste Materials by GC	HP-5ms, 30 m x 0.32 mm, 0.25 µm	19091S-413
		DB-XLB, 30 m x 0.25 mm, 0.25 µm	122-1232
D 6352	Standard Test Method for Boiling Range Distribution of Petroleum Distillates in Boiling Range from 174 to 700 °C by GC	DB-HT SimDis, 5 m x 0.53 mm, 0.15 µm	145-1001
D 6387	Standard Test Methods for Composition of Turpentine and Related Terpene Products by Capillary Gas Chromatography	CP-WAX 52 CB, 30 m x 0.32 mm, 0.50 µm	CP8763
		CP-WAX 52 CB, 30 m x 0.53 mm, 1.00 µm	CP8738
D 6417	Standard Test Method for Estimation of Engine Oil Volatility by Capillary GC	DB-HT SimDis, 5 m x 0.53 mm, 0.15 µm	145-1001
D 6584	Standard Test Method for Determination of Total Monoglyceride, Total Diglyceride, Total Triglyceride, and Free and Total Glycerin in B-100 Biodiesel Methyl Esters by Gas Chromatography	Select Biodiesel, 15 m x 0.32 mm, 0.10 µm	CP9078
D 6806	Standard Practice for Analysis of Halogenated Organic Solvents and Their Admixtures by Gas Chromatography	CP-Sil 5 CB, 50 m x 0.53 mm, 5.00 µm	CP7685
E 1616	Standard Test Method for Analysis of Acetic Anhydride Using GC	HP-1, 50 m x 0.32 mm, 0.52 µm	19091Z-115
E 1863	Standard Test Method for Analysis of Acrylonitrile by GC	DB-WAXetr, 60 m x 0.32 mm, 1.00 µm	123-7364
E 0202	Standard Test Method for Analysis of Ethylene Glycols and Propylene Glycols	DB-624, 30 m x 0.53 mm, 3.00 µm	125-1334
		CP-Wax 57 CB for Gycols and Alcohols, 25 m x 0.25 mm, 0.25 µm	CP7615
E 0475	Standard Test Method for Assay of Di-tert-Butyl Peroxide Using GC	HP-5, 30 m x 0.53 mm, 5.00 µm	19095J-623


GC Capillary Columns

Agilent J&W Ultra Inert GC Columns

Perform trace-level analysis with the utmost confidence

As the GC industry's premier measurement company, Agilent is uniquely positioned to ensure the inertness of the surfaces your sample touches, so you can achieve the parts-per-billion – or parts-per-trillion – detection levels for your most demanding analyses. Agilent Ultra Inert components work together to deliver industry-leading results: the Agilent GC instrument, Ultra Inert liner and Agilent J&W Ultra Inert GC column family.

The Agilent J&W Ultra Inert GC column family pushes industry standards for consistent column inertness and exceptionally low column bleed, resulting in lower detection limits and more accurate data for difficult analytes. Each Ultra Inert column is tested with the industry's most demanding test probe mixture and we prove it with a performance summary sheet shipped with each column.

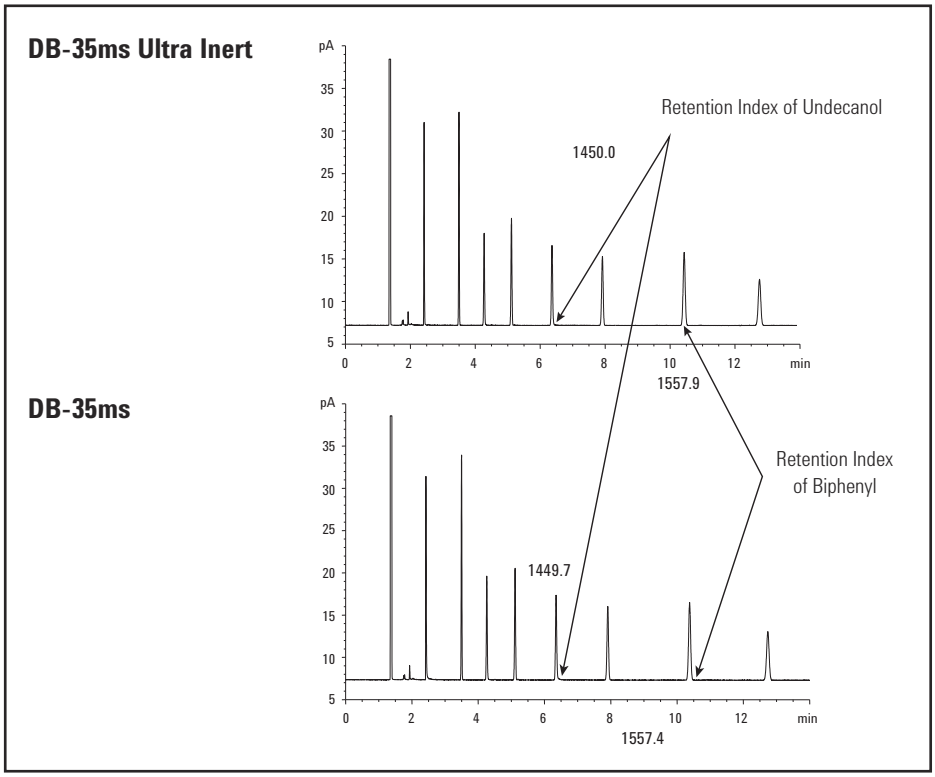

With Agilent J&W Ultra Inert GC columns, selectvity remains the same, allowing you to confidently integrate Ultra Inert columns into your current methods.

The industry's most rigorous test probe mixture ensures consistent column inertness – and results

A strong test probe mixture can highlight deficiencies in column activity, while a weak mixture can actually mask such deficiencies.

The test probes in Agilent's Ultra Inert test probe mixture have low molecular weights, low boiling points and no steric shielding of their active groups. These characteristics allow the probative portion of the test molecules to penetrate – and fully interact with – the stationary phase and column surface.

Commonly used, less demanding test probes		
1. 1-Octanol	4. 2,6-Dimethylaniline	7. 1-Decanol
2. n-Undecane	5. n-Dodecane	8. n-Tridecane
3. 2,6-Dimethylphenol	6. Napthalene	9. Methyldecanoate

TIPS & TOOLS

Clearly Better Inertness


To learn more and order your free poster, visit **www.agilent.com/chem/ultrainert**




Agilent's more demanding Ultra Inert test probe mixture for 5ms, 1ms, and 35ms Ultra Inert columns

Ultra Inert 5ms Columns			Ultra Inert 1ms Columns			Ultra Inert 35ms Columns		
Elution Order	**Test Probe**	**Functional Test**	**Elution Order**	**Test Probe**	**Functional Test**	**Elution Order**	**Test Probe**	**Functional Test**
1.	1-Propionic acid	Basicity	1.	1-Propionic acid	Basicity	1.	1-Octene	Polarity
2.	1-Octene	Polarity	2.	1-Octene	Polarity	2.	1-Butyric acid	Basicity
3.	n-Octane	Hydrocarbon marker	3.	n-Octane	Hydrocarbon marker	3.	n-Nonane	Hydrocarbon marker
4.	4-Picoline	Acidity	4.	1,2-Butanediol	Silanol	4.	4-Picoline	Acidity
5.	n-Nonane	Hydrocarbon marker	5.	4-Picoline	Acidity	5.	n-Propylbenzene	Polarity
6.	Trimethyl phosphate	Acidity	6.	Trimethyl phosphate	Acidity	6.	1-Heptanol	Silanol, Polarity
7.	1,2-Pentanediol	Silanol	7.	n-Propylbenzene	Hydrocarbon marker	7.	1,2-Pentanediol	Silanol
8.	n-Propylbenzene	Hydrocarbon marker	8.	1-Heptanol	Silanol	8.	3-Octanone	Polarity
9.	1-Heptanol	Silanol	9.	3-Octanone	Polarity	9.	Trimethyl phosphate	Acidity
10.	3-Octanone	Polarity	10.	tert-Butylbenzene	Hydrocarbon marker	10.	tert-Butylbenzene	Hydrocarbon marker
11.	n-Decane	Efficiency	11.	n-Decane	Efficiency	11.	n-Undecane	Efficiency

Chemical Structures




2,6-Dimethylphenol




2,6-Dimethylaniline

Weak probe molecules: The acidic and basic portions of these molecules are shielded by the two methyl groups on their phenyl rings, making them less probative.

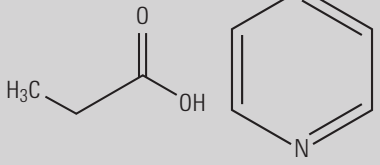

1-Propionic acid

4-Picoline



1-Butyric acid

Strong probe molecules: The probes in Agilent's Ultra Inert test probe mixture are highly probative of the stationary phase and surface. Note, too, that the active end of each compound is available to interact with any active sites on the column.

DB-1ms Ultra Inert

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.18	*20*	*0.18*	*-60 to 325/350*	*121-0122UI*	
0.25	15	0.25	-60 to 325/350	122-0112UI	122-0112UIE
	30	0.25	-60 to 325/350	122-0132UI	122-0132UIE
	60	0.25	-60 to 325/350	122-0162UI	
0.32	15	0.25	-60 to 325/350	123-0112UI	
	30	0.25	-60 to 325/350	123-0132UI	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

HP-1ms Ultra Inert

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.18	*20*	*0.18*	*-60 to 325/350*	*19091S-677UI*	*19091S-677UIE*
0.25	15	0.25	-60 to 325/350	19091S-931UI	19091S-931UIE
	30	0.25	-60 to 325/350	19091S-933UI	19091S-933UIE
		0.50	-60 to 325/350	19091S-633UI	
		1.00	-60 to 325/350	19091S-733UI	19091S-733UIE
0.32	15	0.25	-60 to 325/350	19091S-911UI	
	25	0.52	-60 to 325/350	19091S-612UI	
	30	0.25	-60 to 325/350	19091S-913UI	19091S-913UIE
		1.00	-60 to 325/350	19091S-713UI	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

Similar Phases: SPB-1, Rtx-1, BP-1, OV-1, OV-101, 007-1(MS), SP-2100, SE-30, ZB-1, AT-1, MDN-1, ZB-1, ZB-1ms

TIPS & TOOLS



Learn how to ensure an inert GC flow path with the Agilent Ultra Inert Solutions Brochure. Order yours at **www.agilent.com/chem/Ulorder**

DB-5ms Ultra Inert

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.18	*20*	*0.18*	*-60 to 325/350*	*121-5522UI*		*121-5522UILTM*
		0.36	*-60 to 325/350*	*121-5523UI*		*121-5523UILTM*
0.25	15	0.25	-60 to 325/350	122-5512UI		122-5512UILTM
		1.00	-60 to 325/350	122-5513UI		122-5513UILTM
	25	0.25	-60 to 325/350	122-5522UI		122-5522UILTM
	30	0.25	-60 to 325/350	122-5532UI	122-5532UIE	122-5532UILTM
		0.50	-60 to 325/350	122-5536UI		122-5536UILTM
		1.00	-60 to 325/350	122-5533UI	122-5533UIE	122-5533UILTM
	50	0.25	-60 to 325/350	122-5552UI		
	60	0.25	-60 to 325/350	122-5562UI		
		1.00	-60 to 325/350	122-5563UI		
0.32	30	0.25	-60 to 325/350	123-5532UI	123-5532UIE	123-5532UILTM
		0.50	-60 to 325/350	123-5536UI		123-5536UILTM
		1.00	-60 to 325/350	123-5533UI		123-5533UILTM
	60	1.00	-60 to 325/350	123-5563UI		

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

Similar Phases: Rtx-5ms, Rxi-5ms, Rxi-5Sil MS, VF-5ms, PTE-5, BPX-5, AT-5ms, ZB-5ms, ZB-5MSi, SLB-5ms, Equity-5

HP-5ms Ultra Inert

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
HP-5ms Ultra Inert						
0.18	*20*	*0.18*	*-60 to 325/350*	*19091S-577UI*		*19091S-577UILTM*
0.25	15	0.25	-60 to 325/350	19091S-431UI		19091S-431UILTM
	30	0.25	-60 to 325/350	19091S-433UI	19091S-433UIE	19091S-433UILTM
		0.50	-60 to 325/350	19091S-133UI		19091S-133UILTM
		1.00	-60 to 325/350	19091S-233UI	19091S-233UIE	19091S-233UILTM
	60	0.25	-60 to 325/350	19091S-436UI		
0.32	30	0.25	-60 to 325/350	19091S-413UI		19091S-413UILTM
		1.00	-60 to 325/350	19091S-213UI		19091S-213UILTM

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

Similar Phases: Rtx-5ms, Rxi-5ms, Rxi-5Sil MS, PTE-5, BPX-5, AT-5ms, ZB-5ms, SLB-5ms, Equity-7

DB-35ms Ultra Inert

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.18	*20*	*0.18*	*50 to 340/360*	*121-3822UI*
0.25	15	0.25	50 to 340/360	122-3812UI
	30	0.25	50 to 340/360	122-3832UI
0.32	15	0.25	50 to 340/360	123-3812UI
	30	0.25	50 to 340/360	123-3832UI

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

Similar Phases: Rtx-35, Rtx-35ms, Rxi-35Sil MS, SPB-35, AT-35, Sup-Herb, MDN-35, BPX-34, ZB-35, ZB-35 ht

TIPS & TOOLS

Complete your ultra inert flow path with the industry leading Agilent Ultra Inert Inlet Liner, **www.agilent.com/chem/uiliner**



DB-624 Ultra Inert

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.18	*20*	*1*	*-20 to 260*	*121-1324UI*
0.25	30	1.4	-20 to 260	122-1334UI
	60	1.4	-20 to 260	122-1364UI
0.32	30	1.8	-20 to 260	123-1334UI
	60	1.8	-20 to 260	123-1364UI
0.53	30	3	-20 to 260	125-1334UI
	75	3	-20 to 260	125-1374UI

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

DB-UI 8270D

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.18	*20*	*0.36*	*-60 to 325/350*	*121-9723*
				*621-9723, 6/pk**
0.25	30	0.25	-60 to 325/350	122-9732
			-60 to 325/350	622-9732, 6/pk*
		0.50	-60 to 325/350	122-9736

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

*Only available in the U.S.

Agilent J&W High Efficiency GC Capillary Columns

High efficiency, high throughput, and high resolution without the high costs

This leading-edge column technology is ideal for applications that require faster run times, such as high-throughput screening, fast process monitoring, and fast method development. In fact, Agilent High Efficiency GC columns can reduce your sample run time by 50% or more without compromising resolution.

Unlike other manufacturers' 0.1 mm id columns, Agilent's 0.15 and 0.18 mm id High Efficiency Capillary GC columns are compatible with all standard-pressure capillary GC and GC/MS instruments – without expensive high-pressure modifications. They also give you:

- The flexibility to choose between helium and hydrogen carrier gases. You can stay with a helium carrier if you wish to simplify method development, or switch to a hydrogen carrier to further reduce your analysis time.
- The ability to separate samples using less carrier gas, which can lead to longer intervals between cylinder changes, increased uptime, and a lower cost per sample.

In addition, these flexible columns easily adapt to a wide variety of environmental, petrochemical, flavor/fragrance, clinical toxicology, and pharmaceutical sample matrices.

The Agilent J&W High Efficiency GC columns throughout this section are displayed using italicized descriptions and part numbers in the ordering tables.

Low-bleed GC/MS Columns

There is a rapidly increasing population of benchtop GC/MS instruments in analytical laboratories that analyze a widening range of trace level, higher temperature samples. These samples require increasingly inert, lower bleed, higher temperature columns. In response to this growing need, Agilent Technologies designed several "ms" columns to chromatograph a broader range of low level samples and generate lower bleed even at higher temperatures.

What makes an Agilent J&W low-bleed column exceptional? Unique polymer chemistry and proprietary surface deactivation, both of which have contributed to columns that adhere to the tightest quality control specifications in the industry for bleed, inertness, selectivity and efficiency. Agilent J&W "ms" columns utilize special surface deactivation and siloxane chemistries which enhance the chromatographic performance of siloxane polymers.

The mass spectrum of septum bleed can look very much like GC column bleed, so the two are often confused. An easy way to tell the two apart: column bleed will be indicated by a rise in the baseline, not peaks. If you see bleed peaks, these generally come from lower quality septa or septa being used beyond their operating limits. To minimize septa contributions to background bleed, use quality Agilent BTO, Long Life, or Advanced Green septa.


TIPS & TOOLS

Check out Agilent's complete line of sample preparation products for any type of GC and GC/MS analysis at **www.agilent.com/chem/sampleprep**



DB-1ms

- 100% Dimethylpolysiloxane
- Identical selectivity to DB-1
- Non-polar
- Very low bleed characteristics, ideal for GC/MS
- Improved acid performance compared to standard 100% Dimethylpolysiloxane columns
- Improved signal-to-noise ratio for better sensitivity and mass spectral integrity
- 340/360 °C upper temperature limit
- Excellent general purpose column
- Bonded and cross-linked
- Solvent rinsable



Structure of DB-1ms

Similar Phases: SPB-1, Rtx-1, BP-1, OV-1, OV-101, 007-1(MS), SP-2100, SE-30, ZB-1, AT-1, MDN-1, ZB-1, ZB-1ms


DB-1ms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module	5975T LTM Toroid
0.10	10	0.10	-60 to 340/360	127-0112		127-0112LTM	
		0.40	-60 to 340/360	127-0113			
	20	0.10	-60 to 340/360	127-0122			
		0.40	-60 to 340/360	127-0123		127-0123LTM	
0.18	*20*	*0.18*	*-60 to 340/360*	*121-0122*	*121-0122E*	*121-0122LTM*	*221-0122LTM*
0.20	12	0.33	-60 to 340/350	128-0112		128-0112LTM	
	25	0.33	-60 to 340/350	128-0122	128-0122E	128-0122LTM	
0.25	15	0.25	-60 to 340/360	122-0112	122-0112E	122-0112LTM	222-0112LTM
	30	0.10	-60 to 340/360	122-0131			
		0.25	-60 to 340/360	122-0132	122-0132E		222-0132LTM
	60	0.25	-60 to 340/360	122-0162			
0.32	15	0.25	-60 to 340/360	123-0112			
	30	0.10	-60 to 340/360	123-0131			
		0.25	-60 to 340/360	123-0132		123-0132LTM	
	60	0.25	-60 to 340/360	123-0162			

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

TIPS & TOOLS

Learn how the Agilent 5975T LTM GC/MSD can deliver the rapid, reliable results you need in the field or in the lab, **www.agilent.com/chem/5975T**

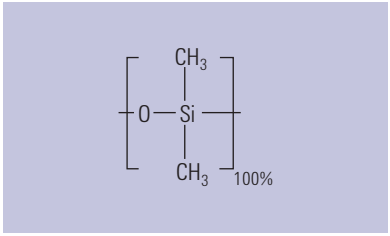

Structure of HP-1ms

HP-1ms

- 100% Dimethylpolysiloxane
- Identical selectivity to HP-1
- Non-polar
- Low bleed characteristics
- Excellent general purpose column
- Improved signal-to-noise ratio for better sensitivity and mass spectral integrity
- Bonded and cross-linked
- Solvent rinsable

Similar Phases: Rtx-1ms, Rxi-1ms, MDN-1, AT-1, ZB-1ms, Equity-1

HP-1ms


ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module	5975T LTM Toroid
0.18	*20*	*0.18*	*-60 to 325/350*	*19091S-677*	*19091S-677E*	*19091S-677LTM*	*29091S-677LTM*
0.20	25	0.33	-60 to 325/350	19091S-602	19091S-602E	19091S-602LTM	
0.25	15	0.25	-60 to 325/350	19091S-931	19091S-931E	19091S-931LTM	29091S-931LTM
	30	0.10	-60 to 325/350	19091S-833		19091S-833LTM	29091S-833LTM
		0.25	-60 to 325/350	19091S-933	19091S-933E	19091S-933LTM	29091S-433LTM
		0.50	-60 to 325/350	19091S-633		19091S-633LTM	
		1.00	-60 to 325/350	19091S-733	19091S-733E	19091S-733LTM	
	60	0.25	-60 to 325/350	19091S-936	19091S-936E		
0.32	15	0.25	-60 to 325/350	19091S-911		19091S-911LTM	
	25	0.52	-60 to 325/350	19091S-612		19091S-612LTM	
	30	0.25	-60 to 325/350	19091S-913	19091S-913E	19091S-913LTM	
		1.00	-60 to 325/350	19091S-713		19091S-713LTM	
	60	0.25	-60 to 325/350	19091S-916			

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

VF-1ms

- Highly inert, non-polar 100% dimethylpolysiloxane phase, low-bleed GC column providing increased sensitivity over a broad array of applications
- Ultra low bleed specification of 1 pA @ 325 °C (30 m, 0.25 mm, 0.25 µm) for trace analysis with MS
- QC test results for retention index, efficiency, selectivity and bleed is reported with every column
- 0.15 mm id columns available for high efficiency GC and GC/MS analyses
- Supplied with EZ-GRIP to simplify column installation, coupling and operation

Similar Phases: Rtx-1ms, Rxi-1ms, MDN-1, AT-1, ZB-1ms, Equity-1

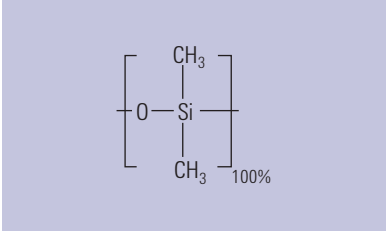

Structure of VF-1ms

VF-1ms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.10	10	0.10	-60 to 325/350	CP8900	
		0.40	-60 to 325/350	CP8901	
	20	0.10	-60 to 325/350	CP8902	
		0.40	-60 to 325/350	CP8903	
0.15	*10*	*0.15*	*-60 to 325/350*	*CP9030*	
	15	*0.15*	*-60 to 325/350*	*CP5881*	
	20	*0.15*	*-60 to 325/350*	*CP9031*	
		0.60	*-60 to 325/350*	*CP9032*	*CP9032I5*
0.20	12	0.33	-60 to 325/350	CP8904	
	25	0.33	-60 to 325/350	CP8905	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

(Continued)



Column shown with EZ-GRIP

VF-1ms


ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	15	0.10	-60 to 325/350	CP8906	CP8906I5
		0.25	-60 to 325/350	CP8907	CP8907I5
		1.00	-60 to 325/350	CP8908	CP8908I5
	25	0.25	-60 to 325/350	CP8909	
		0.40	-60 to 325/350	CP8910	
	30	0.10	-60 to 325/350	CP8911	CP8911I5
		0.25	-60 to 325/350	CP8912	CP8912I5
		1.00	-60 to 325/350	CP8913	CP8913I5
	50	0.25	-60 to 325/350	CP8914	
		0.40	-60 to 325/350	CP8915	
	60	0.25	-60 to 325/350	CP8916	CP8916I5
		1.00	-60 to 325/350	CP8917	CP8917I5
0.32	15	0.10	-60 to 325/350	CP8918	CP8918I5
		0.25	-60 to 325/350	CP8919	
		1.00	-60 to 325/350	CP8920	CP8920I5
	25	0.25	-60 to 325/350	CP8921	
		0.40	-60 to 325/350	CP8922	
	30	0.10	-60 to 325/350	CP8923	
		0.25	-60 to 325/350	CP8924	
		0.50	-60 to 325/350	CP8925	
		1.00	-60 to 325/350	CP8926	
	50	0.25	-60 to 325/350	CP8927	
		0.40	-60 to 325/350	CP8928	
	60	0.25	-60 to 325/350	CP8929	
		1.00	-60 to 325/350	CP8930	
0.53	15	0.50	-60 to 325/350	CP8965	
		1.50	-60 to 325/350	CP8967	
	30	0.50	-60 to 325/350	CP8968	
		1.00	-60 to 325/350	CP8969	
		1.50	-60 to 310/335	CP8970	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

DB-5ms

- Phenyl Arylene polymer virtually equivalent to a (5%-Phenyl)-methylpolysiloxane
- Non-polar
- Very low bleed characteristics, ideal for GC/MS
- Excellent inertness for active compounds
- Improved signal-to-noise ratio for better sensitivity and mass spectral integrity
- Bonded and cross-linked
- Solvent rinsable
- Exact replacement of HP-5TA
- Close equivalent to USP Phase G27
- Test mix available

Similar Phases: Rtx-5ms, Rxi-5ms, Rxi-5Sil MS, PTE-5, BPX-5, AT-5ms, ZB-5ms, ZB-5MSi, SLB-5ms, Equity-5

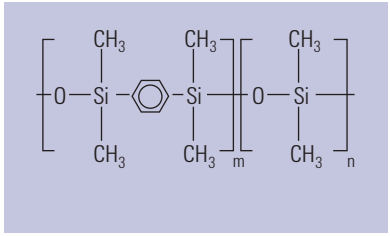

Structure of DB-5ms



TIPS & TOOLS

Learn more about the Agilent 7890A GC System at **www.agilent.com/chem/7890A**


DB-5ms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module	5975T LTM Toroid
0.18	*20*	*0.18*	*-60 to 325/350*	*121-5522*	*121-5522E*	*121-5522LTM*	*221-5522LTM*
		0.36	*-60 to 325/350*	*121-5523*		*121-5523LTM*	
	40	*0.18*	*-60 to 325/350*	*121-5542*			
0.20	12	0.33	-60 to 325/350	128-5512		128-5512LTM	
	25	0.33	-60 to 325/350	128-5522		128-5522LTM	
	50	0.33	-60 to 325/350	128-5552			
0.25	15	0.10	-60 to 325/350	122-5511		122-5511LTM	
		0.25	-60 to 325/350	122-5512		122-5512LTM	222-5512LTM
		0.50	-60 to 325/350	122-5516		122-5516LTM	
		1.00	-60 to 325/350	122-5513		122-5513LTM	
	25	0.25	-60 to 325/350	122-5522		122-5522LTM	
		0.40	-60 to 325/350	122-552A		122-552ALTM	
	30	0.10	-60 to 325/350	122-5531		122-5531LTM	
		0.25	-60 to 325/350	122-5532	122-5532E	122-5532LTM	222-5532LTM
		0.50	-60 to 325/350	122-5536	122-5536E	122-5536LTM	
		1.00	-60 to 325/350	122-5533	122-5533E	122-5533LTM	
	50	0.25	-60 to 325/350	122-5552			
	60	0.10	-60 to 325/350	122-5561			
		0.25	-60 to 325/350	122-5562	122-5562E		
		1.00	-60 to 325/350	122-5563			
0.32	15	0.10	-60 to 325/350	123-5511		123-5511LTM	
		0.25	-60 to 325/350	123-5512		123-5512LTM	
		1.00	-60 to 325/350	123-5513	123-5513E	123-5513LTM	
	25	0.52	-60 to 325/350	123-5526		123-5526LTM	
	30	0.10	-60 to 325/350	123-5531		123-5531LTM	
		0.25	-60 to 325/350	123-5532	123-5532E	123-5532LTM	
		0.50	-60 to 325/350	123-5536		123-5536LTM	
		1.00	-60 to 325/350	123-5533		123-5533LTM	
	60	0.10	-60 to 325/350	123-5561			
		0.25	-60 to 325/350	123-5562			
		0.50	-60 to 325/350	123-5566			
		1.00	-60 to 325/350	123-5563			
0.53	15	1.50	-60 to 300/320	125-5512		125-5512LTM	
	30	0.50	-60 to 300/320	125-5537		125-5537LTM	
		1.00	-60 to 300/320	125-553J		125-553JLTM	
		1.50	-60 to 300/320	125-5532		125-5532LTM	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

HP-5ms

- (5%-Phenyl)-methylpolysiloxane
- Identical selectivity to HP-5
- Non-polar
- Very low bleed characteristics, ideal for GC/MS
- Excellent inertness for active compounds including acidic and basic compounds
- Improved signal-to-noise ratio for better sensitivity and mass spectral integrity
- Bonded and cross-linked
- Solvent rinsable
- Equivalent to USP Phase G27




Structure of HP-5ms

Similar Phases: Rtx-5ms, Rxi-5ms, Rxi-5Sil MS, PTE-5, BPX-5, AT-5ms, ZB-5ms, SLB-5ms, Equity-5

HP-5ms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module	5975T LTM Toroid
0.18	*20*	*0.18*	*-60 to 325/350*	*19091S-577*		*19091S-577LTM*	
0.20	12	0.33	-60 to 325/350	19091S-101		19091S-101LTM	
	25	0.33	-60 to 325/350	19091S-102	19091S-102E	19091S-102LTM	
	50	0.33	-60 to 325/350	19091S-105			
0.25	15	0.10	-60 to 325/350	19091S-331		19091S-331LTM	
		0.25	-60 to 325/350	19091S-431		19091S-431LTM	
		1.00	-60 to 325/350	19091S-231		19091S-231LTM	
	30	0.10	-60 to 325/350	19091S-333		19091S-333LTM	
		0.25	-60 to 325/350	19091S-433	19091S-433E	19091S-433LTM	29091S-433LTM
		0.50	-60 to 325/350	19091S-133		19091S-133LTM	
		1.00	-60 to 325/350	19091S-233	19091S-233E	19091S-233LTM	
	60	0.10	-60 to 325/350	19091S-336			
		0.25	-60 to 325/350	19091S-436	19091S-436E		
0.32	25	0.52	-60 to 325/350	19091S-112	19091S-112E	19091S-112LTM	
	30	0.10	-60 to 325/350	19091S-313		19091S-313LTM	
		0.25	-60 to 325/350	19091S-413	19091S-413E	19091S-413LTM	
		0.50	-60 to 325/350	19091S-113		19091S-113LTM	
		1.00	-60 to 325/350	19091S-213		19091S-213LTM	
	60	0.25	-60 to 325/350	19091S-416			

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers



Structure of VF-5ms

VF-5ms

- Highly inert 5% phenylmethyl column for increased sensitivity, accuracy and instrument uptime
- Minimal column bleed improves sensitivity – ultra low bleed specification of 1 pA @ 325 °C (30 m x 0.25 mm, 0.25 µm)
- Slightly higher polarity than VF-1ms, results in improved selectivity for aromatic compounds; selectivity and excellent inertness make these columns applicable for a wide range of semi-polar and even polar compounds
- 0.15 mm id columns available for high efficiency GC and GC/MS analyses
- QC test results for retention index, efficiency, selectivity and bleed is reported with every column
- Supplied with EZ-GRIP to simplify column installation, coupling and operation

Similar Phases: Rtx-5ms, Rxi-5ms, Rxi-5Sil MS, PTE-5, BPX-5, AT-5ms, ZB-5ms, ZB-5MSi, SLB-5ms, Equity-5

VF-5ms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.10	10	0.40	-60 to 325/350	CP8934	
	20	0.40	-60 to 325/350	CP8933	
0.15	*10*	*0.15*	*-60 to 325/350*	*CP9034*	*CP9034I5*
	15	*0.15*	*-60 to 325/350*	*CP9035*	
	20	*0.15*	*-60 to 325/350*	*CP9036*	*CP9036I5*
		0.30	*-60 to 325/350*	*CP9037*	
		0.60	*-60 to 325/350*	*CP9038*	
	40	*0.15*	*-60 to 325/350*	*CP9039*	*CP9039I5*
		0.60	*-60 to 325/350*	*CP9040*	
0.20	12	0.33	-60 to 325/350	CP8935	CP8935I5
	25	0.33	-60 to 325/350	CP8936	CP8936I5
	50	0.33	-60 to 325/350	CP8937	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

(Continued)

TIPS & TOOLS

As part of Agilent's ongoing commitment to be your partner in chromatography, we have created a series of GC Troubleshooting videos, featuring Daron Decker, GC Applications Specialist, and Herb Brooks, Agilent Service Engineer. To view the videos, visit **www.agilent.com/chem/gctroubleshooting**





VF-5ms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	15	0.10	-60 to 325/350	CP8938	
		0.25	-60 to 325/350	CP8939	
		0.50	-60 to 325/350	CP8963	
		1.00	-60 to 325/350	CP8940	
	25	0.25	-60 to 325/350	CP8941	CP8941I5
		0.40	-60 to 325/350	CP8942	
	30	0.10	-60 to 325/350	CP8943	CP8943I5
		0.25	-60 to 325/350	CP8944	CP8944I5
		0.50	-60 to 325/350	CP8945	
		1.00	-60 to 325/350	CP8946	
	50	0.25	-60 to 325/350	CP8947	
	60	0.10	-60 to 325/350	CP8948	CP8948I5
		0.25	-60 to 325/350	CP8960	CP8960I5
		1.00	-60 to 325/350	CP8949	
0.32	15	0.10	-60 to 325/350	CP8950	
		0.25	-60 to 325/350	CP8951	
		1.00	-60 to 325/350	CP8952	
	25	0.52	-60 to 325/350	CP8953	
	30	0.10	-60 to 325/350	CP8954	CP8954I5
		0.25	-60 to 325/350	CP8955	CP8955I5
		0.50	-60 to 325/350	CP8956	
		1.00	-60 to 325/350	CP8957	CP8957I5
	50	0.25	-60 to 325/350	CP8958	
		0.40	-60 to 325/350	CP8959	
	60	0.25	-60 to 325/350	CP8961	CP8961I5
		1.00	-60 to 325/350	CP8962	
0.53	15	0.50	-60 to 325/350	CP8971	
		1.00	-60 to 325/350	CP8972	
		1.50	-60 to 325/350	CP8973	
	30	0.50	-60 to 325/350	CP8974	
		1.00	-60 to 325/350	CP8975	
		1.50	-60 to 310/335	CP8976	

DB-XLB

- Exceptionally low bleed
- Low polarity
- Extended temperature limit of 340/360 °C
- Unique selectivity
- Excellent inertness for active compounds
- Ideal for confirmational analyses
- Excellent for pesticides, herbicides, PCBs and PAHs
- Ideal for GC/MS
- Bonded and cross-linked
- Solvent rinsable

Note: "DB-XLB is designed for inhibiting column bleed at high temperatures. It also appears to have inadvertently inherited an exceptional ability for separating many PCB congeners when used with MS detection. This stellar performance was maximized after careful optimization of the column dimensions, temperature programs, and carrier gas flow conditions."

(Frame, G. Analytical Chemistry News & Features, Aug. 1, 1997, 468A-475A)


Similar Phases: Rtx-XLB, MDN-12, ZB-XLB, ZB-XLB HT

DB-XLB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.18	*20*	*0.18*	*30 to 340/360*	*121-1222*	*121-1222E*	*121-1222LTM*
	30	*0.18*	*30 to 340/360*	*121-1232*		
0.20	12	0.33	30 to 340/360	128-1212	128-1212E	
	25	0.33	30 to 340/360	128-1222		
0.25	15	0.10	30 to 340/360	122-1211		122-1211LTM
		0.25	30 to 340/360	122-1212		
	30	0.10	30 to 340/360	122-1231		
		0.25	30 to 340/360	122-1232		122-1232LTM
		0.50	30 to 340/360	122-1236		
		1.00	30 to 340/360	122-1233		
	60	0.25	30 to 340/360	122-1262	122-1262E	
0.32	30	0.25	30 to 340/360	123-1232		
		0.50	30 to 340/360	123-1236		
	60	0.25	30 to 340/360	123-1262		
0.53	15	1.50	30 to 320/340	125-1212		125-1212LTM
	30	1.50	30 to 320/340	125-1232		125-1232LTM

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

VF-Xms



Structure of VF-Xms

- High arylene modified phase for accurate results
- Isothermal applications up to 340 °C for a broad application range
- Ideal for confirmational analyses – more polar alternative to 5% phenyl columns
- Ultra low bleed delivers ultimate sensitivity and signal-to-noise ratio
- Provides exceptionally high selectivity for semivolatile compounds such as pesticides and delivers high resolution with short analysis time
- Very unique selectivity for chlorinated compounds
- QC test results for retention index, efficiency, selectivity and bleed is reported with every column
- 0.15 mm id columns available for high efficiency GC and GC/MS analyses
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation

Similar Phases: Rtx-XLB, MDN-12, ZB-XLB, ZB-XLB HT




Column shown with EZ-GRIP

VF-Xms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.15	*20*	*0.15*	*30 to 340/360*	*CP9041*	
0.20	12	0.33	30 to 340/360	CP8800	
	25	0.33	30 to 340/360	CP8801	
0.25	15	0.10	30 to 340/360	CP8802	
		0.25	30 to 340/360	CP8803	
	30	0.10	30 to 340/360	CP8805	
		0.25	30 to 340/360	CP8806	CP8806I5
		0.50	30 to 340/360	CP8807	
		1.00	30 to 340/360	CP8808	
	60	0.25	30 to 340/360	CP8809	
0.32	15	0.25	30 to 340/360	CP8810	
		1.00	30 to 340/360	CP8811	
	30	0.10	30 to 340/360	CP8812	
		0.25	30 to 340/360	CP8813	
		0.50	30 to 340/360	CP8814	
		1.00	30 to 340/360	CP8815	
	60	0.25	30 to 340/360	CP8816	
0.53	15	1.50	30 to 325/340	CP8817	
	30	1.50	30 to 325/340	CP8818	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

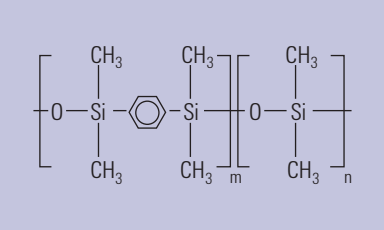

Structure of DB-35ms

DB-35ms

- Virtually equivalent to a (35%-Phenyl)-methylpolysiloxane
- Mid-polarity
- Very low bleed characteristics, ideal for GC/MS
- Extended temperature limit of 340/360 °C
- Excellent inertness for active compounds
- Ideal for confirmational analyses
- Bonded and cross-linked
- Solvent rinsable
- Replaces HP-35ms
- Close equivalent to USP Phase G42

Similar Phases: Rtx-35, Rtx-35ms, Rxi-35Sil MS, SPB-35, AT-35, Sup-Herb, MDN-35, BPX-34, ZB-35, ZB-35 ht

DB-35ms


ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module	5975T LTM Toroid
0.18	*20*	*0.18*	*50 to 340/360*	*121-3822*	*121-3822E*	*121-3822LTM*	*221-3822LTM*
0.20	15	0.33	50 to 340/360	128-3812			
	25	0.33	50 to 340/360	128-3822			
0.25	15	0.25	50 to 340/360	122-3812			222-3812LTM
	30	0.15	50 to 340/360	122-3831			
	30	0.25	50 to 340/360	122-3832	122-3832E	122-3832LTM	222-3832LTM
	60	0.25	50 to 340/360	122-3862			
0.32	15	0.25	50 to 340/360	123-3812			
	30	0.25	50 to 340/360	123-3832	123-3832E		
0.53	30	0.50	50 to 320/340	125-3837		125-3837LTM	
	30	1.00	50 to 320/340	125-3832		125-3832LTM	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

VF-35ms

- Stabilized arylene-modified equivalent of a 35% phenylmethyl phase
- Ideal for dual column confirmational analyses
- Ultra low bleed, highly stable column with a programmable maximum temperature of 360 °C
- Medium polarity column ideal for trace environmental and chemical analyses
- 0.15 mm id columns available for high efficiency GC and GC/MS analyses
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation

Similar Phases: Rtx-35, Rtx-35ms, Rxi-35Sil MS, SPB-35, AT-35, Sup-Herb, MDN-35, BPX-34, ZB-35, ZB-35 ht




Structure of VF-35ms

VF-35ms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.15	*10*	*0.15*	*40 to 340/360*	*CP5887*	
	15	*0.15*	*40 to 340/360*	*CP5888*	
	20	*0.15*	*40 to 340/360*	*CP5889*	
0.20	15	0.33	40 to 340/360	CP8872	
	25	0.33	40 to 340/360	CP8873	
0.25	15	0.25	40 to 340/360	CP8874	
	30	0.10	40 to 340/360	CP8875	
		0.15	40 to 340/360	CP8876	
		0.25	40 to 340/360	CP8877	CP8877I5
		0.50	40 to 340/360	CP8878	CP8878I5
		1.00	40 to 340/360	CP8879	
	60	0.25	40 to 340/360	CP8880	
0.32	15	0.25	40 to 340/360	CP8881	
	30	0.25	40 to 340/360	CP8882	
		0.50	40 to 340/360	CP8883	CP8883I5
		1.00	40 to 340/360	CP8884	
	60	0.25	40 to 340/360	CP8885	
0.53	15	1.00	40 to 325/350	CP8886	
	30	0.50	40 to 325/350	CP8887	
		1.00	40 to 325/350	CP8888	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

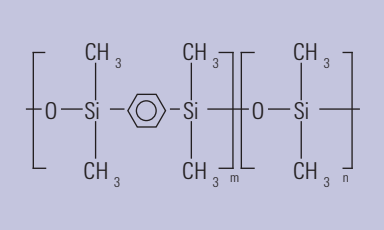

Structure of DB-17ms

DB-17ms

- Virtually equivalent to (50%-Phenyl)-methylpolysiloxane
- 320/340 °C upper temperature limit
- Very low bleed mid-polarity column, ideal for GC/MS
- Excellent inertness for active compounds
- Enhanced mass spectral integrity
- Bonded and cross-linked
- Solvent rinsable
- Excellent choice for CLP pesticides

Similar Phases: Rxi-17Sil MS, Rtx-50, 007-17, SP-2250, SPB-50, BPX-50, SPB-17, AT-50

DB-17ms


ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module	5975T LTM Toroid
0.18	*20*	*0.18*	*40 to 320/340*	*121-4722*	*121-4722E*	*121-4722LTM*	*221-4722LTM*
0.25	15	0.15	40 to 320/340	122-4711		122-4711LTM	
		0.25	40 to 320/340	122-4712		122-4712LTM	222-4712LTM
	30	0.15	40 to 320/340	122-4731		122-4731LTM	
		0.25	40 to 320/340	122-4732	122-4732E	122-4732LTM	222-4732LTM
	60	0.25	40 to 320/340	122-4762			
0.32	15	0.25	40 to 320/340	123-4712		123-4712LTM	
	30	0.25	40 to 320/340	123-4732		123-4732LTM	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

TIPS & TOOLS

View the latest GC column focused applications, products and educational resources at **www.agilent.com/chem/myGCcolumns**

VF-17ms

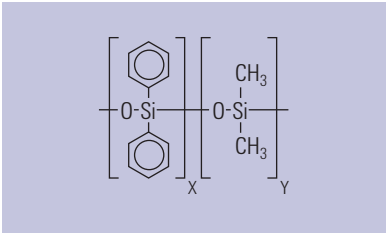

Structure of VF-17ms


- 50% phenyl/50% dimethylpolysiloxane, medium polarity phase
- Ultra low bleed
- Proprietary deactivation technology and manufacturing process improves column stability, resulting in improved column-to-column repeatability and column lifetimes
- Ideal for environmental and clinical methods
- Ultra low bleed specification at 2 pA @ 325 °C (0.25 mm x 30 m, 0.25 µm)
- Ideal EPA confirmation column for ultimate confidence
- Bonded and cross-linked
- Solvent rinsable
- 0.15 mm id columns available for high efficiency GC and GC/MS analyses
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation

Similar Phases: Rxi-17Sil MS, Rtx-50, 007-17, SP-2250, SPB-50, BPX-50, SPB-17, AT-50

VF-17ms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.10	10	0.20	40 to 330/360	CP8977	
0.15	*10*	*0.15*	*40 to 330/360*	*CP5882*	
	15	*0.15*	*40 to 330/360*	*CP5883*	
	20	*0.15*	*40 to 330/360*	*CP5884*	
0.25	15	0.25	40 to 330/360	CP8979	
	15	0.50	40 to 330/360	CP8980	
	30	0.15	40 to 330/360	CP8981	
		0.25	40 to 330/360	CP8982	CP8982I5
		0.50	40 to 330/360	CP8983	
	60	0.25	40 to 330/360	CP8984	
0.32	15	0.15	40 to 330/360	CP8986	
		0.25	40 to 330/360	CP8987	
	30	0.25	40 to 330/360	CP8990	CP8990I5
		0.50	40 to 330/360	CP8991	
0.53	15	0.25	40 to 330/360	CP8994	
		1.00	40 to 330/360	CP8996	
		1.50	40 to 310/340	CP8998	
	30	0.50	40 to 330/360	CP9000	
		1.00	40 to 310/340	CP9001	
		1.50	40 to 310/340	CP9002	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

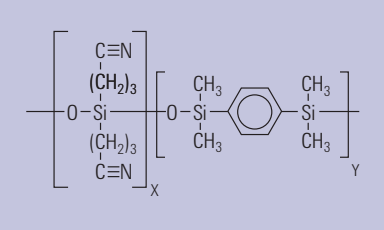

Structure of VF-23ms

VF-23ms

- High polarity and highly substituted cyanopropyl low bleed phase
- Engineered for accurate analysis of very polar analytes
- 100% bonded phase permits column rinsing to enhance column lifetime
- Operating temperature up to 260 °C
- Expands application ranges to higher molecular weight compounds
- 0.15 mm id columns available for high efficiency GC and GC/MS analyses
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation


Similar Phases: SP-2330, Rtx-2330, 007-23, AT-Silar, BPX-70, SP-2340

VF-23ms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.10	10	0.10	40 to 260/260	CP8819	
0.15	*15*	*0.15*	*40 to 260/260*	*CP5886*	
	20	*0.15*	*40 to 260/260*	*CP9042*	
	40	*0.15*	*40 to 260/260*	*CP5885*	
0.25	15	0.25	40 to 260/260	CP8820	CP8820I5
	30	0.15	40 to 260/260	CP8821	CP8821I5
		0.25	40 to 260/260	CP8822	CP8822I5
	60	0.15	40 to 260/260	CP8823	
		0.25	40 to 260/260	CP8824	CP8824I5
0.32	15	0.25	40 to 260/260	CP8825	
	30	0.15	40 to 260/260	CP8826	
		0.25	40 to 260/260	CP8827	
	60	0.15	40 to 260/260	CP8828	
		0.25	40 to 260/260	CP8829	
0.53	15	0.50	40 to 245/245	CP8830	
	30	0.50	40 to 245/245	CP8831	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

VF-200ms

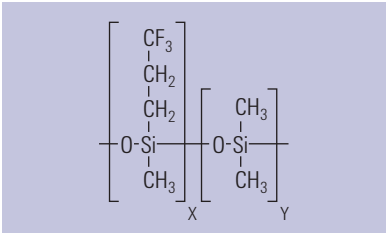

Structure of VF-200ms

- Trifluoropropyl phase has very high temperature stability and can be used routinely up to 350 °C
- Ideally suited for analyses of ketones, aldehydes, nitro- or chloro-containing compounds, PAHs, unsaturated compounds, silanes, and CFCs
- Optimized deactivation for symmetrical peak shape
- Ultra-low bleed for trace analysis
- 0.15 mm id columns available for high efficiency GC and GC/MS analyses
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation

Similar Phases: Rtx-200

VF-200ms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.15	*10*	*0.15*	*0 to 325/350*	*CP5893*	
	20	*0.15*	*0 to 325/350*	*CP5891*	
		0.60	*0 to 325/350*	*CP5892*	
0.25	15	0.25	0 to 325/350	CP8855	CP8855I5
		0.50	0 to 325/350	CP8856	
	30	0.10	0 to 325/350	CP8857	
		0.25	0 to 325/350	CP8858	
		0.50	0 to 325/350	CP8859	CP8859I5
		1.00	0 to 325/350	CP8860	CP8860I5
	60	0.25	0 to 325/350	CP8861	
0.32	15	0.25	0 to 325/350	CP8862	
	30	0.25	0 to 325/350	CP8863	
		0.50	0 to 325/350	CP8864	
		1.00	0 to 325/350	CP8865	CP8865I5
0.53	15	1.00	0 to 300/325	CP8866	
	30	0.50	0 to 300/325	CP8867	
		1.00	0 to 300/325	CP8868	CP8868I5

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

DB-225ms


- Virtually equivalent to (50%-Cyanopropylphenyl)-methylpolysiloxane
- Mid/high polarity
- Excellent for separations of cis- and trans-fatty acid methyl esters (FAMEs)
- Low bleed
- Bonded and cross-linked
- Solvent rinsable
- Close equivalent to USP Phase G7

Similar Phases: SP-2330, Rtx-225, BP-225, OV-225, 007-225, AT-225

DB-225ms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module	5975T LTM Toroid
0.25	15	0.25	40 to 240	122-2912		122-2912LTM	222-2912LTM
	30	0.25	40 to 240	122-2932	122-2932E	122-2932LTM	222-2932LTM
	60	0.25	40 to 240	122-2962			
0.32	30	0.25	40 to 240	123-2932		123-2932LTM	

VF-WAXms

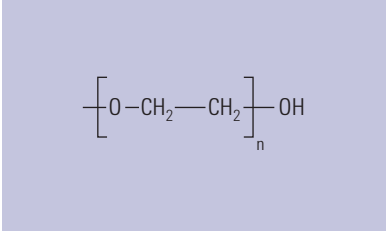

Structure of VF-WAXms

- Specially designed WAX phase designed for accurate MS results with polar compounds
- Operating temperature range of 20 °C to 250 °C
- Improves signal-to-noise ratio for trace analyses
- Ideal for GC/MS food, flavor and fragrance applications, especially where trace analyses are required
- Ultra low bleed provides increased sensitivity and extended column lifetime at higher temperatures
- Improved performance with no change in the typical selectivity of PEG
- 0.15 mm id columns available for high efficiency GC and GC/MS analyses
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation

Similar Phases: SUPELCOWAX 10, SUPEROX II, CB-WAX, Stabilwax, BP-20, 007-CW, Carbowax, Rtx-WAX, ZB-WAX, ZB-WAX plus

VF-WAXms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.10	10	0.10	20 to 250/260	CP9219	
		0.20	20 to 250/260	CP9218	
	20	0.10	20 to 250/260	CP9229	CP9229I5
0.15	*10*	*0.15*	*20 to 250/260*	*CP9200*	
	15	*0.15*	*20 to 250/260*	*CP9201*	
	20	*0.15*	*20 to 250/260*	*CP9220*	
	30	*0.15*	*20 to 250/260*	*CP9202*	
0.25	15	0.25	20 to 250/260	CP9203	
		0.50	20 to 250/260	CP9221	
	25	0.20	20 to 250/260	CP9204	
	30	0.25	20 to 250/260	CP9205	CP9205I5
		0.50	20 to 250/260	CP9222	
		1.00	20 to 240	CP9206	
	60	0.25	20 to 250/260	CP9207	
		0.50	20 to 240	CP9223	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

(Continued)

VF-WAXms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.32	15	0.25	20 to 250/260	CP9209	
		0.50	20 to 250/260	CP9224	
		1.00	20 to 250/260	CP9208	
	30	0.25	20 to 250/260	CP9212	CP9212I5
		0.50	20 to 250/260	CP9210	
		1.00	20 to 240	CP9211	
	60	0.25	20 to 250/260	CP9214	
		0.50	20 to 240	CP9225	CP9225I5
		1.00	20 to 230	CP9213	
0.53	15	1.00	20 to 250/260	CP9226	CP9226I5
		2.00	20 to 240	CP9227	
	30	1.00	20 to 240	CP9215	
		2.00	20 to 230	CP9216	
	60	1.00	20 to 230	CP9228	
		2.00	20 to 220	CP9217	


TIPS & TOOLS

As a special MS-type phase, the VF-WAXms column generates less bleed, and therefore less noise and higher signal-to-noise ratios for critical components.

VF-624ms and VF-1301ms

- VF-624ms is designed for analyzing solvents according to EPA Methods 524, 624 and 8260, as well as USP 467
- VF-1301ms ultra-low-bleed thin-film has a similar selectivity to 624 and is suitable for semivolatile organic solvents, as well as PCBs and pesticides
- Enhanced selectivity for USP 467 eliminates coelution of benzene and 1,2-dichloroethane
- Mid polarity
- Low bleed
- 0.15 mm id columns available for high efficiency GC and GC/MS analyses
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation

Similar Phases: AT-624, Rxi-624 Sil MS, Rtx-624, PE-624, 007-624, 007-502, ZB-624



Structure of VF-624ms and VF-1301ms

VF-624ms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.15	*15*	*0.84*	*-40 to 280/300*	*CP9101*	*CP9101I5*
	20	*0.84*	*-40 to 280/300*	*CP9100*	
	30	*0.84*	*-40 to 280/300*	*CP9109*	
	40	*0.84*	*-40 to 280/300*	*CP9110*	
0.25	30	1.40	-40 to 280/300	CP9102	CP9102I5
	60	1.40	-40 to 280/300	CP9103	CP9103I5
0.32	30	1.80	-40 to 280/300	CP9104	CP9104I5
	60	1.80	-40 to 280/300	CP9105	CP9105I5
0.53	30	3.00	-40 to 280/300	CP9106	CP9106I5
	60	3.00	-40 to 265/280	CP9107	
	75	3.00	-40 to 265/280	CP9108	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

Similar Phases: Rtx-1301, PE-1301

VF-1301ms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.10	10	1.00	-40 to 280/300	CP9066	
0.15	*15*	*0.15*	*-40 to 280/300*	*CP9050*	
	20	*0.15*	*-40 to 280/300*	*CP9051*	
0.25	15	1.00	-40 to 280/300	CP9052	
	30	0.25	-40 to 280/300	CP9053	
		1.00	-40 to 280/300	CP9054	
	60	0.25	-40 to 280/300	CP9055	
		1.00	-40 to 280/300	CP9056	
0.32	15	0.25	-40 to 280/300	CP9057	
		1.00	-40 to 280/300	CP9058	
	30	0.25	-40 to 280/300	CP9059	
		1.00	-40 to 280/300	CP9060	CP9060I5
	60	1.00	-40 to 280/300	CP9061	
0.53	15	1.00	-40 to 280/300	CP9062	
	30	1.00	-40 to 280/300	CP9063	
		1.50	-40 to 280/300	CP9064	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

TIPS & TOOLS


Ensure a lifetime of peak performance and maximum productivity with Agilent's comprehensive GC supplies portfolio, learn more at **www.agilent.com/chem/GCsupplies**



VF-1701ms

- Ultra-low bleed 14% cyanopropyl/phenyl/86% polydimethylsiloxane phase
- Mid polarity
- Ideal for pesticides, PCBs and semi-volatile organic compounds
- Highly inert for difficult analytes such as p,p'-DDT
- Deactivated for accurate trace analysis
- Engineered for reduced bleed, (bleed specification is 2 pA @ 280 °C for a 0.25 mm x 60 m, 0.25 µm id column)
- 0.15 mm id columns available for high efficiency GC and GC/MS analyses
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation

Similar Phases: SPB-1701, Rtx-1701, BP-10, OV-1701, 007-1701, ZB-1701



Structure of VF-1701ms

VF-1701ms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.10	10	0.20	-20 to 280/300	CP9140	
		0.40	-20 to 280/300	CP9141	
	20	0.10	-20 to 280/300	CP9142	
0.15	*15*	*0.10*	*-20 to 280/300*	*CP9175*	
		0.15	*-20 to 280/300*	*CP9143*	
		0.60	*-20 to 280/300*	*CP9144*	
	20	*0.15*	*-20 to 280/300*	*CP9145*	
		0.60	*-20 to 280/300*	*CP9146*	
0.25	15	0.15	-20 to 280/300	CP9147	
		0.25	-20 to 280/300	CP9148	
		1.00	-20 to 280/300	CP9149	CP9149I5
	30	0.15	-20 to 280/300	CP9150	
		0.25	-20 to 280/300	CP9151	CP9151I5
		1.00	-20 to 280/300	CP9152	CP9152I5
	60	0.15	-20 to 280/300	CP9153	
		0.25	-20 to 280/300	CP9154	CP9154I5
		0.50	-20 to 280/300	CP9155	CP9155I5
		1.00	-20 to 280/300	CP9156	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

(Continued)

VF-1701ms

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.32	15	0.15	-20 to 280/300	CP9157	
		0.25	-20 to 280/300	CP9158	
		1.00	-20 to 280/300	CP9159	
	30	0.10	-20 to 280/300	CP9160	
		0.15	-20 to 280/300	CP9161	
		0.25	-20 to 280/300	CP9162	
		1.00	-20 to 280/300	CP9163	
	60	0.15	-20 to 280/300	CP9164	
		0.25	-20 to 280/300	CP9165	
		1.00	-20 to 280/300	CP9166	CP9166I5
0.53	15	1.00	-20 to 280/300	CP9167	
	30	0.10	-20 to 280/300	CP9168	
		0.25	-20 to 280/300	CP9169	
		0.50	-20 to 280/300	CP9170	
		1.00	-20 to 280/300	CP9171	
		1.50	-20 to 280/300	CP9172	
	60	1.00	-20 to 280/300	CP9173	
		1.50	-20 to 265/280	CP9174	


Premium Polysiloxane Columns

Polysiloxanes are the most common stationary phases. They are available in the greatest variety and are stable, robust and versatile. Standard polysiloxanes are characterized by the repeating siloxane backbone. Each silicon atom contains two functional groups. The type and percent level of substitution of the groups distinguish each stationary phase and its properties.

DB-1

- 100% Dimethylpolysiloxane
- Non-polar
- Excellent general purpose column
- Wide range of applications
- Low bleed
- High temperature limit
- Bonded and cross-linked
- Solvent rinsable
- Wide range of column dimensions available
- Equivalent to USP Phase G2

Similar Phases: SPB-1, Rtx-1, BP-1, OV-1, OV-101, 007-1(MS), SP-2100, SE-30, ZB-1, AT-1, MDN-1, ZB-1

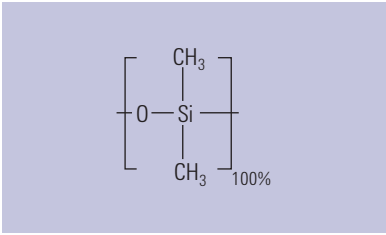

Structure of DB-1

DB-1

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.05	10	0.05	-60 to 325/350	126-1012		126-1012LTM
		0.20	-60 to 325/350	126-1013		126-1013LTM
0.10	5	0.12	-60 to 325/350	127-100A		127-100ALTM
	10	0.10	-60 to 325/350	127-1012	127-1012E	127-1012LTM
		0.40	-60 to 325/350	127-1013	127-1013E	127-1013LTM
	20	0.10	-60 to 325/350	127-1022	127-1022E	127-1022LTM
		0.40	-60 to 325/350	127-1023	127-1023E	127-1023LTM
	40	0.20	-60 to 325/350	127-1046	127-1046E	
		0.40	-60 to 325/350	127-1043		

(Continued)

DB-1

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.15	*10*	*1.20*	*-60 to 325/350*	*12A-1015*		*12A-1015LTM*
0.18	*10*	*0.18*	*-60 to 325/350*	*121-1012*	*121-1012E*	*121-1012LTM*
		0.20	*-60 to 325/350*	*121-101A*		*121-101ALTM*
		0.40	*-60 to 325/350*	*121-1013*	*121-1013E*	*121-1013LTM*
	20	*0.18*	*-60 to 325/350*	*121-1022*	*121-1022E*	*121-1022LTM*
		0.40	*-60 to 325/350*	*121-1023*		*121-1023LTM*
	40	*0.40*	*-60 to 325/350*	*121-1043*	*121-1043E*	
0.20	12	0.33	-60 to 325/350	128-1012		128-1012LTM
	25	0.33	-60 to 325/350	128-1022		128-1022LTM
	30	0.80	-60 to 325/350	128-1034		128-1034LTM
	50	0.33	-60 to 325/350	128-1052		
0.25	15	0.10	-60 to 325/350	122-1011		122-1011LTM
		0.25	-60 to 325/350	122-1012		122-1012LTM
		1.00	-60 to 325/350	122-1013		122-1013LTM
	25	0.25	-60 to 325/350	122-1022		122-1022LTM
	30	0.10	-60 to 325/350	122-1031		122-1031LTM
		0.25	-60 to 325/350	122-1032	122-1032E	122-1032LTM*
		0.50	-60 to 325/350	122-103E		122-103ELTM
		1.00	-60 to 325/350	122-1033	122-1033E	122-1033LTM
	50	0.25	-60 to 325/350	122-1052		
	60	0.10	-60 to 325/350	122-1061		
		0.25	-60 to 325/350	122-1062		
		0.50	-60 to 325/350	122-106E		
		1.00	-60 to 325/350	122-1063		
	100	0.50	-60 to 325/350	122-10AE		
	150	1.00	-60 to 325/350	122-10G3		

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

(Continued)

DB-1

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.32	10	0.50	-60 to 325/350	123-100E		123-100ELTM
	15	0.10	-60 to 325/350	123-1011		123-1011LTM
		0.25	-60 to 325/350	123-1012		123-1012LTM
		1.00	-60 to 325/350	123-1013		123-1013LTM
		3.00	-60 to 280/300	123-1014		123-1014LTM
		5.00	-60 to 280/300	123-1015		123-1015LTM
	25	0.12	-60 to 325/350	123-1027		123-1027LTM
		0.25	-60 to 325/350	123-1022		123-1022LTM
		0.52	-60 to 325/350	123-1026		123-1026LTM
		1.05	-60 to 325/350	123-102F		123-102FLTM
	30	0.10	-60 to 325/350	123-1031		123-1031LTM
		0.25	-60 to 325/350	123-1032		123-1032LTM
		0.50	-60 to 325/350	123-103E		123-103ELTM
		1.00	-60 to 325/350	123-1033	123-1033E	123-1033LTM
		1.50	-60 to 300/320	123-103B		123-103BLTM
		3.00	-60 to 280/300	123-1034		123-1034LTM
		5.00	-60 to 280/300	123-1035		123-1035LTM
	50	0.25	-60 to 325/350	123-1052		
		0.52	-60 to 325/350	123-1056		
		1.05	-60 to 325/350	123-105F		
		1.20	-60 to 325/350	123-105C		
		5.00	-60 to 280/300	123-1055		
	60	0.10	-60 to 325/350	123-1061		
		0.25	-60 to 325/350	123-1062	123-1062E	
		0.50	-60 to 325/350	123-106E		
		1.00	-60 to 325/350	123-1063	123-1063E	
		1.50	-60 to 300/320	123-106B	123-106BE	
		2.00	-60 to 280/300	123-106G		
		3.00	-60 to 280/300	123-1064	123-1064E	
		5.00	-60 to 280/300	123-1065	123-1065E	
0.45	30	1.27	-60 to 325/350	124-1032		124-1032LTM
		2.55	-60 to 260/280	124-1034		124-1034LTM


(Continued)

DB-1

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.53	5	0.88	-60 to 325/350	125-100A		125-100ALTM
		2.65	-60 to 325/350	125-100B		125-100BLTM
		5.00	-60 to 325/350	125-1005		125-1005LTM
	7.5	1.50	-60 to 325/350	125-1002		125-1002LTM
	10	2.65	-60 to 260/280	125-10HB	125-10HBE	125-10HBLTM
		5.00	-60 to 260/280	125-10H5		125-10H5LTM
	15	0.15	-60 to 340/360	125-1011	125-1011E	125-1011LTM
		0.25	-60 to 320/340	125-101K		125-101KLTM
		0.50	-60 to 300/320	125-1017		125-1017LTM
		1.00	-60 to 300/320	125-101J		125-101JLTM
		1.50	-60 to 300/320	125-1012	125-1012E	125-1012LTM
		3.00	-60 to 260/280	125-1014		125-1014LTM
		5.00	-60 to 260/280	125-1015		125-1015LTM
	25	1.00	-60 to 300/320	125-102J		125-102JLTM
		5.00	-60 to 260/280	125-1025		125-1025LTM
	30	0.10	-60 to 340/360	125-1039		
		0.25	-60 to 320/340	125-103K	125-103KE	125-103KLTM
		0.50	-60 to 300/320	125-1037		125-1037LTM
		1.00	-60 to 300/320	125-103J		125-103JLTM
		1.50	-60 to 300/320	125-1032		125-1032LTM
		2.65	-60 to 260/280	125-103B		125-103BLTM
		3.00	-60 to 260/280	125-1034	125-1034E	125-1034LTM
		5.00	-60 to 260/280	125-1035	125-1035E	125-1035LTM
	50	5.00	-60 to 260/280	125-1055		
	60	1.00	-60 to 300/320	125-106J	125-106JE	
		1.50	-60 to 300/320	125-1062	125-1062E	
		3.00	-60 to 260/280	125-1064		
		5.00	-60 to 260/280	125-1065	125-1065E	
	105	5.00	-60 to 260/280	125-10B5		

HP-1

- 100% Dimethylpolysiloxane
- Non-polar
- Excellent general purpose column – "Industry Standard"
- Wide range of applications
- Superior performance for low molecular weight alcohols (< C_5)
- High temperature limit
- Bonded and cross-linked
- Solvent rinsable
- Wide range of column dimensions available
- Equivalent to USP Phase G2

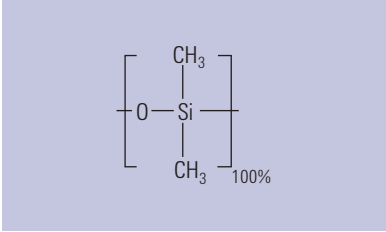

Structure of HP-1

Similar Phases: SPB-1, Rtx-1, BP-1, OV-1, OV-101, 007-1(MS), SP-2100, SE-30, ZB-1, AT-1, MDN-1, ZB-1

HP-1

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.18	*20*	*0.18*	*-60 to 325/350*	*19091Z-577*	*19091Z-577E*	*19091Z-577LTM*
0.20	12	0.33	-60 to 325/350	19091-60312		
	17	0.11	-60 to 325/350	19091Z-008		19091Z-008LTM
	25	0.11	-60 to 325/350	19091Z-002		19091Z-002LTM
		0.33	-60 to 325/350	19091Z-102	19091Z-102E	19091Z-102LTM
		0.50	-60 to 325/350	19091Z-202		19091Z-202LTM
	50	0.11	-60 to 325/350	19091Z-005		
		0.33	-60 to 325/350	19091Z-105		
		0.50	-60 to 325/350	19091Z-205		
0.25	15	0.10	-60 to 325/350	19091Z-331		19091Z-331LTM
		0.25	-60 to 325/350	19091Z-431		19091Z-431LTM
		1.00	-60 to 325/350	19091Z-231		19091Z-231LTM
	30	0.10	-60 to 325/350	19091Z-333		19091Z-333LTM
		0.25	-60 to 325/350	19091Z-433	19091Z-433E	19091Z-433LTM
		1.00	-60 to 325/350	19091Z-233	19091Z-233E	19091Z-233LTM
	60	0.25	-60 to 325/350	19091Z-436		
		1.00	-60 to 325/350	19091Z-236	19091Z-236E	
	100	0.50	-60 to 325/350	19091Z-530	19091Z-530E	


Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

(Continued)

HP-1

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.32	15	0.25	-60 to 325/350	19091Z-411	19091Z-411E	19091Z-411LTM
		1.00	-60 to 325/350	19091Z-211		19091Z-211LTM
	25	0.17	-60 to 325/350	19091Z-012	19091Z-012E	19091Z-012LTM
		0.52	-60 to 325/350	19091Z-112	19091Z-112E	19091Z-112LTM
		1.05	-60 to 325/350	19091Z-212		19091Z-212LTM
	30	0.10	-60 to 325/350	19091Z-313	19091Z-313E	19091Z-313LTM
		0.25	-60 to 325/350	19091Z-413	19091Z-413E	19091Z-413LTM
		1.00	-60 to 325/350	19091Z-213	19091Z-213E	19091Z-213LTM
		3.00	-60 to 260/280	19091Z-513	19091Z-513E	19091Z-513LTM
		4.00	-60 to 260/280	19091Z-613		19091Z-613LTM
		5.00	-60 to 260/280	19091Z-713	19091Z-713E	19091Z-713LTM
	50	0.17	-60 to 325/350	19091Z-015		
		0.52	-60 to 325/350	19091Z-115	19091Z-115E	
		1.05	-60 to 325/350	19091Z-215		
	60	0.25	-60 to 325/350	19091Z-416		
		1.00	-60 to 325/350	19091Z-216	19091Z-216E	
		5.00	-60 to 260/280	19091Z-716		
0.53	5	0.15	-60 to 320/400	19095Z-220		
		0.88	-60 to 320/400	19095Z-020		
			-60 to 325/350	125-100A		
		2.65	-60 to 260/280	19095S-100	19095S-100E	19095S-100LTM
	7.5	5.00	-60 to 260/280	19095Z-627	19095Z-627E	19095Z-627LTM
	10	0.88	-60 to 300/320	19095Z-021	19095Z-021E	19095Z-021LTM
		2.65	-60 to 260/280	19095Z-121	19095Z-121E	19095Z-121LTM
	15	0.15	-60 to 320/400	19095Z-221	19095Z-221E	
		1.50	-60 to 300/320	19095Z-321		19095Z-321LTM
		3.00	-60 to 260/280	19095Z-421	19095Z-421LTM	19095Z-421LTM
		5.00	-60 to 260/280	19095Z-621		19095Z-621LTM
	30	0.88	-60 to 300/320	19095Z-023	19095Z-023E	19095Z-023LTM
		1.50	-60 to 300/320	19095Z-323	19095Z-323E	19095Z-323LTM
		2.65	-60 to 260/280	19095Z-123	19095Z-123E	19095Z-123LTM
		3.00	-60 to 260/280	19095Z-423	19095Z-423E	19095Z-423LTM
		5.00	-60 to 260/280	19095Z-623	19095Z-623E	19095Z-623LTM
	60	5.00	-60 to 260/280	19095Z-626		

CP-Sil 5 CB

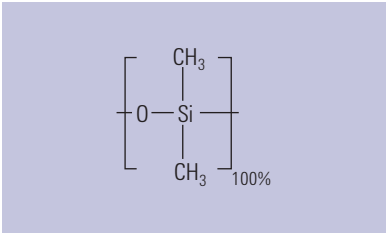

Structure of CP-Sil 5 CB

- 100% dimethylpolysiloxane
- Non-polar
- General purpose phase
- Bonded and cross-linked
- Solvent rinsable
- Available in Fused Silica or UltiMetal
- Separation almost entirely based on boiling points, making this column suitable for a wide range of applications with a broad temperature range
- High temperature limit
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation

Similar Phases: SPB-1, Rtx-1, BP-1, OV-1, OV-101, 007-1(MS), SP-2100, SE-30, ZB-1, AT-1, MDN-1, ZB-1

CP-Sil 5 CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.10	5	0.12	-60 to 330/350	CP7300	
	10	0.10	-60 to 330/350	CP7311	
		0.12	-60 to 330/350	CP7310	CP7310I5
		0.40	-60 to 325/350	CP7312	
	20	0.10	-60 to 330/350	CP7313	
0.15	*10*	*0.12*	*-60 to 330/350*	*CP7684*	*CP7684I5*
		2.00	*-60 to 325/350*	*CP7682*	*CP7682I5*
	25	*0.12*	*-60 to 330/350*	*CP7694*	
		1.20	*-60 to 325/350*	*CP7693*	
		2.00	*-60 to 325/350*	*CP7692*	*CP7692I5*
0.20	12	0.33	-60 to 325/350	CP7602	
	15	0.20	-60 to 330/350	CP7604	
	25	0.33	-60 to 325/350	CP7622	
	30	0.80	-60 to 325/350	CP7633	
	50	0.11	-60 to 330/350	CP7642	
		0.33	-60 to 325/350	CP7643	CP7643I5
		0.50	-60 to 325/350	CP7644	CP7644I5

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

(Continued)

CP-Sil 5 CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	10	0.12	-60 to 330/350	CP7700	
	15	0.25	-60 to 330/350	CP8510	
	25	0.12	-60 to 330/350	CP7710	CP7710I5
		0.25	-60 to 330/350	CP7441	
		0.40	-60 to 325/350	CP7709	
		1.20	-60 to 325/350	CP7670	CP7670I5
	30	0.10	-60 to 330/350	CP8710	
		0.25	-60 to 330/350	CP8741	CP8741I5
		1.00	-60 to 325/350	CP8770	
	50	0.12	-60 to 330/350	CP7720	
		0.25	-60 to 330/350	CP7443	CP7443I5
		0.40	-60 to 325/350	CP7719	CP7719I5
	60	0.25	-60 to 330/350	CP8743	CP8743I5
		1.00	-60 to 325/350	CP8780	CP8780I5
0.32	10	0.12	-60 to 330/350	CP7730	
		1.20	-60 to 325/350	CP7758	CP7758I5
	15	0.10	-60 to 330/350	CP8529	
		0.25	-60 to 325/350	CP8530	
		3.00	-60 to 325/350	CP8550	CP8550I5
		1.00	-60 to 325/350	CP8540	
		5.00	-60 to 300/325	CP8560	CP8560I5
	25	0.12	-60 to 330/350	CP7740	
		0.25	-60 to 325/350	CP7442	
		0.40	-60 to 325/350	CP7739	
		0.52	-60 to 325/350	CP8430	CP8430I5
		1.20	-60 to 325/350	CP7760	CP7760I5
		5.00	-60 to 300/325	CP7680	CP7680I5
	30	0.25	-60 to 325/350	CP8742	CP8742I5
		1.00	-60 to 325/350	CP8760	CP8760I5
		3.00	-60 to 310/335	CP8687	CP8687I5
		5.00	-60 to 300/325	CP8688	CP8688I5
	50	0.12	-60 to 330/335	CP7750	CP7750I5
		0.25	-60 to 325/350	CP7444	CP7444I5
		0.40	-60 to 325/350	CP7749	CP7749I5
		1.20	-60 to 325/350	CP7770	CP7770I5
		5.00	-60 to 300/325	CP7690	CP7690I5
	60	0.25	-60 to 325/350	CP8744	CP8744I5
		1.00	-60 to 325/350	CP8870	
		3.00	-60 to 310/335	CP8689	
		5.00	-60 to 300/325	CP8690	CP8690I5

(Continued)

CP-Sil 5 CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.53	10	1.00	-60 to 315/340	CP7625	
		2.00	-60 to 305/330	CP7620	CP7620I5
		5.00	-60 to 290/325	CP7645	
	15	0.15	-60 to 330/350	CP8673	CP8673I5
		1.50	-60 to 305/330	CP8674	CP8674I5
		3.00	-60 to 300/325	CP8675	
		5.00	-60 to 290/325	CP8676	
	20	5.00	-60 to 290/325	CP8774	
	25	1.00	-60 to 315/340	CP7635	CP7635I5
		2.00	-60 to 305/330	CP7630	
		5.00	-60 to 290/325	CP7675	CP7675I5
	30	1.50	-60 to 305/330	CP8735	CP8735I5
		2.00	-60 to 305/330	CP8730	CP8730I5
		3.00	-60 to 300/325	CP8677	CP8677I5
		5.00	-60 to 290/325	CP8775	CP8775I5
	50	1.00	-60 to 315/340	CP7695	
		2.00	-60 to 305/330	CP7640	
		5.00	-60 to 290/325	CP7685	CP7685I5
	60	1.50	-60 to 305/330	CP8799	
		5.00	-60 to 290/325	CP8685	
	100	0.50	-60 to 325/350	CP7608	
		2.00	-60 to 305/330	CP7650	
		5.00	-60 to 290/325	CP7688	

CP-Sil 5 CB UltiMetal

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.53	10	1.00	-60 to 325/350	CP7120	
		2.00	-60 to 325/350	CP7150	
		5.00	-60 to 325/350	CP6666	CP6666I5
	25	0.50	-60 to 325/350	CP7135	CP7135I5
		2.00	-60 to 325/350	CP7160	
		5.00	-60 to 325/350	CP6670	
	50	0.50	-60 to 325/350	CP7195	
		1.00	-60 to 325/350	CP7140	
		2.00	-60 to 325/350	CP7170	
		5.00	-60 to 325/350	CP6671	

TIPS & TOOLS


Agilent CrossLab GC supplies, including CrossLab Ultra Inert liners, perform seamlessly with a variety of instruments regardless of make or model, including Varian (now Bruker), PerkinElmer, Shimadzu, and Thermo Scientific GC systems. Learn more at **www.agilent.com/chem/CrossLab**



Ultra 1

- 100% Dimethylpolysiloxane
- Non-polar
- Equivalent to HP-1 with tighter specifications for retention index and capacity factors
- Bonded and cross-linked
- Solvent rinsable


Similar Phases: SPB-1, Rtx-1, BP-1, 007-1(MS)



Structure of Ultra 1

Ultra 1

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.20	12	0.33	-60 to 325/350	19091A-101		19091A-101LTM
	17	0.11	-60 to 325/350	19091A-008		19091A-008LTM
		0.33	-60 to 325/350	19091A-108		19091A-108LTM
	25	0.11	-60 to 325/350	19091A-002		19091A-002LTM
		0.33	-60 to 325/350	19091A-102	19091A-102E	19091A-102LTM
	50	0.11	-60 to 325/350	19091A-005		
		0.33	-60 to 325/350	19091A-105		
0.32	25	0.17	-60 to 325/350	19091A-012		19091A-012LTM
		0.52	-60 to 325/350	19091A-112		19091A-112LTM
	50	0.17	-60 to 325/350	19091A-015		
		0.52	-60 to 325/350	19091A-115		

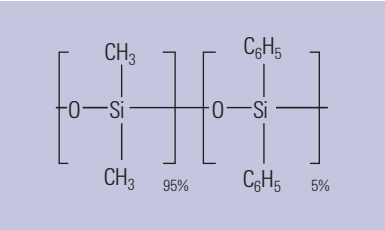

Structure of Ultra 2

Ultra 2

- (5%-Phenyl)-methylpolysiloxane
- Non-polar
- Equivalent to HP-5 with tighter specifications for retention index and capacity factors
- Bonded and cross-linked
- Solvent rinsable

Similar Phases: SPB-5, Rtx-5, BP-5, CB-5, 007-5, 2B-5


Ultra 2

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.20	12	0.33	-60 to 325/350	19091B-101		19091B-101LTM
	25	0.11	-60 to 325/350	19091B-002		19091B-002LTM
		0.33	-60 to 325/350	19091B-102	19091B-102E	19091B-102LTM
	50	0.11	-60 to 325/350	19091B-005		
		0.33	-60 to 325/350	19091B-105	19091B-105E	
0.32	25	0.17	-60 to 325/350	19091B-012	19091B-012E	19091B-012LTM
		0.52	-60 to 325/350	19091B-112		19091B-112LTM
	50	0.17	-60 to 325/350	19091B-015		
		0.52	-60 to 325/350	19091B-115	19091B-115E	

DB-5

- (5%-Phenyl)-methylpolysiloxane
- Non-polar
- Excellent general purpose column
- Wide range of applications
- Low bleed
- High temperature limit
- Bonded and cross-linked
- Solvent rinsable
- Wide range of column dimensions available
- Equivalent to USP Phase G27

Similar Phases: SPB-5, Rtx-5, BP-5, OV-5, 007-2(MPS-5), SE-52, SE-54, XTI-5, PTE-5, ZB-5, AT-5, MDN-5, ZB-5



Structure of DB-5

DB-5

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.10	10	0.10	-60 to 325/350	127-5012	127-5012E	127-5012LTM
		0.17	-60 to 325/350	127-501E	127-501EE	127-501ELTM
		0.33	-60 to 325/350	127-501N		127-501NLTM
		0.40	-60 to 325/350	127-5013		127-5013LTM
	20	0.10	-60 to 325/350	127-5022	127-5022E	127-5022LTM
		0.40	-60 to 325/350	127-5023		127-5023LTM
0.15	*10*	*1.20*	*-60 to 300/320*	*12A-5015*		*12A-5015LTM*
0.18	*10*	*0.18*	*-60 to 325/350*	*121-5012*	*121-5012E*	*121-5012LTM*
		0.40	*-60 to 325/350*	*121-5013*		*121-5013LTM*
	20	*0.18*	*-60 to 325/350*	*121-5022*	*121-5022E*	*121-5022LTM*
		0.40	*-60 to 325/350*	*121-5023*	*121-5023E*	*121-5023LTM*
	40	*0.18*	*-60 to 325/350*	*121-5042*		

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

(Continued)


DB-5

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.20	12	0.33	-60 to 325/350	128-5012		128-5012LTM
	15	0.20	-60 to 325/350	128-50H7		128-50H7LTM
	25	0.33	-60 to 325/350	128-5022		128-5022LTM
	50	0.33	-60 to 325/350	128-5052		
0.25	15	0.10	-60 to 325/350	122-5011		122-5011LTM
		0.25	-60 to 325/350	122-5012		122-5012LTM
		0.50	-60 to 325/350	122-501E		122-501ELTM
		1.00	-60 to 325/350	122-5013		122-5013LTM
	25	0.25	-60 to 325/350	122-5022		122-5022LTM
	30	0.10	-60 to 325/350	122-5031		122-5031LTM
		0.25	-60 to 325/350	122-5032	122-5032E	122-5032LTM
		0.50	-60 to 325/350	122-503E		122-503ELTM
		1.00	-60 to 325/350	122-5033	122-5033E	122-5033LTM
	50	0.25	-60 to 325/350	122-5052		
	60	0.10	-60 to 325/350	122-5061		
		0.25	-60 to 325/350	122-5062		
		0.50	-60 to 325/350	122-506E		
		1.00	-60 to 325/350	122-5063		
0.32	10	0.50	-60 to 325/350	123-500E		123-500ELTM
	15	0.10	-60 to 325/350	123-5011		123-5011LTM
		0.25	-60 to 325/350	123-5012	123-5012E	123-5012LTM
		1.00	-60 to 325/350	123-5013	123-5013E	123-5013LTM
	25	0.17	-60 to 325/350	123-502D		123-502DLTM
		0.25	-60 to 325/350	123-5022		123-5022LTM
		0.52	-60 to 325/350	123-5026		123-5026LTM
		1.05	-60 to 325/350	123-502F		123-502FLTM
	30	0.10	-60 to 325/350	123-5031		123-5031LTM
		0.25	-60 to 325/350	123-5032	123-5032E	123-5032LTM
		0.50	-60 to 325/350	123-503E		123-503ELTM
		1.00	-60 to 325/350	123-5033	123-5033E	123-5033LTM
		1.50	-60 to 325/350	123-503B		123-503BLTM
	50	0.25	-60 to 325/350	123-5052		
		0.52	-60 to 325/350	123-5056		
		1.00	-60 to 325/350	123-5053		
	60	0.25	-60 to 325/350	123-5062		
		1.00	-60 to 325/350	123-5063	123-5063E	

(Continued)

DB-5

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.45	15	1.27	-60 to 300/320	124-5012		124-5012LTM
	30	0.42	-60 to 300/320	124-5037		124-5037LTM
		1.27	-60 to 300/320	124-5032		124-5032LTM
0.53	10	2.65	-60 to 260/280	125-50HB		125-50HBLTM
	15	0.25	-60 to 300/320	125-501K		125-501KLTM
		0.50	-60 to 300/320	125-5017		125-5017LTM
		1.00	-60 to 300/320	125-501J		125-501JLTM
		1.50	-60 to 300/320	125-5012	125-5012E	125-5012LTM
	25	5.00	-60 to 260/280	125-5025		125-5025LTM
	30	0.25	-60 to 300/320	125-503K		125-503KLTM
		0.50	-60 to 300/320	125-5037		125-5037LTM
		0.88	-60 to 300/320	125-503D		125-503DLTM
		1.00	-60 to 300/320	125-503J		125-503JLTM
		1.50	-60 to 300/320	125-5032	125-5032E	125-5032LTM
		2.65	-60 to 260/280	125-503B		125-503BLTM
		3.00	-60 to 260/280	125-5034	125-5034E	125-5034LTM
		5.00	-60 to 260/280	125-5035	125-5035E	125-5035LTM
	60	1.50	-60 to 300/320	125-5062	125-5062E	
		5.00	-60 to 260/280	125-5065	125-5065E	

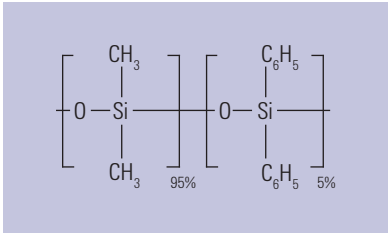

Structure of HP-5

HP-5

- (5%-Phenyl)-methylpolysiloxane
- Non-polar
- Excellent general purpose column
- Wide range of applications
- High temperature limit
- Bonded and cross-linked
- Solvent rinsable
- Wide range of column dimensions available
- Equivalent to USP Phase G27

Similar Phases: SPB-5, Rtx-5, BP-5, OV-5, 007-2(MPS-5), SE-52, SE-54, XTI-5, PTE-5, ZB-5, AT-5, MDN-5, ZB-5

HP-5

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.18	*20*	*0.18*	*-60 to 325/350*	*19091J-577*	*19091J-577E*	*19091J-577LTM*
0.20	12	0.33	-60 to 325/350	19091J-101		19091J-101LTM
	17	0.33	-60 to 325/350	19091J-108		
	25	0.11	-60 to 325/350	19091J-002		19091J-002LTM
		0.33	-60 to 325/350	19091J-102	19091J-102E	19091J-102LTM
		0.50	-60 to 325/350	19091J-202		19091J-202LTM
	50	0.11	-60 to 325/350	19091J-005		
		0.33	-60 to 325/350	19091J-105	19091J-105E	
		0.50	-60 to 325/350	19091J-205		
0.25	5	0.10	-60 to 325/350	19091J-330		19091J-330LTM
	15	0.25	-60 to 325/350	19091J-431	19091J-431E	19091J-431LTM
		1.00	-60 to 325/350	19091J-231		19091J-231LTM
	30	0.10	-60 to 325/350	19091J-333		19091J-333LTM
		0.25	-60 to 325/350	19091J-433	19091J-433E	19091J-433LTM
		1.00	-60 to 325/350	19091J-233		19091J-233LTM
	60	0.25	-60 to 325/350	19091J-436	19091J-436E	
		1.00	-60 to 325/350	19091J-236	19091J-236E	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers


(Continued)

HP-5

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.32	15	0.25	-60 to 325/350	19091J-411		19091J-411LTM
	25	0.17	-60 to 325/350	19091J-012	19091J-012E	19091J-012LTM
		0.52	-60 to 325/350	19091J-112	19091J-112E	19091J-112LTM
		1.05	-60 to 325/350	19091J-212		19091J-212LTM
	30	0.10	-60 to 325/350	19091J-313		19091J-313LTM
		0.25	-60 to 325/350	19091J-413	19091J-413E	19091J-413LTM
		0.50	-60 to 325/350	19091J-113	19091J-113E	19091J-113LTM
		1.00	-60 to 325/350	19091J-213	19091J-213E	19091J-213LTM
	50	0.17	-60 to 325/350	19091J-015	19091J-015E	
		0.52	-60 to 325/350	19091J-115	19091J-115E	
		1.05	-60 to 325/350	19091J-215	19091J-215E	
	60	0.25	-60 to 325/350	19091J-416		
		1.00	-60 to 325/350	19091J-216	19091J-216E	
0.53	10	2.65	-60 to 260/280	19095J-121	19095J-121E	19095J-121LTM
	15	1.50	-60 to 300/320	19095J-321		19095J-321LTM
		5.00	-60 to 260/280	19095J-621		19095J-621LTM
	30	0.88	-60 to 300/320	19095J-023	19095J-023E	19095J-023LTM
		1.50	-60 to 300/320	19095J-323	19095J-323E	19095J-323LTM
		2.65	-60 to 260/280	19095J-123	19095J-123E	19095J-123LTM
		5.00	-60 to 260/280	19095J-623	19095J-623E	19095J-623LTM

TIPS & TOOLS

Learn more about Agilent's top-ranked service and support at **www.agilent.com/chem/services**

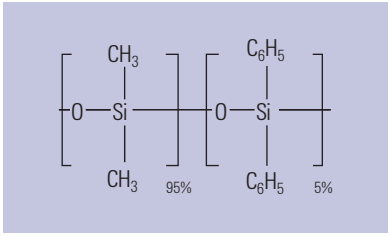

Structure of CP-Sil 8 CB

CP-Sil 8 CB

- (5% phenyl) methylpolysiloxane
- Non-polar
- General purpose phase
- Cross-linked and bonded
- Solvent rinsable
- Low bleed
- High column-to-column reproducibility
- Wide choice of dimensions available
- Available in Fused Silica and UltiMetal
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation

Similar Phases: SPB-5, Rtx-5, BP-5, OV-5, 007-2(MPS-5), SE-52, SE-54, XTI-5, PTE-5, ZB-5, AT-5, MDN-5, ZB-5

CP-Sil 8 CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.10	20	0.10	-60 to 330/350	CP7319	CP7319I5
0.15	*10*	*0.12*	*-60 to 330/350*	*CP7884*	
		1.20	*-60 to 325/350*	*CP7885*	
	25	*0.12*	*-60 to 330/350*	*CP7894*	
0.20	12	0.33	-60 to 325/350	CP7900	
	25	0.33	-60 to 325/350	CP7921	
	50	0.33	-60 to 325/350	CP7941	
	60	0.20	-60 to 330/350	CP7950	
0.25	15	0.25	-60 to 330/350	CP8511	
		1.00	-60 to 325/350	CP8521	
	25	0.12	-60 to 330/350	CP7711	
		0.25	-60 to 330/350	CP7451	CP7451I5
		0.40	-60 to 325/350	CP7759	
		1.20	-60 to 325/350	CP7671	
	30	0.25	-60 to 330/350	CP8751	CP8751I5
		1.00	-60 to 325/350	CP8771	CP8771I5
	50	0.12	-60 to 330/350	CP7721	
		0.25	-60 to 330/350	CP7453	CP7453I5
		0.40	-60 to 325/350	CP7769	
	60	0.10	-60 to 325/350	CP8750	
		0.25	-60 to 330/350	CP8753	
		1.00	-60 to 325/350	CP8781	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

(Continued)




CP-Sil 8 CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.32	10	0.12	-60 to 330/350	CP7731	
		5.00	-60 to 300/325	CP8014	CP8014I5
	15	0.25	-60 to 325/350	CP8531	
		1.00	-60 to 325/350	CP8541	
	25	0.12	-60 to 330/350	CP7741	CP7741I5
		0.25	-60 to 325/350	CP7452	
		0.40	-60 to 325/350	CP7779	
		0.52	-60 to 325/350	CP8431	
		1.20	-60 to 325/350	CP7761	
		5.00	-60 to 300/325	CP7681	CP7681I5
	30	0.10	-60 to 330/350	CP8791	
		0.25	-60 to 325/350	CP8752	CP8752I5
		1.00	-60 to 325/350	CP8761	CP8761I5
	50	0.12	-60 to 330/350	CP7751	CP7751I5
		0.25	-60 to 325/350	CP7454	
		0.40	-60 to 325/350	CP7789	
		1.20	-60 to 325/350	CP7771	
		5.00	-60 to 300/325	CP7691	CP7691I5
	60	0.25	-60 to 325/350	CP8754	
		1.00	-60 to 325/350	CP8871	CP8871I5
0.53	10	2.00	-60 to 305/330	CP7621	
		5.00	-60 to 290/325	CP7646	
	15	1.50	-60 to 305/330	CP8678	
	25	0.15	-60 to 325/350	CP7634	
		2.00	-60 to 305/330	CP7631	
		1.00	-60 to 315/340	CP7636	
		5.00	-60 to 290/325	CP7656	
	30	0.50	-60 to 325/350	CP8716	
		1.50	-60 to 305/330	CP8736	CP8736I5
		5.00	-60 to 290/325	CP8756	CP8756I5
	50	1.00	-60 to 315/340	CP7696	
		2.00	-60 to 305/330	CP7641	
		5.00	-60 to 290/325	CP7666	
	60	1.50	-60 to 305/330	CP8796	
	100	5.00	-60 to 290/325	CP7676	

CP-Sil 8 CB UltiMetal

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.53	25	5.00	-60 to 325/350	CP6680
	50	5.00	-60 to 325/350	CP7196



Structure of CP-Sil 13 CB
(with 14% phenyl substitution)

CP-Sil 13 CB

- 14% phenyl/86% dimethylpolysiloxane
- Mid polarity phase
- Specially developed for the analysis of medium polarity compounds
- Ideal for confirmational analyses using ECD
- Bonded and cross-linked
- Solvent rinsable
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation

Similar Phases: Rtx-20

CP-Sil 13 CB


ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.15	*25*	*0.40*	*-25 to 300/330*	*CP7813*	
0.25	25	0.20	-25 to 300/330	CP7906	
		0.40	-25 to 300/330	CP7916	
		1.20	-25 to 300/330	CP7977	CP7977I5
	50	0.20	-25 to 300/330	CP7907	
		0.40	-25 to 300/330	CP7917	
0.32	25	0.20	-25 to 300/330	CP7926	CP7926I5
		0.40	-25 to 300/330	CP7936	
		1.20	-25 to 300/330	CP7946	
	50	0.20	-25 to 300/330	CP7927	
		0.40	-25 to 300/330	CP7937	
		1.20	-25 to 300/330	CP7947	
0.53	10	1.00	-25 to 300/330	CP7609	
	25	1.00	-25 to 300/330	CP7619	
		2.00	-25 to 300/330	CP7649	
	50	1.00	-25 to 300/330	CP7629	
		2.00	-25 to 300/330	CP7659	
	100	2.00	-25 to 300/330	CP7669	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

DB-35

- (35%-Phenyl)-methylpolysiloxane
- Mid polarity – slightly more polar than HP-35
- Low bleed
- Inert to active solutes
- Ideal for confirmational analyses
- Bonded and cross-linked
- Solvent rinsable
- Equivalent to USP Phase G42


Similar Phases: Rtx-35, Rtx-35ms, Rxi-35Sil MS, SPB-35, AT-35, Sup-Herb, MDN-35, BPX-34, ZB-35, ZB-35 ht



Structure of DB-35

DB-35

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.25	30	0.25	40 to 300/320	122-1932		122-1932LTM
	60	0.25	40 to 300/320	122-1962		
0.32	30	0.25	40 to 300/320	123-1932		123-1932LTM
		0.50	40 to 300/320	123-1933	123-1933E	123-1933LTM
0.53	15	1.00	40 to 280/300	125-1912		125-1912LTM
	30	0.50	40 to 280/300	125-1937		125-1937LTM
		1.00	40 to 280/300	125-1932		125-1932LTM

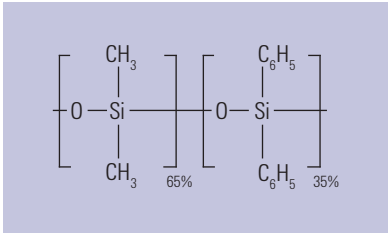

Structure of HP-35

HP-35

- (35%-Phenyl)-methylpolysiloxane
- Mid polarity – slightly less polar than DB-35
- Inert to active solutes
- Ideal for confirmational analyses
- Bonded and cross-linked
- Solvent rinsable
- Equivalent to USP Phase G42

Similar Phases: Rtx-35ms, Rxi-35Sil MS, SPB-35, AT-35, Sup-Herb, MDN-35, BPX-34, ZB-35, ZB-35 ht

HP-35

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.25	15	0.25	40 to 300/320	19091G-131	19091G-131E	19091G-131LTM
	30	0.25	40 to 300/320	19091G-133		19091G-133LTM
0.32	30	0.25	40 to 300/320	19091G-113		19091G-113LTM
		0.50	40 to 300/320	19091G-213		19091G-213LTM

TIPS & TOOLS


Order your free GC troubleshooting and GC column installation posters at **www.agilent.com/chem/GCposteroffer**



DB-17

- (50%-Phenyl)-methylpolysiloxane
- Mid polarity – slightly more polar than HP-50+
- Excellent for confirmational analyses
- Bonded and cross-linked
- Solvent rinsable
- Equivalent to USP Phase G3

Similar Phases: Rtx-50, 007-17(MPS-50), SP-2250, SPB-50, ZB-50, AT-50

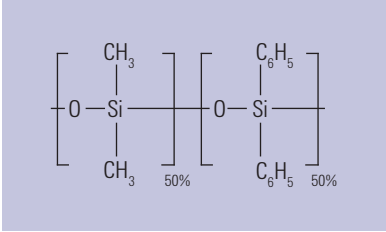


Structure of DB-17

DB-17

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.05	10	0.10	40 to 280/300	126-1713		126-1713LTM
0.10	10	0.10	40 to 280/300	127-1712		127-1712LTM
		0.20	40 to 280/300	127-1713		127-1713LTM
	20	0.10	40 to 280/300	127-1722		127-1722LTM
0.18	*20*	*0.18*	*40 to 280/300*	*121-1722*		*121-1722LTM*
		0.30	*40 to 280/300*	*121-1723*		*121-1723LTM*
0.25	15	0.15	40 to 280/300	122-1711		122-1711LTM
		0.25	40 to 280/300	122-1712		122-1712LTM
		0.50	40 to 280/300	122-1713	122-1713E	122-1713LTM
	30	0.15	40 to 280/300	122-1731	122-1731E	122-1731LTM
		0.25	40 to 280/300	122-1732	122-1732E	122-1732LTM
		0.50	40 to 280/300	122-1733		122-1733LTM
	60	0.25	40 to 280/300	122-1762		
0.32	15	0.15	40 to 280/300	123-1711		123-1711LTM
		0.25	40 to 280/300	123-1712		123-1712LTM
		0.50	40 to 280/300	123-1713		123-1713LTM
	30	0.15	40 to 280/300	123-1731		123-1731LTM
		0.25	40 to 280/300	123-1732	123-1732E	123-1732LTM
		0.50	40 to 280/300	123-1733	123-1733E	123-1733LTM
	60	0.25	40 to 280/300	123-1762		
0.53	5	2.00	40 to 280/300	125-1704		125-1704LTM
	15	0.25	40 to 260/280	125-1711		125-1711LTM
		0.50	40 to 260/280	125-1717		125-1717LTM
		1.00	40 to 260/280	125-1712		125-1712LTM
		1.50	40 to 260/280	125-1713		125-1713LTM
	30	0.25	40 to 260/280	125-1731		125-1731LTM
		0.50	40 to 260/280	125-1737		125-1737LTM
		1.00	40 to 260/280	125-1732	125-1732E	125-1732LTM
		1.50	40 to 260/280	125-1733		125-1733LTM
	60	1.00	40 to 260/280	125-1762		

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

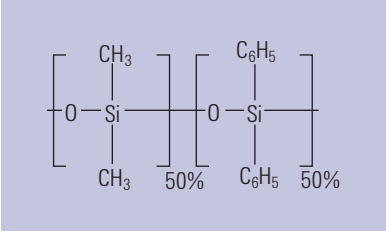

Structure of HP-50+

HP-50+

- (50%-Phenyl)-methylpolysiloxane
- Mid polarity – slightly less polar than DB-17
- Excellent for confirmational analyses
- Bonded and cross-linked
- Solvent rinsable
- Equivalent to USP Phase G3

Similar Phases: Rtx-50, 007-17(MPS-50), SP-2250, SPB-50, ZB-50, AT-50

HP-50+


ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.18	*20*	*0.18*	*40 to 280/300*	*19091L-577*		*19091L-577LTM*
0.20	12	0.31	40 to 280/300	19091L-101		19091L-101LTM
0.25	5	0.15	40 to 280/300	19091L-330		19091L-330LTM
	15	0.25	40 to 280/300	19091L-431		19091L-431LTM
	30	0.15	40 to 280/300	19091L-333		19091L-333LTM
		0.25	40 to 280/300	19091L-433		19091L-433LTM
		0.50	40 to 280/300	19091L-133		19091L-133LTM
0.32	15	0.50	40 to 280/300	19091L-111		19091L-111LTM
	30	0.25	40 to 280/300	19091L-413	19091L-413E	19091L-413LTM
		0.50	40 to 280/300	19091L-113	19091L-113E	19091L-113LTM
	60	0.25	40 to 280/300	19091L-416		
0.53	15	1.00	40 to 260/280	19095L-021		19095L-021LTM
	30	0.50	40 to 260/280	19095L-523	19095L-523E	19095L-523LTM
		1.00	40 to 260/280	19095L-023	19095L-023E	19095L-023LTM

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

CP-Sil 24 CB

- 50% phenyl/50% dimethylpolysiloxane
- Mid polarity phase
- Specially suitable for analysis of amines, drugs and pesticides
- Ideal for analysis using ECD
- Excellent confirmation column in combination with CP-Sil 5 CB or CP-Sil 8 CB
- Bonded and cross-linked
- Solvent rinsable
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation


Similar Phases: Rtx-50, 007-17(MPS-50), SP-2250, SPB-50, ZB-50, AT-50

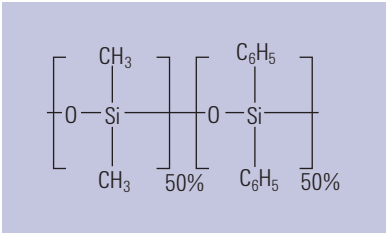

Structure of CP-Sil 24 CB

CP-Sil 24 CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	15	0.25	40 to 280/300	CP7820	
	30	0.25	40 to 280/300	CP7821	
		0.50	40 to 280/300	CP7824	
	60	0.25	40 to 280/300	CP7822	CP7822I5
		0.50	40 to 280/300		CP7825I5
0.32	15	0.25	40 to 280/300	CP7830	CP7830I5
	30	0.25	40 to 280/300	CP7831	CP7831I5
	60	0.25	40 to 280/300	CP7832	
0.53	15	1.00	40 to 265/290	CP7870	
	30	0.50	40 to 280/300	CP7834	CP7834I5
		1.00	40 to 265/290	CP7871	CP7871I5

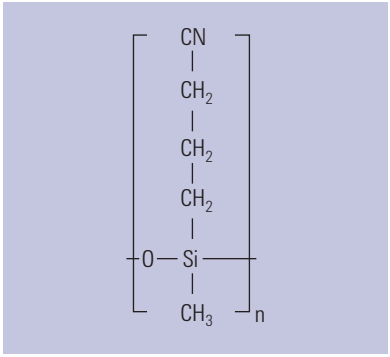

Structure of DB-23

DB-23

- (50%-Cyanopropyl)-methylpolysiloxane
- High polarity
- Designed for separation of fatty acid methyl esters (FAMEs)
- Excellent resolution for cis- and trans-isomers
- Bonded and cross-linked
- Solvent rinsable
- Replaces HP-23
- Close equivalent to USP Phase G5

Similar Phases: SP-2330, Rtx-2330, 007-23, AT-Silar, BPX-70, SP-2340

DB-23


ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.18	*20*	*0.20*	*40 to 250/260*	*121-2323*		*121-2323LTM*
0.25	15	0.25	40 to 250/260	122-2312		122-2312LTM
	30	0.15	40 to 250/260	122-2331		122-2331LTM
		0.25	40 to 250/260	122-2332	122-2332E	122-2332LTM
	60	0.15	40 to 250/260	122-2361	122-2361E	
		0.25	40 to 250/260	122-2362	122-2362E	
0.32	30	0.25	40 to 250/260	123-2332	123-2332E	123-2332LTM
	60	0.25	40 to 250/260	123-2362		
0.53	15	0.50	40 to 230/240	125-2312		125-2312LTM
	30	0.50	40 to 230/240	125-2332		125-2332LTM

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

DB-200

- (35% Trifluoropropyl)-methylpolysiloxane
- 300/320 °C temperature limit
- Mid polarity – more polar than DB-1701 or DB-17
- Ideal for difficult-to-separate positional isomers
- Unique interactions with compounds containing nitro, halogen and carbonyl groups
- Low ECD bleed
- Unique selectivity
- Close equivalent to USP Phase G6


Similar Phases: Rtx-200

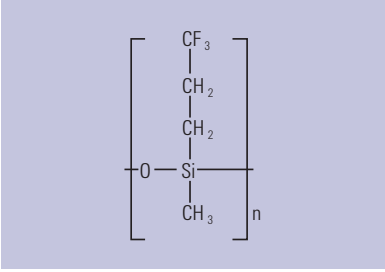

Structure of DB-200

DB-200

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	7890/6890 LTM Module
0.25	30	0.25	30 to 300/320	122-2032	122-2032LTM
		0.50	30 to 300/320	122-2033	122-2033LTM
0.32	30	0.25	30 to 300/320	123-2032	123-2032LTM
		0.50	30 to 300/320	123-2033	123-2033LTM
0.53	30	1.00	30 to 280/300	125-2032	125-2032LTM

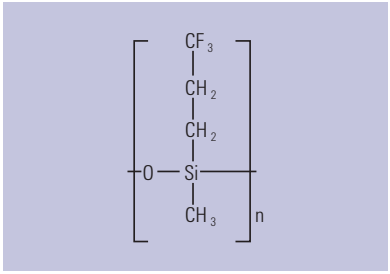

Structure of DB-210

DB-210

- (50%-Trifluoropropyl)-methylpolysiloxane
- High polarity
- Excellent for U.S. EPA Methods 8140 and 609
- Bonded and cross-linked
- Solvent rinsable
- Exact replacement of HP-210
- Close equivalent to USP Phase G6

Similar Phases: SP-2401


DB-210

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.25	15	0.25	45 to 240/260	122-0212		122-0212LTM
	30	0.25	45 to 240/260	122-0232	122-0232E	122-0232LTM
		0.50	45 to 240/260	122-0233		122-0233LTM
0.32	15	0.50	45 to 240/260	123-0213		123-0213LTM
	30	0.25	45 to 240/260	123-0232		123-0232LTM
		0.50	45 to 240/260	123-0233		123-0233LTM
0.53	15	1.00	45 to 220/240	125-0212		125-0212LTM
	30	1.00	45 to 220/240	125-0232		125-0232LTM

DB-225

- (50%-Cyanopropylphenyl)-dimethylpolysiloxane
- Mid/high polarity
- Excellent for separations of cis- and trans-fatty acid methyl esters (FAMEs)
- Bonded and cross-linked
- Solvent rinsable
- Exact replacement of HP-225
- Close equivalent to USP Phase G7

Similar Phases: SP-2330, Rtx-225, BP-225, OV-225, 007-225, AT-225

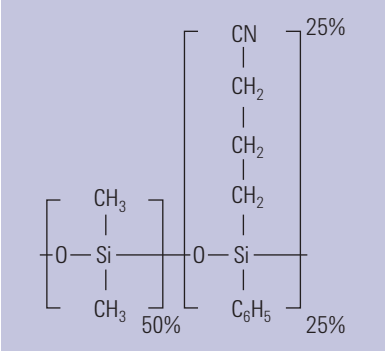

Structure of DB-225


DB-225

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.10	20	0.10	40 to 220/240	127-2222		127-2222LTM
0.18	*20*	*0.20*	*40 to 220/240*	*121-2223*		*121-2223LTM*
0.25	15	0.25	40 to 220/240	122-2212		122-2212LTM
	30	0.15	40 to 220/240	122-2231		122-2231LTM
		0.25	40 to 220/240	122-2232		122-2232LTM
0.32	30	0.25	40 to 220/240	123-2232	123-2232E	123-2232LTM
0.53	15	1.00	40 to 200/220	125-2212		125-2212LTM
	30	0.50	40 to 200/220	125-2237		125-2237LTM
		1.00	40 to 200/220	125-2232		125-2232LTM

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

TIPS & TOOLS

Need assistance selecting a column for your method? Contact our chromatography technical specialists at **www.agilent.com/chem/TechRep**

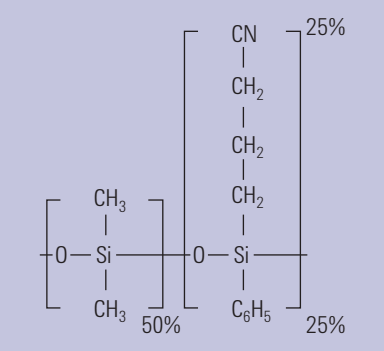

Structure of CP-Sil 43 CB

CP-Sil 43 CB

- 25% cyanopropyl/25% phenyl/50% dimethylpolysiloxane phase
- Mid polarity
- Separates aromatic from aliphatic hydrocarbons with selectivity equivalent to OV-255
- Bonded and cross-linked
- Solvent rinsable
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation

Similar Phases: SP-2330, Rtx-225, BP-225, OV-225, 007-225, AT-225


CP-Sil 43 CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	25	0.20	45 to 200/225	CP7715	CP7715I5
	50	0.20	45 to 200/225	CP7725	CP7725I5
0.32	10	0.20	45 to 200/225	CP7735	
	25	0.20	45 to 200/225	CP7745	

DB-1301

- (6%-Cyanopropyl-phenyl) methylpolysiloxane
- Equivalent to USP Phase G43
- Low/mid polarity
- Bonded and cross-linked
- Exact replacement of HP-1301 and HP-1701
- Solvent rinsable

Similar Phases: Rtx-1301, PE-1301

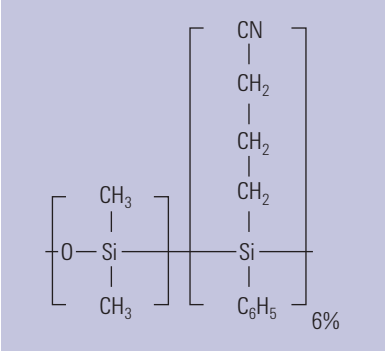


Structure of DB-1301

DB-1301

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.18	*10*	*0.40*	*-20 to 280/300*	*121-1313*		*121-1313LTM*
0.25	30	0.25	-20 to 280/300	122-1332	122-1332E	122-1332LTM
		1.00	-20 to 280/300	122-1333		122-1333LTM
	60	0.25	-20 to 280/300	122-1362		
		1.00	-20 to 280/300	122-1363	122-1363E	
0.32	30	0.25	-20 to 280/300	123-1332		123-1332LTM
		1.00	-20 to 280/300	123-1333		123-1333LTM
	60	1.00	-20 to 280/300	123-1363	123-1363E	
0.53	15	1.00	-20 to 260/280	125-1312		125-1312LTM
	30	1.00	-20 to 260/280	125-1332		125-1332LTM
		1.50	-20 to 260/280	125-1333		125-1333LTM

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

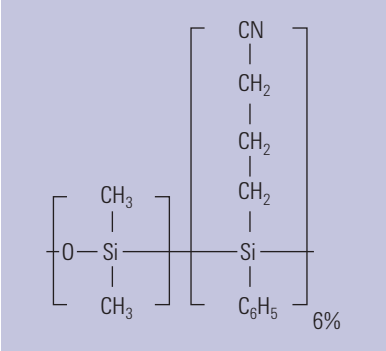

Structure of CP-1301

CP-1301

- 6% cyanopropyl-phenyl/94% dimethylpolysiloxane
- Mid polarity
- Ideal for analysis of herbicides, pesticides and many pharmaceutical products
- High column-to-column reproducibility
- Good inertness for better quality of data, even with thick films
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation
- Bonded and cross-linked
- Solvent rinsable

Similar Phases: Rtx-1301, PE-1301


CP-1301

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	30	1.00	-25 to 265/280	CP8604
	60	0.25	-25 to 280/280	CP8602
		1.00	-25 to 265/280	CP8605
0.32	30	0.25	-25 to 280/280	CP8607
		1.00	-25 to 265/280	CP8610
	60	0.25	-25 to 280/280	CP8608
		1.00	-25 to 265/280	CP8611
0.53	30	1.00	-25 to 265/280	CP8613

DB-1701

- (14% Cyanopropyl-phenyl)-methylpolysiloxane
- Low/mid polarity
- Bonded and cross-linked
- Exact replacement of HP-1301 and HP-1701
- Solvent rinsable

Similar Phases: SPB-1701, Rtx-1701, BP-10, OV-1701, 007-1701, ZB-1701

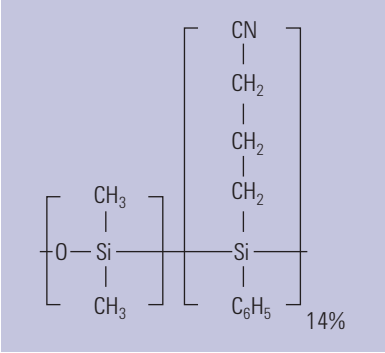

Structure of DB-1701


DB-1701

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.10	20	0.10	-20 to 280/300	127-0722		127-0722LTM
		0.40	-20 to 280/300	127-0723		127-0723LTM
0.18	*10*	*0.40*	*-20 to 280/300*	*121-0713*		*121-0713LTM*
	20	*0.18*	*-20 to 280/300*	*121-0722*		*121-0722LTM*
0.25	15	0.25	-20 to 280/300	122-0712		122-0712LTM
		1.00	-20 to 280/300	122-0713		122-0713LTM
	30	0.15	-20 to 280/300	122-0731		122-0731LTM
		0.25	-20 to 280/300	122-0732	122-0732E	122-0732LTM
		1.00	-20 to 280/300	122-0733	122-0733E	122-0733LTM
	60	0.15	-20 to 280/300	122-0761		
		0.25	-20 to 280/300	122-0762		
		0.50	-20 to 280/300	122-0766		
		1.00	-20 to 280/300	122-0763	122-0763E	
0.32	15	0.25	-20 to 280/300	123-0712		123-0712LTM
		1.00	-20 to 280/300	123-0713		123-0713LTM
	30	0.15	-20 to 280/300	123-0731		123-0731LTM
		0.25	-20 to 280/300	123-0732	123-0732E	123-0732LTM
		1.00	-20 to 280/300	123-0733	123-0733E	123-0733LTM
	50	1.00	-20 to 280/300	123-0753		
	60	0.25	-20 to 280/300	123-0762		
		1.00	-20 to 280/300	123-0763	123-0763E	
0.53	15	1.00	-20 to 260/280	125-0712	125-0712E	125-0712LTM
	30	0.25	-20 to 260/280	125-0731		125-0731LTM
		0.50	-20 to 260/280	125-0737		125-0737LTM
		1.00	-20 to 260/280	125-0732	125-0732E	125-0732LTM
		1.50	-20 to 260/280	125-0733		125-0733LTM
	60	1.00	-20 to 260/280	125-0762	125-0762E	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

TIPS & TOOLS

Agilent also offers DB-624 columns for the analysis of volatile priority pollutants and residual solvents.

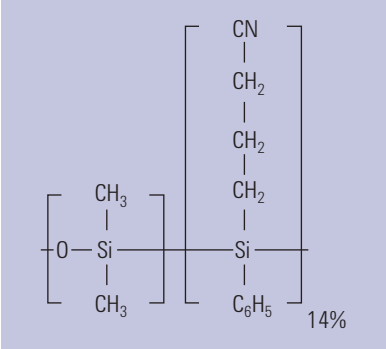

Structure of CP-Sil 19 CB

CP-Sil 19 CB

- 14% cyanopropyl-phenyl/86% dimethylpolysiloxane
- Mid polarity
- Ideal for many environmental, food and beverage, and pharmaceutical applications
- Useful as confirmation column
- Bonded and cross-linked
- Solvent rinsable
- Broad range of configurations available
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation

Similar Phases: SPB-1701, Rtx-1701, BP-10, OV-1701, 007-1701, ZB-1701

CP-Sil 19 CB


ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.10	10	0.20	-25 to 275/300	CP7331	
0.15	*25*	*0.50*	*-25 to 275/300*	*CP7340*	
0.20	25	0.20	-25 to 275/300	CP7360	
0.25	10	0.20	-25 to 275/300	CP7702	
	15	0.15	-25 to 275/300	CP8502	
		0.25	-25 to 275/300	CP8512	CP8512I5
	25	0.20	-25 to 275/300	CP7712	
		0.40	-25 to 275/300	CP7809	
		1.20	-25 to 275/300	CP7672	
	30	0.25	-25 to 275/300	CP8712	CP8712I5
		1.00	-25 to 275/300	CP8562	CP8562I5
	50	0.20	-25 to 275/300	CP7722	
		0.40	-25 to 275/300	CP7819	CP7819I5
	60	0.15	-25 to 275/300	CP8592	CP8592I5
		0.25	-25 to 275/300	CP8722	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

(Continued)

CP-Sil 19 CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.32	10	0.20	-25 to 275/300	CP7732	
	15	0.25	-25 to 275/300	CP8542	CP8542I5
	25	0.20	-25 to 275/300	CP7742	
		0.40	-25 to 275/300	CP7829	
		1.20	-25 to 275/300	CP7762	
	30	0.25	-25 to 275/300	CP8842	
		1.00	-25 to 275/300	CP8762	
	50	0.20	-25 to 275/300	CP7752	
		0.40	-25 to 275/300	CP7839	
		1.20	-25 to 275/300	CP7772	
	60	0.15	-25 to 275/300	CP8662	
		0.25	-25 to 275/300	CP8852	
		1.00	-25 to 275/300	CP8772	CP8772I5
0.53	10	2.00	-25 to 275/300	CP7647	
	15	0.50	-25 to 275/300	CP8663	
	25	1.00	-25 to 275/300	CP7637	
		2.00	-25 to 275/300	CP7657	
	30	1.00	-25 to 275/300	CP8737	
	50	2.00	-25 to 275/300	CP7667	
		1.00	-25 to 275/300	CP7697	

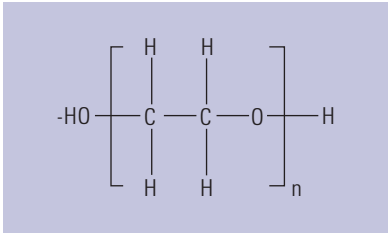

Structure of Polyethylene Glycol (PEG)
This structure is applicable for all
WAX and FFAP phases.

Polyethylene Glycol (PEG) Columns

Agilent offers a full range of PEG columns. Even though each phase is based on the polyethylene glycol polymer, strict control of the cross-linking and deactivation processes result in a variety of unique phase characteristics to meet your varying analysis needs.

DB-WAX and DB-WaxFF

- Polyethylene glycol (PEG)
- Equivalent to USP Phase G16
- High polarity
- Lower temperature limit of 20 °C is the lowest of any bonded PEG phase; improves resolution of low boiling point analytes
- Column-to-column reproducibility
- Bonded and cross-linked
- Exact replacement of HP-WAX
- Solvent rinsable
- DB-WaxFF is a highly reproducible, specially tested microbore DB-Wax for fragrance analysis

Similar Phases: SUPELCOWAX 10, SUPEROX II, CB-WAX, Stabilwax, BP-20, 007-CW, Carbowax, Rtx-WAX, ZB-WAX, ZB-WAX plus

DB-WAX and DB-WaxFF

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module	5975T LTM Toroid
DB-WAX							
0.05	10	0.05	20 to 250/260	126-7012		126-7012LTM	
		0.10	20 to 240/250	126-7013		126-7013LTM	222-7013LTM
0.10	10	0.10	20 to 250/260	127-7012	127-7012E	127-7012LTM	
		0.20	20 to 240/250	127-7013		127-7013LTM	
	20	0.10	20 to 250/260	127-7022		127-7022LTM	
		0.20	20 to 240/250	127-7023	127-7023E	127-7023LTM	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

(Continued)

DB-WAX and DB-WaxFF

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module	5975T LTM Toroid
DB-WAX							
0.18	*10*	*0.18*	*20 to 250/260*	*121-7012*		*121-7012LTM*	
	20	*0.18*	*20 to 250/260*	*121-7022*	*121-7022E*	*121-7022LTM*	
		0.30	*20 to 240/250*	*121-7023*	*121-7023E*	*121-7023LTM*	
	40	*0.18*	*20 to 250/260*	*121-7042*	*121-7042E*		
		0.30	*20 to 240/250*	*121-7043*			
0.20	25	0.20	20 to 250/260	128-7022		128-7022LTM	
	30	0.20	20 to 250/260	128-7032		128-7032LTM	
	50	0.20	20 to 250/260	128-7052			
0.25	15	0.25	20 to 250/260	122-7012	122-7012E	122-7012LTM	
		0.50	20 to 240/250	122-7013		122-7013LTM	
	30	0.15	20 to 250/260	122-7031		122-7031LTM	
		0.25	20 to 250/260	122-7032	122-7032E	122-7032LTM	
		0.50	20 to 240/250	122-7033	122-7033E	122-7033LTM	222-7033LTM
	60	0.15	20 to 250/260	122-7061			
		0.25	20 to 250/260	122-7062	122-7062E		
		0.50	20 to 240/250	122-7063	122-7063E		
0.32	15	0.25	20 to 250/260	123-7012		123-7012LTM	
		0.50	20 to 240/250	123-7013		123-7013LTM	
	30	0.15	20 to 250/260	123-7031		123-7031LTM	
		0.25	20 to 250/260	123-7032	123-7032E	123-7032LTM	
		0.50	20 to 240/250	123-7033	123-7033E	123-7033LTM	
	60	0.25	20 to 250/260	123-7062			
		0.50	20 to 240/250	123-7063	123-7063E		
0.45	30	0.85	20 to 230/240	124-7032		124-7032LTM	
0.53	15	0.50	20 to 230/240	125-7017		125-7017LTM	
		1.00	20 to 230/240	125-7012	125-7012E	125-7012LTM	
	30	0.25	20 to 230/240	125-7031		125-7031LTM	
		0.50	20 to 230/240	125-7037		125-7037LTM	
		1.00	20 to 230/240	125-7032	125-7032E	125-7032LTM	
	60	1.00	20 to 230/240	125-7062	125-7062E		
DB-WaxFF							
0.10	20	0.20	20 to 240/250	127-7023FF			

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

DB-WAXetr

- Polyethylene glycol (PEG)
- Extended Temperature Range (etr)
- High polarity
- Excellent column-to-column repeatability
- Bonded and cross-linked
- Solvent rinsable
- Equivalent to USP Phase G16

Similar Phases: SUPELCOWAX 10, SUPEROX II, CB-WAX, Stabilwax, BP-20, 007-CW, Carbowax, Rtx-WAX, ZB-WAX, ZB-WAX plus

DB-WAXetr

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.20	25	0.40	30 to 250/260	128-7323		128-7323LTM
0.25	30	0.25	30 to 260/280	122-7332	122-7332E	122-7332LTM
		0.50	30 to 250/260	122-7333		122-7333LTM
	60	0.25	30 to 260/280	122-7362		
		0.50	30 to 250/260	122-7363		
0.32	15	0.25	30 to 260/280	123-7312		123-7312LTM
		1.00	30 to 250/260	123-7314		123-7314LTM
	30	0.25	30 to 260/280	123-7332		123-7332LTM
		0.50	30 to 250/260	123-7333		123-7333LTM
		1.00	30 to 250/260	123-7334		123-7334LTM
	50	1.00	30 to 250/260	123-7354	123-7354E	
	60	0.25	30 to 260/280	123-7362		
		0.50	30 to 250/260	123-7363		
		1.00	30 to 250/260	123-7364		
0.53	15	1.00	30 to 240/260	125-7312		125-7312LTM
		2.00	50 to 230/250	125-7314		125-7314LTM
	30	1.00	30 to 240/260	125-7332	125-7332E	125-7332LTM
		1.50	30 to 230/240	125-7333		125-7333LTM
		2.00	50 to 230/250	125-7334	125-7334E	125-7334LTM
	60	1.00	30 to 240/260	125-7362		

HP-INNOWax

- Polyethylene glycol (PEG)
- High polarity
- Highest upper temperature limits of the bonded PEG phases
- Column-to-column repeatability
- Bonded and cross-linked
- Solvent rinsable
- Close equivalent to USP Phase G16

Similar Phases: SUPELCOWAX 10, SUPEROX II, CB-WAX, Stabilwax, BP-20, 007-CW, Carbowax, ZB-WAX, ZB-WAX+

HP-INNOWax

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module	5975T LTM Toroid
0.18	*20*	*0.18*	*40 to 260/270*	*19091N-577*	*19091N-577E*	*19091N-577LTM*	*29091N-577LTM*
0.20	25	0.20	40 to 260/270	19091N-102		19091N-102LTM	
		0.40	40 to 260/270	19091N-202		19091N-202LTM	
	50	0.20	40 to 260/270	19091N-105	19091N-105E		
		0.40	40 to 260/270	19091N-205	19091N-205E		
0.25	4	0.25	40 to 260/270	19091N-130		19091N-130LTM	
	5	0.10	40 to 260/270	19091N-330			
		0.15	40 to 260/270	19091N-030		19091N-030LTM	
	15	0.10	40 to 260/270	19091N-331			
		0.25	40 to 260/270	19091N-131	19091N-131E	19091N-131LTM	
		0.50	40 to 260/270	19091N-231		19091N-231LTM	
	30	0.15	40 to 260/270	19091N-033		19091N-033LTM	
		0.25	40 to 260/270	19091N-133	19091N-133E	19091N-133LTM	29091N-133LTM
		0.50	40 to 260/270	19091N-233	19091N-233E	19091N-233LTM	
	60	0.15	40 to 260/270	19091N-036			
		0.25	40 to 260/270	19091N-136	19091N-136E		
		0.50	40 to 260/270	19091N-236			
0.32	15	0.25	40 to 260/270	19091N-111		19091N-111LTM	
	30	0.15	40 to 260/270	19091N-013		19091N-013LTM	
		0.25	40 to 260/270	19091N-113	19091N-113E	19091N-113LTM	
		0.50	40 to 260/270	19091N-213	19091N-213E	19091N-213LTM	
	60	0.25	40 to 260/270	19091N-116			
		0.50	40 to 260/270	19091N-216	19091N-216E		
0.53	15	1.00	40 to 240/250	19095N-121	19095N-121E	19095N-121LTM	
	30	1.00	40 to 240/250	19095N-123	19095N-123E	19095N-123LTM	
	60	1.00	40 to 240/250	19095N-126			

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers



CP-Wax 52 CB

- Polyethylene glycol phase
- High polarity
- Wider temperature range than non-bonded polyethylene glycols
- Bonded and cross-linked
- Solvent rinsable
- High resolution of low boiling point analytes
- High polarity provides separations for a broad range of applications
- Excellent reproducibility and temperature stability for a variety of EPA and ASTM methods
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation

Note: We recommend the UltiMetal column when working in rugged environments with process or portable instruments.

Similar Phases: SUPELCOWAX 10, SUPEROX II, CB-WAX, Stabilwax, BP-20, 007-CW, Carbowax, HP-INNOWax, Rtx-WAX, ZB-WAX, ZB-WAX+

CP-Wax 52 CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.10	10	0.10	20 to 250/265	CP7334	CP7334I5
		0.20	20 to 250/265	CP7335	
0.15	*15*	*0.15*	*20 to 250/265*	*CP7791*	*CP7791I5*
	25	*0.25*	*20 to 250/265*	*CP7792*	*CP7792I5*
0.20	25	0.20	20 to 250/265	CP7765	
	30	0.20	20 to 250/265	CP7775	
	50	0.20	20 to 250/265	CP7785	
0.25	10	0.20	20 to 250/265	CP7703	
	15	0.25	20 to 250/265	CP8513	
	25	0.20	20 to 250/265	CP7713	CP7713I5
		1.20	20 to 250/265	CP7673	CP7673I5
	30	0.15	20 to 250/265	CP8745	
		0.25	20 to 250/265	CP8713	CP8713I5
		0.50	20 to 250/265	CP8746	CP8746I5
	50	0.20	20 to 250/265	CP7723	CP7723I5
	60	0.25	20 to 250/265	CP8723	CP8723I5
		0.50	20 to 250/265	CP8748	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

(Continued)

CP-Wax 52 CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.32	10	0.20	20 to 250/265	CP7733	CP7733I5
		1.00	20 to 250/265	CP7628	
	15	0.15	20 to 250/265	CP8533	
		0.25	20 to 250/265	CP8543	
		0.50	20 to 250/265	CP8553	
	25	0.20	20 to 250/265	CP7743	
		0.40	20 to 250/265	CP7879	
		1.20	20 to 250/265	CP7763	CP7763I5
	30	0.25	20 to 250/265	CP8843	CP8843I5
		0.50	20 to 250/265	CP8763	CP8763I5
	50	0.20	20 to 250/265	CP7753	CP7753I5
		0.40	20 to 250/265	CP7889	
		1.20	20 to 250/265	CP7773	CP7773I5
	60	0.25	20 to 250/265	CP8853	
		0.50	20 to 250/265	CP8773	
		1.20	20 to 250/265	CP8073	CP8073I5
0.53	10	2.00	20 to 250/265	CP7648	
	15	1.00	20 to 250/265	CP8718	
	25	1.00	20 to 250/265	CP7638	
		2.00	20 to 250/265	CP7658	CP7658I5
	30	1.00	20 to 250/265	CP8738	CP8738I5
	50	1.00	20 to 250/265	CP7698	CP7698I5
		2.00	20 to 250/265	CP7668	
	60	1.00	20 to 250/265	CP8798	
	100	2.00	20 to 250/265	CP7678	

CP-Wax 52 CB UltiMetal

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	Part No.
0.53	10	0.50	20 to 250/275	CP7128
		1.00	20 to 250/275	CP7148
		2.00	20 to 250/275	CP7177
	25	0.50	20 to 250/275	CP7138
		1.00	20 to 250/275	CP7158
		2.00	20 to 250/275	CP7178
	50	0.50	20 to 250/275	CP7198
		1.00	20 to 250/275	CP7168
		2.00	20 to 250/275	CP7179

DB-FFAP

- Nitroterephthalic acid modified polyethylene glycol
- High polarity
- Temperature range from 40 °C to 250 °C
- Designed for the analysis of volatile fatty acids and phenols
- Replaces OV-351
- Bonded and cross-linked
- Solvent rinsable
- Close equivalent to USP Phase G35

Note: We do not recommend the use of water or methanol to rinse DB-FFAP GC columns.

Similar Phases: Stabilwax-DA, Nukol, 007-FFAP, BP21, AT-1000, OV-351

DB-FFAP

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module	5975T LTM Toroid
0.10	10	0.10	40 to 250	127-3212		127-3212LTM	
	15	0.10	40 to 250	127-32H2		127-32H2LTM	
0.25	15	0.25	40 to 250	122-3212		122-3212LTM	222-3212LTM
	30	0.25	40 to 250	122-3232	122-3232E	122-3232LTM	222-3232LTM
		0.50	40 to 250	122-3233		122-3233LTM	
	60	0.25	40 to 250	122-3262	122-3262E		
		0.50	40 to 250	122-3263			
0.32	15	0.25	40 to 250	123-3212		123-3212LTM	
	25	0.50	40 to 250	123-3223		123-3223LTM	
	30	0.25	40 to 250	123-3232	123-3232E	123-3232LTM	
		0.50	40 to 250	123-3233		123-3233LTM	
		1.00	40 to 250	123-3234		123-3234LTM	
	50	0.50	40 to 250	123-3253			
	60	0.25	40 to 250	123-3262			
		0.50	40 to 250	123-3263			
		1.00	40 to 250	123-3264			
0.45	30	0.85	40 to 250	124-3232		124-3232LTM	
0.53	10	1.00	40 to 250	125-32H2		125-32H2LTM	
	15	0.50	40 to 250	125-3217		125-3217LTM	
		1.00	40 to 250	125-3212		125-3212LTM	
	30	0.25	40 to 250	125-3231		125-3231LTM	
		0.50	40 to 250	125-3237		125-3237LTM	
		1.00	40 to 250	125-3232	125-3232E	125-3232LTM	
		1.50	40 to 250	125-3233		125-3233LTM	
	60	1.00	40 to 250	125-3262			

HP-FFAP

- Nitroterephthalic acid modified polyethylene glycol
- High polarity
- Temperature range from 60 °C to 240/250 °C (230/240 °C for 0.53 mm)
- Designed for the analysis of volatile fatty acids and phenols
- Replaces OV-351
- Bonded and cross-linked
- Solvent rinsable
- Close equivalent to USP Phase G35

Note: We do not recommend the use of water or methanol to rinse HP-FFAP GC columns.

Similar Phases: Stabilwax-DA, Nukol, 007-FFAP, BP21, AT-1000, OV-351

HP-FFAP

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.20	25	0.30	60 to 240/250	19091F-102	19091F-102E	19091F-102LTM
	50	0.30	60 to 240/250	19091F-105	19091F-105E	
0.25	30	0.25	60 to 240/250	19091F-433	19091F-433E	19091F-433LTM
0.32	25	0.50	60 to 240/250	19091F-112	19091F-112E	19091F-112LTM
	30	0.25	60 to 240/250	19091F-413		19091F-413LTM
	50	0.50	60 to 240/250	19091F-115	19091F-115E	
0.53	10	1.00	60 to 240	19095F-121		19095F-121LTM
	15	1.00	60 to 240	19095F-120	19095F-120E	19095F-120LTM
	30	1.00	60 to 240	19095F-123	19095F-123E	19095F-123LTM

TIPS & TOOLS

Agilent also offers CAM columns for amine analysis.

CP-Wax 58 FFAP CB

- Nitroterephthalic acid-modified polyethylene glycol phase
- High polarity
- Ideal for analysis of acidic compounds, such as phenols, underivatized and derivatized free fatty acids
- Highest polarity bonded wax column for analyzing polar compounds
- Chemically-bonded
- Solvent rinsable
- High inertness provides excellent peak shape
- Supplied with an EZ-GRIP to simplify column installation, coupling and operation

Similar Phases: SUPELCOWAX 10, SUPEROX II, CB-WAX, Stabilwax, BP-20, 007-CW, Carbowax, Rtx-WAX, ZB-WAX

CP-Wax 58 FFAP CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.20	25	0.30	20 to 250/275	CP7787	CP7787I5
	50	0.30	20 to 250/275	CP7797	
0.25	25	0.20	20 to 250/275	CP7717	CP7717I5
	50	0.20	20 to 250/275	CP7727	
0.32	25	0.20	20 to 250/275	CP7747	CP7747I5
		1.20	20 to 250/275	CP7767	
	50	0.20	20 to 250/275	CP7757	
		0.50	20 to 250/275	CP7778	
		1.20	20 to 250/275	CP7777	
0.53	15	0.50	20 to 250/275	CP7665	
	25	1.00	20 to 250/275	CP7614	CP7614I5
		2.00	20 to 250/275	CP7654	
	50	1.00	20 to 250/275	CP7624	
		2.00	20 to 250/275	CP7664	

TIPS & TOOLS

View the latest GC column focused applications, products and educational resources at **www.agilent.com/chem/myGCcolumns**

Carbowax 20M and HP-20M

- Polyethylene glycol, MW 20,000
- Equivalent to USP Phase G16

Similar Phases: Rt-CW20M F&F

Because the Carbowax 20M and the HP-20M are not bonded or cross-linked, we do not recommend solvent rinsing. DB-WAX is the recommended bonded alternate for the HP-20M.

Carbowax 20M

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	7890/6890 LTM Module
0.25	30	0.25	60 to 220/240	112-2032	112-2032LTM
0.32	30	0.25	60 to 220/240	113-2032	113-2032LTM
	60	0.25	60 to 220/240	113-2062	

HP-20M

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.20	25	0.10	60 to 220	19091W-102		19091W-102LTM
	50	0.10	60 to 220	19091W-105		
0.32	25	0.30	60 to 220	19091W-012	19091W-012E	19091W-012LTM
	50	0.30	60 to 220	19091W-015	19091W-015E	
0.53	10	1.33	60 to 220	19095W-121		19095W-121LTM
	30	1.33	60 to 220	19095W-123		19095W-123LTM



Specialty Columns

Agilent chemists have developed many columns with unique characteristics designed to solve the most difficult separation problems of a given method. As a result, we offer a comprehensive line of specialty or "select" columns for a variety of applications to enhance the standard phase portfolio. With columns for volatiles, pesticides, petrochemicals and more – Agilent exceeds standard QA/QC procedures for the manufacturing and testing of all of our specialty columns to ensure they meet the stringent demands for their application. These columns offer reliable, accurate results with the shortest run times possible on complex sample lists and matrices.

High Temperature Columns

DB-1ht

- 100% Dimethylpolysiloxane
- Non-polar
- Specially processed for extended temperature limit of 400 °C
- High temperature, polyimide-coated, fused silica tubing
- Excellent peak shape and faster elution times for high boilers
- Bonded and cross-linked
- Solvent rinsable

Similar Phases: Rxi-1HT, Stx-1ht, ZB-1ht

DB-1ht

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module	5975T LTM Toroid
0.25	15	0.10	-60 to 400	122-1111	122-1111E		222-1111LTM
	30	0.10	-60 to 400	122-1131			222-1131LTM
0.32	15	0.10	-60 to 400	123-1111		123-1111LTM	
	30	0.10	-60 to 400	123-1131	123-1131E	123-1131LTM	
0.53	30	0.17	-60 to 400	125-1131			

DB-5ht



- (5%-Phenyl)-methylpolysiloxane
- Non-polar
- Specially processed for extended temperature limit of 400 °C
- High temperature, polyimide-coated, fused silica tubing
- Excellent peak shape and faster elution times for high boilers
- Bonded and cross-linked
- Solvent rinsable

Similar Phases: HT5, Stx-5ht, ZB-5ht

DB-5ht

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module	5975T LTM Toroid
0.25	15	0.10	-60 to 400	122-5711	122-5711E	122-5711LTM	222-5711LTM
	30	0.10	-60 to 400	122-5731		122-5731LTM	222-5731LTM
0.32	10	0.10	-60 to 400	123-5701		123-5701LTM	
	15	0.10	-60 to 400	123-5711	123-5711E		
	30	0.10	-60 to 400	123-5731	123-5731E	123-5731LTM	

DB-17ht

- (50%-Phenyl)-methylpolysiloxane
- Mid-polarity
- Extended upper temperature limit of 365 °C
- High temperature, polyimide-coated, fused silica tubing
- Excellent peak shape and faster elution times for high boilers
- Improved resolution for triglycerides
- Ideal for confirmational analyses
- Bonded and cross-linked
- Solvent rinsable

Similar Phases: Rtx-65TG, BPX50

DB-17ht

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.25	5	0.15	40 to 340/365	122-1801		122-1801LTM
	15	0.15	40 to 340/365	122-1811		
	30	0.15	40 to 340/365	122-1831		122-1831LTM
0.32	15	0.15	40 to 340/365	123-1811		
	30	0.15	40 to 340/365	123-1831	123-1831E	
	60	0.15	40 to 340/365	123-1861		



TIPS & TOOLS

Learn more about the Agilent 7890A GC System at **www.agilent.com/chem/7890A**

VF-5ht and VF-5ht UltiMetal

- Enhanced selectivity improves column longevity and reduces downtime
- Superior detector performance provides improved detection limits
- For analyses of high boiling compounds by exhibiting ultra low bleed at high temperatures
- Optimized sensitivity and accuracy for analysis of high molecular weight compounds
- Identical selectivity as VF-5ms (bleed spec of 30 m x 0.25 mm column is < 5 pA at 400 °C)
- UltiMetal technology renders the stainless steel inert and enhances bonding of the stationary phase for improved column lifetime and excellent peak shape

Similar Phases: ZB-5ht, Rxi-5ht

VF-5ht

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	15	0.10	-60 to 400/400	CP9045
	30	0.10	-60 to 400/400	CP9046
0.32	10	0.10	-60 to 400/400	CP9044
	15	0.10	-60 to 400/400	CP9047
	30	0.10	-60 to 400/400	CP9048

Similar Phases: ZB-5ht, Rxi-5ht

VF-5ht UltiMetal

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	15	0.10	-60 to 430/450	CP9090	
		0.10	-60 to 430/450	CP9091*	
	30	0.10	-60 to 430/450	CP9092	CP9092I5
		0.10	-60 to 430/450	CP9093*	
0.32	15	0.10	-60 to 430/450	CP9094	CP9094I5
		0.10	-60 to 430/450	CP9095*	
	30	0.10	-60 to 430/450	CP9096	
		0.10	-60 to 430/450	CP9097*	

*These configurations include a 2 m x 0.53 mm id UltiMetal retention gap which are pre-connected to the VF-5ht UltiMetal column with a high-temperature column connector.

Petroleum Columns

Petroleum applications vary greatly in character. From noble gases to simulated distillation, Agilent offers a broad range of columns designed to meet the needs of the petroleum/petrochemical chromatographer. Refer to the PLOT column section for columns for the analysis of light gases.

Lowox

- Unique selectivity for a wide range of oxygenates
- Minimal particle loss preserves detector performance
- Industry proven for process and portable GC applications (ASTM D 7059)
- Analyze trace level oxygenate impurities in gas and liquid hydrocarbon streams
- High polarity
- Ideal for monitoring catalyst contamination by oxygenates

Lowox

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.53	10	10.00	0 to 350/350	CP8587	CP8587I5

GS-OxyPLOT

- Accurate analysis of ppm/ppb level oxygenates in C_1 to C_{10} hydrocarbons
- Strong selectivity for a wide range of oxygenates (ethers, alcohols, aldehydes, and ketones) in complex matrices such as gaseous hydrocarbons, motor fuels, and crude oil
- Suitable for ASTM methods for oxygenates
- Very high column stability (upper temperature limit of 350 °C) with no column bleed
- Stable phase coating virtually eliminates particle generation and detector spiking
- Excellent for low concentration, quantitative GC analysis
- Ideal for selective heart-cutting applications

GS-OxyPLOT

ID (mm)	Length (m)	Temp Limits (°C)	7 in Cage	5 in Cage
0.53	10	350	115-4912	115-4912E

CP-Sil 5 CB for Formaldehyde

- Optimized for analysis of formaldehyde, water and methanol
- Trace analysis of sulfur compounds possible
- Partial permanent gas analysis possible (especially in switching systems)
- Non-polar phase provides accurate separations based on volatility
- High inertness, elutes sulfur components without absorption for high quality data and low detection limits
- Highest efficiency for this apolar column with the thickest film

CP-Sil 5 CB for Formaldehyde


ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.32	60	8.00	-60 to 300/325	CP7475	CP7475I5

HP-PONA

- 100% Dimethylpolysiloxane
- Configured for the analysis of petroleum process products
- Tested to ensure the resolution of m-xylene from p-xylene and of cyclopentane from 2,3-dimethylbutane
- PONA, PIANO
- High resolution
- Bonded and cross-linked
- Solvent rinsable

Note: 100 psi regulator required to reach optimum carrier gas velocity


Similar Phases: Petrocol DH, SPB-1, 007-1, Rtx-1, MXT-1, Rtx-1PONA, Rtx-DHA

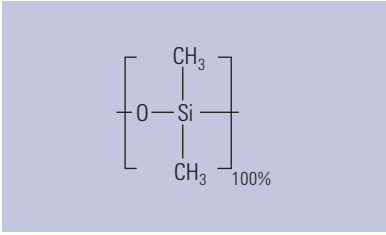

Structure of HP-PONA

HP-PONA

Description	ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
HP-PONA	0.20	50	0.50	-60 to 325/350	19091S-001	19091S-001E
HP-1	0.20	50	0.50	-60 to 325/350	19091Z-205	19091Z-205E
HP-1	0.25	100	0.50	-60 to 325/350	19091Z-530	19091Z-530E

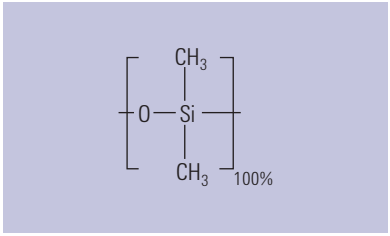

Structure of CP-Sil PONA CB

CP-Sil PONA CB

- High resolution analysis of paraffins, olefins, napthalenes and aromatics in complex hydrocarbon mixtures
- Engineered for hydrocarbon analysis according to ASTM (DHA method)
- Inert to polar compounds for highly accurate data
- Excellent column-to-column reproducibility

Similar Phases: Petrocol DH, SPB-1, 007-1, Rtx-1, MXT-1

CP-Sil PONA CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.21	50	0.50	250/275	CP7531	CP7531I5
0.25	100	0.50	250/275	CP7530	CP7530I5
0.25	150	1.00	250/275	CP7945	


CP-Sil PONA for ASTM D 5134

- Optimized PONA analysis for ASTM D 5134
- Exact dimensions as specified in the ASTM method for full compliance
- Inert to polar additives

CP-Sil PONA for ASTM D 5134

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.21	50	0.50	250/275	CP7531

DB-Petro



Structure of DB-Petro

- 100% Dimethylpolysiloxane
- Configured for the analysis of petroleum process products
- PONA, PIANO
- High resolution
- Bonded and cross-linked
- Solvent rinsable

Note: 100 psi regulator required to reach optimum carrier gas velocity

Similar Phases: Petrocol DH, SPB-1, 007-1, Rtx-1, MXT-1



DB-Petro

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.20	50	0.50	-60 to 325/350	128-1056	
0.25	100	0.50	-60 to 325/350	122-10A6	122-10A6E

HP-1 Aluminum Clad

- 100% Dimethylpolysiloxane
- Aluminum clad fused silica tubing
- For high temperature simulated distillation
- Bonded and cross-linked
- Solvent rinsable

Similar Phases: MXT-1

HP-1 Aluminum Clad

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.53	5	0.09	0 to 350/450	19095S-205
	10	0.09	0 to 350/450	19095S-200

DB-2887

- 100% Dimethylpolysiloxane
- Specifically designed for simulated distillation using ASTM Method D 2887
- Rapid conditioning, fast run time and low bleed when compared to packed columns
- Bonded and cross-linked
- Solvent rinsable

Similar Phases: Petrocol EX2887, MXT-2887, MXT-1, Rtx-2887

DB-2887

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.53	10	3.00	-60 to 350	125-2814	125-2814E	125-2814LTM



DB-HT SimDis

- 100% Dimethylpolysiloxane
- "Boiling point" phase for high temperature simulated distillation
- Durable stainless steel tubing
- 430 °C upper temperature limit
- Distillation range of C_6 to C_{110+}
- Low bleed, even at 430 °C
- Bonded and cross-linked
- Solvent rinsable

Similar Phases: Petrocol EX2887, MXT-2887, Rtx-2887, AC Controls High Temp Sim Dist, AT-2887, ZB-1XT SimDist

DB-HT SimDis


ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.53	5	0.10	-60 to 400/430	145-1009
		0.15	-60 to 400/430	145-1001

CP-SimDist

- For simulated distillation analysis up to C_{100}
- High temperature non-polar stationary phase
- Low bleed improves quantitation
- High temperature polyimide coating extends lifetime

CP-SimDist Fused Silica columns are guaranteed for simulated distillation up to C_{100}. These columns are low bleed, typically only 4-5 pA at 400 °C. The high temperature stationary phase and polyimide coating extend column lifetime.

Similar Phases: Petrocol EX2887, MXT-2887, Rtx-2887, AC Controls High Temp Sim Dist, AT-2887, ZB-1XT SimDist

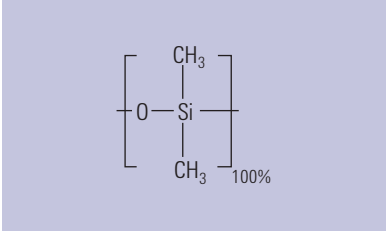

Structure of CP-SimDist

CP-SimDist

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.32	10	0.10	375/400	CP7521	
0.53	5	0.17	375/400	CP7522	CP7522I5
	10	0.10	375/400	CP7541	

TIPS & TOOLS

For optimum performance, ferrules should be replaced every time the column is replaced and during column maintenance.
See pages 33-34



CP-SimDist UltiMetal

- Designed for ASTM D2887 and the extended D2887 method compliance
- Low bleed
- Extended analysis to C_{120} with maximum temperature of 450 °C
- UltiMetal tubing for excellent durability (same id as 0.53 mm id fused silica)
- Excellent retention time repeatability and column lifetime due to special deactivation of UltiMetal surface

Similar Phases: Petrocol EX2887, MXT-2887, Rtx-2887, AC Controls High Temp Sim Dist, AT-2887, ZB-1XT SimDist

CP-SimDist UltiMetal

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.53	5	0.09	450/450	CP7569	CP7569I5
		0.17	450/450	CP7532	CP7532I5
		0.88	450/450	CP7570	
		2.65	400/400	CP7571	
	10	0.17	450/450	CP7542	CP7542I5
		0.06	450/450	CP6540	
		0.53	450/450	CP7592	
		0.88	450/450	CP7512	CP7512I5
		1.20	450/450	CP7562	
		2.65	400/400	CP7582	CP7582I5
		5.00	400/400	CP7572	
	20	0.11	450/450	CP7593	
	25	0.06	450/450	CP6550	
	50	0.06	450/450	CP6560	

CP-Sil 2 CB

- Lowest polarity bonded stationary phase available
- Superior replacement to squalane
- Unique selectivity toward cyclic hydrocarbons
- Separation almost entirely based on boiling point
- Stable at temperatures up to 200 °C

CP-Sil 2 CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	25	0.25	25 to 200/200	CP7714	CP7714I5
	50	0.25	25 to 200/200	CP7724	
0.32	50	0.25	25 to 200/200	CP7754	CP7754I5
	25	1.20	25 to 200/200	CP7764	
	50	1.20	25 to 200/200	CP7774	
0.53	25	2.00	25 to 200/200	CP7653	

CP-TCEP for Alcohols in Gasoline

- Engineered for analysis of alcohols in gasoline
- Excellent peak shape for accurate separations of alcohols
- Temperature stability to 135 °C for high productivity
- Unique selectivity separates benzene after n-dodecane

Similar Phases: Rt-TCEP

CP-TCEP

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	50	0.40	135/140	CP7525	CP7525I5

Select Low Sulfur

- Highest degree of column inertness provides excellent peak shape for active compounds
- Low detection limits for sulfur compounds
- Unique selectivity prevents co-elution and matrix interferences in propylene streams
- Highly permeable PLOT stationary phase provides high retention of volatile compounds
- Unique QC testing results in consistent column inertness performance
- Mechanical stability results in no particle loss

Select Low Sulfur

ID (mm)	Length (m)	Temp Limits (°C)	7 in Cage
0.32	60	185	CP8575

CP-Sil 5 CB for Sulfur

- Optimized for analysis of Volatile Sulfur Compounds
- Trace analysis of sulfur compounds to C_7 mercaptan for high productivity
- Non-polar phase provides accurate separations based on volatility
- High inertness, elutes SO_2 for high quality data and low detection limits

CP-Sil 5 CB for Sulfur

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.32	30	4.00	-60 to 300/325	CP7529	CP7529I5

Select for Permanent Gases – Dual Column

- Set of two parallel columns: CP-Molsieve 5Å for permanent gases and PoraBOND Q for CO_2 analysis
- Isothermal separation at temperatures > 40 °C eliminates the need for cryogenics
- Temperature stability up to 300 °C allows short regeneration times and improves efficiency
- One injector, one detector simplifies operation
- Engineered for fast separation, low level analysis and quantification of argon/oxygen
- Separates permanent gases and CO_2 in a single run
- Coupled, tested and securely mounted on EZ-GRIP column mount
- For resolution of the difficult-to-separate argon/oxygen and helium/neon pairs, use CP7530 Select Permanent Gases/HR (High Resolution) column

Select for Permanent Gases – Dual Column

Description	Temp Limits (°C)	7 in Cage
Select Permanent Gases/CO_2	300/325	CP7429
Select Permanent Gases/HR	300/325	CP7430

Select Al_2O_3 MAPD

- Aluminum oxide PLOT column for the analysis of reactive hydrocarbons such as methyl acetylene and propadiene (MAPD)
- Optimized to improve sensitivity and response
- Faster run improves operating efficiency
- Two-fold higher response for MAPD, especially important when running impurity analyses

Similar Phases: Rt-Alumina BOND/MAPD, MXT-Alumina BOND/MAPD

Select Al_2O_3 MAPD

ID (mm)	Length (m)	Temp Limits (°C)	7 in Cage
0.32	50	-100 to 200/200	CP7431
0.53	25	-100 to 200/200	CP7433
	50	-100 to 200/200	CP7432



Agilent J&W Biodiesel Capillary GC Columns

Biofuels are becoming more attractive as a viable supplement or alternative to petroleum-based fuels. Agilent J&W Biodiesel Capillary GC columns are purposely designed and application-optimized for the analysis of biodiesel to meet ASTM and CEN testing standards.

Biodiesel EN14105 Free/Total Glycerin and Biodiesel ASTM D6584 Free/Total Glycerin

- Designed for the analysis of free and total glycerin in B100 according to EN14105 or ASTM D6584
- Specially processed for extended temperature limit of 400 °C
- High temperature, polyimide-coated fused silica tubing
- Excellent peak shape and extended column life
- Bonded and cross-linked
- Solvent rinsable
- Retention gaps please order P/N 160-BD65-5 (5 m x 0.53 mm)

Biodiesel EN14103 FAME Analysis

- Specially designed for the analysis of esters and linoleic acid methyl esters in B100 using EN14103
- Bonded and cross-linked
- Solvent rinsable

Biodiesel EN14110 Residual Methanol

- Specially designed for the determination of trace methanol in B100 using EN14110
- Bonded and cross-linked
- Solvent rinsable

Biodiesel Capillary GC Columns

Description	ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
Biodiesel ASTM D6584 Free/Total Glycerin	0.32	15	0.10	-60 to 400	123-BD11
Biodiesel EN14105 Free/Total Glycerin	0.32	10	0.10	-60 to 400	123-BD01
Biodiesel EN14103 FAME Analysis	0.32	30	0.25	40 to 260/270	1909BD-113
Biodiesel EN14110 Residual Methanol	0.32	30	1.80	20 to 260/280	123-BD34

Biodiesel Test Samples

Description	Part No.
Biodiesel MSTFA kit, 10 x 1 mL ampoules, N-Methyl-N-(trimethylsilyl)trifluoro-acetamide for ASTM method D6584	5190-1407
Biodiesel D6584 kit 2 internal standard solutions, 1 mL, 5/pk and 2 internal standard solutions, 5 mL	5190-1408
Biodiesel E14105 kit, 4 x 1 mL ampoules 4 standard solutions	5190-1409
Biodiesel Monoglyceride kit, 3 x 1 mL ampoules	5190-1410

Select Biodiesel

- Complete set of biodiesel columns for full compliance and ease-of-use
- UltiMetal technology provides high accuracy and longevity
- Pre-tested for complete confidence in results
- Good column lifetime when operating at temperatures up to 400 °C
- UltiMetal column with ultra stable stationary phase
- Convenient pre-coupled retention gap that is leak tested

Technical Specifications

Method	Analytes	Column	Injector Type	Analysis Time (min)
ASTM D 6584	Free and total glycerine	Select Biodiesel for Glycerides	On-column	32
EN14103	Ester and linoleic acid methyl esters	Select Biodiesel for FAME	Split/splitless	30
EN14105	Free and total glycerine; mono, di- and tri-glycerides	Select Biodiesel for Glycerides	On-column	35
EN14106	Free glycerol	Select Biodiesel for Glycerides	Split/splitless	10
EN14110	Methanol	Select Biodiesel for Methanol	Headspace with split/splitless	10

Select Biodiesel

Description	ID (mm)	Length (m)	Film (µm)	7 in Cage
For gylcerides, UltiMetal, with retention gap	0.32	15	0.10	CP9078
For gylcerides, UltiMetal	0.32	15	0.10	CP9079
For gylcerides, UltiMetal, with retention gap	0.32	10	0.10	CP9076
For gylcerides, UltiMetal	0.32	10	0.10	CP9077
For FAME, fused silica	0.32	30	0.25	CP9080
For Methanol, fused silica	0.32	30	3.00	CP9083
UltiMetal retention gap, methyl deactivated	0.53	2		CP6530

Select Silanes

- Stabilized trifluoropropyl-methyl polysiloxane phase for optimized ppm level analysis of silanes
- High capacity and retention
- Low bleed
- Reduced surface activity provides excellent peak shape
- Thick film offers high sample loading capacity and retention
- Typical applications include alkylated chlorosilanes at % levels as well as impurity analysis
- Valved, direct and split/splitless injections are possible

Select Silanes

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.32	30	1.80	0 to 270/300	CP7434
	60	1.80	0 to 270/300	CP7435
0.53	60	3.00	0 to 270/300	CP7437

CP-Volamine

- Non polar stationary phase
- Excellent stability for samples containing water expands the application range
- Maximum temperature of 265 °C for enhanced productivity
- Highly inert providing sharp amine peaks for accurate results
- Produces symmetrical peaks due to MPD (Multi-Purpose Deactivation) technology
- Excellent performance even when the sample contains high percentages of water
- Ideal for analyzing volatile amines like MMA, DMA and TMA (monomethyl, dimethyl and trimethyl amine)

Similar Phases: Rtx-Volatile Amines

CP-Volamine

ID (mm)	Length (m)	Temp Limits (°C)	7 in Cage	5 in Cage
0.32	15	265/300	CP7446	
	30	265/300	CP7447	CP7447I5
	60	265/275	CP7448	CP7448I5

CP-Sil 8 CB for Amines

- Base deactivated 5% phenyl polydimethylpolysiloxane
- Optimized inertness performance for a broad range of Amine compounds
- Thermal stability up to 350 °C enable separations of Amines up to C_{20} as well as alkanolamines
- Base deactivated columns also available as CP-Wax for Amines

Similar Phases: Rtx-5 Amine

CP-Sil 8 CB for Amines

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.15	*25*	*2.00*	*325/350*	*CP7599*	
0.25	30	0.25	325/350	CP7598	CP7598I5
	30	0.50	325/350	CP7595	CP7595I5
0.32	30	1.00	325/350	CP7596	CP7596I5
0.53	30	1.00	325/350	CP7597	CP7597I5

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

CP-Wax for Volatile Amines and Diamines

Similar Phases: Stabilwax DB

CP-Wax for Volatile Amines and Diamines

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.32	25	1.20	220/220	CP7422	CP7422I5
0.53	25	2.00	220/220	CP7424	

PoraPLOT Amines

- Unique PLOT columns specially designed for high retention of very volatile amines
- High efficiency at temperatures above ambient eliminates the need for cryogenics
- High sensitivity for amines and ammonia

PoraPLOT Amines

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.32	25	10.00	-100 to 220/220	CP7591	CP7591I5
0.53	25	20.00	-100 to 220/220	CP7594	

Pesticides Columns

Agilent J&W low-bleed columns are ideal for the analysis of pesticides. Not only do they possess less bleed than a standard polymer, which improves the signal-to-noise ratio and minimum detectable quantities, but they also have higher upper temperature limits which allow for faster run times. Agilent also offers several common phases with additional pesticide-specific testing to ensure performance for your application.

Note: For CLP pesticides and other methods using electron capture detectors, see DB-35ms, DB-17ms and DB-XLB.

DB-CLP 1 and DB-CLP 2

- Universal column pair designed for pesticides analyses
- EPA Methods: CLP (Contract Lab Program) pesticides, 504.1, 505, 508.1, 551, 552.3, 8081B, 8082A, 8154A
- Ideal for dual column, dual ECD GC analyses
- Mid polarity stabilized phases provide fast and low bleed reliable analyses
- Special testing includes pesticides for proof of performance and column to column reproducibility
- DB-CLP1 primary, DB-CLP2 confirmation

DB-CLP 1 and DB-CLP 2

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.32	30	0.25	50 to 340/360	123-8232
	30	0.5	50 to 340/360	123-8336

TIPS & TOOLS

Check out Agilent's complete line of sample preparation products for any type of GC and GC/MS analysis at **www.agilent.com/chem/sampleprep**



VF-5 Pesticides

- Specially designed for the determination of trace levels of pesticide residue
- Highly inert for enhanced ECD and MS detection
- Tested with key pesticides including endrin and aldrin for optimal performance and consistency of results
- Low bleed

VF-5 Pesticides

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	30	0.25	-60 to 325/350	CP9074
	50	0.25	-60 to 325/350	CP9073
0.32	30	0.25	-60 to 325/350	CP9075

DB-1701P

- Low/mid-polarity
- Exact replacement of HP-PAS1701
- Specifically designed and processed for the analysis of organochlorine pesticides
- ECD tested to ensure minimal pesticide breakdown and low ECD bleed
- Bonded and cross-linked
- Solvent rinsable

Similar Phases: SPB-1701, Rtx-1701, BP-10, CB-1701, OV-1701, 007-1701, ZB-1701P

DB-1701P

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.25	30	0.25	-20 to 280/300	122-7732		122-7732LTM
0.32	25	0.25	-20 to 280/300	123-7722		123-7722LTM
	30	0.25	-20 to 280/300	123-7732	123-7732E	123-7732LTM
0.53	30	1.00	-20 to 260/280	125-7732		125-7732LTM

VF-1701 Pesticides

- Specially designed for the determination of trace levels of pesticide residues
- Columns individually tested with key pesticides, including endrin and aldrin
- Highly inert for improved detection limits for trace pesticide determination
- Proven performance with ECD or MS detection
- Ultra low bleed to improve sensitivity

VF-1701 Pesticides

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	30	0.25	-20 to 280/300	CP9070
	50	0.25	-20 to 280/300	CP9072
0.32	30	0.25	-20 to 280/300	CP9071

CP-Sil 8 CB for Pesticides

- Linear column response down to femtogram level for improved productivity
- Excellent inertness – tested with DDTs to provide very reliable data
- Can be used with on-column injection techniques
- Integrated retention gap helps avoid problems with solvent condensation allowing repeated splitless injections without phase deterioration

CP-Sil 8 CB for Pesticides

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	50	0.12	300/325	CP7481
0.53	50	0.25	300/325	CP7504

CP-Sil 19 CB for Pesticides

- Ideal as a confirmation column for reliable results
- Specified for EPA and CLP analytes for ultimate compliance
- Supplied with a coupled retention gap for on-column injection for best detection limits

CP-Sil 19 CB for Pesticides

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	30	0.25	275/300	CP7406	
	50	0.20	275/300	CP7407	CP7407I5
0.32	30	0.25	275/300	CP7408	
0.53	30	1.00	260/275	CP7409	

DB-608

- Specifically designed for the analysis of chlorinated pesticides and PCBs
- U.S. EPA Methods: 608, 508, 8080
- Excellent inertness and recoveries without pesticide breakdown
- Bonded and cross-linked
- Solvent rinsable
- Exact replacement of HP-608

Similar Phases: SPB-608, NON-PAKD Pesticide, 007-608

DB-608

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	7890/6890 LTM Module	5975T LTM Toroid
0.18	*20*	*0.18*	*40 to 280/300*	*121-6822*	*121-6822LTM*	*221-6822LTM*
0.25	30	0.25	40 to 280/300	122-6832	122-6832LTM	
0.32	30	0.50	40 to 280/300	123-1730	123-1730LTM	
0.45	30	0.70	40 to 260/280	124-1730	124-1730LTM	
0.53	15	0.83	40 to 260/280	125-1710	125-1710LTM	
	30	0.50	40 to 260/280	125-6837	125-6837LTM	
		0.83	40 to 260/280	125-1730	125-1730LTM	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

HP-PAS5

- Non-polar
- Specifically designed and processed for the analysis of organochlorine pesticides
- ECD tested to ensure minimal pesticide breakdown and low ECD bleed
- Bonded and cross-linked
- Solvent rinsable

Similar Phases: SPB-5, RSL-200, Rtx-5, BP-5, CB-5, OV-5, 007-2 (MPS-5), SE-52, SE-54, XTI-5, PTE-5, CC-5, ZB-5

HP-PAS5

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	7890/6890 LTM Module
0.32	25	0.52	-60 to 325/350	19091S-010	19091S-010LTM

Rapid-MS

- Equivalent to 5% phenyl, 95% dimethylpolysiloxane
- Fast analysis time improves productivity
- Reduce analysis time by 3-5x for temperature programmed, and up to a 10x for isothermal runs
- The film thickness from 0.1 to 1 µm ensures high loadability and higher sensitivity
- Low bleed

Note: Rapid-MS columns utilize the high optimal carrier gas velocity obtained when a separation is performed under reduced pressure for fast analysis times

Rapid-MS

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.53	10	0.12	-60 to 325/325	CP8131
		0.25	-60 to 325/325	CP8132
		0.50	-60 to 325/325	CP8133
		1.00	-60 to 325/325	CP8134

Restriction for Rapid-MS

Description	Part No.
Restriction for Rapid-MS, fused silica, 0.1 mm id, 0.6 m, 5/pk	CP8121

PAH Columns

Select PAH

- Full separation for all PAH isomers avoids false positives and inaccurate results
- Full separation of EPA PAHs in less than 7 minutes and EU PAHs in less than 30 minutes including separation of chrysene, triphenylene and benzofluoranthene (type b, j, and k)
- Fast results with no need for further analysis
- Low bleed enhances sensitivity

Select PAH

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.15	*15*	*0.10*	*40 to 325/350*	*CP7461*
0.25	30	0.15	40 to 325/350	CP7462

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

DB-EUPAH

- Specially designed for analysis of EU regulated PAHs
- Individually tested with application-specific QC test probe mixture
- Great resolution of critical isomers, e.g. benzo(b,j,k)fluoranthenes
- Superb thermal stability for accurate analysis of high boiling PAHs, e.g. dibenzopyrenes
- Excellent signal-to-noise ratio
- Optimized column dimensions for proven performance

DB-EUPAH

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.18	*20*	*0.14*	*40 to 320/340*	*121-9627*
0.25	60	0.25	40 to 320/340	122-96L2
0.32	15	0.25	40 to 320/340	123-9612

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

CP-Sil PAH CB UltiMetal

- Separates all 16 PAHs according to EPA Method 610
- High temperature, low bleed phase
- Virtually unbreakable UltiMetal capillary column
- Maximum temperature of 400/425 °C

CP-Sil PAH CB UltiMetal

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	25	0.12	400/425	CP7440

Semivolatiles Columns

Semivolatiles are usually extracted from soil samples or other environmental matrices. GC columns with precise retention time reproducibility and good mass spectrometer performance are key enablers for these often demanding analyses.

DB-UI 8270D for Semivolatiles

- Designed for EPA Method 8270D and other regulated GC/MS semivolatiles analysis
- Special semivolatiles testing ensures poof of column to column performance for trace level analysis
- Excellent 2,4-dinitrophenol response
- Ultra Inertness and Low bleed
- Available in convenient and economical 6 packs (6 for the price of 5)

DB-UI 8270D for Semivolatiles

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.18	*20*	*0.36*	*-60 to 325/350*	*121-9723*
			-60 to 325/350	*621-9723, 6/pk**
0.25	30	0.25	-60 to 325/350	122-9732
			-60 to 325/350	622-9732, 6/pk*
		0.50	-60 to 325/350	122-9736

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

*Only available in the U.S.

CP-Sil 8 CB for PCB

- Engineered for the analysis of PCBs according to DIN method 51527
- Ideal for trace level ECD detection of PCBs
- High temperature stability provides low bleed and extended lifetime

CP-Sil 8 CB for PCB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	50	0.25	300/325	CP7482

DB-5.625

- Close equivalent to a (5%-Phenyl)-methylpolysiloxane
- Non-polar
- Specially processed to exhibit excellent inertness for EPA Semivolatiles Methods 625, 1625, 8270 and CLP protocols*
- Surpasses EPA performance criteria for semivolatiles
- Inert for base, neutral and acidic compounds
- High temperature limit with excellent thermal stability and low bleed
- Bonded and cross-linked
- Solvent rinsable

*Pentachlorophenol, 2,4-dinitrophenol, carbazole, and N-nitrosodiphenylamine used to test response factors.

Similar Phases: XTI-5, Rtx-5, PTE-5, BPX-5

DB-5.625

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	7890/6890 LTM Module
0.18	*20*	*0.18*	*-60 to 325/350*	*121-5621*	*121-5621LTM*
		0.36	*-60 to 325/350*	*121-5622*	*121-5622LTM*
0.25	30	0.25	-60 to 325/350	122-5631	122-5631LTM
		0.50	-60 to 325/350	122-5632	122-5632LTM
		1.00	-60 to 325/350	122-5633	122-5633LTM
	60	0.25	-60 to 325/350	122-5661	
0.32	30	0.25	-60 to 325/350	123-5631	123-5631LTM
		0.50	-60 to 325/350	123-5632	123-5632LTM

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers



HP-5ms Semivolatile

- (5%-Phenyl)-methylpolysiloxane, identical selectivity to HP-5
- Non-polar
- Very low bleed characteristics, ideal for GC/MS
- Specifically tested for inertness for active compounds including acidic and basic compounds
- Improved signal-to-noise ratio for better sensitivity and mass spectral integrity
- Bonded and cross-linked
- Solvent rinsable
- Equivalent to USP Phase G27

Similar Phases: Rtx-5ms, Rxi-5ms, Rxi-5Sil MS, PTE-5, BPX-5, AT-5ms, ZB-5ms, SLB-5ms, Equity-6

HP-5ms Semivolatile

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	7890/6890 LTM Module
0.25	30	0.50	-60 to 325/350	19091S-139	19091S-139LTM

CP-Sil 5/C18 CB for PCB

- Engineered for high resolution PCB analysis
- Lower polarity than 100% polydimethylpolysiloxane due to its C_{18} substitution
- Provides high signal-to-noise ratios for ECD detectors
- Optimized column length for separation of critical isomer pairs: 28/31, 56/60, 149/118, 105/153/132 and 170/190

CP-Sil 5/C18 CB for PCB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	50	0.10	275/300	CP7477
	100	0.10	275/300	CP7476
0.32	100	0.10	275/300	CP7478

DB-Dioxin

- Specifically engineered for the analysis of polychlorinated dibenzodioxins (PCDDs) and dibenzofurans (PCDFs)
- Resolves 2,3,7,8-TCDD and 2,3,7,8-TCDF from all other isomers in one run
- Low bleed
- Bonded and cross-linked
- Solvent rinsable

Note: 100 psi regulator required to reach optimum carrier gas velocity

Similar Phases: SP-2331, 007-23, Rtx-2332, Rtx-Dioxin

DB-Dioxin

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	60	0.15	40 to 250/270	122-2461	122-2461E
		0.25	40 to 250/270	122-2462	
0.32	60	0.15	40 to 250/270	123-2461	
		0.25	40 to 250/270	123-2462	

CP-Sil 88 for Dioxins

- High polarity stationary phase with specific selectivity for dioxins and dibenzofuran separations
- Integrated retention gap eliminates leaks and extends column lifetime with splitless injections
- 2,3,7,8-TCDD can be determined at low concentrations
- For fast runtimes, thin film configurations are available with maximum temperature program limit of 270 °C

Similar Phases: SP-2560, SP-2340, SP-2330, BPX-70, BPX-90

CP-Sil 88 for Dioxins

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	30	0.10	50 to 250/270	CP7497
	50	0.20	50 to 225/240	CP7588
	60	0.10	50 to 250/270	CP7498
0.32	60	0.13	50 to 250/270	CP7499

Volatiles Columns

Agilent offers a selection of advanced polymer chemistries for increasingly demanding volatiles applications. Whether for a primary analytical column or as a complementary confirmation column, Agilent J&W capillaries are chromatographers' first choice.

TIPS & TOOLS

Don't forget, we have special offers throughout the year.

To learn more, visit
www.agilent.com/chem/specialoffers

DB-624 Ultra Inert

- Environmental volatile organic compounds (VOCs) methods
- Excellent for U.S. EPA Methods: 501.3, 502.2, 503.1, 524.2, 601, 602, 8010, 8015, 8020,8240, 8260,
- Industrial chemical analyses – solvents, petrochemicals, specialty chemicals
- Food and beverage – alcohols, fusel oils
- Pharmaceutical residual solvents per USP <467>
- Ultra inertness processing expands application range with excellent peakshape for low molecular weight acidic compounds
- UI testing ensure premium performance column to column
- Identical selectivity to the industry standard DB-624 – upgrade with no change in method required
- Optimized by the inventors of DB-624

DB-624 Ultra Inert

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.18	*20*	*1*	*-20 to 260*	*121-1324UI*
0.25	30	1.4	-20 to 260	122-1334UI
	60	1.4	-20 to 260	122-1364UI
0.32	30	1.8	-20 to 260	123-1334UI
	60	1.8	-20 to 260	123-1364UI
0.53	30	3	-20 to 260	125-1334UI
	75	3	-20 to 260	125-1374UI

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

DB-624

- Specifically designed for the analysis of volatile priority pollutants and residual solvents
- No cryogenics needed for U.S. EPA Method 502.2
- Excellent for U.S. EPA Methods: 501.3, 502.2, 503.1, 524.2, 601, 602, 8010, 8015, 8020, 8240, 8260, and USP 467
- Excellent inertness for active compounds
- Bonded and cross-linked
- Solvent rinsable
- Exact replacement of HP-624
- Equivalent to USP Phase G43

Similar Phases: AT-624, Rxi-624 Sil MS, Rtx-624, PE-624, 007-624, 007-502, ZB-624

DB-624

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module	5975T LTM Toroid
0.18	*20*	*1.00*	*-20 to 280*	*121-1324*	*121-1324E*	*121-1324LTM*	*221-1324LTM*
0.20	25	1.12	-20 to 260	128-1324	128-1324E	128-1324LTM	
0.25	30	1.40	-20 to 260	122-1334	122-1334E	122-1334LTM	222-1334LTM
	60	1.40	-20 to 260	122-1364	122-1364E		
0.32	30	1.80	-20 to 260	123-1334	123-1334E	123-1334LTM	
	60	1.80	-20 to 260	123-1364	123-1364E		
0.45	30	2.55	-20 to 260	124-1334		124-1334LTM	
	75	2.55	-20 to 260	124-1374			
0.53	15	3.00	-20 to 260	125-1314			
	30	3.00	-20 to 260	125-1334	125-1334E	125-1334LTM	
	60	3.00	-20 to 260	125-1364	125-1364E		
	75	3.00	-20 to 260	125-1374	125-1374E		

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

CP-Select 624 CB

- 6% cyanopropyl, 94% dimethylpolysiloxane
- EPA volatiles methods 524.2, 624 and 8015
- Specified by Pharmacopoeia V.3.3.9 for residual solvents
- Excellent column-to-column reproducibility
- Low bleed

Similar Phases: AT-624, Rtx-624, PE-624, 007-624, 007-502, ZB-624

CP-Select 624 CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.15	*25*	*0.84*	*265/280*	*CP7411*	*CP7411I5*
0.25	30	1.40	265/280	CP7412	
	60	1.40	265/280	CP7413	CP7413I5
0.32	30	1.80	265/280	CP7414	CP7414I5
	60	1.80	265/280	CP7415	CP7415I5
0.53	30	3.00	265/280	CP7416	CP7416I5
	75	3.00	265/280	CP7417	
	105	3.00	265/280	CP7418	

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

TIPS & TOOLS

As part of Agilent's ongoing commitment to be your partner in chromatography, we have created a series of GC Troubleshooting videos, featuring Daron Decker, GC Applications Specialist, and Herb Brooks, Agilent Service Engineer. To view the videos, visit **www.agilent.com/chem/gctroubleshooting**



DB-VRX

- Unique selectivity engineered for optimum resolution of volatiles analysis: U.S. EPA Methods 502.2, 524.2 and 8260
- 0.45 mm id columns provide more plates per meter compared to 0.53 mm id columns for the fewest coelutions for GC method (an industry first)*
- No subambient cooling required to resolve the six "gases"
- Fast run time:
  <30 minutes for optimum sample throughput
  <8 minutes with 0.18 mm id
- Low polarity
- Excellent peak shape
- Bonded and cross-linked
- Solvent rinsable

*Two coelutions: 1) m- and p-xylene, for which U.S. EPA does not require separation, and 2) 1,1,2,2-tetrachloroethane and o-xylene which are separated by detectors PID and ELCD, respectively. **Note to GC/MS analysts:** These coeluting compounds have different primary characteristic ions of 83 and 106, respectively.

Similar Phases: VOCOL, NON-PAKD, Rtx-Volatiles, PE-Volatiles, 007-624, Rtx-VRX, Rtx-VGC

DB-VRX

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module	5975T LTM Toroid
0.18	*20*	*1.00*	*-10 to 260*	*121-1524*		*121-1524LTM*	*221-1524LTM*
	40	*1.00*	*-10 to 260*	*121-1544*	*121-1544E*	*121-1544LTM*	
0.25	30	1.40	-10 to 260	122-1534		122-1534LTM	222-1534LTM
	60	1.40	-10 to 260	122-1564	122-1564E		
0.32	30	1.80	-10 to 260	123-1534		123-1534LTM	
	60	1.80	-10 to 260	123-1564	123-1564E		
0.45	30	2.55	-10 to 260	124-1534		124-1534LTM	
	75	2.55	-10 to 260	124-1574			

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

HP-VOC

- Selectivity engineered for U.S. EPA Methods 502.2, 524.2 and 8260
- Low polarity – slightly more polar than DB-VRX
- Excellent peak shape
- Bonded and cross-linked
- Solvent rinsable

Similar Phases: NON-PAKD, Rtx-Volatiles, PE-Volatiles, 007-624, Rtx-VRX, Rtx-VGC

HP-VOC

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	7890/6890 LTM Module	5975T LTM Toroid
0.20	30	1.10	-60 to 280/290	19091R-303	19091R-303LTM	29091R-303LTM
	60	1.10	-60 to 280/290	19091R-306		
0.32	60	1.80	-60 to 280/290	19091R-316		
	90	1.80	-60 to 280/290	19091R-319		
0.53	90	3.00	-60 to 280/290	19095R-429		
	105	3.00	-60 to 280/290	19095R-420		

DB-502.2

- Available in 105 m for volatiles analyses
- Excellent peak shape
- Bonded and cross-linked
- Solvent rinsable

DB-502.2

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	60	1.40	0 to 260/280	122-1464
0.32	60	1.80	0 to 260/280	123-1464
0.45	75	2.55	0 to 260/280	124-1474
	105	2.55	0 to 260/280	124-14A4
0.53	105	3.00	0 to 260/280	125-14A4

DB-MTBE

- Low polarity stationary phase
- Resolves MTBE from 2-methylpentane and 3-methylpentane for better quantitation
- Engineered for purge and trap injection without the need for cryofocusing
- Bonded and cross-linked
- Solvent rinsable

DB-MTBE

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.45	30	2.55	35 to 260/280	124-0034		124-0034LTM
0.53	30	3.00	35 to 260/280	125-0034	125-0034E	125-0034LTM

CP-Select CB for MTBE

- Engineered for analysis of MTBE in reformulated gasoline
- Unique selectivity for MTBE
- Broad dynamic range for quantification of MTBE
- Ideal as primary or confirmation column

CP-Select CB for MTBE

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	50	0.25	200/200	CP7528

DB-TPH

- Specifically designed for the analysis of total petroleum hydrocarbons (TPHs), soil analysis, and LUFT
- Three analyses in one injection – gas range organics, diesel range organics and motor oil
- Fast run time
- Bonded and cross-linked
- Solvent rinsable

DB-TPH

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	7890/6890 LTM Module
0.32	30	0.25	-10 to 320	123-1632	123-1632LTM
0.45	30	1.00	-10 to 290	124-1632	

TIPS & TOOLS

For a precision cut on your capillary column, use Agilent's GC column cutting tool (P/N 5183-4620).



Select Mineral Oil

- Stabilized non-polar bonded phase engineered for fast mineral oil analysis
- Optimized selectivity for reliable Total Petroleum Hydrocarbon (TPH) results per DIN H53 N-ISO 9377-2 methods
- C_4 to C_{40} hydrocarbons can be analyzed in less than ten minutes
- Low bleed
- Available in Fused Silica or UltiMetal
- Fast run time
- High temperature stability up to 375/400 °C
- Available in economical 3 and 6 packs

Note: For optimal injection performance, use the 4 m x 0.53 mm id retention gap

Similar Phases: Rtx-Mineral Oil

Select Mineral Oil

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	Unit	7 in Cage	5 in Cage
0.32	15	0.10	-60 to 390/400	1/pk	CP7491	CP7491I5
	15	0.10	-60 to 390/400	3/pk	CP749103	
	15	0.10	-60 to 390/400	6/pk	CP749106	
Retention gap						
0.53	4		-60 to 325/350	3/pk	CP8015	

Select Mineral Oil UltiMetal


ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.32	15	0.10	-60 to 390/400	CP7493

TIPS & TOOLS

Ensure highest quality gas while keeping gas lines clean and leak-free with Agilent's high-capacity gas filter. Learn more at **www.agilent.com/chem/gasclean**





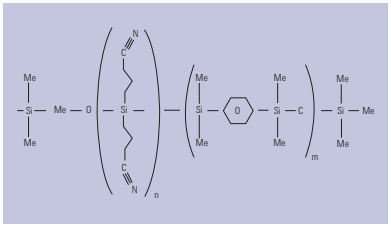

Structure of HP-88

Food, Flavors and Fragrances Columns

Food and flavor analyses place stringent demands on capillary columns. Samples have many components that are difficult to resolve and column-to-column reproducibility becomes critical. Agilent J&W GC columns are ideal for meeting these needs. Our rigorous quality control specifications and extensive QC testing ensure that the column you buy today will perform just like the column you buy tomorrow.

HP-88

- (88%-Cyanopropyl)aryl-polysiloxane
- 250/320 °C upper temperature limits
- High polarity
- Designed for separation of cis-trans fatty acid methyl esters (FAMEs)
- Even better separation than DB-23 of cis-trans isomers

Similar Phases: SP-2560, SP-2340, SP-2330, BPX-70, BPX-90

HP-88

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.25	100	0.25	0 to 250/260	112-88A7	112-88A7E	
	60	0.20	0 to 250/260	112-8867	112-8867E	
	30	0.20	0 to 250/260	112-8837	112-8837E	112-8837LTM

CP-Sil 88

- High selectivity towards positional and geometric isomers for ease-of-use
- Highly substituted cyanopropyl phase
- Highest polarity, non-chemically bonded and stabilized

Similar Phases: SP-2560, SP-2340, SP-2330, BPX-70, BPX-90

CP-Sil 88

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	25	0.20	50 to 225/240	CP6172	CP6172I5
	50	0.20	50 to 225/240	CP6173	CP6173I5
0.32	25	0.20	50 to 225/240	CP6174	CP6174I5
	50	0.20	50 to 225/240	CP6175	

TIPS & TOOLS

Order your free GC troubleshooting and GC column installation posters at **www.agilent.com/chem/GCposteroffer**



Select FAME

- Tuned for optimal cis-tans separation of FAMEs, especially C_{18} isomers
- Excellent peak shape and separation for FAME isomers – especially if one component is present at a higher concentration
- Bonded and cross-linked
- Low bleed
- High efficiency and column loadability
- Column length up to 200 m available for detailed analysis of the C_{18}:1 isomer cluster

Select FAME

ID (mm)	Length (m)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	50	275/290	CP7419	CP7419I5
	100	275/290	CP7420	CP7420I5
	200	275/290	CP7421	

CP-Sil 88 for FAME

- Optimized for analysis of FAME cis/trans isomers
- High polarity stationary phase provides improved efficiency and higher productivity
- Use for FAME separations in the C_6 to C_{26} range

CP-Sil 88 for FAME

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	50	0.20	225/240	CP7488
	60	0.20	225/240	CP7487
	100	0.20	225/240	CP7489

CP-Wax 57 CB

- Unique high polarity bonded wax column
- Industry proven for the analysis of alcohols in the brewing and wine/spirits industry
- Excellent inertness for optimum peak shape of alcohols and glycols
- Offered in 0.15 mm id for significantly high speed throughput

Similar Phases: SUPELCOWAX 10, SUPEROX II, CB-WAX, Stabilwax, BP-20, 007-CW, Carbowax, Rtx-WAX, ZB-WAX

CP-Wax 57 CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.15	*15*	*0.12*	*20 to 200/225*	*CP97711*	*CP97711I5*
	30	*0.12*	*20 to 200/225*	*CP97721*	
0.25	25	0.20	20 to 200/225	CP97713	
	50	0.20	20 to 200/225	CP97723	CP97723I5
	60	0.40	20 to 200/225	CP8120	
0.32	25	0.20	20 to 200/225	CP97743	
		1.20	20 to 200/225	CP97763	CP97763I5
	50	0.20	20 to 200/225	CP97753	CP97753I5
		1.20	20 to 200/225	CP97773	CP97773I5
0.53	25	1.00	20 to 200/225	CP97638	CP97638I5
	25	2.00	20 to 200/225	CP97658	CP97658I5

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

CP-Carbowax 400 for Volatiles in Alcohol

- Designed for the analysis of volatiles in alcoholic beverages
- High resolution for amyl alcohols for accurate quality control
- High efficiency
- Special testing ensure performance and column-to-column reproducibility

CP-Carbowax 400 for Volatiles in Alcohol

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.32	50	0.20	60/80	CP7527	CP7527I5

CP-Wax 57 CB for Glycols and Alcohols

- Optimized for the analysis of glycols, diols and alcohols
- Unique, high polarity wax phase
- Symmetrical peaks providing the most accurate results
- Cross-linked and bonded phase delivers robustness and enhanced column lifetime

CP-Wax 57 CB for Glycols and Alcohols

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	25	0.25	200/200	CP7615	CP7615I5
0.53	25	0.50	225/250	CP7617	CP7617I5

CP-TAP CB for Triglycerides

- Engineered phase for detailed analysis of triglycerides
- Separates complete triglyceride pattern in less than 16 minutes
- Separation based on carbon number and degree of unsaturation
- Stabilized phase for low bleed and enhanced column lifetime
- Available in Fused Silica and UltiMetal

CP-TAP CB for Triglycerides

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	25	0.10	350/360	CP7483

CP-TAP CB UltiMetal

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	25	0.10	355/370	CP7463


CP-FFAP CB for Free Fatty Acids in Dairy Products

- Ideal for flavors, aromas and free fatty acids C_1 to C_{26}
- Separates C_2-C_{24} acids in one run without derivatization
- Chemically-bonded for excellent longevity
- Water and solvent resistant

CP-FFAP CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.15	*25*	*0.25*	*250/275*	*CP7686*	*CP7686I5*
0.32	25	0.30	250/275	CP7485	CP7485I5
0.53	25	1.00	250/275	CP7486	CP7486I5

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

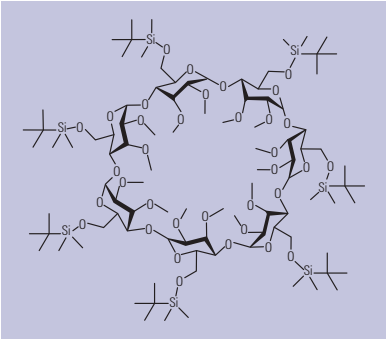

Structure of CycloSil-B

CycloSil-B

- 30% heptakis (2,3-di-O-methyl-6-O-t-butyl dimethylsilyl)-β-cyclodextrin in DB-1701
- Chiral separations without chiral-specific derivatization
- New stationary phase for improved resolution of many chiral separations
- Ideal for many chiral γ-lactones and terpenes

Note: Because CycloSil-B GC columns are not bonded or cross-linked, we do not recommend solvent rinsing.

Similar Phases: LIPODEX C, Rt-β DEXm, β-DEX 110, β-DEX 120

CycloSil-B

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	7890/6890 LTM Module
0.25	30	0.25	35 to 260/280	112-6632	112-6632LTM
0.32	30	0.25	35 to 260/280	113-6632	113-6632LTM

Cyclodex-B

- 10.5% β-cyclodextrin in DB-1701
- Chiral separations without chiral-specific derivatization
- Broad range of resolving potential
- Excellent peak shape

Note: Because Cyclodex-B GC columns are not bonded or cross-linked, we do not recommend solvent rinsing.

Similar Phases: LIPODEX C, Rt-β DEXm, β-DEX 110, β-DEX 120

Cyclodex-B

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.25	30	0.25	50 to 230/250	112-2532	112-2532E	112-2532LTM
	60	0.25	50 to 230/250	112-2562		
0.32	30	0.25	50 to 230/250	113-2532	113-2532E	113-2532LTM

HP-Chiral β

- β-cyclodextrin in (35%-Phenyl)-methylpolysiloxane
- Chiral separations without chiral-specific derivatization
- Phenyl-based polymer provides low bleed and does not interfere with nitrogen-specific detectors
- Available in two concentrations of β-cyclodextrin: 10% and 20%
- 20% β-cyclodextrin best choice for initial screening

Similar Phases: LIPODEX C, Rt-β DEXm, β-DEX 110, β-DEX 120

HP-Chiral β

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
HP-Chiral 10β					
0.25	30	0.25	30 to 240/250	19091G-B133	
0.32	30	0.25	30 to 240/250	19091G-B113	
HP-Chiral 20β					
0.25	30	0.25	30 to 240/250	19091G-B233	19091G-B233E
0.32	30	0.25	30 to 240/250	19091G-B213	19091G-B213E

CP-Chirasil Val

- Designed for separations of optically active compounds including amino acids
- Both antipode phases are available (D and L) for maximum versatility
- Stabilized chiral phase, over 50% cross-linked for longevity
- Tested for separation of amino acid enantiomers
- Low bleed

Note: On Chirasil-L Val, D-amino acids elute before the L-amino acids, while on Chirasil-D-Val, this elution order is reversed. This is especially valuable when determining the optical purity of these compounds. Selecting the column from which the minor compound elutes before the major enantiomers results in the lowest detection levels.

CP-Chirasil Val

Description	ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
Antipode D	0.25	25	0.08	200/200	CP7494	CP7494I5
Antipode L	0.25	25	0.12	200/200	CP7495	CP7495I5

CP-Chirasil-Dex CB

- Cyclodextrin bonded to dimethylpolysiloxane for homogeneous enantioselectivity throughout the column
- High resolution factor between isomers across a broad application range
- Chemically bonded phase for excellent longevity
- No need for derivatization improved productivity
- Low elution temperature of polar compounds
- Suitable for all injection techniques

Similar Phases: LIPODEX C, Rt-β DEXm, β-DEX 110, β-DEX 120

CP-Chirasil-Dex CB

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	25	0.25	200/200	CP7502	CP7502I5
0.32	25	0.25	200/200	CP7503	CP7503I5

CP-Cyclodextrin-β-2,3,6-M-19

- Unique selectivity for optical and positional isomer separations
- High efficiency enables wide range of applications
- Separates o-,m-, and p-xylenes
- Excellent peak shape for underivatized polar compounds

CP-Cyclodextrin-β-2,3,6-M-19

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	25	0.25	225/250	CP7500	CP7500I5
0.32	50	0.25	225/250	CP7501	

TIPS & TOOLS

Agilent CrossLab GC supplies, including CrossLab Ultra Inert liners, perform seamlessly with a variety of instruments regardless of make or model, including Varian (now Bruker), PerkinElmer, Shimadzu, and Thermo Scientific GC systems. Learn more at **www.agilent.com/chem/CrossLab**



Life Sciences Columns

The life sciences offer some difficult challenges to capillary GC chromatographers. These include complex sample matrices, the necessity for low level detection and the chemically active characteristics of many of the samples. In response to this, Agilent offers a line of columns which are designed specifically for drugs of abuse testing.

DB-ALC1 and DB-ALC2

- Reliable blood alcohol analysis
- Optimized primary and confirmation column pair for U.S. blood alcohol analysis
- Faster GC run times
- Improved resolution of key ethanol/acetone peaks
- Available in 0.32 and 0.53 mm id
- Bonded and cross-linked

Similar Phases: Rtx-BAC1, Rtx-BAC2, ZB-BAC-1, ZB-BAC-2

DB-ALC1 and DB-ALC2

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
DB-ALC1						
0.32	30	1.80	20 to 260/280	123-9134		123-9134LTM
0.53	30	3.00	20 to 260/280	125-9134	125-9134E	125-9134LTM
DB-ALC2						
0.32	30	1.20	20 to 260/280	123-9234	123-9234E	123-9234LTM
0.53	30	2.00	20 to 260/280	125-9234		125-9234LTM

VF-DA

- Engineered for drugs of abuse confirmation testing
- High recovery for trace level analysis and excellent resistance to direct methanol injections
- Ultra low bleed

VF-DA

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.20	12	Optimized	-60 to 325/350	CP8964

HP-Blood Alcohol

- Reliable blood alcohol analysis
- Excellent confirmation column with DB-ALC2 for method using t-butanol as internal standard

Similar Phases: Aucune

HP-Blood Alcohol

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.32	7.5	2.00	-60 to 270/290	19091S-510	19091S-510E	19091S-510LTM

DB-5ms EVDX

- Specially configured and tested for drugs of abuse confirmation
- Drug test mix included: caffeine, glutethimide, lidocaine, phenobarbital, EDDP, methaqualone, methadone, cocaine, desipramine, carbamazepine
- DB-5ms EVDX is equivalent to (5%-Phenyl)-methylpolysiloxane
- Consistent retention and peak shape
- Low bleed for GC/MS analysis
- Bonded and cross-linked
- Solvent rinsable

DB-5ms EVDX

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.20	25	0.33	-60 to 325/350	128-8522

DB-Select 624 UI for <467>

- Engineered to optimize pharmaceutical residual solvents analysis per USP Method <467>
- Ultra Inertness and low bleed
- Resolution of USP regulated critical pairs, also separates benzene and 1,2-dichloroethane
- Identical selectivity to the popular VF-624 ms – upgrade with no changes in method.
- UI testing ensures premium performance column to column

DB-Select 624 UI for <467>

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	30	1.4	40 to 260/260	122-0334UI
	60	1.4	40 to 260/260	122-0364UI
0.32	30	1.8	40 to 260/260	123-0334UI
	60	1.8	40 to 260/260	123-0364UI
0.53	30	1.8	40 to 260/260	125-0334UI

HP-Fast Residual Solvent

- Equivalent to USP Phase G43
- Thinner film reduces run time by 2.5 times and increases Minimum Detection Limit (MDL) by 2 times compared to standard film thickness used for this method
- Bonded and cross-linked

Similar Phases: PE-624, 007-624, 007-502, ZB-624

HP-Fast Residual Solvent

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.53	30	1.00	-20 to 260	19095V-420	19095V-420E	19095V-420LTM

Metal Columns

DB-ProSteel and UltiMetal columns are engineered to combine the robustness of stainless steel with advanced surface deactivation for excellent peak shape.

- Configured for high temperature analyses such as simulated distillation
- Wide variety of stationary phases and configurations available
- Ideal for portable and process GC applications
- Superior replacement for MXT/Silco-steel columns

Metal Columns

Phase	ID (mm)	Length (m)	Film (µm)	7 in Cage	5 in Cage
Simulated distillation/high temperature					
DB-HT SimDis	0.53	5	0.10	145-1009	
			0.15	145-1001	
DB-PS2887	0.53	10	3.00	145-2814	
CP-SimDist UltiMetal	0.53	5	0.09	CP7569	CP7569I5
			0.17	CP7532	CP7532I5
			0.88	CP7570	
			2.65	CP7571	
		10	0.06	CP6540	
			0.17	CP7542	CP7542I5
			0.53	CP7592	
			0.88	CP7512	
			1.20	CP7562	
			2.65	CP7582	
			5.00	CP7572	
		20	0.11	CP7593	
		25	0.06	CP6550	
VF-5ht UltiMetal	0.25	15	0.10	CP9090	
	0.32	15	0.10	CP9094	CP9094I5
	0.25	30	0.10	CP9092	
	0.32	30	0.10	CP9096	

(Continued)


Metal Columns

Phase	ID (mm)	Length (m)	Film (µm)	7 in Cage	5 in Cage
Simulated distillation/high temperature					
VF-5ht UltiMetal with Retention Gap UltiMetal	0.25	15	0.10	CP9091	
	0.32	15	0.10	CP9095	
	0.25	30	0.10	CP9093	
	0.32	30	0.10	CP9097	
Standard phases and PEG					
DB-PS1	0.53	15	0.15	145-1011	
		30	1.50	145-1032	
CP-Sil 5 CB	0.53	10	0.50	CP7125	
			1.00	CP7120	
			2.00	CP7150	
			5.00	CP6666	CP6666I5
		25	0.50	CP7135	CP7135I5
			1.00	CP7130	
			2.00	CP7160	
			5.00	CP6670	
		50	0.50	CP7195	
			1.00	CP7140	
			2.00	CP7170	
			5.00	CP6671	
DB-HT SimDis	0.53	5	0.10	145-1009	
			0.15	145-1001	
DB-PS2887	0.53	10	3.00	145-2814	
CP-SimDist UltiMetal, 6/pk	0.53	5	0.09	CP67569	
CP-SimDist UltiMetal	0.53	5	0.09	CP7569	
			0.17	CP7532	
			0.88	CP7570	
			2.65	CP7571	
		10	0.06	CP6540	
			0.17	CP7542	
			0.53	CP7592	
			0.88	CP7512	
			1.20	CP7562	
			2.65	CP7582	
			5.00	CP7572	
		20	0.11	CP7593	
		25	0.06	CP6550	

(Continued)

Metal Columns

Phase	ID (mm)	Length (m)	Film (µm)	7 in Cage	5 in Cage
Standard phases and PEG					
CP-Sil 8 CB UltiMetal	0.53	10	1.00	CP7121	
		25	5.00	CP6680	
		50	5.00	CP7196	
				CP6681	
CP-Sil 13 CB UltiMetal	0.53	25	1.00	CP7141	
		50	0.50	CP7129	
DB-PSWAX	0.53	30	1.00	145-7032	
CP-WAX 52 CB UltiMetal	0.53	10	1.00	CP7148	
			2.00	CP7177	
		25	0.50	CP7138	
			1.00	CP7158	
			2.00	CP7178	
		50	0.50	CP7198	
			1.00	CP7168	
			2.00	CP7179	
PLOT columns					
PoraPLOT Q UltiMetal	0.53	10	20.00	CP6953	CP6953I5
		25	20.00	CP6954	CP6954I5
		50	20.00	CP6955	
CP-Al2O3/KCl UltiMetal	0.53	50	10.00	CP6918	
CP-Al2O3/Na2SO4 UltiMetal	0.53	50	10.00	CP6968	
CP-Molsieve 5Å UltiMetal	0.53	10	50.00	CP6937	
		25	50.00	CP6938	CP6938I5
		50	50		CP6937I5
Select application columns					
DB-PS624	0.53	30	3.00	145-1334	
CP-Sil PAH CB UltiMetal	0.25	25	0.12	CP7440	
CP-TAP CB	0.25	25	0.10	CP7463	
Select Biodiesel With retention gap	0.32	10	0.10	CP9076	
		15	0.10	CP9078	
Select Biodiesel	0.32	10	0.10	CP9077	
		15	0.10	CP9079	

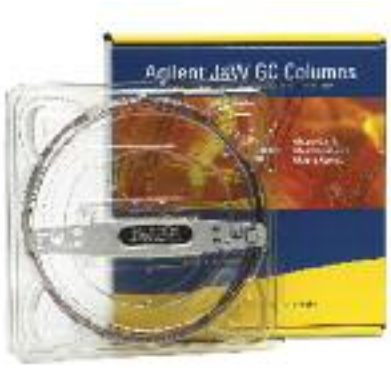

PLOT Columns

PLOT columns are ideal for separating compounds that are gases at room temperatures. Agilent Technologies offers a comprehensive line of PLOT columns for analysis of fixed gases, low molecular weight hydrocarbon isomers, volatile polar compounds and reactive analytes such as sulfur gases, amines and hydrides. Our PLOT phases are offered in dimensions from 0.25 to 0.53 mm id, allowing for easy column selection for various detector and system requirements. For GC/MS systems, we offer several small diameter columns with truly bonded and immobilized stationary phases, eliminating potential detector fouling due to particle generation.

PoraBOND Q

- Bonded PLOT column for more reliable results for analysis of volatile solvents and hydrocarbons
- Extended analysis offers broad application range
- 300/320 °C temperature limits
- Engineered for high stability, withstands repeated water injections
- Proprietary manufacturing technique results in very pure porous polymer with virtually no catalytic activity, allowing operation to 320 °C without decomposition
- Bonding technology results in greatly reduced particle shedding, reduces the needs for particle traps

Similar Phases: Rt-Q BOND, Rt-QPLOT, SupelQ PLOT

PoraBOND Q

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	10	3.00	-100 to 300/300	CP7347	CP7347I5
	25	3.00	-100 to 300/320	CP7348	CP7348I5
0.32	10	5.00	-100 to 300/320	CP7350	CP7350I5
	25	5.00	-100 to 300/320	CP7351	CP7351I5
	50	5.00	-100 to 300/320	CP7352	CP7352I5
0.53	10	10.00	-100 to 300/320	CP7353	CP7353I5
	25	10.00	-100 to 300/320	CP7354	CP7354I5
	50	10.00	-100 to 300/320	CP7355	

PoraBOND U



- Highly stable polar-bonded porous polymer with maximum operating temperature of 300 °C
- Reduced bleed for low detection limits and fast stabilization time
- Bonded PLOT column for excellent longevity
- Ideal for use with method that pressure programs or valve switching

Similar Phases: Rt-U-BOND

PoraBOND U

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.25	10	3.00	-100 to 300/300	CP7347

PoraPLOT Q and PoraPLOT Q-HT

- Recommended for column switching systems that analyze a broad range of polar and apolar volatile compounds
- Water elutes as a sharp peak enabling quantitation
- Retention of target compounds is not influenced by water in the sample
- Long term stability provides repeatable retention times
- Available in Fused Silica and UltiMetal

Similar Phases: Rt-Q BOND, Rt-QPLOT, SupelQ PLOT

PoraPLOT Q

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	10	8.00	-100 to 250/250	CP7548	
	25	8.00	-100 to 250/250	CP7549	CP7549I5
0.32	10	10.00	-100 to 250/250	CP7550	CP7550I5
	25	10.00	-100 to 250/250	CP7551	CP7551I5
	50	10.00	-100 to 250/250	CP7552	
0.53	10	20.00	-100 to 250/250	CP7553	CP7553I5
	25	20.00	-100 to 250/250	CP7554	CP7554I5
	50	20.00	-100 to 250/250	CP7555	

PoraPLOT Q UltiMetal

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.53	10	20.00	-100 to 250/250	CP6953	CP6953I5
	25	20.00	-100 to 250/250	CP6954	CP6954I5
	50	20.00	-100 to 250/250	CP6955	

PoraPLOT Q-HT

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.32	10	10.00	-100 to 290/290	CP7556	
	25	10.00	-100 to 290/290	CP7557	CP7557I5
0.53	10	20.00	-100 to 290/290	CP7558	CP7558I5
	25	20.00	-100 to 290/290	CP7559	CP7559I5

HP-PLOT Q

- Bonded polystyrene-divinylbenzene based column
- Polarity between Porapak-Q and Porapak-N
- Excellent column for C_1 to C_3 isomers and alkanes to C_{12}, CO_2, methane, air/CO, oxygenated compounds, sulfur compounds and solvents
- Replaces packed gas-solid columns
- Separates ethane, ethylene and ethyne (acetylene)
- Improved resolution in less time than conventional packed columns
- Minimal conditioning time required – 1 hour
- Preferred "Q" column due to its robust nature

Similar Phases: Rt-QPLOT, SupelQ PLOT

HP-PLOT Q

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.32	15	20.00	-60 to 270/290	19091P-Q03		19091P-Q03LTM
	30	20.00	-60 to 270/290	19091P-Q04	19091P-Q04E	19091P-Q04LTM
0.53	15	40.00	-60 to 270/290	19095P-Q03	19095P-Q03E	19095P-Q03LTM
	30	40.00	-60 to 270/290	19095P-Q04	19095P-Q04E	19095P-Q04LTM

GS-Q

- Porous divinylbenzene homopolymer
- Polarity between Porapak-Q and Porapak-N
- Separates ethane, ethylene and ethyne (acetylene)
- Not recommended for quantification of polar compounds
- Minimal conditioning time required – 1 hour

Similar Phases: Rt-QPLOT, SupelQ PLOT

GS-Q

ID (mm)	Length (m)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.32	30	-60 to 250	113-3432	113-3432E	113-3432LTM
0.53	10	-60 to 250	115-34H2		115-34H2LTM
	15	-60 to 250	115-3412		115-3412LTM
	25	-60 to 250	115-3422		115-3422LTM
	30	-60 to 250	115-3432	115-3432E	115-3432LTM

TIPS & TOOLS

View the latest GC column focused applications, products and educational resources at **www.agilent.com/chem/myGCcolumns**

PoraPLOT U and PoraPLOT S

- The most polar porous polymer PLOT column ideal for halogenated compounds, C_1-C_6 hydrocarbons, ketones and solvents
- Excellent peak shape of polar and non-polar volatiles
- Water has no effect on retention times and elutes as a sharp quantifiable peak
- Reliable retention time repeatability

PoraPLOT U

Similar Phases: Rt-U-BOND

PoraPLOT U

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	25	8.00	-100 to 190/190	CP7579	
0.32	10	10.00	-100 to 190/190	CP7580	
	25	10.00	-100 to 190/190	CP7581	
0.53	10	20.00	-100 to 190/190	CP7583	CP7583I5
	25	20.00	-100 to 190/190	CP7584	CP7584I5

PoraPLOT S

- Divinylbenzene/vinylpyridine polymer for hydrocarbons and ketones
- Ideal for the analysis of medium polarity volatile including hydrocarbons and ketones
- Higher temperature limit than PoraPLOT U

Similar Phases: Rt-S-BOND, MXT-SBOND

PoraPLOT S

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.53	25	20.00	-100 to 250/250	CP7574	CP7574I5

HP-PLOT U

- Bonded divinylbenzene/ethylene glycol dimethacrylate
- More polar than HP-PLOT Q
- Excellent column for C_1 to C_7 hydrocarbons, CO_2, methane, air/CO, water, oxygenates, amines, solvents, alcohols, ketones, and aldehydes
- Improved resolution in less time than conventional packed columns

Similar Phases: RTU PLOT

HP-PLOT U

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.32	30	10.00	-60 to 190	19091P-U04	19091P-U04E	19091P-U04LTM
0.53	15	20.00	-60 to 190	19095P-U03		19095P-U03LTM
	30	20.00	-60 to 190	19095P-U04	19095P-U04E	19095P-U04LTM

HP-PLOT Al_2O_3 KCl

- Least "polar" Alumina phase
- Aluminum oxide deactivated with KCl
- Standard column choice for light hydrocarbon analysis – C_1 to C_8 hydrocarbon isomers
- Low retention of olefins relative to comparable paraffin
- Excellent for quantitation of dienes, especially propadiene and butadiene from ethylene and propylene streams
- Recommended phase for many ASTM methods
- Preferred KCl deactivated Alumina

Similar Phases: Rt-Alumina PLOT, Alumina PLOT, Al_2O_3/KCl, AB-PLOT Al_2O_3 KCl, AT-Alumina

HP-PLOT Al_2O_3 KCl

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.25	30	5.00	-60 to 200	19091P-K33	19091P-K33E	19091P-K33LTM
0.32	50	8.00	-60 to 200	19091P-K15	19091P-K15E	
0.53	30	15.00	-60 to 200	19095P-K23		19095P-K23LTM
	50	15.00	-60 to 200	19095P-K25	19095P-K25E	

GS-Alumina KCl

- Least "polar" Alumina phase
- Aluminum oxide deactivated with KCl
- Good choice for light hydrocarbon analysis
- Good resolution of propadiene and butadiene from ethylene and propylene streams

Similar Phases: Al_2O_3/KCl, Al_2O_3/Na_2SO_4, Rt-Alumina PLOT, Alumina PLOT, AB-PLOT Al_2O_3 KCl, AT-Alumina

GS-Alumina KCl

ID (mm)	Length (m)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.53	30	-60 to 200	115-3332		115-3332LTM
	50	-60 to 200	115-3352	115-3352E	

CP-Al_2O_3/KCl and CP-Al_2O_3/Na_2SO_4

- Aluminum oxide PLOT columns offer high selectivity for separating ppm levels of C_1-C_5 hydrocarbons in process streams
- High capacity thick films
- No need for sub-ambient cooling
- Choice of two selectivities covers a broad range of applications
- Available in Fused Silica and UltiMetal

Note: The KCl deactivation salt results in a relatively apolar Al_2O_3 surface while the Na_2SO_4 deactivation provides a polar surface. Unsaturated compounds such as ethylene and acetylene (ethyne) are retained longer.

Selectivity Through KCl or Na_2SO_4 Deactivation

Note: Aluminum oxide PLOT columns are deactivated using KCl or NA_2SO_4 treatments which provides a reproducible and stable deactivation up to 200 °C. The KCl salt deactivation results in a relatively apolar Al_2O_3 surface, while the NA_2SO_4 deactivation provides a polar surface. Unsaturated compounds such as ethylene and acetylene (ethyne) are retained longer.

Similar Phases: Al_2O_3/KCl, Rt-Alumina PLOT, Alumina PLOT, RT-Alumina BOND/KCl , Alumina chloride PLOT, AB-PLOT Al_2O_3 KCl

CP-Al_2O_3/KCl

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	25	4.00	-100 to 200/200	CP7576	
	50	4.00	-100 to 200/200	CP7577	CP7577I5
0.32	10	5.00	-100 to 200/200	CP7511	CP7511I5
	50	5.00	-100 to 200/200	CP7515	CP7515I5
	25	5.00	-100 to 200/200	CP7519	CP7519I5
0.53	10	10.00	-100 to 200/200	CP7516	
	25	10.00	-100 to 200/200	CP7517	
	50	10.00	-100 to 200/200	CP7518	

CP-Al_2O_3/KCl UltiMetal

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.53	50	10.00	-100 to 200/200	CP6918

Similar Phases: Al_2O_3/Na_2SO_4, Rt-Alumina PLOT, Alumina PLOT, Rt-Alumina BOND/Na_2SO_4, MXT-AluminaBOND/Na_2SO_4, Alumina sulfate PLOT

CP-Al_2O_3/Na_2SO_4

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	25	4.00	-100 to 200/200	CP7586	
	50	4.00	-100 to 200/200	CP7587	
0.32	10	5.00	-100 to 200/200	CP7561	
	50	5.00	-100 to 200/200	CP7565	CP7565I5
0.53	25	10.00	-100 to 200/200	CP7567	
	50	10.00	-100 to 200/200	CP7568	

CP-Al_2O_3/Na_2SO_4 UltiMetal

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.53	50	10.00	-100 to 200/200	CP6968



HP-PLOT Al_2O_3 S

- Middle range of "polarity" for Alumina phases
- Aluminum oxide deactivated with sodium sulfate
- Excellent general use column for light hydrocarbon analysis – C_1 to C_8 hydrocarbon isomers
- Best for resolving acetylene from butane and propylene from isobutane

Similar Phases: Al_2O_3/Na_2SO_4, Rt-Alumina PLOT, Alumina PLOT, Rt-Alumina BOND/Na_2SO_4, MXT-AluminaBOND/Na_2SO_4, Alumina sulfate PLOT, AT-Alumina

HP-PLOT Al_2O_3 S

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.25	30	5.00	-60 to 200	19091P-S33		19091P-S33LTM
0.32	25	8.00	-60 to 200	19091P-S12		19091P-S12LTM
	50	8.00	-60 to 200	19091P-S15	19091P-S15E	
0.53	15	15.00	-60 to 200	19095P-S21		19095P-S21LTM
	30	15.00	-60 to 200	19095P-S23		19095P-S23LTM
	50	15.00	-60 to 200	19095P-S25	19095P-S25E	

GS-Alumina



- Most "polar" Alumina phase
- Aluminum oxide with proprietary deactivation
- Excellent general use column for light hydrocarbon analysis – C_1 to C_8 hydrocarbon isomers
- Separates C_1 to C_4 saturated and unsaturated hydrocarbons
- Best for resolving cyclopropane from propylene
- Faster, more efficient and provides more sensitivity than packed equivalents
- Minimal conditioning time required
- Preferred substitution for sodium sulfate deactivated Alumina because of its regenerative nature

Note: Alumina columns have a tendency to adsorb water and CO_2 which, over time, results in changes in retention time. We use an advanced, proprietary deactivation process which allows for rapid regeneration. Fully water saturated GS-Alumina columns regenerate in 7 hours or less at 200 °C.

Similar Phases: Al_2O_3/KCl, Al_2O_3/Na_2SO_4, Rt-Alumina PLOT, Alumina PLOT, AB-PLOT Al_2O_3 KCl, AT-Alumina

GS-Alumina

ID (mm)	Length (m)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.53	30	-60 to 200	115-3532	115-3532E	115-3532LTM
	50	-60 to 200	115-3552		

HP-PLOT Al_2O_3 M

- Most "polar" Alumina phase (similar to GS-Alumina)
- Aluminum oxide deactivated with proprietary deactivation
- Good general use column for light hydrocarbon analysis – C_1 to C_8 hydrocarbon isomers
- Good for resolving acetylene from butane and propylene from isobutane

Similar Phases: AB-PLOT Al_2O_3 M, BGB-PLOT Al_2O_3 M, AT-Alumina

HP-PLOT Al_2O_3 M

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.32	50	8.00	-60 to 200	19091P-M15	19091P-M15E	
0.53	30	15.00	-60 to 200	19095P-M23		19095P-M23LTM
	50	15.00	-60 to 200	19095P-M25		

GS-GasPro

- Unique bonded silica PLOT column technology
- Excellent choice for light hydrocarbons and sulfur gases
- Retention stability not affected by water
- Separates CO and CO_2 on a single column
- Ideal PLOT column for GC/MS – no particles

Similar Phases: CP-Silica PLOT

GS-GasPro

ID (mm)	Length (m)	Temp Limits (°C)	7 in Cage
0.32	5	-80 to 260/300	113-4302
	15	-80 to 260/300	113-4312
	30	-80 to 260/300	113-4332
	60	-80 to 260/300	113-4362

CP-SilicaPLOT

- No influence of water on retention times
- Elution of CO_2 and sulfur gases at ppm levels
- Separates cyclopropane from propylene
- Ideal for a wide range of applications such as COS in ethylene, freons, hydrocarbons, propylene and sulfur compounds
- High selectivity for C_1-C_4 isomers in the presence of water
- No negative influence on retention or peak shape when water is present in the sample
- Inert surface preparation results in no decomposition pentadienes or freons

Similar Phases: GS-GasPro

CP-SilicaPLOT

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	30	3.00	-80 to 225/225	CP8564	
	60	3.00	-80 to 225/225	CP8565	
0.32	10	4.00	-80 to 225/225	CP8574	
	15	4.00	-80 to 225/225	CP8566	CP8566I5
	30	4.00	-80 to 225/225	CP8567	CP8567I5
	60	4.00	-80 to 225/225	CP8568	CP8568I5
0.53	30	6.00	-80 to 225/225	CP8570	CP8570I5
	60	6.00	-80 to 225/225	CP8571	

TIPS & TOOLS

Ensure a lifetime of peak performance and maximum productivity with Agilent's comprehensive GC supplies portfolio, learn more at **www.agilent.com/chem/GCsupplies**



CarboBOND and CarboPLOT P7

- Single column solution for ASTM D 2505 for higher productivity
- Stable and robust for high repeatability of results
- Available in bonded and PLOT versions for improved versatility and enhanced productivity

CarboBOND

CarboBOND

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.53	25	5.00	-100 to 200/300	CP7371
		10.00	-100 to 200/300	CP7374
	50	5.00	-100 to 200/300	CP7372
		10.00	-100 to 200/300	CP7375

CarboPLOT P7

CarboPLOT P7

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage
0.53	10	25.00	-200 to 115/115	CP7513
	25	25.00	-200 to 115/115	CP7514

GS-CarbonPLOT

- High stability, bonded carbon layer stationary phase
- Unique selectivity for inorganic and organic gases
- Extended temperature limit of 360 °C
- Ideal for GC/MS – no particle generation
- Retention stability not affected by water

Similar Phases: Carbopack, CLOT, Carboxen-1006 PLOT

GS-CarbonPLOT

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	7890/6890 LTM Module
0.32	15	1.50	0 to 360	113-3112	
	30	1.50	0 to 360	113-3132	113-3132LTM
		3.00	0 to 360	113-3133	113-3133LTM
	60	1.50	0 to 360	113-3162	
0.53	15	3.00	0 to 360	115-3113	
	30	3.00	0 to 360	115-3133	115-3133LTM

HP-PLOT Molesieve

- A PLOT column for the analysis of permanent gases
- O_2, N_2, CO and CH_4 resolve in less than 5 min
- Durable molecular sieve 5Å coating minimizes baseline spiking and damage to multiport valves
- Select a thick film for Ar/O_2 separation without cryogenic cooling
- Select thin film HP-PLOT Molesieve columns for routine air monitoring applications
- Replaces GS-Molesieve

Note: Molecular sieve columns will absorb water, which, over time results in changes in retention time. We use an advanced, proprietary deactivation process which allows for rapid regeneration. Fully saturated HP-PLOT Molesieve columns regenerate in 7 hours or less at 200 °C.

Similar Phases: Rt-Msieve 5A, MXT-Msieve 5A

HP-PLOT Molesieve

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.32	15	25.00	-60 to 300	19091P-MS7		19091P-MS7LTM
	30	12.00	-60 to 300	19091P-MS4	19091P-MS4E	19091P-MS4LTM
		25.00	-60 to 300	19091P-MS8		19091P-MS8LTM
0.53	15	25.00	-60 to 300	19095P-MS5		19095P-MS5LTM
		50.00	-60 to 300	19095P-MS9		19095P-MS9LTM
	30	25.00	-60 to 300	19095P-MS6	19095P-MS6E	19095P-MS6LTM
		50.00	-60 to 300	19095P-MS0	19095P-MS0E	19095P-MS0LTM

CP-Molsieve 5Å

- Separate argon and oxygen at ambient temperature to reduce costs
- High efficiency for increased productivity
- Symmetrical peaks for accurate results

Similar Phases: Rt-Msieve 5A, MXT-Msieve 5A, Mol Sieve 5A PLOT

CP-Molsieve 5Å

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.25	25	30.00	-200 to 350/350	CP7533	
0.32	10	30.00	-200 to 350/350	CP7535	CP7535I5
	25	30.00	-200 to 350/350	CP7536	CP7536I5
	30	10.00	-200 to 350/350	CP7534	CP7534I5
	50	30.00	-200 to 350/350	CP7540	CP7540I5
0.53	10	50.00	-200 to 350/350	CP7537	
	15	15.00	-200 to 350/350	CP7543	
	25	50.00	-200 to 350/350	CP7538	CP7538I5
	30	15.00	-200 to 350/350	CP7544	CP7544I5
	50	50.00	-200 to 350/350	CP7539	

CP-Molsieve 5Å UltiMetal

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage
0.53	10	50.00	-200 to 350/350	CP6937	CP6937I5
	25	50.00	-200 to 350/350	CP6938	CP6938I5

Particle Traps for Use with PLOT Columns

Though highly stabilized, it is impossible to guarantee that no particles will dislodge from the column wall. When used in valve-switching applications, the use of a particle trap can prevent scarring of the rotors.

Particle Traps for Use with PLOT Columns

ID (mm)	Length (m)	Part No.
0.32	2.5	5181-3351
0.53	2.5	5181-3352

Particle Traps for PoraPLOT Columns

ID (mm)	Length (m)	Material	Part No.
0.32	2.5	Fused Silica	CP4016
0.53	2.5	Fused Silica	CP4017
0.53	2.5	UltiMetal	CP4018*

*Includes CP-UltiMetal connector

Particle Trap Connectors for PoraPLOT Columns

ID (mm)	Material	Unit	Part No.
0.25/0.32	Fused Silica	10/pk	CP4788
0.53	Fused Silica	10/pk	CP4789
0.25	UltiMetal	5/pk	CP4795
0.53	UltiMetal	5/pk	CP4796

Columns with Non-Bonded Stationary Phases



Whenever possible Agilent recommends the use of bonded and cross-linked polymers. Bonded polymers are more rugged, will have longer lifetimes and can be solvent rinsed. However, Agilent recognizes that some methods have been developed on non-bonded phases and therefore maintains these columns to support established methods.

HP-101

- 100% Dimethylpolysiloxane

Because HP-101 columns are not bonded or cross-linked, we do not recommend solvent rinsing.

HP-101

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.20	10	0.20	-60 to 280	19091Y-101		
	25	0.20	-60 to 280	19091Y-102		19091Y-102LTM
	50	0.20	-60 to 280	19091Y-105		
	12	0.25	-60 to 280	19091-60010	19091-60010E	
0.32	25	0.30	-60 to 280	19091Y-012	19091Y-012E	19091Y-012LTM
	50	0.30	-60 to 280	19091Y-015		

HP-17

- 50% Phenyl and 50% Methyl siloxane

Because the HP-17 is not bonded or cross-linked, we do not recommend solvent rinsing.

HP-17

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	7890/6890 LTM Module
0.53	10	2.00	25 to 260/280	19095L-121	19095L-121LTM

CAM

- Base deactivated polyethylene glycol
- Specifically designed for amine analysis
- Excellent peak shape for primary amines
- Replaces HP-Basicwax

Because the CAM is not bonded or cross-linked, we do not recommend solvent rinsing.

CAM

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	5 in Cage	7890/6890 LTM Module
0.25	15	0.25	60 to 220/240	112-2112		112-2112LTM
	30	0.25	60 to 220/240	112-2132		112-2132LTM
		0.50	60 to 220/240	112-2133		112-2133LTM
	60	0.25	60 to 220/240	112-2162		
0.32	30	0.25	60 to 220/240	113-2132	113-2132E	113-2132LTM
		0.50	60 to 220/240	113-2133	113-2133E	113-2133LTM
0.53	30	1.00	60 to 200/220	115-2132		115-2132LTM

DX-1 and DX-4

- DX-1: 90% Dimethylpolysiloxane 10% Polyethylene Glycol
- DX-4: 15% Dimethylpolysiloxane 85% Polyethylene Glycol

Because DX series GC columns are not bonded and cross-linked, we do not recommend solvent rinsing.

DX-1

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	7890/6890 LTM Module
0.25	30	1.00	50 to 250/270	122-6133	
0.32	30	1.00	50 to 250/270	123-6133	123-6133LTM

DX-4

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	7890/6890 LTM Module
0.25	30	0.25	50 to 250/270	122-6432	122-6432LTM
	60	0.25	50 to 250/270	122-6462	
0.32	15	0.25	50 to 250/270	123-6412	123-6412LTM
	30	0.25	50 to 250/270	123-6432	123-6432LTM
	60	0.25	50 to 250/270	123-6462	

SE-30 and SE-54

- SE-30: 100% Dimethylpolysiloxane
- SE-54: (5%-Phenyl)(1%-Vinyl)-methylpolysiloxane

Because SE series GC columns are not bonded or cross-linked, we do not recommend solvent rinsing.

SE-30

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	7890/6890 LTM Module
0.32	30	0.25	0 to 325/350	113-3032	113-3032LTM

SE-54

ID (mm)	Length (m)	Film (µm)	Temp Limits (°C)	7 in Cage	7890/6890 LTM Module
0.25	30	0.25	0 to 325/350	112-5432	112-5432LTM
	60	0.25	0 to 325/350	112-5462	
0.32	30	0.25	0 to 325/350	113-5432	113-5432LTM

Guard Columns

- DuraGuard and EZ-Guard columns with "built-in" guard columns, no press-fit connectors
- Minimize front-end contamination and increase column lifetime
- Aid in focusing sample onto the front of the column for better peak shape
- Minimize MSD contamination originating from the column (when used in transfer line)

Guard columns (or retention gaps) are often added to the front of the analytical column to protect against contamination, or to act as a band-focusing device for liquid samples introduced by on-column and splitless injection techniques.

When resolution or response in a chromatogram diminishes, remove a coil from the guard column so that peak shapes will improve. By removing a coil, the column length is shortened and peaks will elute somewhat faster. For best results, check the integration time windows of your data system.

DuraGuard

DuraGuard

Phase	ID (mm)	Length (m)	Film (µm)	Guard Length (m)	Part No.
DB-1	0.25	30	0.25	10	122-1032G
DB-XLB	0.25	30	0.25	10	122-1232G
DB-5ms	0.25	30	0.25	10	122-5532G
			0.50	10	122-5536G
			1.00	10	122-5533G
		60	0.25	10	122-5562G
	0.32	30	1.00	10	123-5533G
	0.53	30	0.50	10	125-5537G
DB-5.625	*0.18*	*20*	*0.36*	*5*	*121-5622G5*
	0.25	*30*	*0.25*	*5*	*122-5631G5*
DB-1701	0.53	30	1.00	10	125-0732G
DB-624	0.53	30	3.00	5	125-1334G5

Agilent J&W High Efficiency GC columns are displayed using italicized descriptions and part numbers

TIPS & TOOLS

Column contamination from sample matrix components is the number one cause of column failure. Use Agilent DuraGuard GC columns with built-in guard if you do not want to use column connectors.



A special tab clearly distinguishes the EZ-Guard guard column section from the analytical column

EZ-Guard

EZ-Guard

Phase	ID (mm)	Length (m)	Film (µm)	Guard Length (m)	Part No.
VF-1ms	0.20	12	0.33	5	CP9023
	0.25	30	0.25	5	CP9010
			0.25	10	CP9011
VF-5ms	0.25	15	0.25	5	CP9021
		30	0.25	5	CP9012
			0.25	10	CP9013
			0.50	5	CP9014
			0.50	10	CP9015
		60	0.25	5	CP9016
	0.53	30	0.25	10	CP9020
VF-Xms	0.25	30	0.10	10	CP9022
			0.25	5	CP9018
			0.25	10	CP9019
VF-17ms	0.25	30	0.25	5	CP9024
			0.25	10	CP9025
VF-1701ms	0.25	30	0.25	5	CP9176
			0.25	10	CP9177
VF-35ms	0.25	30	0.25	5	CP9026
			0.25	10	CP9027

Agilent J&W LTM Column Modules



Agilent J&W LTM Column Modules for 7890 and 6890 Series GC Systems

This groundbreaking column technology is designed specifically for Agilent 7890A and 6890 series gas chromatographs, and delivers:

- The capacity to run up to four column modules simultaneously – with four different temperature programs – to maximize your productivity
- Rapid temperature programming rates of up to 1800 °C/min for higher analysis speeds
- Faster cooling times – as low as one minute or less – to decrease idling and downtime
- Shorter analytical cycle times than conventional air-bath GC oven techniques
- Excellent retention time repeatability and performance – comparable to conventional GC

Most Agilent J&W Capillary GC columns – including Wall Coated Open Tubular (WCOT) and Porous Layer Open Tubular (PLOT) columns – can be used for LTM column modules.



Agilent J&W LTM Column Modules for 5975T Transportable GC/MS Systems

This groundbreaking column technology is designed specifically for Agilent 5975T GC/MS systems. These modules include an integrated 3 in LTM capillary column toroid assembly with heated transfer lines, cooling fan assembly and sheet metal enclosure. Replacement column toroid assemblies are also available. Benefits of the LTM column modules include:

- Faster heating and cooling times – as low as one minute or less – for more rapid analytical cycle times than standard air-bath GC oven techniques
- Excellent retention time repeatability and performance comparable to conventional GC
- Less power consumption for longer in-field operation
- Integrated module design to facilitate easy column module change in the field

TIPS & TOOLS

Agilent LTM column module technology is compatible with metal capillary columns. However, LTM modules are generally not recommended for fast GC applications because of their poor cooling performance compared to fused silica capillaries.



Shorten analytical cycle times and boost your high speed gas chromatography capabilities

Agilent J&W LTM column modules combine a high quality fused silica capillary column with heating and temperature sensing components for a low thermal mass column assembly. The LTM column module contains a patented design which heats and cools the column very efficiently for significantly shorter analytical cycle times compared to conventional air-bath GC oven techniques, while simultaneously using less power.

Agilent offers LTM technology for our popular 7890 and 6890 Series GC systems, as well as the new 5875T GC/MS. Compatible with Agilent LTM and LTM II series GC systems and retrofit upgrades.

All LTM column modules are packaged with:

- Two 1 m guard columns (one each for the inlet and detector) made from deactivated fused silica tubing of the same id as the analytical column
- Five non-reusable ferrules that fit the dimensions of the analytical and guard columns

For more information, visit **www.agilent.com/chem/LTMcol**

TIPS & TOOLS

LTM column modules should never be programmed beyond the GC column temperature limits recommended by Agilent. For very fast ramping applications (e.g. 600 °C/min), limiting the maximum temperatures to 10-20 °C below the GC column temperature limits can increase the lifetime of the column modules.

Agilent J&W LTM Column Modules for 5975T Transportable GC/MS Systems

Phase	ID (mm)	Length (m)	Film (µm)	Toroid Assembly	Column Module
DB-5ms Ultra Inert	0.18	20	0.18	221-5522UILTM	G3900-63014
	0.25	15	0.25	222-5512UILTM	G3900-63031
		30	0.25	222-5532UILTM	G3900-63005
HP-5ms Ultra Inert	0.18	20	0.18	29091S-577UILTM	G3900-63039
	0.25	15	0.25	29091S-431UILTM	G3900-63038
		30	0.25	29091S-433UILTM	G3900-63001
DB-1	0.25	30	0.25	222-1032LTM	G3900-63002
DB-1ms	0.18	20	0.18	221-0122LTM	G3900-63009
	0.25	15	0.25	222-0112LTM	G3900-63016
		30	0.25	222-0132LTM	G3900-63017
DB-1ht	0.25	15	0.10	222-1111LTM	G3900-63018
		30	0.10	222-1131LTM	G3900-63019
HP-1ms	0.18	20	0.18	29091S-677LTM	G3900-63040
	0.25	30	0.10	29091S-833LTM	G3900-63041
		15	0.25	29091S-931LTM	G3900-63042
DB-5ms	0.18	20	0.18	221-5522LTM	G3900-63013
	0.25	15	0.25	222-5512LTM	G3900-63030
		30	0.25	222-5532LTM	G3900-63004
DB-5ht	0.25	15	0.10	222-5731LTM	G3900-63033
		30	0.10	222-5711LTM	G3900-63032





(Continued)



Agilent J&W LTM Column Modules for 5975T Transportable GC/MS Systems

Phase	ID (mm)	Length (m)	Film (µm)	Toroid Assembly	Column Module
HP-5ms	0.25	30	0.25	29091S-433LTM	G3900-63007
DB-35ms	0.18	20	0.18	221-3822LTM	G3900-63011
	0.25	15	0.25	222-3812LTM	G3900-63026
		30	0.25	222-3832LTM	G3900-63027
DB-17ms	0.18	20	0.18	221-4722LTM	G3900-63012
	0.25	15	0.25	222-4712LTM	G3900-63028
		30	0.25	222-4732LTM	G3900-63029
DB-225ms	0.25	15	0.25	222-2912LTM	G3900-63022
		30	0.25	222-2932LTM	G3900-63023
DB-1701	0.25	30	0.25	222-0732LTM	G3900-63003
DB-WAX	0.25	15	0.50	222-7013LTM	G3900-63034
		30	0.50	222-7033LTM	G3900-63035
HP-INNOWax	0.18	20	0.18	29091N-577LTM	G3900-63036
	0.25	30	0.25	29091N-133LTM	G3900-63008
DB-FFAP	0.25	15	0.25	222-3212LTM	G3900-63024
		30	0.25	222-3232LTM	G3900-63025
DB-608	0.18	20	0.18	221-6822LTM	G3900-63015
DB-VRX	0.18	20	1.00	221-1524LTM	G3900-63006
	0.25	30	1.40	222-1534LTM	G3900-63021
DB-624	0.18	20	1.00	221-1324LTM	G3900-63010
	0.25	30	1.40	222-1334LTM	G3900-63020
HP-VOC	0.20	30	1.12	29091R-303LTM	G3900-63037

Fused Silica Tubing

Deactivated Tubing

Deactivated tubing can be used as retention gaps, guard columns, or transfer lines. Our standard deactivation process is a phenyl methyl deactivation – the preferred choice for most applications due to its inertness and robustness.

Deactivated Fused Silica

ID (mm)	OD (mm)	Length (m)	Part No.
0.05	0.36	1	160-2655-1
		5	160-2655-5
		10	160-2655-10
0.10	0.19	1	160-1010-1
		5	160-1010-5
		10	160-1010-10
	0.36	1	160-2635-1
		5	160-2635-5
		5	19091-60620E
		10	160-2635-10
0.15	0.36	1	160-2625-1
		5	160-2625-5
		10	160-2625-10
0.18	0.34	1	160-2615-1
		5	160-2615-5
		10	160-2615-10
0.20	0.36	1	160-2205-1
		5	160-2205-5
		10	160-2205-10

(Continued)

Deactivated Fused Silica

ID (mm)	OD (mm)	Length (m)	Part No.
0.25	0.36	1	160-2255-1
		5	160-2255-5
		10	160-2255-10
		30	160-2255-30
0.32	0.43	1	160-2325-1
		5	160-2325-5
		10	160-2325-10
		30	160-2325-30
0.45	0.67	1	160-2455-1
		5	160-2455-5
		10	160-2455-10
0.53	0.67	1	160-2535-1
		5	160-2535-5
		10	160-2535-10
		30	160-2535-30

Deactivated Fused Silica High Temperature (400 °C)

ID (mm)	OD (mm)	Length (m)	Part No.
0.05	0.36	5	160-2815-5
0.10	0.36	5	160-2825-5
0.25	0.35	5	160-2845-5
		10	160-2845-10
0.32	0.43	5	160-2855-5
		10	160-2855-10
0.53	0.67	5	160-2865-5
		10	160-2865-10

ProSteel Deactivated Fused Silica

ID (mm)	OD (mm)	Length (m)	Part No.
0.53	0.67	5	160-4535-5

Undeactivated Fused Silica

Undeactivated tubing or bare fused silica is commonly used for capillary electrophoresis. It can also be used for transfer lines and other applications where inertness is not critical.

Undeactivated Fused Silica

ID (mm)	OD (mm)	Length (m)	Part No.
0.02	0.36	5	160-2660-5
0.05	0.36	5	160-2650-5
		10	160-2650-10
0.075	0.36	5	160-2644-5
		10	160-2644-10
0.10	0.36	5	160-2634-5
		10	160-2634-10
0.18	0.34	5	160-2610-5
		10	160-2610-10
0.20	0.36	5	160-2200-5
		10	160-2200-10
		50	19091-20050
0.25	0.36	5	160-2250-5
		10	160-2250-10
0.32	0.43	5	160-2320-5
		10	160-2320-10
		50	19091-21050
0.45	0.67	5	160-2450-5
		10	160-2450-10
0.53	0.67	5	160-2530-5
		10	160-2530-10

Agilent J&W Packed GC Columns



Agilent J&W Packed GC Columns are designed and manufactured to offer excellent and reproducible performance for all sample types associated with packed column separations, most important in the hydrocarbon processing industry.

The highly efficient and rigorous packing technology used in Agilent J&W Packed GC Columns assures column-to-column reproducibility and ultimate efficiency, while the UltiMetal treated stainless steel tubing allows for improved inertness and peak shape performance.

You can choose from a wide range of tubing materials – including stainless steel, UltiMetal, nickel, glass, copper and PTFE – plus hundreds of stationary phases, packings, and supports.

And, you can create your custom configurations by visiting
www.agilent.com/chem/packedcolumnsordering

Agilent J&W Packed GC Columns for Agilent 7820, 7890, and 6890 Instruments

Carbosieve S

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
20 in (0.51 m)	1/8	2	80/100	G3591-80105	G3591-81105	G3591-82105

15% Carbowax 1540

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
15 ft (4.57 m)	1/8	2	Chromosorb WHP	60/80	G3591-80095	G3591-81095	G3591-82095

5% Carbowax 20M (G16, G$1)

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
7.22 ft (2.2 m)	1/8	2	Chromosorb WHP	100/120	G3591-80084	G3591-81084	G3591-82084

20% Carbowax 20M (G16, G$1)

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
9.84 ft (3 m)	1/8	2	Chromosorb WHP	100/120	G3591-80099	G3591-81099	G3591-82099

7% Carbowax M + 3% Polyphenolether 6 ring + 2% KOH

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
4 ft (1.22 m)	1/8	2	Chromosorb W AW	80/100	G3591-80050	G3591-81050	G3591-82050

Carboxen-1000

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
1.5 ft (0.46 m)	1/8	2	80/100	G3591-80125	G3591-81125	G3591-82125
10 ft (3.05 m)	1/8	2	60/80	G3591-80055	G3591-81055	G3591-82055

Chromosorb 101

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
6 ft (1.83 m)	1/8	2	80/100	G3591-80021	G3591-81021	G3591-82021

Chromosorb 102

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
2 ft (0.61 m)	1/8	2	80/100	G3591-80139	G3591-81139	G3591-82139

25% DC-200

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
15 ft (4.57 m)	1/8	2	Chromosorb PAW	80/100	G3591-80001	G3591-81001	G3591-82001

30% DC-200

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
20 ft (6.1 m)	1/8	2	Chromosorb PAW	100/120	G3591-80140	G3591-81140	G3591-82140
30 ft (9.14 m)	1/8	2	Chromosorb PAW	80/100	G3591-80082	G3591-81082	G3591-82082

35% DC-200

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
10 ft (3.05 m)	1/8	2	Chromosorb PAW	80/100	G3591-80030	G3591-81140	G3591-82030
30 ft (9.14 m)	1/8	2	Chromosorb PAW	80/100	G3591-80032	G3591-81032	G3591-82032
3 ft (0.91 m)	1/8	2	Chromosorb PAW	80/100	G3591-80039	G3591-81039	G3591-82039
5 ft (1.52 m)	1/8	2	Chromosorb PAW	80/100	G3591-80027	G3591-81027	G3591-82027

15% Hallcomid m-18

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
9.84 ft (3 m)	1/8	2	Chromosorb WHP	100/120	G3591-80067	G3591-81067	G3591-82067

30% DC 200/500

Length	OD (in)	ID (mm)	Support	Mesh	UltiMetal	Nickel	Stainless Steel
30 ft (9.14 m)	1/8	2	Chromosorb PAW	68/80			G3591-80161
2 ft (0.61 m)	1/8	2	Chromosorb PAW	60/80			G3591-80160
30 ft (9.14 m)	1/8	2	Chromosorb PAW	60/80		G3591-82161	
2 ft (0.61 m)	1/8	2	Chromosorb PAW	60/80		G3591-82160	
2 ft (0.61 m)	1/8	2	Chromosorb PAW	60/80	G3591-81160		
30 ft (9.14 m)	1/8	2	Chromosorb PAW	60/80	G3591-81161		

HayeSep D

Length	OD (in)	ID (mm)	Mesh	Stainless Steel
6.56 ft (2 m)	1/8	2	80/100	G3591-80158

HayeSep DB

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
30 ft (9.14 m)	1/8	2	100/120	G3591-80088	G3591-81088	G3591-82088

HayeSep N

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
6 ft (1.83 m)	1/8	2	80/100	G3591-80037	G3591-81037	G3591-82037
7 ft (2.13 m)	1/8	2	60/80	G3591-80060	G3591-81060	G3591-82060
8 ft (2.44 m)	1/8	2	80/100	G3591-80011	G3591-81011	G3591-82011
20 ft (6.1 m)	1/8	2	80/100	G3591-80045	G3591-81045	G3591-82045

HayeSep N + HayeSep R 1:1

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
8 ft (2.44 m)	1/8	2	45/60	G3591-80091	G3591-81091	G3591-82091

HayeSep Q

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
1.64 ft (0.5 m)	1/8	2	80/100	G3591-80023	G3591-81023	G3591-82023
3 ft (0.91 m)	1/8	2	80/100	G3591-80020	G3591-81020	G3591-82020
3.3 ft (1 m)	1/8	2	80/100		G3591-81148	
3.9 ft (1.2 m)	1/8	2	80/100			G3591-82159
4 ft (1.22 m)	1/8	2	80/100	G3591-80019	G3591-81019	G3591-82019
6 ft (1.83 m)	1/8	2	80/100	G3591-80004	G3591-81004	G3591-82004
8 ft (2.44 m)	1/8	2	80/100	G3591-80047	G3591-81047	G3591-82047
9 ft (2.74 m)	1/8	2	80/100	G3591-80033	G3591-81033	G3591-82033
10 ft (3.05 m)	1/8	2	80/100	G3591-80002	G3591-81002	G3591-82002
12 ft (3.66 m)	1/8	2	80/100	G3591-80121	G3591-81121	G3591-82121
5.91 ft (1.8 m)	1/8	2	80/100	G3591-70011		
3.28 ft (1 m)	1/8	2	80/100	G3591-70007		
6.56 ft (2 m)	1/8	2	80/100	G3591-70005		
9.84 ft (3 m)	1/8	2	80/100	G3591-70006		

HayeSep R

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
6 ft (1.83 m)	1/8	2	80/100	G3591-80102	G3591-81102	G3591-82102
12 ft (3.66 m)	1/8	2	80/100	G3591-80100	G3591-81100	G3591-82100

HayeSep T

Length	OD (in)	ID (mm)	Mesh	UltiMetal	PTFE
1.64 ft (0.5 m)	1/8	2	80/100	G3591-81150	
1.64 ft (0.5 m)	1/8	2	60/80		G3591-74001

TIPS & TOOLS

To learn more about Agilent J&W Packed GC Columns please visit **www.agilent.com/chem/packedcolumns.**



MolSieve 5Å

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
1 ft (0.30 m)	1/8	2	60/80	G3591-80077	G3591-81077	G3591-82077
3 ft (0.91 m)	1/8	2	60/80	G3591-80103	G3591-81103	G3591-82103
3 ft (0.91 m)	1/8	2	80/100	G3591-80074	G3591-81074	G3591-82074
3 ft (0.91 m)	1/8	2	100/120	G3591-80075	G3591-81075	G3591-82075
3.3 ft (1 m)	1/8	2	60/80		G3591-81149	
4 ft (1.22 m)	1/8	2	45/60	G3591-80090	G3591-81090	G3591-82090
6 ft (1.83 m)	1/8	2	60/80	G3591-80035	G3591-81035	G3591-82035
4 ft (1.22 m)	1/8	2	60/80	G3591-80104	G3591-81104	G3591-82104
6 ft (1.83 m)	1/8	2	60/80	G3591-80017	G3591-81017	G3591-82017
7 ft (2.13 m)	1/8	2	45/60	G3591-80062	G3591-81062	G3591-82062
8 ft (2.44 m)	1/8	2	60/80	G3591-80022	G3591-81022	G3591-82022
9 ft (2.74 m)	1/8	2	60/80	G3591-80046	G3591-81046	G3591-82046
9 ft (2.74 m)	1/8	2	80/100	G3591-80064	G3591-81064	G3591-82064
15 ft (4.57 m)	1/8	2	45/60	G3591-80061	G3591-81061	G3591-82061
20 ft (6.1 m)	1/8	2	45/60	G3591-80107		
20 ft (6.1 m)	1/8	2	60/80	G3591-80056	G3591-81056	G3591-82056
25 ft (7.62 m)	1/8	2	60/80	G3591-80065	G3591-81065	G3591-82065
6.56 ft (2 m)	1/8	2	45/60	G3591-70013		
3.28 ft (1 m)	1/8	2	80/100	G3591-70008		
1.97 ft (0.6 m)	1/4	2	80/100	G3591-70004		
6.56 ft (2 m)	1/8	2	80/100	G3591-70003		
6.56 ft (2 m)	1/8	2	60/80	G3591-70002		

MolSieve 13X

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
2 ft (0.61 m)	1/8	2	45/60	G3591-80031	G3591-81031	G3591-82031
3 ft (0.91 m)	1/8	2	45/60	G3591-80028	G3591-81028	G3591-82028
4 ft (1.22 m)	1/8	2	45/60	G3591-80012	G3591-81012	G3591-82012
4.9 ft (1.5 m)	1/8	2	80/100	G3591-80085	G3591-81085	G3591-82085
6 ft (1.83 m)	1/8	2	60/80	G3591-80035	G3591-81035	G3591-82035
9 ft (2.74 m)	1/8	2	45/60	G3591-80054	G3591-81054	G3591-82054
10 ft (3.05 m)	1/8	2	46/60	G3591-80003	G3591-81003	G3591-82003
10 ft (3.05 m)	1/16	1	60/80	G3591-80097	G3591-81097	G3591-82097
10 ft (3.05 m)	1/8	2	60/80	G3591-80101	G3591-81101	G3591-82101
10 ft (3.05 m)	1/8	2	80/100	G3591-80043	G3591-81043	G3591-82043
12 ft (3.66 m)	1/8	2	60/80	G3591-80058	G3591-81058	G3591-82058
15 ft (4.57 m)	1/8	2	45/60	G3591-80098	G3591-81098	G3591-82098
9.84 ft (3 m)	1/8	2	45/60	G3591-70017		
9.84 ft (3 m)	1/8	2	80/100	G3591-70015		

1.5% OV-101

Length	OD (in)	ID (mm)	Support	Mesh	UltiMetal	Nickel	Stainless Steel
2 ft (0.61 m)	1/8	2	Chromosorb GHP	100/120			G3591-80162
2 ft (0.61 m)	1/8	2	Chromosorb GHP	100/120		G3591-82162	
2 ft (0.61 m)	1/8	2	Chromosorb GHP	100/120	G3591-81162		

10% OV-101

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
2.6 ft (0.79 m)	1/8	2	Chromosorb WHP	60/80	G3591-80048	G3591-81048	G3591-82048
5 ft (1.52 m)	1/8	2	Chromosorb PAW	80/100	G3591-80093	G3591-81093	G3591-82093

20% OV-101

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
4 ft (1.22 m)	1/8	2	Chromosorb WHP	80/100	G3591-80025	G3591-81025	G3591-82025

10% PEG-20M

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
6.56 ft (2 m)	1/8	2	Chromosorb W	80/100	G3591-80119	G3591-81119	G3591-82119

20% PEG-20M

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
6.56 ft (2 m)	1/8	2	Chromosorb W	80/100	G3591-80122	G3591-81122	G3591-82122
13.1 ft (4 m)	1/8	2	Chromosorb W	80/100	G3591-80123	G3591-81123	G3591-82123

Porapak N

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
3 ft (0.91 m)	1/8	2	80/100	G3591-80072	G3591-81072	G3591-82072
3.9 ft (1.2 m)	1/8	2	60/80	G3591-80087	G3591-81087	G3591-82087
6 ft (1.83 m)	1/8	2	80/100	G3591-80036	G3591-81036	G3591-82036
8.2 ft (2.5 m)	1/8	2	50/80	G3591-80086	G3591-81086	G3591-82086
9 ft (2.74 m)	1/8	2	80/100	G3591-80044	G3591-81044	G3591-82044
12 ft (3.66 m)	1/8	2	60/80	G3591-80059	G3591-81059	G3591-82059

Porapak N + Porapak R 1:1

Length	OD (in)	ID (mm)	Mesh	Stainless Steel
12 ft (3.66 m)	1/8	2	50/80	G3591-80110

Porapak Q

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
3 ft (0.91 m)	1/8	2	80/100	G3591-80135	G3591-81135	G3591-82135
6 ft (1.83 m)	1/8	2	60/80	G3591-80136	G3591-81136	G3591-82136
6 ft (1.83 m)	1/8	2	80/100	G3591-80005	G3591-81005	G3591-82005
6 ft (1.83 m)	1/8	2	80/100	G3591-80013	G3591-81013	G3591-82013
8 ft (2.44 m)	1/8	2	60/80	G3591-80137	G3591-81137	G3591-82137
8.2 ft (2.5 m)	1/8	2	80/100	G3591-80083	G3591-81083	G3591-82083
9 ft (2.74 m)	1/8	2	80/100	G3591-80016	G3591-81016	G3591-82016
13 ft (3.96 m)	1/8	2	80/100	G3591-80053	G3591-81053	G3591-82053
15 ft (4.57 m)	1/8	2	80/100	G3591-80066	G3591-81066	G3591-82066
25 ft (7.62 m)	1/8	2	100/120	G3591-80052	G3591-81052	G3591-82052
30 ft (9.14 m)	1/16	1	80/100	G3591-80096	G3591-81096	G3591-82096
3.28 ft (1 m)	1/8	2	80/100	G3591-70014		
5.91 ft (1.8 m)	1/8	2	80/100	G3591-70010		
9.84 ft (3 m)	1/8	2	80/100	G3591-70009		
6.56 ft (2 m)	1/8	2	80/100	G3591-70001		
4.92 ft (1.5 m)	1/8	2	50/80	G3591-70018		

Porapak QS

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
6.56 ft (2 m)	1/8	2	80/100	G3591-80157		
8 ft (2.44 m)	1/8	2	80/100	G3591-80051	G3591-81051	G3591-82051
5.91 ft (1.8 m)	1/8	2	80/100	G3591-70010		
9.84 ft (3 m)	1/8	2	80/100	G3591-70009		

Porapak R

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
6 ft (1.83 m)	1/8	2	60/80	G3591-80106	G3591-81106	G3591-82106

Porapak T

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
1.5 ft (0.46 m)	1/8	2	80/100	G3591-80138	G3591-81138	G3591-82138
6.56 ft (2 m)	1/8	2	80/100	G3591-80120	G3591-81120	G3591-82120

20% Sebaconitrile

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
2 ft (0.61 m)	1/8	2	Chromosorb PAW	80/100	G3591-80029	G3591-81029	G3591-82029
19.7 ft (6 m)	1/8	2	Chromosorb PAW	80/100	G3591-80071	G3591-81071	G3591-82071
30 ft (9.14 m)	1/8	2	Chromosorb PAW	80/100	G3591-80026	G3591-81026	G3591-82026

20% Sebaconitrile/2% H_3PO_4

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
2 ft (0.61 m)	1/8	2	Chromosorb PAW	80/100	G3591-80015	G3591-81015	G3591-82015
30 ft (9.14 m)	1/8	2	Chromosorb PAW	80/100	G3591-80014	G3591-81014	G3591-82014

Silica Gel

Length	OD (in)	ID (mm)	Mesh	Stainless Steel	UltiMetal	Nickel
2 ft (0.61 m)	1/8	2	60/80	G3591-80141	G3591-81141	G3591-82141
4 ft (1.22 m)	1/8	2	60/80	G3591-80142	G3591-81142	G3591-82142
6 ft (1.83 m)	1/8	2	60/80	G3591-80108		

0.1% SP-1000

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
7 ft (2.13 m)	1/8	2	Carbopak C	80/100	G3591-80063	G3591-81063	G3591-82063

25% SP-2100

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
1.64 ft (0.5 m)	1/16	1	Chromosorb PAW	80/100	G3591-80007	G3591-81007	G3591-82007
5.7 ft (1.75 m)	1/16	1	Chromosorb PAW	80/100	G3591-80008	G3591-81008	G3591-82008
15 ft (4.57 m)	1/8	2	Chromosorb PAW	80/100	G3591-80068	G3591-81068	G3591-82068

20% TCEP

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
1.84 ft (0.56 m)	1/16	1	Chromosorb PAW	80/100	G3591-80006	G3591-81006	G3591-82006
5 ft (1.52 m)	1/8	2	Chromosorb PAW	80/100	G3591-80094	G3591-81094	G3591-82094
15 ft (4.57 m)	1/8	2	Chromosorb PAW	80/100	G3591-80049	G3591-81049	G3591-82049

10% UC W982

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
1.5 ft (0.46 m)	1/8	2	Chromosorb PAW	80/100	G3591-80034	G3591-81034	G3591-82034
2 ft (0.61 m)	1/8	2	Chromosorb PAW	80/100	G3591-80040	G3591-81040	G3591-82040

12% UC W982

Length	OD (in)	ID (mm)	Support	Mesh	Stainless Steel	UltiMetal	Nickel
2 ft (0.61 m)	1/8	2	Chromosorb PAW	80/100	G3591-80000	G3591-81000	G3591-82000

Agilent J&W Packed GC Columns for All Instruments

30% DC 200/500

Length	OD (in)	ID (mm)	Support	Mesh	UltiMetal
2 ft (0.61 m)	1/8	2	Chromosorb PAW	60/80	CP2057
30 ft (9.14 m)	1/8	2	Chromosorb PAW	60/80	CP2058*

*Preconditioned and pretested

HayeSep D

Length	OD (in)	ID (mm)	Mesh	UltiMetal
6.56 ft (2 m)	1/8	2	80/100	CP1482

HayeSep DB

Length	OD (in)	ID (mm)	Mesh	UltiMetal
40 ft (12.2 m)	1/8	2	80/100	CP2047

HayeSep N

Length	OD (in)	ID (mm)	Mesh	UltiMetal
1.64 ft (0.5 m)	1/16	1	80/100	CP1307*
1.64 ft (0.5 m)	1/8	2	80/100	CP1480
6 ft (1.83 m)	1/8	2	80/100	CP2068*

*Preconditioned and pretested

HayeSep P

Length	OD (in)	ID (mm)	Mesh	UltiMetal
6 ft (1.83 m)	1/8	2	80/100	CP2062

HayeSep Q

Length	OD (in)	ID (mm)	Mesh	UltiMetal
0.82 ft (0.25 m)	1/16	1	80/100	CP1308*
1.64 ft (0.5 m)	1/8	2	80/100	CP81073*
3.28 ft (1 m)	1/8	2	80/100	CP81069*
4.92 ft (1.5 m)	1/16	1	80/100	CP1305*

*Preconditioned and pretested

HayeSep R

Length	OD (in)	ID (mm)	Mesh	UltiMetal
3.28 ft (1 m)	1/8	2	80/100	CP86678*
8.53 ft (2.6 m)	1/8	2	80/100	CP86677*
12 ft (3.66 m)	1/8	2	80/100	CP2055*

*Preconditioned and pretested

MolSieve 5Å

Length	OD (in)	ID (mm)	Mesh	UltiMetal
3.28 ft (1 m)	1/8	2	60/80	CP81025*
4.92 ft (1.5 m)	1/16	1	80/100	CP1306*
5 ft (1.52 m)	1/8	2	80/100	CP2046
6 ft (1.83 m)	1/8	2	45/60	CP2065
10 ft (3.05 m)	1/8	2	80/100	CP2045
13.1 ft (4 m)	1/8	2	80/100	CP1483*

*Preconditioned and pretested

MolSieve 13X

Length	OD (in)	ID (mm)	Mesh	UltiMetal
3 ft (0.91 m)	1/8	2	45/60	CP2059*
3.94 ft (1.2 m)	1/16	1	80/100	CP1309*
4 ft (1.22 m)	1/8	2	45/60	CP2060
4.92 ft (1.5 m)	1/8	2	80/100	CP81071*

*Preconditioned and pretested

1.5% OV-101

Length	OD (in)	ID (mm)	Support	Mesh	UltiMetal
2 ft (0.61 m)	1/8	2	Chromosorb G HP	100/120	CP2056

Porapak QS

Length	OD (in)	ID (mm)	Mesh	UltiMetal
6.56 ft (2 m)	1/8	2	80/100	CP1481

10% SE-30

Length	OD (in)	ID (mm)	Mesh	UltiMetal
2.5 ft (0.76 m)	1/8	2	80/100	CP2073

Silica Gel

Length	OD (in)	ID (mm)	Mesh	UltiMetal
10 ft (3.05 m)	1/8	2	60/80	CP2050

20% TCEP

Length	OD (in)	ID (mm)	Mesh	UltiMetal
1.84 ft (0.56 m)	1/16	0.75	80/100	CP2071
15 ft (4.57 m)	1/8	2	80/100	CP2072



Custom GC Column Ordering

Even though we offer over a thousand readily available columns, Agilent recognizes that sometimes you need something a little out of the ordinary. That's why we developed our Custom Column Shop. If you can't find what you're looking for in our standard order guides, we will design, build, and test capillary GC columns to meet your needs.

- We can create columns with non-standard lengths or unusual film thickness.
- We can connect columns together in series or as dual columns.
- We recognize that sometimes customers have specific column performance requirements for their applications that might not be met with standard test mixes. As a result, we can also custom-test your columns with your desired test mixture and test conditions to meet specific performance requirements.
- We can create DuraGuard or EZ-Guard columns with an integrated guard column (retention gap). Most phases can be manufactured with a built-in guard column, which means you get the advantages of a guard column without the union. Available in DB, CP and VF phases.

Custom columns are ordered using the P/Ns below. Be sure to provide the details of your desired custom service or column including phase, length, id, and film thickness.

- 100-2000 Custom Capillary DB & HP columns
- 100-6000 Custom Capillary CP & VF columns
- 100-9000 UltiMetal treated tubing and parts
- 100-2000 LTM – Custom Low Thermal Mass column configurations
- 100-5000 Custom packed columns or bulk phases/supports

Contact your local Agilent office or Authorized Agilent Distributor to receive a quote for your custom column needs. You can find order forms in the back of Agilent's Essential Chromatography Catalog.

Customers in the United States, Canada, and Puerto Rico can request a custom column quote online at **www.agilent.com/chem/CustomColumn**

Agilent J&W GC Column Test Standards

Compare your column's performance to the test chromatogram shipped with your Agilent J&W column. The column test standard contains components that test the column for resolution characteristics, efficiency, and inertness. The test mixes are supplied at a concentration of 250 ng/µL in 2 mL vials. Match the phase and column diameter in the chart below to find the test mix for your column.

Agilent J&W GC Column Test Standards

Column Description	Microbore (0.05 & 0.10 mm ID) Part No.	Capillary (0.18 & 0.32 mm ID) Part No.	Megabore (0.45 & 0.53 mm ID) Part No.
OV-351		200-0032	
DB-1ht		200-0010	
DB-1	200-0010	200-0310	200-0110
DB-5	200-0010	200-0310	200-0110
DB-5ht		200-0010	
DB-5ms		200-0185	200-0185
DB-624		200-0113	200-0113
DB-2887			200-0110
DB-WAX	200-0070	200-0370	200-0070
DB-WAXetr		200-0370	200-0070
SE-30		200-0010	
SE-52		200-0010	
SE-54		200-0010	200-0010
HP-1		5080-8858	8500-6812
HP-5		5080-8858	8500-6812
HP-FFAP	8500-6813	8500-6813	8500-6813
GS-OxyPLOT			5188-5379

Test Standards for Agilent J&W CP and VF Columns

Test Mix 31 Hazardous, 1/pk	Part No.
VF-1ms	CP0031
VF-5ms	CP0031
VF-17ms	CP0031
VF-35ms	CP0031
VF-Xms	CP0031
VF-1301ms	CP0031
VF-200ms	CP0031
VF Rapid-MS	CP0031
CP-Sil 5 CB	CP0031
CP-Sil 8 CB	CP0031
CP-Sil 24 CB	CP0031
CP-1301	CP0031
Test Mix 5, 1/pk	**Part No.**
CP-Sil 43 CB	CP0005

TIPS & TOOLS

Ensure highest quality gas while keeping gas lines clean and leak-free with Agilent's high-capacity gas filter. Learn more at **www.agilent.com/chem/gasclean**



Column Installation and Troubleshooting



Quick reference guides and tips to ensure peak performance

Agilent J&W GC columns are backed by decades of chromatography experience, so you can count on superior quality and dependability. And you can help ensure maximum performance, efficiency, and column life by implementing the most current installation and troubleshooting procedures.

In this section, you'll discover tips, techniques, and easy-reference guides that will help you:

- Confidently install any capillary column
- Condition and test new columns
- Alleviate and avoid column performance degradation due to thermal damage, oxygen damage, and other factors
- Pinpoint and fix the most common column problems

So you'll expand your hours of continuous operation, decrease downtime, and get the reproducible results that your lab demands.

Capillary Column Installation Quick Reference Guide

For more detailed installation information, refer to the GC Column Installation Guide which is provided with your column, or visit **www.agilent.com/chem/columninstall**

Precolumn Installation Check List

1. Replace oxygen, moisture, and hydrocarbon traps as needed.
2. Clean the injection port, replace critical injection port seals, replace injection port liners, and change septa as needed.
3. Check detector seals, and replace as necessary. Clean or replace detector jets as necessary.
4. Carefully inspect the column for damage or breakage.
5. Check your GC manufacturer's gas pressure requirements and verify gas cylinder delivery pressures to ensure that an adequate supply of carrier, makeup, and fuel gases are available. Minimum recommended carrier gas purity percentages are: Helium 99.995% and Hydrogen 99.995%, with H_20 < 1ppm and O_2 < 0.5ppm.
6. Gather the necessary installation tools: You will need a column cutter, column nuts, column nut wrench, ferrules, a magnifying loupe, and typewriter correction fluid.

Table 6:

Ferrule Sizes

Column ID	Ferrule ID (mm)
0.10	0.4
0.18	0.4
0.20	0.4
0.25	0.4
0.32	0.5
0.45	0.8
0.53	0.8

Installing the Column

1. Uncoil approximately 0.5 m of tubing (1 coil ~ 0.5 m) from the column basket at both ends of the column for injector and detector installation. Avoid using sharp bends in the tubing.
2. Mount the column in the oven. Use a handling bracket if available.
3. Install the column nut and Graphite/Vespel or Graphite ferrule at each column end; pull the nut and ferrule down the tubing approximately 15 cm. (**Table 6**)
4. Score (scratch) the column. Use a light touch to score the column about 4 to 5 cm from each end.

Installing the Column



5. Make a clean break. Grasp the column between the thumb and forefinger as close to the score point as possible. Gently pull and bend the column. The column should part easily. If the column does not break easily, do not force it. Score the column again in a different place (farther from the end than before) and try again for a clean break.
6. Use a magnifying loupe to inspect the cut. Make sure the cut is square across the tubing with no polyimide or "glass" fragments at the end of the tube.
7. Install the column in the inlet. Check the GC manufacturer's instrument manual for the correct insertion distance in the injection port type being used. Slide the column nut and ferrule to the proper distance and then mark the correct distance on the column with typewriter correction fluid just behind the column nut. Allow the fluid to dry. Insert the column into the injector. Finger tighten the column nut until it starts to grab the column, and then tighten the nut an additional 1/4 to 1/2 turn, so that the column cannot be pulled from the fitting when gentle pressure is applied. Verify that the correct column insertion distance has been maintained by looking at the typewriter correction fluid mark.
8. Turn on the carrier gas and establish the proper flow rate. Set head pressure, split flow, and septum purge flow to appropriate levels. See **Table 7** for nominal head pressures. If fusing a split/splitless inlet, check that the purge (split) valve is "on" (open).
9. Confirm carrier gas flow through the column. Immerse the end of the column in a vial of solvent and check for bubbles.
10. Install the column into the detector. Check the instrument manufacturer's manual for the proper insertion distance.
11. Check for leaks. **This is very important.** Do not heat the column without thoroughly checking for leaks.
12. Establish proper injector and detector temperatures.
13. Establish proper makeup and detector gas flows. Ignite or turn "on" the detector.
14. Purge the column for a minimum of 10 min at ambient temperature. Add the appropriate additional purge time following inlet or trap maintenance.
15. Inject non-retained substance to check for proper injector installation. Examples: butane or methane (FID), headspace vapors from Acetonitrile (NPD), headspace vapors from methylene chloride (ECD), air (TCD), argon (mass spectrometer). Proper installation is indicated by a symmetrical non-retained peak. If tailing is observed, reinstall the column into the inlet.

TIPS & TOOLS

Learn more about Agilent's top-ranked service and support at **www.agilent.com/chem/services**

Conditioning and Testing the Column

1. Set oven temperature 20 °C above the maximum temperature of the analysis or at the maximum temperature of the column (whichever is lower) for 2 hours. If after 10 min at the upper temperature the background does not begin to fall, immediately cool the column and check for leaks.
2. If you are using Vespel or Graphite/Vespel ferrules, recheck column nut tightness after the conditioning process.
3. Confirm final proper average linear velocity by injecting a non-retained substance again.

Table 7:

Approximate Head Pressures (psig)						
	Column ID (mm)					
Column Length (m)	**0.18**	**0.2**	**0.25**	**0.32**	**0.45**	**0.53**
10	5-10					
12		10-15				
15			8-12	5-10		1-2
20	10-20					
25		20-30				
30			15-25	10-20	3-5	2-4
40	20-40					
50		40-60				
60			30-45	20-30	6-10	4-8
75					8-14	5-10
105						7-15

Causes of Column Performance Degradation

Column Breakage

Fused silica columns break wherever there is a weak point in the polymide coating. The polymide coating protects the fragile but flexible fused silica tubing. The continuous heating and cooling of the oven, vibrations caused by the oven fan, and being wound on a circular cage all place stress on the tubing. Eventually breakage occurs at a weak point. Weak spots are created where the polymide coating is scratched or abraded. This usually occurs when a sharp point or edge is dragged over the tubing. Column hangers and tags, metal edges in the GC oven, column cutters, and miscellaneous items on the lab bench are just some of the common sources of sharp edges or points.

It is rare for a column to spontaneously break. Column manufacturing practices tend to expose any weak tubing and eliminate it from use in finished columns. Larger diameter columns are more prone to breakage. This means that greater care and prevention against breakage must be taken with 0.45-0.53 mm id tubing than with 0.18-0.32 mm id tubing.

A broken column is not always fatal. If a broken column was maintained at a high temperature either continuously or with multiple temperature program runs, damage to the column is very likely. The back half of the broken column has been exposed to oxygen at elevated temperatures which rapidly damages the stationary phase. The front half is fine since carrier gas flowed through this length of column. If a broken column has not been heated or only exposed to high temperatures or oxygen for a very short time, the back half has probably not suffered any significant damage.

A union can be installed to repair a broken column. Any suitable union will work to rejoin the column. Problems with dead volume (peak tailing) may occur with improperly installed unions.



Thermal Damage

Exceeding a column's upper temperature limit results in accelerated degradation of the stationary phase and tubing surface. This results in the premature onset of excessive column bleed, peak tailing for active compounds and/or loss of efficiency (resolution). Fortunately, thermal damage is a slower process, thus prolonged times above the temperature limit are required before significant damage occurs. Thermal damage is greatly accelerated in the presence of oxygen. Overheating a column with a leak or high oxygen levels in the carrier gas results in rapid and permanent column damage.

Setting the GC's maximum oven temperature at or only a few degrees above the column's temperature limit is the best method to prevent thermal damage. This prevents the accidental overheating of the column. If a column is thermally damaged, it may still be functional. Remove the column from the detector. Heat the column for 8-16 hours at its isothermal temperature limit. Remove 10-15 cm from the detector end of the column. Reinstall the column and condition as usual. The column usually does not return to its original performance; however, it is often still functional. The life of the column will be reduced after thermal damage.

Oxygen Damage

Oxygen is an enemy to most capillary GC columns. While no column damage occurs at or near ambient temperatures, severe damage occurs as the column temperature increases. In general, the temperature and oxygen concentration at which significant damage occurs is lower for polar stationary phases. It is constant exposure to oxygen that is the problem. Momentary exposure such as an injection of air or a very short duration septum nut removal is not a problem.

A leak in the carrier gas flow path (e.g., gas lines, fittings, injector) is the most common source of oxygen exposure. As the column is heated, very rapid degradation of the stationary phase occurs. This results in the premature onset of excessive column bleed, peak tailing for active compounds and/or loss of efficiency (resolution). These are the same symptoms as for thermal damage. Unfortunately, by the time oxygen damage is discovered, significant column damage has already occurred. In less severe cases, the column may still be functional but at a reduced performance level. In more severe cases, the column is irreversibly damaged.

Maintaining an oxygen and leak-free system is the best prevention against oxygen damage. Good GC system maintenance includes periodic leak checks of the gas lines and regulators, regular septa changes, using high quality carrier gases, installing and changing oxygen traps, and changing gas cylinders before they are completely empty.

Chemical Damage



There are relatively few compounds that damage stationary phases. Introducing nonvolatile compounds (e.g., salts) in a column often degrades performance, but damage to the stationary phase does not occur. These residues can often be removed and performance returned by solvent rinsing the column.

Inorganic or mineral bases and acids are the primary compounds to avoid introducing into a column. The acids include hydrochloric (HCl), sulfuric (H_2SO_4), nitric (HNO_3), phosphoric (H_3PO_4), and chromic (CrO_3). The bases include potassium hydroxide (KOH), sodium hydroxide (NaOH), and ammonium hydroxide (NH_4OH). Most of these acids and bases are not very volatile and accumulate at the front of the column. If allowed to remain, the acids or bases damage the stationary phase. This results in the premature onset of excessive column bleed, peak tailing for active compounds and/or loss of efficiency (resolution). The symptoms are very similar to thermal and oxygen damage. Hydrochloric acid and ammonium hydroxide are the least harmful of the group. Both tend to follow any water that is present in the sample. If the water is not or only poorly retained by the column, the residence time of the HCl and NH_4OH in the column is short. This tends to eliminate or minimize any damage by these compounds. Thus, if HCl or NH_4OH are present in a sample, using conditions or a column with no water retention will render these compounds relatively harmless to the column.

The only organic compounds that have been reported to damage stationary phases are perfluoroacids. Examples include trifluoroacetic, pentafluoropropanoic, and heptafluorobutyric acid. They need to be present at high levels (e.g., 1% or higher). Most of the problems are experienced with splitless or Megabore direct injections where large volumes of the sample are deposited at the front of the column.

Since chemical damage is usually limited to the front of the column, trimming or cutting 0.5-1 meter from the front of the column often eliminates any chromatographic problems. In more severe cases, five or more meters may need to be removed. The use of a guard column or retention gap will minimize the amount of column damage; however, frequent trimming of the guard column may be necessary. The acid or base often damages the surface of the deactivated fused silica tubing which leads to peak shape problems for active compounds.

Column Contamination

Column contamination is one of the most common problems encountered in capillary GC. Unfortunately, it mimics a very wide variety of problems and is often misdiagnosed as another problem. A contaminated column is usually not damaged, but it may be rendered useless.

There are two basic types of contaminants: nonvolatile and semivolatile. Nonvolatile contaminants or residues do not elute and accumulate in the column. The column becomes coated with these residues which interfere with the proper partitioning of solutes in and out of the stationary phase. Also, the residues may interact with active solutes resulting in peak adsorption problems (evident as peak tailing or loss of peak size). Active solutes are those containing a hydroxyl (-OH) or amine (-NH) group, and some thiols (-SH) and aldehydes. Semivolatile contaminants or residues accumulate in the column, but eventually elute. Hours to days may elapse before they completely leave the column. Like nonvolatile residues, they may cause peak shape and size problems, and, in addition, are usually responsible for many baseline problems (instability, wander, drift, ghost peaks, etc.).

Contaminants originate from a number of sources, with injected samples being the most common. Extracted samples are among the worst types. Biological fluids and tissues, soils, waste and ground water, and similar types of matrices contain high amounts of semivolatile and nonvolatile materials. Even with careful and thorough extraction procedures, small amounts of these materials are present in the injected sample. Several to hundreds of injections may be necessary before the accumulated residues cause problems. Injection techniques such as on-column, splitless, and Megabore direct place a large amount of sample into the column, thus column contamination is more common with these injection techniques.

Occasionally, contaminants originate from materials in gas lines and traps, ferrule and septa particles, or anything coming in contact with the sample (vials, solvents, syringes, pipettes, etc.). These types of contaminants are probably responsible when a contamination problem suddenly develops and similar samples in previous months or years did not cause any problems.

Minimizing the amount of semivolatile and nonvolatile sample residues is the best method to reduce contamination problems. Unfortunately, the presence and identity of potential contaminants are often unknown. Rigorous and thorough sample cleanup is the best protection against contamination problems. The use of a guard column or retention gap often reduces the severity or delays the onset of column contamination induced problems. If a column becomes contaminated, it is best to solvent rinse the column to remove the contaminants.

Maintaining a contaminated column at high temperatures for long periods of time (often called baking-out a column) is not recommended. Baking-out a column may convert some of the contaminating residues into insoluble materials that cannot be solvent rinsed from the column. If this occurs, the column cannot be salvaged in most cases. Sometimes the column can be cut in half and the back half may still be useable. Baking-out a column should be limited to 1-2 hours at the isothermal temperature limit of the column.

TIPS & TOOLS

Column contamination from sample matrix components is the number one cause of column failure. Use Agilent DuraGuard GC columns with built-in guard if you do not want to use column connectors.

Solvent Rinsing Columns

Solvent rinsing columns involves removing the column from the GC and passing milliliters of solvent through the column. Any residues soluble in the rinse solvents are washed from the column. Injecting large volumes of solvent while the column is still installed is not rinsing and doing so will not remove any contaminants from the column. **A capillary GC column must have a bonded and cross-linked stationary phase before it can be solvent rinsed.** Solvent rinsing a non-bonded stationary phase results in severe damage to the column.

A column rinse kit is used to force solvent through the column (see picture). The rinse kit is attached to a pressurized gas source (N_2 or He), and the column is inserted into the rinse kit. Solvent is added to the vial, and the vial is pressurized using the gas source. The pressure forces solvent to flow through the column. Residues dissolve into the solvent and are backflushed out of the column with the solvent. The solvent is then purged from the column, and the column is properly conditioned.

Before rinsing a column, cut about 0.5 meter from the front (i.e., injector end) of the column. Insert the detector end of the column into the rinse kit. Multiple solvents are normally used to rinse columns. Each successive solvent must be miscible with the previous one. High boiling point solvents should be avoided especially as the last solvent. The sample matrix solvent(s) is often a good choice.

Methanol, methylene chloride and hexane are recommended and work very well for the majority of cases. Acetone can be substituted for methylene chloride to avoid using halogenated solvents; however, methylene chloride is one of the best rinsing solvents. If aqueous based samples (e.g., biological fluids and tissues) were injected, use water before the methanol. Some residues originating from aqueous based samples are only soluble in water and not organic solvents. Water and alcohols (e.g., methanol, ethanol, isopropanol) should be used to rinse bonded polyethylene glycol based stationary phases (e.g., DB-WAX, DB-WAXetr, DB-FFAP, HP-Innowax) **only as a last resort**.

Table 8 lists the suggested solvent volumes for different diameter columns. Using larger solvent volumes is not harmful, but rarely better and merely wasteful. After adding the first solvent, pressurize the rinse kit, but stay below 20 psi. Use the highest pressure that keeps the solvent flow rate below 1 mL/min. Except for most 0.53 mm id columns, the rinse kit pressure will reach 20 psi before the flow rate reaches 1 mL/min. Longer rinse times are required when using heavy or viscous solvents, and for longer or smaller diameter columns. When all or most of the first solvent has entered the column, add the next solvent. The previous solvent does not have to vacate the column before the next solvent is started through the column.

After the last solvent has left the column, allow the pressurizing gas to flow through the column for 5-10 min. Install the column in the injector and turn on the carrier gas. Allow the carrier gas to flow through the column for 5-10 min. Attach the column to the detector (or leave it unattached if preferred). Using a temperature program starting at 40-50 °C, heat the column at 2-3 °/min until the upper temperature limit is reached. Maintain this temperature for 1-4 hours until the column is fully conditioned.



Column rinse kit, 430-3000

Table 8:

Solvent Volumes for Rinsing Columns

Column ID (mm)	Solvent Volume (mL)
0.18-0.2	3-4
0.25	4-5
0.32	6-7
0.45	7-8
0.53	10-12

Using larger volumes will not damage the column



Column Storage

Capillary columns should be stored in their original box when removed from the GC. Place a GC septa over the ends to prevent debris from entering the tubing. Upon reinstallation of the column, the column ends need to be trimmed by 2-4 cm to ensure that a small piece of septa is not lodged in the column.

If a column is left in a heated GC, there should always be carrier gas flow. The carrier gas flow can be turned off only if the oven, injector, detector and transfer lines are turned off (i.e., not heated). Without carrier gas flow, damage to the heated portion of the column occurs.

Evaluating the Problem

The first step in any troubleshooting effort is to step back and evaluate the situation. Rushing to solve the problem often results in a critical piece of important information being overlooked or neglected. In addition to the problem, look for any other changes or differences in the chromatogram. Many problems are accompanied by other symptoms. Retention time shifts, altered baseline noise or drift, or peak shape changes are only a few of the other clues that often point to or narrow the list of possible causes. Finally, make note of any changes or differences involving the sample. Solvents, vials, pipettes, storage conditions, sample age, extraction, preparation techniques, or any other factor influencing the sample environment can be responsible.

Checking the Obvious

A surprising number of problems involve fairly simple and often overlooked components of the GC system or analysis. Many of these items are transparent in the daily operation of the GC and are often taken for granted ("set it and forget it"). The areas and items to check include:

- Gases: pressures, carrier gas average linear velocity, and flow rates (detector, split vent, septum purge)
- Temperatures: column, injector, detector, and transfer lines
- System parameters: purge activation times, detector attenuation and range, mass ranges, etc.
- Gas lines and traps: cleanliness, leaks, and expiration
- Injector consumables: septa, liners, O-rings, and ferrules
- Sample integrity: concentration, degradation, solvent, and storage
- Syringes: handling technique, leaks, needle sharpness, and cleanliness
- Data system: settings and connections

The Most Common Problems



Ghost Peaks or Carryover

System contamination is responsible for most ghost peaks or carryover problems. If the extra ghost peaks are similar in width to the sample peaks (with similar retention times), the contaminants were likely introduced into the column at the same time as the sample. The extra compounds may be present in the injector (i.e., contamination) or in the sample itself. Impurities in solvents, vials, caps and syringes are only some of the possible sources. Injecting sample and solvent blanks may help to find possible sources of the contaminants. If the ghost peaks are much broader than the sample peaks, the contaminants were most likely already in the column when the injection was made. These compounds were still in the column when a previous GC run was terminated. They elute during a later run and are often very broad. Sometimes numerous ghost peaks from multiple injections overlap and elute as a hump or blob. This often takes on the appearance of baseline drift or wander.

Increasing the final temperature or time in the temperature program is one method to minimize or eliminate a ghost peak problem. Alternatively, a short bake-out after each run or series of runs may remove the highly retained compounds from the column before they cause a problem.

Condensation Test

Use this test whenever injector or carrier gas contamination problems are suspected (e.g., ghost peaks or erratic baseline).

1. Leave the GC at 40-50 °C for 8 or more hours.
2. Run a blank analysis (i.e., start the GC, but with no injection) using the normal temperature conditions and instrument settings.
3. Collect the chromatogram for this blank run.
4. Immediately repeat the blank run as soon as the first one is completed. Do not allow more than 5 min to elapse before starting the second blank run.
5. Collect the chromatogram for the second blank run and compare it to the first chromatogram.
6. If the second chromatogram contains a substantially larger amount of peaks and baseline instability, the incoming carrier gas line or the carrier gas is contaminated.
7. If the second chromatogram contains few peaks or very little baseline drift, the carrier gas and incoming carrier gas lines are relatively clean.

Troubleshooting Guides

Excessive Baseline Noise

Possible Cause	Solution	Comments
Injector contamination	Clean the injector; replace liner, gold seal	Try a condensation test; gas lines may also need cleaning
Column contamination	Bake-out the column	Limit the bake-out to 1-2 hours
	Solvent rinse the column	Only for bonded and cross-linked phases
		Check for inlet contamination
Detector contamination	Clean the detector	Usually the noise increases over time and not suddenly
Contaminated or low quality gases	Use better grade gases; also check for expired gas traps or leaks	Usually occurs after changing a gas cylinder
Column inserted too far into the detector	Reinstall the column	Consult GC manual for proper insertion distance
Incorrect detector gas flow rates	Adjust the flow rates to the recommended values	Consult GC manual for proper flow rates
Leak when using an MS, ECD, or TCD	Find and eliminate the leak	Usually at the column fittings or injector
Old detector filament, lamp or electron multiplier	Replace appropriate part	
Septum degradation	Replace septum	For high temperature applications use an appropriate septum

Baseline Instability or Disturbances

Possible Cause	Solution	Comments
Injector contamination	Clean the injector	Try a condensation test; gas lines may also need cleaning
Column contamination	Bake-out the column	Limit a bake-out to 1-2 hours
Unequilibrated detector	Allow the detector to stabilize	Some detectors may require up to 24 hours to fully stabilize
Incompletely conditioned column	Fully condition the column	More critical for trace level analyses
Change in carrier gas flow rate during the temperature program	Normal in many cases	MS, TCD and ECD respond to changes in carrier gas flow rate

Tailing Peaks

Possible Cause	Solution	Comments
Column contamination	Trim the column	Remove 0.5-1 m from the front of the column
	Solvent rinse the column	Only for bonded and cross-linked phases
		Check for inlet contamination
Column activity	Irreversible; Replace the column	Only affects active compounds
Solvent-phase polarity mismatch	Change sample solvent to a single solvent	More tailing for the early eluting peaks or those closest to the solvent front
	Use a retention gap	3-5 m retention gap is sufficient
Solvent effect violation for splitless or on-column injections	Decrease the initial column temperature	Peak tailing decreases with retention
Too low of a split ratio	Increase the split ratio	Flow from split vent should be 20 mL/min or higher
Poor column installation	Reinstall the column	More tailing for early eluting peaks
Some active compounds always tail	None	Most common for amines and carboxylic acids

Split Peaks

Possible Cause	Solution	Comments
Injection technique	Change technique	Usually related to erratic plunger depression or having sample in the syringe needle; Use an auto injector
Mixed sample solvent	Change sample solvent to a single solvent	Worse for solvents with large differences in polarity or boiling points
Poor column installation	Reinstall the column	Usually a large error in the insertion distance
Sample degradation in the injector	Reduce the injector temperature	Peak broadening or tailing may occur if the temperature is too low
	Change to an on-column injection	Requires an on-column injector
Poor sample focusing	Use a retention gap	For splitless and on-column injection

Retention Time Shift

Possible Cause	Solution	Comments
Change in carrier gas velocity	Check the carrier gas velocity	All peaks will shift in the same direction by approximately the same amount
Change in column temperature	Check the column temperature	Not all peaks will shift by the same amount
Change in column dimension	Verify column identity	
Large change in compound concentration	Try a different sample concentration	May also affect adjacent peaks; Sample overloading is corrected with an increase in split ratio or sample dilution
Leak in the injector	Leak check the injector	A change in peak size usually occurs
Blockage in a gas line	Clean or replace the plugged line	More common for the split line; also check flow controllers and solenoids
Septum leak	Replace septum	Check for needle barb
Sample solvent incompatibility	Change sample solvent to a single solvent Use a retention gap	For splitless injection

Change in Peak Size

Possible Cause	Solution	Comments
Change in detector response	Check gas flows, temperatures and settings	All peaks may not be equally affected
	Check background level or noise	May be caused by system contamination and not the detector
Change in the split ratio	Check split ratio	All peaks may not be equally affected
Change in the purge activation time	Check the purge activation line	For splitless injection
Change in injection volume	Check the injection technique	Injection volumes are not linear
Change in sample concentration	Check and verify sample concentration	Changes may also be caused by degradation, evaporation, or variances in sample temperature or pH
Leak in the syringe	Use a different syringe	Sample leaks past the plunger or around the needle; Leaks are not often readily visible
Column contamination	Trim the column	Remove 0.5-1 m from the front of the column
	Solvent rinse the column	Only for bonded and cross-linked phases
Column activity	Irreversible	Only affects active compounds
Coelution	Change column temperature or stationary phase	Decrease column temperature and check for the appearance of a peak shoulder or tail
Change in injector discrimination	Maintain the same injector parameters	Most severe for split injections
Sample flashback	Inject less, use a larger liner, reduce the inlet temperature	Less solvent and higher flow rates are most helpful
Decomposition from inlet contamination	Clean the injector; replace liner, gold seal	Only use deactivated liners and glass wool in the inlet

Loss of Resolution

Possible Cause	Solution	Comments
Decrease in separation		
Different column temperature	Check the column temperature	Differences in other peaks will be visible
Different column dimensions or phase	Verify column identity	Differences in other peaks will be visible
Coelution with another peak	Change column temperature	Decrease column temperature and check for the appearance of a peak shoulder or tail
Increase in peak width		
Change in carrier gas velocity	Check the carrier gas velocity	A change in the retention time also occurs
Column contamination	Trim the column	Remove 0.5-1 m from the front of the column
	Solvent rinse the column	Only for bonded and cross-linked phases
Change in the injector	Check the injector settings	Typical areas: split ratio, liner, temperature, injection volume
Change in sample concentration	Try a different sample concentration	Peak widths increase at higher concentrations
Improper solvent effect, lack of focusing	Lower oven temperature, better solvent, sample phase polarity match, use a retention gap	For splitless injection

Product Index

Agilent J&W GC Columns

Application and Method Guides
ASTM Methods 229-236
Application Cross Reference Guide 210-212
EPA Methods
Drinking Water 213-216
Solid Waste 220-227
Waste Water 217-220
United States Pharmacopoeia (USP) GC Phases 228
Capillary Columns
By Group
Foods, Flavors and Fragrances 352
High Temperature 314
Life Sciences 362
Low-bleed GC/MS 244
Non-Bonded 387
PAH 338
PLOT 368
Pesticides 315
Petroleum 318
Polyethylene Glycol (PEG) 304
Premium Polysiloxane 269
Semivolatiles 340
Ultra Inert 237
Volatiles 344
By Stationary Phase
Biodiesel 328
CAM 388
CP Wax 58 FFAP CB 312
CP-1301 300
CP-Al2O3/KCl 375-377
CP-Al2O3/Na2SO4 375-377
CP-Carbowax 400 for Volatiles in Alcohol 356
CP-Chirasil Val 360
CP-Chirasil-Dex CB 360
CP-Cyclodextrin-B-2,3,6-M-19 361
CP-FFAP CB for Free Fatty Acids in Dairy Products 358
CP-Molsieve 5Å 385
CP-Select 624 CB 346
CP-Select CB for MTBE 350
CP-Sil 13 CB 288
CP-Sil 19 CB 302-303
CP-Sil 19 CB for Pesticides 336
CP-Sil 2 CB 325
CP-Sil 24 CB 293
CP-Sil 43 CB 298
CP-Sil 5 CB 275-278
CP-Sil 5 CB for Formaldehyde 319
CP-Sil 5 CB for Sulfur 326
CP-Sil 5/C18 CB for PCB 342
CP-Sil 8 CB 286-287
CP-Sil 8 CB for Amines 332
CP-Sil 8 CB for PCB 340
CP-Sil 8 CB for Pesticides 335
CP-Sil 88 353
CP-Sil 88 for Dioxins 343
CP-Sil 88 for FAME 354
CP-Sil PAH CB UltiMetal 339
CP-Sil PONA CB 320
CP-Sil PONA for ASTM D 5134 320
CP-SilicaPLOT 381
CP-SimDist 323
CP-TAP CB for Triglycerides 357
CP-TCEP for Alcohols in Gasoline 325
CP-Volamine 331
CP-Wax 52 CB 308-309
CP-Wax 57 CB 355
CP-Wax 57 CB for Glycols and Alcohols 356
CP-Wax for Volatile Amines and Diamines 332
CarboBOND 382
CarboPLOT P7 382
Carbowax 20M 313
CycloSil-B 358
Cyclodex-B 359
DB-1 269-272
DB-1301 299
DB-17 291
DB-1701 301
DB-1701P 334
DB-17ht 316
DB-17ms 258
DB-1ht 314
DB-1ms 245
DB-1ms Ultra Inert 240
DB-200 295
DB-210 296
DB-225 297
DB-225ms 262
DB-23 294
DB-2887 322
DB-35 289
DB-35ms 256
DB-35ms Ultra Inert 242
DB-5 281-283
DB-5.625 341
DB-502.2 349
DB-5ht 315
DB-5ms 249-250
DB-5ms EVDX 363
DB-5ms Ultra Inert 241
DB-608 336
DB-624 344-345
DB-624 Ultra Inert 242, 344
DB-ALC 1 362
DB-ALC 2 362
DB-CLP 1 333
DB-CLP 2 333
DB-Dioxin 343
DB-EUPAH 338
DB-FFAP 310
DB-HT Sim Dis 322
DB-MTBE 349
DB-Petro 321
DB-Select 624 UI for <467> 364
DB-TPH 350
DB-UI 8270D 242
DB-UI 8270D for Semivolatiles 340
DB-VRX 347
DB-WAX 304-305
DB-WAX FF 304-305
DB-WAXetr 306
DB-XLB 254
DX-1 389
DX-4 389
GS-Alumina 379
GS-Alumina KCl 375
GS-CarbonPLOT 383
GS-GasPro 380
GS-OxyPLOT 318
GS-Q 372
HP-1 273-274
HP-1 Aluminum Clad 321
HP-101 387
HP-17 387
HP-1ms 246
HP-1ms Ultra Inert 240
HP-20M 313
HP-35 290
HP-5 284-285
HP-50+ 292
HP-5ms 251
HP-5ms Semivolatile 342
HP-5ms Ultra Inert 241
HP-88 352
HP-Blood Alcohol 363
HP-Chiral B 359
HP-FFAP 311
HP-Fast Residual Solvent 364
HP-INNOWax 307
HP-PAS5 336-337
HP-PLOT Al2O3 KCl 374
HP-PLOT Al2O3 M 380
HP-PLOT Al2O3 S 378
HP-PLOT Molesieve 384
HP-PLOT Q 371
HP-PLOT U 374
HP-PONA 319
HP-VOC 346-348
Lowox 318
PoraBOND Q 368
PoraBOND U 369
PoraPLOT Amines 332
PoraPLOT Q 369-370
PoraPLOT Q-HT 369-370
PoraPLOT S 372-373
PoraPLOT U 372-373
Rapid-MS 337
SE-30 390
SE-54 390
Select Al2O3 MAPD 327
Select Biodiesel 330
Select FAME 353-354
Select Low Sulfur 326
Select Mineral Oil 351
Select PAH 338
Select Silanes 331
Select for Permanent Gases 327
Ultra 1 278-279
Ultra 2 280
VF-1301ms 266
VF-1701 Pesticides 335
VF-1701ms 267-268
VF-17ms 259
VF-1ms 247-248
VF-200ms 261
VF-23ms 260

VF-35ms....257
VF-5 Pesticides....333-334
VF-5ht....317
VF-5ms....252-253
VF-624ms....265
VF-DA....362
VF-WAXms....263-264
VF-Xms....255
Metal Columns....365
Column Selection
Column Diameter....204-205
Column Film Thickness....208-209
Column Length....206-207
Polarity....200-201
Selecting Stationary Phases....196-199
Custom Ordering....410
Fused Silica Tubing
Deactivated....397-398
Undeactivated....399
Guard Columns
DuraGuard....391
EZ-Guard....392
Installation and Troubleshooting
Causes of Column Performance Degradation....417-419
Quick Reference Guide....414-416
Troubleshooting Guides
Baseline Instability or Disturbances....424
Change in Peak Size....426
Excessive Baseline Noise....424
Loss of Resolution....427
Retention Time Shift....426
Split Peaks....425
Tailing Peaks....425
LTM Column Modules....393-394
Packed Columns
For Agilent 7820, 7890, and 6890 Instruments
0.1% SP-1000....407
1.5% OV-101....405
10% OV-101....405
10% PEG-20M....405
10% UC W982....407
12% UC W982....407
15% Carbowax 1540....400
15% Hallcomid m-18....402
20% Carbowax 20M....400
20% OV-101....405
20% PEG-20M....405
20% Sebaconitrile....406
20% Sebaconitrile/2% H3PO4....407
20% TCEP....407
25% DC-200....401
25% SP-2100....407
30% DC 200/500....402
30% DC-200....401
35% DC-200....401
5% Carbowax 20M....400
7% Carbowax M + 3% Polyphenolether 6 ring + 2% KOH....401
Carbosieve S....400
Carboxen-1000....401
Chromosorb 101....401
Chromosorb 102....401
HayeSep D....402
HayeSep DB....402
HayeSep N....402
HayeSep N + HayeSep R 1:1....402
HayeSep Q....403
HayeSep R....403
HayeSep T....403
MolSieve 13X....404
MolSieve 5Å....404
Porapak N....405
Porapak N + Porapak R 1:1....405
Porapak Q....406
Porapak QS....406
Porapak R....406
Porapak T....406
Silica Gel....407
For All Instruments
1.5% OV-101....409
10% SE-30....409
20% TCEP....409
30% DC 200/500....408
HayeSep D....408
HayeSep DB....408
HayeSep N....408
HayeSep P....408
HayeSep Q....408
HayeSep R....408
MolSieve 13X....409
MolSieve 5Å....409
Porapak QS....409
Silica Gel....409
Test Standards....411-412

Agilent Supplies

Bulk GC Supplies....14
Capillary Column Ferrules
Column Nuts....33-34
Ferrule Selection Recommendations....30-31
For LTM Rapid Heating/Cooling System....35
For NCD and SCD....35
Reducing....35
Specialty....33-34
Straight....35
Capillary Flow Technology
Column/Retention Gap Installation....37
Ferrules....37
Fittings....37
Ultimate Union....36-37
Column Connectors and Splitters
Graphpak....39
Press-fit....38
Column Nuts....33-34
Detector Systems
Electron Capture Detector (ECD)....86-87
Flame Ionization Detector (FID)....78
Flame Photometric Detector (FPD)....94
Nitrogen Chemiluminescence Detector (NCD)....106
Nitrogen Phosphorus Detector (NPD)....101
Sulfur Chemiluminescence Detector (SCD)....107
Thermal Conductivity Detector (TCD)....89-91
GC/MS
220-MS....136
240-MS Ion Trap....134-135
7000A Triple Quadropole GC/MS....132-133
Cleaning and Maintenance....116-117
Electron Multipliers....127
GC/MSD Interface....122-123
Ion Source
Chemical Ionization (CI) Ion Source....121
Electron Impact (EI) Ion Source....119-120
MSD Contamination....110-111
MSD Filaments....125
Maintenance Schedule....109
Mass Spectrometer Symptoms....114-116
Quadropole Mass Filter....126
QuickSwap MS Interface....124
Standards
Analyzer Kit Standards....137
Test and Performance Samples....137-138
Vacuum Systems and Pumps
Diffusion Pump....130
Foreline Pump....131
Pressure Symptoms....128-129
Inlet Liners
Specialty Injection
Direct Connect....28
MultiMode Inlet Heavy Matrix....27
PTV....28
Split, Original Deactivation....25
Splitless, Original Deactivation....26
Ultra Inert....24
Inlet Septa
Advanced Green....17
Bleed and Temperature Optimized (BTO)....16
General Purpose....19
Long-Life....17
Inlet Systems
Cool On-Column....66
Flip Top Inlet Sealing System....57
Inlet Convenience Kits....55
Multimode....64
Programmable Temperature Vaporizer (PTV)....69-70
Purged Packed....74-75
Split/Splitless Inlet Seals....56, 58-59
Liner O-rings....29
Maintenance Schedule....12-13
Markes Thermal Desorption....53-54
Merlin Microseal....20-21
Oven Exhaust Deflector....107
Purge and Trap Systems
Archon....52
Teledyne Tekmar....50-51
Sample Introduction Systems
7693A Automatic Liquid Sampler....43-44
7697A Headspace Sampler....45-47
Automatic Liquid Sampler....44
G1883A Network Headspace Sampler....49
G1888A Network Headspace Sampler....48
G3520A XLSI Accessory....46
Standards....108
Valves and Loops....40

Applications

Energy and Fuels....552
Environmental
Air Analysis....473
Hydrocarbons....429
Pesticides and Herbicides....434
Semivolatiles....458
Volatiles....468
Food, Flavor and Fragrance....478

Industrial Chemical 487
Life Science....521

CrossLab Supplies

Bruker, Varian GC Systems
Autosampler Syringes....158
Capillary Column Ferrules 157
Column Nuts 158
Detector Replacement
Flame Ionization Detector (FID)....166
Pulsed Flame Photometric Detector (PFPD)....167-168
Thermal Conductivity Detector (TCD)....166
Thermionic Specific Detector (TSD)....168
Injector Replacement
1041 Packed/Wide Bore On-Column (PWOC) injector 165
1061 Packed/530 µm Capillary Column Injector....164
1079 Large Volume Injector (LVI)....162
1093 Cool On-Column (COC) Injector 163
1177 Split/Splitless Injector....161-168
Inlet Liners
1060/1061 Injector....156
1075/1077 Injector....156
1078/1079 Injector....155-156
1093/1094 Injector....155-156
1177 Injector 154-160
Inlet Septa....159-160
Liner O-rings....156
Packed Column Ferrules....158
CTC GC Autosamplers
Autosampler Syringes....187
Column Ferrules....143
Inlet Liners 140-141
Inlet Septa
Advanced Green 151
Bleed and Temperature Optimized (BTO) 150
General Purpose 153
Long-Life....152
Liner O-rings 142
Perkin Elmer GC Systems
Autosampler Syringes....173
Capillary Column Ferrules 171
Column Nuts 172
Inlet Liners
AutoSystem....169-174
AutoSystem XL....169-174
Clarus....169-174
Inlet Septa....174
Liner O-rings....170
Packed Column Ferrules....172
Shimadzu GC Systems
Autosampler Syringes....180
Capillary Column Ferrules 179
Column Nuts 180
Inlet Liners
14 Systems....178
17A Systems....177
2010 and 2010 Plus Systems....176
2014 Systems....175-180
Inlet Septa....181
Liner O-rings....178
Packed Column Ferrules....179
Syringes 145-146
Thermo Scientific GC Systems
Autosampler Syringes....184
Capillary Column Ferrules 183
Column Nuts 184
Inlet Liners
Focus Systems....182-186
Trace Systems....182-186
Inlet Septa....185-186
Liner O-rings....183

Part Number Index

0100-1104 35
0100-1324 35
0100-1325 35
0100-1326 35
0100-1331 35
0100-1332 ..... 35, 77, 91
0100-1342 35
0100-1344 35
0100-1365 35
0100-1375 ..... 35, 72
0100-1378 35
0100-1379 35
0100-1381 35
0100-2594 46
0101-0282 42
0101-0299 42
0101-0300 42
0101-0301 42
0101-0302 42
0101-0303 42
0101-0355 41
0101-0403 41
0101-0532 41
0101-0584 40
0101-0585 40
0101-0633 41
0101-0636 40
0101-0637 40
0101-0638 40
0101-0639 40
0410105017 48
0510-1306 62
0515-0655 105
0515-0680 99
0515-0683 100
0515-1084 99
0515-1799 76
0515-2495 105
0515-2711 76
0515-2712 84
05890-61525 43
05890-80660 41
05921-21170 ..... 34, 117
05970-60045 138
05971-20134 120
05971-20143 120
05971-60140 125
05971-60561 116
05971-80102 127
05971-80103 ..... 127, 133
05980-20018 116
05980-60051 ..... 116, 133
05988-20066 ..... 34, 117
05990-60075 138
07673-20570 44
07673-40180 43
07673-60840 44
07675-80050 42
0854-0141 99
0905-1284 105
0905-1463 132
0905-1610 99
0905-2580 105
0960-0897 125
1000-1437 100
1000-1438 100
112-2032 313
112-2032LTM 313
112-2112 388
112-2112LTM 388
112-2132 388
112-2132LTM 388
112-2133 388
112-2133LTM 388
112-2162 388
112-2532 359
112-2532E 359
112-2532LTM 359
112-2562 359
112-5432 390
112-5432LTM 390
112-5462 390
112-6632 358
112-6632LTM 358
112-8837 352
112-8837E 352
112-8837LTM 352
112-8867 352
112-8867E 352
112-88A7 352
112-88A7E 352
113-2032 313
113-2032LTM 313
113-2062 313
113-2132 388
113-2132E 388
113-2132LTM 388
113-2133 388
113-2133E 388
113-2133LTM 388
113-2532 359
113-2532E 359
113-2532LTM 359
113-3032 390
113-3032LTM 390
113-3112 383
113-3132 383
113-3132LTM 383
113-3133 383
113-3133LTM 383
113-3162 383
113-3432 372
113-3432E 372
113-3432LTM 372
113-4302 380
113-4312 380
113-4332 ..... 234, 380
113-4362 ..... 229, 380
113-5432 390
113-5432LTM 390
113-6632 358
113-6632LTM 358
115-2132 ..... 233, 388
115-2132LTM 388
115-3113 383
115-3133 383
115-3133LTM 383
115-3332 375
115-3332LTM 375
115-3352 375
115-3352E 375
115-3412 372
115-3412LTM 372
115-3422 372
115-3422LTM 372
115-3432 372
115-3432E 372
115-3432LTM 372
115-34H2 372
115-34H2LTM 372
115-3532 ..... 229-230, 379
115-3532E 379
115-3532LTM 379
115-3552 ..... 230, 236, 379
115-4912 318
115-4912E 318
121-0122 245
121-0122E 245
121-0122LTM 245
121-0122UI 240
121-0713 301
121-0713LTM 301
121-0722 ..... 214, 301
121-0722LTM 301
121-1012 270
121-1012E 270
121-1012LTM 270
121-1013 270
121-1013E 270
121-1013LTM 270
121-101A 270
121-101ALTM 270
121-1022 270
121-1022E 270
121-1022LTM 270
121-1023 270
121-1023LTM 270
121-1043 270
121-1043E 270
121-1222 254
121-1222E 254
121-1222LTM 254
121-1232 254
121-1313 299
121-1313LTM 299
121-1324 ..... 215, 219, 225-226, 235, 345
121-1324E 345
121-1324LTM 345
121-1324UI 226, 242, 344
121-1524 ..... 215, 219, 225-226, 235, 347
121-1524LTM 347
121-1544 347
121-1544E 347
121-1544LTM 347
121-1722 291
121-1722LTM 291
121-1723 291
121-1723LTM 291
121-2223 297
121-2223LTM 297
121-2323 294
121-2323LTM 294
121-3822 256
121-3822E 256
121-3822LTM 256
121-3822UI 242
121-4722 258
121-4722E 258
121-4722LTM 258
121-5012 281
121-5012E 281
121-5012LTM 281
121-5013 281
121-5013LTM 281
121-5022 281
121-5022E 281
121-5022LTM 281
121-5023 281
121-5023E 281
121-5023LTM 281
121-5042 281
121-5522 250
121-5522E 250
121-5522LTM 250
121-5522UI 214, 241
121-5522UILTM 241
121-5523 250
121-5523LTM 250
121-5523UI 241
121-5523UILTM 241
121-5542 250
121-5621 341
121-5621LTM 341
121-5622 341
121-5622G5 391
121-5622LTM 341
121-6822 336
121-6822LTM 336
121-7012 305
121-7012LTM 305
121-7022 305
121-7022E 305
121-7022LTM 305
121-7023 305
121-7023E 305
121-7023LTM 305
121-7042 305
121-7042E 305
121-7043 305
121-9627 338
121-9723 ..... 212, 226, 242, 340
122-0112 245
122-0112E 245
122-0112LTM 245
122-0112UI 240
122-0112UIE 240
122-0131 245
122-0132 ..... 223, 245
122-0132E 245
122-0132UI 240
122-0132UIE 240
122-0162 245
122-0162UI 240
122-0212 296
122-0212LTM 296
122-0232 296
122-0232E 296
122-0232LTM 296
122-0233 ..... 215, 296
122-0233LTM 296
122-0334UI 364
122-0364UI 364

122-0712 301
122-0712LTM 301
122-0713 301
122-0713LTM 301
122-0731 301
122-0731LTM 301
122-0732 ..... 214, 216, 301
122-0732E 301
122-0732LTM 301
122-0733 ..... 223, 301
122-0733E 301
122-0733LTM 301
122-0761 301
122-0762 301
122-0763 301
122-0763E 301
122-0766 301
122-1011 270
122-1011LTM 270
122-1012 270
122-1012LTM 270
122-1013 270
122-1013LTM 270
122-1022 270
122-1022LTM 270
122-1031 270
122-1031LTM 270
122-1032 270
122-1032E 270
122-1032G 391
122-1032LTM 270
122-1033 ..... 215, 270
122-1033E 270
122-1033LTM 270
122-103E 270
122-103ELTM 270
122-1052 270
122-1061 270
122-1062 270
122-1063 270
122-106E 229, 270
122-10A6 321
122-10A6E 234, 321
122-10AE 270
122-10G3 270
122-1111 314
122-1111E 314
122-1131 314
122-1211 254
122-1211LTM 254
122-1212 254
122-1231 254
122-1232 ..... 215, 217, 221, 233-236, 254
122-1232G 391
122-1232LTM 254
122-1233 254
122-1236 ..... 213, 254
122-1262 254
122-1262E 254
122-1332 299
122-1332E 299
122-1332LTM 299
122-1333 ..... 215, 299
122-1333LTM 299
122-1334 ..... 213, 217, 220-221, 345
122-1334E 345
122-1334LTM 345
122-1334UI 213, 220-221, 242, 344
122-1362 299
122-1363 299
122-1363E 299
122-1364 ..... 213, 215, 217, 219, 235, 345
122-1364E 345
122-1364UI 213, 215, 225, 242, 344
122-1464 349
122-1534 ..... 213, 217, 220-221, 347
122-1534LTM 347
122-1564 ..... 213, 215, 217, 219-220, 225-226, 235, 347
122-1564E 347
122-1711 291
122-1711LTM 291
122-1712 291
122-1712LTM 291
122-1713 291
122-1713E 291
122-1713LTM 291
122-1731 291
122-1731E 291
122-1731LTM 291
122-1732 291
122-1732E 291
122-1732LTM 291
122-1733 291
122-1733LTM 291
122-1762 291
122-1801 316
122-1801LTM 316
122-1811 316
122-1831 316
122-1831LTM 316
122-1932 289
122-1932LTM 289
122-1962 289
122-2032 295
122-2032LTM 295
122-2033 295
122-2033LTM 295
122-2212 297
122-2212LTM 297
122-2231 297
122-2231LTM 297
122-2232 297
122-2232LTM 297
122-2312 294
122-2312LTM 294
122-2331 294
122-2331LTM 294
122-2332 294
122-2332E 294
122-2332LTM 294
122-2361 294
122-2361E 294
122-2362 ..... 236, 294
122-2362E 294
122-2461 343
122-2461E 343
122-2462 343
122-2912 262
122-2912LTM 262
122-2932 ..... 234, 262
122-2932E 262
122-2932LTM 262
122-2962 262
122-3212 310
122-3212LTM 310
122-3232 310
122-3232E 310
122-3232LTM 310
122-3233 310
122-3233LTM 310
122-3262 310
122-3262E 310
122-3263 310
122-3812 256
122-3812UI 242
122-3831 256
122-3832 ..... 213, 218, 224, 234-235, 256
122-3832E 256
122-3832LTM 256
122-3832UI 219, 242
122-3862 256
122-4711 258
122-4711LTM 258
122-4712 258
122-4712LTM 258
122-4731 258
122-4731LTM 258
122-4732 ..... 218, 223, 258
122-4732E 258
122-4732LTM 258
122-4762 258
122-5011 282
122-5011LTM 282
122-5012 ..... 234, 282
122-5012LTM 282
122-5013 282
122-5013LTM 282
122-501E 282
122-501ELTM 282
122-5022 282
122-5022LTM 282
122-5031 282
122-5031LTM 282
122-5032 ..... 235, 282
122-5032E 282
122-5032LTM 282
122-5033 ..... 220, 282
122-5033E 282
122-5033LTM 282
122-503E 282
122-503ELTM 282
122-5052 282
122-5061 282
122-5062 282
122-5063 282
122-506E 282
122-5511 250
122-5511LTM 250
122-5512 250
122-5512LTM 250
122-5512UI 215, 241
122-5512UILTM 241
122-5513 250
122-5513LTM 250
122-5513UI 241
122-5513UILTM 241
122-5516 250
122-5516LTM 250
122-5522 250
122-5522LTM 250
122-5522UI 241
122-5522UILTM 241
122-552A 250
122-552ALTM 250
122-5531 250
122-5531LTM 250
122-5532 ..... 213, 215-216, 221-224, 250
122-5532E 250
122-5532G 391
122-5532LTM 250
122-5532UI 214, 216-219, 241
122-5532UIE 241
122-5532UILTM 241
122-5533 ..... 215, 222-223, 227, 250
122-5533E 250
122-5533G 391
122-5533LTM 250
122-5533UI 214, 224, 241
122-5533UIE 241
122-5533UILTM 241
122-5536 ..... 218, 250
122-5536E 250
122-5536G 391
122-5536LTM 250
122-5536UI 241
122-5536UILTM 241
122-5552 250
122-5552UI 241
122-5561 250
122-5562 250
122-5562E 250
122-5562G 391
122-5562UI 218-219, 227, 241
122-5563 250
122-5563UI 241
122-5631 341
122-5631G5 391
122-5631LTM 341
122-5632 341
122-5632LTM 341
122-5633 341
122-5633LTM 341
122-5661 341
122-5711 315
122-5711E 315
122-5711LTM 315
122-5731 315
122-5731LTM 315
122-6133 389
122-6432 389
122-6432LTM 389
122-6462 389
122-6832 ..... 217-218, 336
122-6832LTM 336
122-7012 305
122-7012E 305
122-7012LTM 305
122-7013 ..... 221, 305
122-7013LTM 305
122-7031 305
122-7031LTM 305
122-7032 ..... 229, 305
122-7032E 305
122-7032LTM 305
122-7033 ..... 220, 227, 305
122-7033E 305
122-7033LTM 305
122-7061 305
122-7062 305
122-7062E 305
122-7063 305
122-7063E 305
122-7332 306
122-7332E 306
122-7332LTM 306

122-7333 306
122-7333LTM 306
122-7362 306
122-7363 306
122-7732 ..... 234-235, 334
122-7732LTM 334
122-96L2 338
122-9732 ..... 226, 242, 340
122-9736 ..... 242, 340
123-0112 245
123-0112UI 240
123-0131 245
123-0132 245
123-0132LTM 245
123-0132UI 240
123-0162 245
123-0213 296
123-0213LTM 296
123-0232 296
123-0232LTM 296
123-0233 296
123-0233LTM 296
123-0334UI 364
123-0364UI 364
123-0712 301
123-0712LTM 301
123-0713 301
123-0713LTM 301
123-0731 301
123-0731LTM 301
123-0732 301
123-0732E 301
123-0732LTM 301
123-0733 301
123-0733E 301
123-0733LTM 301
123-0753 301
123-0762 301
123-0763 301
123-0763E 301
123-100E 271
123-100ELTM 271
123-1011 271
123-1011LTM 271
123-1012 271
123-1012LTM 271
123-1013 271
123-1013LTM 271
123-1014 271
123-1014LTM 271
123-1015 271
123-1015LTM 271
123-1022 ..... 234, 271
123-1022LTM 271
123-1026 271
123-1026LTM 271
123-1027 271
123-1027LTM 271
123-102F 271
123-102FLTM 271
123-1031 271
123-1031LTM 271
123-1032 271
123-1032LTM 271
123-1033 ..... 233, 271
123-1033E 271
123-1033LTM 271
123-1034 271
123-1034LTM 271
123-1035 271
123-1035LTM 271
123-103B 271
123-103BLTM 271
123-103E 218, 223-224, 271
123-103ELTM 271
123-1052 271
123-1055 271
123-1056 271
123-105C 271
123-105F 271
123-1061 271
123-1062 271
123-1062E 271
123-1063 271
123-1063E 271
123-1064 271
123-1064E 271
123-1065 271
123-1065E 271
123-106B 271
123-106BE 271
123-106E 230, 271
123-106G 271
123-1111 314
123-1111LTM 314
123-1131 314
123-1131E 314
123-1131LTM 314
123-1232 254
123-1236 ..... 214, 216, 218, 222, 254
123-1262 254
123-1332 299
123-1332LTM 299
123-1333 299
123-1333LTM 299
123-1334 345
123-1334E 345
123-1334LTM 345
123-1334UI 242, 344
123-1363 299
123-1363E 299
123-1364 345
123-1364E 345
123-1364UI 226, 242, 344
123-1464 349
123-1534 ..... 234, 347
123-1534LTM 347
123-1564 347
123-1564E 347
123-1632 ..... 235, 350
123-1632LTM 350
123-1711 291
123-1711LTM 291
123-1712 291
123-1712LTM 291
123-1713 291
123-1713LTM 291
123-1730 ..... 214, 233, 336
123-1730LTM 336
123-1731 291
123-1731LTM 291
123-1732 291
123-1732E 291
123-1732LTM 291
123-1733 291
123-1733E 291
123-1733LTM 291
123-1762 291
123-1811 316
123-1831 316
123-1831E 316
123-1861 316
123-1932 289
123-1932LTM 289
123-1933 289
123-1933E 289
123-1933LTM 289
123-2032 295
123-2032LTM 295
123-2033 295
123-2033LTM 295
123-2232 297
123-2232E 297
123-2232LTM 297
123-2332 294
123-2332E 294
123-2332LTM 294
123-2362 294
123-2461 343
123-2462 343
123-2932 262
123-2932LTM 262
123-3212 310
123-3212LTM 310
123-3223 310
123-3223LTM 310
123-3232 ..... 232, 310
123-3232E 310
123-3232LTM 310
123-3233 310
123-3233LTM 310
123-3234 310
123-3234LTM 310
123-3253 310
123-3262 310
123-3263 310
123-3264 310
123-3812 256
123-3812UI 242
123-3832 ..... 222, 225, 256
123-3832E 256
123-3832UI 214, 216, 218, 225, 242
123-4712 258
123-4712LTM 258
123-4732 ..... 218, 258
123-4732LTM 258
123-500E 282
123-500ELTM 282
123-5011 282
123-5011LTM 282
123-5012 282
123-5012E 282
123-5012LTM 282
123-5013 282
123-5013E 282
123-5013LTM 282
123-5022 282
123-5022LTM 282
123-5026 282
123-5026LTM 282
123-502D 282
123-502DLTM 282
123-502F 282
123-502FLTM 282
123-5031 282
123-5031LTM 282
123-5032 282
123-5032E 282
123-5032LTM 282
123-5033 ..... 233, 282
123-5033E 282
123-5033LTM 282
123-503B 282
123-503BLTM 282
123-503E 282
123-503ELTM 282
123-5052 282
123-5053 282
123-5056 282
123-5062 282
123-5063 282
123-5063E 282
123-5511 250
123-5511LTM 250
123-5512 250
123-5512LTM 250
123-5513 250
123-5513E 250
123-5513LTM 250
123-5526 250
123-5526LTM 250
123-5531 250
123-5531LTM 250
123-5532 ..... 218, 223, 250
123-5532E 250
123-5532LTM 250
123-5532UI 225, 241
123-5532UIE 241
123-5532UILTM 241
123-5533 ..... 227, 250
123-5533G 391
123-5533LTM 250
123-5533UI 241
123-5533UILTM 241
123-5536 ..... 218, 223-224, 250
123-5536LTM 250
123-5536UI 241
123-5536UILTM 241
123-5561 250
123-5562 250
123-5563 250
123-5563UI 241
123-5566 250
123-5631 341
123-5631LTM 341
123-5632 341
123-5632LTM 341
123-5701 315
123-5701LTM 315
123-5711 315
123-5711E 315
123-5731 315
123-5731E 315
123-5731LTM 315
123-6133 389
123-6133LTM 389
123-6412 389
123-6412LTM 389
123-6432 389
123-6432LTM 389
123-6462 389
123-7012 305
123-7012LTM 305
123-7013 305
123-7013LTM 305
123-7031 305
123-7031LTM 305
123-7032 305
123-7032E 305
123-7032LTM 305

123-7033 305
123-7033E 305
123-7033LTM 305
123-7062 ..... 232, 305
123-7063 305
123-7063E 305
123-7312 306
123-7312LTM 306
123-7314 306
123-7314LTM 306
123-7332 306
123-7332LTM 306
123-7333 306
123-7333LTM 306
123-7334 306
123-7334LTM 306
123-7354 306
123-7354E 306
123-7362 306
123-7363 306
123-7364 ..... 236, 306
123-7722 334
123-7722LTM 334
123-7732 334
123-7732E 334
123-7732LTM 334
123-8232 ..... 213-214, 216, 222, 225, 333
123-8336 ..... 213-214, 216, 222, 225, 333
123-9134 362
123-9134LTM 362
123-9234 362
123-9234E 362
123-9234LTM 362
123-9612 338
123-BD01 329
123-BD11 329
123-BD34 329
124-0034 349
124-0034LTM 349
124-1032 271
124-1032LTM 271
124-1034 271
124-1034LTM 271
124-1334 ..... 231, 234, 345
124-1334LTM 345
124-1374 ..... 217, 345
124-1474 349
124-14A4 349
124-1534 ..... 232, 347
124-1534LTM 347
124-1574 ..... 232, 347
124-1632 350
124-1730 336
124-1730LTM 336
124-3232 ..... 233, 310
124-3232LTM 310
124-5012 283
124-5012LTM 283
124-5032 283
124-5032LTM 283
124-5037 283
124-5037LTM 283
124-7032 ..... 231, 233, 305
124-7032LTM 305
125-0034 349
125-0034E 349
125-0034LTM 349
125-0212 ..... 230, 296
125-0212LTM 296
125-0232 296
125-0232LTM 296
125-0334UI 364
125-0712 301
125-0712E 301
125-0712LTM 301
125-0731 301
125-0731LTM 301
125-0732 301
125-0732E 301
125-0732G 391
125-0732LTM 301
125-0733 301
125-0733LTM 301
125-0737 301
125-0737LTM 301
125-0762 301
125-0762E 301
125-1002 272
125-1002LTM 272
125-1005 272
125-1005LTM 272
125-100A 272, 274
125-100ALTM 272
125-100B 272
125-100BLTM 272
125-1011 272
125-1011E 272
125-1011LTM 272
125-1012 272
125-1012E 272
125-1012LTM 272
125-1014 272
125-1014LTM 272
125-1015 272
125-1015LTM 272
125-1017 272
125-1017LTM 272
125-101J 272
125-101JLTM 272
125-101K 272
125-101KLTM 272
125-1025 272
125-1025LTM 272
125-102J 272
125-102JLTM 272
125-1032 272
125-1032LTM 272
125-1034 ..... 234, 272
125-1034E 272
125-1034LTM 272
125-1035 ..... 229, 235-236, 272
125-1035E 272
125-1035LTM 272
125-1037 272
125-1037LTM 272
125-1039 272
125-103B 272
125-103BLTM 272
125-103J 272
125-103JLTM 272
125-103K 272
125-103KE 272
125-103KLTM 272
125-1055 272
125-1062 272
125-1062E 272
125-1064 272
125-1065 272
125-1065E 272
125-106J 272
125-106JE 272
125-10B5 272
125-10H5 272
125-10H5LTM 272
125-10HB 272
125-10HBE 272
125-10HBLTM 272
125-1131 314
125-1212 254
125-1212LTM 254
125-1232 254
125-1232LTM 254
125-1312 299
125-1312LTM 299
125-1314 345
125-1332 299
125-1332LTM 299
125-1333 299
125-1333LTM 299
125-1334 ..... 230-231, 236, 345
125-1334E 345
125-1334G5 391
125-1334LTM 345
125-1334UI 242, 344
125-1364 345
125-1364E 345
125-1374 ..... 217, 345
125-1374E 345
125-1374UI 242, 344
125-14A4 349
125-1704 291
125-1704LTM 291
125-1710 336
125-1710LTM 336
125-1711 291
125-1711LTM 291
125-1712 291
125-1712LTM 291
125-1713 291
125-1713LTM 291
125-1717 291
125-1717LTM 291
125-1730 ..... 233, 336
125-1730LTM 336
125-1731 291
125-1731LTM 291
125-1732 291
125-1732E 291
125-1732LTM 291
125-1733 291
125-1733LTM 291
125-1737 291
125-1737LTM 291
125-1762 291
125-1912 289
125-1912LTM 289
125-1932 289
125-1932LTM 289
125-1937 289
125-1937LTM 289
125-2032 295
125-2032LTM 295
125-2212 ..... 223, 297
125-2212LTM 297
125-2232 297
125-2232LTM 297
125-2237 297
125-2237LTM 297
125-2312 294
125-2312LTM 294
125-2332 294
125-2332LTM 294
125-2814 ..... 230-231, 234, 322
125-2814E 322
125-2814LTM 322
125-3212 310
125-3212LTM 310
125-3217 310
125-3217LTM 310
125-3231 310
125-3231LTM 310
125-3232 310
125-3232E 310
125-3232LTM 310
125-3233 310
125-3233LTM 310
125-3237 310
125-3237LTM 310
125-3262 310
125-32H2 310
125-32H2LTM 310
125-3832 256
125-3832LTM 256
125-3837 256
125-3837LTM 256
125-5012 ..... 223, 283
125-5012E 283
125-5012LTM 283
125-5017 283
125-5017LTM 283
125-501J 283
125-501JLTM 283
125-501K 283
125-501KLTM 283
125-5025 283
125-5025LTM 283
125-5032 ..... 233, 283
125-5032E 283
125-5032LTM 283
125-5034 283
125-5034E 283
125-5034LTM 283
125-5035 283
125-5035E 283
125-5035LTM 283
125-5037 283
125-5037LTM 283
125-503B 283
125-503BLTM 283
125-503D 283
125-503DLTM 283
125-503J 283
125-503JLTM 283
125-503K 283
125-503KLTM 283
125-5062 283
125-5062E 283
125-5065 283
125-5065E 283
125-50HB 283
125-50HBLTM 283
125-5512 250
125-5512LTM 250
125-5532 250
125-5532LTM 250
125-5537 250
125-5537G 391
125-5537LTM 250

125-553J....250
125-553JLTM....250
125-6837....220-222, 225-226, 336
125-6837LTM....336
125-7012....305
125-7012E....305
125-7012LTM....305
125-7017....305
125-7017LTM....305
125-7031....305
125-7031LTM....305
125-7032....230-231, 305
125-7032E....305
125-7032LTM....305
125-7037....305
125-7037LTM....305
125-7062....305
125-7062E....305
125-7312....306
125-7312LTM....306
125-7314....306
125-7314LTM....306
125-7332....306
125-7332E....306
125-7332LTM....306
125-7333....306
125-7333LTM....306
125-7334....306
125-7334E....306
125-7334LTM....306
125-7362....306
125-7732....334
125-7732LTM....334
125-9134....362
125-9134E....362
125-9134LTM....362
125-9234....362
125-9234LTM....362
126-1012....269
126-1012LTM....269
126-1013....269
126-1013LTM....269
126-1713....291
126-1713LTM....291
126-7012....304
126-7012LTM....304
126-7013....304
126-7013LTM....304
127-0112....245
127-0112LTM....245
127-0113....245
127-0122....245
127-0123....245
127-0123LTM....245
127-0722....301
127-0722LTM....301
127-0723....301
127-0723LTM....301
127-100A....269
127-100ALTM....269
127-1012....269
127-1012E....269
127-1012LTM....269
127-1013....269
127-1013E....269
127-1013LTM....269
127-1022....269
127-1022E....269
127-1022LTM....269
127-1023....269
127-1023E....269
127-1023LTM....269
127-1043....269
127-1046....269
127-1046E....269
127-1712....291
127-1712LTM....291
127-1713....291
127-1713LTM....291
127-1722....291
127-1722LTM....291
127-2222....297
127-2222LTM....297
127-3212....310
127-3212LTM....310
127-32H2....310
127-32H2LTM....310
127-5012....281
127-5012E....281
127-5012LTM....281
127-5013....281
127-5013LTM....281
127-501E....281
127-501EE....281
127-501ELTM....281
127-501N....281
127-501NLTM....281
127-5022....281
127-5022E....281
127-5022LTM....281
127-5023....281
127-5023LTM....281
127-7012....304
127-7012E....304
127-7012LTM....304
127-7013....304
127-7013LTM....304
127-7022....304
127-7022LTM....304
127-7023....304
127-7023E....304
127-7023FF....305
127-7023LTM....304
128-0112....245
128-0112LTM....245
128-0122....245
128-0122E....245
128-0122LTM....245
128-1012....270
128-1012LTM....270
128-1022....270
128-1022LTM....270
128-1034....270
128-1034LTM....270
128-1052....270
128-1056....235, 321
128-1212....254
128-1212E....254
128-1222....254
128-1324....345
128-1324E....345
128-1324LTM....345
128-3812....256
128-3822....256
128-5012....282
128-5012LTM....282
128-5022....282
128-5022LTM....282
128-5052....282
128-50H7....282
128-50H7LTM....282
128-5512....250
128-5512LTM....250
128-5522....250
128-5522LTM....250
128-5552....250
128-7022....305
128-7022LTM....305
128-7032....305
128-7032LTM....305
128-7052....305
128-7323....306
128-7323LTM....306
128-8522....363
12A-1015....270
12A-1015LTM....270
12A-5015....281
12A-5015LTM....281
1300502506....48
1390-1023....76
14-8911-003....51
1400-0015....105
145-1001....236, 322, 365-366
145-1009....322, 365-366
145-1011....234, 366
145-1032....366
145-1334....367
145-2814....365-366
145-7032....367
1500334701....166, 168
1530-2163....42
1530-2167....42
1535-4952....40, 46
1535-4954....40
160-1010-1....397
160-1010-10....397
160-1010-5....397
160-2200-10....399
160-2200-5....399
160-2205-1....397
160-2205-10....397
160-2205-5....397
160-2250-10....399
160-2250-5....399
160-2255-1....398
160-2255-10....398
160-2255-30....398
160-2255-5....37, 46, 398
160-2320-10....399
160-2320-5....399
160-2325-1....398
160-2325-10....398
160-2325-30....398
160-2325-5....37, 46, 398
160-2450-10....399
160-2450-5....399
160-2455-1....398
160-2455-10....398
160-2455-5....46, 398
160-2530-10....399
160-2530-5....399
160-2535-1....398
160-2535-10....398
160-2535-30....398
160-2535-5....37, 46, 398
160-2610-10....399
160-2610-5....399
160-2615-1....397
160-2615-10....397
160-2615-5....397
160-2625-1....37, 397
160-2625-10....37, 397
160-2625-5....37, 397
160-2634-10....399
160-2634-5....399
160-2635-1....397
160-2635-10....397
160-2635-5....397
160-2644-10....399
160-2644-5....399
160-2650-10....399
160-2650-5....399
160-2655-1....397
160-2655-10....397
160-2655-5....397
160-2660-5....399
160-2815-5....398
160-2825-5....398
160-2845-10....398
160-2845-5....398
160-2855-10....398
160-2855-5....398
160-2865-10....398
160-2865-5....398
160-4535-5....46, 398
18596-40015....44
18710-20119....81, 85, 104-105
18710-60170....85, 91
18711-60060....91
18713-60040....88
18713-60050....88
18740-20800....63
18740-20880....56, 63
18740-60830....62
18740-60835....62, 64, 71-72, 76-77
18740-60840....27
18740-80190....27
18740-80200....26
18740-80220....26
18789-60060....105
18789-80070....81
18900-20250....42
18900-20280....42
18900-20281....42
18900-20300....42
18900-60640....108
18900-80255....42
19091-20050....399
19091-21050....399
19091-60010....387
19091-60010E....387
19091-60312....273
19091-60620E....397
19091A-002....279
19091A-002LTM....279
19091A-005....279
19091A-008....279
19091A-008LTM....279
19091A-012....279
19091A-012LTM....279
19091A-015....279
19091A-101....279
19091A-101LTM....279
19091A-102....279
19091A-102E....279
19091A-102LTM....279
19091A-105....279
19091A-108....279
19091A-108LTM....279
19091A-112....279

19091A-112LTM....279
19091A-115....279
19091B-002....280
19091B-002LTM....280
19091B-005....280
19091B-012....280
19091B-012E....280
19091B-012LTM....280
19091B-015....280
19091B-101....280
19091B-101LTM....280
19091B-102....280
19091B-102E....280
19091B-102LTM....280
19091B-105....280
19091B-105E....280
19091B-112....280
19091B-112LTM....280
19091B-115....280
19091B-115E....280
19091F-102....311
19091F-102E....311
19091F-102LTM....311
19091F-105....311
19091F-105E....311
19091F-112....311
19091F-112E....311
19091F-112LTM....311
19091F-115....311
19091F-115E....311
19091F-413....311
19091F-413LTM....311
19091F-433....311
19091F-433E....311
19091F-433LTM....311
19091G-113....290
19091G-113LTM....290
19091G-131....290
19091G-131E....290
19091G-131LTM....290
19091G-133....290
19091G-133LTM....290
19091G-213....290
19091G-213LTM....290
19091G-B113....359
19091G-B133....359
19091G-B213....359
19091G-B213E....359
19091G-B233....359
19091G-B233E....359
19091J-002....284
19091J-002LTM....284
19091J-005....284
19091J-012....285
19091J-012E....285
19091J-012LTM....285
19091J-015....285
19091J-015E....285
19091J-101....284
19091J-101LTM....284
19091J-102....284
19091J-102E....284
19091J-102LTM....284
19091J-105....284
19091J-105E....284
19091J-108....284
19091J-112....285
19091J-112E....285
19091J-112LTM....285
19091J-113....285
19091J-113E....285
19091J-113LTM....285
19091J-115....285
19091J-115E....285
19091J-202....284
19091J-202LTM....284
19091J-205....284
19091J-212....285
19091J-212LTM....285
19091J-213....285
19091J-213E....285
19091J-213LTM....285
19091J-215....285
19091J-215E....285
19091J-216....285
19091J-216E....285
19091J-231....284
19091J-231LTM....284
19091J-233....220, 284
19091J-233LTM....284
19091J-236....284
19091J-236E....284
19091J-313....285
19091J-313LTM....285
19091J-330....284
19091J-330LTM....284
19091J-333....284
19091J-333LTM....284
19091J-411....285
19091J-411LTM....285
19091J-413....285
19091J-413E....285
19091J-413LTM....285
19091J-416....285
19091J-431....284
19091J-431E....284
19091J-431LTM....284
19091J-433....284
19091J-433E....284
19091J-433LTM....284
19091J-436....284
19091J-436E....284
19091J-577....284
19091J-577E....284
19091J-577LTM....284
19091L-101....292
19091L-101LTM....292
19091L-111....292
19091L-111LTM....292
19091L-113....292
19091L-113E....292
19091L-113LTM....292
19091L-133....292
19091L-133LTM....292
19091L-330....292
19091L-330LTM....292
19091L-333....292
19091L-333LTM....292
19091L-413....292
19091L-413E....292
19091L-413LTM....292
19091L-416....292
19091L-431....292
19091L-431LTM....292
19091L-433....292
19091L-433LTM....292
19091L-577....292
19091L-577LTM....292
19091N-013....307
19091N-013LTM....307
19091N-030....307
19091N-030LTM....307
19091N-033....307
19091N-033LTM....307
19091N-036....307
19091N-102....307
19091N-102LTM....307
19091N-105....307
19091N-105E....307
19091N-111....307
19091N-111LTM....307
19091N-113....233, 307
19091N-113E....307
19091N-113LTM....307
19091N-116....229, 236, 307
19091N-130....307
19091N-130LTM....307
19091N-131....307
19091N-131E....307
19091N-131LTM....307
19091N-133....307
19091N-133E....307
19091N-133LTM....307
19091N-136....229, 307
19091N-136E....307
19091N-202....307
19091N-202LTM....307
19091N-205....307
19091N-205E....307
19091N-213....307
19091N-213E....307
19091N-213LTM....307
19091N-216....232-233, 307
19091N-216E....307
19091N-231....221, 307
19091N-231LTM....307
19091N-233....227, 307
19091N-233E....307
19091N-233LTM....307
19091N-236....307
19091N-330....307
19091N-331....307
19091N-577....307
19091N-577E....307
19091N-577LTM....307
19091P-K15....374
19091P-K15E....374
19091P-K33....374
19091P-K33E....374
19091P-K33LTM....374
19091P-M15....380
19091P-M15E....380
19091P-MS4....384
19091P-MS4E....384
19091P-MS4LTM....384
19091P-MS7....384
19091P-MS7LTM....384
19091P-MS8....384
19091P-MS8LTM....384
19091P-QO3....371
19091P-QO3LTM....371
19091P-QO4....371
19091P-QO4E....371
19091P-QO4LTM....371
19091P-S12....378
19091P-S12LTM....378
19091P-S15....378
19091P-S15E....378
19091P-S33....378
19091P-S33LTM....378
19091P-UO4....374
19091P-UO4E....374
19091P-UO4LTM....374
19091R-303....348
19091R-303LTM....348
19091R-306....215, 219, 225, 348
19091R-316....348
19091R-319....348
19091S-001....233-234, 319
19091S-001E....319
19091S-010....337
19091S-010LTM....337
19091S-101....251
19091S-101LTM....251
19091S-102....251
19091S-102E....251
19091S-102LTM....251
19091S-105....251
19091S-112....251
19091S-112E....251
19091S-112LTM....251
19091S-113....218, 223-224, 251
19091S-113LTM....251
19091S-133....215, 218, 222-223, 226-227, 251
19091S-133LTM....251
19091S-133UI....219, 224, 241
19091S-133UILTM....241
19091S-139....342
19091S-139LTM....342
19091S-213....227, 233, 251
19091S-213LTM....251
19091S-213UI....241
19091S-213UILTM....241
19091S-231....251
19091S-231LTM....251
19091S-233....251
19091S-233E....251
19091S-233LTM....251
19091S-233UI....214, 241
19091S-233UIE....241
19091S-233UILTM....241
19091S-313....251
19091S-313LTM....251
19091S-331....251
19091S-331LTM....251
19091S-333....251
19091S-333LTM....251
19091S-336....251
19091S-413....236, 251
19091S-413E....251
19091S-413LTM....251
19091S-413UI....225, 241
19091S-413UILTM....241
19091S-416....251
19091S-431....251
19091S-431LTM....251
19091S-431UI....215, 241
19091S-431UILTM....241
19091S-433....215, 234-235, 251
19091S-433E....251
19091S-433LTM....251
19091S-433UI....214, 216, 219, 241
19091S-433UIE....241
19091S-433UILTM....241
19091S-436....251
19091S-436E....251
19091S-436UI....241
19091S-510....363
19091S-510E....363

19091S-510LTM....363
19091S-577....251
19091S-577LTM....251
19091S-577UI....214, 241
19091S-577UILTM....241
19091S-602....246
19091S-602E....246
19091S-602LTM....246
19091S-612....246
19091S-612LTM....246
19091S-612UI....240
19091S-633....246
19091S-633LTM....246
19091S-633UI....240
19091S-677....246
19091S-677E....246
19091S-677LTM....246
19091S-677UI....240
19091S-677UIE....240
19091S-713....231, 234, 246
19091S-713LTM....246
19091S-713UI....240
19091S-733....246
19091S-733E....246
19091S-733LTM....246
19091S-733UI....240
19091S-733UIE....240
19091S-833....246
19091S-833LTM....246
19091S-911....246
19091S-911LTM....246
19091S-911UI....240
19091S-913....246
19091S-913E....246
19091S-913LTM....246
19091S-913UI....240
19091S-913UIE....240
19091S-916....246
19091S-931....246
19091S-931E....246
19091S-931LTM....246
19091S-931UI....240
19091S-931UIE....240
19091S-933....246
19091S-933E....246
19091S-933LTM....246
19091S-933UI....240
19091S-933UIE....240
19091S-936....246
19091S-936E....246
19091W-012....313
19091W-012E....313
19091W-012LTM....313
19091W-015....313
19091W-015E....313
19091W-102....313
19091W-102LTM....313
19091W-105....313
19091Y-012....387
19091Y-012E....387
19091Y-012LTM....387
19091Y-015....387
19091Y-101....387
19091Y-102....387
19091Y-102LTM....387
19091Y-105....387
19091Z-002....273
19091Z-002LTM....273
19091Z-005....273
19091Z-008....273
19091Z-008LTM....273
19091Z-012....274
19091Z-012E....274
19091Z-012LTM....274
19091Z-015....274
19091Z-102....273
19091Z-102E....273
19091Z-102LTM....273
19091Z-105....273
19091Z-112....274
19091Z-112E....274
19091Z-112LTM....274
19091Z-115....232, 236, 274
19091Z-115E....274
19091Z-202....273
19091Z-202LTM....273
19091Z-205....273, 319
19091Z-205E....319
19091Z-211....274
19091Z-211LTM....274
19091Z-212....274
19091Z-212LTM....274
19091Z-213....274
19091Z-213E....274
19091Z-213LTM....274
19091Z-215....274
19091Z-216....274
19091Z-216E....274
19091Z-231....273
19091Z-231LTM....273
19091Z-233....273
19091Z-233E....273
19091Z-233LTM....273
19091Z-236....235-236, 273
19091Z-236E....273
19091Z-313....274
19091Z-313E....274
19091Z-313LTM....274
19091Z-331....273
19091Z-331LTM....273
19091Z-333....273
19091Z-333LTM....273
19091Z-411....274
19091Z-411E....274
19091Z-411LTM....274
19091Z-413....274
19091Z-413E....274
19091Z-413LTM....274
19091Z-416....274
19091Z-431....273
19091Z-431LTM....273
19091Z-433....273
19091Z-433E....273
19091Z-433LTM....273
19091Z-436....273
19091Z-513....274
19091Z-513E....274
19091Z-513LTM....274
19091Z-530....234, 273, 319
19091Z-530E....273, 319
19091Z-577....273
19091Z-577E....273
19091Z-577LTM....273
19091Z-613....235, 274
19091Z-613LTM....274
19091Z-713....274
19091Z-713E....274
19091Z-713LTM....274
19091Z-716....274
19095F-120....311
19095F-120E....311
19095F-120LTM....311
19095F-121....311
19095F-121LTM....311
19095F-123....311
19095F-123E....311
19095F-123LTM....311
19095J-023....285
19095J-023E....285
19095J-023LTM....285
19095J-121....285
19095J-121E....285
19095J-121LTM....285
19095J-123....285
19095J-123E....285
19095J-123LTM....285
19095J-321....223, 285
19095J-321LTM....285
19095J-323....285
19095J-323E....285
19095J-323LTM....285
19095J-621....285
19095J-621LTM....285
19095J-623....236, 285
19095J-623E....285
19095J-623LTM....285
19095L-021....292
19095L-021LTM....292
19095L-023....292
19095L-023E....292
19095L-023LTM....292
19095L-121....387
19095L-121LTM....387
19095L-523....292
19095L-523E....292
19095L-523LTM....292
19095N-121....307
19095N-121E....307
19095N-121LTM....307
19095N-123....307
19095N-123E....307
19095N-123LTM....307
19095N-126....307
19095P-K23....229, 374
19095P-K23LTM....374
19095P-K25....236, 374
19095P-K25E....374
19095P-M23....380
19095P-M23LTM....380
19095P-M25....380
19095P-MS0....229, 384
19095P-MS0E....384
19095P-MS0LTM....384
19095P-MS5....384
19095P-MS5LTM....384
19095P-MS6....384
19095P-MS6E....384
19095P-MS6LTM....384
19095P-MS9....229, 384
19095P-MS9LTM....384
19095P-QO3....229, 233, 235, 371
19095P-QO3E....371
19095P-QO3LTM....371
19095P-QO4....234-235, 371
19095P-QO4E....371
19095P-QO4LTM....371
19095P-S21....378
19095P-S21LTM....378
19095P-S23....229, 378
19095P-S23LTM....378
19095P-S25....232, 378
19095P-S25E....378
19095P-UO3....374
19095P-UO3LTM....374
19095P-UO4....235, 374
19095P-UO4E....374
19095P-UO4LTM....374
19095R-420....348
19095R-429....348
19095S-100....274
19095S-100E....274
19095S-100LTM....274
19095S-200....321
19095S-205....321
19095V-420....364
19095V-420E....364
19095V-420LTM....364
19095W-121....313
19095W-121LTM....313
19095W-123....313
19095W-123LTM....313
19095Z-020....230, 274
19095Z-021....230, 274
19095Z-021E....274
19095Z-021LTM....274
19095Z-023....274
19095Z-023E....274
19095Z-023LTM....274
19095Z-121....274
19095Z-121E....274
19095Z-121LTM....274
19095Z-123....274
19095Z-123E....274
19095Z-123LTM....274
19095Z-220....274
19095Z-221....274
19095Z-221E....274
19095Z-321....274
19095Z-321LTM....274
19095Z-323....274
19095Z-323E....274
19095Z-323LTM....274
19095Z-421....274
19095Z-421LTM....274
19095Z-423....274
19095Z-423E....274
19095Z-423LTM....274
19095Z-621....233, 274
19095Z-621LTM....274
19095Z-623....274
19095Z-623E....274
19095Z-623LTM....274
19095Z-626....236, 274
19095Z-627....234, 274
19095Z-627E....274
19095Z-627LTM....274
1909BD-113....329
19231-20910....84
19231-20940....84
19231-20990....84
19231-21050....84
19231-21060....84
19231-60680....84-85
19231-80520....84-85, 105
19231-80530....84-85, 105
19233-20625....88
19233-20755....88
19234-60700....76
19234-60715....76
19234-60720....77, 84, 88, 105

19243-000681 64
19243-00070 63
19243-80530 77
19243-80540 77
19243-80570 76-77
19244-80540 76-77
19244-80560 ..... 81, 85, 104-105
19244-80610 ..... 84-85, 105
19244-80620 ..... 81, 104
19251-00100 63
19251-60540 ..... 25, 63
19251-60575 62
19256-00090 100
19256-00200 100
19256-00320 100
19256-20550 99
19256-20580 99
19256-20590 99
19256-20690 99
19256-20705 99
19256-20900 100
19256-20910 100
19256-60510 100
19256-60700 99
19256-60800 99
19256-80000 100
19256-80010 100
19256-80030 99
19256-80045 99
19256-80560 99
19256-80600 99
19258-20830 49
19258-20870 49
19298-60500 108
19301-00150 85
19301-20720 85
19301-60660 85
19325-60660 41
19354-60510 108
200-0010 411
200-0032 411
200-0070 411
200-0110 411
200-0113 411
200-0185 411
200-0310 411
200-0370 411
200187500 166
200187600 168
200193800 ..... 166, 168
210-3003 26
210-3003-5 26
210-4004-5 25
210-4022-5 25
2100003100 168
2100003200 ..... 166, 168
2190-0584 99
221-0122LTM 245, 395
221-1324LTM 345, 396
221-1524LTM 347, 396
221-3822LTM 256, 396
221-4722LTM 258, 396
221-5522LTM 250, 395
221-5522UILTM 395
221-6822LTM 336, 396
222-0112LTM 245, 395
222-0132LTM 245, 395
222-0732LTM 396
222-1032LTM 395
222-1111LTM 314, 395
222-1131LTM 314, 395
222-1334LTM 345, 396
222-1534LTM 347, 396
222-2912LTM 262, 396
222-2932LTM 262, 396
222-3212LTM 310, 396
222-3232LTM 310, 396
222-3812LTM 256, 396
222-3832LTM 256, 396
222-4712LTM 258, 396
222-4732LTM 258, 396
222-5512LTM 250, 395
222-5512UILTM 395
222-5532LTM 250, 395
222-5532UILTM 395
222-5711LTM 315, 395
222-5731LTM 315, 395
222-7013LTM 304, 396
222-7033LTM 305, 396
2302533140 48
2307230001 48
2307232901 48
232-2790010-EHS 49
232-2790012-EHS 49
2321700003 48-49
2321700004 48-49
2322590004 48-49
2322590005 48-49
2322700011 48
2710100200 135
2710100400 135
2710100500 135
2722990700 136
2735000500 135
2740236100 168
2740292400 167
2740928202 168
29091N-133LTM 307, 396
29091N-577LTM 307, 396
29091R-303LTM 348, 396
29091S-431UILTM 395
29091S-433LTM 246, 251, 396
29091S-433UILTM 395
29091S-577UILTM 395
29091S-677LTM 246, 395
29091S-833LTM 246, 395
29091S-931LTM 246, 395
2950-0232 41
301-011-HSP 49
301-015-HSP 49
301-016-HSP 49
301-017-HSP 49
301-152-HSP 49
301-169-HSP 49
301-170-HSP 49
301-205-HSP 49, 62
301-211-HSP 49
301-212-HSP 49
3150-0602 71
3162-1057 132
321-002-HSP 49
321-055-HSP 49
321-056-HSP 49
321-057-HSP 49
325-062-HSP 49
325-132-HSP 49
325-185-HSP 49
3600500001 49
3600500002 49
390607400 168
390607401 168
390607900 168
390812700 164-165
390820601 161-165
390842300 161-165
391821100 163
391866306 163
391866308 161
391867600 162
392017401 134
392027300 135-136
392027500 136
392030500 135-136
392035300 135-136
392043700 136
392047100 136
392511901 167-168
392512800 168
392513800 167
392514300 167-168
392514500 167-168
392515101 167
392515102 167
392515103 167
392515104 167
392515105 167
392515500 167-168
392517100 167
392517600 167
392517700 167
392517800 167
392517901 167
392519200 167
392543101 165
392544001 162
392544011 162
392544391 167
392548201 165
392548301 164
392560591 166
392561290 166
392567111 134
392585291 166
392585292 166
392595501 164-165
392597101 161
392597301 161
392597302 161
392597303 161
392597501 161
392599401 161
392599411 161
392599501 161
392609901 21
392609902 21
392609903 21
393001991 136
393010918 134
393010920 134
393010924 134
393011391 136
393031501 136
393050292 136
393050293 136
393050392 136
393050393 136
393050492 136
393050493 136
393053501 136
393053502 ..... 134, 136
393060191 136
393065201 138
393082491 134
393101291 134
393112601 135
393112702 135
393113001 135
393161001 134
393164493 134
393167593 134
393171201 134
393175101 134
393847701 135
394958700 166
394966601 162-163
4177-0607 46
500-1200 38
500-2114 33
500-2118 33
5020-8292 34
5020-8293 34
5020-8294 34
5021-7133 39
5021-7134 39
5021-7136 39
5021-7137 39
5021-7146 39
5021-7148 39
5021-7164 39
5021-7166 39
5021-7168 39
5021-7169 39
5021-7170 39
5040-4669 47
5060-9086 108
5061-5869 63
5061-5886 100
5061-5890 100
5061-5896 ..... 116, 133
5062-0208 47
5062-3506 ..... 33, 117
5062-3507 33
5062-3508 ..... 33, 117
5062-3511 33
5062-3512 33
5062-3513 33
5062-3514 33
5062-3515 33
5062-3516 33
5062-3525 ..... 39, 71-72
5062-3538 33
5062-3587 ..... 26, 63
5062-9508 40
5062-9509 40
5062-9510 40
5062-9511 40
5080-4978 85
5080-5400 ..... 116, 133
5080-8716 108
5080-8728-100 19
5080-8728-50 19
5080-8732 76-77
5080-8750 77
5080-8751 77
5080-8755 108
5080-8756 108
5080-8759 108
5080-8761 108
5080-8768 108
5080-8769 108

5080-8773 ..... 91, 105
5080-8774 ..... 76-77, 88, 91, 99, 105
5080-8853 ..... 33, 91, 105
5080-8858 411
5080-8894-100 19
5080-8896-50 19
5080-8898 76-77
5180-4103 91-92
5180-4105 ..... 76-77, 88, 91, 105
5180-4150 85
5180-4152 85
5180-4153 ..... 63, 85
5180-4165 82
5180-4168 ..... 29, 62
5180-4173 ..... 29, 62
5180-4181 84
5180-8830 76
5181-1260 19
5181-1261 19
5181-1291 41
5181-1292 41
5181-3308 33
5181-3311 84
5181-3315 26
5181-3316 ..... 26, 62
5181-3316i 26
5181-3322 33
5181-3323 ..... 33, 117
5181-3351 386
5181-3352 386
5181-3382 77
5181-3395 38
5181-3396 38
5181-3397 38
5181-3398 38
5181-7459 40
5181-7460 40
5181-8815 20
5181-8816 20
5181-8818 ..... 26, 63
5181-8830 ..... 34, 63, 77, 91, 105, 117
5181-8833 20
5181-8836 46
5181-8838 63
5181-8839 20
5181-8863 116
5181-8866 68
5182-0551 43
5182-0739 76
5182-0773 51
5182-0774 51
5182-0775 51
5182-0781 51
5182-0783 51
5182-0794 50
5182-0795 50
5182-0796 50
5182-0831 68
5182-0832 68
5182-0833 68
5182-0836 68
5182-0837 47
5182-0838 47
5182-0840 47
5182-0844 50
5182-0845 50
5182-0846 50
5182-0847 50
5182-0848 50
5182-0849 50
5182-0850 50
5182-0851 50
5182-0852 50
5182-0853 20
5182-3438 21
5182-3439 21
5182-3442 20
5182-3444 ..... 20, 64, 71, 77
5182-3445 ..... 20, 64, 71, 76-77
5182-3450 85
5182-3466 117
5182-3477 92
5182-8815 76
5182-9651 73
5182-9652 ..... 56, 63
5182-9673 92
5182-9676 92
5182-9677 92
5182-9679 92
5182-9722 105
5182-9733 48-49
5182-9747 71
5182-9748 71-72
5182-9749 71
5182-9754 71
5182-9756 71
5182-9757 71-72
5182-9758 71-72
5182-9759 71-72
5182-9760 71-72
5182-9761 71
5182-9762 71
5182-9763 71-72
5182-9768 71
5182-9769 71
5182-9770 71
5182-9775 71-72
5183-0318 73
5183-0379 88
5183-2007 ..... 101, 105
5183-2036 ..... 28, 73
5183-2037 ..... 28, 73
5183-2038 ..... 28, 73
5183-2058 73
5183-2096 116
5183-4477 47
5183-4647 ..... 24-26, 62
5183-4691 25
5183-4692 25
5183-4693 26
5183-4694 26
5183-4695 26
5183-4696 ..... 26, 62
5183-4697 27
5183-4698 27
5183-4699 27
5183-4700 27
5183-4701 24-28
5183-4702 ..... 24-28, 62
5183-4703 26
5183-4704 26
5183-4705 26
5183-4706 26
5183-4707 26
5183-4708 26
5183-4709 26
5183-4710 26
5183-4711 25
5183-4712 25
5183-4713 25
5183-4732 ..... 34, 63, 91
5183-4741 52
5183-4757 ..... 16, 62-64, 77
5183-4757-100 16
5183-4758 16
5183-4759 17
5183-4759-100 17
5183-4760 17
5183-4761 17
5183-4761-100 17
5183-4762 17
5184-3569 117
5184-3570 117
5184-3571 ..... 117, 124
5188-1447 51
5188-1448 51
5188-2717 ..... 57, 63
5188-5241 63
5188-5245 99
5188-5311 29
5188-5312 34
5188-5313 ..... 28, 73
5188-5315 35
5188-5316 108
5188-5317 108
5188-5347 138
5188-5348 138
5188-5356 ..... 28, 73
5188-5357 138
5188-5361 ..... 35, 37, 41, 124
5188-5362 ..... 35, 37, 41, 124
5188-5363 ..... 35, 37, 41, 124
5188-5365 ..... 29, 62-64
5188-5366 ..... 29, 57, 62
5188-5367 ..... 56, 63
5188-5372 85
5188-5379 411
5188-5953 99
5188-6471 27
5188-6493 ..... 55, 62
5188-6494 ..... 55, 62
5188-6495 ..... 55, 63
5188-6496 ..... 55, 62
5188-6497 ..... 55, 62
5188-6498 ..... 55, 77
5188-8813 51
5188-8814 51
5188-8815 51
5188-8816 51
5188-8817 51
5188-8818 51
5188-8819 51
5188-8820 51
5188-8821 51
5188-8822 51
5190-0468 137
5190-0471 137
5190-0472 137
5190-0473 137
5190-0490 137
5190-0493 137
5190-0494 137
5190-1407 329
5190-1408 329
5190-1409 329
5190-1410 329
5190-1426 ..... 28, 73
5190-1437 46
5190-1438 46
5190-1441 137
5190-1445 51
5190-1446 51
5190-2209 ..... 14, 56
5190-2231 51
5190-2232 51
5190-2233 51
5190-2234 51
5190-2235 51
5190-2265 48
5190-2266 48
5190-2268 ..... 14, 29, 57
5190-2269 ..... 14, 29
5190-2270 ..... 14, 26
5190-2271 ..... 14, 26
5190-2272 ..... 14, 26
5190-2275 ..... 14, 25
5190-2292 24
5190-2293 24
5190-2294 24
5190-2295 ..... 24, 62
5190-2296 ..... 27, 64
5190-2297 ..... 24, 27
5190-3157 ..... 14, 16
5190-3158 ..... 14, 17
5190-3162 24
5190-3163 24
5190-3164 24
5190-3165 24
5190-3166 ..... 24, 62
5190-3167 24
5190-3168 24
5190-3169 ..... 24, 62
5190-3170 ..... 14, 24
5190-3171 ..... 14, 24
5190-3172 ..... 14, 24
5190-3173 ..... 14, 24
5190-3976 52
5190-3978 52
5190-3983 24
5190-4006 ..... 24, 27
5190-4007 24
5190-4022 14
5190-4023 14
5190-4024 14
5190-4047 ..... 24, 27
5190-4048 ..... 24, 27
5190-4054 33
5958-9441 44
5958-9442 44
5958-9443 44
5958-9444 44
5958-9445 44
5958-9450 44
5982-0024 137
5982-0025 137
6040-0289 ..... 131, 133
6040-0621 132
6040-0809 131-132
6040-0834 131
621-9723 ..... 242, 340
622-9732 ..... 242, 340
6410090050 48
705-0825 38
705-0903 38
705-0905 38
705-0925 38
7200008400 161-165
8001-0004 180
8001-0005 180
8001-0006 180
8001-0007 180

8001-0010 180
8001-0011 180
8001-0012 180
8001-0013 180
8001-0014 180
8001-0101 175-177
8001-0102 175, 177
8001-0103 175-177
8001-0104 176
8001-0105 178
8001-0106 175-176
8001-0151 175-177
8001-0152 175, 177
8001-0153 175-177
8001-0154 176
8001-0155 178
8001-0156 175-176
8001-0157 175-177
8001-0158 175-177
8001-0159 175-177
8001-0160 175-177
8001-0162 176
8001-0163 176
8001-0201 178
8001-0202 178
8001-0203 178
8001-0211 179
8001-0212 179
8001-0213 179
8001-0214 179
8001-0221 179
8001-0222 179
8001-0223 179
8001-0224 179
8001-0311 180
8001-0312 180
8002-0001 184
8002-0002 184
8002-0003 184, 187
8002-0004 184, 187
8002-0005 184, 187
8002-0101 182
8002-0102 182
8002-0103 182
8002-0104 182
8002-0105 182
8002-0106 182
8002-0107 182
8002-0151 182
8002-0152 182
8002-0153 182
8002-0154 182
8002-0155 182
8002-0156 182
8002-0157 182
8002-0159 182
8002-0160 182
8002-0161 182
8002-0201 183
8002-0203 183
8002-0204 183
8002-0211 183
8002-0212 183
8002-0213 183
8002-0214 183
8002-0215 183
8002-0216 183
8002-0217 183
8002-0220 183
8002-0221 183
8002-0222 183
8002-0311 184
8002-0312 184
8003-0001 173
8003-0002 173
8003-0003 173
8003-0004 173
8003-0005 173
8003-0006 173
8003-0007 173
8003-0008 173
8003-0101 169
8003-0102 169
8003-0103 169
8003-0104 170
8003-0105 169
8003-0106 169
8003-0107 169
8003-0108 170
8003-0109 170
8003-0110 169
8003-0111 169
8003-0151 169
8003-0152 169
8003-0153 169
8003-0154 170
8003-0155 170
8003-0157 169
8003-0158 169
8003-0159 169
8003-0160 169
8003-0162 169
8003-0163 170
8003-0165 169
8003-0166 169
8003-0202 170
8003-0203 170
8003-0204 170
8003-0205 170
8003-0211 172
8003-0212 172
8003-0216 171
8003-0219 172
8003-0221 172
8003-0222 172
8003-0223 172
8003-0311 172
8004-0001 158
8004-0002 158
8004-0003 158
8004-0004 158
8004-0005 158
8004-0006 158
8004-0007 158
8004-0101 154
8004-0102 154
8004-0103 154
8004-0104 154
8004-0105 154
8004-0106 154
8004-0107 154
8004-0108 155
8004-0109 155
8004-0110 155
8004-0111 156
8004-0112 155
8004-0113 154
8004-0114 154
8004-0116 154
8004-0118 155
8004-0119 154
8004-0151 154
8004-0152 154
8004-0153 154
8004-0154 154
8004-0155 154
8004-0156 154
8004-0157 154
8004-0158 154
8004-0159 155
8004-0160 155
8004-0161 155
8004-0162 155, 163
8004-0163 156
8004-0164 155, 162
8004-0165 154, 161
8004-0167 155, 163
8004-0168 156, 164
8004-0170 154
8004-0171 155
8004-0173 154
8004-0176 155
8004-0178 154
8004-0201 156, 159, 161, 174, 181, 185
8004-0202 156, 161
8004-0203 156
8004-0204 156, 162
8004-0211 157
8004-0212 157
8004-0213 157
8004-0214 157
8004-0215 157
8004-0216 157
8004-0217 158, 163-165
8004-0218 157
8004-0219 157
8004-0311 158, 161-165
8004-0312 158, 163
8010-0201 151, 159, 161, 185
8010-0202 151, 159, 185
8010-0203 151, 159, 164-165, 185
8010-0204 151, 159, 185
8010-0205 151, 159, 185
8010-0206 151, 159, 185
8010-0207 151, 159, 174, 185
8010-0208 151, 159, 174, 185
8010-0209 151, 159, 162-163, 185
8010-0210 151, 159, 185
8010-0211 151, 185-186
8010-0212 151, 185-186
8010-0213 151, 185
8010-0214 151, 185
8010-0215 151, 181
8010-0216 151, 181
8010-0217 150, 159-161, 185
8010-0218 150-153, 159, 174, 181, 185-186
8010-0219 150, 159, 164-165, 185
8010-0220 150, 159, 185
8010-0221 150, 159, 185
8010-0222 150, 159, 185
8010-0223 150, 159, 174, 185
8010-0224 150, 159, 174, 185
8010-0225 150, 159, 162-163, 185
8010-0226 150, 159, 185
8010-0227 150, 185
8010-0228 150, 185
8010-0229 150, 185
8010-0230 150, 185
8010-0231 150, 181
8010-0232 150, 181
8010-0233 152, 160-161, 186
8010-0234 152, 160, 186
8010-0239 152, 160, 174, 186
8010-0240 152, 160, 174, 186
8010-0241 152, 160, 162-163, 186
8010-0242 152, 160, 186
8010-0243 152, 186
8010-0244 152, 186
8010-0245 152, 186
8010-0246 152, 186
8010-0249 153, 160, 186
8010-0250 153, 160, 186
8010-0251 153, 160, 186
8010-0252 153, 160, 186
8010-0253 153, 160, 186
8010-0254 153, 160, 186
8010-0255 153, 160, 174, 186
8010-0256 153, 160, 174, 186
8010-0257 153, 160, 186
8010-0258 153, 160, 186
8010-0259 153, 186
8010-0260 153, 186
8010-0261 153, 186
8010-0262 153, 186
8010-0263 153, 181
8010-0264 153, 181
8010-0301 157, 171
8010-0302 157, 171
8010-0303 157, 171
8010-0304 157, 171
8010-0305 158, 163-165, 172
8010-0306 157, 171
8010-0307 157, 171
8010-0308 157, 171
8010-0309 157, 171
8010-0310 171, 179, 183
8010-0311 171, 179, 183
8010-0312 171, 179
8010-0313 171, 179
8010-0314 172, 179
8010-0315 172, 179
8010-0351 158, 184, 187
8010-0352 184, 187
8010-0353 184, 187
8010-0354 184, 187
8010-0355 184, 187
8010-0356 187
8010-0357 187
8010-0358 187
8010-0359 187
8010-0360 187
8010-0361 187
8010-0362 187
8010-0363 187
8010-0364 187
8010-0365 187
8010-0366 187
8010-0367 184, 187
8010-0368 184
8010-0401 170, 183
8500-0656 116, 138
8500-1233 116
8500-4789 63
8500-5440 138
8500-5808 138
8500-5851 138
8500-5995 138
8500-6812 411

8500-6813....411
8500-8510....138
8650-0029....116, 133
8650-0030....116, 133
8660-0791....116, 133
8710-0510....34, 117
8710-0899....117
8710-0900....117
8710-1220....117
8710-1346....85
8710-1561....85
8710-1615....117
8710-1622....117
8829951700....135
8829953800....135
9300003590....134
9301-0713....21, 73
9301-0723....43
9301-0892....21, 73
9301-0985....85
9301-1031....43
9310-4828....116, 133
998-0000053-EHS....49
C-102SSC....54
C-AT010C....54
C-B010M....53
C-BIO10....53
C-BTX1UG....54
C-CF020....53
C-CPLOK....53
C-DF010....53
C-G1CM10....54
C-GAT010C....54
C-GT010....53
C-HY010C....54
C-PL010....53
C-TBE10....53
C-TBP1C1C....54
C-TBP1CXC....54
C-TBP1TC....53
C-TNXTA....53
C-UN010C....54
CP0005....412
CP0031....412
CP1305....408
CP1306....409
CP1307....408
CP1308....408
CP1309....409
CP1480....408
CP1481....409
CP1482....408
CP1483....409
CP17973....132
CP17974....132
CP2045....409
CP2046....409
CP2047....408
CP2050....409
CP2055....408
CP2056....409
CP2057....408
CP2058....408
CP2059....409
CP2060....409
CP2062....408
CP2065....409
CP2068....408
CP2071....409
CP2072....409
CP2073....409
CP4016....386
CP4017....386
CP4018....386
CP4788....386
CP4789....386
CP4795....386
CP4796....386
CP5850....230
CP5881....247
CP5882....259
CP5883....259
CP5884....259
CP5885....260
CP5886....260
CP5887....257
CP5888....257
CP5889....257
CP5891....261
CP5892....261
CP5893....261
CP6172....353
CP6172I5....353
CP6173....353
CP6173I5....353
CP6174....353
CP6174I5....353
CP6175....353
CP6530....330
CP6540....324, 365-366
CP6550....324, 365-366
CP6560....324
CP6666....278, 366
CP6666I5....278, 366
CP6670....278, 366
CP6671....278, 366
CP6680....287, 367
CP6681....367
CP67569....366
CP6918....367, 376
CP6937....367, 385
CP6937I5....367, 385
CP6938....367, 385
CP6938I5....367, 385
CP6953....367, 370
CP6953I5....367, 370
CP6954....367, 370
CP6954I5....367, 370
CP6955....367, 370
CP6968....367, 377
CP7120....278, 366
CP7121....367
CP7125....366
CP7128....309
CP7129....367
CP7130....366
CP7135....278, 366
CP7135I5....278, 366
CP7138....309, 367
CP7140....278, 366
CP7141....367
CP7148....309, 367
CP7150....278, 366
CP7158....309, 367
CP7160....278, 366
CP7168....309, 367
CP7170....278, 366
CP7177....309, 367
CP7178....309, 367
CP7179....309, 367
CP7195....278, 366
CP7196....287, 367
CP7198....309, 367
CP7300....275
CP7310....275
CP7310I5....275
CP7311....275
CP7312....275
CP7313....275
CP7319....286
CP7319I5....286
CP7331....302
CP7334....308
CP7334I5....308
CP7335....308
CP7340....302
CP7347....368-369
CP7347I5....368
CP7348....368
CP7348I5....368
CP7350....231, 368
CP7350I5....368
CP7351....232-233, 368
CP7351I5....368
CP7352....368
CP7352I5....368
CP7353....231, 368
CP7353I5....368
CP7354....221, 232-233, 368
CP7354I5....368
CP7355....368
CP7360....302
CP7371....382
CP7372....382
CP7374....229, 382
CP7375....382
CP7406....336
CP7407....336
CP7407I5....336
CP7408....336
CP7409....336
CP7411....346
CP7411I5....346
CP7412....346
CP7413....346
CP7413I5....346
CP7414....230, 346
CP7414I5....346
CP7415....346
CP7415I5....346
CP7416....346
CP7416I5....346
CP7417....230, 346
CP7418....346
CP7419....354
CP7419I5....354
CP7420....354
CP7420I5....354
CP7421....354
CP7422....332
CP7422I5....332
CP7424....332
CP7428....232
CP7429....327
CP7430....327
CP7431....327
CP7432....327
CP7433....327
CP7434....331
CP7435....331
CP7437....331
CP7440....339, 367
CP7441....276
CP7442....276
CP7443....276
CP7443I5....276
CP7444....276
CP7444I5....276
CP7446....331
CP7447....331
CP7447I5....331
CP7448....331
CP7448I5....331
CP7451....286
CP7451I5....286
CP7452....287
CP7453....286
CP7453I5....286
CP7454....287
CP7461....338
CP7462....338
CP7463....357, 367
CP7475....319
CP7475I5....319
CP7476....342
CP7477....342
CP7478....342
CP7481....335
CP7482....232, 340
CP7483....357
CP7485....358
CP7485I5....358
CP7486....230, 358
CP7486I5....358
CP7487....354
CP7488....229-230, 354
CP7489....354
CP7491....351
CP749103....351
CP749106....351
CP7491I5....351
CP7493....351
CP7494....360
CP7494I5....360
CP7495....360
CP7495I5....360
CP7497....343
CP7498....343
CP7499....343
CP7500....361
CP7500I5....361
CP7501....361
CP7502....360
CP7502I5....360
CP7503....360
CP7503I5....360
CP7504....335
CP7511....376
CP7511I5....376
CP7512....324, 365-366
CP7512I5....324
CP7513....382
CP7514....382
CP7515....230, 376
CP7515I5....376
CP7516....376
CP7517....376
CP7518....229-230, 376
CP7519....376
CP7519I5....376

CP7521....323
CP7522....323
CP7522I5....323
CP7525....231-233, 235, 325
CP7525I5....325
CP7527....356
CP7527I5....356
CP7528....350
CP7529....234, 326
CP7529I5....326
CP7530....320
CP7530I5....320
CP7531....233, 320
CP7531I5....320
CP7532....230, 324, 365-366
CP7532I5....324, 365
CP7533....229, 385
CP7534....385
CP7534I5....385
CP7535....385
CP7535I5....385
CP7536....385
CP7536I5....385
CP7537....229, 385
CP7538....385
CP7538I5....385
CP7539....385
CP7540....385
CP7540I5....385
CP7541....323
CP7542....324, 365-366
CP7542I5....324, 365
CP7543....385
CP7544....385
CP7544I5....385
CP7548....369
CP7549....369
CP7549I5....369
CP7550....369
CP7550I5....369
CP7551....369
CP7551I5....369
CP7552....369
CP7553....369
CP7553I5....369
CP7554....230, 369
CP7554I5....369
CP7555....369
CP7556....370
CP7557....370
CP7557I5....370
CP7558....229, 370
CP7558I5....370
CP7559....370
CP7559I5....370
CP7561....377
CP7562....324, 365-366
CP7565....377
CP7565I5....377
CP7567....232, 377
CP7568....377
CP7569....324, 365-366
CP7569I5....324, 365
CP7570....230, 324, 365-366
CP7571....324, 365-366
CP7572....324, 365-366
CP7574....373
CP7574I5....373
CP7576....376
CP7577....376
CP7577I5....376
CP7579....373
CP7580....373
CP7581....373
CP7582....230, 324, 365-366
CP7582I5....324
CP7583....373
CP7583I5....373
CP7584....373
CP7584I5....373
CP7586....377
CP7587....377
CP7588....218-219, 227, 343
CP7591....332
CP7591I5....332
CP7592....231, 324, 365-366
CP7593....324, 365-366
CP7594....332
CP7595....332
CP7595I5....332
CP7596....217, 332
CP7596I5....332
CP7597....222, 332
CP7597I5....332
CP7598....224, 332
CP7598I5....332
CP7599....332
CP7602....275
CP7604....275
CP7608....277
CP7609....288
CP7614....233, 312
CP7614I5....312
CP7615....236, 356
CP7615I5....356
CP7617....356
CP7617I5....356
CP7619....288
CP7620....277
CP7620I5....277
CP7621....287
CP7622....275
CP7624....312
CP7625....277
CP7628....309
CP7629....288
CP7630....277
CP7631....287
CP7633....275
CP7634....287
CP7635....277
CP7635I5....277
CP7636....287
CP7637....303
CP7638....309
CP7640....277
CP7641....287
CP7642....275
CP7643....275
CP7643I5....275
CP7644....275
CP7644I5....275
CP7645....277
CP7646....287
CP7647....303
CP7648....309
CP7649....288
CP7650....277
CP7653....325
CP7654....221, 312
CP7656....287
CP7657....303
CP7658....309
CP7658I5....309
CP7659....288
CP7664....312
CP7665....312
CP7666....287
CP7667....303
CP7668....309
CP7669....288
CP7670....276
CP7670I5....276
CP7671....286
CP7672....302
CP7673....308
CP7673I5....308
CP7675....277
CP7675I5....277
CP7676....287
CP7678....309
CP7680....276
CP7680I5....276
CP7681....287
CP7681I5....287
CP7682....275
CP7682I5....275
CP7684....275
CP7684I5....275
CP7685....236, 277
CP7685I5....277
CP7686....358
CP7686I5....358
CP7688....277
CP7690....276
CP7690I5....276
CP7691....287
CP7691I5....287
CP7692....275
CP7692I5....275
CP7693....275
CP7694....275
CP7695....277
CP7696....287
CP7697....303
CP7698....309
CP7698I5....309
CP7700....276
CP7702....302
CP7703....308
CP7709....276
CP7710....276
CP7710I5....276
CP7711....286
CP7712....302
CP7713....308
CP7713I5....308
CP7714....325
CP7714I5....325
CP7715....298
CP7715I5....298
CP7717....312
CP7717I5....312
CP7719....276
CP7719I5....276
CP7720....276
CP7721....286
CP7722....302
CP7723....308
CP7723I5....308
CP7724....325
CP7725....298
CP7725I5....298
CP7727....312
CP7730....276
CP7731....287
CP7732....303
CP7733....309
CP7733I5....309
CP7735....298
CP7739....276
CP7740....276
CP7741....287
CP7741I5....287
CP7742....303
CP7743....309
CP7745....298
CP7747....312
CP7747I5....312
CP7749....276
CP7749I5....276
CP7750....276
CP7750I5....276
CP7751....287
CP7751I5....287
CP7752....303
CP7753....309
CP7753I5....309
CP7754....325
CP7754I5....325
CP7757....312
CP7758....276
CP7758I5....276
CP7759....286
CP7760....276
CP7760I5....276
CP7761....287
CP7762....303
CP7763....309
CP7763I5....309
CP7764....325
CP7765....308
CP7767....312
CP7769....286
CP7770....276
CP7770I5....276
CP7771....287
CP7772....303
CP7773....309
CP7773I5....309
CP7774....325
CP7775....308
CP7777....312
CP7778....312
CP7779....287
CP7785....308
CP7787....312
CP7787I5....312
CP7789....287
CP7791....308
CP7791I5....308
CP7792....308
CP7792I5....308
CP7797....312
CP7809....302
CP7813....288
CP7819....302
CP7819I5....302
CP7820....293
CP7821....293

CP7822....293
CP7822I5....293
CP7824....293
CP7825I5....293
CP7829....303
CP7830....293
CP7830I5....293
CP7831....293
CP7831I5....293
CP7832....293
CP7834....293
CP7834I5....293
CP7839....303
CP7870....293
CP7871....293
CP7871I5....293
CP7879....309
CP7884....286
CP7885....286
CP7889....309
CP7894....286
CP7900....286
CP7906....288
CP7907....288
CP7916....288
CP7917....288
CP7921....286
CP7926....288
CP7926I5....288
CP7927....288
CP7936....288
CP7937....288
CP7941....286
CP7945....320
CP7946....288
CP7947....288
CP7950....286
CP7977....288
CP7977I5....288
CP8014....287
CP8014I5....287
CP8015....351
CP8073....309
CP8073I5....309
CP81025....409
CP81069....408
CP81071....409
CP81073....408
CP8120....355
CP8121....337
CP8131....337
CP8132....337
CP8133....337
CP8134....337
CP8430....231, 276
CP8430I5....276
CP8431....287
CP8502....302
CP8510....276
CP8511....286
CP8512....302
CP8512I5....302
CP8513....308
CP8521....286
CP8529....276
CP8530....276
CP8531....287
CP8533....309
CP8540....276
CP8541....287
CP8542....303
CP8542I5....303
CP8543....309
CP8550....276
CP8550I5....276
CP8553....309
CP8560....276
CP8560I5....276
CP8562....302
CP8562I5....302
CP8564....381
CP8565....381
CP8566....381
CP8566I5....381
CP8567....381
CP8567I5....381
CP8568....381
CP8568I5....381
CP8570....381
CP8570I5....381
CP8571....381
CP8574....381
CP8575....326
CP8587....318
CP8587I5....318
CP8592....302
CP8592I5....302
CP8602....300
CP8604....300
CP8605....300
CP8607....300
CP8608....300
CP8610....300
CP8611....300
CP8613....300
CP8662....303
CP8663....303
CP86677....408
CP86678....408
CP8673....277
CP8673I5....277
CP8674....277
CP8674I5....277
CP8675....277
CP8676....277
CP8677....231-232, 277
CP8677I5....277
CP8678....287
CP8685....277
CP8687....231-232, 276
CP8687I5....276
CP8688....276
CP8688I5....276
CP8689....276
CP8690....276
CP8690I5....276
CP8710....276
CP8712....302
CP8712I5....302
CP8713....308
CP8713I5....308
CP8716....287
CP8718....309
CP8722....302
CP8723....308
CP8723I5....308
CP8730....277
CP8730I5....277
CP8735....229-232, 277
CP8735I5....277
CP8736....220, 287
CP8736I5....287
CP8737....303
CP8738....230-231, 236, 309
CP8738I5....309
CP8741....276
CP8741I5....276
CP8742....276
CP8742I5....276
CP8743....276
CP8743I5....276
CP8744....276
CP8744I5....276
CP8745....308
CP8746....308
CP8746I5....308
CP8748....308
CP8750....286
CP8751....227, 286
CP8751I5....286
CP8752....287
CP8752I5....287
CP8753....286
CP8754....287
CP8756....287
CP8756I5....287
CP8760....230, 232, 276
CP8760I5....276
CP8761....287
CP8761I5....287
CP8762....303
CP8763....230-231, 236, 309
CP8763I5....309
CP8770....276
CP8771....286
CP8771I5....286
CP8772....303
CP8772I5....303
CP8773....233, 309
CP8774....277
CP8775....235, 277
CP8775I5....277
CP8780....276
CP8780I5....276
CP8781....286
CP8791....287
CP8796....287
CP8798....231, 309
CP8799....277
CP8800....255
CP8801....255
CP8802....255
CP8803....255
CP8805....255
CP8806....255
CP8806I5....255
CP8807....255
CP8808....255
CP8809....255
CP8810....255
CP8811....255
CP8812....255
CP8813....255
CP8814....255
CP8815....255
CP8816....255
CP8817....255
CP8818....255
CP8819....260
CP8820....260
CP8820I5....260
CP8821....260
CP8821I5....260
CP8822....260
CP8822I5....260
CP8823....260
CP8824....260
CP8824I5....260
CP8825....260
CP8826....260
CP8827....260
CP8828....260
CP8829....260
CP8830....260
CP8831....260
CP8842....303
CP8843....309
CP8843I5....309
CP8852....303
CP8853....309
CP8855....261
CP8855I5....261
CP8856....261
CP8857....261
CP8858....219, 261
CP8859....261
CP8859I5....261
CP8860....218, 261
CP8860I5....261
CP8861....261
CP8862....261
CP8863....261
CP8864....261
CP8865....261
CP8865I5....261
CP8866....223, 261
CP8867....261
CP8868....224, 261
CP8868I5....261
CP8870....276
CP8871....287
CP8871I5....287
CP8872....257
CP8873....257
CP8874....257
CP8875....257
CP8876....257
CP8877....218, 225, 257
CP8877I5....257
CP8878....257
CP8878I5....257
CP8879....222, 257
CP8880....257
CP8881....257
CP8882....257
CP8883....257
CP8883I5....257
CP8884....257
CP8885....257
CP8886....257
CP8887....257
CP8888....224, 257
CP8900....247
CP8901....247
CP8902....247
CP8903....247
CP8904....247
CP8905....247
CP8906....231-232, 235, 248
CP8906I5....248

CP8907....248
CP8907I5....248
CP8908....248
CP8908I5....248
CP8909....248
CP8910....248
CP8911....248
CP8911I5....248
CP8912....248
CP8912I5....248
CP8913....215, 248
CP8913I5....248
CP8914....248
CP8915....248
CP8916....248
CP8916I5....248
CP8917....248
CP8917I5....248
CP8918....248
CP8918I5....248
CP8919....248
CP8920....248
CP8920I5....248
CP8921....248
CP8922....248
CP8923....248
CP8924....213, 220, 248
CP8925....248
CP8926....213, 248
CP8927....248
CP8928....248
CP8929....248
CP8930....248
CP8933....252
CP8934....252
CP8935....252
CP8935I5....252
CP8936....252
CP8936I5....252
CP8937....252
CP8938....253
CP8939....215, 253
CP8940....253
CP8941....253
CP8941I5....253
CP8942....253
CP8943....218, 253
CP8943I5....253
CP8944....214-219, 223-224, 226-227, 253
CP8944I5....253
CP8945....218, 226-227, 253
CP8946....214, 222, 226-227, 253
CP8947....253
CP8948....218, 253
CP8948I5....253
CP8949....253
CP8950....253
CP8951....253
CP8952....253
CP8953....253
CP8954....253
CP8954I5....253
CP8955....213, 227, 253
CP8955I5....253
CP8956....253
CP8957....215, 225, 253
CP8957I5....253
CP8958....253
CP8959....253
CP8960....219, 253
CP8960I5....253
CP8961....253
CP8961I5....253
CP8962....253
CP8963....253
CP8964....362
CP8965....248
CP8967....223, 248
CP8968....248
CP8969....224, 248
CP8970....248
CP8971....253
CP8972....253
CP8973....223, 253
CP8974....253
CP8975....224, 253
CP8976....218, 221-222, 224, 253
CP8977....259
CP8979....259
CP8980....259
CP8981....259
CP8982....218, 259
CP8982I5....259
CP8983....219, 259
CP8984....259
CP8986....259
CP8987....259
CP8990....259
CP8990I5....259
CP8991....213, 259
CP8994....259
CP8996....259
CP8998....259
CP9000....259
CP9001....221, 259
CP9002....222, 259
CP9010....392
CP9011....392
CP9012....392
CP9013....392
CP9014....392
CP9015....392
CP9016....392
CP9018....392
CP9019....392
CP9020....392
CP9021....392
CP9022....392
CP9023....392
CP9024....392
CP9025....392
CP9026....392
CP9027....392
CP9030....247
CP9031....247
CP9032....247
CP9032I5....247
CP9034....252
CP9034I5....252
CP9035....252
CP9036....252
CP9036I5....252
CP9037....252
CP9038....252
CP9039....252
CP9039I5....252
CP9040....252
CP9041....255
CP9042....260
CP9044....317
CP9045....317
CP9046....317
CP9047....317
CP9048....317
CP9050....266
CP9051....266
CP9052....266
CP9053....266
CP9054....215, 266
CP9055....266
CP9056....266
CP9057....266
CP9058....266
CP9059....266
CP9060....266
CP9060I5....266
CP9061....266
CP9062....266
CP9063....266
CP9064....266
CP9066....266
CP9070....213-214, 218-219, 225, 335
CP9071....335
CP9072....335
CP9073....334
CP9074....213-215, 218-219, 225, 334
CP9075....334
CP9076....330, 367
CP9077....330, 367
CP9078....236, 330, 367
CP9079....330, 367
CP9080....330
CP9083....330
CP9090....317, 365
CP9091....317, 366
CP9092....317, 365
CP9092I5....317
CP9093....317, 366
CP9094....317, 365
CP9094I5....317, 365
CP9095....317, 366
CP9096....317, 365
CP9097....317, 366
CP9100....265
CP9101....265
CP9101I5....265
CP9102....213, 215, 217, 265
CP9102I5....265
CP9103....213, 215, 221, 225-226, 265
CP9103I5....265
CP9104....265
CP9104I5....265
CP9105....217, 219, 226, 265
CP9105I5....265
CP9106....265
CP9106I5....265
CP9107....221, 265
CP9108....217, 219, 265
CP9109....265
CP9110....265
CP9140....267
CP9141....267
CP9142....267
CP9143....267
CP9144....267
CP9145....267
CP9146....267
CP9147....267
CP9148....267
CP9149....267
CP9149I5....267
CP9150....267
CP9151....214, 216, 267
CP9151I5....267
CP9152....267
CP9152I5....267
CP9153....267
CP9154....267
CP9154I5....267
CP9155....267
CP9155I5....267
CP9156....267
CP9157....268
CP9158....268
CP9159....268
CP9160....268
CP9161....268
CP9162....268
CP9163....213, 268
CP9164....268
CP9165....268
CP9166....268
CP9166I5....268
CP9167....268
CP9168....268
CP9169....268
CP9170....268
CP9171....221-224, 268
CP9172....268
CP9173....268
CP9174....268
CP9175....267
CP9176....392
CP9177....392
CP9200....263
CP9201....263
CP9202....263
CP9203....263
CP9204....263
CP9205....263
CP9205I5....263
CP9206....217, 263
CP9207....263
CP9208....264
CP9209....264
CP9210....264
CP9211....264
CP9212....264
CP9212I5....264
CP9213....264
CP9214....264
CP9215....220, 224, 227, 264
CP9216....264
CP9217....264
CP9218....263
CP9219....263
CP9220....263
CP9221....263
CP9222....263
CP9223....263
CP9224....264
CP9225....264
CP9225I5....264
CP9226....221, 264
CP9226I5....264
CP9227....264
CP9228....264
CP9229....263
CP9229I5....263

CP97638....355
CP97638I5....355
CP97658....355
CP97658I5....355
CP97711....355
CP97711I5....355
CP97713....355
CP97721....355
CP97723....355
CP97723I5....355
CP97743....355
CP97753....355
CP97753I5....355
CP97763....355
CP97763I5....355
CP97773....355
CP97773I5....355
CR213105....157
DY50295500....52
DY50296800....52
DY50390600....52
DY50402400....52
DY50540700....52
DY50546100....52
DY50548400....52
DY50549100....52
DY50549290....52
DY50549500....52
DY50551400....52
DY50559800....52
DY50559900....52
DY50572600....52
DY50573990....52
DY50574190....52
DY50574500....52
DY70001990....52
DY70007701....52
DY70007791....52
DY70008101....52
DY70008590....52
G1072-20008....120
G1099-20030....117
G1099-20130....120
G1099-20132....120
G1099-20133....120
G1099-20136....120
G1099-60566....116
G1099-80001....127
G1099-80039....131-132
G1099-80053....121, 125, 133
G1530-61950....84
G1530-80650....107
G1531-00105....84
G1531-20550....82
G1531-20690....84
G1531-20700....84
G1531-20740....85
G1531-21090....84
G1531-40020....105
G1531-60680....85
G1531-60690....85
G1531-60700....84
G1531-80560....81, 104-105
G1531-80620....81, 104
G1532-20710....91
G1532-60675....93
G1532-60685....93
G1532-60690....93
G1532-60695....93
G1532-80540....91
G1533-80565....88
G1534-20530....105
G1534-20590....105
G1534-40020....105
G1534-40030....105
G1534-60570....101, 105
G1534-60610....105
G1534-80500....105
G1534-80510....105
G1534-80540....105
G1534-80580....104
G1534-80590....104
G1535-00010....100
G1535-00030....100
G1535-60600....99
G1535-60610....100
G1535-80520....100
G1540-85010....108
G1543-00060....76
G1543-00085....76
G1543-00100....76
G1543-00155....76
G1543-20580....76
G1543-20765....76
G1543-61540....76
G1544-20590....63
G1544-60575....62
G1544-60585....62
G1544-60610....63
G1544-80530....63
G1544-80580....62
G1544-80700....28
G1544-80730....28
G1544-80731....28
G1580-60060....41
G1580-60062....41
G1580-60575....62
G1580-60585....62
G1580-80060....41
G1580-80062....41
G1888-60701....49
G1888-60702....48
G1888-60703....48
G1888-60704....48
G1946-00034....132
G1946-20168....76, 84
G1999-20021....120-121
G1999-20430....121
G1999-20432....121
G1999-20433....121
G1999-20443....121
G1999-20444....121
G1999-20446....121
G1999-60412....121
G1999-80410....132
G2397-20540....88
G2397-80520....88
G2589-20043....120
G2589-20044....120
G2589-20045....120
G2589-20100....120
G2617-20510....71-72
G2617-60506....71-72
G2617-60507....71-72
G2617-60508....71-72
G2617-60510....71-72
G2617-60517....72
G2617-60518....72
G2617-80540....71
G2617-80550....72
G2618-80500....71
G2619-60501....71-72
G2630-60710....107
G2630-61230....93
G2855-20530....37, 41
G2855-20555....37, 41
G2855-20590....37, 46
G2855-40001....46
G2855-60200....37, 41, 46, 117
G2855-60570....46, 117
G2933-85001....107
G2933-85003....107
G3163-20530....120
G3170-20126....120-121
G3170-20530....120
G3170-20540....121
G3170-60050....120, 125, 133
G3170-80001....125, 133
G3170-80002....116, 133
G3170-80008....127
G3170-80100....127
G3170-80103....127, 133
G3182-61580....36
G3182-61581....36
G3184-60065....37
G3185-60300....124
G3185-60361....124
G3185-60362....124
G3185-60363....124
G3185-60364....124
G3430-40035....55, 62
G3430-60011....62
G3431-00005....64, 76
G3431-60680....85
G3431-80507....84
G3431-80509....84
G3432-00003....76
G3432-00004....76
G3432-60220....93
G3432-60221....93
G3433-63000....88
G3434-60806....101
G3434-67500....105
G3434-67540....105
G3451-80501....76
G3452-60100....62
G3452-60730....64
G3452-60730....62
G3452-60835....46
G3480-67585....62
G3500-80000....72
G3500-80001....72
G3504-20504....34
G3510-20018....64
G3520-20210....46
G3520-67001....46
G3591-70001....406
G3591-70002....404
G3591-70003....404
G3591-70004....404
G3591-70005....403
G3591-70006....403
G3591-70007....403
G3591-70008....404
G3591-70009....406
G3591-70010....406
G3591-70011....403
G3591-70013....404
G3591-70014....406
G3591-70015....404
G3591-70017....404
G3591-70018....406
G3591-74001....403
G3591-80000....407
G3591-80001....401
G3591-80002....403
G3591-80003....404
G3591-80004....403
G3591-80005....406
G3591-80006....407
G3591-80007....407
G3591-80008....407
G3591-80011....402
G3591-80012....404
G3591-80013....406
G3591-80014....407
G3591-80015....407
G3591-80016....406
G3591-80017....404
G3591-80019....403
G3591-80020....403
G3591-80021....401
G3591-80022....404
G3591-80023....403
G3591-80025....405
G3591-80026....406
G3591-80027....401
G3591-80028....404
G3591-80029....406
G3591-80030....401
G3591-80031....404
G3591-80032....401
G3591-80033....403
G3591-80034....407
G3591-80035....404
G3591-80036....405
G3591-80037....402
G3591-80039....401
G3591-80040....407
G3591-80043....404
G3591-80044....405
G3591-80045....402
G3591-80046....404
G3591-80047....403
G3591-80048....405
G3591-80049....407
G3591-80050....401
G3591-80051....406
G3591-80052....406
G3591-80053....406
G3591-80054....404
G3591-80055....401
G3591-80056....404
G3591-80058....404
G3591-80059....405
G3591-80060....402
G3591-80061....404
G3591-80062....404
G3591-80063....407
G3591-80064....404
G3591-80065....404
G3591-80066....406
G3591-80067....402
G3591-80068....407
G3591-80071....406
G3591-80072....405
G3591-80074....404
G3591-80075....404
G3591-80077....404
G3591-80082....401
G3591-80083....406

G3591-80084....400
G3591-80085....404
G3591-80086....405
G3591-80087....405
G3591-80088....402
G3591-80090....404
G3591-80091....402
G3591-80093....405
G3591-80094....407
G3591-80095....400
G3591-80096....406
G3591-80097....404
G3591-80098....404
G3591-80099....400
G3591-80100....403
G3591-80101....404
G3591-80102....403
G3591-80103....404
G3591-80104....404
G3591-80105....400
G3591-80106....406
G3591-80107....404
G3591-80108....407
G3591-80110....405
G3591-80119....405
G3591-80120....406
G3591-80121....403
G3591-80122....405
G3591-80123....405
G3591-80125....401
G3591-80135....406
G3591-80136....406
G3591-80137....406
G3591-80138....406
G3591-80139....401
G3591-80140....401
G3591-80141....407
G3591-80142....407
G3591-80157....406
G3591-80158....402
G3591-80162....405
G3591-81000....407
G3591-81001....401
G3591-81002....403
G3591-81003....404
G3591-81004....403
G3591-81005....406
G3591-81006....407
G3591-81007....407
G3591-81008....407
G3591-81011....402
G3591-81012....404
G3591-81013....406
G3591-81014....407
G3591-81015....407
G3591-81016....406
G3591-81017....404
G3591-81019....403
G3591-81020....403
G3591-81021....401
G3591-81022....404
G3591-81023....403
G3591-81025....405
G3591-81026....406
G3591-81027....401
G3591-81028....404
G3591-81029....406
G3591-81031....404
G3591-81032....401
G3591-81033....403
G3591-81034....407
G3591-81035....404
G3591-81036....405
G3591-81037....402
G3591-81039....401
G3591-81040....407
G3591-81043....404
G3591-81044....405
G3591-81045....402
G3591-81046....404
G3591-81047....403
G3591-81048....405
G3591-81049....407
G3591-81050....401
G3591-81051....406
G3591-81052....406
G3591-81053....406
G3591-81054....404
G3591-81055....401
G3591-81056....404
G3591-81058....404
G3591-81059....405
G3591-81060....402
G3591-81061....404
G3591-81062....404
G3591-81063....407
G3591-81064....404
G3591-81065....404
G3591-81066....406
G3591-81067....402
G3591-81068....407
G3591-81071....406
G3591-81072....405
G3591-81074....404
G3591-81075....404
G3591-81077....404
G3591-81082....401
G3591-81083....406
G3591-81084....400
G3591-81085....404
G3591-81086....405
G3591-81087....405
G3591-81088....402
G3591-81090....404
G3591-81091....402
G3591-81093....405
G3591-81094....407
G3591-81095....400
G3591-81096....406
G3591-81097....404
G3591-81098....404
G3591-81099....400
G3591-81100....403
G3591-81101....404
G3591-81102....403
G3591-81103....404
G3591-81104....404
G3591-81105....400
G3591-81106....406
G3591-81119....405
G3591-81120....406
G3591-81121....403
G3591-81122....405
G3591-81123....405
G3591-81125....401
G3591-81135....406
G3591-81136....406
G3591-81137....406
G3591-81138....406
G3591-81139....401
G3591-81140....401
G3591-81141....407
G3591-81142....407
G3591-81148....403
G3591-81149....404
G3591-81150....403
G3591-81160....402
G3591-81161....402
G3591-81162....405
G3591-82000....407
G3591-82001....401
G3591-82002....403
G3591-82003....404
G3591-82004....403
G3591-82005....406
G3591-82006....407
G3591-82007....407
G3591-82008....407
G3591-82011....402
G3591-82012....404
G3591-82013....406
G3591-82014....407
G3591-82015....407
G3591-82016....406
G3591-82017....404
G3591-82019....403
G3591-82020....403
G3591-82021....401
G3591-82022....404
G3591-82023....403
G3591-82025....405
G3591-82026....406
G3591-82027....401
G3591-82028....404
G3591-82029....406
G3591-82030....401
G3591-82031....404
G3591-82032....401
G3591-82033....403
G3591-82034....407
G3591-82035....404
G3591-82036....405
G3591-82037....402
G3591-82039....401
G3591-82040....407
G3591-82043....404
G3591-82044....405
G3591-82045....402
G3591-82046....404
G3591-82047....403
G3591-82048....405
G3591-82049....407
G3591-82050....401
G3591-82051....406
G3591-82052....406
G3591-82053....406
G3591-82054....404
G3591-82055....401
G3591-82056....404
G3591-82058....404
G3591-82059....405
G3591-82060....402
G3591-82061....404
G3591-82062....404
G3591-82063....407
G3591-82064....404
G3591-82065....404
G3591-82066....406
G3591-82067....402
G3591-82068....407
G3591-82071....406
G3591-82072....405
G3591-82074....404
G3591-82075....404
G3591-82077....404
G3591-82082....401
G3591-82083....406
G3591-82084....400
G3591-82085....404
G3591-82086....405
G3591-82087....405
G3591-82088....402
G3591-82090....404
G3591-82091....402
G3591-82093....405
G3591-82094....407
G3591-82095....400
G3591-82096....406
G3591-82097....404
G3591-82098....404
G3591-82099....400
G3591-82100....403
G3591-82101....404
G3591-82102....403
G3591-82103....404
G3591-82104....404
G3591-82105....400
G3591-82106....406
G3591-82119....405
G3591-82120....406
G3591-82121....403
G3591-82122....405
G3591-82123....405
G3591-82125....401
G3591-82135....406
G3591-82136....406
G3591-82137....406
G3591-82138....406
G3591-82139....401
G3591-82140....401
G3591-82141....407
G3591-82142....407
G3591-82159....403
G3591-82162....405
G3880-20030....117
G3880-80010....125
G3880-80011....125
G3900-63001....395
G3900-63002....395
G3900-63003....396
G3900-63004....395
G3900-63005....395
G3900-63006....396
G3900-63007....396
G3900-63008....396
G3900-63009....395
G3900-63010....396
G3900-63011....396
G3900-63012....396
G3900-63013....395
G3900-63014....395
G3900-63015....396
G3900-63016....395
G3900-63017....395
G3900-63018....395
G3900-63019....395
G3900-63020....396
G3900-63021....396
G3900-63022....396
G3900-63023....396

G3900-63024....396
G3900-63025....396
G3900-63026....396
G3900-63027....396
G3900-63028....396
G3900-63029....396
G3900-63030....395
G3900-63031....395
G3900-63032....395
G3900-63033....395
G3900-63034....396
G3900-63035....396
G3900-63036....396
G3900-63037....396
G3900-63038....395
G3900-63039....395
G3900-63040....395
G3900-63041....395
G3900-63042....395
G4513-20561....43
G4513-40525....43
G4513-40529....43
G4513-80209....21
G4513-80213....21
G4514-60710....43
G4514-67505....43
G4525-60701....43
G4525-60702....43
G4525-60703....43
G4525-60704....43
G4556-60019....46
G4556-60125....46
G4556-60690....46
G4556-67010....46
G4556-80101....47
G4556-80102....47
G4556-80103....47
G4556-80105....47
G4556-80106....47
G4556-80108....47
G4556-80109....47
G4556-80111....47
G4556-80112....47
G4556-80113....47
G4556-80115....47
G4556-80116....47
G4556-80118....47
G4556-80119....47
G4556-80126....47
G4556-80128....47
G4556-90500....46
G6600-60037....107
G6600-60038....106
G6600-67006....107
G6600-67007....106
G6600-67008....106-107
G6600-67009....106
G6600-80018....35, 106-107
G6600-80042....106
G6600-80043....106-107, 132
G6600-80044....106-107
G6600-80045....106
G6600-80050....106
G6600-80051....106-107
G6600-80063....106
G6600-85000....107
G6600-85001....106-107
G6600-85002....106-107
IDP3TS....131
MKI-C-QSC10....53
MKI-MTD-1169....53
MKI-MTD-1204....53
MKI-U-COV06....53
MKI-U-COV07....53
MKI-U-COV10....53
MKI-U-DISK1....53
MKI-U-DISK3....53
MKI-U-T11GPC....53
MKI-U-T11GPC-2S....53
MKI-U-T12ME....53
MKI-U-T12ME-2S....53
MKI-U-T3ATX....53
MKI-U-T3ATX-2S....53
MKI-UTD-5064....53
MKI-UTD-5105....53
MKI-Z-0285....53
MKI-Z-0351....53
RDT-1020....46
UMC-2....132

Application Title Index

1,3-Butadiene 561
1,3-Butadiene Purity 562
122-5512UI 141
15+1 EU Priority PAHs 433
69 Component FAME Mix 496

A

Acids 495
Acrylate Impurities I 527
Acrylate Impurities II 528
Acrylates 528
Agilent's Ultra Inert Test Probe Mixture 458
Alcohol Beverage Standard 492
Alcohols I 501
Alcohols II 505
Alcohols III 505
Aldehydes and Acids 511
Aldehydes and Ketones 512
Alditol Acetates 493
Amines and Alcohols 506
Amines and Nitriles 510
Amines in Water 511
Amphetamines and Precursors – TMS Derivatives 536
Anabolic Steroids 548
Analysis of Acetylenes Mixture 534
Analysis of Amino Alcohols in Water 506
Analysis of Ethanolamines 506
Analysis of Fragrance and Allergens 485
Analysis of Gases C1 to C4 576
Analysis of Oxygenates in a C1 to C5 Hydrocarbon Mix 575
Analysis of Polycyclic Aromatic Hydrocarbons 431
Analysis of Semivolatiles 437
Analysis of Solvents 526
Anesthetics 543
Anilines 529
Anticonvulsants 543
Antiepileptic Drugs 544
Antihistamines 544
Aroclors 1016-1268 (without 1221) 441
Aromatic Solvents 503
Aromatics Analysis – ASTM D16 Analytes 568
Aromatics Analysis – Ethylbenzene Impurities 568
Aromatics I 514
Aromatics II 515
Aromatics in Finished Gasoline – ASTM Method 5769 571
Aspirin and Ibuprofen in Methanol 547

B

Bacterial Fatty Acid Methyl Esters 495
Barbiturates 537
Baseline Resolution of Air/CO, COBenzodiazepines I 536
Benzodiazepines II 540
Blood Alcohols I (Static Headspace/Split) 538
Blood Alcohols II (Static Headspace/Split) 538
Blood Pollutants I 549
Blood Pollutants II 549
Boiling Point Elution Order for Homologous Series 197
Bourbon 493
Butter Triglycerides I 499
Butter Triglycerides II 499

C

CCLP Pesticides 441
Canola Oil Margarine Partially Hydrogenated FAMEs AOCS Method 1c-89 499
Chiral Compounds in Essential Oils and Fragrances 484
Chlorinated Isooctane 523
Chlorinated Pesticides, EPA Method 508 448
Citrus Flavored Carbonated Beverage (Soda) 492
Cold-Pressed Orange Oil 489
Common Drug Screen 541
Common Industrial Solvents 525
Congeners in DIN Method PCBs 459

D

DNPH Derivative 513
Denatured Fuel Ethanol – ASTM D5501 570
Detailed Hydrocarbon Analysis of Petroleum Naphthas Through N-nonane Using ASTM D-5134 576
Determination of Chlorophenols in Water and Soil 430
Deviation from Boiling Point Order 197
Diesel Analysis 575
Diesel Fuel 431
Dioxins and Dibenzofurans 432
Dipole Interactions 198
Direct Comparison for Rapid CLP (Contract Laboratory Program) Pesticide Analysis 440
Direct Injection of Gasoline and Diesel Fuel in Methylene Chloride 575
Drug Screen 540

E

EPA 625 Halogenated Pesticides on "1701" Type Phases 455
EPA Air Analysis Compendium Method TO-14 Standard 473
EPA Air Analysis Method TO-15 (1 ppbV Standard) 477
EPA Method 525.2 445
EPA Method 551 470
EPA Method 552.2 467
EPA Volatiles by GC/MS (Split Injector) 444, 471
Esters I 517
Esters II 518
Esters III 518
Ethers 519
Ethoxyethanol 507
Ethylene 559
Ethylene Glycol Mixture 521
Ethylene Oxide 531
Ethylene Oxide Synthetic Standard 569
European Red List Volatiles 470
Extended Analyte List for EPA Method 8021 468
Extended Hydrocarbon Analysis I 563
Extended Hydrocarbon Analysis II 564
Extended Temperature Program Resolving Congeners 52 and 138 460

F

FAME Standard 497-498
FAMEs 485
Fast Analysis of Aromatic Solvent 552
Fast Analysis of Permanent Gases and COFast Separation of Silanes 533
Fast VOC Analysis 469
Fast analysis of lemon oil using Rapid-MS 488
Fast screening of FAME isomers in butter 500
Fentanyls 545
Flavor Mixture 487
Formaldehyde Underivatized 513
Formaldehyde, 50ppb 474
Fragrance Allergens 487
Fragrance Reference Standard 482-483
Free Organic Acids/C4-C5 Isomers 508
Free Phenols 455
Free Steroids 548

G

Gasoline Unleaded ASTM D 5769 574
Glycols I 519
Glycols II 520
Glycols III 520
Glycols/Diols 522

H

Hallucinogens 545
Halocarbons 531
Halogenated Hydrocarbons I 502
Halogenated Hydrocarbons II 522
Halothane 532
Herbicides I 453
Herbicides II 453
High Resolution Phenol Analysis by GC/MS 466
High Resolution Separation of Xylene Isomers 532
High Speed VOC, EPA Method 8260 442
Hydrogen Bonding Interactions 199

I

Impurities in Ethylbenzene 516
Impurities in Ethylene 559
Impurities in Mixed Xylenes 532
Impurities in Propylene 560
Impurities in Styrene 516
Impurities in p-Xylene – ASTM D3798 569
Inorganic Gases 504
Inorganic Hydride Gases 533

L

Lavender Oil Characterization....480
Lemon Oil....488

M

Marijuana (Δ9-THC) and Major Metabolites – TMS Derivatives....548
Menthol....484
Mercaptans....567
Methyl Tert-Butyl Ether (MTBE) FID, Extended 8020 Analysis....429

N

Narcotics....537
Narcotics and Adulterants....546
Natural Gas....558
Nitrogen Based Solvents I....526
Nitrogen Based Solvents II....527
Nitrogen Containing Herbicides (EPA Method 507)....454
Nitrogen/Phosphorus Containing Pesticides, EPA Method 507....452
Noble Gases....557
n-Paraffin Standard....554

O

Organic Acids....494, 507
Organochlorine Pesticides....452
Organochlorine Pesticides I....449
Organochlorine Pesticides I EPA Method 8081A....447, 456
Organochlorine Pesticides II....449
Organochlorine Pesticides II EPA Method 8081A....457
Organochlorine Pesticides III....450
Organochlorine Pesticides IV....450
Organochlorine Pesticides to EPA 625 via GC/MS....456
Organochlorine Pesticides, DB-5/DB-1701P....451
Organohalide Pesticides in Water, EPA Method 505....448
Organophosphorus Pesticide Residues in Olive Oil Extract....486
Organotin Compounds I....461
Organotin Compounds II....461
Over-the-Counter Pain Killers – TMS Derivatives....547
Oxygenates....570
Oxygenates in Gasoline ASTM D5599 (GC-OFID)....570

P

PAHs....465
PBDEs....443
PBDEs by ECD....430
PCBs by EPA Method 8082....460
PFBHA Derivative....514
PONA Mix as Specified by AFNOR Method #2....571
Peppermint Oil....489
Perfume....484
Permanent Gases....557
Permanent Gases on a Thick Film Molsieve Column....476
Pesticides in sunflower oil....500
Pesticides, EPA 508.1....438
Phenols....464
Phenols According to EPA Method 8040....466
Phenols I....504
Phenols II....530
Phenols III....530
Phenoxy Acid Herbicides – Methyl Derivatives, EPA 8151A....439
Phenyl Content Retention....199
Polarity – Retention Relationship....200
Polyethylene....574
Polyethyleneamines....509
Polymer Additives....533
Primary Amines....509
Propylene....560
Pyrethrins....461
Pyrolysates of Polystyrene....517

R

Reference Gas Oil....572
Refinery Gas....565
Refinery Gas I....553
Regular Unleaded Gasoline (California Phase 1) – "Normal" GC Run I....573
Regular Unleaded Gasoline (California Phase 1) – "Normal" GC Run II....573
Residual Solvents....551
Residual Solvents, DMI Diluent....539
Residual Solvents, USP 467....550
Rosemary Oil....491

S

Sedative Hypnotics....546
Selected Oxygenates....557
Semivolatile Compounds, US EPA Method 8270....462
Separation of TMS-derivatized sugars using VF-1ms....494
Separation of *cis*-trans FAME isomers....496
Simulated Distillation....572
Solvents I....523
Solvents II....524
Solvents III....524
Solvents IV....525
Spearmint Oil (Western)....490
Strawberry Syrup....493
Substituted Anilines....529
Sulfur Compounds in Naphtha....568
Sulfur Compounds in Natural Gas – Synthetic Mixture....567
Sulfur Compounds in Propylene (1 ppm)....555, 566
Sulfur Gas Analysis in Light Hydrocarbon Streams I....565
Sulfur Gas Analysis in Light Hydrocarbon Streams II....566
Sulfur Gases....534
Sulfur Impurities in Propylene....555
Sulfur in Air....474

T

Tetrachlorodibenzo-p-furans....459
Tocopherols....545
Trace Active Amines, 10 ng on-column....508
Trace Level Polycyclic Aromatic Hydrocarbon (PAH) Analyses....458
Trace Oxygenates in Light Hydrocarbon Matrices....556
Trace Sulfur Compounds in Methane (50 ppbv)....556
Tricyclic Antipsychotics....544
Triethylene Glycol and Impurities....521

U

US EPA Method 551.1....436
US EPA Method 8061 (Phthalate Esters)....463
US EPA Method 8270 Short Mix....463
Underivatized Drugs of Abuse – Agilent Fast Toxicology Analyzer....539
Unleaded Gasoline....429, 553
Urine Drug Screen....542

V

Volatile Amines....508
Volatile Sulfur Compounds....554

Y

Ylang Ylang Oil....490-491

Compound Index

A

Acealdehyde....556
Acenaphthalene....465
Acenaphthalene-d10....446
Acenaphthene....431, 458, 462, 465
Acenaphthene-d10....445, 462-463
Acenaphthylene....431, 445, 458, 462
Acephate....486
Acetal (acetaldehyde diethyl acetal)....519
Acetaldehyde....474, 477, 492-493, 512, 538, 549, 575
Acetaminophen....541, 547
Acetic acid....435, 492-495, 507, 511
Acetic acid, ethyl ester....570
Acetic acid, methyl ester....570
Acetone....442, 444, 471, 474, 477-478, 482-483, 492, 494, 512, 524-526, 532, 538-539, 549-550, 556-557, 575
Acetone-d6....474
Acetonitrile....442, 524, 526-527, 535, 539, 549-550
Acetyl aldehyde....478
Acetylcedrene....484
6-Acetylcodeine....537, 546
Acetylene....559-565
Acetylsalicylic acid (aspirin)....547
Acifluorofen....439
Acrolein....442, 512, 526-527
Acrylamide....510
Acrylic acid....435
Acrylonitrile....442, 444, 471, 526-527
Adrin....448
Alachlor....435, 438, 445, 447-448, 451-453, 456-457
Aldrin....434-435, 438, 440-441, 445, 447-452, 456-457
Alfentanyl....545
Allobarbital....537, 541
Allyl acrylate....528
Allyl alcohol....442, 556
Allyl butyrate....482-483
Allyl chloride....442, 444, 468, 471
Allyl ether....519
Allyl ethyl ether....519
Alphenal....537
Alprazolam....141, 536, 539-540
Ametryn....445, 452-453
2-Aminoazotoluene....529
4-Aminobiphenyl....463
2-Amino-1-butanol....506
2-Amino-ethanol....506
Aminoethylethanolamine....511
n-(2-Aminoethyl) piperazine....511
2-Aminonaphthalene....529
1-Amino-4-nitronaphthalene....465
5-Amino-1-pentanol....506
1-Amino-2-propaol....506
Amitriptyline....542
Amobarbital....537, 541
Amphetamine....536, 539, 542
Amyl acetate....478, 493, 517-518
Amyl alcohol....478, 549
n-Amyl alcohol....492
Amyl butyrate....493
Amyl cinnamic alcohol....485
Amyl cinnamyl alcohol....487
Amyl cinnamyl aldehyde....485
n-Amyl mercaptan....567
tert-Amyl mercaptan....567
tert-Amyl methyl ether (TAME)....429, 442, 519, 556, 570, 574-575
n-Amyl salicylate....482-484
5α-Androstan-17α-ol-3-one (Stanolone)....548
Androsterone....548
5-β-Androsterone....548
Aniline....462-463, 510, 529
Anisic alcohol....485
Anisyl alcohol....487
Antazoline....544
Anthracene....431, 445, 458, 462, 465
Anthracene-d10....446
Aprobarbital....537, 541
Arabinitol....493
Arabitol....494
Arachidic acid (eicosanoic acid)....494
Arachidic acid methyl ester....497-498
Arachidonic acid methyl ester....497-498
Argon....476, 557
Arsine....533
Atraton....452-453
Atrazine....438, 445-446, 448, 452-454
Azinphos-ethyl....486
Azinphos-methyl....486
Azobenzene....462
Azulene....465

B

Balan....454
Barbital....537
Behenic acid methyl ester....497-498
Benactyzine....541
Bentazone....439
Benthiocarb....446
Benylamine....509
Benzaldehyde....482-483, 487, 512
Benzaldehyde, 3 methoxy....478
Benz[a]anthracene....433, 445, 458
Benz[a]anthracene-7,12-dione....465
1,2-Benzanthracene....465
Benzene....429, 442, 444, 468-469, 471, 473, 477, 503, 514-516, 523-524, 526, 532, 535, 549-553, 561-564, 568, 571, 574, 576
Benzene-d6....571
Benzene ethanol....482-484
α-Benzene hexachloride (BHC)....434-435, 438, 440-441, 445, 447-452, 456-457
β- Benzene hexachloride....434-435, 438, 440-441, 445, 447-452, 456-457
δ-Benzene hexachloride....434-435, 438, 440-441, 445, 447-452, 456-457
γ-Benzene hexachloride....434-435, 438, 440-441, 445, 447-452, 456-457
Benzidene....432
Benzidine....462-463, 529
Benzo[a]anthracene....431, 462
Benzocaine....543
Benzo[b]fluoranthene....431, 433, 445, 458, 462-463, 465
Benzo[j]fluoranthene....433
Benzo[k]fluoranthene....431, 433, 445, 458, 462-463, 465
Benzo[c]fluorene....433
2,3-Benzofluorene....465
Benzo[g,h,i]perylene....431-433, 445, 458, 462, 465
Benzo[a]pyrene....431, 433, 445, 458, 462, 465
Benzo[e]pyrene....465
Benzoic acid....462
Benzonitrile....510, 526-527
Benzophenone....482-483
5,6-Benzoquinoline....465
Benzothiophene....568
Benzphetamine....536, 541
Benzyl acetate....482-484, 490-491, 517-518
Benzyl alcohol....462, 482-483, 485, 487, 501, 505
Benzylamine....510
Benzyl benzoate....463, 482-485, 487, 490-491, 493
Benzyl butyl phthalate....445
Benzyl chloride....442, 468, 477
Benzyl cinnamate....485, 487
Benzyl ether....519
n-Benzylmethylamine....510
Benzyl salicylate....482, 484-485, 487, 490-491
α-Bergamotene....480
trans-α-Bergamotene....488
Bifenthrin....446
Bioallethrin....446
Biphenyl....465
β-Bisabolene....483, 488, 491
α-Bisabolol....480
Borneol....480, 482-484, 491
Borneol acetate....480
Bornyl acetate....481-482
α-Bourbonene....479
β-Bourbonene....479, 489-490
Bromacil....445-446, 452-454
Bromazepam....536, 540
Bromoacetic acid....467
Bromoacetone....442
4-Bromoaniline....510, 529
Bromobenzene....442, 444, 468-469, 471, 514-515
2-Bromobiphenyl....447, 456-457
Bromochloroacetic acid....467
Bromochloroacetonitrile....436, 470
Bromochlorodifluoromethane....454
Bromochloromethane....442, 444, 468-469, 471, 473-474, 477, 522
Bromodichloroacetic acid....467
Bromodichloromethane....436, 442, 444, 468-471, 477, 522
2-Bromo-4,6-dinitroaniline....529
Bromoethane (ethyl bromide)....477, 522
Bromofluorobenzene....469
4-Bromofluorobenzene....442, 444, 471, 473-474, 477
Bromoform....436, 442, 444, 468-471, 477, 522
Bromofos....500
Bromomethane....442, 444, 468-469, 471, 473, 477
1-Bromo-2-nitrobenzene....435, 447, 456-457
Bromopheniramine....541, 544
4-Bromophenyl-phenylether....462
3-Bromopyridine....510
Bromotrifluoromethane....454
Buclizine....544
Bufotenine....545
Butabarbital....537, 541
Butacaine....543
Butachlor....445, 452-453
1,2-Butadiene....534, 561-562
1,3-Butadiene....477, 534, 559-566
Butalbital....537
Butanal....511
Butane....574, 576
n-Butane....534, 553, 558-565, 570-571
n-Butane/*cis*-2-Butene....566
1,3-Butanediol....519-520, 522
1,4-Butanediol....519-520
2,3-Butanediol....519-520
2,3-Butanedione....478, 482-483
1-Butanethiol....554-556, 566
Butanol....526-528
1-Butanol....442, 478, 501, 505, 549, 570, 575
2-Butanol....535, 478, 539, 551
n-Butanol....492, 524, 550
sec-Butanol....492, 501, 505, 524-525, 550, 570
tert-Butanol....501, 505, 524, 550, 570
2-Butanone (MEK)....442, 444, 471, 474, 477, 512, 526, 539, 549, 551, 575
2-Butanthiol....556
Butene....517
Butene-1....559, 561-562
1-Butene....517, 534, 559-560, 563-566
cis-2-Butene....559-565
trans-2-Butene....559-566
1-Butene/methyl acetylene....565
2-Buten-1-ol (crotyl alcohol)....501, 505
3-Buten-1-ol....501, 505
Butethal....537
bis(2-n-butoxyethyl) phthalate....463
Butyl acetate....517-518, 527-528
n-Butyl acetate....525
sec-Butyl acetate....517-518
tert-Butyl acetate....517-518
Butyl acrylate....527-528
n-Butyl acrylate....528
n-Butyl alcohol....525, 556

sec-Butyl alcohol 524, 549, 556
tert-Butyl alcohol 442, 549, 556
Butylaldehyde 478, 556
Butylate 445, 452
Butylated hydroxy toluene (BHT) 485, 492, 533
Butylbenzene 442, 514-515, 553
n-Butylbenzene 444, 468, 471, 503, 532, 552, 568, 571
sec-Butylbenzene 442, 444, 468-469, 471, 503, 514-515, 552-553, 568
tert-Butylbenzene 442, 444, 468-469, 471, 503, 514-515, 552, 568,576
Butyl benzyl phthalate 462-463
Butyl caproate 518
Butyl cellosolve 501, 505, 525
Butyl cellosolve acetate 525
Butyl ether 519
Butyl ethyl ether 519
Butyl heptanoate 518
1-Butyl mercaptan 567
n-Butyl mercaptan 567
sec-Butyl methacrylate 528
Butyl methyl ether 519
tert-Butyl methyl ether (MTBE) 477
Butylpentyltin 461
Butyl propionate 518, 527-528
Butyl valerate 518
2-Butyne (dimethylacetylene) 561-562
1-Butyne (ethylacetylene) 561-562
2-*sec*-Butyl-4,-dinitrophenol (Dinoseb) 466
tert-Butyl mercaptan 556, 567
4-*tert*-Butyltoluene 514-515
Butyraldehyde 512, 575
Butyric acid 494-495, 507-508, 511
n-Butyric acid 435
Butyric acid methyl ester 497-498

C

Cadinene 489
δ-Cadinene 481-483, 491
γ-Cadinene 480-481
Caffeine 536, 540-541, 546-547
Camphene 480, 482-484, 488, 491
Camphor 480, 482-483, 491
Capric acid methyl ester 497-498
Caproic acid (hexanoic acid) 494, 507
Caproic acid methyl ester 497-498
Caprylic acid methyl ester 497-498
Captafol 435, 447, 456-457
Captan 447, 451, 456-457
Carbamazepine 543
Carbazepine 540
Carbazole 462, 465
Carbepoxide 10/11 544
Carbinoxamine 544
Carbon dioxide (CO2) 473, 476, 504, 553, 558, 576
Carbon disulfide (CS2) 444, 471, 474, 477, 554-555, 566
Carbon monoxide (CO-air) 476, 553, 557-558, 576
Carbon tetrachloride 436, 442, 444, 468-471, 473, 477, 502, 522, 535, 549
Carbonyl sulfide (COS) 474, 504, 534, 553-556, 566
Carbophenothion 451, 486
Carboxin 445, 452-453
3-Carene 480
Δ-Carane 481
Carfentanyl 545
cis-Carveol 487, 490
trans-Carveol 479, 487, 490
l-Carvone 479
(+/-)-Carvone 490
cis-Carvyl acetate 479, 490
Caryophyllene 480
α-Caryophyllene 491
β-Caryophyllene 479, 481-483, 488-491
Caryophyllene oxide 480
Celestocide 482
Cellosolve acetate 525
Cetearyl decanoate 482-483
Cetearyl octanoate 482-483
Chloral hydrate 436, 470
Chloramben 439
Chlorcyclizine 541, 544
α-Chlordane 434-435, 438, 440-441, 445, 447-451, 456-457
δ-Chlordane 448
γ-Chlordane 434-435, 438, 440-441, 445, 447-451, 456-457
Chlordiazepoxide 536
Chloroacetic acid 467
Chloroacetonitrile 442, 444, 471
2-Chloroaniline 510, 529
3-Chloroaniline 510, 529
4-Chloroaniline 462, 510, 529
Chlorobenzene 442, 444, 468-469, 471, 473, 477, 503, 514-515, 523
Chlorobenzene-d5 ....473-474, 477
Chlorobenzilate 435, 438, 445, 447-448, 451, 456-457
4-Chlorobenzonitrile 510
2-Chlorobiphenyl 445
1-Chlorobutane 442, 444, 471, 502, 522, 549
2-Chlorobutane 549
Chlorodibromoacetic acid 467
1-Chloro-1,1-difluoroethane 454
Chlorodifluoromethane 454
2-Chloro-4,6-dinitroaniline 529
Chloroethane 442, 444, 454, 468-469, 471, 473, 477
2-Chloroethanol 442, 531
bis(2-chloroethoxy) methane 462
bis(2-chloroethyl) ether 462
2-Chloroethyl vinyl ether 468
1-Chloro-3-fluorobenzene 444, 468, 471
Chloroform 436, 442, 444, 468-471, 473, 477, 502, 522, 524, 535, 549-551
1-Chlorohexane 442, 502, 522
1-Chloro isooctane 523
3-Chloro isooctane 523
4-Chloro isooctane 523
bis(2-chloroisopropyl) ether 462, 468
Chloromethane 442, 444, 454, 468-469, 471, 473, 477
4-Chloro-2-methylaniline 529
4-Chloromethyl 2,2'-dimethyl pentane 523
2-Chloro-5-methylphenol 464
4-Chloro-2-methylphenol 464
4-Chloro-3-methylphenol 455, 462, 464, 466, 504
2-Chloronaphthalene 462
Chloroneb 435, 438, 445, 447-448, 451, 456-457
2-Chloro-4-nitroaniline 529
4-Chloro-2-nitroaniline 529
1-Chloro-4-nitrobenzene 514-515
4-Chloro-3-nitrobenzotrifluoride 447, 456-457
Chloropentafluoroethane 454
2-Chlorophenol 430, 455, 462, 464, 466, 504, 530
3-Chlorophenol 430
4-Chlorophenol 430, 464
4-Chlorophenyl-phenyl ether 462
Chloropicrin 436, 470
Chloroprene 468
2-Chloropropane 468, 569
3-Chloropropene (allyl chloride) 477, 502, 522
3-Chloropropionitrile 442
Chloropropylate 435, 447, 456-457
Chloropyrifos 500
4-Chlorostyrene 514-515
2-Chloro-1,1,1,2-tetrafluoroethane 454
Chlorothalonil 435, 438, 445, 447-448, 456-457
2-Chlorotoluene 442, 444, 468-469, 471, 503, 514-515
3-Chlorotoluene 503, 514-515
4-Chlorotoluene 442, 444, 468, 471, 503, 514-515, 523
Chlorotrifluoromethane 454
Chlorpheniramine 541, 544
Chlorpothixene 544
Chlorpropham 445, 452
Chlorpyrifos 451, 453, 486
4-Chlortestosterone-17-acetate (Clostebal) 548
Cholesterol 548
Chrysene 431, 433, 445, 458, 462, 465
Chrysene-d12 ....445-446, 462-463
1,8-Cineol 479, 482-483, 489-490
Cineole 484
Cinerin I 461
Cinerin II 461
Cinnamaldehyde 485, 487
trans-Cinnamaldehyde 484
Cinnamic alcohol 487
Cinnamyl acetate 487, 490
trans-Cinnamyl acetate 491
Cinnamyl alcohol 485
Cinnamyl cinnamate 482-483
Cinnamyl phenyl acetate 482-483
Cinnanzine 544
Citral (geranial) 487
Citronellal 482, 484, 488-489
Citronellic acid 435
Citronellol 481-485, 487, 493
Citronellyl acetate 482-483
Citronellyl formate 481-482
Citronellyl propionate 482
Citronellyl tiglate 482-483
cis-Citronellyl tiglate 487
trans-Citronellyl tiglate 487
Clemizole 544
Clobazam 536, 540
Clonazepam 141, 536, 539-540
Cocaine 539-542, 546
Codeine 537, 539, 541-542, 546
Commamyl acetate 484
α-Copaene 479, 482-483, 491
Coprostane (5-α-cholestane) 548
Cotinine 542
Coumarin 484-485, 487
2-Cresol 530
3-Cresol 530
4-Cresol 530
m-Cresol 466, 530
o-Cresol 466, 530
p-Cresol 466, 530
Crotonaldehyde 442, 512
Cumene 429, 516, 523, 532, 552, 568
Cumic aldehyde 480
Cyanazine 438, 445, 453
2-Cyanopyridine 510
3-Cyanopyridine 510
Cyclizine 544
Cycloate 445, 452
Cyclohexane 477, 523-524, 526, 535, 539, 550, 552-553, 563-564, 568
Cyclohexanol 501, 505
Cyclohexanone 512, 525
2-Cyclohexyl-4,6-dinitrophenol 464
Cyclohexyl methacrylate 528
Cyclopentane 563-564, 571, 576
Cyclopenta[c,d]pyrene 433
Cyclopentanol 501, 505
Cyclopentanone 512
Cyclopentene 563-564
1-Cyclopentene 571
Cyclopentylbarbital 537
Cyclopropane 559-562
Cyheptamide 542
o-Cymene 480
p-Cymene 482-483, 492
r-Cymene 479,488-490

D

Dacthal (DCPA methyl ester) 445, 447, 453, 456-457
Dalapon 439, 467
Decachlorobiphenyl 434-435, 440-441, 449-451, 460
Decanal 488-489, 511
Decane 197, 199-200, 523, 552, 568, 574
n-Decane 197, 208, 458, 553, 571-572
1,10-Decanediol 519-520, 522
Decanoic acid 494, 511
Decanol 492
1-Decanol 501, 505
n-Decylamine 509-510

Dehydroisoandrosterone (Prasterone) 548
1-Dehydrotestosterone (Boldenone) 548
1-Dehydrotestosterone acetate 548
1-Dehydrotestosterone benzoate 548
1-Dehydrotestosterone undecylenate 548
Delorazepam 540
Demoxepam 536, 540
Desalkyl Aurazepam 536
Desipramine 540
Desmethyldiazepam 540
n-Desmethyl methsuximide 543
Dextromethorphan 537
Diacetone-alcohol 525
Diacetyl 492
Diacetylmorphine (Heroin) 141, 537, 539-541, 546
Di-allate A 447, 456-457
Di-allate B 447, 456-457
Diallate isomers 435
2,4-Diaminoanisole 529
2,4-Diaminotoluene 529
3,4-Diaminotoluene 510
Diamyl phthalate 463
Diazepam 536, 539-542
Diazinon 445, 452, 486
Dibenz[a,h]anthracene 431, 433, 445, 458, 462
1,2,3,4-Dibenzanthracene 465
1,2,5,6-Dibenzanthracene 465
Dibenzo-p-dioxin 465
Dibenzofuran 462, 465
Dibenzo[a,e]pyrene 433
Dibenzo[a,h]pyrene 433
Dibenzo[a,i]pyrene 433
Dibenzo[a,l]pyrene 433
Dibenzothiophene 465
Dibenzyl ether 482-483
Dibenzyl phthalate 463
Diborane 533
Dibromoacetic acid 467
Dibromoacetonitrile 436, 470
1,2-Dibromobenzene 473
4,4'-Dibromobiphenyl 438
Dibromochloromethane 436, 442, 444, 468-471, 477
1,2-Dibromo-3-chloropropane 435-436, 442, 444, 447, 456-457, 468-471
1,2-Dibromo-3-chloropropane (DBCP) 502, 522
1,2-Dibromoethane 436, 442, 444, 468, 470-471, 473, 477, 502, 522
Dibromofluoromethane 442
Dibromomethane 442, 444, 468-469, 471, 522
1,2-Dibromomethane 469
2,6-Dibromo-4-nitroaniline 529
4,4'-Dibromooctafluorobiphenyl 439
2,4-Dibromophenol 464
1,2-Dibromopropane 470
2,3-Dibromopropionic acid 467
1,2-Dibromo-1,1,2,2-tetrafluoroethane 454
α,α-Dibromo-m-xylene 447, 456-457
Dibucaine 543
Dibutylchlorendate 447, 456-457
tert-Dibutyl disulfide 567
Dibutyl ether 527-528
Dibutylpentyltin 461
Di-n-butyl phthalate 445, 462-463
Dicamba 439
Dichlobenil 453
Dichlone 435
Dichloroacetic acid 467
Dichloroacetonitrile 436, 470
3,4-Dichloroaniline 510, 529
1,2-Dichlorobenzene 442, 444, 462, 468-469, 471, 473, 477, 503, 514-515, 523
1,3-Dichlorobenzene 204, 206, 442, 444, 462, 468-469, 471, 473, 477, 503, 514-515, 523
1,4-Dichlorobenzene 204, 206, 442, 444, 462-463, 468-469, 471, 473, 477, 503, 514-515, 523
1,4-Dichlorobenzene-d4 442, 462-463
3,3'-Dichlorobenzidine 462-463, 529
3,5-Dichlorobenzoic acid 439
2,3-Dichlorobiphenyl 445
p,p'-Dichlorobiphenyl 451
cis-Dichlorobutene 442
cis-1,4-Dichlorobutene 468
trans-Dichlorobutene 442
trans-1,4-Dichloro-2-butene 444, 471, 502, 522
Dichlorodifluoromethane 442, 444, 454, 468, 471, 473, 477
Dichlorodimethyl silane 533
1,1-Dichloroethane 442, 444, 468-471, 473, 477, 502, 522
1,2-Dichloroethane 442, 444, 468, 470-471, 473, 477, 502, 522, 535
Dichloroethane-d4 442
1,1-Dichloroethene 442, 444, 468-469, 471, 473, 477, 502, 522
cis-1,2-Dichloroethene 442, 444, 468, 471, 473, 477
trans-1,2-Dichloroethene 442, 444, 468-469, 471, 477, 522
1,1-Dichloroethylene 470, 535
cis-1,2-Dichloroethylene 535
trans-1,2-Dichloroethylene 535
1,1-Dichloro-1-fluoroethane 454
Dichlorofluoromethane 454, 469
Dichloromethane 454, 525-526, 533, 535, 570
Dichloromethyl silane 533
2,6-Dichloro-4-nitroaniline 529
2,3-Dichlorophenol 430, 464
2,4-Dichlorophenol 430, 455, 462, 464, 466, 504, 530
2,5-Dichlorophenol 430, 464
2,6-Dichlorophenol 430, 464, 466
3,4-Dichlorophenol 430, 464
3,5-Dichlorophenol 430, 464
1,1-Dichloropropane 522
1,2-Dichloropropane 442, 444, 468-469, 471, 473, 477, 502, 522
1,3-Dichloropropane 442, 444, 468, 471, 522
2,2-Dichloropropane 442, 444, 468-469, 471, 522
1,3-Dichloro-2-propanol 442
1,1-Dichloro-2-propanone 436, 444, 470-471
1,1-Dichloropropene 442, 444, 468, 471
cis-1,2-Dichloropropene 502
trans-1,2-Dichloropropene 502
cis-1,3-Dichloropropene 442, 444, 468-469, 471, 473, 477, 522
trans-1,3-Dichloropropene 442, 444, 468-469, 471, 473, 477, 522
Dichlorotetrafluoroethane 477
1,2-Dichloro-1,1,2,2-tetrafluoroethane 454, 473
2,2-Dichloro-1,1,1-trifluoroethane 454
Dichlorvos 445, 452
Dicyclohexylamine 509-510
Dicyclohexyl phthalate 463
Dieldrin 434-435, 438, 440-441, 445, 447-452, 456-457, 500
Diethanolamine (DEA) 506
Diethylamine 510
2,6-Diethylaniline 510
n,n-Diethylaniline 510
Diethylbenzene 568
1,2-Diethylbenzene 552, 571
1,3-Diethylbenzene 552, 571
1,4-Diethylbenzene 571
Diethylene glycol 520-521
Diethylene glycol dimethyl ether (diglyme) 519-520
Diethylene glycol monobutyl ether 519-520
Diethylene glycol monoethyl ether 519-520
Diethylene glycol monomethyl ether 519-520
Diethylenetriamine 511
Diethyl ether 444, 471, 526, 532, 535, 549, 551, 556, 570, 575
1,2-Diethyl-4-ethylbenzene 571
1,3-Diethyl-5-ethylbenzene 571
Diethyl formamide (DEF) 445
Diethyl phthalate 445, 462-463, 484
Diethyl sulfide 554-556
Diethyltryptamine 545
1,4-Difluorobenzene 444, 471, 473-474, 477
1,1-Difluoroethane 454
Difolotan 453
Dihexyl phthalate 463
9,10-Dihydroanthracene 465
trans-Dihydrocarveol acetate 479
Dihydrocarvone 479, 490
trans-Dihydrocarvyl 490
Dihydrocodeine 537
Dihydropentaborane 533
Diisobutyl phthalate 463
Diisopropylamine 510
1,3-Diisopropylbenzene 503, 514-515
1,4-Diisopropylbenzene 503, 514-515
Diisopropyl ether (DIPE) 442, 429, 556, 570, 575
Dimenhydrinate 541, 544
Dimethoate 446, 486
3,3'-Dimethoxybenzidine 529
1,2-Dimethoxyethane 539, 570
n,n-Dimethylacetamide 539
Dimethylamine 508
Dimethylamphetamine 536
2,4-Dimethylaniline 510
2,6-Dimethylaniline 510, 529
7,12-Dimethylbenz[a]anthracene 465
1,2-Dimethylbenzene 484
n,n -Dimethylbenzylamine 510
2,2-Dimethylbutane 563-564, 571, 574
2,3-Dimethylbutane 563-564, 571, 574
Dimethyl ether 556
Dimethylformamide (DMF) 524, 526-527, 550
n,n-Dimethylformamide (DMF) 526, 539
2,6-Dimethylhept-5-enal 482-483
2,2-Dimethylhexane 444, 471, 574
1,3-Dimethyl-2-imidazolidinone (DMI) 539
2,6-Dimethylnaphthalene 465
1,2-Dimethyl-2-nitrobenzene 446
1,3-Dimethyl-2-nitrobenzene 445
2,2-Dimethylpentane 571, 574
2,3-Dimethylpentane 563-564, 574
2,4-Dimethylpentane 563-564, 571, 574
Dimethylpentyltin 461
3,6-Dimethylphenanthrene 465
2,3-Dimethylphenol 464
2,4-Dimethylphenol 455, 462, 464, 466, 504
2,5-Dimethylphenol 464
2,6-Dimethylphenol 464
3,4-Dimethylphenol 464
Dimethyl phthalate 445, 462-463
Dimethyl sulfide 474, 526, 554-556, 566-567
Dimethyl sulfoxide (DMSO) 526-527, 539, 549
Dimethyl-tetrachloro-terephthalate (DCPA) 435, 438-439, 448, 451
2,5-Dimethylthiophene 554
Dimethyltryptamine 545
2,4-Dinitroaniline 529
2,2'-Dinitrobiphenyl 465
2,7-Dinitrofluorene 465
4,6-Dinitro-2-methylphenol 462
1,3-Dinitronaphthalene 465
1,5-Dinitronaphthalene 465
2,4-Dinitrophenol 455,462-464, 466, 504, 530
2,5-Dinitrophenol 464
2,4-Dinitrotoluene 445, 462
2,6-Dinitrotoluene 445, 462
Di-n-octyl phthalate 462-463
Dinonyl phthalate 463
Dinoseb 439, 464
1,3-Dioxalane 519
1,4-Dioxane 442, 477, 519, 524-526, 535, 550, 552, 568
Diphenamid 445, 452-453
Diphenhydramine 544
Diphenylaniline 510
9,10-Diphenylanthracene 465
Diphenyl isophthalate 463
Diphenyl oxide 482-483
Diphenyl phthalate 463
Diphenylpyraline 544
Dipropylene glycol 519-520
Dipropyl ether 575
Disulfoton 445, 452
Diuron 453

cis-13,16-Docosadienoic acid methyl ester....497-498
cis-4,7,10,13,16,19-Docosahexaenoic acid methyl ester....497-498
Dodecahydrotriphenylene....465
γ-Dodecalactone....482-483
Dodecane....197, 199-200, 523, 552-553, 568
n-Dodecane....197, 208, 557, 571-572
Dodecanoic acid....494
Dodecanal....489
Dodecanol....482-483
n-Dotriacontane....572
Doxylamine....541, 544
Droperidol....546
Dursban (Chlorpyrifos)....445-446

E

cis-11,14-Eicosadienoic acid methyl ester....497-498
Eicosane....482
n-Eicosane....572
cis-5,8,11,14,17-Eicosapentaenoic acid methyl ester....497-498
cis-8,11,14-Eicosatrienoic acid methyl ester....498
cis-11,14,17-Eicosatrienoic acid methyl ester....497-498
cis-11-Eicosenoic acid methyl ester....497-498
Elaidic acid methyl ester....497-498
Endosulfan I....434-435, 438, 440-441, 445, 447-452, 456-457
Endosulfan II....434-435, 438, 440-441, 445, 447-452, 456-457
α-Endosulfan....500
b Endosulfan....500
Endosulfan sulfate....434-435, 438, 440-441, 445, 447-452, 456-457, 500
Endrin....434-435, 438, 440-441, 445, 447-452, 456-457
Endrin aldehyde....434-435, 438, 440-441, 445, 447-452, 456-457
Endrin ketone....434-435, 440-441, 445, 447, 449-451, 456-457
Ephedrine....536
Epiandrosterone (*trans*-androsterone)....548
Epichlorohydrin....442, 519
Eptam....454
EPTC....445, 452-453
Erucic acid methyl ester....497-498
Erythritol....494
Esfenvalerate....446
Estazolam....536
17-α-Estradiol....548
β-Estradiol....548
Estriol....548
Estrone....548
Ethane....534, 558-560, 563-566, 571, 576
Ethanol....442, 478, 492-493, 501, 505, 523-528, 535, 538-539, 549-551, 556, 570-571, 575
Ethchlorvynol....546
Ethinamate....546
2-(Ethlamino)-ethanol....506
Ethoprop....445, 452-453
Ethosuximide....543
Ethotoin....544
2-Ethoxyethanol (Cellosolve)....501, 505, 507, 535, 539
2-Ethoxyethyl acetate....507, 517-518
bis(2-ethoxyethyl) phthalate....463
Ethyl acetate....551
Ethyl acelytene....534
Ethyl acetate....442, 477-478, 482-483, 492-493, 517-518, 524-528, 535, 539, 549-550
Ethyl acrylate....517-518, 526-528
Ethyl alcohol....507
Ethyl and dimethyl thiophenes....568
Ethylbenzene....429, 442, 444, 468-469, 471, 473, 477, 503, 514-516, 523, 532, 539, 549, 552-553, 563-564, 568-569, 571, 574, 576
Ethylbenzene-d10....571
Ethyl benzoate....493, 517-518
2-Ethyl-1-butanol....505
Ethyl butanonate....478
Ethyl butyrate....482-483, 493, 518
Ethyl caprate....478
Ethyl caproate....518
Ethyl caprylate....478
Ethyl cellosolve....525
Ethyl decanoate....482-483
Ethyl disulfide....554
Ethyl dodecanoate....482-483
Ethylene....534, 553, 559-560, 563-565, 576
Ethylene/acetylene....566
Ethylenediamine....511
Ethylene glycol....501, 505, 519-522, 531, 549
Ethylene glycol/monoacetate....507
Ethylene glycol monobutyl ether....519-520
Ethylene glycol monoethyl ether....519-520
Ethylene glycol/monoformate....507
Ethylene glycol monomethyl ether....519-520
Ethylene glycol phenyl ether....522
Ethylene oxide....504, 507, 531, 569
Ethyl ether....442, 519, 524, 550
Ethyl formate....492, 507, 517-518, 524, 549
Ethyl heptanoate....482-483
Ethyl hexadecanoate....482-483
Ethyl hexanoate....482-483
2-Ethyl hexanoic acid....435
2-Ethyl-1-hexanol....492, 501, 505
bis-2-ethylhexyl adipate....445
bis(2-ethylhexyl) phthalate....445, 462-463
Ethyl isovalerate....482-483
Ethyl mercaptan....554-556, 566-567
Ethyl methacrylate....442, 444, 471, 528
Ethyl methyl sulfide....554
Ethylmorphine....537
Ethyl nonanoate....482-483
Ethyl octadecanoate....482-483
Ethyl octanoate....482-483
Ethyl parathion....500
Ethyl pentadecanoate....482-483
Ethyl pentanoate....482-483
a-Ethylphenethyl alcohol....501, 505
b-Ethylphenethyl alcohol....501, 505
2-Ethylphenol....530
4-Ethylphenol....530
Ethyl-3-phenyl oxiran carboxylate....493
Ethyl propanoate....478
Ethyl propionate....482-483, 517-518, 527-528
Ethyl-*tert*-butyl ether (ETBE)....429, 442, 556, 570, 575
Ethyl tetradecanoate....482-483
2-Ethylthiophene....554
4-Ethyltoluene....477
m-Ethyltoluene....552, 568
p-Ethyltoluene....552, 568
Ethyl undecanoate....482-483
Ethyl valerate....518
Ethyl vinyl ether....519
Etridiazole....435, 438, 448, 451
Eucalyptol....480-481
Eugenol....485, 487
Eugenyl acetate....482-483
Eugenyl methyl ether....483
Evernyl....482

F

Faneosolacetate....490
Farnescene....491
β-Farnesene....480
trans-β-Farnesene....479, 481, 490
Farnesol....487
Farnesol 1....487
Farnesyl acetate....491
Fenamiphos....445-446, 452
Fenarimol....445, 452
Fenchone....487
Fenchyl acetate....482
Fenitrothion....486, 500
Fentanyl....540, 545
Fenthion....486
Fenvalerate....446
Florazone....482-483
Flunitrazepam....141, 536, 539-540
Fluoranthene....431-432, 458, 462, 465
Fluorene....431, 445, 458, 462, 465
Fluorobenzene....442, 444, 468-469, 471, 514-515
2-Fluorobiphenyl....462
2-Fluorophenol....462
Flurazepam....540, 542
Fluridone....445, 452-453
Fonofos....453
Formaldehyde....474, 477, 513
Formaldehyde-DNPH....513
Formaldehyde-PFBHA....514
Formic acid....435, 494, 507
Frambione (raspberry ketone)....482-483
Fucitol....493
Furan....519
Furfural....482-483, 512
Furfuryl alcohol....501, 505

G

Galactitol....493-494
Geranial....482-483, 488-489
Geranial acetate....491
Geraniol....482-483, 485, 487, 490, 493
cis-Geraniol....480
trans-Geraniol....487
Geranyl acetate....480, 482-483, 488, 490
Geranyl butyrate....483
Geranyl formate....482-483
Geranyl-2-methyl valerate....482
Geranyl tiglate....482-483
Germacrene-d....479-480, 489-491
Gesatamine (Atraton)....445
Glucitol....493
Glucuron acid....494
Glucuron acid-1,5-lacton....494
Glutethimide....540, 546
Glycidol....501, 505
3,7-Guaiadiene....482
α-Gurjunene....491

H

Halazepam....536, 540
Haloperidol....546
Halothane....532
Helium....476
Heneicosane....482
Heneicosanoic acid methyl ester....497-498
1,7-Hepatanediol....522
Heptachlor....434-435, 438, 440-441, 445, 447-452, 456-457
Heptachlor epoxide....434-435, 438, 440-441, 445, 447-452, 456-457
2,2',3,3',4,4',6-Heptachlorobiphenyl....445
Heptadecane....461
n-Heptadecane....572
Heptadecanoic acid methyl ester....497-498
Heptadec-1-ene....482
cis-10-Heptadecenoic acid methyl ester....497-498
Heptanal....478, 511-512
Heptane....516, 523, 539, 549, 552, 568, 576
n-Heptane....477, 524, 535, 550, 553, 563-564, 571-572
1,7-Heptanediol....519-520
1-Heptanethiol....554
Heptanoic acid....494, 507, 511
n-Heptanoic acid....435
1-Heptanol....458, 501, 505
2-Heptanol....501, 505
3-Heptanol....501, 505
2-Heptanone....512
3-Heptanone....512
4-Heptanone....512
cis-4-Hepten-1-ol....501, 505
trans-2-Hepten-1-ol....501, 505
Hercolyn D (tetrahydro & dihydro methyl abietate)....482
Hexabromobenzene (HBB)....438, 448, 451

Hexabromobiphenyl....446
Hexachlorobenzene....435, 445, 447-448, 451, 456-457, 462
2,2',4,4',5,6'-Hexachlorobiphenyl....445
Hexachlorobutadiene....442, 444, 462, 468-469, 471, 477, 502, 522
Hexachloro-1,3-butadiene....473
β-Hexachlorocyclohexane (HCH)....500
δ- Hexachlorocyclohexane....500
γ- Hexachlorocyclohexane....500
Hexachlorocyclopentadiene....435, 438, 445, 448, 462, 502, 522
Hexachloroethane....442, 444, 462, 471, 502, 522
Hexachloropentadiene....447, 456-457
n-Hexadecane....197, 572
Hexadecanoic acid....494
2,4-Hexadienal....481
Hexanal....478, 511-512
Hexane....444, 471, 523-524, 526, 539, 549, 551, 570, 574, 576
n-Hexane....477, 524, 535, 550, 553, 558-560, 563-564, 571-572
1,6-Hexanediol....519-520
1-Hexanethiol....554
Hexanoic acid....511
Hexanol....197, 199-200, 482-483
1-Hexanol....478, 501, 505
2-Hexanol....501, 505
3-Hexanol....501, 505
2-Hexanone....444, 471, 477, 512
3-Hexanone....512
n-Hexatriacontane....572
Hexazinone....445-446, 452-454
cis-2-Hexene....563-564
trans-2-Hexene....563-564
cis-2-Hexen-1-ol....501, 505
cis-3-Hexen-1-ol....501, 505
Hexobarbital....537, 541
Hexyl acetate....483
Hexyl butyrate....480
Hexyl cinnamaldeyde....487
Hexyl cinnamic aldehyde....485
Hexylene glycol....482-483
Hexyl 2-ethylhexyl phthalate....463
1-Hexyl mercaptan....567
n-Hexyl mercaptan....567
Hexyl methacrylate....528
α-Humulene....488
Hydrocarbon....516
Hydrocodone....539, 541
Hydrogen sulfide (H2S)....474, 504, 534, 553-556, 558, 566-567
Hydroxy acetate....507
Hydroxy citronellal....482-483, 485, 487
4-Hydroxy-4-methyl-2-pentanone....501, 505
Hydroxyphenamate....541
Hydroxypropionitrile....442
Hydroxypropyl acrylate....528
Hydroxyzine....544

I

Ibogaine....540, 545
Ibuprofen....541, 547
Imipramine....542
Indan....571
Indeno[1,2,3-cd]pyrene....431, 433, 445, 458, 462
Inositol....493
Iodobenzene....514-515
Iodoform....502, 522
Iodomethane....444, 468, 471, 502, 522
Irgafos....533
Irganox....533
Isoamyl acetate....478, 493, 517-518
Isoamyl alcohol....478, 492
Isoamyl butyrate....493
Isoamyl mercaptan....567
Isoamyl salicylate....482, 484
Isoborneol....482-483-484, 491
Isobutane....558-566, 574
Isobutanol....442, 492-493, 501, 505, 525-528, 556, 570
Iso-butene....534
Iso-buteraldehyde....557
Isobutyl acetate....478, 482-483, 517-518, 524, 527-528
Isobutyl acrylate....527-528
Isobutyl alcohol....478
Isobutylaldehyde....478, 556
Isobutylbenzene....503, 514-515, 553
Isobutylene....559-562
Isobutyl mercaptan....567
Isobutyl propionate....527-528
Isobutyraldehyde....512, 575
Isobutyric acid....435, 494-495, 507-508, 511
Isocaproic acid....494, 507
Isodrin....435, 447, 451, 456-457
Isoeugenol....485, 487
trans-Isoeugenol....487
Isomenthol....481
Isomenthone....479, 481-483
d-Isomethone....489
a-Isomethyl ionone....487
Isonox 129....533
Isooctane....429, 523-524, 535, 551, 553, 563-564, 571
Isopentane....553, 558-566, 570-571
Isopentanoic acid....435
Isophorone....445, 462
Isoprene....561-564
Isopropanol....478, 501, 505, 524-525, 538, 550, 556
Isopropyl acetate....517-518, 524-525, 539
Isopropyl acrylate....527-528
Isopropyl alcohol....442, 477, 524, 549
Isopropyl amine (IPA)....506, 549
Isopropylbenzene (cumene)....442, 444, 468-469, 471, 503, 514-516, 553, 563-564, 568
Isopropyl ether....519
Isopropyl mercaptan....567
Isopropylmyristate....482 -483
2-Isopropylphenol....530
Isopropyltoluene....442
4-Isopropyltoluene....469
p-Isopropyltoluene....444, 468, 471
Isovaleraldehyde....556, 575
Isovaleric acid....494-495, 507, 511

J

Jasmolin I....461
Jasmolin II....461
cis-Jasmone....479, 490

K

Kelthane....435, 447, 456-457
Kepone....446
Ketamine....546
Ketimine....545
Krypton....557

L

Lactose....494
Lactulose....494
Lauric acid methyl ester....497-498
Lavandulol....480
Lavandulyl acetate....480
Levulinic acid....435
Lidocaine....540, 543, 546
Lignoceric acid methyl ester....497-498
Lilial....485, 487
Limonen....489
Limonene....479, 482-484, 487, 489-492
δ-Limonene....480-481, 488
Linalool....479, 482-485, 487-492
β-Linalool....480
Linalool acetate....480
cis-Linalool oxide....483
trans-Linalool oxide....482, 483
Linalyl acetate....482-484
Lindane....448
Linoleic acid methyl ester....497-498
Linolelaidic acid methyl ester....497-498
Linolenic acid methyl ester....497-498
γ-Linolenic acid methyl ester....497-498
Lofentanyl....545
Lorazepam....536, 539-540
Lormetazepam....536
Lyral....485
Lyral 1....487
Lyral 2....487
Lysergic acid diethylamide (LSD)....540, 545

M

β-Maaliene....481
Malathion....446, 486, 500
Manitol....494
Mannitol....493
Meclizine....544
Medazepam....536, 540
Menthofuran....481
Menthol....481, 484, 489
Menthone....481-483
Menthyl acetate....489
Meperidine....539, 542
Mephobarbital....537
Mepivacaine....543
Meprobamate....541, 546
Merphos....445, 452
Mescaline....545
Mesitylene....523
Mesityl oxide....525
Mesterolone....548
Methacrolein....512, 526-527
Methacrylic acid....435
Methacrylonitrile....442, 444, 471, 526-527
Methadone....539-540, 542
Methamidophos....486
Methamphetamine....536, 539, 542
Methandrostenolone....548
Methane....476, 526, 534-535, 553, 557-560, 563-566, 576
Methanol (MeOH)....478, 492-493, 501, 505-506, 513, 523-528, 535, 538-539, 549-551, 553, 556-557, 570, 575
Methapyrilene....541, 544
Methaqualone....540, 546
Methidathion....486
Methofuran....489
Methohexital....537
Methone....489-490
Methoprene....461
Methoxychlor....434-435, 438, 440-441, 445, 447-451, 456-457
2-Methoxyethanol (methyl Cellosolve)....501, 505, 526
bis(4-methoxyethyl) phthalate....463
2-Methoxy-5-methylaniline....529
1-Methoxy-2-propanol....539
Methsuximide....543
3-Methy-1-butanol....535
Methycyclohexane....535
Methyl acetate....517-518, 527-528, 535
Methyl acetylene....566
Methyl acrylate....442, 444, 471, 527-528
Methylamine....508
4-Methylaminorex....545
2-Methylanthracene....465
9-Methylanthracene....465
r-Methylansiole....490
Methyl arachidate....495
Methyl benzoate....483, 490-491, 517-518
2-Methyl butanal....511
2-Methylbutane....574
2-Methyl-1-butanol (active amyl alcohol)....493, 501, 505
2-Methyl-2-butanol (*tert*-amyl alcohol)....501, 505
3-Methyl-1-butanol (isoamyl alcohol)....493, 501, 505

3-Methyl-2-butanone 512, 535
2-Methyl-1-butene 571
2-Methyl-2-butene 559, 563-564, 571
3-Methyl-1-butene 561-564
trans-2-Methyl-2-butenoic acid 508
2-Methyl-3-buten-2-ol 501, 505
3-Methyl-2-buten-1-ol 501, 505
2-Methylbutyl acetate 517-518
2-Methylbutyl alcohol 482-483
3-Methylbutyl alcohol 482-483
Methyl-*tert*-butyl ether (MTBE) 429, 442, 444, 471, 519, 523, 539, 549, 556-557, 570-571, 575
Methyl butyrate 482-483
2-Methyl butyric acid 508
Methyl chavicol 485
3-Methylcholanthrene 465
2-Methyl-4-chloro-phenoxy acetic acid (MCPA) 439
Methylchlorophenoxy propionic acid (MCPP) 439
5-Methylchrysene 433
Methyl-cresol 482
Methyl-para-cresol 483
Methyl-ρ-cresol 491
Methylcyclohexane 539, 563-564, 574
Methylcyclopentane 553, 563-564, 571, 574
1-Methyl-1-cyclopentene 571
Methyl decanoate 518
Methyl-2,4-dichlorophenylacetate 439
Methyl diethanolamine (MDEA) 506
4-Methyl-2,5-dimethoxyamphetamine 536
2-Methyl-4,6-dinitrophenol 455, 463-464, 466, 504
Methyl disulfide 554
Methyl dodecanoate 518
Methyl eicosenoate 518
Methyl elaidate 495
Methylene chloride 442, 444, 468-469, 471, 473, 477, 502, 522, 524, 539, 549-550
4,4'-Methylenedianiline 529
Methylenedioxy-amphetamine (MDA) 536, 539, 542
3,4-Methylenedioxy-ethylamphetamine 536, 539, 542
Methylenedioxy methamphetamine (MDMA) 539, 542
3,4-Methylenedioxy methylamphetamine 536
Methyl ephedrine 536
1-Methyl-2-ethylbenzene 571
1-Methyl-3-ethylbenzene 571
1-Methyl-4-ethylbenzene 571
Methyl ethyl ketone (MEK) 524-525, 550, 556
Methyl ethyl sulfide 556
Methyl eugenol 485
2-Methylfluoranthene 465
Methyl formate 517-518, 525
3-0-Methylglucose 1 494
3-0-Methylglucose 2 494
Methyl heptadecanoate 495
2-Methylheptane 553, 563-564, 571
3-Methylheptane 563-564, 571
4-Methylheptane 553
Methyl heptin carbonate 485, 487
Methyl hexadecanoate 518
2-Methylhexane 563-564, 574
3-Methylhexane 563-564, 574
Methyl 2-hydroxydecanoate 495
Methyl 2-hydroxydodecanoate 495
Methyl 3-hydroxydodecanoate 495
Methyl 2-hydroxyhexadecanoate 495
Methyl 2-hydroxytetradecanoate 495
Methyl 3-hydroxytetradecanoate 495
Methyl g-ionone 485
α-Methyl ionone 484
Methyl isobutyl ketone 524-525, 539
Methyl laurate 495
Methyl mercaptan 474, 554-556, 566-567
Methyl methacrylate 442, 444, 471, 527-528
Methyl *cis*-9,10-methylene octadecanoate 495
Methyl *cis*-9,10-methyl hexadecanoate 495
Methyl 14-methylhexadecanoate 495
Methyl 12-methyltetradecanoate 495
Methyl monoethanolamine (MMEA) 506
Methyl myristate 495
1-Methylnaphthalene 465, 571
2-Methylnaphthalene 462, 465, 571
2-Methyl-5-nitroaniline 529
Methyl nonadecanoate 495
Methyl octadecanoate 518
Methyl octine carbonate 485, 487
Methyl oleate 495
Methyl palmitate 495
Methyl palmitoleate 495
2-Methylpantane 574
Methyl paraoxon 445
Methyl parathion 500
Methyl pentadecanoate 495
2-Methylpentane 429, 563-564, 571
3-Methylpentane 429, 523, 563-564, 571, 574
2-Methyl-2 pentanol 556
3-Methyl-3-pentanol 505
4-Methyl-2-pentanol 501, 505
2-Methyl-3-pentanone 512
4-Methyl-2-pentanone (MIBK) 444, 471, 477, 512
2-Methyl-1-pentene 563-564, 571
4-Methyl-1-pentene 563-564
bis(4-methyl-2-pentyl) phthalate 463
2-Methylphenol 462, 464
3-Methylphenol 464
4-Methylphenol 462, 464
a-Methylphenyl alcohol 501
5-Methyl-5-phenylhydantoin 543
2-Methyl-1-propanethiol 554-556, 566
2-Methyl-2-propanethiol 554-555, 566
2-Methyl-1-propanol (isobutanol) 575
2-Methyl-2-propanol (*tert*-butanol) 539, 575
Methyl propionate 517-518, 527-528
1-Methyl-1-propnaethiol 555, 566
1-Methyl-3-propylbenzene 571
1-Methyl-1-propyl mercaptan 567
2-Methyl-1-propyl mercaptan 567
2-Methyl-2-propyl mercaptan 567
2-Methyl pyridine 432
1-Methyl-2-pyrrolidine 510
1-Methyl-2-pyrrolidinone 526-527
n-Methylpyrrolidone 539
Methyl stearate 495
4-Methylstyrene 514-515
α-Methylstyrene 514-516, 552, 568
Methyl sulfide 534
17α-Methyltestosterone 548
Methyl tetradecanoate 518
2-Methylthiophene 554
3-Methylthiophene 554
Methyl thiophenes 568
Methyl tridecanoate 495
Methyltripentyltin 461
Methylundecanoate 495
Metolachlor 438, 445, 452-453
Metribuzin 438, 445, 452-453
Mevinphos 445, 452
MGK 264 ....445, 452
Endo-MGK 264 461
Exo-MGK 264 461
Mirex 435, 446-447, 451, 456-457
Molinate 445, 452-453
6-Monoacetylmorphine 537
Mono-ethanolamine (MEA) 506
Mono ethylene glycol 506
Monuron 453
Morphine 537, 541, 546
Musk ketone 484
Musk T (ethylene brassylate) 482-483
Musk xylene 484
Myrcene 479, 482-484, 488-490
β-Myrcene 480-481
Myristic acid methyl ester 497-498
Myristoleic acid methyl ester 497-498

N

Naphthalene 197, 199-200, 429, 431, 442, 444, 458, 462, 465, 468-469, 471, 523, 553, 571
Naphthalene-d8 ....462-463, 571
1-Naphthol 530
Napropamide 445, 452-453
Nefopam 543
Neomenthol 484, 489
Neon 476, 557
Neral 482-483, 487-489
Nerol 481
Nerol acetate 480
cis-Nerolidol 482
trans-Nerolidol 482
Nervonic acid methyl ester 497-498
Neryl acetate 482-483, 488
Nicotinamine 536
Nicotine 539-541, 547
Nitrazepam 141, 536, 539
2-Nitroaniline 462, 510, 529
3-Nitroaniline 462, 510, 529
4-Nitroaniline 462, 510, 529
Nitrobenzene 442, 444, 462, 471, 514-515
Nitrobenzene-d5 462
2-Nitrobiphenyl 465
3-Nitrobiphenyl 465
4-Nitrobiphenyl 465
Nitrofen 435
Nitrogen 476, 504, 532, 557
Nitromethane 535
1-Nitronaphthalene 465
2-Nitronaphthalene 465
Nitrophen 446
2-Nitrophenol 455, 462, 464, 466, 504, 530
3-Nitrophenol 464
4-Nitrophenol 439, 455, 463-462, 464, 466, 504
Nitropropane 525
2-Nitropropane 442, 444, 471
n-Nitrosodimethylamine 432, 462, 463
n-Nitrosodiphenylamine 462
n-Nitroso-di-n-propylamine 462
2-Nitrotoluene 503, 514-515
3-Nitrotoluene 503, 514-515
4-Nitrotoluene 503, 514-515
cis-Nonachlor 448
trans-Nonachlor 435, 445, 447-448, 456-457
Nonadecane 483
Nonadec-1-ene 482-483
γ-Nonalactone 482-483
Nonanal 488-489
Nonane 523, 552, 568, 574, 576
n-Nonane 458, 553, 563-564, 571-572
1,9-Nonanediol 519-520, 522
Nonanol 492
1-Nonanol 501, 505
Nonyl aldehyde 512
n-Nonylamine 509-510
Nootkatone 489
Norcodeine 537
Nordazepam 536
Norethandrolone 548
Norflurazon 445-446, 452-453
Normorphine 537
19-Nortestosterone (Nandrolone) 548
19-Nortestosterone-17-decanoate 548
19-Nortestosterone-17-propionate 548

O

trans-Ocimene 479
β-*cis*-Ocimene 479-480, 489-490
β-*trans*-Ocimene 480
1,2,3,4,6,7,8,9-OCDF 432
1,2,3,4,6,7,8,9-Octachlorodibenzodioxin (OCDD) 432
2,2',3,3',4,5',6,6'-Octachlorobiphenyl 445
n-Octacosane 572
Octadecane 461

n-Octadecane....572
Octadecanoic acid....494
Octanal....478, 488-489, 511
Octane....523, 552, 568, 574, 576
n-Octane....458, 553, 563-564, 571-572
1,8-Octanediol....519-520
Octanoic acid....494, 511
Octanol....482-483, 488, 492
1-Octanol....501, 505
3-Octanol....479, 489-490
3-Octanone....458, 480
1-Octene....458
1-Octen-3-ol....480, 489
Octen-1-ol acetate....480
Octyl acetate....482-483
3-Octyl acetate....479, 490
Octyl aldehyde....512
n-Octylamine....509-510
n-Octyl mercaptan....567
Oleic acid methyl ester....497-498
Omethoate....486
Ordram....454
Ortho xylene....532
Oxadiazon....454
Oxazepam....536, 539-540
Oxazopam....536
Oxychlordane....446
Oxycodone....141, 539
4,4′-Oxydianiline....529
Oxygen....476, 557
Oxymetholone....548
Oxymorphone....541

P

Paarlan....454
Palmitic acid methyl ester....497-498
Palmitoleic acid methyl ester....497-498
Paraldehyde....442
Parathion....446, 486
Parathion-methyl....486
Pebulate....452-453
Pentaborane....533
Pentachlorobenzene....514-515
2,2',3',4,6-Pentachlorobiphenyl....445
Pentachloroethane....442, 444, 471, 502, 522
Pentachloronitrobenzene....435, 438, 447, 451, 456-457
Pentachlorophenol....439, 445, 455, 462-464, 466, 504
n-Pentadecane....197, 557, 572
Pentadecanoic acid methyl ester....497-498
10-Pentadecenoic acid methyl ester....497-498
cis-1,3-Pentadiene....561-562
trans-1,3-Pentadiene....561-562
Pentafluorobenzene....442, 444, 471
Pentafluoroethane....454
Pentamethylbenzene....571
Pentamethyl disiloxane....533
Pentanal....511
Pentane....502, 517, 526, 570, 574, 576
i-Pentane....576
n-Pentane....553, 558-566, 570-572
1,2-Pentanediol....458
1,5-Pentanediol....519-520
2,3-Pentanedione (acetyl propionyl)....478, 482-483
1-Pentanethiol....554
n-Pentanoic acid....435
1-Pentanol....501, 505, 539
2-Pentanol....478, 501, 505
3-Pentanol....478, 501, 505
2-Pentanone....442, 512, 524
3-Pentanone....512
Pentene-1....559, 561-562
1-Pentene....559-560, 563-564, 571
cis-2-Pentene....559, 561-564
trans-2-Pentene....559, 561-564
4-Pentenoic acid....508
trans-2-Pentenoic acid....508
trans-3-Pentenoic acid....508
1-Penten-3-ol....501, 505
2-Penten-1-ol....501, 505
Pentobarbital....537, 541
Pentyl ether....519
1-Pentyl mercaptan....567
cis-Permethrin....435, 438, 445, 447-448, 451, 456-457
trans-Permethrin....435, 438, 445, 447-448, 451, 456-457
Perthane....435, 447, 456-457
Perylene....465
Perylene-d12....445-446, 462-463
α-Phellandrene....488
Phenacetin....536, 541
Phenanthrene....431, 445, 458, 462, 465
Phenanthrene-d10....445, 462-463
Phencyclidine (PCP)....539-540, 542, 545
Phenethylalcohol....492
Pheniramine....544
Phenmetrazine....541
Phenobarbital....537, 540-541, 543-544
Phenol....197, 199-200, 430, 455, 462, 464, 466, 504, 530
Phenol-d5....462
2-Phenoxyethanol....501, 505
Phensuximide....543
Phentermine....536, 539
Phenyl acetaldehyde....485, 487
Phenylacetone....536
Phenylacetylene....552, 568
9-Phenylanthracene....465
Phenyl ephedrine....536
Phenylethyl acetate....478, 482
Phenylethylamine....510
Phenyl ethyl cinnamate....482-483
Phenylethylmalonamide....543-544
Phenylethyl tiglate....482-483
2-Phenylnaphthalene....465
Phenyltoloxamine....544
Phenytoin....543-544
Phorate....453
Phosphine....533
Picloram....439
4-Picoline....458
α-Pinene....479-483, 489-491
β-Pinene....479, 481-484, 488-491
Piperazine....511
Piperitone....489
Pirimiphos-methyl....486
Polyethylene glycol....521
Polymethoxyflavones....489
Prazepam....536, 540
Prebane (Terbutryne)....445
Primidone....543-544
Procaine....541, 543, 546
Progesterone....548
Promazine....544
Promethazine....544
Prometon....445, 452-453
Prometryn....452
Prometryne....445-446, 453
Promofos....500
Pronamide....445, 452-453
Propachlor....435, 438, 445, 447-448, 451, 453-454, 456-457
Propadiene....534, 559-562
Propanal....477
Propane....517, 558-566, 571, 574, 576
1,3-Propanediol....519-520
1,2-Propanediol (propylene glycol)....519-520
1-Propanethiol....554-555, 566
2-Propanethiol....554-556, 566
Propanil....453
Propanoic acid....511
Propanol....474
1-Propanol....442, 501, 505, 535, 538-539, 549, 570, 575
1-Propanol....478, 526
2-Propanol....526, 535, 539, 570
n-Propanol....492-493, 524-525, 550, 556
2-Propanone....570
Propargyl alcohol....442
Propazine....445-446, 452-454
Propene....477
2-Propen-1-ol (allyl alcohol)....501, 505
Propiolactone....442
Propiomazine....546
Propionaldehyde (propanol)....512, 556, 575
Propionic acid....435, 492, 494-495, 507
1-Propionic acid....458
Propionitrile....442, 444, 471, 510, 526-527
Proposyphene....542
Propyl acetate....478, 517-518, 535
Propylbenzene....442, 514-516, 523, 552-553, 568
n-Propylbenzene....444, 458, 468-469, 471, 503, 516, 563-564, 568, 571
Propyl benzoate....517-518
Propyl butyrate....518
Propyl caproate....518
Propylene....517, 553, 555, 559-566, 576
Propylene glycol....501, 505
Propylene glycol dimethyl ether....519-520
Propyl ether....519, 556
Propyl formate....517-518
1-Propyl mercaptan....567
2-Propyl mercaptan....567
n-Propyl mercaptan....567
2-Propyl pentanoic acid....435
Propyl propionate....517-518
Propyl valerate....518
Propyne (methylacetylene)....559-564
2-Propyn-1-ol (propargyl alcohol)....501, 505
Prowl....454
Psilocin....545
Pulegone....489
Pyrazole....510
Pyrene....431, 445, 458, 462, 465
Pyrene-d10....445
Pyrethrin I....461
Pyrethrin II....461
Pyridazine....510
Pyridine....442, 462, 510, 524, 526-527, 535, 550
Pyrilamine....544
Pyrimidine....510
Pyrimiphos ethyl....500
Pyrimiphos methyl....500
Pyrithyldione....546
Pyrrobutamine....541

Q

Quinine....546

R

Rhamnitol....493-494
Rhamnose 1....494
Rhamnose 2....494
Ribitol....493-494
Ribose 2....494
Rosatol (rosetone)....483
Rose oxide, *cis*-rose....482-483
Rose oxide, *trans*-rose....482-483

S

Sabinene....479, 482, 488-490
trans-Sabinene hydrate....479, 489-490
Salicylamide....543
α-Santoloene....480
Secbumeton....453
Secobarbital....537, 541
Selenide....533
Sencor....454
α-Sinensal....489
β-Sinensal....489
Simazine....438, 445, 448, 452-454
Simetryn....445, 452-453
Sorbitol....494

Stanozolol....548
Stearic acid methyl ester....497-498
Stigmasterol....548
Stirofos....452
Strawberry aldehyde....493
Strychnine....539, 546
Styrene....442, 444, 468, 471, 473, 477, 503, 514-517, 523, 532, 552, 563-564, 568
Styrene dimer....517
Styrene oxide....514-515
Styrene trimer....517
Sucrose....494
Sufentanyl....545
Sulfallate....453
Sulfur dioxide....504, 534
Sulpiride....546
Sutan....454

T

Talbutal....537, 546
Tebuthiuron....445, 452
Temazepam....141, 536, 539-540
Tenocyclidine (TCP)....545
Terbacil....445, 452-454
Terbufos....445, 452-453
Terbus sulfone....446
Terbuthylazine....453
Terbutryn....452-453
Terphenyl-d14....462
Terpinene....489, 491
α-Terpinene....479, 488-490
γ-Terpinene....479, 481-483, 490, 492
Terpinen-4-ol....479-480, 482-483, 488-490, 492
α-Terpineol....482-484, 488-490, 491-492
α-Terpinol....480
Terpinolene....479, 483, 488, 490
γ-Terpinolene....489
Terrazole....445, 447, 456-457
Testosterone....548
Tetraborane....533
Tetrabutyltin....461
Tetracaine....543
1,2,4,5-Tetrachlorobenzene....514-515
2,2',4,4'-Tetrachlorobiphenyl....445
2,3,7,8-Tetrachlorodibenzodioxin (TCDD)....432
2,3,7,8-Tetrachlorodibenzofuran (TCDF)....432
1,1,1,2-Tetrachloroethane....442, 444, 468-469, 471, 502, 522
1,1,2,2-Tetrachloroethane....442, 444, 468, 471, 473, 477, 502, 522
Tetrachloroethene....442, 444, 468-471, 473, 477, 522
Tetrachloroethlyene....436, 470
2,3,4,5-Tetrachlorophenol....430, 464
2,3,4,6-Tetrachlorophenol....430, 464
2,3,5,6-Tetrachlorophenol....430, 464, 466
Tetrachloro-m-xylene....434-435, 440-441, 447, 451, 456-457, 460
2,4,5,6-Tetrachloro-m-xylene....449-450
Tetrachlorvinphos (Stirifos)....445
n-Tetracontane....572
n-Tetracosane....572
Tetradecane....571
n-Tetradecane....197, 557, 572
Tetradecanoic acid....494
Tetraethylenepentamine....511
1,1,1,2-Tetrafluoroethane....454
1,1,2,2-Tetrafluoroethane....454
Tetrahydofuran....526
Tetrahydrocannabinol....539
δ9-Tetrahydrocannabinol....548
1,2,3,4-Tetrahydrofluoranthene....465
Tetrahydrofuran (THF)....444, 471, 477, 519, 524, 539, 550
Tetrahydropyran....519
Tetrahydrothiophene....554
1,2,3,5-Tetramethylbenzene....571
1,2,4,5-Tetramethylbenzene....553, 571
Tetrapentyltin....461
Thenyldiamine....541
Thiamylal....537
Thiazopyr....446
Thioacetamide (TAA)....570
4,4'-Thiodianiline....529
Thiopental....537
Thiophene....554-556, 566-568
Thioridazine....544
Thonzylamine....544
Threhalose....494
Threitol....494
Thujone....487
α-Thujone....482, 488
β-Thujone....488
Tillam (Pebulate)....445, 454
Tinuvin P....533
α-Tocopherol....545
β-Tocopherol....545
δ-Tocopherol....545
γ-Tocopherol....545
Tolban....454
o-Tolidine....529
m-Tolualdehyde....512
o-Tolualdehyde....512
p-Tolualdehyde....512
Toluene....197, 199-200, 429, 442, 444, 468-469, 471, 473, 477, 503, 514-517, 523-525, 532, 535, 539, 549-550, 552-553, 561-564, 568-569, 571, 574, 576
Toluene-d8....442, 473
Tonalid....482-484
Trazodone....539
Treflan....454
γ-Trepinene....488
Triademefon....452
Triadimefon....445
Triazolam....536, 540
Tribromoacetic acid....467
2,4,6-Tribromophenol....462
Tributylpentyltin....461
Trichloroacetic acid....467
Trichloroacetonitrile....436, 470
2,4,5-Trichloroaniline....529
1,2,3-Trichlorobenzene....442, 444, 468-469, 471, 514-515
1,2,4-Trichlorobenzene....442, 444, 462, 468-469, 471, 473, 477, 514-515
1,3,5-Trichlorobenzene....514-515
2,4,5-Trichlorobiphenyl....445
Trichloroethane....524
1,1-Trichloroethane....549
1,1,1-Trichloroethane....436, 442, 444, 468-471, 473, 477, 502, 522, 535
1,1,2-Trichloroethane....436, 442, 444, 468-469, 471, 473, 477, 502, 522
Trichloroethene....442, 444, 468-471, 473, 477, 522
Trichloroethylene....436, 470, 524, 526, 535, 550
Trichlorofluoromethane....442, 444, 454, 468-469, 471, 473, 477
Trichloromethane....526
Trichloromethyl silane....533
2,3,4-Trichlorophenol....430, 464, 466
2,3,5-Trichlorophenol....430, 464, 466
2,3,6-Trichlorophenol....430, 464, 466
2,4,5-Trichlorophenol....430, 462, 464, 466
2,4,6-Trichlorophenol....430, 455, 462, 464, 466, 530
3,4,5-Trichlorophenol....430, 464
2,4,5-Trichlorophenoxyacetic acid....439
1,2,3-Trichloropropane....436, 442, 444, 467-468, 471, 502, 522
1,1,1-Trichloropropanone....470
1,1,1-Trichloro-2-propanone....436
1,1,2-Trichlorotrifluoroethane....502, 522
1,1,2-Trichloro-1,2,2-trifluoroethane....454, 473, 477
Tricosanoic acid methyl ester....497-498
Tricyclazole....445, 452-453
Tridecane....552-553, 568
n-Tridecane....197, 557
Tridecanoic acid methyl ester....497-498
Triethanolamine (TEA)....506
Triethylamine....510, 526-527
Triethylene glycol....521
Triethylene glycol dimethyl ether....519-520
Triethylenetetramine....511
1,1,1-Trifluoroethane....454
Trifluoromethane....454
Trifluorotoluene....468
α,α,α-Trifluorotoluene....429
Triflupromazine....544
Trifluralin....435, 438, 445, 447-448, 451, 456-457
Trimethylamine....508
2,4,5-Trimethylaniline....529
1,2,3-Trimethylbenzene (hemimellitene)....429, 514-515, 553, 571, 574, 576
1,2,4-Trimethylbenzene (pseudocumene)....429, 442, 444, 468-469, 471, 473, 477, 514-515, 523, 553, 563-564, 571
1,3,5-Trimethylbenzene (mesitylene)....429, 442, 444, 468-469, 471, 473, 477, 514-515, 563-564, 571
Trimethylchloro silane....533
3,5,5-Trimethylhexanol....482-483
2,3,3-Trimethylpentane....553, 571
2,3,4-Trimethylpentane....563-564
2,2,4-Trimethylpentane....477
2,3,5-Trimethylphenol....530
Trimethyl phosphate....458
Trimipramine....540
2,4,6-Trinitrophenol....504
1,3,5-Trioxane....478
Tripelennamine....544
Triphenyl phosphate....445-446, 486
Triprolidine....544

U

Undecane....523, 552, 568, 574
n-Undecane....197, 208, 553, 571-572
Undecanoic acid methyl ester....497-498

V

Valencene....489
Valeraldehyde....512, 556, 575
Valeric acid....494, 507, 508, 511
Valerolactone....508
Vanillin....487
Verapamil....539
Vernam....454
Vernolate....445, 452-453
Vertenex....482-483
Vinclozolin....500
Vinclozoline....446
Vinyl acetate....477, 517-518
Vinyl chloride....442, 444, 468-469, 471, 473, 477
Vinyl-trimethyl silane....533
Viridiflorol....479, 489-490

W

Water (H2O)....507, 553, 558, 570

X

Xenon....557
m-Xylene....429, 442, 444, 468-469, 471, 473, 477, 503, 514-516, 523, 525, 532-533, 552, 563-564, 568-569, 571, 574, 576
o-Xylene....429, 442, 444, 468-469, 471, 473, 477, 503, 514-516, 523, 525, 532, 539, 549, 552-553, 563-564, 568-569, 571, 574, 576
p -Xylene....429, 442, 444, 468-469, 471, 473, 477, 503, 514-516, 523, 525, 532, 552-553, 563-564, 568-569, 571, 574, 576
m,p-Xylene....429, 539, 549
2,3-Xylenol....530
2,4-Xylenol....530
2,5-Xylenol....530
2,6-Xylenol....530
3,4-Xylenol....530
3,5-Xylenol....530
Xylose 1....494
Xylose 2....494

Ordering Information

Easy Ordering Terms and Conditions

Discounts and Delivery

Agilent Technologies specializes in fast delivery. In the US, if you call before 2 PM EST, we will ship your order that day. You may also request overnight express delivery before 6 PM EST and you will have your order the next day. Volume discounts on a variety of individual products are offered when the entire quantity is shipped to one address at one time.

A shipping and handling fee will be added to your order unless the purchase is over $2000 US for orders place online or over $4000 for orders place via phone. Special shipping (i.e., overnight in the US) is available in most regions at an additional cost.

Agilent is required to collect all state and local sales taxes unless the buyer's tax-exempt certificate is on file with Agilent Technologies. Please be prepared to provide a copy if it is not on file, when placing your order.

Please check with your Agilent Customer Service Representative, local Authorized Distributor, or the Agilent website for current prices, special offers, promotions and discounts when placing your order.

Satisfaction Guaranteed

If you are not satisfied with your Agilent product within the first 60 days, you may return your purchase in its original condition for a full refund or credit. A return policy statement is included in every Agilent shipment and posted under Product Information on the website. In the US and Canada, please call for a Return Authorization form and return instructions at **1-800-227-9770**. If your Agilent product was purchased from a distributor, please contact the distributor.

Shipping Damages

If items are damages in transit, please follow the instructions below:

- If a shipment is visibly damaged upon arrival, do not accept it until the person making the delivery has endorsed the bill of lading with statement for the extent of the damage.
- If any damage is found after unpacking, retain all cartons and inner packaging and immediately request an inspection from the carrier.
- Notify the Agilent Customer Contact Center at **1-800-227-9770** about the damaged shipment so that we can make the appropriate sales adjustment and/or provide you with return instructions (Sales order number, product number and quantity damaged will be needed).

Easy Ways To Order

- Phone: **1-800-227-9770** (option 1, 1) in the US and Canada – Mon-Fri, 8AM to 8PM EST
- Fax: **1-302-633-8901** in the US
- Email: **cag_sales-na@agilent.com** in the US and Canada
- Online: **www.agilent.com/chem** in the US and Canada

Payment Options

- In the US, Visa, MasterCard, Discover and American Express are accepted with a minimum order of $20 (not applicable in all countries).
- Email ePay@agilent.com to make an electronic payment using the ACH/EFT (Automated Clearing House/Electronic Funds Transfer) method.
- Establish a charge account through your Agilent Customer Service Representative or Your Local Agilent sales office. An account number will be assigned to you for charging your purchases. Payment terms are net 30 days from the invoice date. All orders are subject to credit approval.

We will be happy to supply a price quote via, phone, email or fax if you need it in writing.

Warranties

All Agilent Technologies products in this catalog are designed and manufactured to stringent standards under the Agilent quality system registered to ISO 9001. At Agilent, we back every product with a 90-day warranty and a money-back guarantee. If Agilent receives notice of defects during the warranty period. Agilent shall, at its option, either repair or replace products which prove to be defective. If Agilent is unable, within a reasonable time, to repair or replace any product to a condition as warranted, the buyer shall be entitled to a refund of the purchase price upon return of the product to Agilent. The warranty period for each product begins on the day of shipment.

This warranty shall not apply to any defect, failure, or damage caused by improper use or improper or inadequate maintenance or care. This warranty is exclusive and no other warranty, whether written or oral, is expressed or implied. Agilent specifically disclaims the implied warranties of merchantability and fitness for particular purposes. The remedies provided herein are the buyer's sole and exclusive remedies. In no event shall Agilent be liable for direct, indirect, special, incidental, or consequential damages (including loss of profits) whether based on contract, tort, or any other legal theory.

For more information

Buy online:
www.agilent.com/chem/store

Contact us:
www.agilent.com/chem/contactus

This information is subject to change without notice.

© Agilent Technologies, Inc. 2012
Printed in Canada October 31, 2012
5991-1058EN

Scan the QR code
with your smartphone
for more information



The Measure of Confidence

Agilent Technologies